

# Review of Antimicrobial Nanocoatings in Medicine and Dentistry: Mechanisms of Action, Biocompatibility Performance, Safety, and Benefits Compared to Antibiotics

James Butler, Richard D. Handy, Mathew Upton, and Alexandros Besinis\*



Cite This: *ACS Nano* 2023, 17, 7064–7092



Read Online


ACCESS |

Metrics & More

Article Recommendations

**ABSTRACT:** This review discusses topics relevant to the development of antimicrobial nanocoatings and nanoscale surface modifications for medical and dental applications. Nanomaterials have unique properties compared to their micro- and macro-scale counterparts and can be used to reduce or inhibit bacterial growth, surface colonization and biofilm development. Generally, nanocoatings exert their antimicrobial effects through biochemical reactions, production of reactive oxygen species or ionic release, while modified nanotopographies create a physically hostile surface for bacteria, killing cells via biomechanical damage. Nanocoatings may consist of metal nanoparticles including silver, copper, gold, zinc, titanium, and aluminum, while nonmetallic compounds used in nanocoatings may be carbon-based in the form of graphene or carbon nanotubes, or composed of silica or chitosan. Surface nanotopography can be modified by the inclusion of nanoprotusions or black silicon. Two or more nanomaterials can be combined to form nanocomposites with distinct chemical or physical characteristics, allowing combination of different properties such as antimicrobial activity, biocompatibility, strength, and durability. Despite their wide range of applications in medical engineering, questions have been raised regarding potential toxicity and hazards. Current legal frameworks do not effectively regulate antimicrobial nanocoatings in matters of safety, with open questions remaining about risk analysis and occupational exposure limits not considering coating-based approaches. Bacterial resistance to nanomaterials is also a concern, especially where it may affect wider antimicrobial resistance. Nanocoatings have excellent potential for future use, but safe development of antimicrobials requires careful consideration of the “One Health” agenda, appropriate legislation, and risk assessment.

**KEYWORDS:** antimicrobial, resistance, antibacterial, antibiofilm, antibiotics, nanoparticle, nanomaterial, nanocoating, surface, safety

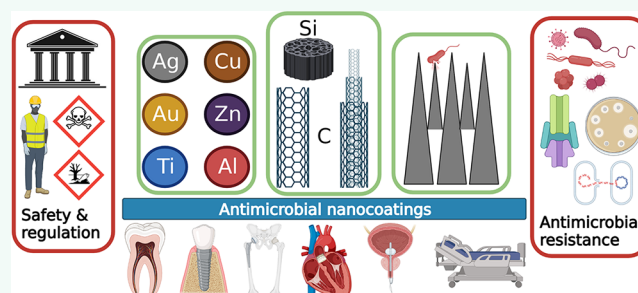


Engineered nanomaterials (ENMs) are clusters of atoms forming structures that have at least one dimension in the size range of 1–100 nm and can be found in different shapes and forms including nanoparticles, nanocrystals, nanorods and nanofibers.<sup>1</sup> The behavior of ENMs can differ significantly from that of their bulk counterparts because their properties are not determined by their mass or chemical composition exclusively, as with most macro-materials. Certain factors affect the biological interactions of ENMs including their particle size,<sup>2,3</sup> shape and surface area to volume ratio,<sup>4,5</sup> crystallinity<sup>6</sup> and surface charge.<sup>7</sup> The unique properties and behaviors of nanomaterials in comparison to their micro- and macro-scale counterparts are the driving force behind the growing body of research in nanotechnology, which allows


materials to be developed with specific desired properties. A range of ENMs have been found to have potent antimicrobial properties and as such have enormous potential in medical engineering applications where inhibition of bacterial growth and colonization is important. In recent years, the mechanisms of action of ENMs have become better understood and the exact

**Received:** December 16, 2022

**Accepted:** March 17, 2023

**Published:** April 7, 2023



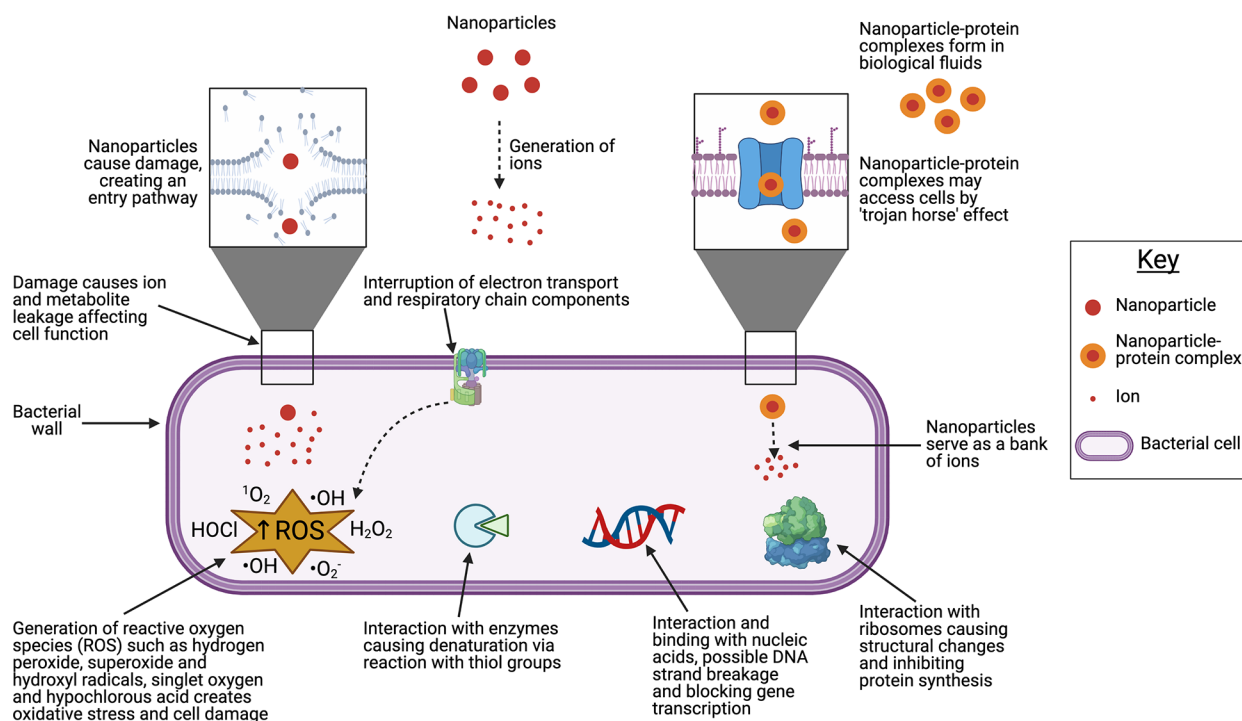

**Figure 1.** Antimicrobial mechanisms of nanoparticles. Nanoparticles gain entry by damaging the cell wall. Damage to the cell wall by nanoparticle entry may itself lead to leakage of ions and metabolites, conferring an antimicrobial effect. Nanoparticles act as a reservoir of ions which go on to interact intracellularly with ribosomes, nucleic acids, and enzymes, disrupting normal function. Interruption of the respiratory chain leads to generation of reactive oxygen species which create oxidative stress and damage cell components. Figure was created using [BioRender.com](https://www.biorender.com).

effects that ENMs can have on bacterial or eukaryotic cells are finally being described, allowing optimization of their antimicrobial performance while maintaining biocompatibility and reducing ecological impact.

This review addresses the state of up-to-date research on the development, application and testing of ENMs with intrinsic antimicrobial properties as surface coatings for medical and dental applications. There are plentiful publications examining nanomaterials as antimicrobial agents<sup>8–11</sup> or as carriers for antimicrobial drug delivery.<sup>12,13</sup> However, this review discusses the use of ENMs in the form of antimicrobial surface nanocoatings and modification of the surface nanotopography to achieve infection prevention and control (IPC) in medicine and dentistry. The electronic search was conducted by applying a combination of subject terms and keywords on databases including PubMed, Scopus, Google Scholar, and Web of Science. The keywords applied to the searches were: (nanomaterial OR nanoparticle OR nanocoating OR nanotechnology) AND (antimicrobial OR antibacterial OR antifungal OR antibiofilm OR infection). Quality criteria included an assessment of experimental design and appropriate controls, comparisons, and conclusions in the published and peer-reviewed English-language literature. Publications with insufficient detail or relevance, poor descriptions of methodology, lack of replication, or inadequate material characterization were excluded. Examples were also chosen to show a representative selection of materials and applications; these selected examples from the published literature are presented in [Tables 1–4](#). Representative example images of nanocoatings are also shown in [Figures 2 and 4](#). The aims of this review are: (a) to present and discuss the types of antimicrobial nanocoatings available where the nanomaterial itself is intrinsically antimicrobial and assess

their reported efficacy, (b) to evaluate the importance and relevance of nanocoatings and surface nanotopography as alternative antimicrobial strategies in the wider context of antimicrobial resistance and infection prevention and control, and (c) to discuss the general pitfalls and safety considerations associated with clinical applications.

## ANTIMICROBIAL MECHANISMS OF NANOPARTICLES

The antimicrobial mechanisms of nanoparticles (NPs) are increasingly being understood in detail and are summarized in [Figure 1](#). Generally, these mechanisms can be classified as direct contact-mediated killing and ion-mediated killing. Direct contact-mediated killing involves NP anchorage to and infiltration of the bacterial cell wall; this leads to membrane damage, leakage of cellular contents and ultimately may alone result in bacterial death.<sup>14–17</sup> In this way, large NPs that cannot translocate the bacterial cell wall can still exert bactericidal effects by adsorption and thereby causing mechanical deformation leading to cell rupture and death.<sup>18</sup> Upon penetration of the cell wall, NPs gain access to the cell interior and interfere with the function of intracellular biomolecules or structures such as proteins, organelles, and DNA either by direct interactions or by generation of ions. It is possible that NPs may also gain access to the cell without causing membrane damage by way of the protein corona effect, in which NPs in biological environments become modified by adsorption of biomolecules to their surface.<sup>19,20</sup> Protein-occluded NPs become akin to a “trojan horse” and gain easier entry into the cell; however, while this has been shown to occur in eukaryotic cells,<sup>21,22</sup> it is not known whether the mechanism can be generalized to include bacteria.

The generation of ions (e.g., Ag<sup>+</sup> or Cu<sup>2+</sup>) is broadly correlated with NP surface area, with greater surface area leading to greater ion production and thus greater antimicrobial activity.<sup>23</sup> NPs may function as a “bank” of ions once inside the cell, continuously releasing them and prolonging or strengthening the antibacterial effect. Liberated metal cations can interact with thiol (sulfhydryl) groups in bacterial enzymes, forming stable bonds and disrupting function in essential molecules involved in transmembrane energy generation and electrolyte transport.<sup>24</sup> Metal cations such as Ag<sup>+</sup> can uncouple the respiratory electron transport chain from oxidative phosphorylation and interfere with penetration of H<sup>+</sup> and phosphate into membranes.<sup>25–27</sup> Within the bacterial cell, metal cations can form complexes with nuclear material by intercalation between base pairs, disrupting hydrogen bonds and ultimately preventing effective cell division.<sup>28,29</sup> The production of reactive oxygen species (ROS), either by disruption of the thioredoxin system<sup>30</sup> or by interaction with the respiratory chain and interruption of intracellular O<sub>2</sub> reduction,<sup>31</sup> is a major ion-mediated killing mechanism.

Generally, the mechanisms mentioned above overlap and cumulatively contribute to an antimicrobial effect. In some cases, however, certain mechanisms are considered to be more prominent for specific nanomaterials than for others. For example, nanosilver binds to the thiol groups of cysteine residues, which are frequently crucial for many proteins to maintain their integrity and function.<sup>32</sup> Meanwhile, for nanomaterials consisting of oxides, such as TiO<sub>2</sub>, ZnO, CuO and Al<sub>2</sub>O<sub>3</sub>, toxicity to bacteria is predominantly the result of ROS generation.<sup>33–35</sup> However, it is also clear that nonoxide NPs such as Se NPs<sup>36</sup> and NPs composed of Ag, Cu, Fe, Mn, Co, Au, or Pt also generate ROS.<sup>37</sup>

## BIOFILM DEVELOPMENT AND ANTIMICROBIAL RESISTANCE

Biofilms are communities of bacteria organized into localized, heterogeneous and sessile aggregations that form when bacteria accumulate and adhere to surfaces, forming a thin but robust layer. The bacteria in biofilms are embedded within and secrete a mixture of biomolecules making up a dynamic matrix collectively termed extracellular polymeric substances (EPS). The EPS is composed of a complex assembly of protein, polysaccharide, and extracellular DNA, resulting in a three-dimensional architecture.<sup>38,39</sup> The EPS has several roles including physical protection from shear forces, antimicrobials, and immune responses, enabling the diffusion of nutrients through the biofilm, and facilitating horizontal transfer of genes.<sup>40,41</sup> The EPS layer confers a level of hydrophobicity which prevents permeation by most extraneous molecules and makes the biofilm very resilient, with some authors even referring to it as “omniphobic” — *i.e.*, repelling all substances.<sup>42</sup> Experiments conducted *in vitro* have demonstrated that bacteria residing in mature biofilms can be between 10–1,000 fold more resistant to antibiotics than their equivalent planktonic cells, demonstrating the extremely robust nature of biofilms once formed.<sup>43,44</sup> In this way, biofilm formation represents a major strategy allowing bacteria to defend against antimicrobial attack, facilitating resistance. Biofilms are ubiquitous in the environment, increasingly being considered the predominant means by which microbes thrive in their niche,<sup>45</sup> including in the human body, but can present particular health concerns due to their ability to harbor pathogens and resist disinfectants<sup>46,47</sup> and antibiotics.<sup>48–51</sup>


Antimicrobial resistance (AMR) is the outcome of microorganisms changing over time to be able to survive exposure to antimicrobial medicines such as antibiotics which are designed to kill them or inhibit their growth. The recent repeated warnings regarding the rise of AMR in bacteria, the major clinical challenges that this imposes,<sup>52</sup> and the various national and international efforts to develop novel antimicrobials in order to maintain our ability to fight bacterial infections underscore the importance of antimicrobial nanomaterials to biomedical research, engineering, and clinical practice. One study found that the burden of antibiotic-resistant infections is comparable to the cumulative burden of influenza, tuberculosis, and HIV, most seriously affecting children aged <1 year and the elderly aged >65 years.<sup>53</sup> Furthermore, it was reported that about 75% of the total antibiotic-resistant infection burden was associated with healthcare and 39% of all antibiotic-resistant infections are caused by bacteria with resistance to last-line or last-resort antibiotics, indicating that they are very difficult or even potentially impossible to treat. The UK government-commissioned O’Neill review<sup>54</sup> on drug-resistant infections reported that at current rates, by 2050, AMR will lead to 10 million deaths a year, a 2.0–3.5% reduction in gross domestic product and will cost the world up to US\$100 trillion. A study of the global AMR burden in 2019 estimated that 4.95 million deaths were associated with bacterial AMR, with 1.27 million deaths directly attributable to AMR.<sup>55</sup> Unfortunately, the discovery and development of new antibiotics is not straightforward; no majorly impactful classes of antibiotics were introduced between 1962 and 2000,<sup>56</sup> although the approval of daptomycin<sup>57</sup> by the US Food and Drug Administration (FDA) in 2003 is often cited as one example of success. The global antibiotics market is dominated by classes introduced half a century ago<sup>56</sup> and the majority of the pharmaceutical industry has dismantled or scaled back its antibiotic research laboratories, leaving an inadequate antibiotic pipeline and lack of industry infrastructure and expertise.<sup>58,59</sup> The divestment in antibiotic R&D by the pharmaceutical industry is largely driven by poor returns on investment and it is now widely acknowledged that reimbursement for antibiotic development needs to be delinked from sales volumes.<sup>60</sup> There are several international initiatives now in place that aim to “fix” the antibiotic R&D funding model: a UK scheme is being trialed where the Government will pay manufacturers a fixed fee for access to new antibiotics; similar approaches are being adopted in Germany and Sweden with a premium being paid for selected antibacterial agents; and in the US the PASTEUR Act will ensure annual revenues for new antibiotics meet a minimum level that is acceptable to industry.<sup>61</sup>

To address the recommendations of the O’Neill report, and ultimately reduce the global burden of AMR, both new antibiotics and new alternative antimicrobial strategies are urgently needed. As biofilms—once formed—provide such an effective barrier against antimicrobial attack, novel strategies which inhibit biofilm formation must be sought.


## USE OF NANOCOATINGS AS A STRATEGY FOR INFECTION PREVENTION AND CONTROL

As the effectiveness of currently available antibiotics is being undermined by rising AMR, nanotechnology seems to be a promising alternative strategy for treatment or IPC. Certain types of free NPs suspended in solutions have been found to be highly effective antimicrobials under *in vitro* conditions.<sup>62–64</sup> However, their application in an immobilized form, such as



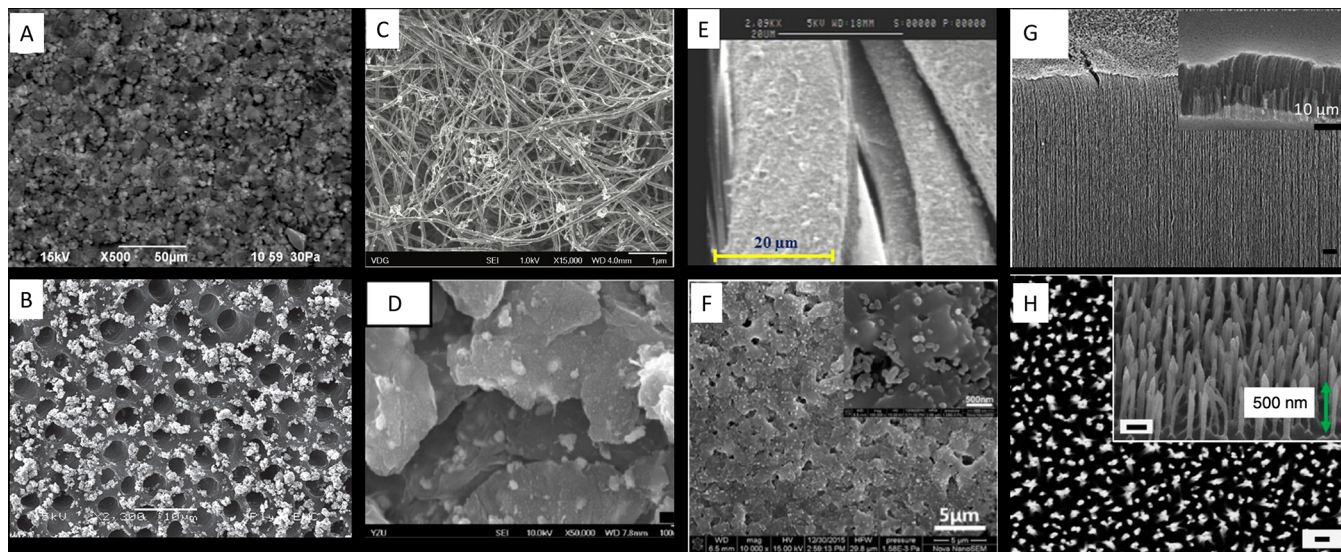

**Figure 2.** Representative scanning electron micrographs of antimicrobial nanocoatings. (A) Poly(methyl methacrylate) and silver nanoparticles deposited on silicon wafers. Reprinted with permission from ref 76. Copyright 2017 Elsevier. (B) Dentine coated with silver nanoparticles. Reprinted with permission from ref 77. Copyright 2014 Taylor & Francis Ltd. (C) Multiwalled carbon nanotubes decorated with silver nanoparticles. Reprinted with permission under a Creative Commons CC BY 3.0 License from ref 78. Copyright 2014 Hindawi Publishing Corporation. (D) Silver nanoparticles and zinc oxide nanoparticles embedded on graphene oxide. Reprinted with permission under a Creative Commons CC BY 4.0 License from ref 79. Copyright 2019 MDPI. (E) Fabric coated with poly(styrenesulfonate), chitosan and silver nanoparticles. Reprinted with permission from ref 80. Copyright 2020 Elsevier. (F) Silica nanoparticles applied to a titanium substrate by a microarc oxidation technique. Reprinted with permission from ref 81. Copyright 2017 Elsevier. (G) High aspect ratio ( $30\ \mu\text{m}$ ) vertically aligned carbon nanotubes. Reprinted with permission from ref 82. Copyright 2018 American Chemical Society. (H) Upper surface of black silicon with the green arrow indicating the relative height of the nanoprotrusion on the surface. Reprinted with permission from ref 83. Copyright 2013 Springer Nature.

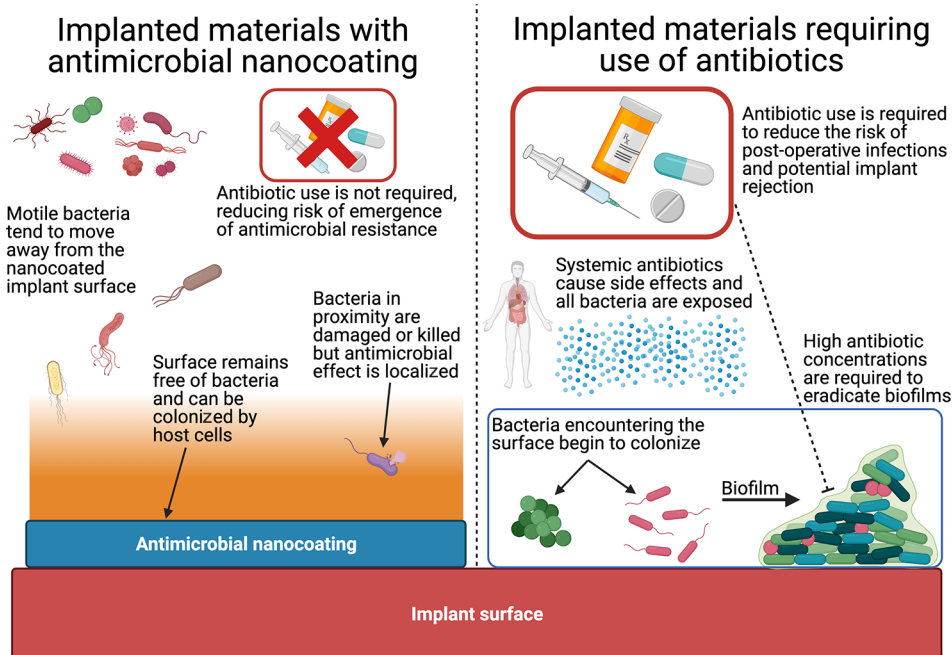

**Figure 3.** Advantages of implanted materials incorporating antimicrobial nanocoatings over those without. Implanted materials without antimicrobial nanocoatings become colonized by bacteria encountering the surface and forming biofilms. Prophylactic antibiotics are often given systemically, bringing side effects to the patient and exposing all bacteria to antibiotics, raising the risk of antimicrobial resistance. High doses of antibiotics are also required to eradicate mature biofilms. When antimicrobial nanocoatings are incorporated on the surfaces of implanted materials, the surface remains uncolonized and antibiotic use may not be required, leading to fewer patient side effects and less exposure of bacteria to antibiotics. While the antimicrobial effects of nanocoatings are local compared to systemic antibiotics, nanocoatings exert an antimicrobial effect beyond the immediate surface and cause bacteria nearby to move away or become damaged. Figure was created using [BioRender.com](https://www.biorender.com).



nanocoatings, is a way to maximize their antibacterial efficacy while minimizing material loss (see representative examples in Figure 2). Regarding surface application of antimicrobials, the ideal scenario for IPC would be inhibition of initial biofilm formation, which requires interruption of bacterial adherence to substrates or early toxicity to bacteria. A “race for the surface” effect has been suggested, in which the first cells colonizing a surface tend to be the ones to successfully develop a community on that surface.<sup>65,66</sup> An experimental setup investigating the “race for the surface” between eukaryotic U2OS osteosarcoma cells and *Staphylococcus epidermidis* demonstrated realistic competition between cells, which can be affected by conditions such as medium flow rate and initial bacterial inoculum.<sup>67</sup> This antagonistic effect between eukaryotic cells and bacteria could be the key to a successful strategy relying on the use of antimicrobial nanocoatings; preventing bacteria from initially establishing dominance on surfaces while allowing cells (e.g., host cells in the case of implanted biomaterials) to adhere.

The use of implanted biomaterials and medical devices continues to increase year upon year mainly because of the aging population and advancement of medical engineering. Implants may include joint replacements, internal fixation orthopedic implants (e.g., screws, pins, plates), bone cements, dental and maxillofacial implants, tissue engineering scaffolds, artificial heart valves, pacemakers, stents, catheters, and wound dressings. Despite their high success rate, implants can still fail because of lack of biocompatibility and immunological rejection. However, development of peri-implantitis, which is caused by infection, remains the most common reason for implant failure.<sup>68</sup> Infections caused by colonization of medical or dental implants can result in patient morbidity and mortality, as well as the need for repeated surgeries with associated financial cost, patient distress and wasted resources. Application of suitable nanocoatings to the surface of implants could offer IPC through inhibition of bacterial colonization and biofilm formation.<sup>69</sup> Around half of all nosocomial infections are associated with indwelling medical devices,<sup>70</sup> and in addition to the medical devices that come in direct contact with human tissues, there are a wealth of other surfaces in a clinical environment which can serve as reservoirs of pathogenic microbes. Examples include high-touch surfaces such as preparation surfaces in hospital kitchens and operating theaters, door handles, bedrails, taps, bedding, patient gowns, and scrubs. Detergents and disinfectants are currently used to improve hospital cleanliness but clearly have failed to eliminate the problem,<sup>71–73</sup> and resistance is emerging.<sup>74,75</sup> Applying durable antimicrobial nanocoatings to those surfaces could reduce the spread of infection since they could offer a long-lasting effect.

In the context of implanted biomaterials, antimicrobial nanocoatings offer advantages over antibiotics (Figure 3). One advantage is the exertion of effects locally rather than systemically, as the immediate surface is protected by the nanocoating while other tissues distant from the implant site are not exposed to the antimicrobial. Related to this, nanocoatings may improve the patient experience by avoiding the side effects<sup>84</sup> and complications<sup>85</sup> of antibiotics. Furthermore, antimicrobial nanocoatings would facilitate a reduction in antibiotic usage, allowing them to be reserved for other essential therapeutic applications, and may thereby reduce the opportunity for selection of antibiotic resistant bacteria.

## FACTORS AFFECTING ANTIMICROBIAL ACTIVITY OF ENMS

The activity of nanoparticulate metals differs from that of their bulk counterparts with factors such as NP size, shape, surface charge and elemental composition, playing a pivotal role in not only their physical and chemical characteristics but also their antimicrobial behavior. Due to the differing dimensions among published research and frequent lack of a systematic or easily comparable approach, it can be difficult to determine which properties confer the most potent antimicrobial effects. In some cases, it is difficult to conclude which properties are optimal given that different authors tend not to compare the same conditions, and thus there is generally a lack of direct replication of studies. It is clear though that there are complex interactions between size, shape, method of production and exposure conditions which affect overall antimicrobial activities. A greater understanding and appreciation of these properties and their combined effects on ENM antimicrobial activity will allow better fine-tuning of effects and improve suitability of ENMs to their applications.<sup>86</sup>


**Size.** Baker et al.<sup>87</sup> investigated the effect of size on antibacterial activity in silver NPs and found that NPs with a mean size of 15 nm exhibited higher antibacterial activity against *Escherichia coli* compared to those of 75 nm. Bactericidal properties against other Gram-negative bacteria including *Pseudomonas aeruginosa*, *Vibrio cholerae*, and *Salmonella* Typhi have also been found to be optimal for particles having a diameter of approximately 1–10 nm.<sup>88</sup> The trend of antimicrobial activity increasing with decreasing NP size has been confirmed by multiple other studies.<sup>89–91</sup>

**Shape (Particle Morphology).** In general, spherical NPs are the most common, but other shapes including rods, cubes, flakes, and tubes are available. Some authors suggest that triangular nanoplates have the strongest biocidal activity,<sup>92</sup> while others suggest cubic NPs are the most effective due to the exposed planes.<sup>93</sup> The differences in activity related to particle shape or morphology appear to be due to variations in ionic release as an expression of the total surface area.<sup>94</sup> Thus, particle morphology could be a valuable variable used to tune nanoparticle effects for intended applications, facilitating a controlled design.<sup>86</sup>

**Surface Charge.** Zinc oxide NPs with a positive surface charge have been shown to exhibit antimicrobial activity against both Gram positive and Gram-negative bacteria, while NPs of the same size but with negative surface charge did not exhibit any inhibition of bacterial growth. This is hypothesized to be due to the positive surface charge of the NPs enhancing ROS production and applying mechanical stress on the negatively charged bacterial membrane.<sup>95</sup> Zwitterion-modified silver NPs have been shown to be designed to shift their surface charge in response to differing pH conditions, allowing more targeted antimicrobial activity. This is achieved by NPs responding to physiological pH in healthy tissues while adhering to negatively charged bacteria at infectious sites with lower pH values.<sup>96</sup>

## TYPES OF NANOCOATINGS

Nanomaterials can vary significantly in shape, size, elemental composition, synthesis, presentation, and surface modifications, which means that there is a wide range of different types of nanocoatings available or currently under development. In this review, nanocoatings have been classified according to the family of materials they consist of: metal and metal oxide NPs (Table

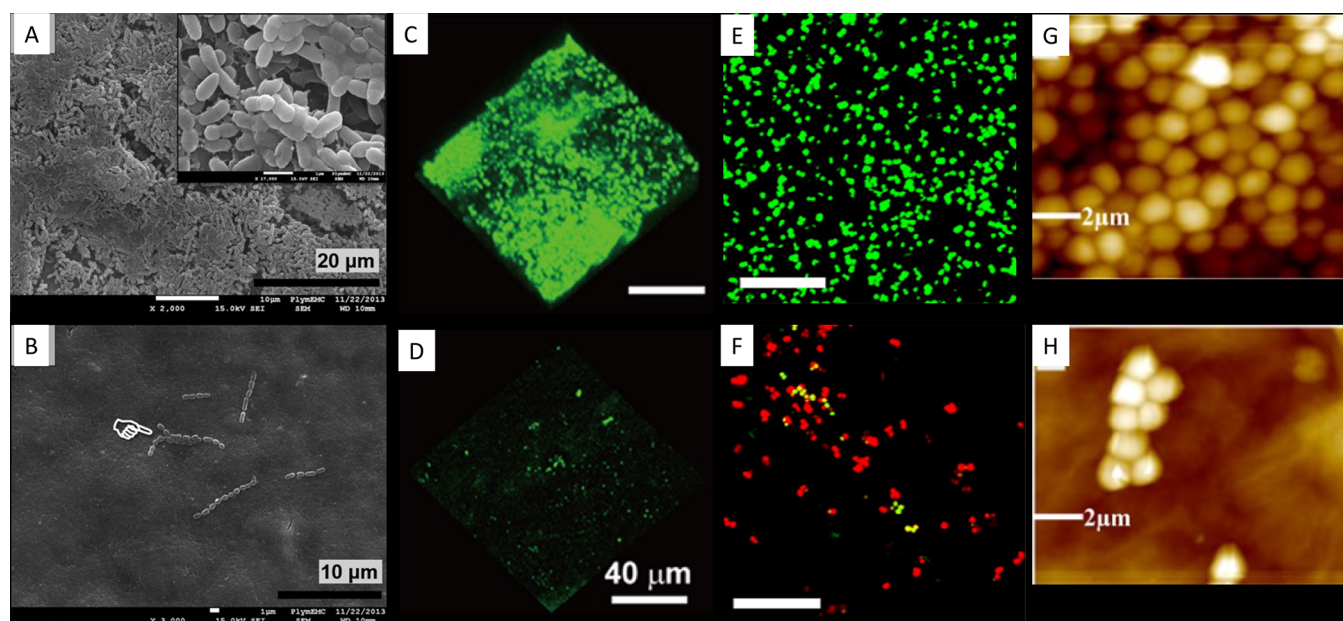

**Figure 4.** Representative examples of nano-coated surfaces showing antimicrobial activity compared to uncoated controls. (A) *Streptococcus sanguinis* biofilm on the surface of uncoated control titanium alloy implants compared to (B) absence of biofilm formation on those implants following application of a dual layer silver-hydroxyapatite nano-coating. Reprinted with permission from ref 69. Copyright 2017 Taylor & Francis Ltd. (C) Confocal laser scanning microscopy live/dead image of *Streptococcus mutans* biofilm on uncoated Invisalign aligners compared to (D) reduced biofilm formation on gold nanocluster-coated aligners. Reprinted with permission from ref 129. Copyright 2020 American Chemical Society. (E) Confocal laser scanning microscopy live/dead image of *Staphylococcus aureus* biofilm on control surfaces compared to (F) surfaces coated with stearic acid nanostructures where fewer live bacteria and far more dead bacteria were present. Reprinted with permission from ref 130. Copyright 2017 Elsevier. (G) Atomic force microscopy image of *Staphylococcus aureus* biofilm on a control surface compared to (H) limited biofilm formation on surfaces coated with graphene oxide. Reprinted with permission from ref 131. Copyright 2017 American Chemical Society.

1), ceramic, and nonmetallic NPs, including carbon-based nanomaterials (Table 2). Representative example images from studies describing antimicrobial nano-coatings can be seen in Figure 4.

**Metal and Metal Oxide Nano-coatings.** Metal compounds have been used as antimicrobial agents since antiquity with silver, zinc, titanium, copper and gold having received the most interest, each showing different properties and antimicrobial efficacy.<sup>97</sup>

**Silver Nano-coatings.** Bulk metallic silver (Ag) has been known for its inherent antimicrobial properties since 4000 BCE,<sup>98,99</sup> well before the introduction of the first antibiotics. More recently, Ag has been used in medical devices such as wound dressings and catheters to restrict or impede bacterial growth and biofilm formation.<sup>100–102</sup>

Silver nanoparticles (Ag NPs) applied as nano-coatings have been investigated in the context of medical implants and prostheses. In the oral cavity, bacteria must adhere to surfaces and form biofilms to survive and proliferate; nutrients in aqueous environments tend to accumulate on surfaces, and adhesion allows bacteria to resist the shear forces of salivary fluid movement and passage to the gastrointestinal tract beyond.<sup>103</sup> As such, prevention of initial bacterial adherence and biofilm formation or reducing the rate of biofilm development and maturation appear to be the major goals of antimicrobial surface coatings in dentistry. Ag NPs have been applied in the form of nano-coatings directly to the surface of dentine.<sup>77</sup> The Ag nano-coatings were found to be stable in biological fluids, prevent biofilm formation, and inhibit bacterial growth in the surrounding media. Ag NPs in this form were also found to be more bactericidal toward the oral pathogen *Streptococcus mutans*

when compared to the oral disinfectant chlorhexidine. Despite Ag NPs being equally as bactericidal as silver nitrate ( $\text{AgNO}_3$ ), they did not cause dentine discoloration. Similar nano-coatings were later studied following application to titanium alloy orthopedic medical implants; silver-plated discs exhibited the highest antibacterial activity and strongest antibiofilm activity while experiencing very little material loss as a result of silver dissolution from the nano-coatings.<sup>69</sup> Ag nano-coatings applied to the surface of silicone maxillofacial prostheses were found to prevent fungal infection caused by *Candida albicans in vitro*, while being highly biocompatible with dermal fibroblasts.<sup>104</sup> These studies have demonstrated that application of silver nano-coatings to medical implants and tissues is a promising alternative antimicrobial strategy that also addresses potential biocompatibility issues. However, it should be noted that these studies were exclusively performed *in vitro*.

Meran et al.<sup>104</sup> suggested good compatibility between Ag NPs and eukaryotic cells, a critical issue in nanomaterial development for clinical applications. A major advantage of Ag NPs is their low toxicity to mammalian cells relative to their bactericidal concentration. This means that although it is possible for them to be toxic to mammalian cells, this can only be possible at concentrations higher than those required to demonstrate bactericidal activity. The minimum inhibitory concentration (MIC) or minimum bactericidal concentration (MBC) of Ag NPs can be difficult to reliably determine using visual methods alone and turbidity corrections must be made because turbidity caused by NP dispersions can mask absorbance caused by bacterial growth at NP concentrations above  $12.5 \mu\text{g mL}^{-1}$ .<sup>62</sup> Corrections are particle-specific as NP properties such as size, shape and crystallinity affect measurements of absorbance.

Reported MIC values for Ag NPs include  $67 \mu\text{g mL}^{-1}$  against a  $6 \times 10^5 \text{ CFU mL}^{-1}$  inoculum of *Streptococcus mutans*<sup>105</sup> or  $4.9 \pm 2.7 \mu\text{g mL}^{-1}$  against a  $1.5 \times 10^5 \text{ CFU mL}^{-1}$  inoculum of the same bacterium and an MBC of  $6.25 \mu\text{g mL}^{-1}$ .<sup>106</sup> These findings highlight the extent to which seemingly similar studies can provide quite varying results, with proteins present in different growth media and the resulting protein corona effect being responsible for those differences.<sup>107,108</sup> An MBC of  $6.25 \mu\text{g mL}^{-1}$  has also been reported for the pathogens *Listeria monocytogenes*, *Escherichia coli* O157:H7, *Salmonella* Typhimurium, and *Vibrio parahaemolyticus*.<sup>109</sup> The minimum concentration having damaging effects on eukaryotic cells has consistently been found to be above  $5 \mu\text{g mL}^{-1}$  in different cell lines.<sup>110–112</sup> Other studies on Ag NPs have reported much higher values as minimum cytotoxic concentrations:  $30 \mu\text{g mL}^{-1}$ <sup>113</sup> or even  $61 \mu\text{g mL}^{-1}$ .<sup>114</sup> These data suggest that there is likely to be a sufficient window of concentration within which to design nanocoatings with appropriate nanoparticle release profiles. A balance must be achieved, generating a high enough concentration of Ag NPs in the local environment to have sufficient effect on bacteria without causing such a high material release as to lead to host cell toxicity or local tissue damage.

The balance of robust antibacterial efficacy with minimal toxicity to eukaryotic cells has been investigated using a porous poly(methyl methacrylate) (PMMA) substrate, a biomaterial highly susceptible to bacterial colonization, combined with a coating of immobilized Ag NPs.<sup>76</sup> The Ag NP thin film was applied using pulsed laser deposition, a process optimized by varying the total laser pulses to alter the thickness of the film. The study showed that it was feasible to develop a manufacturing process to apply the optimal amount of Ag NPs to a PMMA medical implant, minimizing the risk of bacterial colonization while simultaneously reducing the risk of a patient adverse reaction.

Agnihotri et al.<sup>115</sup> investigated Ag NPs immobilized on a functionalized silica surface. Their findings underscored contact killing as the predominant bactericidal mechanism in this context, and showed that immobilized (*i.e.*, surface-coated) NPs demonstrated greater efficacy than colloidal NPs of the same size and morphology. The tested Ag NP-glass surface was shown to be bactericidal for all three bacterial strains (two of *Escherichia coli* and one of *Bacillus subtilis*) investigated at both initial bacterial densities ( $10^3$  and  $10^5 \text{ CFU mL}^{-1}$ ), and complete disinfection (quantified by viable counts of zero in duplicate) was achieved within 2 h for all test conditions. As would be expected, a higher initial bacterial load resulted in a longer time to disinfection, highlighting the importance of standardizing and reporting this value in future work. It was also found that coated surfaces could be reused many times without loss of antibacterial activity; complete disinfection of an initial bacterial load of  $10^3 \text{ CFU mL}^{-1}$  of *Escherichia coli* was achieved within 50 min, even when the surface was used for the 11<sup>th</sup> time. Disinfection was still achieved even when ionic silver release from the surface was very low ( $0.0109 \mu\text{g mL}^{-1}$ ).<sup>115</sup> It would be valuable to investigate how more relevant physiological media containing proteins and other solutes can affect the efficacy of this type of coating; it is well-known that exposure of Ag NPs to physiological media containing proteins and other biomolecules compared to deionized water tends to cause greater agglomeration and more pronounced loss of antimicrobial activity,<sup>116</sup> though this effect may potentially be circumvented by surface coating treatments aiming to prevent NP agglomeration. The relevance of this effect also depends upon the intended application of the

nanocoating; it would be less relevant in a setting where nanocoatings are applied to clinical environmental surfaces (*e.g.*, bed rails, hospital fabrics, and door handles) compared to implanted medical devices that are exposed to high concentrations of biomolecules.

**Copper Nanocoatings.** Similar to Ag, copper (Cu) has been known to have biocidal effects since antiquity, with some more recent applications testing its use for high-touch surfaces (*e.g.*, door handles, bathroom fixtures, and hospital bed rails)<sup>117</sup> and fabrics.<sup>118</sup> Despite the encouraging evidence on antimicrobial activity, concerns about the toxicity and ecological impact of Cu NPs are likely to be the reason preventing further investigation of their use as antimicrobial nanocoatings. There is evidence that Cu NPs are toxic to mammalian somatosensory neurons, with greatest toxicity resulting from smaller NP size and higher concentrations.<sup>119</sup> This is a significant finding as nanomaterials can be transported in a retrograde manner from nerve endings in skin to neurons in the dorsal root ganglion.<sup>120</sup> Additionally, Cu NPs have been reported to be acutely toxic to zebrafish (*Danio rerio*), with the gill being the primary target,<sup>121</sup> and cause retardation of zebrafish embryonic development and morphological malformation of larvae.<sup>122</sup> The fate of Cu NPs in the environment is also different to that of other nanomaterials. For instance, sulfidation of CuO NPs to form  $\text{Cu}_2\text{S}$  or CuS in environments with augmented sulfide levels, such as in wastewater treatment plants, increases solubility rather than decreasing it (as is the case with Ag and ZnO NPs) and leads to greater  $\text{Cu}^{2+}$  release,<sup>123</sup> therefore resulting in increased toxicity to aquatic organisms.<sup>124</sup>

Despite the ecotoxicity concerns around Cu nanomaterials, there have been reports on their use as part of antimicrobial strategies. In order to combine and maximize the effects of the high surface area to volume ratio of NPs and the high aspect ratio of MWCNTs, CuO NPs have been investigated as an application to MWCNTs in contact with eukaryotic cells. Additionally, decoration of CuO NPs onto MWCNTs was anticipated to limit absorption of NPs by the human body as well as reduce the loss of NPs to the environment, addressing the ecological concerns to some extent. Mean average sizes of both cupric (CuO) and cuprous ( $\text{Cu}_2\text{O}$ ) NPs were  $<10 \text{ nm}$ , which is generally at the smaller end of the spectrum for NPs. Cytotoxicity to human dermal fibroblasts only occurred at a relatively high concentration of  $150 \mu\text{g mL}^{-1}$ , while at  $100 \mu\text{g mL}^{-1}$ , some changes to cell morphology were observed but the proportions of live and dead cells remained unaffected. Comparatively, marked antibacterial activity was observed at 60 and  $50 \mu\text{g mL}^{-1}$ . Biofilm development by *Methylobacterium* spp. was inhibited at biocompatible concentrations, and furthermore the CuO/MWCNTs effectively managed to remove preformed biofilms. This study invokes optimism for the synergistic bactericidal and antibiofilm properties of CuO NPs decorated on MWCNTs.

Other studies have confirmed the potent antibacterial activity of CuO NPs when applied as coatings against *Escherichia coli*,<sup>125</sup> *Staphylococcus aureus*,<sup>126</sup> and *Pseudomonas aeruginosa*<sup>127</sup> as well as antibiotic resistant bacteria such as methicillin-resistant *Staphylococcus aureus*.<sup>128</sup> LewisOscar et al.<sup>127</sup> demonstrated that CuO NPs had a strong antibiofilm effect, with a maximum of 94% biofilm inhibition against clinical strains of *Pseudomonas aeruginosa*, at a concentration of only  $0.1 \mu\text{g mL}^{-1}$ . This relatively low concentration demonstrating such potent antibiofilm effects makes CuO NPs an attractive option for antimicrobial nanocoating development. In addition, CuO NPs



at that concentration inhibited the production of EPS by up to 93%, complementing the principal antibiofilm properties by preventing the formation of a protective EPS layer by the proportion of bacteria able to form a biofilm. These findings highlight the potent antibiofilm properties that CuO NPs have and which would be highly relevant to antimicrobial nano-coatings.

**Gold Nanocoatings.** Gold (Au) has been used as an anti-inflammatory agent for the chronic inflammatory disease rheumatoid arthritis, specifically as a disease-modifying antirheumatic drug. However, use of Au salts was replaced by alternative drugs in the 1990s due to adverse effects, limited efficacy and slow relief of symptoms.<sup>132</sup> While this was a setback for the use of Au in modern medicine, more recently Au has been reconsidered for use in nanomedicine.<sup>133</sup> Research suggests Au NPs have potentially reduced relative toxicity and lower masses required to achieve therapeutic efficacy, which makes them an attractive option. However, other studies have exhibited opposing results disputing their potential for clinical use.

Au NPs have been reported to lack inherent antibacterial properties altogether<sup>134,135</sup> or to inhibit biofilm formation without having toxic effects against pathogens.<sup>136</sup> Other studies have suggested that they do have an antibacterial effect, but this is weak, with high MIC values measured (e.g., 197  $\mu\text{g mL}^{-1}$  against *Streptococcus mutans*).<sup>106</sup> Another study found no concentration-dependent effects of Au NPs against *Escherichia coli*, but did report that Au NPs affected cell division.<sup>137</sup> There is evidence that Au NPs have antifungal effects, with one study reporting excellent size-dependent antifungal activity against *Candida* isolates.<sup>138</sup>

Presumably due to their lack of clear potent antibacterial effects, there is little evidence in the published literature describing the use of Au NPs in antimicrobial coatings. Adsorption of Au NPs on a silica surface tested against *Escherichia coli* and *Staphylococcus aureus* did not demonstrate any bactericidal properties.<sup>139</sup> Au NPs can be applied as a shell around a dielectric core to produce an Au nanoshell, while these structures are physiologically inert, they can have photothermal effects and generate significant heat by their strong surface plasmon resonance. The plasmon resonance can be tuned to different wavelengths by varying the relative size of the dielectric core and the thickness of the Au layer.<sup>140</sup> These Au nanoshells were applied to a silicone catheter surface and tested for antimicrobial activity against a drug-resistant strain of *Enterococcus faecalis* using a near-infrared diode laser to produce heat with potentially bactericidal effects. Application of the laser for 5 and 10 min resulted in severely diminished surviving bacterial numbers, with scanning electron microscopy showing thermally induced rupturing of bacterial cell walls.<sup>141</sup> The success of the nanoshell coating becoming antimicrobial upon exposure to the near-infrared laser suggests a possible mechanism where segments of silicone catheter or other materials could be coated and subsequently sterilized on a regular basis. The comparative effects on bacteria in biofilms should also be investigated, though due to the physical method of bacterial killing, it is unlikely that biofilm formation alone would protect bacteria from the relatively high local temperatures (73 °C) encountered.

There is another field of research examining the use of Au NPs in combination with other molecules to deliver an antimicrobial effect, for example, by doping Au NPs with a tRNA analogue,<sup>142</sup> loading them with 5-fluorouracil, an anticancer drug,<sup>143</sup> or by coating them with the antibiotic amoxicillin.<sup>144</sup> This type of application has previously been reviewed<sup>145</sup> and is beyond the

scope of this review because in those cases, the nanomaterial itself was not the active antimicrobial but acted as a carrier for drug delivery.

**Zinc Nanocoatings.** Zinc NPs are most used as antimicrobials in the form of zinc oxide (ZnO). A proposed benefit for ZnO nanocoatings applied to orthopedic or dental implants is the effect of zinc in augmenting bone formation by stimulation of osteoblast activity and cell proliferation.<sup>146,147</sup> Zinc also has a role as a cofactor for collagen synthesis, and supports bone mineralization via alkaline phosphatase.<sup>148</sup> This strong association with bone formation and mineralization makes ZnO NPs ideal candidates for use in antimicrobial nanocoatings near calcified tissues, such as bone scaffolds and joint replacement implants. The antimicrobial effects of ZnO NPs appear to be high, albeit potentially dependent on the morphology of the nanocoating. The strongest antimicrobial effect has been observed for nanomaterials with rod-like morphology and a high degree of crystallinity.<sup>149</sup> These findings were contradicted by another study<sup>150</sup> showing that ZnO nanocoatings had strong antibacterial activity toward *Escherichia coli* and *Staphylococcus aureus*, but no significant differences between particle morphologies were observed. Light-producing biosensor versions of the bacterial cells acting as reporters (constitutively expressing the *Lux* operon and emitting a light signal correlating with cell numbers) allowed real-time measurement of the antibacterial effect, demonstrating that a long incubation was not necessary; the antibacterial effects of ZnO nanocoatings were apparent even after short exposure times. Antibacterial effect also increases with thicker films of NPs, affecting the bacterial generation time and essentially retarding growth and leading to fewer bacterial cells present.<sup>151</sup> Thicker films consist of larger quantities of NPs and presumably result in higher local concentrations of ions following NP dissolution.

Despite ZnO NPs showing good bactericidal efficacy, their biocompatibility and cytotoxic effects must also be considered. It has been reported that ZnO nanofilms significantly decrease cell viability (as confirmed by MTT assay) of cultured macrophages by 54% and 65% depending on NP size (100 and 20 nm, respectively) after a 48 h incubation, although no cytotoxicity was measured after 24 h.<sup>152</sup> This initial lack of cytotoxic effect suggests a gradual release of material which accumulates over time to produce a more cytotoxic concentration, or alternatively could suggest a time-dependent cytotoxic effect. This contrasts with the alternative toxicokinetics where most material is released faster in the short term, causing higher toxicity in the early stages. A later report highlighted that direct exposure of cells to ZnO nanofilms could cause apoptosis and necrosis, two forms of both controlled and uncontrolled eukaryotic cell death, in a murine macrophage cell line.<sup>153</sup> Depending on the type of bioassay employed (MTT versus LDH), cells grown on ZnO nanofilms showed a 43–68% loss of viability following a 24 h exposure compared to controls, with cells separately exposed to undiluted extracts from the coatings showing even greater viability loss. Two diluted coating extracts, 25% and 50% (corresponding to concentrations of 3.03 and 6.07  $\mu\text{g mL}^{-1}$ , respectively) showed no cytotoxic effects against macrophages, indicating a tolerable concentration of ZnO NPs, but it was unclear whether these concentrations would have an antimicrobial effect. Petrochenko et al.<sup>153</sup> highlighted the importance of using both direct-exposure and extract-based methods to assess toxicity, as nanocoatings show gradual material release which can accumulate to a toxic level over time and extracts can simulate the result of this

Table 1. Summary of Additional Selected Examples from the Published Literature Regarding Application of Metal and Metal Oxide Nanoparticles as Antimicrobial Nanocoatings

Nanocoating description	Aim of application	Key methods <sup>a</sup>	Target organisms	Key results <sup>a</sup>	Source
Quaternary ammonium-modified gold nanoclusters	Orthodontic devices	48 h disc immersion in bacterial suspension CVSA and CLSM biofilm quantification	<i>Streptococcus mutans</i>	Reduced biofilm mass (85%) and viability (95%)	129
Nickel–titanium wires coated with ZnO NPs by an electrochemical deposition method	Orthodontic wires	Biocompatibility for oral keratinocytes Agar diffusion test	<i>Streptococcus pyogenes</i> , <i>Staphylococcus aureus</i> , <i>Escherichia coli</i>	Good nanocoating stability No hemolysis and negligible cellular toxicity found ZOIs observed against all bacteria investigated (mean 3.57–6.25 mm), with stronger activity against Gram positives (mean 4.25–6.25 mm)	178
ZnO NPs (12–27 nm) applied to TiZrNb alloy by plasma electrolytic oxidation	Dental and orthopedic implants	Sample immersion in bacterial suspension Adherent cells enumerated	<i>Staphylococcus aureus</i>	>2 log reduction in biofilm after 2 h ZnO NPs-containing ceramic oxide coating hydrophobicity may affect eukaryotic cell attachment	179
Ti or Ti–Zr surfaces were coated with a dual layer of ZnO nanoparticles and nanorods synthesized by a hydrothermal method	Dental implants to prevent peri-implantitis	Biocompatibility tested by seeding with U2OS cells and performing Alamar blue testing Sample immersion in bacterial suspension Viable counts after 6 or 48 h	<i>Escherichia coli</i> , <i>Staphylococcus aureus</i>	Rapid release from ZnO nanoparticles with up to 2-fold higher short-term antibacterial activity Slower release from ZnO nanorods with longer-term antibacterial properties 30–70% <i>Staphylococcus aureus</i> biofilm inhibition after 6 h	180
Ag NPs (38 nm) from silver nitrate applied to surgical nylon threads	Antimicrobial wound dressing material	SEM to assess antibiofilm activity on surfaces coated with bacterial suspension after 2 h <i>In vivo</i> activity in rats measured by implantation Agar diffusion test with AgNO <sub>3</sub> solution and sterile water controls	6 Gram positive bacteria, 4 Gram-negative	<i>In vivo</i> <i>Staphylococcus aureus</i> inhibition (60–80%) over 2 weeks	181
Silver NPs deposited on both sides of cotton gauzes by technology based on <i>in situ</i> photoreduction of AgNO <sub>3</sub>	Application to prevent wound infections	Agar diffusion tests	3 molds 1 yeast <i>Staphylococcus aureus</i>	Growth and biofilm proliferation significantly reduced (3.5–4.5 log) 0.5% (w/v) had little effect on cell viability and high stability 4% (w/v) showed 80% reduced cell viability and several fold higher silver release	182
A “simultaneous sonochemical/enzymatic process” used to apply ZnO NPs to cotton	Medical textiles	Sample immersed in bacterial suspension and cells enumerated, CLSM and SEM Cytotoxicity on mouse embryonic fibroblasts and human keratinocytes with MTT assay	<i>Escherichia coli</i> , <i>Staphylococcus aureus</i>	Nonwashed samples were up to 98% more efficacious against <i>Escherichia coli</i> Cellulase treatment improved durability of antimicrobial effect Biofilm formation inhibited by ZnO (85%) and CuO (70%) Effect was solely antibiofilm	183
Coatings of ZnO (120–180 nm) or CuO (18–20 nm) NPs were applied to a teeth model	Antibiofilm coatings to improve oral health	Durability evaluated after 10 wash cycles Biofilm assays on artificial teeth CVSA after 24 h Fixed teeth visualize with SEM	<i>Streptococcus mutans</i>		184
TiO <sub>2</sub> nanocoatings on Ti implants formed by an aqueous plasma electrodeposition technique	Photoactivated antimicrobial properties for titanium implants	TiO <sub>2</sub> -coated Ti specimen activated with infrared laser for 30 s Samples immersed in bacterial suspension Real time <i>in situ</i> imaging with live/dead-CLSM	<i>Staphylococcus aureus</i>	5 min exposure reduced viability to 23% 30 min exposure reduced viability to 9%	185

<sup>a</sup>CVSA: crystal violet solubilization assay; CLSM: confocal laser scanning microscopy; SEM: scanning electron microscopy; ZOI: zone of inhibition.

accumulation. It is difficult to draw wide conclusions based on these individual studies, but there are indications that ZnO nano-coatings could have inherent biocompatibility issues. Research efforts to address the biocompatibility of ZnO nano-coatings have been scant, with most studies looking at ZnO coatings at particle sizes greater than the nanoscale. A more recent study investigating the *in vitro* biocompatibility of ZnO nanofilms at the nanoscale found that direct exposure to ZnO nanofilms reduced cell viability of mouse fibroblasts due to inhibition of cell adhesion, regardless of ZnO crystallinity.<sup>154</sup> This study appears to agree with that published by Petrochenko et al.<sup>153</sup> and provides further evidence of the adverse effects of ZnO nano-coatings on eukaryotic (*i.e.*, host) cells, leading to concerns over the safety and biocompatibility of ZnO nano-coatings *in vivo*.

**Titanium Nano-coatings.** Titanium (Ti) and its alloys are the industry standard for implanted biomaterials due to their inherent biocompatibility, inert chemistry, strength, corrosion resistance, and lack of toxicity.<sup>155</sup> Ti NPs have also been the subject of extensive research due to their well-established photocatalytic properties,<sup>156</sup> further enhanced by the high surface area of NPs, providing antimicrobial properties.<sup>157</sup> Titanium dioxide (TiO<sub>2</sub>) is most associated with this application, and exists in three main forms: anatase, rutile, and brookite. Anatase is the most photochemically active phase of TiO<sub>2</sub>, though combinations of different phases may show heightened activity compared to anatase alone.<sup>158,159</sup> The high photoactivity and stability of TiO<sub>2</sub>, along with its relatively low cost and lack of toxicity has led to its consideration as a potentially self-disinfecting or self-sterilizing surface coating.<sup>160,161</sup> An advantage of a photocatalytic self-disinfecting surface is that there is no necessity to add other chemical reagents; the only requirements would be oxygen, water and light.<sup>162</sup> The band gap energy of anatase TiO<sub>2</sub> is approximately 3.2 eV, corresponding to activation by photons with wavelength shorter than 385 nm and therefore to UVA light.<sup>163</sup> However, since only 8% of solar radiation is UV, there is a need to develop photocatalysts which can be activated predominantly by visible light (42% of solar radiation), especially if a surface is intended for environmental use with activation by sunlight.<sup>164</sup> The extent to which activation by sunlight is a relevant mechanism will depend on the intended application of TiO<sub>2</sub> nano-coatings; activation of antimicrobial properties by the ambient lighting on a hospital ward or similar environment would be highly beneficial.

The nature of the antimicrobial mechanism based on ROS production suggests that TiO<sub>2</sub> nano-coatings can be hostile to both bacterial cells and eukaryotes, limiting their use *in vivo*. Several studies have reported that TiO<sub>2</sub> NPs exhibit toxicity, including evidence of genotoxicity, in both light and dark conditions.<sup>165–168</sup> The production and toxicity of ROS are indiscriminate, and therefore there is a presumption that ROS are likely to damage all cells within the vicinity.<sup>163</sup> Despite this, TiO<sub>2</sub> nano-coatings have been investigated in a dental context, applied to orthodontic brackets.<sup>169</sup> Brackets coated with nitrogen-doped TiO<sub>2</sub> nanofilms were shown to cause significant CFU reductions over 90 days compared to uncoated brackets when tested with the oral pathogen *Streptococcus mutans*. To date, there is little robust evidence regarding safety of TiO<sub>2</sub> nano-coatings to oral cells, but additional research exposing eukaryotic cells to these coatings and their associated ROS, over relevant time periods, will be crucial prior to clinical testing. However, it should also be remembered that TiO<sub>2</sub> is already

heavily used as an additive (E171) in the food industry<sup>170</sup> as a mixture of micro- and nanosized particles for food coloring purposes. E171 has been found to induce ROS generation in a cell-free environment but not in exposed Caco-2 cells, induce single-strand DNA breaks and cause chromosome damage.<sup>171</sup> However, no acceptable daily intake is currently defined in the European Union (EU) due to TiO<sub>2</sub> bioavailability being found to be low and independent of particle size, the vast majority of TiO<sub>2</sub> being eliminated unchanged in feces, and a maximum of 0.1% being absorbed by gut-associated lymphoid tissue and distributed to organs.<sup>172</sup>

Equally important to the development of implanted biomaterials utilizing a TiO<sub>2</sub> photocatalytic surface is the longevity of antibacterial activity following cessation of UV irradiation. While environmental surfaces can be suitable for continuous or repeated photocatalytic activation where antibacterial effects are immediate but short-lived following cessation, this model may not be suitable for implanted biomaterials which are inaccessible. A nanocomposite of resin and TiO<sub>2</sub> NPs demonstrated detectable antibacterial effects for 30 min following cessation of UV irradiation.<sup>173</sup> The post-UV treatment effect was tested against five bacterial strains: *Escherichia coli*, *Staphylococcus epidermidis*, *Streptococcus pyogenes*, *Streptococcus mutans* and *Enterococcus faecalis*. Although UV treatment did not affect bacterial adhesion to coated specimens, the viability of bacteria was reduced by 37%. This finding is particularly relevant because the highest risk of bacterial colonization for implanted biomaterials is prior to or during implantation. Maintaining a UV-induced antibacterial effect for even 30 min following cessation of irradiation may allow enough time for implant surfaces to self-disinfect following implantation and reduce the possibility of biofilm development and subsequent infection, which can in certain cases result in implant failure.

**Aluminum Nano-coatings.** Aluminum oxide (Al<sub>2</sub>O<sub>3</sub>, also termed alumina) NPs have been shown to have some antimicrobial effects, albeit at very high concentrations (1000 μg mL<sup>-1</sup>) when tested against *Escherichia coli*.<sup>174</sup> It was postulated that while they exhibit toxicity to bacteria through surface charge interactions with cell membranes and walls, their free radical scavenging properties may limit intense antimicrobial action and disruption of the cell wall. Essentially, they may simultaneously exhibit antimicrobial properties by one mechanism while reducing that antimicrobial effect by another. A similar MIC in the range of 1700–3400 μg mL<sup>-1</sup> was reported for a multidrug-resistant strain of *Staphylococcus aureus*.<sup>175</sup> More recent work has demonstrated antibacterial activity at a concentration 1 order of magnitude lower (100 μg mL<sup>-1</sup>) against both *Escherichia coli* and *Staphylococcus aureus*.<sup>176</sup> The EC<sub>50</sub> (half maximal effective concentration) of Al<sub>2</sub>O<sub>3</sub> NPs against *Pseudomonas putida* has even been reported at 0.5 μg mL<sup>-1</sup> over 16 h.<sup>177</sup> The differences in values between these reports demonstrate the confounding factors of NP size, shape and synthesis method and suggest that they could be as important as concentration in terms of antimicrobial activity. Nevertheless, most studies investigate alumina NPs in the form of nanosolutions with very little evidence in the literature where they have been used as nano-coatings.

**Nonmetallic Nanomaterials. Carbon-Based Nano-coatings.** There are a number of unique carbon-based nanomaterials (CBNMs), primarily allotropes of carbon such as graphene, with intrinsic antimicrobial properties and distinct material properties which make them useful for a range of applications in



medicine and dentistry. A key property of CBNMs is their excellent biocompatibility, resulting in their testing in a range of biomedical applications including drug delivery, biosensor development, diagnostics and therapeutics.<sup>186</sup> The various types of CBNMs available, in addition to graphene, include single- and multiwalled carbon nanotubes, fullerenes, and nanodiamonds.<sup>187</sup>

**Graphene.** Graphene consists of a single layer of carbon atoms arranged hexagonally and is the base component of materials including carbon nanotubes (CNTs), diamond, charcoal, graphite, and fullerenes (collectively referred to as graphene-based materials, GBMs). GBMs have intrinsic antimicrobial properties and appear to exert stronger effects if presented as coatings.<sup>188</sup> Graphene can disrupt the bacterial cell membrane, most likely due to its physically sharp structure, interfering with the membrane potential and inducing membrane stress.<sup>189,190</sup>

While graphene in free-floating form exerts its bactericidal effect through both biomechanical interactions and ROS-mediated biochemical responses, surface-immobilization of graphene as a coating appears to limit the mechanism to primarily physical interactions causing cell membrane damage.<sup>191</sup> Superoxide ion-induced ROS production does not appear to occur; however, oxidative stress can be produced by oxidation of glutathione, a redox mediator in bacteria.<sup>192,193</sup> Like some other nanomaterials, the direct biomechanical mechanism of bactericidal activity offers the potential to be effective against drug-resistant pathogens, helping to protect surfaces from colonization. It has been suggested that graphene has antibacterial activity due to its ability to transfer electrons away from bacteria, as they maintain a negative resting membrane potential and require proper electron movement for the functioning of the respiratory chain.<sup>194</sup> As graphene is an excellent electron acceptor, physical contact between bacteria and graphene may be sufficient to cause the bacteria to steadily lose electrons, interrupting the electron transport chain and leading to bacterial cell death. This effect also depends on the properties of the underlying substrate, in particular the substrate's electrical conductivity.<sup>195</sup> Research into the use of GBMs as antimicrobial coatings is still at a comparatively early stage, with relatively few publications available compared to the other groups of nanomaterials presented in this review; however, multiple methods of GBM application to relevant substrates have been reported.

Graphene was applied in the form of immobilized graphene nanoplatelets (*i.e.*, stacked graphene sheets with thickness of 2–10 layers) to the surface of silicone rubber to offer antimicrobial protection against *Staphylococcus epidermidis*. Independent of application methodology, the oxidized form of graphene had augmented bactericidal properties versus the nonoxidized form which may be explained by additional exertion of oxidative stress and production of ROS, leading to lipid peroxidation, mitochondrial dysfunction and protein inactivation.<sup>196,197</sup>

Graphene nanoplatelets have also been applied by spray coating onto a segment of silicone catheter.<sup>198</sup> Spray coating has the advantage of simple adjustment of coating thickness by altering the number of passes of the nozzle over the sample surface. Dybowska et al.<sup>198</sup> found that the graphene nanoplatelet coating was an effective antibiofilm agent preventing mature biofilm formation. However, graphene nanoplatelets decorated with Ag NPs were found to be even more effective indicating possible graphene-nanosilver synergism.

Other studies have investigated the potentially higher antimicrobial efficacy of graphene oxide (GO) nanocoatings. GO coatings have been applied to a polymeric substrate by

immersion of plasma activated silicone films in a GO dispersion.<sup>199</sup> Both colony counting and live/dead assay results showed considerable antibacterial activity against *Escherichia coli* and *Staphylococcus aureus*, with stronger activity against the former. That study concluded that the majority of bactericidal activity was the result of oxidative stress mechanisms, rather than physical or mechanical cell damage, due to the “edge-free” nature of the coating. However, this would not seem to eliminate possible antibacterial mechanisms involving interruption of electron transport. In a different study, GO-coated surfaces were prepared by two different methods, and effective inhibition of biofilm formation was reported for both *Escherichia coli* and *Staphylococcus aureus*.<sup>131</sup> The synthesis method was a major factor affecting antibacterial efficacy, as different methods resulted in variations in functional groups present as well as nanosheet size, roughness, porosity, and thickness. These factors were significant as confirmed by the increased bacterial adhesion on the rougher nanocoating with less uniform thickness. In addition to GO coatings, reduced GO (rGO) coatings have been synthesized using the whole cell biomass of the fungus *Rhizopus oryzae*, coated on aluminum.<sup>200</sup> Both the GO and rGO coatings showed excellent bactericidal activity against *Escherichia coli* (72% and 93% respectively), although their activity was lower than that shown for the same nanomaterials in a dispersed phase (80% and 97%); potentially because immobilization as a coating prevented access of the nanomaterials to intracellular compartments. Findings regarding bactericidal activity of the coatings were confirmed by live/dead assay, which also revealed reduced bacterial adherence to the rGO coatings and suggested that its more hydrophobic nature prevented cell attachment in addition to direct bactericidal activity. These findings indicate that GO and its variants have impressive potential to be used as antimicrobial nanocoatings, combining relatively facile and eco-friendly synthesis with potent antibacterial and biocompatible properties.

**Carbon Nanotubes.** CNTs are forms of graphene arranged in a cylindrical structure and can be structured with a single wall (SWCNTs) or multiple walls (MWCNTs). The single versus multiwalled nature is one of the variable properties of CNTs, along with diameter, length, surface functionalization (*e.g.*, addition of chemical groups), and chirality. There is a strong evidence base to support the antibacterial properties of CNTs,<sup>201</sup> but only a few reports of applications as surface coatings. CNTs have been reported to be compatible with photodynamic antimicrobial chemotherapy, where light is used to activate or tune the antimicrobial effects. This approach has been shown to be effective against both *Staphylococcus aureus*<sup>202</sup> and *Escherichia coli*.<sup>203</sup> Antimicrobial and antibiofilm activity have been suggested to be the result of ROS generation which allows antimicrobial photodynamic inactivation via cell membrane damage.

Carbon nanotubes have been applied as an antimicrobial coating to paper, which can widen the range of surfaces that can be coated to protect against bacterial colonization and transmission in healthcare settings.<sup>204</sup> Direct interaction of bacteria with paper coated with acid functionalized SWCNTs for 1 h resulted in substantial morphological changes with loss of shape and integrity, explained by damaged cell walls leading to osmotic swelling. Both *Staphylococcus aureus* and *Escherichia coli* experienced these morphological changes, but those were more severe for *Staphylococcus aureus*; probably because of the greater rigidity of the *Escherichia coli* cell wall.

Table 2. Summary of Additional Selected Examples from the Published Literature Regarding Application of Nonmetallic Nanomaterials as Antimicrobial Nanocoatings

Nanocoating description	Aim of application	Key methods <sup>a</sup>	Target organisms	Key results <sup>a</sup>	Source
Dual layer cotton coated with chitosan nanofibers incorporating <i>Agrimonia eupatoria</i> extract	Therapeutic wound dressings	Agar slurries of bacteria spread on surfaces Slurries released and bacteria enumerated MTT used for <i>in vitro</i> cytotoxicity against human dermal fibroblasts	<i>Pseudomonas aeruginosa</i> , <i>Staphylococcus aureus</i>	Coatings with and without extract inhibited bacterial growth Inhibition was greater (>98%) in extract-containing group No cytotoxicity seen against human dermal fibroblasts	214
Graphene nanoplatelets incorporated in polyurethane by melt blending and dip coating	Catheters	Bacterial culture deposited on surfaces Nonadherent bacteria enumerated after 24 h Adherent bacteria visualized by FM Surfaces seeded with bacteria	<i>Staphylococcus epidermidis</i>	Dip-coated surfaces caused 30–100% decrease in metabolic activity and 57–82% decrease in viability Bactericidal activity upon contact not shown toward adherent or planktonic cells for melt blended samples	215
Composite of graphite nanoplatelets and low-density polyethylene produced with graphite nanoplatelets oriented in a controlled manner, exposed by etching	Antibacterial surfaces for biomedical devices	Bacteria enumerated after 24 h Surfaces investigated with SEM, live/dead and reactive oxygen staining and FM <i>In vitro</i> cytotoxicity evaluated against SH-SY5Y and HUH-7 cells	<i>Escherichia coli</i> , <i>Staphylococcus epidermidis</i>	Bactericidal activity against <i>S. epidermidis</i> (95%) and <i>E. coli</i> (90%) was dependent on nanoflake orientation and density - in one group viability loss was >99.99% for both bacteria Reduced bacterial adhesion and surface colonization seen with live/dead staining No toxicity against SH-SY5Y or HUH-7 cells	216
Graphene coating developed using a one-step laser-induced method	Antibacterial coatings for water robots	Samples placed on agar plates inoculated with bacteria followed by 10 min solar treatment Bacteria enumerated after 12 h SEM to visualize samples	<i>Escherichia coli</i>	>99.8% reduction in viable bacteria SEM showed no bacteria on graphene-coated glass samples but dense ones on untreated surfaces	217
Hydroxyapatite coating on titanium by microarc oxidation followed by loading of chitosan by dip-coating	Titanium implants	Surfaces seeded with bacteria and enumerated after 24 h Agar diffusion and UV spectrophotometry Biocompatibility and osteogenic properties evaluated with MC3T3-E1 cells Bacterial viability quantified following surface contact	<i>Escherichia coli</i>	Up to 65% antibacterial activity demonstrated and improved with increasing chitosan but decreased over time No cytotoxicity or morphology differences found Cells proliferated faster on surfaces lacking chitosan and cell numbers decreased as chitosan content increased Antibacterial activity of >36% demonstrated and improved with chitosan and alginate	218
Titanium implants coated with chitosan and alginate by spin coating	Titanium implants	<i>In vitro</i> cytotoxicity against L929 fibroblasts Bacterial cultures filtered through GO-modified membranes Cell morphology observed by SEM Surfaces seeded with bacterial suspensions for biofilm assays CVSA quantification after 24 h	<i>Escherichia coli</i> , <i>Staphylococcus aureus</i>	No cytotoxicity and biocompatibility demonstrated >70% bactericidal activity against both target bacteria with effects increasing over time Bactericidal activity <i>S. aureus</i> $\gg$ <i>E. coli</i> SEM showed bacteria on coated membranes had compromised cellular integrity Reduced biofilm biomass on coated versus uncoated membranes	219
Graphene oxide (GO) applied to polyvinylidene fluoride by vacuum filtration	Antibiofouling coatings in wastewater treatment technologies	Immersion in bacterial culture and adhered cells enumerated after 24 h Fixed samples viewed with SEM	<i>Escherichia coli</i> , <i>Staphylococcus aureus</i>	Changes in morphology and suppressed colonization for <i>E. coli</i> by 54–77% but not for <i>S. aureus</i> GO coating may enhance cytocompatibility as osteogenesis markers upregulated	220
GO applied to polyetheretherketone by dipping method	Bioactive implant material for bone tissue engineering	CCK-8 kit and CLSM for <i>in vitro</i> cytotoxicity toward human osteoblast-like MG-63 cells	<i>Escherichia coli</i> , <i>Staphylococcus aureus</i>	No GO leaching detected Reduced adhesion of <i>S. aureus</i> (86%) and <i>P. aeruginosa</i> (64%)	221
Polycarbonate urethane was coated with a thin film of GO	Medical implants	Immersion in bacterial culture and adhered cells enumerated after 24 h GO leaching and hemolysis (ISO 10993-4) measured	<i>Pseudomonas aeruginosa</i> , <i>Staphylococcus aureus</i>		222

Table 2. continued

Nanocoating description	Aim of application	Key methods <sup>a</sup>	Target organisms	Key results <sup>a</sup>	Source
GO-coated surfaces were prepared by Hummers' method and an "improved" method	Antimicrobial surface coatings for biomedical applications	<i>In vitro</i> adhesion and proliferation measured with L929 fibroblasts by FM and MTT assay Immersion in bacterial culture for 24 h with viable cell enumeration Biofilm assays in GO plated 96 well plates CVSA and microscopic visualization and quantification after 24 h	<i>Escherichia coli</i> , <i>Staphylococcus aureus</i>	GO coating induced hemolysis more than controls (0.055% vs 0.02%), but was <5% (ISO 10993-4) L929 cell proliferation unaffected compared to control Antibacterial activity seen in all treatment groups Smoother surface in "improved" method—fewer pores and less <i>E. coli</i> biofilm inhibition Increasing GO content increased <i>E. coli</i> biofilm inhibition by up to 150% but not <i>S. aureus</i> , remaining around 75%	223

<sup>a</sup>CVSA: crystal violet solubilization assay; CLSM: confocal laser scanning microscopy; SEM: scanning electron microscopy; FM: fluorescence microscopy; UV: ultraviolet; MTT: 3-(4,5-dimethylthiazol-2-yl)-2,5-diphenyltetrazolium bromide; CCK: cell counting kit.

The mechanical properties of CNTs can also be useful in producing an antibacterial effect. Vertically aligned carbon nanotubes (VACNTs) have a very high aspect ratio with extreme flexibility, meaning that they deform in contact with bacteria before releasing their stored elastic energy. Arrays or "forests" of VACNTs with gaps smaller than the size of bacterial cells have been found to have potent bactericidal activity against *Pseudomonas aeruginosa* and *Staphylococcus aureus*.<sup>82</sup> The proposed mechanism of action involves CNTs retracting and stretching in response to cell attachment, with release of the stored elastic energy resulting in tearing of the adsorbed bacterial cell. This mechanical killing mechanism is an attractive complement to other mechanisms involving oxidative stress or disruption of biomolecules, with the additional benefit of killing both Gram positive and Gram-negative bacteria.

**Silica Nanocoatings.** Silica nanoparticles (SiO<sub>2</sub> NPs) have exhibited potent antibacterial effects expressed by high killing efficacy (>99%) against *Pseudomonas aeruginosa* and *Escherichia coli* biofilms, while demonstrating good clinical biocompatibility by inhibiting fibroblast proliferation less than conventional antiseptics.<sup>205</sup> Attachment of SiO<sub>2</sub> NPs to tissue culture polystyrene has been shown to reduce the attachment and growth of *Candida albicans*,<sup>206</sup> and SiO<sub>2</sub> NPs have also been found to be useful as abrasives for tooth polishing when tested on human teeth *ex vivo*.<sup>207</sup>

SiO<sub>2</sub> NPs have been deposited as a coating on titanium substrates by an electrophoretic-enhanced microarc oxidation technique and tested against *Staphylococcus aureus* and *Escherichia coli*.<sup>81</sup> The coated substrate showed slightly reduced bacterial growth, but cell morphology was the same when compared to uncoated substrates. Results showed that coated surfaces slightly inhibited bacterial adhesion and growth, but this effect was greatly enhanced by addition of octenidine, a cationic surfactant and antiseptic. The authors attributed the antibacterial properties of the SiO<sub>2</sub> coating without octenidine to the highly porous structure of the surface, suggesting that bacteria became physically trapped which resulted in restricted movement and proliferation. This is analogous to the "trap-killing" previously reported against *Staphylococcus aureus* on Ag nanocoatings applied to titanium.<sup>208</sup>

Coatings of SiO<sub>2</sub> NPs have been applied to tiles and tested for antifungal activity against *Acremonium kiliense*, *Acremonium strictum*, and *Fusarium solani*. Measurements of the fungal growth showed a reduction by 27.5%, 21.5% and 37.5%, respectively.<sup>209</sup> Antifungal activity was also found to be higher for silica–titania core–shell NPs when compared to pure SiO<sub>2</sub> NPs, suggesting that it was the layer of titania enhancing their antimicrobial performance.

**Chitosan Nanocoatings.** Chitosan is a polycationic polymer obtained commercially from shrimp and crab shell chitin by alkaline deacetylation, usually by sodium hydroxide.<sup>210</sup> Both chitin and chitosan are biocompatible, biodegradable and nontoxic, though chitosan is favored due to its higher solubility and enhanced antimicrobial activity.<sup>211</sup>


A hybrid nanomaterial incorporating chitosan and silica was applied to the surface of titanium implants and tested as an antibacterial coating.<sup>212</sup> Chitosan was the intended antibacterial component, whereas silica was selected for its osteogenic properties. The nanocoating was synthesized following the sol–gel process with chitosan covalently bonded to the silica network. Work using human fibroblasts demonstrated that the hybrid nanocoating was not cytotoxic, and cell proliferation was supported on the nanocoated surfaces, suggesting good



Table 3. Summary of Additional Selected Examples from the Published Literature Regarding Surface Nanotopography Modifications Acting as Antimicrobial Nanocoatings

Nanocoating description	Aim of application	Key methods <sup>a</sup>	Target organisms	Key results	Source
Titanium/mica/glass surfaces modified using self-assembling nanostructures composed of fluorinated phenylalanine	Biofilm control for biomedicine	Immersion in bacterial suspension after 24 h	<i>Enterococcus faecalis</i>	Viability (ATP production) reduced for <i>E. faecalis</i> (94%) and <i>S. mutans</i> (99%)	252
A one-step etching technique was used to render aluminum alloys with micro- and nanoscale roughness	Engineered surfaces to minimize the spread of nosocomial pathogens	ATP luminescence assay for viability after 24 h SEM to visualize biofilms Immersion in bacterial suspension	<i>Streptococcus mutans</i>	Reduced bacterial adherence and metabolism affected	
Metal organic framework nanodagger arrays	Safe and clean antimicrobial surfaces for medical devices	After 4 h, nonadherent cells removed and samples incubated in broth SEM and live/dead staining with CLSM used to visualize bacteria after 20 h Surfaces seeded with microbial suspensions Attached microbes enumerated after 18 h Surfaces live/dead stained for visualization SEM to observe morphological changes	<i>Escherichia coli</i> <i>Staphylococcus aureus</i> "Nosocomial pathogens" recovered from patients <i>Escherichia coli</i> <i>Staphylococcus aureus</i> <i>Candida albicans</i>	97% lysis of adherent <i>E. coli</i> within 30 min 28% kill of <i>S. aureus</i> attached to engineered surface versus 3% on control surfaces Disrupted morphology and >80% cell lysis for <i>P. aeruginosa</i> and <i>E. coli</i> , 25% for <i>K. pneumoniae</i> Log reductions in viability for <i>E. coli</i> (7 log) <i>S. aureus</i> (8) and <i>Candida albicans</i> (4) Good surface durability (for <i>E. coli</i> ) over 2 months with no growth on treated surface vs 4 log on controls	253
Nanostructure arrays assembled from fatty acids assembled on graphite surfaces	Mechanobactericidal surfaces not requiring use of antibacterial chemicals	Immersion in bacterial suspension Aliquots taken for enumeration after 1, 3, and 6 h Adherent cells visualized with live/dead stain and CLSM after 18 h	<i>Pseudomonas aeruginosa</i> <i>Staphylococcus aureus</i>	>90% antibacterial activity against <i>P. aeruginosa</i> 73→95% activity against <i>S. aureus</i>	130
Diamond nanocoating arrays fabricated by microwave plasma chemical vapor deposition then bias-assisted reactive ion etching	Biomaterials to reduce medical device-associated infections	Immersion in bacterial suspension Adherent cells visualized with live/dead stain after 1 h SEM for unstained surfaces	<i>Pseudomonas aeruginosa</i>	>90% of both bacterial species killed after 6 h in contact assays High proportions of cells with damaged membranes on nanopatterned surfaces Bacteria viewed in many orientations on nanopatterned surfaces—only horizontal on control surfaces	255

<sup>a</sup>ATP: adenosine triphosphate; SEM: scanning electron microscopy; CLSM: confocal laser scanning microscopy.

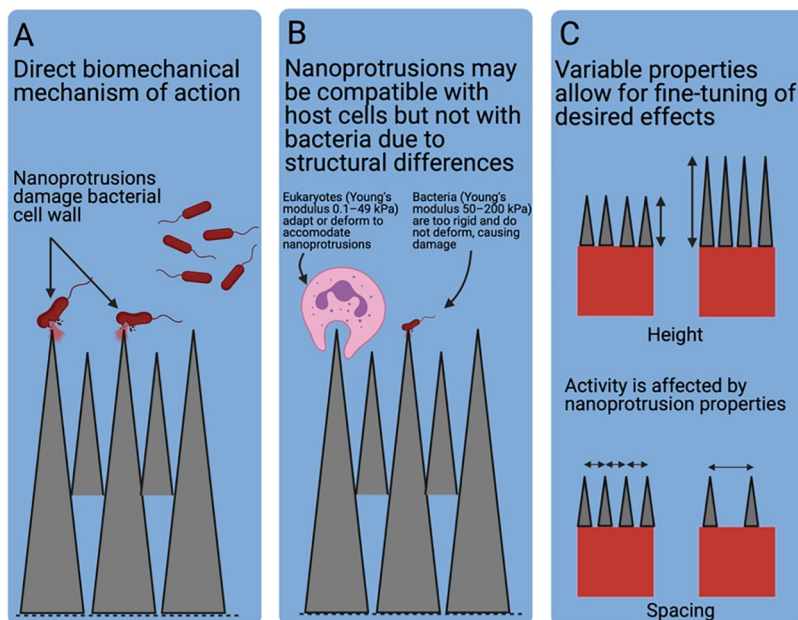

**Figure 5.** Advantages of nanoprotusions and their potential to be fine-tuned. The direct biomechanical mechanism of action (A) of nanoprotusions avoids possible concerns regarding resistance to antimicrobial agents, however the surfaces can be designed to be compatible with host cells while hostile to bacteria due to cellular structural differences as quantified by Young's modulus (B). The antimicrobial and biocompatible properties of nanoprotusions can be fine-tuned by modifying certain variables such as nanoprotusion height and spacing (C). Features of graphic not to scale. Figure was created using [BioRender.com](https://www.bio-render.com/).

biocompatibility. Significant antibacterial performance against *Staphylococcus aureus* was demonstrated for 5–10% chitosan, with antibacterial activity increasing with chitosan content. It is important to be aware of the hydrophilicity or hydrophobicity of any nanocoating, as this can impact directly upon interactions with the biological environment and dictate cell attachment.<sup>213</sup> Palla-Rubio et al.<sup>212</sup> found that adding chitosan decreased hydrophilicity of the coatings and reported contact angles for optimal biological interactions from 60 to 80°.

**Surface Nanotopography.** Modification of surface nanotopography has been explored as an alternative antibiofilm strategy to the application of nanocoatings (Table 3). Certain nanotopography features, such as nanospikes or other controlled surface patterns, have been found to either hinder bacterial adherence or cause cell death by physically damaging the structure of the bacterial cell wall<sup>224,225</sup> as well as by inhibiting cell division or by causing oxidative stress.<sup>226</sup> The main advantage of this approach is that there are no biologically or chemically active substances involved that may leach from the surface over time, potentially causing local tissue or environmental toxicity and leading to long-term reduction or loss of antimicrobial efficacy. However, it is possible that nanopatterned surfaces may still become damaged following environmental exposure (e.g., corrosion, abrasion), or nanotopographical details become masked by contaminants in the immediate environment. A natural buildup of biomolecules could potentially occlude the surface nanotopography and even enhance microbial adhesion; akin to the formation of a “conditioning film” which forms on abiotic surfaces upon contact with biological fluids containing proteins and polysaccharides and facilitates attachment of biofilm-forming cells.<sup>227</sup> An additional caveat of modifying the surface nanotopography is the effect on biocompatibility. It is generally anticipated that rendering a surface inhospitable to bacteria by modifying its physical nanotopography would also affect the

ability of eukaryotic cells to adhere and proliferate; a major issue for medical implants where the surface needs to be nontoxic while allowing integration with the adjacent host tissues. Some studies have reported that topographical features can affect immune cell function, raising questions about the indirect effect on biocompatibility and long-term host integration in addition to the more immediate effects on host cells. The morphology and spatial orientation of macrophages, key innate phagocytic cells with roles in determining downstream immune responses, are affected by topography and this may affect macrophage differentiation and the type and level of cytokine secretion. This suggests that physical cues, including surface topography, could modulate differentiation toward M1 (proinflammatory) or M2 (pro-healing/homeostatic) phenotypes.<sup>228,229</sup> While this suggests that nanotopographical modifications should be applied with care, it could also present an opportunity for surfaces to be designed to stimulate a desired anti-inflammatory and pro-healing environment and thereby improve biomaterial integration.

It should be noted that some of the terminology in this area is not well-defined or standardized, with different publications describing types of nanostructures in different ways (e.g., nanopillars, nanoneedles, nanospikes, nanocones). Due to this potential ambiguity, the more general term “nanoprotusions” is used in this review.

**The Role of Surface Roughness.** There is general acceptance of the idea that bacteria are more likely to adhere to rougher surfaces due to the increased contact area, as well as the defects in the surface (pits, bumps or troughs) which provide protection from shear forces or contact abrasion with other surfaces (see review by Crawford et al.<sup>230</sup>). This has led to a common belief that smoother surfaces will reduce bacterial adhesion and so are the best strategy for inhibition of biofilm formation.<sup>231</sup> However, a certain degree of nuance should be considered as there is some conflicting data from a range of studies which collectively find

that surface roughness alone is not a good predictor of bacterial adhesion or colonization. Previous conclusions concerning surface roughness and bacterial adhesion have often failed to take into account bacterial appendages such as flagella which are able to aid in attachment by reaching crevices much smaller than the bacterial cells themselves<sup>232</sup> (evidence reviewed by Mi et al.<sup>233</sup>). It could be that smoother surfaces are indeed more hostile surfaces for adhesion, but due to the very small size of these appendages, surfaces must be far smoother with fewer nanoscale defects than previously considered. Other factors such as surface free energy, wettability/hydrophobicity, surface chemistry and phenotypic differences between bacteria should also be considered central to affecting the likelihood of successful adhesion.<sup>234</sup> There is also a dilemma for the development of surfaces intended for implantation *in vivo*; a roughness of 1–2  $\mu\text{m}$  is deemed necessary for osseointegration and the long-term success of the implant.<sup>235</sup> The relationship between surface characteristics or topography and biofilm development has been reviewed in detail by Teughels et al.<sup>236</sup>

**Nanoprotrusions.** Surfaces can be modified to have physical protrusions on the nanoscale similar to those observed in nature, for example on insect wings (cicada and dragonfly) and indeed natural nanotopography has been the inspiration for a number of biomimetic engineered surface modifications.<sup>237</sup> These surfaces exert antimicrobial activity by direct biomechanical disruption of bacterial structures such as the cell wall or envelope<sup>238</sup> by penetrating bacterial cell walls and causing irreversible cell damage (Figure 5A). Additionally, shear forces induced when bacteria move laterally relative to the nanoprotrusions increase the damage to the cell wall, also resulting in antimicrobial activity.<sup>239</sup> The activity and specificity of nanoprotrusions may be dictated by their spacing and width (Figure 5C). In terms of bacterial variables, antimicrobial efficacy is thought to depend on cell shape and cell wall rigidity.<sup>240</sup> Evidence suggests that the rigidity or stiffness of bacterial cell walls is significantly greater than that of eukaryotic cell membranes, with the Young's modulus (a measure of resistance to elastic deformation where larger numbers indicate increased stiffness) of human mesenchymal stem cells in the region of 0.09–49 kPa compared to 50–200 kPa for certain bacterial cell envelopes, though it should be noted that these values are affected by cell type and viability or membrane integrity.<sup>241,242</sup> This difference in cell wall rigidity between eukaryotes and prokaryotes could explain why some nanostructured surfaces facilitate eukaryotic cell proliferation but result in cell death for bacteria (Figure 5B). Eukaryotic cells have been shown to be able to stretch and distort to accommodate the shape of nanostructures, either growing around them or sitting on top and distorting to accommodate their shape, thereby avoiding membrane damage and cell death.<sup>243</sup> When exposed to nanostructured surfaces, flexibility and adaptability appear to be superior to a rigid or stiff structure. Within prokaryotes, it has also been reported that Gram-negative bacteria are more susceptible to killing by nanopatterned structures such as cicada wings, with Gram positive bacteria showing greater resistance, presumably due to their thicker cell wall and differences in rigidity.<sup>225</sup>

Arrays of  $\text{TiO}_2$  nanowires have been shown to be selectively bactericidal against *Pseudomonas aeruginosa* with no activity against *Staphylococcus aureus*.<sup>244</sup> Although this may be partly explained by the previous points regarding Gram-negative bacterial cell wall thickness, Diu et al.<sup>244</sup> suggested that bacterial motility may also be associated with stronger bactericidal effects. Upon investigation with a panel of Gram positive and Gram-

negative bacteria, significantly higher bactericidal activity was indeed found against motile versus nonmotile bacteria. Antimicrobial efficacy against *Staphylococcus aureus* has also been shown by using gold<sup>245</sup> and titanium<sup>246</sup> nanoprotusions.

**Black Silicon.** Black silicon, a surface-modified variant of silicon produced by reactive-ion etching techniques, has been shown to kill a variety of bacteria (both Gram positive and Gram-negative) and endospores by surface contact.<sup>225</sup> Nanoprotrusions of black silicon are sharper, more distinct, and approximately double the height of those found on a dragonfly wing. The high bactericidal efficiency of black silicon was particularly noteworthy, with a reported killing rate of  $\sim 450,000$  cells  $\text{min}^{-1} \text{cm}^{-2}$ . Combining this evidence with known minimum infective doses (MIDs) for certain bacteria, one may conclude that 1  $\text{cm}^2$  of black silicon could be capable of killing the MID of *Staphylococcus aureus* 810 times or that of *Pseudomonas aeruginosa* 77,400 times over 3 h. However, black silicon may not be as efficient against spores since it has been found that it was not able to kill or rupture dormant spores of *Bacillus subtilis*, *Bacillus cereus* or *Bacillus megaterium*, although germinated *Bacillus subtilis* spores were rapidly killed.<sup>225</sup> This lends insight into the possible limits of mechanical bactericidal approaches.<sup>247</sup> The efficacy of black silicon surfaces against *Escherichia coli* has also been confirmed, with nanoprotrusion density reported to be more important than length. Interestingly, *Streptococcus gordonii* was unaffected by the surfaces; most likely due to its small size, thicker cell wall and/or lack of motility leading to less lateral movement.<sup>248</sup> This highlights that antimicrobial effects are dependent on microbe properties, and it is unlikely that any nanocoating will be effective against all microorganisms, all the time. Regarding different properties such as nanoprotrusion height, density and aspect ratio, one study found that three black silicon surfaces with apparently similar nanoarchitecture had different bactericidal efficiencies against different bacteria, though no single variable could be directly correlated with bactericidal efficiency.<sup>249</sup> This suggests that the variations in properties affecting bactericidal efficiency are subtle, making it difficult to reach a conclusion regarding the best nanotopography for antibacterial properties, and demonstrating that further investigation is needed.

Available data suggest that black silicon may be best suited for use in antimicrobial nanocoatings on unimplanted materials but not *in vivo*, due to its reported ability to rupture mammalian cells (e.g., mouse osteoblasts).<sup>250</sup> This is in contrast to another study showing that black silicon favored the proliferation of eukaryotic cells (*Cercopithecus aethiops* kidney fibroblast-like cells) without eliciting a host inflammatory response *in vivo* in mice.<sup>251</sup> Clearly there is need for further research on the biocompatibility of black silicon as it is possible that it may be specific to certain types of eukaryotic cells used, test conditions or specific properties of the surface.

**Nanocomposites.** A composite can broadly be defined as a “multicomponent material comprising multiple different phase domains in which at least one phase domain is a continuous phase”,<sup>256</sup> and these domains are combined to achieve properties not exhibited by any single constituent part.<sup>257</sup> In the case of nanocomposites, the same definition applies, but at least one of the phases has one dimension at the nanoscale ( $<100$  nm).<sup>256,258</sup> Generally, antimicrobial nanocomposites tend to take the form of biomaterials with a structural matrix phase, such as a polymer, and antimicrobial NPs (dispersed phase) acting as a filler within that matrix. Thus, biomaterials



Table 4. Summary of Additional Selected Examples from the Published Literature Regarding Application of Nanocomposites as Antimicrobial Nanocoatings

Nanocoating description	Aim of application	Key methods	Target organisms	Key results	Source
Dental resin with 70% Bis-GMA and 30% TEGDMA with SiO <sub>2</sub> and different proportions by weight of MgO NPs	Photocurable dental resin composite with antibacterial properties	Samples seeded with bacterial suspension Viable counts performed on bacteria liberated from samples into saline after 16–18 h	<i>Streptococcus mutans</i>	Antibacterial activity correlated with proportion of MgO NPs - 1% MgO NP reduced viability by 67.7% and 4% MgO NP by 99.4%	267
A composite dental resin modified by incorporation of TiO <sub>2</sub> NPs or a TiO <sub>2</sub> /Ag nanocomposite	Antibacterial dental restorative material	Immersion in bacterial suspension for 1 h and further broth added Nonadherent cells enumerated after 18 h  Biofilm established by immersion for 7 days	<i>Streptococcus mutans</i>	0.5%, 1% and 2% TiO <sub>2</sub> and 1% and 2% TiO <sub>2</sub> /Ag NPs significantly inhibited bacterial growth 2% TiO <sub>2</sub> and TiO <sub>2</sub> /Ag NPs significantly reduced biofilm formation	268
ZnO quantum dots incorporated into hydroxyethyl methacrylate and mixed with Bis-GMA	Antimicrobial adhesive resins for application in tooth restoration	Adherent cells enumerated Immersion in bacterial suspension Adherent cells enumerated after 24 h Cytotoxicity evaluated against human fibroblasts	<i>Streptococcus mutans</i>	2.16 log reduction in biofilm in treated samples No cytotoxicity observed	269
Transbond XT pastes prepared with 1%, 5% and 10% hydroxyapatite/Ag NPs. Resins light-cured for 20 s from each side	Modified orthodontic adhesives to reduce development of caries	Immersion in bacterial suspension Adherent cells enumerated after 72 h	<i>Lactobacillus acidophilus</i> <i>Streptococcus mutans</i> <i>Streptococcus sanguinis</i>	>50% reduction in biofilm formation for all bacteria Leaching demonstrated, causing dose-dependent loss of bacterial viability	270
Ag NPs and amorphous calcium phosphate NPs incorporated into the Scotchbond multipurpose bonding system	Dental adhesives with antibacterial properties to reduce development of caries	Aliquots of leached components inoculated with bacterial Viable cells enumerated after 24 h Dental plaque microcosm model Immersion in saliva combined with broth Live/dead staining and enumeration of adherent cells after 2 days Metabolic activity (MTT assay) and lactic acid production measured	Saliva microbes from healthy donors	Damaged bacteria in treatment group and >50% less live staining vs controls Significant reduction of biofilms vs controls 50% reduction in cell viability (MTT) and lactic acid production vs controls	271
Orthodontic composite paste blended with TiO <sub>2</sub> NPs	Antibacterial orthodontic composites	Immersion in bacterial suspension Viable cells enumerated after 48 h	<i>Streptococcus mutans</i>	>8-fold lower bacterial recovery from experimental specimens versus controls Antibacterial effect lasted 30 days after curing	272

already in use can be modified to incorporate NPs which confer an antimicrobial effect (Table 4).

An example of a nanocomposite is the incorporation of Ag NPs in poly(lactic-co-glycolic acid) (PLGA) grafts, conferring antibacterial properties against an antibiotic-resistant strain of *Staphylococcus aureus* and showing good biocompatibility with MC3T3-E1 preosteoblasts.<sup>259</sup> This antimicrobial nanocomposite graft was intended for use to improve healing of infected bone defects, and results with infected femoral defects in rats showed greatly improved healing within 12 weeks without evidence of residual bacteria, compared to control grafts which failed to heal in the continued presence of bacteria. Similarly, selenium NPs have been immobilized within PLGA and used to coat bone scaffolds. These materials with a nanocomposite selenium NP-PLGA coating showed antibacterial activity against *Staphylococcus aureus* and *Staphylococcus epidermidis*, and thus offer a potential antibacterial scaffold coating material for use in bone tissue engineering.<sup>260</sup>

The use of composites is common in dentistry due to favorable esthetics and longevity, and their strength and toughness comparable to dental amalgams.<sup>261,262</sup> This popularity and the relevance of antibacterial activity and tissue integration to dentistry make dental composites ideal candidates for the inclusion of antimicrobial NPs as fillers. A resin-based dental material incorporating a AgBr/cationic polymer nanocomposite was found to have potent bactericidal activity against *Streptococcus mutans*, a relevant oral pathogen, preventing biofilm formation.<sup>263</sup> Cytotoxicity measured against macrophages was found to be close to that of unmodified resins. Furthermore, the addition of the nanoparticles to the matrix increased the Vickers hardness of the resins, whereas it did not adversely affect their flexural strength. The combination of antimicrobial properties, host biocompatibility and favorable mechanical properties is essential for the development of an effective antimicrobial dental nanocomposite.

Other studies have reported similar success with the modification of dental resins with nanomaterials for improved antibacterial properties and biocompatibility. PMMA has been mixed with modified cellulose nanocrystals decorated with Ag NPs to improve mechanical properties and provide antibacterial activity against *Staphylococcus aureus* and *Escherichia coli*, while causing almost no toxicity to L929 fibroblasts.<sup>264</sup> PMMA modified with TiO<sub>2</sub> NPs has also been shown to inhibit the growth of *Candida scottii*,<sup>265</sup> and PMMA incorporating CuO and TiO<sub>2</sub> NPs showed significant antimicrobial activity against *Streptococcus salivarius*, *Streptococcus sanguinis*, and *Candida dubliniensis*, while some groups were also active against *Streptococcus mutans*. However, TiO<sub>2</sub> experimental groups did not show antimicrobial activity against *Streptococcus mutans*.<sup>266</sup>

## SAFETY OF MEDICINES AND MEDICAL DEVICES CONTAINING NANOCOATINGS

**The Safety of Patients.** The regulatory procedures for approving new nanomedicines and medical devices have been extensively discussed.<sup>273–276</sup> The pathways and regulations for approving a nanomedicine are generally the same as any other type of medicine. Indeed, the concern from the scientific community is that more nanospecific guidance is needed to smooth the regulatory process along in a safe way that accounts for the novel behaviors and properties of ENMs.<sup>273,275</sup> Briefly, in the EU, any medicine intended for human use will undergo clinical trials for safety and efficacy according to the Clinical Trials Directive (Directive 2001/20/EC) which sets out the

implementation of good clinical practice for such trials, and various codes relating to medicinal products for humans (e.g., Directive 2004/27/EC). Furthermore, regulation EC number 726/2004 indicates the procedure for the authorization and supervision of medicinal products, and this also established the European Medicines Agency (EMA) as an organization with oversight of national level authorities within Europe (Regulation (EC) no. 26/2004). Currently, the EMA offers no overarching guidance on nanospecific issues within those regulations. However, pragmatically, one might also argue that adding to the regulation every time a new type of medicine came along would soon make a cumbersome and unworkable process, and it is for the clinical trial to tease out the substance-specific safety concerns. In the United States, the FDA provides federal regulations on the safety of medicines (e.g., Federal Regulations 21). In 2017, the FDA issued some draft guidance on nanomaterials in drugs and biological products,<sup>277</sup> but similar to Europe and globally, nanospecific guidance is still being developed. Nonetheless, regardless of geographical location or jurisdiction, the key principles in the safety of medicines should apply. These include demonstrating that the new product is effective for its intended clinical use or more effective than the existing medicine or medical device, and it must be safe for the patient.<sup>273</sup>

In the case of dentistry, in the EU, Annex I of the Medical Devices Directive 93/42/EC traditionally identified requirements on the use of devices that could include dentures and dental implants. This was one part of several pieces of regulation, and for simplicity, these were repealed in 2017 in favor of a more streamlined document (Regulation (EU) 2017/745). The transition period to the new regulation is now complete, and Directive 2017/745 has been mandatory since May 2021. In the UK, following Brexit, the Medicines and Healthcare products Regulatory Agency (MHRA) retained responsibility for medical devices, including those with dental applications under the Medical Devices Regulations 2002<sup>278</sup> and its amendments, which essentially implements the EU directives. In the United States, the FDA has responsibility for medical devices, and there are a series of steps necessary to bring a product to market, and new devices should be registered with the FDA, undergo premarket safety screening, etc. Most of the regulation is detailed in the FDA's 'Title 21 Code of Federal Regulation (CFR), parts 800–1299'.<sup>279</sup> Again, all these regulations are intended to be generic and there is no guidance specifically on medical devices containing ENMs, antimicrobials, or other chemical substances. The intended use is a crucial aspect in deciding which regulations need to be followed. So, for example, an ENM coated with an antimicrobial substance might be considered as an antimicrobial drug if it was given systemically or orally, but the same composite material would be considered a medical device if it was part of a dental implant. There are some difficulties in this approach to regulation, for example, where the nanocoating is bioactive and therefore might be both a drug and part of a medical device.

Nonetheless, such regulations ensure that nanosafety can be addressed before a nanomedicine or medical device becomes available for clinical use. Risk is essentially a function of both the type of exposure and the hazard (toxicity), and there are now numerous reviews of the toxicity of ENMs.<sup>107,280–285</sup> For patients, the route of exposure is defined by the intended treatment method (oral, topical, injection to systemic circulation, etc.) and the cumulative dose will be a function of ENM concentration in the medicine, its bioavailability, and the

treatment duration. The concern for antimicrobial nanomedicines is that the biocidal component of the material might also be toxic to human cells or tissue. For antimicrobial ENMs made from nutritionally required metals such as zinc or copper, there may be less concern for health because these metals are already in the human body and are homeostatically regulated. However, this is not the case for ENMs made of nonessential toxic metals such as Ag NPs, where the concern is for potential hazard to the internal organs of the patient and/or long-term bioaccumulation. The challenge is to find an effective dose that has the desired antimicrobial effect without causing harm to the surrounding tissue, and in the case of silver, that is certainly possible.<sup>104,286</sup> The durability of the coating is also a toxicological concern. For example, whether an organic polymer or carbon-based coating could be metabolized to toxic metabolites, but this problem is no different from many traditional medicines that are degraded, and this would be identified in pharmacokinetic studies in Phase 0 clinical trials (animal studies). In other circumstances, it may be desirable for the surface coating to slowly dissolve to release an active biocide (e.g., slow release of silver ions from Ag NPs). This approach is fine provided that the dissolution kinetics of the material are well-defined in the intended tissue or body fluid, thus enabling some understanding of the possible hazard.

For medical devices, the safety concerns are around the use of the device and the effect that may have on the patient. However, for items such as medical instruments or implants, the surgical risks of the operation itself might be similar if the item was nanoenhanced or not. Crucially, the antimicrobial nanocoating on a medical implant would help to minimize the risk of postoperative infection from the wound site, since the biocidal properties of the material would persist after the wound is closed. Similarly, instruments and other devices with antimicrobial coatings would be less likely to introduce infection in the first place. However, the use of surgical disinfectants such as iodine or chlorhexidine should continue since the risk of side effect such as inflammation or dermatitis from the disinfectant is tiny (<1%)<sup>287</sup> and the relative risks of similar effects from nanocoatings on medical devices will remain unclear until a substantial data set has been collected on use in patients.

In terms of the safety regulations, antimicrobial nanocoatings have some potential advantages over traditional antibiotics. First, there is an assumption that the problem of antibiotic resistance would be less likely to arise from ENMs, and there is evidence that ENMs can tackle antibiotic resistant infections.<sup>288</sup> Second, nanocoatings have the potential to give persistent antimicrobial activity after surgery, at a time when the postoperative benefits of traditional antibiotics are in doubt.<sup>289</sup> Finally, many of the antimicrobial nanocoatings can be made of substances that already occur naturally in the human body (zinc, copper) or are part of our diet (e.g., chitosan from shellfish). Thus, there would be less concerns for risk assessment compared to an entirely foreign chemical that is not normally found in the body. However, a quantitative systematic risk analysis comparing antibiotics with ENMs in patient care has not yet been done and the benefits should be weighed against the risks. For example, we may need to be cautious with the use of metallic nanocoatings as antimicrobials because microbes often have genes associated with antibiotic resistance and metal homeostasis on the same plasmid, and there is evidence of metallic ENMs promoting the transfer of antibiotic resistance to other microbes in ecosystems.<sup>290</sup> There are also theoretical concerns that ENMs in the particulate form may be seen as antigens by the

immune system,<sup>291</sup> although this has not been substantiated in patients, and in any case, adverse effects on immunity or acute inflammation reactions should be detected in early clinical trials before a product comes to market. The schemes that allow clinicians to report the adverse side effects of approved medicines are also not nano-specific. For example, it is not possible to search the MHRA database ('yellow card scheme')<sup>292</sup> for "nanomaterials" as all substances are listed by their brand names. Similarly, the FDA Adverse Event Reporting System and the 'EudraVigilance' reporting scheme in the EU both use brand names. In any event, of those nanomedicines approved so far, very few, if any, are based on a coating-mediated effect.<sup>293</sup>

**Occupation Exposure of the Practitioner.** In the workplace, safe systems of work are intended to prevent exposure so that there is negligible risk to employees. This approach is used for all new chemicals including ENMs.<sup>294–296</sup> Potential exposure of the practitioner (e.g., medical doctor, nursing staff, dentist, etc.) could arise from incidental inhalation or ingestion of the ENM, or dermal contact. Of course, the usual practice of wearing surgical gloves, a face mask, not eating or drinking while treating patients should minimize these exposure routes. The health concerns for the practitioner would include contact dermatitis caused by handling the novel antimicrobial, the effects of accidental/incidental ingestion or respiratory exposure on health, especially with repeated doses over the working week or longer. These are concerns that apply to all substances in the clinical workplace, but there are some nanospecific issues around setting occupational exposure limits (OELs) for ENMs.<sup>296</sup> First, uncertainties in the exposure scenario (e.g., exactly how the ENM behaves in aerosols during use, etc.) and the bioavailable dose of ENMs have led to the use of a wide range of extrapolation factors, and therefore a broad range of suggested OELs, even for the same material.<sup>296</sup> Furthermore, most of the OEL studies to date have been on pure ENMs,<sup>296</sup> and not ENMs applied as coatings, and seemingly not as antibiotic coatings. There are also some specific concerns for the development of antibiotic resistance in the workforce. The latter has been indicated for staff working on the manufacturing of traditional antibiotics,<sup>297</sup> but the situation is unclear for medical practitioners who would be exposed to much lower quantities in the clinic, or whether novel antimicrobial ENMs (e.g., those made of metals) might present a similar concern for antibiotic resistance in medical staff.

In dentistry, one special concern might be respiratory exposure to the ENMs during dental repairs such as drilling or activities involving abrasion of the tooth. Inevitably, these activities will create an aerosol, but the risks to both practitioners and the patient are yet to be evaluated for ENMs, or ENMs with antimicrobial coatings. Interestingly, with respect to dental prosthetics, the main concern for chemical exposure is during the manufacture and adjustment of the prosthetic, for example, respiratory exposure to ultrafine particles during modeling the shape of the prosthetic with acrylic materials, sandblasting, working with metal alloys, or preparing porcelain veneers.<sup>298</sup> However, how any hazard quotients or calculation of lifetime cancer risk would be altered by including antimicrobial ENMs in such prosthetics is unknown. Clearly, further research is needed on workplace exposure to ENMs and specifically on antimicrobial ENMs that may have coatings and be made of several chemical substances.



## CONCERNS REGARDING BACTERIAL RESISTANCE TO ANTIMICROBIAL NANOMATERIALS

Although widely reported advantages of antimicrobial nanomaterials are their multiplicity of bacterial targets, and their mechanisms of action which generally differ from those of antibiotics, it is unlikely that they are exempt from the development of bacterial resistance. Where the antimicrobial takes the form of individual agents such as NPs, it is possible for bacteria to develop resistance through sequestration or aggregation of NPs,<sup>299</sup> efflux,<sup>300,301</sup> or reduction of ions.<sup>302</sup> In the case of engineered surfaces with nanotopographical modifications, it is less clear which mechanisms could evolve, though these could incorporate thickening of the cell wall to avoid mechanical disruption, changes to cellular elasticity to reduce rigidity, or changes to surface charge (as in the polymyxin resistance mechanism)<sup>303</sup> to introduce repellence from the surface to avoid contact with nanostructures.

A particular concern, in the wider context of AMR, is the possibility of the use of non-antibiotic antimicrobials leading to promotion of resistance against antibiotics. This may take the form of co-resistance, where genes conferring resistance to both antibiotics and non-antibiotics are present in the same cell, or cross-resistance, where resistance to a non-antibiotic also results in resistance to an antibiotic (e.g., efflux pumps).<sup>304</sup> The prevalence of, e.g., silver resistance genes, appears to be low (3.6% in hospital isolates reported), and the presence of resistance genes in the bacterial genome does not necessarily result in phenotypic resistance.<sup>305</sup> Generally, bacteria more readily develop resistance to antibiotics than to antimicrobial nanoparticles, with resistance to the latter requiring slower, stepwise increases in concentration when investigated *in vitro*.<sup>306</sup> This suggests that while widespread resistance may not currently be apparent, it is likely to develop eventually with increasing clinical use of antimicrobial nanomaterials.

Multiple studies have reported that certain nanomaterials enhance the transmission of antibiotic resistance genes in *Escherichia coli*, *Staphylococcus aureus*, and *Pseudomonas putida* by transformation and conjugation, two mechanisms of horizontal gene transfer in bacteria. Lu et al.<sup>307</sup> reported that both Ag NPs and Ag<sup>+</sup> increase conjugative transfer frequency by inducing ROS overproduction and increasing membrane permeability at environmentally and clinically relevant concentrations. Ding et al.<sup>308</sup> reported that Al<sub>2</sub>O<sub>3</sub> NPs, but not bulk Al<sub>2</sub>O<sub>3</sub>, promote plasmid-mediated transformation. This effect was reported to likely be due to Al<sub>2</sub>O<sub>3</sub> NP-induced damage to the cell membrane allowing plasmids to enter bacteria. This report was later followed up by a finding that certain nanometal oxides (Al<sub>2</sub>O<sub>3</sub> and ZnO) augment the mutation frequencies of drug-resistant *Escherichia coli* isolates, whereas the corresponding metal ions have weaker effects.<sup>309</sup> Another study has reported that ZnO and TiO<sub>2</sub> NPs oppositely impact the transformation efficiency of *Bacillus subtilis*, by modifying the induction of competence; the first step of the transformation process.<sup>310</sup> The authors showed that two oligopeptide ABC transporters were differentially expressed in response to NPs and thus the effect was due to a physiological adaptation rather than due to cell injury. In contrast, Ag NPs had no significant effect on competence under the same experimental conditions. This was a clear description of NPs in the physiological induction of horizontal gene transfer in bacteria. There are scenarios independent of genetic changes which may also lend a form of resistance to bacteria in a community, for example, *Pseudomonas*

*aeruginosa* produces the metabolite pyocyanin which reduces Ag<sup>+</sup> to nontoxic Ag<sup>0</sup>; co-incubation experiments have showed increased survival of Ag<sup>+</sup>-exposed bacteria if other pyocyanin-producing bacteria were present as the reduction of local Ag<sup>+</sup> rendered their environment less toxic.<sup>302</sup> This is particularly relevant to polymicrobial biofilms where the prevalence of a pyocyanin-producing *Pseudomonas aeruginosa* subset could lend protection to the rest of the biofilm. Another example is  $\beta$ -lactamase-producing bacteria conferring resistance to  $\beta$ -lactam antibiotics to nearby susceptible bacteria due to the excretion of  $\beta$ -lactamase enzymes.<sup>311</sup> This form of cooperative resistance is independent of genetic modification or the acquisition of resistance elements from other cells.

These studies collectively show that the development of resistance to antimicrobial nanomaterials is inevitable and reinforce the idea that NPs may have the potential to affect dissemination of antibiotic resistance in bacteria, potentially affecting the long-term antibacterial efficacy of nanocoatings as well as posing a public health concern by leading to wider AMR. More generally, this highlights the potential hazards of introducing nanomaterials into the environment without complete understanding of their wider consequences. The vast majority of research conducted on NPs has been conducted in *in vitro* settings and clinical applications will lead to unquantifiable consequences. The extent to which these effects are relevant to nanocoatings needs to be investigated; it has not been demonstrated that nanoparticles presented as surface coatings have a comparable effect regarding competence or induction of horizontal gene transfer. The role of bacterial stress and the potential for nanocoatings to produce subinhibitory or sublethal concentrations of antimicrobials, encouraging more rapid emergence of resistance, needs to be more thoroughly investigated.

## CONCLUSIONS

In this review, a range of different nanocoatings have been evaluated. In general, these nanocoatings take two major forms: those carrying active antimicrobial nanoparticles, and those relying on a biomechanical mechanism of action, such as nanoprotusions. For every introduction of a potential antimicrobial nanocoating, a number of possible new nanocomposite coatings are also produced, allowing the strengths of multiple approaches to be combined. Traditional medical and scientific research has generally favored siloed, individual-disciplined approaches to problems, but serious and impending public health emergencies, such as AMR and its implications for healthcare-acquired infections, require a more multidisciplinary and collaborative approach. The development of antimicrobial nanocoatings is the prototypic example of the interface between microbiology and biomedical engineering. It appears from the evidence synthesized here that antimicrobial nanocoatings will play a significant role in the future protection of surfaces from bacterial colonization, whether those surfaces are environmental or implanted in nature. The benefits of antimicrobial nanocoatings over conventional antibiotics allow targeted effects rather than dispersed and potentially unintended consequences, and combined strategies may be most favorable. A cautious approach should be adopted, ensuring continued biocompatibility, long-term biological activity and minimal ecological impacts, as well as careful consideration of the consequences for bacterial resistance and interactions with AMR. Without doubt, the increasing use of nanomaterials in medicine and dentistry will require the construction of new legislative and regulatory

frameworks to ensure safety is maintained and the benefits are maximized. Current evidence suggests an optimistic and exciting future for the use of antimicrobial nanocoatings in improving clinical outcomes in medicine and dentistry.

## AUTHOR INFORMATION

### Corresponding Author

Alexandros Besinis – School of Engineering, Computing and Mathematics, Faculty of Science and Engineering, University of Plymouth, Plymouth PL4 8AA, United Kingdom; Peninsula Dental School, Faculty of Health, University of Plymouth, Plymouth PL4 8AA, United Kingdom;  
Email: alexander.besinis@plymouth.ac.uk

### Authors

James Butler – School of Engineering, Computing and Mathematics, Faculty of Science and Engineering, University of Plymouth, Plymouth PL4 8AA, United Kingdom; Present Address: Department of Clinical and Biomedical Sciences, Exeter Medical School, Faculty of Health and Life Sciences, University of Exeter, Exeter EX1 2LU, United Kingdom;  
orcid.org/0000-0003-1998-1219

Richard D. Handy – School of Biological and Marine Sciences, Faculty of Science and Engineering, University of Plymouth, Plymouth PL4 8AA, United Kingdom

Mathew Upton – School of Biomedical Sciences, Faculty of Health, University of Plymouth, Plymouth PL4 8AA, United Kingdom

Complete contact information is available at:  
<https://pubs.acs.org/10.1021/acsnano.2c12488>

### Notes

The authors declare no competing financial interest.

## ACKNOWLEDGMENTS

This work received no specific grant from any funding agency. The authors acknowledge internal PhD project funding from the School of Engineering, Computing and Mathematics at the University of Plymouth, which supported J.B.

## VOCABULARY

**Engineered nanomaterials**, intentionally manufactured materials containing particles with one or more external dimensions in the size range 1–100 nm; **nanocoating**, a layer or film of particles with one or more external dimensions in the size range 1–100 nm applied to a surface to protect it or improve its function in some capacity; **biofilm**, any consortium of microorganisms in which cells aggregate and become enclosed in a self-produced exopolysaccharide matrix; **antimicrobial resistance**, the outcome of microorganisms changing over time to be able to survive exposure to antimicrobial medicines such as antibiotics which are designed to kill them or inhibit their growth; **surface nanotopography**, the arrangement of physical surface features at the nanoscopic scale

## REFERENCES

- (1) Masciangioli, T.; Zhang, W. Environmental Technologies at the Nanoscale. *Environ. Sci. Technol.* **2003**, *37*, 102–108.
- (2) Oberdörster, G.; Finkelstein, J. N.; Johnston, C.; Gelein, R.; Cox, C.; Baggs, R.; Elder, A. C. Acute Pulmonary Effects of Ultrafine Particles in Rats and Mice. *Res. Rep. - Health Eff. Inst.* **2000**, *96*, 75–86.
- (3) Besinis, A.; van Noort, R.; Martin, N. Remineralization Potential of Fully Demineralized Dentin Infiltrated with Silica and Hydroxyapatite Nanoparticles. *Dent. Mater.* **2014**, *30*, 249–262.
- (4) Atluri, R.; Jensen, K. A. In *Modelling the Toxicity of Nanoparticles*; Lang, T., Bañares, M. A., Rallo, R., Eds.; 3–23, Springer International Publishing, 2017.
- (5) Navya, P. N.; Daima, H. K. Rational Engineering of Physicochemical Properties of Nanomaterials for Biomedical Applications with Nanotoxicological Perspectives. *Nano Convergence* **2016**, *3*, 1 DOI: 10.1186/s40580-016-0064-z.
- (6) Sayes, C. M.; Wahi, R.; Kurian, P. A.; Liu, Y.; West, J. L.; Ausman, K. D.; Warheit, D. B.; Colvin, V. L. Correlating Nanoscale Titania Structure with Toxicity: a Cytotoxicity and Inflammatory Response Study with Human Dermal Fibroblasts and Human Lung Epithelial Cells. *Toxicol. Sci.* **2006**, *92*, 174–185.
- (7) Besinis, A.; van Noort, R.; Martin, N. Infiltration of Demineralized Dentin with Silica and Hydroxyapatite Nanoparticles. *Dent. Mater.* **2012**, *28*, 1012–1023.
- (8) Allaker, R. P.; Memarzadeh, K. Nanoparticles and the Control of Oral Infections. *Int. J. Antimicrob. Agents* **2014**, *43*, 95–104.
- (9) Khezerlou, A.; Alizadeh-Sani, M.; Azizi-Lalabadi, M.; Ehsani, A. Nanoparticles and their Antimicrobial Properties Against Pathogens Including Bacteria, Fungi, Parasites and Viruses. *Microb. Pathog.* **2018**, *123*, 505–526.
- (10) Dizaj, S. M.; Lotfipour, F.; Barzegar-Jalali, M.; Zarrintan, M. H.; Adibkia, K. Antimicrobial Activity of the Metals and Metal Oxide Nanoparticles. *Mater. Sci. Eng., C* **2014**, *44*, 278–284.
- (11) Song, W.; Ge, S. Application of Antimicrobial Nanoparticles in Dentistry. *Molecules* **2019**, *24*, 1033.
- (12) Makowski, M.; Silva, I. C.; Pais do Amaral, C.; Goncalves, S.; Santos, N. C. Advances in Lipid and Metal Nanoparticles for Antimicrobial Peptide Delivery. *Pharmaceutics* **2019**, *11*, 588.
- (13) Gao, W.; Chen, Y.; Zhang, Y.; Zhang, Q.; Zhang, L. Nanoparticle-Based Local Antimicrobial Drug Delivery. *Adv. Drug Delivery Rev.* **2018**, *127*, 46–57.
- (14) Seong, M.; Lee, D. G. Silver Nanoparticles Against *Salmonella enterica* Serotype Typhimurium: Role of Inner Membrane Dysfunction. *Curr. Microbiol.* **2017**, *74*, 661–670.
- (15) Wang, H.; Jiang, Y.; Zhang, Y.; Zhang, Z.; Yang, X.; Ali, M. A.; Fox, E. M.; Gobius, K. S.; Man, C. Silver Nanoparticles: A Novel Antibacterial Agent for Control of *Cronobacter sakazakii*. *J. Dairy Sci.* **2018**, *101*, 10775.
- (16) Lemire, J. A.; Harrison, J. J.; Turner, R. J. Antimicrobial Activity of Metals: Mechanisms, Molecular Targets and Applications. *Nat. Rev. Microbiol.* **2013**, *11*, 371.
- (17) Xie, Y.; He, Y.; Irwin, P. L.; Jin, T.; Shi, X. Antibacterial Activity and Mechanism of Action of Zinc Oxide Nanoparticles against *Campylobacter jejuni*. *Appl. Environ. Microbiol.* **2011**, *77*, 2325.
- (18) Linklater, D. P.; Baulin, V. A.; Le Guével, X.; Fleury, J.-B.; Hanssen, E.; Nguyen, T. H. P.; Juodkazis, S.; Bryant, G.; Crawford, R. J.; Stoodley, P. Antibacterial Action of Nanoparticles by Lethal Stretching of Bacterial Cell Membranes. *Adv. Mater.* **2020**, *32*, 2005679.
- (19) Monopoli, M. P.; Åberg, C.; Salvati, A.; Dawson, K. A. Biomolecular Coronas Provide the Biological Identity of Nanosized Materials. *Nat. Nanotechnol.* **2012**, *7*, 779–786.
- (20) Nel, A. E.; Mädler, L.; Velegol, D.; Xia, T.; Hoek, E. M. V.; Somasundaran, P.; Klaessig, F.; Castranova, V.; Thompson, M. Understanding Biophysicochemical Interactions at the Nano–Bio Interface. *Nat. Mater.* **2009**, *8*, 543–557.
- (21) Mazzolini, J.; Weber, R. J.; Chen, H. S.; Khan, A.; Guggenheim, E.; Shaw, R. K.; Chipman, J. K.; Viant, M. R.; Rappoport, J. Z. Protein Corona Modulates Uptake and Toxicity of Nanoceria via Clathrin-Mediated Endocytosis. *Biol. Bull. (Chicago, IL, U. S.)* **2016**, *231*, 40–60.
- (22) Francia, V.; Yang, K.; Deville, S.; Reker-Smit, C.; Nelissen, I.; Salvati, A. Corona Composition Can Affect the Mechanisms Cells Use to Internalize Nanoparticles. *ACS Nano* **2019**, *13*, 11107–11121.
- (23) Zawadzka, K.; Kadziola, K.; Felczak, A.; Wronska, N.; Piwonski, I.; Kisielowska, A.; Lisowska, K. Surface Area or Diameter - Which

Factor Really Determines the Antibacterial Activity of Silver Nanoparticles Grown on TiO<sub>2</sub> coatings? *New J. Chem.* **2014**, *38*, 3275–3281.

(24) Klueh, U.; Wagner, V.; Kelly, S.; Johnson, A.; Bryers, J. D. Efficacy of Silver-Coated Fabric to Prevent Bacterial Colonization and Subsequent Device-Based Biofilm Formation. *J. Biomed. Mater. Res.* **2000**, *53*, 621–631.

(25) Holt, K. B.; Bard, A. J. Interaction of Silver (I) Ions with the Respiratory Chain of *Escherichia coli*: an Electrochemical and Scanning Electrochemical Microscopy Study of the Antimicrobial Mechanism of Micromolar Ag<sup>+</sup>. *Biochemistry* **2005**, *44*, 13214–13223.

(26) Schreurs, W. J.; Rosenberg, H. Effect of Silver Ions on Transport and Retention of Phosphate by *Escherichia coli*. *J. Bacteriol.* **1982**, *152*, 7–13.

(27) Dibrov, P.; Dzioba, J.; Gosink, K. K.; Häse, C. C. Chemiosmotic Mechanism of Antimicrobial Activity of Ag in *Vibrio cholerae*. *Antimicrob. Agents Chemother.* **2002**, *46*, 2668.

(28) Arakawa, H.; Neault, J. F.; Tajmir-Riahi, H. A. Silver(I) Complexes with DNA and RNA Studied by Fourier Transform Infrared Spectroscopy and Capillary Electrophoresis. *Biophys. J.* **2001**, *81*, 1580–1587.

(29) Barras, F.; Aussel, L.; Ezraty, B. Silver and Antibiotic, New Facts to an Old Story. *Antibiotics* **2018**, *7*, 79.

(30) Liao, X.; Yang, F.; Li, H.; So, P.-K.; Yao, Z.; Xia, W.; Sun, H. Targeting the Thioredoxin Reductase–Thioredoxin System from *Staphylococcus aureus* by Silver Ions. *Inorg. Chem.* **2017**, *56*, 14823–14830.

(31) Long, Y. M.; Hu, L. G.; Yan, X. T.; Zhao, X. C.; Zhou, Q. F.; Cai, Y.; Jiang, G. B. Surface Ligand Controls Silver Ion Release of Nanosilver and its Antibacterial Activity Against *Escherichia coli*. *Int. J. Nanomed.* **2017**, *12*, 3193–3206.

(32) Jiang, H. S.; Zhang, Y.; Lu, Z. W.; Lebrun, R.; Gontero, B.; Li, W. Interaction Between Silver Nanoparticles and Two Dehydrogenases: Role of Thiol Groups. *Small* **2019**, *15*, 1900860.

(33) Xia, T.; Kovochich, M.; Liang, M.; Mädler, L.; Gilbert, B.; Shi, H.; Yeh, J. I.; Zink, J. I.; Nel, A. E. Comparison of the Mechanism of Toxicity of Zinc Oxide and Cerium Oxide Nanoparticles Based on Dissolution and Oxidative Stress Properties. *ACS Nano* **2008**, *2*, 2121–2134.

(34) Applerot, G.; Lipovsky, A.; Dror, R.; Perkas, N.; Nitzan, Y.; Lubart, R.; Gedanken, A. Enhanced Antibacterial Activity of Nanocrystalline ZnO Due to Increased ROS-Mediated Cell Injury. *Adv. Funct. Mater.* **2009**, *19*, 842–852.

(35) Akhtar, M. J.; Ahamed, M.; Kumar, S.; Siddiqui, H.; Patil, G.; Ashquin, M.; Ahmad, I. Nanotoxicity of Pure Silica Mediated through Oxidant Generation Rather Than Glutathione Depletion in Human Lung Epithelial Cells. *Toxicology* **2010**, *276*, 95–102.

(36) Huang, T.; Holden, J. A.; Heath, D. E.; O'Brien-Simpson, N. M.; O'Connor, A. J. Engineering Highly Effective Antimicrobial Selenium Nanoparticles Through Control of Particle Size. *Nanoscale* **2019**, *11*, 14937–14951.

(37) Kessler, A.; Hedberg, J.; Blomberg, E.; Odnevall, I. Reactive Oxygen Species Formed by Metal and Metal Oxide Nanoparticles in Physiological Media - A Review of Reactions of Importance to Nanotoxicity and Proposal for Categorization. *Nanomaterials* **2022**, *12*, 1922.

(38) Donlan, R. M. Biofilms: Microbial Life on Surfaces. *Emerg. Infect. Dis.* **2002**, *8*, 881–890.

(39) Singh, S.; Singh, S. K.; Chowdhury, I.; Singh, R. Understanding the Mechanism of Bacterial Biofilms Resistance to Antimicrobial Agents. *Open Microbiol. J.* **2017**, *11*, 53–62.

(40) Flemming, H.-C.; Wingender, J. The Biofilm Matrix. *Nat. Rev. Microbiol.* **2010**, *8*, 623.

(41) Madsen, J. S.; Burmølle, M.; Hansen, L. H.; Sørensen, S. J. The Interconnection Between Biofilm Formation and Horizontal Gene Transfer. *FEMS Immunol. Med. Microbiol.* **2012**, *65*, 183–195.

(42) Garcia, C. F.; Stangl, F.; Gotz, A.; Zhao, W. N.; Sieber, S. A.; Opitz, M.; Lileig, O. Topographical Alterations Render Bacterial Biofilms Susceptible to Chemical and Mechanical Stress. *Biomater. Sci.* **2019**, *7*, 220–232.

(43) Ceri, H.; Olson, M. E.; Stremick, C.; Read, R. R.; Morck, D.; Buret, A. The Calgary Biofilm Device: New Technology for Rapid Determination of Antibiotic Susceptibilities of Bacterial Biofilms. *J. Clin. Microbiol.* **1999**, *37*, 1771–1776.

(44) Abdi-Ali, A.; Mohammadi-Mehr, M.; Agha Alaei, Y. Bactericidal Activity of Various Antibiotics against Biofilm-Producing *Pseudomonas aeruginosa*. *Int. J. Antimicrob. Agents* **2006**, *27*, 196–200.

(45) Stoodley, P.; Sauer, K.; Davies, D. G.; Costerton, J. W. Biofilms as Complex Differentiated Communities. *Annu. Rev. Microbiol.* **2002**, *56*, 187–209.

(46) Bridier, A.; Briandet, R.; Thomas, V.; Dubois-Brissonnet, F. Resistance of Bacterial Biofilms to Disinfectants: a Review. *Biofouling* **2011**, *27*, 1017–1032.

(47) Bressler, D.; Balzer, M.; Dannehl, A.; Flemming, H.-C.; Wingender, J. Persistence of *Pseudomonas aeruginosa* in Drinking-Water Biofilms on Elastomeric Material. *Water Sci. Technol.: Water Supply* **2009**, *9*, 81–87.

(48) Høiby, N.; Bjarnsholt, T.; Givskov, M.; Molin, S.; Ciofu, O. Antibiotic Resistance of Bacterial Biofilms. *Int. J. Antimicrob. Agents* **2010**, *35*, 322–332.

(49) Høiby, N.; Bjarnsholt, T.; Givskov, M.; Molin, S.; Ciofu, O. Antibiotic resistance of bacterial biofilms. *Int. J. Antimicrob. Agents* **2010**, *35*, 322–332.

(50) Yan, J.; Bassler, B. L. Surviving as a Community: Antibiotic Tolerance and Persistence in Bacterial Biofilms. *Cell Host Microbe* **2019**, *26*, 15–21.

(51) Hathroubi, S.; Mekni, M. A.; Domenico, P.; Nguyen, D.; Jacques, M. Biofilms: Microbial Shelters Against Antibiotics. *Microb. Drug Resist.* **2017**, *23*, 147–156.

(52) Arias, C. A.; Murray, B. E. Antibiotic-Resistant Bugs in the 21st Century — A Clinical Super-Challenge. *N. Engl. J. Med.* **2009**, *360*, 439–443.

(53) Cassini, A.; Högberg, L. D.; Plachouras, D.; Quattrocchi, A.; Hoxha, A.; Simonsen, G. S.; Colomb-Cotinat, M.; Kretzschmar, M. E.; Devleeschauwer, B.; Cecchini, M.; et al. Attributable Deaths and Disability-Adjusted Life-Years Caused By Infections with Antibiotic-Resistant Bacteria in the EU and the European Economic Area in 2015: a Population-Level Modelling Analysis. *Lancet Infect. Dis.* **2019**, *19*, 56–66.

(54) O'Neill, J. *Tackling Drug-Resistant Infections Globally: Final Report and Recommendations*; United Kingdom Government, 2016.

(55) Murray, C. J. L.; Ikuta, K. S.; Sharara, F.; Swetschinski, L.; Robles Aguilar, G.; Gray, A.; Han, C.; Bisignano, C.; Rao, P.; Wool, E.; et al. Global Burden of Bacterial Antimicrobial Resistance in 2019: a Systematic Analysis. *Lancet* **2022**, *399*, 629–655.

(56) Fischbach, M. A.; Walsh, C. T. Antibiotics for Emerging Pathogens. *Science* **2009**, *325*, 1089–1093.

(57) Steenbergen, J. N.; Alder, J.; Thorne, G. M.; Tally, F. P. Daptomycin: a Lipopeptide Antibiotic for the Treatment of Serious Gram-Positive Infections. *J. Antimicrob. Chemother.* **2005**, *55*, 283–288.

(58) Laxminarayan, R.; Duse, A.; Wattal, C.; Zaidi, A. K. M.; Wertheim, H. F. L.; Sumpradit, N.; Vlieghe, E.; Hara, G. L.; Gould, I. M.; Goossens, H.; et al. Antibiotic Resistance—The Need for Global Solutions. *Lancet Infect. Dis.* **2013**, *13*, 1057–1098.

(59) World Health Organization. *Antibacterial Agents in Clinical and Preclinical Development: an Overview and Analysis*; World Health Organization, 2020.

(60) Rex, J. H.; Outterson, K. Antibiotic Reimbursement in a Model Delinked from Sales: a Benchmark-Based Worldwide Approach. *Lancet Infect. Dis.* **2016**, *16*, 500–505.

(61) Gotham, D.; Moja, L.; van der Heijden, M.; Paulin, S.; Smith, I.; Beyer, P. Reimbursement Models to Tackle Market Failures for Antimicrobials: Approaches Taken in France, Germany, Sweden, the United Kingdom, and the United States. *Health Policy* **2021**, *125*, 296–306.

(62) Besinis, A.; De Peralta, T.; Handy, R. D. The Antibacterial Effects of Silver, Titanium Dioxide and Silica Dioxide Nanoparticles Compared to the Dental Disinfectant Chlorhexidine on *Streptococcus mutans* Using a Suite of Bioassays. *Nanotoxicology* **2014**, *8*, 1–16.



- (63) Ahamed, M.; Alhadlaq, H. A.; Khan, M. A. M.; Karuppiah, P.; Al-Dhabi, N. A. Synthesis, Characterization, and Antimicrobial Activity of Copper Oxide Nanoparticles. *J. Nanomater.* **2014**, *2014*, 637858.
- (64) Zhou, Y.; Kong, Y.; Kundu, S.; Cirillo, J. D.; Liang, H. Antibacterial Activities of Gold and Silver Nanoparticles against *Escherichia coli* and *Bacillus Calmette-Guérin*. *J. Nanobiotechnol.* **2012**, *10*, 19.
- (65) Gristina, A. G.; Naylor, P.; Myrvik, Q. Infections from Biomaterials and Implants: A Race for the Surface. *Med. Prog. Technol.* **1988**, *14*, 205–224.
- (66) Gristina, A. Biomaterial-Centered Infection: Microbial Adhesion Versus Tissue Integration. *Science* **1987**, *237*, 1588–1595.
- (67) Subbiahdoss, G.; Kuijter, R.; Grijpma, D. W.; van der Mei, H. C.; Busscher, H. J. Microbial Biofilm Growth vs. Tissue Integration: “The race for the surface” Experimentally Studied. *Acta Biomater.* **2009**, *5*, 1399–1404.
- (68) Paquette, D. W.; Brodala, N.; Williams, R. C. Risk Factors for Endosseous Dental Implant Failure. *Dent. Clin. North Am.* **2006**, *50*, 361–374.
- (69) Besinis, A.; Hadi, S. D.; Le, H. R.; Tredwin, C.; Handy, R. D. Antibacterial Activity and Biofilm Inhibition by Surface Modified Titanium Alloy Medical Implants Following Application of Silver, Titanium Dioxide and Hydroxyapatite Nanocoatings. *Nanotoxicology* **2017**, *11*, 327–338.
- (70) Darouiche, R. O. Treatment of Infections Associated with Surgical Implants. *N. Engl. J. Med.* **2004**, *350*, 1422–1429.
- (71) Costa, D. M.; Johani, K.; Melo, D. S.; Lopes, L. K. O.; Lopes Lima, L. K. O.; Tipple, A. F. V.; Hu, H.; Vickery, K. Biofilm Contamination of High-Touched Surfaces in Intensive Care Units: Epidemiology and Potential Impacts. *Letts. Appl. Microbiol.* **2019**, *68*, 269–276.
- (72) Coll, F.; Harrison, E. M.; Toleman, M. S.; Reuter, S.; Raven, K. E.; Blane, B.; Palmer, B.; Kappeler, A. R. M.; Brown, N. M.; Török, M. E. Longitudinal Genomic Surveillance of MRSA in the UK Reveals Transmission Patterns in Hospitals and the Community. *Sci. Transl. Med.* **2017**, *9*, eaak9745 DOI: 10.1126/scitranslmed.aak9745.
- (73) Vickery, K.; Deva, A.; Jacombs, A.; Allan, J.; Valente, P.; Gosbell, I. B. Presence of Biofilm Containing Viable Multiresistant Organisms Despite Terminal Cleaning on Clinical Surfaces in an Intensive Care Unit. *J. Hosp. Infect.* **2012**, *80*, 52–55.
- (74) Pidot, S. J.; Gao, W.; Buultjens, A. H.; Monk, I. R.; Guerillot, R.; Carter, G. P.; Lee, J. Y. H.; Lam, M. M. C.; Grayson, M. L.; Ballard, S. A. Increasing Tolerance of Hospital *Enterococcus faecium* to Handwash Alcohols. *Sci. Transl. Med.* **2018**, *10*, aar6115 DOI: 10.1126/scitranslmed.aar6115.
- (75) Mc Carlie, S.; Boucher, C. E.; Bragg, R. R. Molecular Basis of Bacterial Disinfectant Resistance. *Drug Resistance Updates* **2020**, *48*, 100672.
- (76) Petrochenko, P. E.; Zheng, J.; Casey, B. J.; Bayati, M. R.; Narayan, R. J.; Goering, P. L. Nanosilver-PMMA Composite Coating Optimized to Provide Robust Antibacterial Efficacy While Minimizing Human Bone Marrow Stromal Cell Toxicity. *Toxicol. In Vitro* **2017**, *44*, 248–255.
- (77) Besinis, A.; De Peralta, T.; Handy, R. D. Inhibition of Biofilm Formation and Antibacterial Properties of a Silver Nano-Coating on Human Dentine. *Nanotoxicology* **2013**, *8*, 745–754.
- (78) Larrude, D. G.; Maia da Costa, M. E. H.; Freire, F. L. Synthesis and Characterization of Silver Nanoparticle-Multiwalled Carbon Nanotube Composites. *J. Nanomater.* **2014**, *2014*, 654068.
- (79) Hsueh, Y.-H.; Hsieh, C.-T.; Chiu, S.-T.; Tsai, P.-H.; Liu, C.-Y.; Ke, W.-J. Antibacterial Property of Composites of Reduced Graphene Oxide with Nano-Silver and Zinc Oxide Nanoparticles Synthesized Using a Microwave-Assisted Approach. *Int. J. Mol. Sci.* **2019**, *20*, 5394.
- (80) Gadkari, R. R.; Ali, S. W.; Joshi, M.; Rajendran, S.; Das, A.; Alagirusamy, R. Leveraging Antibacterial Efficacy of Silver Loaded Chitosan Nanoparticles on Layer-By-Layer Self-Assembled Coated Cotton Fabric. *Int. J. Biol. Macromol.* **2020**, *162*, 548–560.
- (81) Xu, G.; Shen, X.; Dai, L.; Ran, Q.; Ma, P.; Cai, K. Reduced Bacteria Adhesion on Octenidine Loaded Mesoporous Silica Nanoparticles Coating on Titanium Substrates. *Mater. Sci. Eng., C* **2017**, *70*, 386–395.
- (82) Linklater, D. P.; De Volder, M.; Baulin, V. A.; Werner, M.; Jessl, S.; Golozar, M.; Maggini, L.; Rubanov, S.; Hanssen, E.; Juodkakis, S.; et al. High Aspect Ratio Nanostructures Kill Bacteria via Storage and Release of Mechanical Energy. *ACS Nano* **2018**, *12*, 6657–6667.
- (83) Ivanova, E. P.; Hasan, J.; Webb, H. K.; Gervinskas, G.; Juodkakis, S.; Truong, V. K.; Wu, A. H. F.; Lamb, R. N.; Baulin, V. A.; Watson, G. S.; et al. Bactericidal Activity of Black Silicon. *Nat. Commun.* **2013**, *4*, 2838.
- (84) Cunha, B. A. Antibiotic Side Effects. *Med. Clin. North Am.* **2001**, *85*, 149–185.
- (85) Wright, J.; Paauw, D. S. Complications of Antibiotic Therapy. *Med. Clin. North Am.* **2013**, *97*, 667–679.
- (86) Gilbertson, L. M.; Albalghiti, E. M.; Fishman, Z. S.; Perreault, F.; Corredor, C.; Posner, J. D.; Elimelech, M.; Pfefferle, L. D.; Zimmerman, J. B. Shape-Dependent Surface Reactivity and Antimicrobial Activity of Nano-Cupric Oxide. *Environ. Sci. Technol.* **2016**, *50*, 3975–3984.
- (87) Baker, C.; Pradhan, A.; Pakstis, L.; Pochan, D. J.; Shah, S. I. Synthesis and Antibacterial Properties of Silver Nanoparticles. *J. Nanosci. Nanotechnol.* **2005**, *5*, 244–249.
- (88) Morones, J. R.; Elechiguerra, J. L.; Camacho, A.; Holt, K.; Kouri, J. B.; Ramirez, J. T.; Yacaman, M. J. The Bactericidal Effect of Silver Nanoparticles. *Nanotechnology* **2005**, *16*, 2346–2353.
- (89) Lok, C. N.; Ho, C. M.; Chen, R.; He, Q. Y.; Yu, W. Y.; Sun, H.; Tam, P. K.; Chiu, J. F.; Che, C. M. Silver Nanoparticles: Partial Oxidation and Antibacterial Activities. *J. Biol. Inorg. Chem.* **2007**, *12*, 527–534.
- (90) Choi, O.; Hu, Z. Size Dependent and Reactive Oxygen Species Related Nanosilver Toxicity to Nitrifying Bacteria. *Environ. Sci. Technol.* **2008**, *42*, 4583–4588.
- (91) Agnihotri, S.; Mukherji, S.; Mukherji, S. Size-Controlled Silver Nanoparticles Synthesized Over the Range 5–100 nm Using the Same Protocol and Their Antibacterial Efficacy. *RSC Adv.* **2014**, *4*, 3974–3983.
- (92) Pal, S.; Tak, Y. K.; Song, J. M. Does the Antibacterial Activity of Silver Nanoparticles Depend on the Shape of the Nanoparticle? A Study of the Gram-Negative Bacterium *Escherichia coli*. *Appl. Environ. Microbiol.* **2007**, *73*, 1712–1720.
- (93) Wang, L.; He, H.; Yu, Y.; Sun, L.; Liu, S.; Zhang, C.; He, L. Morphology-Dependent Bactericidal Activities of Ag/CeO<sub>2</sub> Catalysts Against *Escherichia coli*. *J. Inorg. Biochem.* **2014**, *135*, 45–53.
- (94) Cheon, J. Y.; Kim, S. J.; Rhee, Y. H.; Kwon, O. H.; Park, W. H. Shape-Dependent Antimicrobial Activities of Silver Nanoparticles. *Int. J. Nanomed.* **2019**, *14*, 2773–2780.
- (95) Arakha, M.; Saleem, M.; Mallick, B. C.; Jha, S. The Effects of Interfacial Potential on Antimicrobial Propensity of ZnO Nanoparticle. *Sci. Rep.* **2015**, *5*, 9578.
- (96) Qiao, Z.; Yao, Y.; Song, S.; Yin, M.; Luo, J. Silver Nanoparticles with pH Induced Surface Charge Switchable Properties for Antibacterial and Antibiofilm Applications. *J. Mater. Chem. B* **2019**, *7*, 830–840.
- (97) Allaker, R. P. The Use of Nanoparticles to Control Oral Biofilm Formation. *J. Dent. Res.* **2010**, *89*, 1175–1186.
- (98) Alexander, J. W. History of the Medical Use of Silver. *Surg. Infect.* **2009**, *10*, 289–292.
- (99) Klasesen, H. J. Historical Review of the Use of Silver in the Treatment of Burns. I. Early uses. *Burns* **2000**, *26*, 117–130.
- (100) Politano, A. D.; Campbell, K. T.; Rosenberger, L. H.; Sawyer, R. G. Use of Silver in the Prevention and Treatment of Infections: Silver Review. *Surg. Infect.* **2013**, *14*, 8–20.
- (101) Saint, S.; Elmore, J. G.; Sullivan, S. D.; Emerson, S. S.; Koepsell, T. D. The Efficacy of Silver Alloy-Coated Urinary Catheters in Preventing Urinary Tract Infection: a Meta-Analysis. *Am. J. Med.* **1998**, *105*, 236–241.
- (102) Rupp, M. E.; Fitzgerald, T.; Marion, N.; Helget, V.; Puumala, S.; Anderson, J. R.; Fey, P. D. Effect of Silver-Coated Urinary Catheters: Efficacy, Cost-Effectiveness, and Antimicrobial Resistance. *Am. J. Infect. Control* **2004**, *32*, 445–450.

- (103) Busscher, H. J.; van der Mei, H. C. How Do Bacteria Know They Are On A Surface and Regulate Their Response to an Adhering State? *PLoS Pathog* **2012**, *8*, e1002440.
- (104) Meran, Z.; Besinis, A.; De Peralta, T.; Handy, R. D. Antifungal Properties and Biocompatibility of Silver Nanoparticle Coatings on Silicone Maxillofacial Prostheses *In Vitro*. *J. Biomed. Mater. Res., Part B* **2018**, *106*, 1038–1051.
- (105) Espinosa Cristóbal, L.; Martínez-Castañón, G.-A.; Martínez-Martínez, R.; Loyola-Rodríguez, J.; Patiño-Marín, N.; Reyes-Macías, J. F.; Ruiz, F. Antibacterial Effect of Silver Nanoparticles against *Streptococcus mutans*. *Mater. Lett.* **2009**, *63*, 2603–2606.
- (106) Hernandez-Sierra, J. F.; Ruiz, F.; Pena, D. C.; Martínez-Gutiérrez, F.; Martínez, A. E.; Guillen Ade, J.; Tapia-Perez, H.; Castanon, G. M. The Antimicrobial Sensitivity of *Streptococcus mutans* to Nanoparticles of Silver, Zinc Oxide, and Gold. *Nanomedicine: NBM* **2008**, *4*, 237–240.
- (107) Besinis, A.; De Peralta, T.; Tredwin, C. J.; Handy, R. D. Review of Nanomaterials in Dentistry: Interactions with the Oral Micro-environment, Clinical Applications, Hazards, and Benefits. *ACS Nano* **2015**, *9*, 2255–2289.
- (108) Lynch, I.; Cedervall, T.; Lundqvist, M.; Cabaleiro-Lago, C.; Linse, S.; Dawson, K. A. The Nanoparticle–Protein Complex as a Biological Entity; a Complex Fluids and Surface Science Challenge for the 21st Century. *Adv. Colloid Interface Sci.* **2007**, *134*, 167–174.
- (109) Zarei, M.; Jamnejad, A.; Khajehali, E. Antibacterial Effect of Silver Nanoparticles Against Four Foodborne Pathogens. *Jundishapur J. Microbiol.* **2014**, *7*, 8720.
- (110) Samberg, M. E.; Oldenburg, S. J.; Monteiro-Riviere, N. A. Evaluation of Silver Nanoparticle Toxicity in Skin *In Vivo* and Keratinocytes *In Vitro*. *Environ. Health Perspect.* **2010**, *118*, 407–413.
- (111) Braydich-Stolle, L.; Hussain, S.; Schlager, J. J.; Hofmann, M.-C. *In Vitro* Cytotoxicity of Nanoparticles in Mammalian Germline Stem Cells. *Toxicol. Sci.* **2005**, *88*, 412–419.
- (112) Hussain, S. M.; Hess, K. L.; Gearhart, J. M.; Geiss, K. T.; Schlager, J. J. *In Vitro* Toxicity of Nanoparticles in BRL 3A Rat Liver Cells. *Toxicol. In Vitro* **2005**, *19*, 975–983.
- (113) Panacek, A.; Kolar, M.; Vecerova, R.; Pucek, R.; Soukupova, J.; Krystof, V.; Hamal, P.; Zboril, R.; Kvittek, L. Antifungal Activity of Silver Nanoparticles against *Candida* spp. *Biomaterials* **2009**, *30*, 6333–6340.
- (114) Arora, S.; Jain, J.; Rajwade, J. M.; Paknikar, K. M. Interactions of Silver Nanoparticles with Primary Mouse Fibroblasts and Liver Cells. *Toxicol. Appl. Pharmacol.* **2009**, *236*, 310–318.
- (115) Agnihotri, S.; Mukherji, S.; Mukherji, S. Immobilized Silver Nanoparticles Enhance Contact Killing and Show Highest Efficacy: Elucidation of the Mechanism of Bactericidal Action of Silver. *Nanoscale* **2013**, *5*, 7328–7340.
- (116) Silva-Bermudez, P.; Rodil, S. E. An Overview of Protein Adsorption on Metal Oxide Coatings for Biomedical Implants. *Surf. Coat. Technol.* **2013**, *233*, 147–158.
- (117) Grass, G.; Rensing, C.; Solioz, M. Metallic Copper as an Antimicrobial Surface. *Appl. Environ. Microbiol.* **2011**, *77*, 1541–1547.
- (118) Perelshtein, I.; Applerot, G.; Perkash, N.; Wehrschuetz-Sigl, E.; Hasmann, A.; Guebitz, G.; Gedanken, A. CuO–cotton Nanocomposite: Formation, Morphology, and Antibacterial Activity. *Surf. Coat. Technol.* **2009**, *204*, 54–57.
- (119) Prabhu, B. M.; Ali, S. F.; Murdock, R. C.; Hussain, S. M.; Srivatsan, M. Copper Nanoparticles Exert Size and Concentration Dependent Toxicity on Somatosensory Neurons of Rat. *Nanotoxicology* **2010**, *4*, 150–160.
- (120) Praetorius, M.; Brunner, C.; Lehnert, B.; Klingmann, C.; Schmidt, H.; Staecker, H.; Schick, B. Transsynaptic Delivery of Nanoparticles to the Central Auditory Nervous System. *Acta Otolaryngol.* **2007**, *127*, 486–490.
- (121) Griffitt, R. J.; Weil, R.; Hyndman, K. A.; Denslow, N. D.; Powers, K.; Taylor, D.; Barber, D. S. Exposure to Copper Nanoparticles Causes Gill Injury and Acute Lethality in Zebrafish (*Danio rerio*). *Environ. Sci. Technol.* **2007**, *41*, 8178–8186.
- (122) Bai, W.; Tian, W.; Zhang, Z.; He, X.; Ma, Y.; Liu, N. Q.; Chai, Z. Effects of Copper Nanoparticles on the Development of Zebrafish Embryos. *J. Nanosci. Nanotechnol.* **2010**, *10*, 8670–8676.
- (123) Ma, R.; Stegemeyer, J.; Levard, C.; Dale, J. G.; Noack, C. W.; Yang, T.; Brown, G. E.; Lowry, G. V. Sulfidation of Copper Oxide Nanoparticles and Properties of Resulting Copper Sulfide. *Environ. Sci.: Nano* **2014**, *1*, 347–357.
- (124) Lead, J. R.; Batley, G. E.; Alvarez, P. J. J.; Croteau, M. N.; Handy, R. D.; McLaughlin, M. J.; Judy, J. D.; Schirmer, K. Nanomaterials in the Environment: Behavior, Fate, Bioavailability, and Effects - An Updated Review. *Environ. Toxicol. Chem.* **2018**, *37*, 2029–2063.
- (125) Yahia Cherif, A.; Arous, O.; Mameri, N.; Zhu, J.; Ammi Said, A.; Vankelecom, I.; Simoens, K.; Bernaerts, K.; Van der Bruggen, B. Fabrication and Characterization of Novel Antimicrobial Thin Film Nano-Composite Membranes Based on Copper Nanoparticles. *J. Chem. Technol. Biotechnol.* **2018**, *93*, 2737–2747.
- (126) Hasheminya, S.-M.; Rezaei Mokarram, R.; Ghanbarzadeh, B.; Hamishekar, H.; Kafil, H. S. Physicochemical, Mechanical, Optical, Microstructural and Antimicrobial Properties of Novel Kefiran-Carboxymethyl Cellulose Biocomposite Films as Influenced by Copper Oxide Nanoparticles (CuONPs). *Food Packag. Shelf Life* **2018**, *17*, 196–204.
- (127) LewisOscar, F.; MubarakAli, D.; Nithya, C.; Priyanka, R.; Gopinath, V.; Alharbi, N. S.; Thajuddin, N. One Pot Synthesis and Anti-Biofilm Potential of Copper Nanoparticles (CuNPs) Against Clinical Strains of *Pseudomonas aeruginosa*. *Biofouling* **2015**, *31*, 379–391.
- (128) Kruk, T.; Szczepanowicz, K.; Stefańska, J.; Socha, R. P.; Warszński, P. Synthesis and Antimicrobial Activity of Monodisperse Copper Nanoparticles. *Colloids Surf., B* **2015**, *128*, 17–22.
- (129) Xie, Y.; Zhang, M.; Zhang, W.; Liu, X.; Zheng, W.; Jiang, X. Gold Nanoclusters-Coated Orthodontic Devices Can Inhibit the Formation of *Streptococcus mutans* Biofilm. *ACS Biomater. Sci. Eng.* **2020**, *6*, 1239–1246.
- (130) Ivanova, E. P.; Nguyen, S. H.; Guo, Y.; Baulin, V. A.; Webb, H. K.; Truong, V. K.; Wandiyanto, J. V.; Garvey, C. J.; Mahon, P. J.; Mainwaring, D. E.; et al. Bactericidal Activity of Self-Assembled Palmitic and Stearic Fatty Acid Crystals on Highly Ordered Pyrolytic Graphite. *Acta Biomater* **2017**, *59*, 148–157.
- (131) Yadav, N.; Dubey, A.; Shukla, S.; Saini, C. P.; Gupta, G.; Priyadarshini, R.; Lochab, B. Graphene Oxide-Coated Surface: Inhibition of Bacterial Biofilm Formation due to Specific Surface-Interface Interactions. *ACS Omega* **2017**, *2*, 3070–3082.
- (132) Kean, W. F.; Kean, I. R. L. Clinical Pharmacology of Gold. *Inflammopharmacology* **2008**, *16*, 112–125.
- (133) Thakor, A. S.; Jokerst, J.; Zavaleta, C.; Massoud, T. F.; Gambhir, S. S. Gold Nanoparticles: a Revival in Precious Metal Administration to Patients. *Nano Lett.* **2011**, *11*, 4029–4036.
- (134) Amin, R. M.; Mohamed, M. B.; Ramadan, M. A.; Verwanger, T.; Krammer, B. Rapid and Sensitive Microplate Assay for Screening the Effect of Silver and Gold Nanoparticles on Bacteria. *Nanomedicine* **2009**, *4*, 637–643.
- (135) Shankar, S.; Jaiswal, L.; Aparna, R.; Prasad, V. Synthesis, Characterization, *In Vitro* Biocompatibility, and Antimicrobial Activity of Gold, Silver and Gold Silver Alloy Nanoparticles Prepared from *Lansium domesticum* Fruit Peel Extract. *Mater. Lett.* **2014**, *137*, 75–78.
- (136) Yu, Q.; Li, J.; Zhang, Y.; Wang, Y.; Liu, L.; Li, M. Inhibition of Gold Nanoparticles (AuNPs) on Pathogenic Biofilm Formation and Invasion to Host Cells. *Sci. Rep.* **2016**, *6*, 26667 DOI: 10.1038/srep26667.
- (137) Chatterjee, S.; Bandyopadhyay, A.; Sarkar, K. Effect of Iron Oxide and Gold Nanoparticles on Bacterial Growth Leading Towards Biological Application. *J. Nanobiotechnol.* **2011**, *9*, 34.
- (138) Ahmad, T.; Wani, I. A.; Lone, I. H.; Ganguly, A.; Manzoor, N.; Ahmad, A.; Ahmed, J.; Al-Shihri, A. S. Antifungal Activity of Gold Nanoparticles Prepared by Solvothermal Method. *Mater. Res. Bull.* **2013**, *48*, 12–20.
- (139) Mukha, I.; Eremenko; Korchak, G.; Michienkova. Antibacterial Action and Physicochemical Properties of Stabilized Silver and Gold



- Nanostructures on the Surface of Disperse Silica. *J. Water Resour. Prot.* **2010**, *2*, 131–136.
- (140) Pham, T.; Jackson, J. B.; Halas, N. J.; Lee, T. R. Preparation and Characterization of Gold Nanoshells Coated with Self-Assembled Monolayers. *Langmuir* **2002**, *18*, 4915–4920.
- (141) Khantamat, O.; Li, C.-H.; Yu, F.; Jamison, A. C.; Shih, W.-C.; Cai, C.; Lee, T. R. Gold Nanoshell-Decorated Silicone Surfaces for the Near-Infrared (NIR) Photothermal Destruction of the Pathogenic Bacterium *E. faecalis*. *ACS Appl. Mater. Interfaces* **2015**, *7*, 3981–3993.
- (142) Cui, Y.; Zhao, Y.; Tian, Y.; Zhang, W.; Lü, X.; Jiang, X. The Molecular Mechanism of Action of Bactericidal Gold Nanoparticles on *Escherichia coli*. *Biomaterials* **2012**, *33*, 2327–2333.
- (143) Tiwari, P. M.; Vig, K.; Dennis, V. A.; Singh, S. R. Functionalized Gold Nanoparticles and their Biomedical Applications. *Nanomaterials* **2011**, *1*, 31–63.
- (144) Silvero, J.; Rocca, D. M.; de la Villarmois, E. A.; Fournier, K.; Lanterna, A. E.; Pérez, M. F.; Becerra, M. C.; Scaiano, J. C. Selective Photoinduced Antibacterial Activity of Amoxicillin-Coated Gold Nanoparticles: From One-Step Synthesis to *in Vivo* Cytocompatibility. *ACS Omega* **2018**, *3*, 1220–1230.
- (145) Allahverdiyev, A. M.; Kon, K. V.; Abamor, E. S.; Bagirova, M.; Rafailovich, M. Coping with Antibiotic Resistance: Combining Nanoparticles with Antibiotics and Other Antimicrobial Agents. *Expert Rev. Anti-Infect. Ther.* **2011**, *9*, 1035–1052.
- (146) Shen, X.; Hu, Y.; Xu, G.; Chen, W.; Xu, K.; Ran, Q.; Ma, P.; Zhang, Y.; Li, J.; Cai, K. Regulation of the Biological Functions of Osteoblasts and Bone Formation by Zn-Incorporated Coating on Microrough Titanium. *ACS Appl. Mater. Interfaces* **2014**, *6*, 16426–16440.
- (147) Huo, K.; Zhang, X.; Wang, H.; Zhao, L.; Liu, X.; Chu, P. K. Osteogenic Activity and Antibacterial Effects on Titanium Surfaces Modified with Zn-Incorporated Nanotube Arrays. *Biomaterials* **2013**, *34*, 3467–3478.
- (148) Costa, B. C.; Rodrigues, E. A.; Tokuhara, C. K.; Oliveira, R. C.; Lisboa-Filho, P. N.; Rocha, L. A. ZnO Nanoparticles with Different Sizes and Morphologies for Medical Implant Coatings: Synthesis and Cytotoxicity. *BioNanoScience* **2018**, *8*, 587–595.
- (149) Ruiz-Gómez, M. A.; Figueroa-Torres, M. Z.; Alonso-Lemus, I. L.; Vega-Becerra, O. E.; González-López, J. R.; Zaldívar-Cadena, A. A. Electroless Controllable Growth of ZnO Films and their Morphology-Dependent Antimicrobial Properties. *J. Hazard. Mater.* **2018**, *347*, 39–47.
- (150) Heinonen, S.; Kannisto, M.; Nikkanen, J.-P.; Huttunen-Saarivirta, E.; Karp, M.; Levänen, E. Photocatalytic and Antibacterial Properties of ZnO Films with Different Surface Topographies on Stainless Steel Substrate. *Thin Solid Films* **2016**, *616*, 842–849.
- (151) Carvalho, P.; Sampaio, P.; Azevedo, S.; Vaz, C.; Espinós, J. P.; Teixeira, V.; Carneiro, J. O. Influence of Thickness and Coatings Morphology in the Antimicrobial Performance of Zinc Oxide Coatings. *Appl. Surf. Sci.* **2014**, *307*, 548–557.
- (152) Petrochenko, P. E.; Skoog, S. A.; Zhang, Q.; Comstock, D. J.; Elam, J. W.; Goering, P. L.; Narayan, R. J. Cytotoxicity of Cultured Macrophages Exposed to Antimicrobial Zinc Oxide (ZnO) Coatings on Nanoporous Aluminum Oxide Membranes. *Biomatter* **2013**, *3*, 25528 DOI: 10.4161/biom.25528.
- (153) Petrochenko, P. E.; Zhang, Q.; Bayati, R.; Skoog, S. A.; Phillips, K. S.; Kumar, G.; Narayan, R. J.; Goering, P. L. Cytotoxic Evaluation of Nanostructured Zinc Oxide (ZnO) Thin Films and Leachates. *Toxicol. In Vitro* **2014**, *28*, 1144–1152.
- (154) Lewinski, N. A.; Avrutin, V.; Izadi, T.; Secondo, L. E.; Ullah, M. B.; Özgür, Ü.; Morkoc, H.; Topsisakal, E. Influence of ZnO Thin Film Crystallinity on: *In Vitro* Biocompatibility. *Toxicol. Res. (Cambridge, U. K.)* **2018**, *7*, 754–759.
- (155) Nag, S.; Banerjee, R. Fundamentals of Medical Implant Materials. *ASM Handbook* **2012**, *23*, 6–17.
- (156) Fujishima, A.; Honda, K. Electrochemical Photolysis of Water at a Semiconductor Electrode. *Nature* **1972**, *238*, 37.
- (157) Huang, Y.-Y.; Choi, H.; Kushida, Y.; Bhayana, B.; Wang, Y.; Hamblin, M. R. Broad-Spectrum Antimicrobial Effects of Photocatalysis Using Titanium Dioxide Nanoparticles Are Strongly Potentiated by Addition of Potassium Iodide. *Antimicrob. Agents Chemother.* **2016**, *60*, 5445.
- (158) Shah, R. R.; Kaewgun, S.; Lee, B. I.; Tzeng, T.-R. J. The Antibacterial Effects of Biphasic Brookite-Anatase Titanium Dioxide Nanoparticles on Multiple-Drug-Resistant *Staphylococcus aureus*. *J. Biomed. Nanotechnol.* **2008**, *4*, 339–348.
- (159) Miyagi, T.; Kamei, M.; Mitsubashi, T.; Ishigaki, T.; Yamazaki, A. Charge Separation at the Rutile/Anatase Interface: a Dominant Factor of Photocatalytic Activity. *Chem. Phys. Lett.* **2004**, *390*, 399–402.
- (160) Gaya, U. I.; Abdullah, A. H. Heterogeneous Photocatalytic Degradation of Organic Contaminants over Titanium Dioxide: A Review of Fundamentals, Progress and Problems. *J. Photochem. Photobiol., C* **2008**, *9*, 1–12.
- (161) Muranyi, P.; Schraml, C.; Wunderlich, J. Antimicrobial Efficiency of Titanium Dioxide-Coated Surfaces. *J. Appl. Microbiol.* **2009**, *108*, 1966–1973.
- (162) Visai, L.; De Nardo, L.; Punta, C.; Melone, L.; Cigada, A.; Imbriani, M.; Arciola, C. R. Titanium Oxide Antibacterial Surfaces in Biomedical Devices. *Int. J. Artif. Organs* **2011**, *34*, 929–946.
- (163) Vatansever, F.; de Melo, W. C. M. A.; Avci, P.; Vecchio, D.; Sadasivam, M.; Gupta, A.; Chandran, R.; Karimi, M.; Parizotto, N. A.; Yin, R.; et al. Antimicrobial Strategies Centered Around Reactive Oxygen Species – Bactericidal Antibiotics, Photodynamic Therapy, and Beyond. *FEMS Microbiol. Rev.* **2013**, *37*, 955–989.
- (164) Binas, V.; Venieri, D.; Kotzias, D.; Kiriakidis, G. Modified TiO<sub>2</sub> Based Photocatalysts for Improved Air and Health Quality. *J. Materiomics* **2017**, *3*, 3–16.
- (165) Shukla, R. K.; Sharma, V.; Pandey, A. K.; Singh, S.; Sultana, S.; Dhawan, A. ROS-Mediated Genotoxicity Induced by Titanium Dioxide Nanoparticles in Human Epidermal Cells. *Toxicol. In Vitro* **2011**, *25*, 231–241.
- (166) Ramkumar, K. M.; Manjula, C.; GnanaKumar, G.; Kanjwal, M. A.; Sekar, T. V.; Paulmurugan, R.; Rajaguru, P. Oxidative Stress-Mediated Cytotoxicity and Apoptosis Induction by TiO<sub>2</sub> Nanofibers in HeLa Cells. *Eur. J. Pharm. Biopharm.* **2012**, *81*, 324–333.
- (167) Dalai, S.; Pakrashi, S.; Chandrasekaran, N.; Mukherjee, A. Acute Toxicity of TiO<sub>2</sub> Nanoparticles to *Ceriodaphnia dubia* Under Visible Light and Dark Conditions in a Freshwater System. *PLoS One* **2013**, *8*, e62970.
- (168) Dalai, S.; Pakrashi, S.; Kumar, R. S. S.; Chandrasekaran, N.; Mukherjee, A. A Comparative Cytotoxicity Study of TiO<sub>2</sub> Nanoparticles Under Light and Dark Conditions at Low Exposure Concentrations. *Toxicol. Res. (Cambridge, U. K.)* **2012**, *1*, 116–130.
- (169) Salehi, P.; Babanouri, N.; Roiein-Peikar, M.; Zare, F. Long-Term Antimicrobial Assessment of Orthodontic Brackets Coated with Nitrogen-Doped Titanium Dioxide Against *Streptococcus mutans*. *Prog. Orthod.* **2018**, *19*, 35.
- (170) Hwang, J.-S.; Yu, J.; Kim, H.-M.; Oh, J.-M.; Choi, S.-J. Food Additive Titanium Dioxide and Its Fate in Commercial Foods. *Nanomaterials* **2019**, *9*, 1175.
- (171) Proquin, H.; Rodríguez-Ibarra, C.; Moonen, C. G. J.; Urrutia Ortega, I. M.; Briedé, J. J.; de Kok, T. M.; van Loveren, H.; Chirino, Y. I. Titanium Dioxide Food Additive (E171) Induces ROS Formation and Genotoxicity: Contribution of Micro and Nano-Sized Fractions. *Mutagenesis* **2017**, *32*, 139–149.
- (172) Re-evaluation of Titanium Dioxide (E171) as a Food Additive. *EFSA J.* **2016**, *14*, e04545.
- (173) Cai, Y.; Strømme, M.; Welch, K. Photocatalytic Antibacterial Effects Are Maintained On Resin-Based TiO<sub>2</sub> Nanocomposites After Cessation of UV Irradiation. *PLoS One* **2013**, *8*, e75929.
- (174) Sadiq, I. M.; Chowdhury, B.; Chandrasekaran, N.; Mukherjee, A. Antimicrobial Sensitivity of *Escherichia coli* to Alumina Nanoparticles. *Nanomedicine: NBM* **2009**, *5*, 282–286.
- (175) Ansari, M. A.; Khan, H. M.; Khan, A. A.; Pal, R.; Cameotra, S. S. Antibacterial Potential of Al<sub>2</sub>O<sub>3</sub> Nanoparticles Against Multidrug Resistance Strains of *Staphylococcus aureus* Isolated from Skin Exudates. *J. Nanopart. Res.* **2013**, *15*, 1970.



- (176) Manikandan, V.; Jayanthi, P.; Priyadharsan, A.; Vijayaparthap, E.; Anbarasan, P. M.; Velmurugan, P. Green Synthesis of pH-responsive  $\text{Al}_2\text{O}_3$  Nanoparticles: Application to Rapid Removal of Nitrate Ions with Enhanced Antibacterial Activity. *J. Photochem. Photobiol., A: Chemistry* **2019**, *371*, 205–215.
- (177) Doskocz, N.; Affek, K.; Załęska-Radziwiłł, M. Effects of Aluminium Oxide Nanoparticles on Bacterial Growth. *E3S Web Conf.* **2019**, *17*, 00019.
- (178) Hammad, S. M.; El-Wassefy, N. A.; Shamaa, M. S.; Fathy, A. Evaluation of Zinc-Oxide Nanocoating on the Characteristics and Antibacterial Behavior of Nickel-Titanium Alloy. *Dental Press J. Orthod* **2020**, *25*, 51–58.
- (179) Oleshko, O.; Husak, Y.; Korniienko, V.; Pshenychnyi, R.; Varava, Y.; Kalinkevich, O.; Pisarek, M.; Grundsteins, K.; Pogorielova, O.; Mishchenko, O.; et al. Biocompatibility and Antibacterial Properties of ZnO-Incorporated Anodic Oxide Coatings on TiZrNb Alloy. *Nanomaterials* **2020**, *10*, 2401.
- (180) Wang, X.; Fan, H.; Zhang, F.; Zhao, S.; Liu, Y.; Xu, Y.; Wu, R.; Li, D.; Yang, Y.; Liao, L.; et al. Antibacterial Properties of Bilayer Biomimetic Nano-ZnO for Dental Implants. *ACS Biomater. Sci. Eng.* **2020**, *6*, 1880–1886.
- (181) Thapa, R.; Bhagat, C.; Shrestha, P.; Awal, S.; Dudhagara, P. Enzyme-Mediated Formulation of Stable Elliptical Silver Nanoparticles Tested Against Clinical Pathogens and MDR Bacteria and Development of Antimicrobial Surgical Thread. *Ann. Clin. Microbiol. Antimicrob.* **2017**, *16*, 39.
- (182) Paladini, F.; Di Franco, C.; Panico, A.; Scamarcio, G.; Sannino, A.; Pollini, M. *In Vitro* Assessment of the Antibacterial Potential of Silver Nano-Coatings on Cotton Gauzes for Prevention of Wound Infections. *Materials* **2016**, *9*, 411.
- (183) Petkova, P.; Francesko, A.; Perelshtein, I.; Gedanken, A.; Tzanov, T. Simultaneous Sonochemical-Enzymatic Coating of Medical Textiles with Antibacterial ZnO Nanoparticles. *Ultrason. Sonochem.* **2016**, *29*, 244–250.
- (184) Eshed, M.; Lellouche, J.; Matalon, S.; Gedanken, A.; Banin, E. Sonochemical Coatings of ZnO and CuO Nanoparticles Inhibit *Streptococcus mutans* Biofilm Formation on Teeth Model. *Langmuir* **2012**, *28*, 12288–12295.
- (185) Aboelzahab, A.; Azad, A.-M.; Dolan, S.; Goel, V. Mitigation of *Staphylococcus aureus*-Mediated Surgical Site Infections with IR Photoactivated  $\text{TiO}_2$  coatings on Ti Implants. *Adv. Healthcare Mater.* **2012**, *1*, 285–291.
- (186) Szunerits, S.; Boukherroub, R. Antibacterial Activity of Graphene-Based Materials. *J. Mater. Chem. B* **2016**, *4*, 6892–6912.
- (187) Cha, C.; Shin, S. R.; Annabi, N.; Dokmeci, M. R.; Khademhosseini, A. Carbon-Based Nanomaterials: Multifunctional Materials for Biomedical Engineering. *ACS Nano* **2013**, *7*, 2891–2897.
- (188) Henriques, P. C.; Borges, I.; Pinto, A. M.; Magalhães, F. D.; Gonçalves, I. C. Fabrication and Antimicrobial Performance of Surfaces Integrating Graphene-Based Materials. *Carbon* **2018**, *132*, 709–732.
- (189) Akhavan, O.; Ghaderi, E. Toxicity of Graphene and Graphene Oxide Nanowalls Against Bacteria. *ACS Nano* **2010**, *4*, 5731–5736.
- (190) Chen, J.; Peng, H.; Wang, X.; Shao, F.; Yuan, Z.; Han, H. Graphene Oxide Exhibits Broad-Spectrum Antimicrobial Activity Against Bacterial Phytopathogens and Fungal Conidia by Intertwining and Membrane Perturbation. *Nanoscale* **2014**, *6*, 1879–1889.
- (191) Choudhary, P.; Parandhaman, T.; Ramalingam, B.; Duraipandy, N.; Kiran, M. S.; Das, S. K. Fabrication of Nontoxic Reduced Graphene Oxide Protein Nanoframework as Sustained Antimicrobial Coating for Biomedical Application. *ACS Appl. Mater. Interfaces* **2017**, *9*, 38255–38269.
- (192) Liu, S.; Zeng, T. H.; Hofmann, M.; Burcombe, E.; Wei, J.; Jiang, R.; Kong, J.; Chen, Y. Antibacterial Activity of Graphite, Graphite Oxide, Graphene Oxide, and Reduced Graphene Oxide: Membrane and Oxidative Stress. *ACS Nano* **2011**, *5*, 6971–6980.
- (193) Gurunathan, S.; Han, J. W.; Abdal Dayem, A.; Eppakayala, V.; Kim, J. H. Oxidative Stress-Mediated Antibacterial Activity of Graphene Oxide and Reduced Graphene Oxide in *Pseudomonas aeruginosa*. *Int. J. Nanomed.* **2012**, *7*, 5901–5914.
- (194) Lovley, D. R.; Coates, J. D.; Blunt-Harris, E. L.; Phillips, E. J. P.; Woodward, J. C. Humic Substances as Electron Acceptors for Microbial Respiration. *Nature* **1996**, *382*, 445–448.
- (195) Li, J.; Wang, G.; Zhu, H.; Zhang, M.; Zheng, X.; Di, Z.; Liu, X.; Wang, X. Antibacterial Activity of Large-Area Monolayer Graphene Film Manipulated by Charge Transfer. *Sci. Rep.* **2014**, *4*, 4359.
- (196) Zou, X.; Zhang, L.; Wang, Z.; Luo, Y. Mechanisms of the Antimicrobial Activities of Graphene Materials. *J. Am. Chem. Soc.* **2016**, *138*, 2064–2077.
- (197) Hegab, H. M.; ElMekawy, A.; Zou, L.; Mulcahy, D.; Saint, C. P.; Ginic-Markovic, M. The Controversial Antibacterial Activity of Graphene-Based Materials. *Carbon* **2016**, *105*, 362–376.
- (198) Dybowska, S.; Kotela, A.; Krzemi, ski, J.; Wróblewska, M.; Marchel, H.; Romaniec, M.; gosz, P.; Jakubowska, M. Graphene Nanolayers as a New Method for Bacterial Biofilm Prevention: Preliminary Results. *Journal of AOAC International* **2017**, *100*, 900–904.
- (199) Liu, Y.; Wen, J.; Gao, Y.; Li, T.; Wang, H.; Yan, H.; Niu, B.; Guo, R. Antibacterial Graphene Oxide Coatings on Polymer Substrate. *Appl. Surf. Sci.* **2018**, *436*, 624–630.
- (200) Choudhary, P.; Das, S. K. Bio-Reduced Graphene Oxide as a Nanoscale Antimicrobial Coating for Medical Devices. *ACS Omega* **2019**, *4*, 387–397.
- (201) Mocan, T.; Matea, C. T.; Pop, T.; Mosteanu, O.; Buzoianu, A. D.; Suci, S.; Puia, C.; Zdrehus, C.; Iancu, C.; Mocan, L. Carbon Nanotubes as Anti-Bacterial Agents. *Cell. Mol. Life Sci.* **2017**, *74*, 3467–3479.
- (202) Sah, U.; Sharma, K.; Chaudhri, N.; Sankar, M.; Gopinath, P. Antimicrobial Photodynamic Therapy: Single-Walled Carbon Nanotube (SWCNT)-Porphyrin Conjugate for Visible Light Mediated Inactivation of *Staphylococcus aureus*. *Colloids Surf. B* **2018**, *162*, 108–117.
- (203) Vt, A.; Paramanatham, P.; Sb, S. L.; Sharan, A.; Alsaedi, M. H.; Dawoud, T. M. S.; Asad, S.; Busi, S. Antimicrobial Photodynamic Activity of Rose Bengal Conjugated Multi Walled Carbon Nanotubes Against Planktonic Cells and Biofilm of *Escherichia coli*. *Photodiagnosis and Photodynamic Therapy* **2018**, *24*, 300–310.
- (204) Deokar, A. R.; Lin, L.-Y.; Chang, C.-C.; Ling, Y.-C. Single-Walled Carbon Nanotube Coated Antibacterial Paper: Preparation and Mechanistic Study. *J. Mater. Chem. B* **2013**, *1*, 2639–2646.
- (205) Hetrick, E. M.; Shin, J. H.; Paul, H. S.; Schoenfisch, M. H. Anti-Biofilm Efficacy of Nitric Oxide-Releasing Silica Nanoparticles. *Biomaterials* **2009**, *30*, 2782–2789.
- (206) Cousins, B. G.; Allison, H. E.; Doherty, P. J.; Edwards, C.; Garvey, M. J.; Martin, D. S.; Williams, R. L. Effects of a Nanoparticulate Silica Substrate on Cell Attachment of *Candida albicans*. *J. Appl. Microbiol.* **2007**, *102*, 757–765.
- (207) Gaikwad, R. M.; Sokolov, I. Silica Nanoparticles to Polish Tooth Surfaces for Caries Prevention. *Journal of Dental Research* **2008**, *87*, 980–983.
- (208) Jia, Z.; Xiu, P.; Li, M.; Xu, X.; Shi, Y.; Cheng, Y.; Wei, S.; Zheng, Y.; Xi, T.; Cai, H.; et al. Bioinspired Anchoring AgNPs Onto Micro-Nanoporous  $\text{TiO}_2$  Orthopedic Coatings: Trap-Killing of Bacteria, Surface-Regulated Osteoblast Functions and Host Responses. *Biomaterials* **2016**, *75*, 203–222.
- (209) Verma, J.; Bhattacharya, A. Development of Coating Formulation with Silica-Titania Core-Shell Nanoparticles Against Pathogenic Fungus. *R. Soc. Open Sci.* **2018**, *5*, 180633.
- (210) Rabea, E. I.; Badawy, M. E. T.; Stevens, C. V.; Smagghe, G.; Steurbaut, W. Chitosan as Antimicrobial Agent: Applications and Mode of Action. *Biomacromolecules* **2003**, *4*, 1457–1465.
- (211) Jayakumar, R.; Prabakaran, M.; Nair, S. V.; Tamura, H. Novel Chitin and Chitosan Nanofibers in Biomedical Applications. *Biotechnology Advances* **2010**, *28*, 142–150.
- (212) Palla-Rubio, B.; Araújo-Gomes, N.; Fernández-Gutiérrez, M.; Rojo, L.; Suay, J.; Gurruchaga, M.; Goñi, I. Synthesis and Characterization of Silica-Chitosan Hybrid Materials as Antibacterial Coatings for Titanium Implants. *Carbohydr. Polym.* **2019**, *203*, 331–341.

- (213) Rupp, F.; Gittens, R. A.; Scheideler, L.; Marmur, A.; Boyan, B. D.; Schwartz, Z.; Geis-Gerstorfer, J. A Review on the Wettability of Dental Implant Surfaces I: Theoretical and Experimental Aspects. *Acta Biomater* **2014**, *10*, 2894–2906.
- (214) Mouro, C.; Dunne, C. P.; Gouveia, I. C. Designing New Antibacterial Wound Dressings: Development of a Dual Layer Cotton Material Coated with Poly(Vinyl Alcohol) Chitosan Nanofibers Incorporating *Agrimonia eupatoria* L. Extract. *Molecules* **2021**, *26*, 83.
- (215) Borges, I.; Henriques, P. C.; Gomes, R. N.; Pinto, A. M.; Pestana, M.; Magalhães, F. D.; Gonçalves, I. C. Exposure of Smaller and Oxidized Graphene on Polyurethane Surface Improves its Antimicrobial Performance. *Nanomaterials* **2020**, *10*, 349.
- (216) Pandit, S.; Gaska, K.; Mokkaapati, V. R. S. S.; Celauro, E.; Derouiche, A.; Forsberg, S.; Svensson, M.; Kádár, R.; Mijakovic, I. Precontrolled Alignment of Graphite Nanoplatelets in Polymeric Composites Prevents Bacterial Attachment. *Small* **2020**, *16*, 1904756.
- (217) Jiang, N.; Wang, Y.; Chan, K. C.; Chan, C.-Y.; Sun, H.; Li, G. Additive Manufactured Graphene Coating with Synergistic Photo-thermal and Superhydrophobic Effects for Bactericidal Applications. *Global Challenges* **2020**, *4*, 1900054.
- (218) Li, B.; Xia, X.; Guo, M.; Jiang, Y.; Li, Y.; Zhang, Z.; Liu, S.; Li, H.; Liang, C.; Wang, H. Biological and Antibacterial Properties of the Micro-Nanostructured Hydroxyapatite/Chitosan Coating on Titanium. *Sci. Rep.* **2019**, *9*, 14052 DOI: 10.1038/s41598-019-49941-0.
- (219) Vakili, N.; Asefnejad, A. Titanium Coating: Introducing an Antibacterial and Bioactive Chitosan-Alginate Film on Titanium by Spin Coating. *Biomedical Engineering* **2020**, *65*, 621–630.
- (220) Farid, M. U.; Guo, J.; An, A. K. Bacterial Inactivation and *In Situ* Monitoring of Biofilm Development on Graphene Oxide Membrane Using Optical Coherence Tomography. *J. Membr. Sci.* **2018**, *564*, 22–34.
- (221) Ouyang, L.; Deng, Y.; Yang, L.; Shi, X.; Dong, T.; Tai, Y.; Yang, W.; Chen, Z.-G. Graphene-Oxide-Decorated Microporous Polyether-etherketone with Superior Antibacterial Capability and *In Vitro* Osteogenesis for Orthopedic Implant. *Macromol. Biosci.* **2018**, *18*, 1800036.
- (222) Thampi, S.; Nandkumar, A. M.; Muthuvijayan, V.; Parameswaran, R. Differential Adhesive and Bioactive Properties of the Polymeric Surface Coated with Graphene Oxide Thin Film. *ACS Appl. Mater. Interfaces* **2017**, *9*, 4498–4508.
- (223) Yadav, N.; Dubey, A.; Shukla, S.; Saini, C. P.; Gupta, G.; Priyadarshini, R.; Lochab, B. Graphene Oxide-Coated Surface: Inhibition of Bacterial Biofilm Formation due to Specific Surface–Interface Interactions. *ACS Omega* **2017**, *2*, 3070–3082.
- (224) Ivanova, E. P.; Hasan, J.; Webb, H. K.; Truong, V. K.; Watson, G. S.; Watson, J. A.; Baulin, V. A.; Pogodin, S.; Wang, J. Y.; Tobin, M. J.; et al. Natural Bactericidal Surfaces: Mechanical Rupture of *Pseudomonas aeruginosa* Cells by Cicada Wings. *Small* **2012**, *8*, 2489–2494.
- (225) Ivanova, E. P.; Hasan, J.; Webb, H. K.; Gervinskas, G.; Juodkazis, S.; Truong, V. K.; Wu, A. H. F.; Lamb, R. N.; Baulin, V. A.; Watson, G. S.; et al. Bactericidal Activity of Black Silicon. *Nat. Commun.* **2013**, *4*, 2838.
- (226) Jenkins, J.; Mantell, J.; Neal, C.; Gholinia, A.; Verkade, P.; Nobbs, A. H.; Su, B. Antibacterial Effects of Nanopillar Surfaces Are Mediated by Cell Impedance, Penetration and Induction of Oxidative Stress. *Nat. Commun.* **2020**, *11*, 1626.
- (227) Banerjee, I.; Pangule, R. C.; Kane, R. S. Antifouling Coatings: Recent Developments in the Design of Surfaces That Prevent Fouling by Proteins, Bacteria, and Marine Organisms. *Adv. Mater.* **2011**, *23*, 690–718.
- (228) McWhorter, F. Y.; Wang, T.; Nguyen, P.; Chung, T.; Liu, W. F. Modulation of Macrophage Phenotype By Cell Shape. *Proc. Natl. Acad. Sci. U. S. A.* **2013**, *110*, 17253–17258.
- (229) Chen, S.; Jones, J. A.; Xu, Y.; Low, H. Y.; Anderson, J. M.; Leong, K. W. Characterization of Topographical Effects on Macrophage Behavior in a Foreign Body Response Model. *Biomaterials* **2010**, *31*, 3479–3491.
- (230) Crawford, R. J.; Webb, H. K.; Truong, V. K.; Hasan, J.; Ivanova, E. P. Surface Topographical Factors Influencing Bacterial Attachment. *Adv. Colloid Interface Sci.* **2012**, *179*, 142–149.
- (231) Mitik-Dineva, N.; Wang, J.; Mocanasi, R. C.; Stoddart, P. R.; Crawford, R. J.; Ivanova, E. P. Impact of Nano-Topography on Bacterial Attachment. *Biotechnology Journal* **2008**, *3*, 536–544.
- (232) Friedlander, R. S.; Vlamakis, H.; Kim, P.; Khan, M.; Kolter, R.; Aizenberg, J. Bacterial Flagella Explore Microscale Hummocks and Hollows to Increase Adhesion. *Proc. Natl. Acad. Sci. U. S. A.* **2013**, *110*, 5624–5629.
- (233) Mi, G.; Shi, D.; Wang, M.; Webster, T. J. Reducing Bacterial Infections and Biofilm Formation Using Nanoparticles and Nanostructured Antibacterial Surfaces. *Adv. Healthcare Mater.* **2018**, *7*, 1800103.
- (234) Zheng, S.; Bawazir, M.; Dhall, A.; Kim, H.-E.; He, L.; Heo, J.; Hwang, G. Implication of Surface Properties, Bacterial Motility, and Hydrodynamic Conditions on Bacterial Surface Sensing and Their Initial Adhesion. *Front. Bioeng. Biotechnol.* **2021**, *9*, 9.
- (235) Albrektsson, T.; Wennerberg, A. Review Focusing on Topographic and Chemical Properties of Different Surfaces and *In Vivo* Responses to Them. *Int. J. Prosthodont.* **2004**, *17*, 536–543.
- (236) Teughels, W.; Van Assche, N.; Sliopen, I.; Quirynen, M. Effect of Material Characteristics and/or Surface Topography on Biofilm Development. *Clin. Oral Implants Res.* **2006**, *17*, 68–81.
- (237) Ivanova, E. P.; Hasan, J.; Webb, H. K.; Truong, V. K.; Watson, G. S.; Watson, J. A.; Baulin, V. A.; Pogodin, S.; Wang, J. Y.; Tobin, M. J.; et al. Natural Bactericidal Surfaces: Mechanical Rupture of *Pseudomonas aeruginosa* Cells by Cicada Wings. *Small* **2012**, *8*, 2489–2494.
- (238) Pogodin, S.; Hasan, J.; Baulin, V. A.; Webb, H. K.; Truong, V. K.; Phong Nguyen, T. H.; Boshkovik, V.; Fluke, C. J.; Watson, G. S.; Watson, J. A.; et al. Biophysical Model of Bacterial Cell Interactions with Nanopatterned Cicada Wing Surfaces. *Biophys. J.* **2013**, *104*, 835–840.
- (239) Bandara, C. D.; Singh, S.; Afara, I. O.; Wolff, A.; Tesfamichael, T.; Ostrikov, K.; Oloyede, A. Bactericidal Effects of Natural Nanotopography of Dragonfly Wing on *Escherichia coli*. *ACS Appl. Mater. Interfaces* **2017**, *9*, 6746–6760.
- (240) Li, X.; Chen, T. Enhancement and Suppression Effects of a Nanopatterned Surface on Bacterial Adhesion. *Phys. Rev. E* **2016**, *93*, 052419 DOI: 10.1103/PhysRevE.93.052419.
- (241) Tuson, H. H.; Auer, G. K.; Renner, L. D.; Hasebe, M.; Tropini, C.; Salick, M.; Crone, W. C.; Gopinathan, A.; Huang, K. C.; Weibel, D. B. Measuring the Stiffness of Bacterial Cells from Growth Rates in Hydrogels of Tunable Elasticity. *Mol. Microbiol.* **2012**, *84*, 874–891.
- (242) Nikolaeva, N. I.; Muller, T.; Williams, D. J.; Liu, Y. Changes in the Stiffness of Human Mesenchymal Stem Cells with the Progress of Cell Death as Measured by Atomic Force Microscopy. *J. Biomech.* **2014**, *47*, 625–630.
- (243) Hanson, L.; Lin, Z. C.; Xie, C.; Cui, Y.; Cui, B. Characterization of the Cell–Nanopillar Interface by Transmission Electron Microscopy. *Nano Lett.* **2012**, *12*, 5815–5820.
- (244) Diu, T.; Faruqui, N.; Sjöström, T.; Lamarre, B.; Jenkinson, H. F.; Su, B.; Ryadnov, M. G. Cicada-Inspired Cell-Instructive Nanopatterned Arrays. *Sci. Rep.* **2014**, *4*, 7122.
- (245) Wu, S.; Zuber, F.; Brugger, J.; Maniura-Weber, K.; Ren, Q. Antibacterial Au Nanostructured Surfaces. *Nanoscale* **2016**, *8*, 2620–2625.
- (246) Sjöström, T.; Nobbs, A. H.; Su, B. Bactericidal Nanospire Surfaces via Thermal Oxidation of Ti Alloy Substrates. *Mater. Lett.* **2016**, *167*, 22–26.
- (247) Ghosh, S.; Niu, S.; Yankova, M.; Mecklenburg, M.; King, S. M.; Ravichandran, J.; Kalia, R. K.; Nakano, A.; Vashishta, P.; Setlow, P. Analysis of Killing of Growing Cells and Dormant and Germinated Spores of *Bacillus* Species by Black Silicon Nanopillars. *Sci. Rep.* **2017**, *7*, 17768 DOI: 10.1038/s41598-017-18125-z.
- (248) Hazell, G.; May, P. W.; Taylor, P.; Nobbs, A. H.; Welch, C. C.; Su, B. Studies of Black Silicon and Black Diamond as Materials for Antibacterial Surfaces. *Biomater. Sci.* **2018**, *6*, 1424–1432.



- (249) Bhadra, C. M.; Werner, M.; Baulin, V. A.; Truong, V. K.; Kobaisi, M. A.; Nguyen, S. H.; Balcytis, A.; Juodkakis, S.; Wang, J. Y.; Mainwaring, D. E.; et al. Subtle Variations in Surface Properties of Black Silicon Surfaces Influence the Degree of Bactericidal Efficiency. *Nano-Micro Lett.* **2018**, *10*, 36.
- (250) Hasan, J.; Raj, S.; Yadav, L.; Chatterjee, K. Engineering a Nanostructured "Super Surface" with Superhydrophobic and Superkilling Properties. *RSC Adv.* **2015**, *5*, 44953–44959.
- (251) Pham, V. T. H.; Truong, V. K.; Orłowska, A.; Ghanaati, S.; Barbeck, M.; Booms, P.; Fulcher, A. J.; Bhadra, C. M.; Buividas, R.; Baulin, V.; et al. Race for the Surface: Eukaryotic Cells Can Win. *ACS Appl. Mater. Interfaces* **2016**, *8*, 22025–22031.
- (252) Ya'ari, S.; Halperin-Sternfeld, M.; Rosin, B.; Adler-Abramovich, L. Surface Modification by Nano-Structures Reduces Viable Bacterial Biofilm in Aerobic and Anaerobic Environments. *Int. J. Mol. Sci.* **2020**, *21*, 7370.
- (253) Hasan, J.; Jain, S.; Padmarajan, R.; Purighalla, S.; Sambandamurthy, V. K.; Chatterjee, K. Multi-Scale Surface Topography to Minimize Adherence and Viability of Nosocomial Drug-Resistant Bacteria. *Mater. Des.* **2018**, *140*, 332–344.
- (254) Yuan, Y.; Zhang, Y. Enhanced Biomimic Bactericidal Surfaces by Coating with Positively-Charged ZIF Nano-Dagger Arrays. *Nanomedicine: NBM* **2017**, *13*, 2199–2207.
- (255) Fisher, L. E.; Yang, Y.; Yuen, M.-F.; Zhang, W.; Nobbs, A. H.; Su, B. Bactericidal Activity of Biomimetic Diamond Nanocone Surfaces. *Biointerphases* **2016**, *11*, 011014.
- (256) Work, W. J.; Horie, K.; Hess, M.; Stepto, R. F. T. Definition of Terms Related to Polymer Blends, Composites, and Multiphase Polymeric Materials (IUPAC Recommendations 2004). *Pure Appl. Chem.* **2004**, *76*, 1985–2007.
- (257) Jones, R. M. *Mechanics of Composite Materials*, 2nd ed.; CRC Press, 1998.
- (258) Chen, B.; Evans, J. R. G.; Greenwell, H. C.; Boulet, P.; Coveney, P. V.; Bowden, A. A.; Whiting, A. A Critical Appraisal of Polymer–Clay Nanocomposites. *Chem. Soc. Rev.* **2008**, *37*, 568–594.
- (259) Zheng, Z.; Yin, W.; Zara, J. N.; Li, W.; Kwak, J.; Mamidi, R.; Lee, M.; Siu, R. K.; Ngo, R.; Wang, J.; et al. The Use of BMP-2 Coupled–Nanosilver-PLGA Composite Grafts to Induce Bone Repair in Grossly Infected Segmental Defects. *Biomaterials* **2010**, *31*, 9293–9300.
- (260) Stevanović, M.; Filipović, N.; Djurdjević, J.; Lukić, M.; Milenković, M.; Boccaccini, A. 45S5Bioglass®-based Scaffolds Coated with Selenium Nanoparticles or with Poly(lactide-co-glycolide)/Selenium Particles: Processing, Evaluation and Antibacterial Activity. *Colloids Surf., B* **2015**, *132*, 208–215.
- (261) Ferracane, J. L. Resin Composite - State of the Art. *Dent Mater.* **2011**, *27*, 29–38.
- (262) Szczesio-Włodarczyk, A.; Sokolowski, J.; Kleczewska, J.; Bociog, K. Ageing of Dental Composites Based on Methacrylate Resins - A Critical Review of the Causes and Method of Assessment. *Polymers* **2020**, *12*, 882.
- (263) Cao, W.; Zhang, Y.; Wang, X.; Chen, Y.; Li, Q.; Xing, X.; Xiao, Y.; Peng, X.; Ye, Z. Development of a Novel Resin-Based Dental Material with Dual Biocidal Modes and Sustained Release of Ag<sup>+</sup> Ions Based on Photocurable Core-Shell AgBr/Cationic Polymer Nanocomposites. *J. Mater. Sci.: Mater. Med.* **2017**, *28*, 103.
- (264) Chen, S.; Yang, J.; Jia, Y.-G.; Lu, B.; Ren, L. A Study of 3D-Printable Reinforced Composite Resin: PMMA Modified with Silver Nanoparticles Loaded Cellulose Nanocrystal. *Materials* **2018**, *11*, 2444.
- (265) Totu, E. E.; Nechifor, A. C.; Nechifor, G.; Aboul-Enein, H. Y.; Cristache, C. M. Poly(methyl methacrylate) with TiO<sub>2</sub> Nanoparticles Inclusion for Stereolithographic Complete Denture Manufacturing - the Future in Dental Care for Elderly Edentulous Patients? *J. Dent* **2017**, *59*, 68–77.
- (266) Giti, R.; Zomorodian, K.; Firouzmandi, M.; Zareshahrabadi, Z.; Rahmannasab, S. Antimicrobial Activity of Thermocycled Polymethyl Methacrylate Resin Reinforced with Titanium Dioxide and Copper Oxide Nanoparticles. *Int. J. Dent.* **2021**, *2021*, 6690806.
- (267) Wu, Z.; Xu, H.; Xie, W.; Wang, M.; Wang, C.; Gao, C.; Gu, F.; Liu, J.; Fu, J. Study on a Novel Antibacterial Light-Cured Resin Composite Containing Nano-MgO. *Colloids Surf., B* **2020**, *188*, 110774.
- (268) Dias, H. B.; Bernardi, M. I. B.; Bauab, T. M.; Hernandez, A. C.; de Souza Rastelli, A. N. Titanium Dioxide and Modified Titanium Dioxide by Silver Nanoparticles as an Anti-Biofilm Filler Content for Composite Resins. *Dent. Mater.* **2019**, *35*, 36–46.
- (269) Garcia, I. M.; Leitune, V. C. B.; Visioli, F.; Samuel, S. M. W.; Collares, F. M. Influence of Zinc Oxide Quantum Dots in the Antibacterial Activity and Cytotoxicity of an Experimental Adhesive Resin. *J. Dent. (Oxford, U. K.)* **2018**, *73*, 57–60.
- (270) Sodagar, A.; Akhavan, A.; Hashemi, E.; Arab, S.; Pourhajibagher, M.; Sodagar, K.; Kharrazifard, M. J.; Bahador, A. Evaluation of the Antibacterial Activity of a Conventional Orthodontic Composite Containing Silver/Hydroxyapatite Nanoparticles. *Prog. Orthod* **2016**, *17*, 40.
- (271) Melo, M. A. S.; Cheng, L.; Zhang, K.; Weir, M. D.; Rodrigues, L. K. A.; Xu, H. H. K. Novel Dental Adhesives Containing Nanoparticles of Silver and Amorphous Calcium Phosphate. *Dent. Mater.* **2013**, *29*, 199–210.
- (272) Poosti, M.; Ramazan-zadeh, B.; Zebbarj, M.; Javadzadeh, P.; Naderinasab, M.; Shakeri, M. T. Shear Bond Strength and Antibacterial Effects of Orthodontic Composite Containing TiO<sub>2</sub> Nanoparticles. *Eur. J. Orthod.* **2013**, *35*, 676–679.
- (273) Juillerat-Jeanneret, L.; Dusinska, M.; Fjellbø, L. M.; Collins, A. R.; Handy, R. D.; Riediker, M. Biological Impact Assessment of Nanomaterial Used in Nanomedicine. Introduction to the NanoTEST Project. *Nanotoxicology* **2015**, *9*, 5–12.
- (274) Paradise, J. Regulating Nanomedicine at the Food and Drug Administration. *AMA J. Ethics* **2019**, *21*, 347–355.
- (275) Foulkes, R.; Man, E.; Thind, J.; Yeung, S.; Joy, A.; Hoskins, C. The Regulation of Nanomaterials and Nanomedicines for Clinical Application: Current and Future Perspectives. *Biomater. Sci.* **2020**, *8*, 4653–4664.
- (276) Đorđević, S.; Gonzalez, M. M.; Conejos-Sánchez, I.; Carreira, B.; Pozzi, S.; Acúrcio, R. C.; Satchi-Fainaro, R.; Florindo, H. F.; Vicent, M. J. Current Hurdles to the Translation of Nanomedicines from Bench to the Clinic. *Drug Delivery Transl. Res.* **2022**, *12*, 500–525.
- (277) Food and Drug Administration. *Drug Products, Including Biological Products, that Contain Nanomaterials: Guidance for Industry*; Food and Drug Administration, 2017.
- (278) *The Medical Devices Regulations 2002*; Consumer Protection: United Kingdom; 2002; Vol. 618. <https://www.legislation.gov.uk/uksi/2002/618/data.pdf> (accessed 23 November 2022).
- (279) Food and Drug Administration. *Code of Federal Regulations, Title 21, Parts 800–1299*, 2022. <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfcfr/CFRSearch.cfm?CFRPartFrom=800&CFRPartTo=1299> (accessed).
- (280) Oberdörster, G.; Stone, V.; Donaldson. Toxicology of Nanoparticles: A Historical Perspective. *Nanotoxicology* **2007**, *1*, 2–25.
- (281) Savolainen, K.; Pyllkänen, L.; Norppa, H.; Falck, G.; Lindberg, H.; Tuomi, T.; Vippola, M.; Alenius, H.; Hämeri, K.; Koivisto, J.; et al. Nanotechnologies, Engineered Nanomaterials and Occupational Health and Safety – A Review. *Saf. Sci.* **2010**, *48*, 957–963.
- (282) Pietrousti, A.; Stockmann-Juvala, H.; Lucaroni, F.; Savolainen, K. Nanomaterial Exposure, Toxicity, and Impact on Human Health. *Wiley Interdiscip. Rev. Nanomed. Nanobiotechnol.* **2018**, *10*, 1513 DOI: 10.1002/wnan.1513.
- (283) Riediker, M.; Zink, D.; Kreyling, W.; Oberdörster, G.; Elder, A.; Graham, U.; Lynch, I.; Duschl, A.; Ichihara, G.; Ichihara, S.; et al. Particle Toxicology and Health - Where Are We? *Part. Fibre Toxicol* **2019**, *16*, 19.
- (284) Bondarenko, O.; Mortimer, M.; Kahru, A.; Feliu, N.; Javed, I.; Kallinen, A.; Lin, S.; Xia, T.; Song, Y.; Davis, T. P.; et al. Nanotoxicology and Nanomedicine: The Yin and Yang of Nano-Bio Interactions for the New Decade. *Nano Today* **2021**, *39*, 101184.
- (285) Domingues, C.; Santos, A.; Alvarez-Lorenzo, C.; Concheiro, A.; Jarak, I.; Veiga, F.; Barbosa, I.; Dourado, M.; Figueiras, A. Where Is Nano Today and Where Is It Headed? A Review of Nanomedicine and the Dilemma of Nanotoxicology. *ACS Nano* **2022**, *16*, 9994–10041.



- (286) Salaie, R. N.; Besinis, A.; Le, H.; Tredwin, C.; Handy, R. D. The Biocompatibility of Silver and Nanohydroxyapatite Coatings on Titanium Dental Implants with Human Primary Osteoblast Cells. *Mater. Sci. Eng., C* **2020**, *107*, 110210.
- (287) Wade, R. G.; Burr, N. E.; McCauley, G.; Bourke, G.; Efthimiou, O. The Comparative Efficacy of Chlorhexidine Gluconate and Povidone-Iodine Antiseptics for the Prevention of Infection in Clean Surgery: A Systematic Review and Network Meta-Analysis. *Ann. Surg.* **2021**, *274*, 274.
- (288) Makabenta, J. M. V.; Nabawy, A.; Li, C. H.; Schmidt-Malan, S.; Patel, R.; Rotello, V. M. Nanomaterial-Based Therapeutics for Antibiotic-Resistant Bacterial Infections. *Nat. Rev. Microbiol.* **2021**, *19*, 23–36.
- (289) de Jonge, S. W.; Boldingh, Q. J. J.; Solomkin, J. S.; Dellinger, E. P.; Egger, M.; Salanti, G.; Allegranzi, B.; Boormeester, M. A. Effect of Postoperative Continuation of Antibiotic Prophylaxis on the Incidence of Surgical Site Infection: A Systematic Review and Meta-Analysis. *Lancet Infect. Dis.* **2020**, *20*, 1182–1192.
- (290) Zhang, S.; Wang, Y.; Song, H.; Lu, J.; Yuan, Z.; Guo, J. Copper Nanoparticles and Copper Ions Promote Horizontal Transfer of Plasmid-Mediated Multi-Antibiotic Resistance Genes Across Bacterial Genera. *Environ. Int.* **2019**, *129*, 478–487.
- (291) Dobrovolskaia, M. A.; McNeil, S. E. Immunological Properties of Engineered Nanomaterials. *Nat. Nanotechnol.* **2007**, *2*, 469–478.
- (292) Medicines & Healthcare products Regulatory Agency. *Yellow Card reporting site*. <https://yellowcard.mhra.gov.uk/> (accessed 23 November 2022).
- (293) Ventola, C. L. Progress in Nanomedicine: Approved and Investigational Nanodrugs. *Pharm. Ther.* **2017**, *42*, 742–755.
- (294) Handy, R. D.; Shaw, B. J. Toxic Effects of Nanoparticles and Nanomaterials: Implications for Public Health, Risk Assessment and the Public Perception of Nanotechnology. *Health Risk Soc.* **2007**, *9*, 125–144.
- (295) Hunt, G.; Lynch, I.; Cassee, F.; Handy, R. D.; Fernandes, T. F.; Berges, M.; Kuhlbusch, T. A. J.; Dusinska, M.; Riediker, M. Towards a Consensus View on Understanding Nanomaterials Hazards and Managing Exposure: Knowledge Gaps and Recommendations. *Materials* **2013**, *6*, 1090–1117.
- (296) Mihalache, R.; Verbeek, J.; Graczyk, H.; Murashov, V.; van Broekhuizen, P. Occupational Exposure Limits for Manufactured Nanomaterials, a Systematic Review. *Nanotoxicology* **2017**, *11*, 7–19.
- (297) Verma, N. Risk Assessment Studies of the Impact of Occupational Exposure of Pharmaceutical Workers on the Development of Antimicrobial Drug Resistance. *J. Occup. Environ. Hyg.* **2020**, *17*, 437–446.
- (298) Arsal Yildirim, S.; Pekey, B.; Pekey, H. Assessment of Occupational Exposure to Fine Particulate Matter in Dental Prosthesis Laboratories in Kocaeli, Turkey. *Environ. Monit. Assess.* **2020**, *192*, 667.
- (299) Panáček, A.; Kvítek, L.; Směkalová, M.; Večřová, R.; Kolář, M.; Röderová, M.; Dyčka, F.; Šebela, M.; Pruček, R.; Tomanec, O.; et al. Bacterial Resistance to Silver Nanoparticles and How to Overcome It. *Nat. Nanotechnol.* **2018**, *13*, 65–71.
- (300) Randall, C. P.; Gupta, A.; Jackson, N.; Busse, D.; O'Neill, A. J. Silver Resistance in Gram-Negative Bacteria: a Dissection of Endogenous and Exogenous Mechanisms. *J. Antimicrob. Chemother.* **2015**, *70*, 1037–1046.
- (301) Delmar, J. A.; Su, C.-C.; Yu, E. W. Structural Mechanisms of Heavy-Metal Extrusion by the Cus Efflux System. *Biometals* **2013**, *26*, 593–607.
- (302) Muller, M. Bacterial Silver Resistance Gained by Cooperative Interspecies Redox Behavior. *Antimicrob. Agents Chemother.* **2018**, *62*, 18.
- (303) Moffatt, J. H.; Harper, M.; Boyce, J. D. Mechanisms of Polymyxin Resistance. *Adv. Exp. Med. Biol.* **2019**, *1145*, 55–71.
- (304) Pal, C.; Asiani, K.; Arya, S.; Rensing, C.; Stekel, D. J.; Larsson, D. G. J.; Hobman, J. L. In *Advances in Microbial Physiology*; Poole, R. K., Ed.; Academic Press, 2017; Vol. 70, pp 261–313.
- (305) Finley, P. J.; Norton, R.; Austin, C.; Mitchell, A.; Zank, S.; Durham, P. Unprecedented Silver Resistance in Clinically Isolated *Enterobacteriaceae*: Major Implications for Burn and Wound Management. *Antimicrob. Agents Chemother.* **2015**, *59*, 4734.
- (306) Ellis, D. H.; Maurer-Gardner, E. I.; Sulentic, C. E. W.; Hussain, S. M. Silver Nanoparticle Antibacterial Efficacy and Resistance Development in Key Bacterial Species. *Biomed. Phys. Eng. Express* **2018**, *5*, 015013.
- (307) Lu, J.; Wang, Y.; Jin, M.; Yuan, Z.; Bond, P.; Guo, J. Both Silver Ions and Silver Nanoparticles Facilitate the Horizontal Transfer of Plasmid-Mediated Antibiotic Resistance Genes. *Water Res.* **2020**, *169*, 115229.
- (308) Ding, C.; Pan, J.; Jin, M.; Yang, D.; Shen, Z.; Wang, J.; Zhang, B.; Liu, W.; Fu, J.; Guo, X.; et al. Enhanced Uptake of Antibiotic Resistance Genes in the Presence of Nanoalumina. *Nanotoxicology* **2016**, *10*, 1051–1060.
- (309) Zhang, Y.; Gu, A. Z.; Xie, S.; Li, X.; Cen, T.; Li, D.; Chen, J. Nano-Metal Oxides Induce Antimicrobial Resistance via Radical-Mediated Mutagenesis. *Environ. Int.* **2018**, *121*, 1162–1171.
- (310) Eymard-Vernain, E.; Luche, S.; Rabilloud, T.; Lelong, C. Impact of Nanoparticles on the *Bacillus subtilis* (3610) Competence. *Sci. Rep.* **2018**, *8*, 2978.
- (311) Brook, I. Beta-Lactamase-Producing Bacteria in Mixed Infections. *Clin. Microbiol. Infect.* **2004**, *10*, 777–784.