



REVIEW

REVISED **A review of ultrasound contrast media [version 3; peer review: 2 approved]**

Ammar A. Oglat

Department of Medical Imaging, Faculty of Applied Medical Sciences, The Hashemite University, Zarqa, 13133, Jordan., The Hashemite University, Az-Zarqa, Zarqa Governorate, 13133, Jordan

V3 **First published:** 07 Nov 2023, **12:**1444
<https://doi.org/10.12688/f1000research.140131.1>
Second version: 11 Mar 2024, **12:**1444
<https://doi.org/10.12688/f1000research.140131.2>
Latest published: 04 Jun 2024, **12:**1444
<https://doi.org/10.12688/f1000research.140131.3>

Abstract

Efforts have been made over the last five decades to create effective ultrasonic contrast media (UCM) for cardiac and noncardiac applications. The initial UCM was established in the 1980s, following publications from the 1960s that detailed the discovery of ultrasonic contrast enhancement using small gaseous bubbles in echocardiographic examinations. An optimal contrast agent for echography should possess the following characteristics: non-toxicity, suitability for intravenous injection, ability to traverse pulmonary, cardiac, and capillary circulations, and stability for recirculation. Definity, Optison, Sonazoid, and SonoVue are examples of current commercial contrast media. These contrast media have shown potential for various clinical reasons, both on-label and off-label. Several possible UCMs have been developed or are in progress. Advancements in comprehending the physical, chemical, and biological characteristics of microbubbles have significantly improved the visualization of tumor blood vessels, the identification of areas with reduced blood supply, and the enhanced detection of narrowed blood vessels. Innovative advances are expected to enhance future applications such as ultrasonic molecular imaging and therapeutic utilization of microbubbles.

Keywords

contrast agents for ultrasound, Microbubbles, echocardiographic, M-mode

Open Peer Review

Approval Status

	1	2
version 3 (revision) 04 Jun 2024		
version 2 (revision) 11 Mar 2024	 view	 view
version 1 07 Nov 2023	 view	

- Hamad Yahia Abu Mhanna**, Universiti Sains Malaysia, Minden Heights, Malaysia
- Haytham Alewaidat** , Jordan University of Science and Technology, Irbid, Jordan

Any reports and responses or comments on the article can be found at the end of the article.

Corresponding author: Ammar A. Oglat (ammar.oglat@yahoo.com)

Author roles: Oglat AA: Conceptualization, Data Curation, Formal Analysis, Investigation, Methodology, Resources, Writing – Original Draft Preparation, Writing – Review & Editing

Competing interests: No competing interests were disclosed.

Grant information: The author(s) declared that no grants were involved in supporting this work.

Copyright: © 2024 Oglat AA. This is an open access article distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

How to cite this article: Oglat AA. **A review of ultrasound contrast media [version 3; peer review: 2 approved]** F1000Research 2024, 12:1444 <https://doi.org/10.12688/f1000research.140131.3>

First published: 07 Nov 2023, 12:1444 <https://doi.org/10.12688/f1000research.140131.1>

REVISED Amendments from Version 2

1. The grammatical and typo errors in all manuscript sections are corrected.
2. The conclusion is rephrased in a good Scientific way.

Any further responses from the reviewers can be found at the end of the article

Introduction

In obstetrics, cardiology, and radiology, ultrasound imaging is a common clinical tool for the morphological examination of soft tissues.^{1–7} As an ultrasonic wave—a longitudinal wave—travels through the body, tissue surfaces with various acoustic characteristics, such as speed of sound and density, produce reflections. The same transmitting transducer captures these scattered impulses and uses them to create an image. However, because of the size and characteristics of red blood cells, the intrinsic scattering from the blood pool is often several orders of magnitude lower than tissue at standard diagnostic frequencies (1–9 MHz). As a result, blood appears black on typical ultrasound images, making it difficult to determine the properties of blood flow. Doppler techniques can be used to measure blood velocity in bigger veins by comparing the relative motion of red blood cells to the surrounding tissue.^{8,9} This technique is frequently used in clinical settings (*e.g.*, obstetrics,¹⁰ assessment of peripheral artery disease,¹¹ cardiology¹²). However, this method has drawbacks when applied to areas with poor blood flow, significant tissue motion, and/or low hematocrit percentage.^{13–15}

Ultrasound imaging's diagnostic applications have significantly expanded during the past few decades. The advancement of UCM has resulted in the presentation of valuable physiological and pathological information, as well as the accessibility of perfusion imaging for cardiac or tumor tissue in routine clinical decision-making.^{16,17} The early 1960s saw the first reports of the ultrasonic contrast effect was studies by Joyner. Further research revealed the existence of UCM made of saline, indocyanine green, hydrogen peroxide, dextrose, and renografin.^{16,18} UCM comprise of a suspension of small spheres of gas with a poor solubility in blood (*e.g.*, perfluorocarbon), often ranging in size from below 10 μm in diameter. The relatively large size of UCMs guarantees that they remain strictly intravascular and function as red blood cell tracers, in contrast to contrast media employed in other modalities like (magnetic resonance imaging) MRI and computer tomography (CT).¹⁹

Around 1980, achieving stability long enough for the UCM to reach the correct heart was one of the primary objectives in creating efficient UCMs. Left heart contrast was not possible until the 1990s because lung capillaries are effective filters. In 1995, contrast-enhancing substances with enhanced blood pool enhancement capabilities first surfaced. The next goal was to create bubbles that would allow for real-time imaging. In order to achieve this, air was substituted with weakly soluble gases, such as perfluorocarbons, which increased bubble endurance and allowed the development of software algorithms that could effectively distinguish UCM from tissue signals.^{20–23}

Microbubbles vibrate about their equilibrium radius in an ultrasonic field due to the compressibility of their gas cores, and they have scattering cross-sections that are many orders of magnitude higher than a solid particle of the same size.^{16,24,25} A thin biocompatible encapsulation layer, often a phospholipid monolayer, stabilizes the bubbles by striking a balance between their ability to vibrate freely and their resistance to dissolving in-vivo during timeframes important for imaging, like half-lives of minutes.^{26,27}

Contrast echocardiography has a virtually limitless potential. Contrast echocardiography is currently the subject of extensive interest and research, as this review demonstrates. The creation of novel contrast-producing chemicals is arguably the most intriguing component of this research. It will be fascinating to watch how these different agents grow. Ideally, one or more of these novel agents will be able to cross the capillaries, allowing for peripheral venous injection-based visualization of the left side of the heart.

Emerging technique

Over the world, contrast-enhanced ultrasound imaging is used in numerous medical and off-label applications. On multiple fronts, including the creation of novel pulse sequences and image processing techniques, the development of devices, and the creation of remote monitoring for ultrasonic therapies, this field is seeing cutting-edge breakthroughs at the same time.

Contrast media

The only UCM that has received clinical approval is microbubbles. These bubbles have the advantage of remaining intravascular because of their size, making it possible to perform diagnostic tests that would be challenging with diffusible

tracers. The use of these “conventional” UCM is being expanded, though, to include molecular-based imaging, imaging of the extravascular space, and as a platform for both imaging and therapeutic administration.^{28–32}

Creation of the “optimal” UCM

Extensive study was done beginning in 1980 to establish contrast echocardiography as a recognized diagnostic method.³³ Ophir and Parker (1989) provided a summary of UCM’s application in medical imaging.³⁴ Free gas bubbles, encapsulated gas bubbles, colloidal suspensions, emulsions, and aqueous solutions were the five categories of agents that were categorized according to their physical characteristics. Producing the “perfect” contrast media that would satisfy the following requirements was still a major difficulty in those days. Such as, distribution of the substance inside the myocardial or heart chambers, which is indicative of regional blood flow; agent’s capacity to endure after an intravenous infusion during an imaging test; containing microbubbles with a diameter of less than 8 mm (smaller than red blood cells), allowing passage via the pulmonary system and the body’s smallest capillaries; good safety profile, physiological inert; and strong, regulated, and echogenic acoustic interaction.

Synthesis of functionalized microbubbles

In 1984 (Feinstein *et al.* 1984), cavitation was used to create microbubbles after inserting the tip of a sonicator horn into a solution of human serum albumin.¹⁷ This solved the problem of creating stable encapsulated microbubbles that could survive passage through the heart and the pulmonary capillary network. After a peripheral venous injection, these microbubbles could be seen in the left heart. Due to the creation of functionalized microbubbles,³⁵ or microbubbles with one or more targeted moieties inserted into the phospholipid encapsulation,³⁶ non-invasive imaging of pathophysiological events has recently been demonstrated to be viable with ultrasound. Target sites have focused on internal vasculature processes such inflammation,³⁷ angiogenesis,³⁸ and thrombus formation³⁹ since microbubbles are purely intravascular. See [Table 1](#).

The development of the first microbubbles that met the majority of the requirements for an intravenous UCM also sparked intense research by doctors, scientists, and the makers of ultrasound equipment to explain the physical phenomena and apply what they learned to therapeutic settings.

There were several technologies looked at to stabilize the microbubbles. For the purpose of lowering surface tension and stabilizing the gas core against quick dissolution, thin shells consisting of protein, polymer, or phospholipids were utilized. Unfortunately, due to the high solubility of air in water, the first-generation agents still had poor stability and relatively short circulation times. By substituting perfluorinated gases with low solubility in water, such as sulphur hexafluoride, perfluoropropane, or perfluorobutane for air during circulation, persistence during circulation was dramatically improved, resulting in sufficient persistence of the agent in the blood circulation for clinical use.⁴¹

There are many ultrasound-sensitive sub-micron agents currently being researched. This research is motivated by the enhanced-permeability and retention effect,⁴² whereby small nanometer sized particles locally extravasate from leaky blood vessels and accumulate in the perivascular space of solid tumors. Phase-shift droplets,⁴³ nanobubbles,⁴⁴ gas vesicles,⁴⁵ echogenic liposomes,⁴⁶ and polymeric nanoparticles⁴⁷ are a few of the more common examples. Although research into the physics of acoustic droplet vaporization is still ongoing, it is most probable that both intrinsic and external elements play a role in the process.

Ultrasound imaging techniques using UCM

Vibrating microbubbles’ nonlinear nature is essential to their efficiency as an ultrasonic contrast agent. These emissions allow for the separation of bubble signals from the surrounding (about linear) tissue from those within tiny vessels. Thus, certain microbubble imaging modes were created concurrently with the advancements in UCM and as a result of a better knowledge of non-linear microbubble behavior; these are now used in the majority of clinical ultrasound systems.^{48–50} The first methods of bubble identification were harmonic imaging, which involved gathering and filtering energy from

Table 1. Lists the most popular microbubble-based intravenous UCM at various stages of development.⁴⁰

Trademark name	Manufacturer	Formulations
Bisphere	Point Biomedical	Albumin/air
Echogen	Sonus Pharmaceuticals	Surfactant
Echovist	Schering AG	Galactose/air
Optison	Amersham Health Inc.	Protein-type A/perfluoropropane

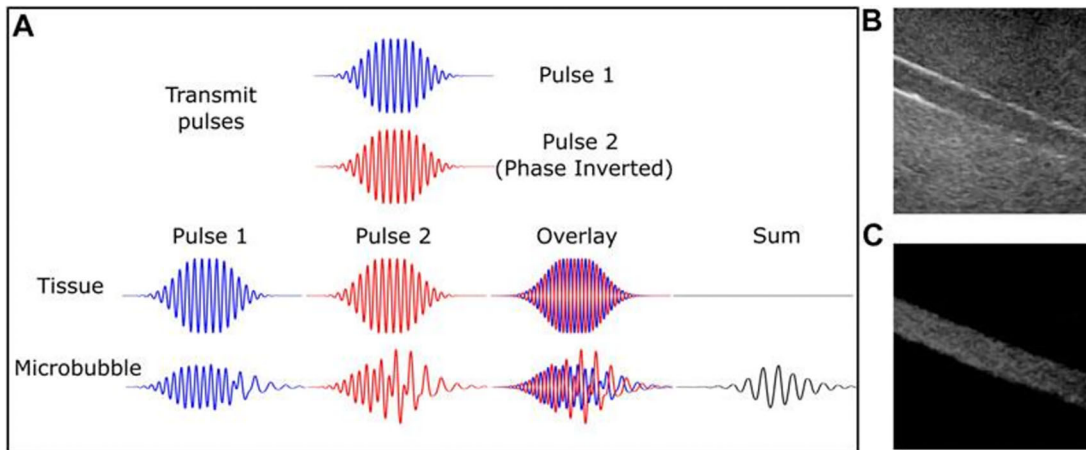


Figure 1. Microbubble-specific imaging sequences capture the nonlinear signal from the contrast agent while excluding tissue with linear scattering. Pulse inversion diagram (A). Two 180-degree pulses produce tissue echoes that are out of phase. Microbubbles are nonlinear; hence, this is not true. Microbubbles produce a strong echo, while linear tissue almost totally cancels it off. B-mode and contrast-specific imaging of an 8-mm artery phantom exhibit microbubble-specific imaging's improved vascular contrast. The Philips iU22 scanner, C5-2 probe, and Definity™ contrast medium were used to record this. This source provides this number. Microbubble-specific imaging sequences exclude linear scattering tissue and capture a nonlinear contrast agent signal. Yusefi, H., & Helfield, B. (2022), https://www.frontiersin.org/files/Articles/791145/fphy-10-791145-HTML/image_m/fphy-10-791145-g002.jpg, CC BY 4.0.²⁸

the receive signal at the second harmonic, which is twice the driving frequency. Because the second harmonic signal produced by microbubbles is substantially greater than the second harmonic signal produced by tissue, it has a higher signal-to-noise ratio than the fundamental energy. The success of low mechanical index (MI) (0.1) contrast-specific imaging, which is primarily employed for real-time perfusion and intra-cavitary measurements, is particularly explained by the non-linear shell behavior. Furthermore, a number of diagnostic imaging procedures and/or quantification strategies are founded on the distinct and extremely sensitive attribute of microbubble destruction.⁵¹ See Figure 1.

In other words, the reflection pattern from the bubble to the ultrasound signal is significantly altered by UCM. They start by greatly boosting the backscattered signal.²³ UCM resonate linearly in response to acoustic pressure. Acoustic pressure increases cause nonlinear vibrational patterns to manifest.⁵² Only at higher mechanical indices (MI) do tissues create harmonic resonances, making it easy to distinguish between the signal's tissue or UCM origin. Multiples of the natural frequencies are received using filter devices, allowing for some background (non-UCM) signal reduction. Microbubbles are disrupted by high pressure levels, which results in strong signals and signals with various properties.

M-mode echocardiograms using UCM

Understanding the interaction between ultrasonic waves and gaseous microbubbles was made much easier by using the process utilized to explain the set of echoes first discovered on M-mode echocardiograms. The strong compressibility of the gas core appears to be particularly significant since it produces frequency-dependent volume pulsations with a clear maximum at the resonance frequency, which is inversely proportional to the size of the microbubbles.^{24,53} However, In the following circumstances, UCM is advised by cardiologic guidelines: if the left ventricular (LV) cavum does not have two continuous segments, If the original spectrum signals are insufficient, to enhance Doppler evaluations, when periodic evaluation of the ejection fraction is necessary given the reduced variability caused by UCM, and in the case of Takotsubo myopathy, left ventricular (LV) aneurysms, and intracavitary thrombi.^{52,54,55}

Microbubbles-based color Doppler ultrasound

Acoustic color Doppler is an imaging method that overlays color-coded maps of tissue velocity on grey-scale images of tissue anatomy. It combines anatomical information acquired from ultrasonic pulse-echo techniques with velocity information derived from ultrasonic Doppler techniques. The technique is most frequently used to visualize blood flow through the heart, arteries, and veins, but it can also be used to visualize the movements of solid tissues like the walls of the heart. vectors. Almost all commercial ultrasound equipment now provides color Doppler imaging, which has been proven to be very useful in determining blood flow in a variety of clinical circumstances. Although the technique for getting velocity information is quite similar to the technique for getting anatomical information, there are a number of

reasons why it is technically more difficult. It also has a few flaws, the biggest of which is that, in conventional systems, the velocities measured and subsequently displayed are the components of the flow velocity directly towards or away from the transducer, whereas the method's ideal output would provide data on the magnitude and direction of the three-dimensional flow vectors.^{56–61}

In conjunction with color or power Doppler, stimulated acoustic emission is employed in high mechanical index (MI) imaging. A high MI ultrasound impulse is used to deflate the microbubbles, and the signal that is received is a complicated mixture of ultrasound waves that causes a Doppler shift.⁶² It is especially helpful when a UCM with tissue specificity, is in its late stages.²⁰ Color Doppler imaging has been shown that despite the poor spatial resolution, real-time imaging was possible due to the tiny size of the picture window.⁶³

Recently, the use of ultrasound color Doppler has been shown to monitor bubbles during ultrasound therapy. An active ultrasound imaging method called color Doppler uses the phase shifts between the echoes of imaging pulses to measure velocities. In the aforementioned investigation, an increase in the color Doppler signal was connected with the formation of cavitation bubbles on their own under a high-pressure ultrasonic beam. The rise was utilized to evaluate tissue fractionation and was related to the mobility of the surrounding tissue brought on by cavitation within the focused location. Although this method is helpful for high-pressure therapy, it does not reveal how net bubbles flow through the field.^{64,65}

Modern commercial UCM

All currently marketed UCM are made up of an inert gas enclosed in a shell. The gas determines solubility and most of the acoustic qualities of the bubbles, while the shell mostly affects the viscoelastic properties, such as stability and durability.⁶⁶ Perfluorocarbon bubbles, which range in size almost 10 μm and are real blood pool agents, allow transit through the pulmonary vascular system, which is necessary for entry to the systemic circulation.⁵² Soft shell materials have better nonlinear oscillations and are made of phospholipids or other surfactants.⁶⁷ There are also protein-shelled microbubbles that contain an albumin shell around perfluoropropane gas.

Conclusion

Contrast agent microbubble vibration basics and its applications in common contrast-imaging are outlined in this paper. Over the span of the last fifty years, UCM imaging has made substantial progress. Previously, the primary clinical emphasis was on echocardiography, while myocardial perfusion was considered the ultimate goal and an attractive market for contrast echo. The primary purpose of echocardiography was to enhance the visibility of the LV by making it more opaque, hence improving the clarity of the LV endocardial border. UCM imaging is a safe and effective method for many clinical applications, and its use is growing. Due to increased clinical awareness of ultrasound's advantages as well as collaborative research projects between physicists, chemists, engineers, and clinicians on the study of microbubble behavior, signal processing methods, contrast agent synthesis, and device development, this imaging technology has achieved tremendous success to date.

Data availability

Underlying data

No data are associated with this article.

References

- Oglat AA, *et al.*: **A review of medical doppler ultrasonography of blood flow in general and especially in common carotid artery.** *J Med Ultrasound.* 2018; **26**(1): 3–13.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Oglat AA, *et al.*: **A new scatter particle and mixture fluid for preparing blood mimicking fluid for wall-less flow phantom.** *J Med Ultrasound.* 2018; **26**(3): 134–142.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Ammar AO, *et al.*: **Characterization and construction of a robust and elastic wall-less flow phantom for high pressure flow rate using Doppler ultrasound applications.** *Nat Eng Sci.* 2018; **3**(3): 359–377.
[Publisher Full Text](#)
- Oglat AA, *et al.*: **Artifacts in diagnostic ultrasonography.** Los Angeles, CA: SAGE Publications Sage CA; 2020.
- Shalbi SM, *et al.*: **A brief review for common doppler ultrasound flow phantoms.** *J Med Ultrasound.* 2020; **28**(3): 138–142.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Dakok KK, *et al.*: **A review of carotid artery phantoms for doppler ultrasound applications.** *J Med Ultrasound.* 2021; **29**(3): 157–166.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Athamnah SI, *et al.*: **Diagnostic breast elastography estimation from doppler imaging using central difference (CD) and least-squares (LS) algorithms.** *Biomedical Signal Processing and Control.* 2021; **68**: 102667.
[Publisher Full Text](#)
- Oglat AA, Dheyab MA: **Performance evaluation of ultrasonic imaging system (Part I).** *J Med Ultrasound.* 2021; **29**(4): 258–263.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)

9. Oglat AAJB: **Performance Evaluation of an Ultrasonic Imaging System Using Tissue-Mimicking Phantoms for Quality Assurance.** *Biomimetics.* 2022; **7**(3): 130.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
10. Mone F, et al.: **The clinical application of Doppler ultrasound in obstetrics.** *Obstet Gynaecol.* 2015; **17**(1): 13–19.
[Publisher Full Text](#)
11. Grant EG, et al.: **Carotid artery stenosis: gray-scale and Doppler US diagnosis—Society of Radiologists in Ultrasound Consensus Conference.** *Radiology.* 2003; **229**(2): 340–346.
[PubMed Abstract](#) | [Publisher Full Text](#)
12. Quiñones MA, et al.: **Recommendations for quantification of Doppler echocardiography: a report from the Doppler Quantification Task Force of the Nomenclature and Standards Committee of the American Society of Echocardiography.** *J Am Soc Echocardiogr.* 2002; **15**(2): 167–184.
[PubMed Abstract](#) | [Publisher Full Text](#)
13. Cobbold RS: *Foundations of biomedical ultrasound.* Oxford University Press; 2006.
14. Jensen JA: *Estimation of blood velocities using ultrasound: a signal processing approach.* Cambridge University Press; 1996.
15. Szabo TL: *Diagnostic ultrasound imaging: inside out.* Academic Press; 2004.
16. Gramiak R, Shah PM: **Echocardiography of the aortic root.** *Investig Radiol.* 1968; **3**(5): 356–366.
[Publisher Full Text](#)
17. Feinstein SB, et al.: **Microbubble dynamics visualized in the intact capillary circulation.** *J Am Coll Cardiol.* 1984; **4**(3): 595–600.
[PubMed Abstract](#) | [Publisher Full Text](#)
18. Forsberg F, et al.: **Effect of filling gases on the backscatter from contrast microbubbles: theory and in vivo measurements.** *Ultrasound Med Biol.* 1999; **25**(8): 1203–1211.
[Publisher Full Text](#)
19. Becher H, Burns PN: *Handbook of contrast echocardiography: Left ventricular function and myocardial perfusion.* Springer Science & Business Media; 2012.
20. Cosgrove D: **Ultrasound contrast agents: an overview.** *Eur J Radiol.* 2006; **60**(3): 324–330.
[Publisher Full Text](#)
21. Goldberg BB, et al.: **Ultrasound contrast agents: a review.** *Ultrasound Med Biol.* 1994; **20**(4): 319–333.
[Publisher Full Text](#)
22. Ignee A, et al.: **Ultrasound contrast agents.** *Endosc Ultrasound.* 2016; **5**(6): 355–362.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
23. Calliada F, et al.: **Ultrasound contrast agents: basic principles.** *Eur J Radiol.* 1998; **27**: S157–S160.
[Publisher Full Text](#)
24. Medwin HJU: **Counting bubbles acoustically: a review.** *Ultrasonics.* 1977; **15**(1): 7–13.
[Publisher Full Text](#)
25. Covella M, et al.: **Echocardiographic aortic root dilatation in hypertensive patients: a systematic review and meta-analysis.** *J Hypertens.* 2014; **32**(10): 1928–1935.
[Publisher Full Text](#)
26. Unger EC, et al.: **Therapeutic applications of lipid-coated microbubbles.** *Adv Drug Deliv Rev.* 2004; **56**(9): 1291–1314.
[PubMed Abstract](#) | [Publisher Full Text](#)
27. Garg S, Thomas A, Borden M: *The Effect of Lipid Monolayer In-Plane Rigidity on Vivo;* 2013.
28. Yusefi H, Helfield B: **Ultrasound contrast imaging: Fundamentals and emerging technology.** *Front Phys.* 2022; **10**: 100.
[Publisher Full Text](#)
29. Frinking PJ, et al.: **Ultrasound contrast imaging: current and new potential methods.** *Ultrasound Med Biol.* 2000; **26**(6): 965–975.
[PubMed Abstract](#) | [Publisher Full Text](#)
30. Averkiou M, et al.: **Ultrasound contrast imaging research.** *Ultrasound Q.* 2003; **19**(1): 27–37.
[Publisher Full Text](#)
31. Correas J-M, et al.: **Ultrasound contrast agents: properties, principles of action, tolerance, and artifacts.** *Eur Radiol.* 2001; **11**: 1316–1328.
[PubMed Abstract](#) | [Publisher Full Text](#)
32. Sofuni A, et al.: **Differential diagnosis of pancreatic tumors using ultrasound contrast imaging.** *J Gastroenterol.* 2005; **40**: 518–525.
[Publisher Full Text](#)
33. Senior R, et al.: **Clinical practice of contrast echocardiography: recommendation by the European Association of Cardiovascular Imaging (EACVI) 2017.** *Eur Heart J Cardiovasc Imaging.* 2017; **18**(11): 1205–1205af.
[PubMed Abstract](#) | [Publisher Full Text](#)
34. Ophir J, Parker KJ: **Contrast agents in diagnostic ultrasound.** *Ultrasound Med Biol.* 1989; **15**(4): 319–333.
[Publisher Full Text](#)
35. Lindner JR: **Microbubbles in medical imaging: current applications and future directions.** *Nat Rev Drug Discov.* 2004; **3**(6): 527–533.
[PubMed Abstract](#) | [Publisher Full Text](#)
36. Langeveld SA, Meijlink B, Kooiman K: **Phospholipid-coated targeted microbubbles for ultrasound molecular imaging and therapy.** *Curr Opin Chem Biol.* 2021; **63**: 171–179.
[PubMed Abstract](#) | [Publisher Full Text](#)
37. Wang Y, et al.: **Clopidogrel with aspirin in acute minor stroke or transient ischemic attack (CHANCE) trial: one-year outcomes.** *Circulation.* 2015; **132**(1): 40–46.
[Publisher Full Text](#)
38. Willmann JK, et al.: **Targeted contrast-enhanced ultrasound imaging of tumor angiogenesis with contrast microbubbles conjugated to integrin-binding knottin peptides.** *J Nucl Med.* 2010; **51**(3): 433–440.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
39. Hamilton AJ, et al.: **Intravascular ultrasound molecular imaging of atheroma components in vivo.** *J Am Coll Cardiol.* 2004; **43**(3): 453–460.
[PubMed Abstract](#) | [Publisher Full Text](#)
40. Frinking P, et al.: **Three decades of ultrasound contrast agents: a review of the past, present and future improvements.** *Ultrasound Med Biol.* 2020; **46**(4): 892–908.
[PubMed Abstract](#) | [Publisher Full Text](#)
41. Schneider M, et al.: **BR1: a new ultrasonographic contrast agent based on sulfur hexafluoride-filled microbubbles.** *Investig Radiol.* 1995; **30**(8): 451–457.
[PubMed Abstract](#) | [Publisher Full Text](#)
42. Matsumura Y, Maeda H: **A new concept for macromolecular therapeutics in cancer chemotherapy: mechanism of tumorotropic accumulation of proteins and the antitumor agent smancs.** *Cancer Res.* 1986; **46**(12_Part_1): 6387–6392.
43. Sheeran PS, Dayton PA: **Phase-change contrast agents for imaging and therapy.** *Curr Pharm Des.* 2012; **18**(15): 2152–2165.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
44. Helfield B, Zou Y, Matsuura N: **Acoustically-stimulated nanobubbles: opportunities in medical ultrasound imaging and therapy.** *Front Phys.* 2021; **9**: 654374.
[Publisher Full Text](#)
45. Shapiro MG, et al.: **Biogenic gas nanostructures as ultrasonic molecular reporters.** *Nat Nanotechnol.* 2014; **9**(4): 311–316.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
46. Kopechek JA, et al.: **Acoustic characterization of echogenic liposomes: Frequency-dependent attenuation and backscatter.** *J Acoust Soc Am.* 2011; **130**(5): 3472–3481.
[Publisher Full Text](#)
47. Kwan JJ, et al.: **Ultrasound-propelled nanocups for drug delivery.** *Small.* 2015; **11**(39): 5305–5314.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
48. Burns PJC: **Harmonic imaging: principles and preliminary results.** *Clin Radiol.* 1996; **51**: 50–55.
49. Wei K, et al.: **Quantification of myocardial blood flow with ultrasound-induced destruction of microbubbles administered as a constant venous infusion.** *Circulation.* 1998; **97**(5): 473–483.
[PubMed Abstract](#) | [Publisher Full Text](#)
50. Averkiou MA, et al.: **Imaging methods for ultrasound contrast agents.** *Ultrasound Med Biol.* 2020; **46**(3): 498–517.
[Publisher Full Text](#)
51. Albrecht T, et al.: **Improved detection of hepatic metastases with pulse-inversion US during the liver-specific phase of SHU 508A: multicenter study.** *Radiology.* 2003; **227**(2): 361–370.
[PubMed Abstract](#) | [Publisher Full Text](#)
52. Appis AW, et al.: **Update on the safety and efficacy of commercial ultrasound contrast agents in cardiac applications.** *Echo Res Pract.* 2015; **2**(2): R55–R62.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
53. Hu Y-Z, et al.: **Ultrasound microbubble contrast agents: application to therapy for peripheral vascular disease.** *Adv Ther.* 2009; **26**: 425–434.
[PubMed Abstract](#) | [Publisher Full Text](#)
54. Albrecht T, et al.: **Comparison of bolus and infusion of the ultrasound contrast media levovist for color doppler ultrasound of renal arteries.** *Rofo.* 2000; **172**(10): 824–829.
[PubMed Abstract](#) | [Publisher Full Text](#)

55. Porter TR, *et al.*: **Guidelines for the cardiac sonographer in the performance of contrast echocardiography: a focused update from the American Society of Echocardiography.** *J Am Soc Echocardiogr.* 2014; **27**(8): 797–810.
[PubMed Abstract](#) | [Publisher Full Text](#)
56. Arning C, *et al.*: **Revision of DEGUM ultrasound criteria for grading internal carotid artery stenoses and transfer to NASCET measurement.** *Ultraschall Med.* 2010; **31**(3): 251–257.
[Publisher Full Text](#)
57. Udesen J, *et al.*: **Examples of in vivo blood vector velocity estimation.** *Ultrasound Med Biol.* 2007; **33**(4): 541–548.
[PubMed Abstract](#) | [Publisher Full Text](#)
58. Thalhammer C, *et al.*: **Colour-coded duplex sonography after renal transplantation.** *Ultraschall Med.* 2007; **28**(1): 6–27. quiz 25.
[Publisher Full Text](#)
59. Parikh S, Shah R, Kapoor P: **Portal vein thrombosis.** *Am J Med.* 2010; **123**(2): 111–119.
[Publisher Full Text](#)
60. Baik SKJL: **Haemodynamic evaluation by Doppler ultrasonography in patients with portal hypertension: a review.** *Liver Int.* 2010; **30**(10): 1403–1413.
[Publisher Full Text](#)
61. Whittingham TA: **Medical diagnostic applications and sources.** *Prog Biophys Mol Biol.* 2007; **93**(1-3): 84–110.
[Publisher Full Text](#)
62. Albrecht T, *et al.*: **Stimulated acoustic emissions with the ultrasound contrast medium levovist: a clinically useful contrast effect with liver-specific properties.** *Rofo.* 2000; **172**(1): 61–67.
[PubMed Abstract](#) | [Publisher Full Text](#)
63. Dietrich CF, *et al.*: **Improved differentiation of pancreatic tumors using contrast-enhanced endoscopic ultrasound.** *Clin Gastroenterol Hepatol.* 2008; **6**(5): 590–597.e1.
[Publisher Full Text](#)
64. Zhang X, *et al.*: **Real-time feedback of histotripsy thrombolysis using bubble-induced color Doppler.** *Ultrasound Med Biol.* 2015; **41**(5): 1386–1401.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
65. Evans DH, Jensen JA, Nielsen MB: **Ultrasonic colour Doppler imaging.** *Interface Focus.* 2011; **1**(4): 490–502.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
66. Paefgen V, Doleschel D, Kiessling F: **Evolution of contrast agents for ultrasound imaging and ultrasound-mediated drug delivery.** *Front Pharmacol.* 2015; **6**: 197.
[Publisher Full Text](#)
67. Leong-Poi H, *et al.*: **Influence of microbubble shell properties on ultrasound signal: Implications for low-power perfusion imaging.** *J Am Soc Echocardiogr.* 2002; **15**(10): 1269–1276.
[PubMed Abstract](#) | [Publisher Full Text](#)

Open Peer Review

Current Peer Review Status:  

Version 2

Reviewer Report 29 May 2024

<https://doi.org/10.5256/f1000research.163423.r254669>

© 2024 Alewaidat H. This is an open access peer review report distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.



Haytham Alewaidat 

¹ Faculty of Applied Medical Sciences, Jordan University of Science and Technology, Irbid, Jordan

² Faculty of Applied Medical Sciences, Jordan University of Science and Technology, Irbid, Jordan

This review shows An ideal contrast medium for echography should be nontoxic, capable of being injected intravenously, able to travel through pulmonary, cardiac, and capillary circulations, and stable for recirculation

The comments are below:

The author mentioned each detail about the contrast media used in ultrasound, such as the composition, applications, stability, currently commercially available ultrasound contrast agents, and ultrasound contrast agent imaging.

Examples of current commercial contrast media include Definity, Optison, Sonazoid, and SonoVue, which have demonstrated potential for various clinical purposes, both on- and off-label.

Please check the grammatical and typo errors in all manuscript sections.

The contents of this review reflects an excellent scientific subject.

Please note that the conclusion part requires a small correction.

Is the topic of the review discussed comprehensively in the context of the current literature?

Yes

Are all factual statements correct and adequately supported by citations?

Yes

Is the review written in accessible language?

Yes

Are the conclusions drawn appropriate in the context of the current research literature?

Yes

Competing Interests: No competing interests were disclosed.

Reviewer Expertise: Medical Imaging

I confirm that I have read this submission and believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.

Reviewer Report 27 March 2024

<https://doi.org/10.5256/f1000research.163423.r254568>

© 2024 Abu Mhanna H. This is an open access peer review report distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.



Hamad Yahia Abu Mhanna

¹ Universiti Sains Malaysia, Minden Heights, Pulau Pinang, Malaysia

² Universiti Sains Malaysia, Minden Heights, Pulau Pinang, Malaysia

I agree with all modifications made by the authors

Is the topic of the review discussed comprehensively in the context of the current literature?

Yes

Are all factual statements correct and adequately supported by citations?

Yes

Is the review written in accessible language?

Yes

Are the conclusions drawn appropriate in the context of the current research literature?

Yes

Competing Interests: No competing interests were disclosed.

Reviewer Expertise: Medical Imaging

I confirm that I have read this submission and believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.

Version 1

Reviewer Report 05 March 2024

<https://doi.org/10.5256/f1000research.153460.r248551>

© 2024 Abu Mhanna H. This is an open access peer review report distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.



Hamad Yahia Abu Mhanna

¹ Universiti Sains Malaysia, Minden Heights, Pulau Pinang, Malaysia

² Universiti Sains Malaysia, Minden Heights, Pulau Pinang, Malaysia

³ Universiti Sains Malaysia, Minden Heights, Pulau Pinang, Malaysia

Minor comments:

1. The title is accurately representing the content of the article.
2. Kindly make the contribution of this review clearer in the **abstract** section.
3. In the **abstract** section, please rephrase most of the sentences using academic language.
4. The **introduction** part is written in a thorough and complete manner. However, in the second paragraph, this is a run on sentence and hard to follow. "Throughout the past few decades, ultrasound imaging's diagnostic uses have greatly increased. The development of UCM has led to the provision of new useful physiologic and pathologic data, and the availability of perfusion imaging of cardiac or tumor tissue for everyday clinical decision-making." Recommend breaking it up for clarity.
5. The **caption** of **Figure** (1) is too long and make the reader confused. Please rewrite it again in a brief way.
6. Some of grammatical errors in the **conclusion** section need correction.
7. Number of references is enough for this manuscript. Good
8. Make sure that all **sentences** are linked together and all **values** in this study are true.

Is the topic of the review discussed comprehensively in the context of the current literature?

Yes

Are all factual statements correct and adequately supported by citations?

Yes

Is the review written in accessible language?

Yes

Are the conclusions drawn appropriate in the context of the current research literature?

Yes

Competing Interests: No competing interests were disclosed.

Reviewer Expertise: Medical Imaging

I confirm that I have read this submission and believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.

Author Response 07 Mar 2024

Ammar A. Oglat

Responses to Reviewer's Comments

Title: A review of ultrasound contrast media

Dear Editor-in-Chief,

The author sincerely appreciates the reviewers' technical comments and the useful suggestions offered to us to revise our manuscript. My response to reviewers' comments point by point are listed hereafter.

Comments from Reviewer #1:

1. The title is accurately representing the content of the article.

Answer: Esteemed reviewer, Thank you for your helpful comments. Yes, I tried to make the title comprehensive to cover all the manuscript content.

1. Kindly make the contribution of this review clearer in the abstract section.

Answer: The mentioned comment is corrected. The whole abstract is modified and the contribution of this review is simplify and clarify.

1. In the abstract section, please rephrase most of the sentences using academic language.

Answer: The abstract section is modified and rephrased to be in a good scientific manner.

1. The introduction part is written in a thorough and complete manner. However, in the second paragraph, this is a run on sentence and hard to follow. "Throughout the past few decades, ultrasound imaging's diagnostic uses have greatly increased. The development of UCM has led to the provision of new useful physiologic and pathologic data, and the availability of perfusion imaging of cardiac or tumor tissue for everyday clinical decision-making." Recommend breaking it up for clarity.

Answer: Noted and done.

1. The caption of Figure (1) is too long and make the reader confused. Please rewrite it again in a brief way.

Answer: Yes. The caption is modified and shortened.

1. Some of grammatical errors in the conclusion section need correction.

Answer: Ok. Noted and the conclusion is edited.

1. Number of references is enough for this manuscript. Good

Answer: Thank you very much for your valuable comments and scientific support.

1. Make sure that all sentences are linked together and all values in this study are true.
Answer: I made a double check if all values in the manuscript again and there is no any error or mistake.

Dear Respected reviewer. Thank you very much for your valuable comments which enhance the manuscript with scientific information. Appreciate

Competing Interests: There is no conflict of interest

The benefits of publishing with F1000Research:

- Your article is published within days, with no editorial bias
- You can publish traditional articles, null/negative results, case reports, data notes and more
- The peer review process is transparent and collaborative
- Your article is indexed in PubMed after passing peer review
- Dedicated customer support at every stage

For pre-submission enquiries, contact research@f1000.com

F1000Research