

Model for the diffuse reflectance in spatial frequency domain imaging (Erratum)

Anouk L. Post,^{a,b} Dirk J. Faber,^b and Ton G. van Leeuwen^b


^aThe Netherlands Cancer Institute, Department of Surgery, Amsterdam, The Netherlands

^bAmsterdam University Medical Centers, Department of Biomedical Engineering and Physics, Amsterdam, The Netherlands


[DOI: [10.1117/1.JBO.29.6.069801](https://doi.org/10.1117/1.JBO.29.6.069801)]

This article [*J. Biomed. Opt.* **28**(4), 046002 (2023) doi: [10.1117/1.JBO.28.4.046002](https://doi.org/10.1117/1.JBO.28.4.046002)] was originally published on 7 April 2023 with an error in the legend of Fig. 2.

Original figure:

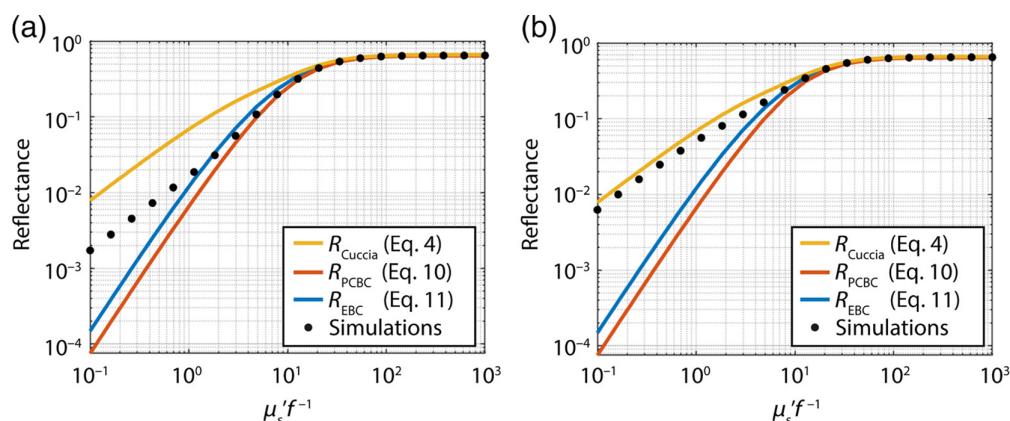

Corrected figure:

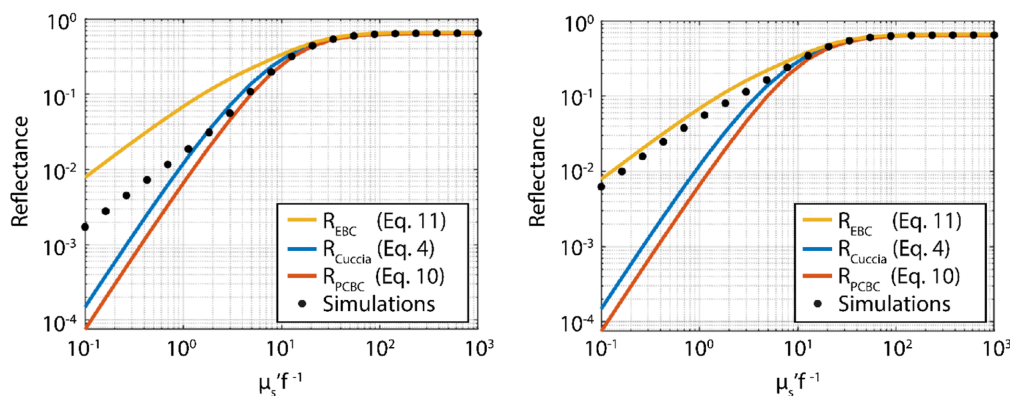

In the original figure, the colored lines in the graph were mislabeled in the legend. The caption for Fig. 2 is unchanged in the corrected version. More importantly, the labeling error impacted neither the analysis nor the description of the results. The article was corrected and republished on 3 June 2024.