

1 **Discrepancies in readouts between Infinium MethylationEPIC v2.0 and v1.0**
2 **reflected in DNA methylation-based tools: implications and considerations for**
3 **human population epigenetic studies**

4
5 Beryl C. Zhuang^{†1,2}, Marcia Smiti Jude^{†1,2}, Chaini Konwar^{1,2}, Natan Yusupov^{3,4}, Calen P.
6 Ryan⁵, Hannah-Ruth Engelbrecht^{1,18}, Joanne Whitehead^{1,2}, Alexandra A. Halberstam^{3,6}, Julia L.
7 MacIsaac^{1,2}, Kristy Dever^{1,2}, Toan Khanh Tran⁷, Kim Korinek⁸, Zachary Zimmer^{9,10}, Nanette R.
8 Lee¹¹, Thomas W. McDade^{12,13}, Christopher W. Kuzawa¹⁴, Kim M. Huffman¹⁵, Daniel W.
9 Belsky^{5,16}, Elisabeth B. Binder³, Darina Czamara³, Keegan Korthauer^{1,17}, Michael S. Kobor^{*1,18}

10
11 † These authors contributed equally and should be considered as co-first authors

12 * Please address all correspondence concerning this article to Dr. Michael S. Kobor at
13 michael.kobor@ubc.ca

- 14
15 1. BC Children's Hospital Research Institute, 950 West 28th Avenue, Vancouver, BC, V5Z
16 4H4, Canada
17 2. Department of Medical Genetics, Faculty of Medicine, University of British Columbia,
18 Vancouver, BC, V6T 1Z3, Canada
19 3. Department Genes and Environment, Max Planck Institute of Psychiatry, Munich, 80804,
20 Germany
21 4. International Max Planck Research School for Translational Psychiatry (IMPRS-TP),
22 Munich, 80804, Germany

- 23 5. Robert N. Butler Columbia Aging Center, Mailman School of Public Health, Columbia
24 University, New York, NY 10032, USA
- 25 6. Harvard Medical School/ MIT Institute of Technology MD-PhD program, Boston,
26 Massachusetts, MA 02115, USA
- 27 7. Family Medicine Department, Hanoi Medical University, Hanoi, Vietnam
- 28 8. Department of Sociology, University of Utah, Salt Lake City, Utah, UT 84112, USA
- 29 9. Department of Family Studies and Gerontology, Mount Saint Vincent University, Halifax,
30 NS, B3M 2J6, Canada
- 31 10. Canada Research Chair, Global Aging and Community Initiative, Canada
- 32 11. USC-Office of Population Studies Foundation, Inc., University of San Carlos, Cebu City,
33 Philippines
- 34 12. Department of Anthropology, Northwestern University, Evanston, Illinois, IL 60208 USA
- 35 13. Program in Child and Brain Development, CIFAR, Toronto, Ontario, Canada
- 36 14. Department of Anthropology and Institute for Policy Research, Northwestern University,
37 Evanston, Illinois, IL 60208, USA
- 38 15. Duke University School of Medicine, Durham, NC, 27701, USA
- 39 16. Department of Epidemiology, Columbia University Mailman School of Public Health,
40 New York, NY 10032, USA
- 41 17. Department of Statistics, Faculty of Science, University of British Columbia, Vancouver,
42 BC, V6T 1Z4, Canada
- 43 18. Edwin S.H. Leong Centre for Healthy Aging and Department of Medical Genetics,
44 University of British Columbia, Vancouver, BC, V6T 1Z4, Canada
- 45

46 **Keywords**

47 Epigenetics, DNA methylation, Illumina EPIC array, epigenetic clocks, inflammation and
48 lifestyle biomarkers, cell type deconvolution, replicate probes

49

50

51

52

53

54

55

56

57

58

59

60

61

62

63

64

65

66

67

68

69 **Abstract**

70 **Background:**

71 The recently launched DNA methylation profiling platform, Illumina MethylationEPIC
72 BeadChip Infinium microarray v2.0 (EPICv2), is highly correlated with measurements obtained
73 from its predecessor MethylationEPIC BeadChip Infinium microarray v1.0 (EPICv1). However,
74 the concordance between the two versions in the context of DNA methylation-based tools,
75 including cell type deconvolution algorithms, epigenetic clocks, and inflammation and lifestyle
76 biomarkers has not yet been investigated. To address this, we profiled DNA methylation on both
77 EPIC versions using matched venous blood samples from individuals spanning early to late
78 adulthood across four cohorts.

79 **Findings:**

80 Within each cohort, samples primarily clustered by the EPIC version they were measured on.
81 High concordance between EPIC versions at the array level, but variable concordance at the
82 individual probe level was noted. Significant differences between versions in estimates from
83 DNA methylation-based tools were observed, irrespective of the normalization method, with
84 some nuanced differences across cohorts and tools. Adjusting for EPIC version or calculating
85 estimates separately for each version largely mitigated these version-specific discordances.

86 **Conclusions:**

87 Our work illustrates the importance of accounting for EPIC version differences in research
88 scenarios, especially in meta-analyses and longitudinal studies, when samples profiled across

89 different versions are harmonized. Alongside DNA methylation-based tools, our observations
90 also have implications in interpretation of epigenome-wide association studies (EWAS) findings,
91 when results obtained from one version are compared to another, particularly for probes that are
92 poorly concordant between versions.

93

94

95

96

97

98

99

100

101

102

103

104

105

106

107

108

109

110

111

112 **Background**

113 Infinium Methylation BeadChip microarrays have been widely used to cost-effectively measure
114 the human DNA methylome in large scale and population-wide studies[1–3]. The recently
115 developed Illumina MethylationEPIC BeadChip Infinium microarray v2.0 (900K, EPICv2)
116 features a total of 936,866 probes, encompassing ~77% of the probes in the previous version, the
117 MethylationEPIC BeadChip Infinium microarray v1.0 B5 (850K, EPICv1), and over 200,000
118 new probes designed for increased coverage of enhancers, open chromatin regions, and CTCF-
119 binding domains[4]. EPICv2 also differs from its predecessor in the overall probe content and
120 utility, with annotation to the most recent GRCh38/h38 human genome build, differences in
121 probe design type and strand switches, and incorporation of new “nv” probes targeting recurrent
122 somatic cancer mutations. Unlike EPICv1 where each probe is unique, EPICv2 includes ~5100
123 probes that each have between 2-10 replicates, differentiated based on their probe names and
124 sequences[5]. Approximately 143,000 poorly performing probes on the EPICv1 have been
125 removed from the EPICv2, ~73% of which are likely to be influenced by underlying sequence
126 polymorphisms[6,7]. Overall, these modifications in EPICv2 intend to provide wider coverage of
127 the DNA methylome, with optimized performance across primary tissues and cancer cell lines,
128 and extended reliability across diverse human populations[6,7].

129
130 Previous iterations of Illumina Infinium microarrays (27K, 450K and EPICv1) have been widely
131 used to develop DNA methylation-based bioinformatic tools including cell type deconvolution
132 algorithms[8–10], a rapidly increasing and diverse set of epigenetic clocks[11–18], interleukin 6
133 (IL-6) and C-reactive protein (CRP) inflammation markers[19,20], and lifestyle biomarker
134 predictors such as smoking and alcohol use[21]. Simplistically speaking, these tools are based on

135 the strong correlations of DNA methylation levels at specific cytosine-guanine dinucleotides
136 (CpGs) with measured cell types, chronological age, and biomarker measures, respectively. The
137 currently available tools have been exclusively trained on one or more of the previous generation
138 of microarrays[11–14,16,17], and many, but not all, of predictive CpGs employed by these tools
139 are retained on EPICv2[6]. Illustrating the relevance of array iteration, estimates from some of
140 these DNA methylation-based tools, while highly correlated, are significantly different between
141 450K and EPICv1[22–24]. At a more basic level, DNA methylation profiles derived from a
142 limited set of human cell lines suggest a high agreement between EPICv1 and EPICv2. Given the
143 extensive use of Illumina DNA methylation arrays in primary human samples, and importantly,
144 across large population studies, it is imperative to determine the concordance of EPICv1 and
145 EPICv2 in these more complex yet highly relevant research settings.

146

147 Here, we used an unprecedented set of 67 primary human population samples and five technical
148 replicates to systematically assess the concordance of inferred estimates derived from a broad set
149 of DNA methylation-based tools between EPICv1 and EPICv2. We also tested whether EPIC
150 version differences might affect meta-analyses, which harness statistical power that comes from
151 combining multiple cohorts, and longitudinal studies, which often include samples profiled on
152 different arrays/versions. Specifically, we created sets of matched venous blood samples from 67
153 individuals across a diverse collection of four populations spanning early to late adulthood, and
154 profiled the DNA methylome using the EPICv1 and EPICv2 arrays. Using this unique dataset,
155 we tested the concordance of the two EPIC versions at both array and probe levels and illustrated
156 the potential contribution of EPIC version to overall DNA methylation variation. To explore if
157 these version differences are reflected in DNA methylation-based tools, including immune cell

158 type deconvolution algorithms, epigenetic clocks, inflammation and lifestyle biomarkers, we
159 compared their estimates between the two EPIC versions, and confirmed that these differences
160 persisted irrespective of data preprocessing methods. We also demonstrated different
161 remediation methods to account for these EPIC version discrepancies in epigenetic
162 investigations. Collectively, this work encourages careful consideration while harmonizing data
163 profiled on the two EPIC versions and comparing epigenome-wide association studies' (EWAS)
164 findings from one version to another.

165 **Results**

166 **Unsupervised clustering analyses of samples was primarily determined by EPIC version**

167 To compare the two most recent generations of Illumina MethylationEPIC BeadChip Infinium
168 microarrays, we measured the DNA methylomes of a subset of venous whole blood samples on
169 both EPICv1 and EPICv2 across three cohorts in the Kobor Lab, Vancouver, Canada (in-house
170 facility): (i) Vietnam Health and Aging Study (VHAS)[25], (ii) Cebu Longitudinal Health and
171 Nutrition Survey (CLHNS)[26], and (iii) Comprehensive Assessment of Long-term Effects of
172 Reducing Intake of Energy (CALERIE)[27], and an external cohort processed in a different
173 facility (Max Planck Institute of Psychiatry in Munich, Germany): Biological Classification of
174 Mental Disorders study (BeCOME)[28] (Table 1, Figure 1). These four cohorts represented
175 distinct demographic and biological characteristics such as sex and age range. Using
176 unsupervised hierarchical clustering in a cohort-wise manner across the 721,378 probes shared
177 between EPICv1 and EPICv2, we noted that samples exclusively clustered by EPIC version
178 (Figure 2B and 2C). Consistently, when smaller subsets of predictive CpGs employed by DNA
179 methylation-based tools were used for clustering, we still noted some separation of samples by

180 EPIC version, although not to the same extent as the clustering on shared probes (Supplementary
181 Figure 1). When clustering was performed on all the three cohorts processed by the in-house
182 facility, we similarly observed a clear demarcation of samples first by EPIC version, followed by
183 cohort despite their distinct characteristics (Figure 2A). Perhaps not surprisingly, when samples
184 from BeCOME were combined with the other three cohorts, we observed samples clustering by
185 the facility they were processed in, while still separating by EPIC version within the two
186 facilities (Supplementary Figure 2). Our findings remained consistent when we performed
187 unsupervised clustering using principal component analysis (PCA). The top three PC loadings,
188 corresponding to >98% of DNA methylation variation, were significantly associated with EPIC
189 version (Supplementary Figure 3). Overall, EPIC version was the primary contributor to
190 clustering of samples and explained a large proportion of DNA methylation variation.

191

192 **EPICv1 and EPICv2 probes shared consistently high correlation at array level but not at**
193 **the individual probe level**

194 Within three cohorts, technical replicate samples derived from the same individual after bisulfite
195 conversion were quantified on both EPIC versions at least twice, allowing us to examine the
196 technical variation within each version. Given that all samples were matched on both versions,
197 we were also able to compare these technical replicate samples between versions. We first used
198 Spearman correlation to assess array level concordance in technical replicates, calculated by
199 averaging DNA methylation (β) values across shared probes on per sample basis. We showed
200 high concordance between both between-versions and within-version technical replicates, though
201 the latter was relatively more correlated (between-versions correlations: 0.9737-0.9774; within-
202 version: 0.9858-0.9916). Next, we determined the reliability of technical replicates both

203 between- and within-version using intra-class correlation coefficients (ICC), and found slightly
204 lower agreement in between-versions technical replicates (0.9947-0.9958) than within-version
205 (0.9972-0.9983) (Supplementary Table 1). Finally, we assessed the error in technical replicates
206 between and within EPIC versions using root mean square root error (RMSE). As expected, the
207 mean RMSE between-versions (0.0367-0.0416) was slightly higher than the within-version
208 (0.0214-0.0264) (Supplementary Table 1).

209

210 Extending beyond the technical replicates to all the matched samples profiled on each version,
211 we noted high array level Spearman correlation ranging from 0.968 to 0.981 between EPICv1
212 and EPICv2, though this was at the array level (Supplementary Table 2). In contrast to the strong
213 array level concordance, Spearman correlations at the probe level, calculated as the concordance
214 of β values of individual probes across samples between versions, were not as congruent.
215 Specifically, only ~25% the probes per cohort had Spearman correlations greater than 0.70 while
216 the remaining ~75% probes showed a low mean correlation of <0.30 (Supplementary Table 3).
217 One plausible explanation for low probe level correlations of the majority of probes may be low
218 inter-sample variability. It has been previously reported that probes with a narrow range of DNA
219 methylation β values across samples tend to have poor correlations[22]. To test this, we
220 calculated pooled standard deviation (SD) across samples on a cohort basis, and defined the first
221 lower quartile (≈ 0.01 for each cohort) as the pooled SD threshold to denote low variability
222 (Supplementary Table 2). Supporting our hypothesis, we found that probes with Spearman
223 correlations ≤ 0.70 had significantly lower pooled SD or low variability compared to probes with
224 higher correlations (Supplementary Table 3). Specifically, of the probes with Spearman
225 correlation ≤ 0.70 , ~30% exhibited low inter-sample variability; in contrast, of probes with

226 Spearman correlation > 0.70 , only 0.069-5.577% exhibited low variability (Supplementary Table
227 6). We also cross-referenced these poorly-concordant probes, which we defined as probes with
228 low correlation despite their high variability, with low quality and unreliable probes identified in
229 previous annotations of the Illumina arrays[5,29–31]. Specifically, 0.11-2.39% of these poorly-
230 concordant probes overlapped with previously identified as cross hybridizing to multiple
231 genomic locations or mapped to genetic variant sites across all cohorts [5,29–31]
232 (Supplementary Table 4). Of the 82 probes that have undergone design type switches in
233 EPICv2[6], 27-40 probes also overlapped with our poorly-concordant probes in the four cohorts.
234 Overall, only a small fraction (~10%) of these poorly-concordant probes overlapped with probes
235 of bad quality, design type switch[6], and cross hybridization to the genome[5,29–31]
236 (Supplementary Table 5), while the rest still remained unexplained. In contrast, of the highly
237 correlated or low variability probes, ~80% overlapped with platform-bias free and high-
238 confidence mapping probes recently identified in cell lines[32], confirming the agreement of the
239 readouts at these probes (Supplementary Table 5).

240

241 We used the first lower quartile as the pooled SD threshold and Spearman correlation ≤ 0.70 to
242 denote probes with low concordance and high variability, however we acknowledge that there is
243 a continuum in the relationship between variability and correlation (Figure 2). To examine if a
244 more lenient threshold of variability and correlation would result in fewer unreliable probes
245 shared between versions, we additionally employed a pooled SD threshold of 0.05 and Spearman
246 correlation threshold of 0.50. When we relaxed the pooled SD threshold to 0.05, while
247 maintaining the Spearman correlation threshold of 0.70, the percentage of unreliable probes
248 reduced to 1.7-6.5% of the probes shared between versions; a further decrease to less than 0.6%

249 of shared probes was noted when the Spearman correlation threshold was reduced to 0.50
250 (Supplementary Table 6). In summary, we observed high concordance at the array level between
251 versions; however, on the probe level, there were a subset of probes with low concordance
252 between versions regardless of high inter-sample variability.

253 **Immune cell type proportions inferred by IDOL and auto probe selection methods were**
254 **significantly different between EPIC versions**

255 Cellular composition is a key contributor to whole blood DNA methylation variation and has
256 been associated with disease phenotypes and often included as a covariate in statistical models to
257 account for cell type heterogeneity[33–35]. Most studies do not measure actual cell counts and
258 rely on predicted values from DNA methylation-based algorithms. Given that these algorithms
259 use references profiled on previous arrays/versions, we tested whether there were differences in
260 cell type proportions estimated from the two EPIC versions using one of the most commonly
261 used cell type deconvolution methods for whole blood[10]. We compared the proportions of
262 twelve immune cell types using the *FlowSorted.Blood.EPIC* R package with two commonly used
263 probe selection methods: IDOL and auto. The IDOL method includes 1200 pre-selected probes,
264 which has over 99% coverage in EPICv2 (Table 2 and Supplementary material), and the auto
265 method includes 1200 probes independently selected for each EPIC version as described in
266 Methods. On comparing the probes selected for each EPIC version using the auto method, we
267 identified a large overlap of over 90% probes between the two EPIC versions, with only 10%
268 these auto-selected probes overlapping with the pre-selected IDOL probes (Supplementary
269 Figure 4).

270

271 We found high Spearman correlations between cell type proportions inferred on EPICv1 and
272 EPICv2, with an average correlation of 0.883 by the IDOL method and 0.890 by the auto method
273 (Supplementary Tables 7-8). Despite their high correlation, we identified significant differences
274 in estimated proportions of five and nine cell types between EPICv1 and EPICv2 using the IDOL
275 and auto methods, respectively, across the three in-house cohorts, with four cell types (Bas,
276 CD8mem, Mono, NK) commonly identified in both methods. Consistent findings were observed
277 in BeCOME with the auto method; two additional cell types (CD8mem and NK) showed
278 significant proportional differences between versions when the IDOL method was used
279 (Supplementary Figure 5, Supplementary Tables 7-8). Overall, estimated proportions were
280 significantly different between the EPIC versions across multiple cell types, and these findings
281 remained consistent irrespective of the probe selection method, albeit with varying effect sizes
282 depending on cell type and cohort (Figure 3, Supplementary Figure 5-6, and Supplementary
283 Tables 7-8).

284 **Epigenetic ages and EAAs were significantly different between EPIC versions depending**
285 **on analysis method**

286 Epigenetic clocks are based on the property that DNA methylation levels at specific CpGs highly
287 correlate with chronological age or age-related outcomes[11–14,16,17]. In order to evaluate the
288 concordance between EPICv1 and EPICv2 in the context of these DNA methylation-based tools,
289 we compared estimates from seven widely used first- and second- generation epigenetic clocks
290 in VHAS, CLHNS, and CALERIE (see Methods). Across these seven epigenetic clocks, ~77-
291 96% of predictive CpGs were retained on EPICv2 (Table 2 and Supplementary material). We
292 identified high Pearson correlations of 0.807-0.996 between chronological age and epigenetic
293 age obtained from both EPICv1 and EPICv2 (Supplementary Table 9). EPICv2 epigenetic ages

294 for all clocks were highly correlated with EPICv1 epigenetic ages (0.879-0.996), with
295 differences in epigenetic ages between technical replicates being 0.151-4.206 (Supplementary
296 Table 10), although we noted significant differences in epigenetic ages between EPICv2 and
297 EPICv1 in Hannum, Horvath skin and blood, and PhenoAge, with these differences ranging in
298 effect size from 0.267-4.137 (Supplementary Table 10, Supplementary Figure 7A). Consistent
299 with these results, in the external validation cohort BeCOME, EPICv1 and EPICv2 epigenetic
300 ages were highly correlated with chronological age and yet there were significant epigenetic age
301 differences between versions in all epigenetic clocks except again Horvath pan-tissue
302 (Supplementary Tables 9-10, Supplementary Figure 8A).

303

304 We also estimated epigenetic age acceleration (EAA), a measure of rate of aging which has been
305 associated with health outcomes, by considering samples profiled on each EPIC version
306 separately and in a combined manner (see Methods). Irrespective of how matched samples on the
307 two EPIC versions were considered for EAA calculation, we noted modest to high correlation
308 (0.574-0.960) of EAA between the EPIC versions. When EAA was calculated separately by
309 versions, we noted no significant differences between EPICv1 and EPICv2 (Supplementary
310 Table 11, Figure 4B, Supplementary Figures 9B and 10B). When clock estimates from the EPIC
311 versions were combined prior to EAA calculation, there were significant differences between
312 EPICv1 and EPICv2 for all clock EAAs except Horvath pan-tissue (Supplementary Table 11,
313 Figure 4C, Supplementary Figures 9C and 10C). To next test whether the different EPIC
314 versions contribute to observed EAA differences, we combined epigenetic ages in both EPIC
315 versions and then calculated EAAs by including version as a covariate in the linear regression. In
316 doing so, we noted that there were no significant EAA differences between the two EPIC

317 versions, akin to when EAA was calculated separately by version (Supplementary Table 11,
318 Figure 4D, Supplementary Figures 9D and 10D). We repeated the same analyses using
319 epigenetic clocks estimated based on principal components (PC clocks) rather than individual
320 predictive CpGs, as they have been shown to overcome unreliability in clock estimates due to
321 technical noise[36]. Once again, we noted that there were no significant EAA differences when
322 EAA was calculated for each EPIC version separately. When EAAs were calculated on
323 combined sets of matched samples, we noted significant differences in PCHorvath skin and
324 blood and PCPhenoAge, and these differences were no longer significant with EPIC version
325 adjustment (Supplementary Figures 11-13). Consistent with other cohorts, in BeCOME, we
326 noted similar findings in epigenetic ages, EAAs, and PC clocks estimates (Supplementary Table
327 11, Supplementary Figure 8 and 14).

328

329 On next evaluating the DunedinPACE, DNAmTL, and epiTOC clocks, we observed a high
330 correlation (0.699-0.983) of clock estimates between EPICv1 and EPICv2 (Supplementary Table
331 12). Unlike the epigenetic clocks above, when we examined the EPIC versions separately, we
332 noted that DNAmTL estimates were significantly different between versions in all four cohorts,
333 while DunedinPACE and epiTOC estimates were significantly different in three out of the four
334 cohorts (Supplementary Tables 11-12, Figure 5, and Supplementary Figures 8-10).

335 **Estimated CRP and smoking scores were significantly different between EPIC versions**

336 DNA methylation-based estimates of IL-6, CRP, smoking, and alcohol use are widely used as
337 reliable proxies of actual measurements in epigenetic studies[37]. Similar to other tools,
338 approximately 90% predictive CpGs were retained on EPICv2 (Table 2 and Supplementary

339 material) and estimates between EPICv1 and EPICv2 were modestly to highly correlated (0.788-
340 0.993) (Supplementary Table 13). When estimates were calculated separately by versions (EPIC
341 versions separate), we identified significantly different IL-6, CRP, alcohol, and smoking scores
342 between EPICv1 and EPICv2 in at least one of the four cohorts. When estimates from the EPIC
343 versions were first combined and then adjusted for version, as expected, we noted no significant
344 differences between EPICv1 and EPICv2 in any of these four predictors (Supplementary Table
345 13, Supplementary Figure 15).

346

347 **EPIC version differences remained significant irrespective of the choice of normalization**
348 **method, while upstream batch correction eliminated such differences**

349 Given the effect of data normalization on epigenetic clock estimations[23,38], we examined
350 whether normalization methods affect the observed differences between EPIC versions, obtained
351 after applying functional normalization (funnorm). To test this, we combined the shared probes
352 on the two EPIC versions and applied Beta-MIXture Quantile (BMIQ) normalization, and
353 subsequently calculated epigenetic ages, EAAs, and inflammation and lifestyle biomarker
354 estimates. Overall, the differences in estimates of these DNA methylation-based tools between
355 EPIC versions when BMIQ normalization was applied were consistent with those obtained in
356 functional normalized data, specifically in Horvath skin and blood and PhenoAge which were
357 consistent across the three in-house cohorts (Supplementary Figures 7, 16-21).

358

359 Next, we also examined if applying EPIC version correction using batch correction algorithms
360 can circumvent version-specific effects and eliminate the observed differences in DNA
361 methylation-based estimates between EPICv1 and EPICv2, given the observed contribution of

362 EPIC version in explaining DNA methylation variation. We tested this by combining common
363 probes on EPICv1 and EPICv2 after functional normalization or BMIQ normalization, and
364 sequentially adjusted for EPIC version, chip and sample position on chip (row) effects as
365 applicable using the ComBat function implemented in the *sva* R package[39]. As expected, when
366 epigenetic clocks, inflammation and lifestyle biomarkers were calculated using version-corrected
367 input β values, there were no significant differences in estimates between the EPIC versions
368 (Supplementary Figures 7, 22-24).

369

370 **Discussion**

371 Various generations of DNA methylation arrays, largely manufactured by Illumina, have had
372 tremendous impact on the field of epigenetics, enabling large population studies of human health
373 and disease. The most recently released Illumina EPICv2 microarray provides wider coverage of
374 the DNA methylome compared to its predecessor EPICv1, yet at the same time eliminates
375 approximately one-fifth of the previous probes. This then might create challenges for the utility
376 and transferability of the myriad bioinformatic tools developed for the EPICv1, especially if
377 some of the missing probes were included in a particular tool. Here, using matched venous blood
378 samples from 67 adults across four geographically diverse populations, we comprehensively
379 examined the concordance between EPIC versions in a wide range of commonly used DNA
380 methylation-based tools. Overall, our study identified notable differences between the two EPIC
381 versions at various levels, and provided some insights into possible remediation approaches.
382 First, we observed overall high array level concordance but variable probe level concordance,
383 with a subset of probes displaying poor agreement between versions despite high inter-sample
384 variability. Second, EPIC version differences were identified across all cohorts in DNA

385 methylation-based tools, including epigenetic clocks, inflammation and lifestyle biomarkers, and
386 cell type predictors. Third, discordance between EPIC versions was dampened by the manner of
387 statistical accounting of EPIC version. Fourth, irrespective of the choice of normalization method
388 EPIC version differences still persisted. Overall, our work emphasizes careful consideration of
389 research settings when i) samples across both EPIC versions are harmonized, and ii) findings
390 derived from one EPIC version are compared to those derived from the other version.

391
392 Initial comparisons of EPIC versions that were confined to immortalized cell lines and a limited
393 number of human primary samples reported generally good array level correlations between the
394 two EPIC versions[5–7]. However, these studies were not powered to investigate concordance at
395 the probe level nor did they compare DNA methylation-based tools such as epigenetic clocks,
396 cell types, and biomarker predictors, particularly across geographically diverse settings, which
397 are highly relevant for human population epigenetic studies. Using this population-based
398 framework, unsupervised clustering on samples across the three in-house cohorts (VHAS,
399 CLHNS, and CALERIE) using the shared probes between EPICv1 and EPICv2 showed that
400 samples clustered based on the EPIC version on which they were measured, despite cohort-
401 specific characteristics. Perhaps not surprisingly, given the differences in sample handling and
402 processing inherent to different experimental facilities, inclusion of the external validation cohort
403 BeCOME showed that samples clustered by facility first. However, performing these analyses on
404 each cohort separately, we again found that EPIC version was the principal driver of DNA
405 methylation variation, irrespective of the facility in which these samples were processed in. This
406 separation by EPIC version may be due to the variable concordance of individual probes between
407 the two versions. This was in general agreement with previous work which showed low

408 reliability across shared probes measured on previous iterations of Illumina arrays, namely 450K
409 and EPICv1[22,40,41]. While a small proportion of these poorly-concordant probes, skewed
410 toward lower inter-sample variability, could be attributed to their non-specific probe
411 hybridization to the genome, underlying genetic variation, or technical differences such as
412 altered EPICv2 probe design[5,6,29–31], the majority remain unexplained by these factors.
413 Further, these poorly-concordant probes will have implications in interpretation of EWAS
414 results, where validation of findings from one EPIC version to another may be challenging.

415
416 We observed significant systematic differences in measures derived from DNA methylation-
417 based tools. In the context of cell type prediction algorithms, there were significant differences in
418 proportions of various cell types, when using either the IDOL or auto prediction methods. These
419 differences may be reflective of version incompatibility between the reference library used, built
420 on previous Illumina microarrays, and EPICv2[10]. Further, they may be compounded by the
421 compositional nature of cell type estimates, meaning that any changes in the proportion of even
422 one cell type will influence the proportions of other cell types. Similarly, in the epigenetic clock
423 and biomarker predictors, we noted discordance in estimates obtained between EPICv1 and
424 EPICv2, though these observations were generally consistent across cohorts and tools with some
425 nuanced differences. It is reasonable to speculate that this discordance between versions may be
426 due to the varying number and weights of predictive CpGs absent on either EPIC version, and
427 the influence of subsequent imputation performed by the clock algorithms to account for this
428 missingness. However, our analyses using BMIQ normalization which only used shared probes
429 between the versions and thus had the same absent predictive CpGs in both versions, still showed

430 differences in estimates and EAAs, suggesting that absent CpGs are not the main contributor to
431 the version differences.

432

433 Although epigenetic clocks are often analyzed as direct comparisons of epigenetic ages as
434 described above, it has been noted that a regression-based measure of epigenetic age, EAA, is
435 more appropriate in most cases as it is robust to data preprocessing[11,23,37,38]. On calculating
436 EAAs by taking the common approach of including all samples in a cohort irrespective of
437 version, we noted that EAA estimates were different between versions, suggesting that this
438 method of calculating EAA is still sensitive to inherent variation between EPICv1 and EPICv2.
439 Using an alternate approach, when we calculated EAA estimates separately for samples profiled
440 on each EPIC version, we found that these differences were no longer significant. This indicates
441 that EAAs may be a suitable measure of epigenetic aging when version is taken into
442 consideration while calculating EAA. Similarly, we noted consistent differences between
443 versions in inflammation and lifestyle biomarker predictor scores, emphasizing again that it is
444 important to account for systematic version differences when calculating DNA methylation-
445 based measures.

446

447 Including EPIC version as a covariate in statistical models or employing version correction using
448 ComBat may be options to handle version-specific discrepancies, however, these approaches are
449 not appropriate in cases when EPIC version is fully or partially confounded with biological
450 variables. Our matched and balanced study design allowed us to correct for version using
451 ComBat, which expectedly dampened version differences. In cases of unbalanced study designs,
452 any adjustment for EPIC version can incorrectly remove important biological variation as well as

453 introduce false biological signals[42–45]. This ideal - and perhaps even unrealistic - scenario
454 starkly contrasts with a typical meta-analysis, where a researcher might wish to combine results
455 from multiple distinct sample groups measured on different EPIC versions. Furthermore, another
456 research setting that presents a similar challenge is a longitudinal study design, where the aim is
457 to explore DNA methylation changes over time. In such cases, when samples from each
458 timepoint are measured on different EPIC versions, it inevitably results in a confound between
459 the variable of interest, i.e., timepoint and EPIC version, thereby not enabling any version
460 correction. If samples from the previous timepoint are still available, one feasible approach is to
461 include a small number of these samples profiled on the previous EPIC version alongside
462 samples from the new timepoint to be profiled on EPICv2 such that any between version
463 differences can be monitored. It is also known that DNA methylation-based tools are sensitive to
464 normalization methods [23,37,38], and it is important to explore the contribution of such
465 approaches to observed EPIC version differences noted in the present study. By employing two
466 distinct normalization methods, namely funnorm and BMIQ, we found similar differences in
467 DNA methylation-based estimates based on version, irrespective of normalization method used.
468
469 On the strength of our matched sample design utilizing four different human cohorts, our study
470 improves the current understanding of the applicability of DNA methylation-based tools for
471 EPICv1 and EPICv2, however, there are several limitations. Our analyses may be limited by
472 relatively modest sample sizes within each cohort, despite this, our study includes matched
473 samples collected from adults with a wide age range and across diverse geographical regions.
474 While the time between EPICv1 and EPICv2 measurement varied across the cohorts, it offers a
475 more realistic representation of research settings where samples are collected and quantified

476 across multiple batches on different EPIC versions. Next, given that the training datasets of the
477 investigated epigenetic clocks were predominantly composed of European populations, the
478 suitability of investigated clocks may not be well established in our investigated Asian cohorts,
479 VHAS and CLHNS respectively [46–48]. However, differences in these cohorts were similar to
480 CALERIE and BeCOME, which are comprised primarily of individuals of European descent,
481 indicating that our findings were not limited to specific populations. Further, we compared
482 EPICv2 cell type proportions and biomarker scores to EPICv1, although we recognize that actual
483 cell counts and biomarker measurements would be more appropriate as the ground truth and
484 would be useful in validating our DNA methylation-based estimates. In spite of this, the primary
485 aim of the current work is to investigate the concordance in estimates between versions, and not
486 to evaluate the accuracy of biomarker prediction. Finally, although our study focused on venous
487 blood, a commonly used tissue in epigenetics research, we speculate that these EPIC version
488 differences will hold true in other tissue types as well. While multiple tissue types were not
489 collected in all of these cohorts, we had access to matched capillary and venous blood samples in
490 VHAS, which allowed us to at least test and confirm the consistency of our findings in another
491 blood preparation.

492 **Conclusions**

493 With the rapid generation of DNA methylation data profiled on the newer iterations of the
494 Illumina microarrays, integrating samples across these platforms poses a challenge, owing to
495 discrepancies in probe content among arrays/versions. Our findings highlight differences in the
496 new EPICv2 compared to EPICv1, demonstrate the influence of EPIC version on the majority of
497 commonly used DNA methylation-based tools, and provide possible remediation approaches to
498 minimize technical variation which may arise from inconsistencies between versions. We

499 therefore encourage careful consideration when harmonizing and interpreting DNA methylation
500 data across multiple arrays/versions to ensure reliability and reproducibility in epigenetics
501 analyses.

502 **Methods**

503 **Description of cohorts**

504 To compare the performance of the two most recent generations of MethylationEPIC BeadChip
505 Infinium microarrays in the context of DNA methylation-based clocks, biomarkers and cell type
506 proportion estimates, we measured the DNA methylomes of a subset of venous whole blood
507 samples on both EPICv1 and EPICv2 selected from the (i) Vietnam Health and Aging Study
508 (VHAS)[25], (ii) Cebu Longitudinal Health and Nutrition Survey (CLHNS)[26], and (iii)
509 Comprehensive Assessment of Long-term Effects of Reducing Intake of Energy (CALERIE)[27]
510 cohorts. The VHAS cohort additionally includes matched capillary blood samples, randomized
511 using the same array design on both EPIC versions, such that the concordance between EPICv1
512 and EPICv2 can be assessed in capillary blood as well ($n = 24 \times 2$ blood collection methods \times 2
513 versions). Samples from VHAS, CLHNS and CALERIE were processed in the same facility
514 (Kobor Lab, University of British Columbia and BC Children's Hospital Research Institute,
515 Vancouver, Canada). To compare our findings from the three cohorts processed in-house to
516 those from an external facility, we used an independent validation cohort, BeCOME. In this
517 dataset, DNA methylation was measured on EPICv1 and EPICv2 using matched samples at the
518 Max Planck Institute of Psychiatry in Munich, Germany (Table 1). The time between EPICv1
519 and EPICv2 array quantification was approximately one month and two years for VHAS and
520 CLHNS respectively. EPICv1 and EPICv2 array quantification was carried out at the same time

521 for CALERIE and BeCOME. Given that the demographic characteristics across the cohorts are
522 different (Table 1), we performed all analyses independently on the cohorts and reported the
523 findings in a cohort-specific manner, excluding the unsupervised clustering analyses as described
524 below.

525

526 **DNA methylation profiling, sample and probe quality control**

527 Using similar protocols for all three cohorts, DNA was extracted from samples, bisulfite
528 converted using EZ-96 DNA Methylation kits (Zymo Research, Irvine, CA), hybridized to the
529 MethylationEPIC BeadChip Infinium microarray v1.0 B5 (EPICv1) and Infinium
530 MethylationEPIC v2.0 (EPICv2) arrays, and scanned with the Illumina iScan 2000 to obtain
531 IDAT files that capture raw DNA methylation intensities. IDATs were read using *minfi* R
532 package to obtain β values that represent DNA methylation intensities for each CpG site ranging
533 from 0 (fully unmethylated) to 1 (fully methylated). Technical replicates derived from the same
534 sample after bisulfite conversion were quantified to monitor technical variation within each
535 EPIC version, independently for each cohort. Both VHAS and CALERIE included two technical
536 replicates each on EPICv1 and EPICv2, and CLHNS included one technical replicate on EPICv2
537 and no technical replicate on EPICv1. The external validation cohort BeCOME did not include
538 any technical replicates on either EPIC version. Sample quality control checks were performed
539 as described in previous publications[33,49]. Blood samples collected in the three cohorts and
540 the external validation cohort passed all 17 Illumina quality control metrics in the *ewastools* R
541 package[50,51], and detection *p*-value, beadcount, average methylated and unmethylated
542 intensity metrics in the *minfi* R package (Supplementary Table 14). We also performed sample
543 identity checks using unsupervised hierarchical clustering analysis on the 57 single nucleotide

544 polymorphism (SNP) probes that are common to both EPIC versions, and noted that matched
545 samples from the same individual assessed on EPICv1 and EPICv2 grouped together.

546

547 In order to identify EPICv1 and EPICv2 probes of poor quality, we performed quality control
548 checks using the detectionP and beadcount functions in the *minfi* and *wateRmelon* R packages,
549 respectively. Probes with detection p-value > 0.01 or beadcount < 3 in greater than 1% of the
550 samples were flagged (VHAS- EPICv1: 59,233, EPICv2: 46,735, common to both versions:
551 4,826; CLHNS-EPICv1: 23,793, EPICv2: 17,587, common to both versions: 991; CALERIE-
552 EPICv1: 29,608, EPICv2: 24,872, common to both versions: 1,292; BeCOME-EPICv1: 12,511,
553 EPICv2: 20411, common to both versions: 2,714), but all probes in EPICv1 and EPICv2 were
554 retained for subsequent analyses.

555

556 **Unsupervised clustering analyses on DNA methylation data**

557 To perform unsupervised hierarchical clustering on samples, we calculated array level Spearman
558 correlations using the 721,378 probes shared between EPICv1 and EPICv2 in pair-wise manner
559 for all the samples in the four cohorts. Array level Spearman correlations were then clustered by
560 the complete linkage method with Euclidean distance using the *hclust* function implemented in
561 the *stats* R package[52] and visualized by *heat*map in the *heatmap* R package[53]. We first
562 performed clustering on each of the four cohorts separately, then by combining the three cohorts
563 processed in the in-house facility (VHAS, CLHNS and CALERIE), and finally by combining all
564 four cohorts regardless of processing facility. Grouping cohorts once again in a similar manner,
565 we performed principal component analyses (PCA) using the shared probes between the EPIC

566 versions. We tested the association between each of the top five PC loadings and EPIC version,
567 cohort, and sex by employing one-way analysis of variance (ANOVA) or t-tests and applying a
568 Bonferroni multiple test correction. The percentage of DNA methylation variation explained by
569 each variable (EPIC version, cohort, and sex) was calculated as the ANOVA or t-test R-squared
570 value. It should be noted that while performing the PCA on each cohort independently, we did
571 not test the association between PC loadings and sex in the CLHNS cohort since this cohort
572 comprises of only females; for the other three cohorts, associations with EPIC version, cohort,
573 and sex were tested.

574 **DNA methylation data preprocessing and replicate probe analyses**

575 To account for color and probe-type bias, we performed functional normalization (funnorm) with
576 background correction and dye-bias normalization (noob) in the *minfi* R package[54,55]
577 independently on EPICv1 and EPICv2 samples for each cohort. Cohort-specific technical
578 replicate sample correlations were used to monitor preprocessing (technical replicates were not
579 available in the BeCOME external validation cohort). Between technical replicate samples on the
580 same EPIC version, improved Spearman correlations of whole array β values and reduced root
581 mean square error (RMSE) were observed as processing progressed from raw (VHAS: Spearman
582 $\rho = 0.9832$, RMSE = 0.0306; CLHNS: Spearman $\rho = 0.9890$, RMSE = 0.0235; CALERIE:
583 Spearman $\rho = 0.9859$, RMSE = 0.0349) to funnorm normalized data (VHAS: Spearman $\rho =$
584 0.9851, RMSE=0.0288; CLHNS: Spearman $\rho = 0.9917$, RMSE = 0.0231, CALERIE:
585 Spearman $\rho = 0.9887$, RMSE = 0.0223). Array level reliability of within- and between-EPIC
586 version technical replicates were assessed by intra-class correlation coefficients (ICC) with the
587 two-way random-effects model as previously described[40,56]. Specifically, array level ICC was
588 calculated using the technical replicates as the repeated measures (“raters”) and each probe

589 represented a “target” or “subject”. Within-EPIC version ICCs were calculated based on the
590 technical replicates within the same EPIC version, while between-EPIC version ICC were based
591 on the matched technical replicates on EPICv1 and EPICv2.

592

593 To calculate estimates of DNA methylation-based tools, noob corrected data was used as input
594 for cell type deconvolution, and funnorm normalized data was used as input for epigenetic clocks
595 and biomarkers. In addition, to test whether normalization methods influence DNA methylation-
596 based tools, we compared estimates calculated by combining the common probes on EPICv1 and
597 EPICv2 after noob correction in a cohort-wise manner for VHAS, CLHNS, CALERIE, and
598 BeCOME, and subsequently applying Beta-Mixture Quantile (BMIQ) normalization
599 implemented in the *wateRmelon* R package[57]. Due to their type I and type II design switch
600 between EPICv1 and EPICv2[6], 82 probes were removed prior to BMIQ normalization. To
601 account for any systematic bias in DNA methylation measurements[39] and subsequently test
602 whether there are differences in DNA methylation-based estimates between EPIC versions, we
603 applied batch correction for EPIC version, chip and row on funnorm normalized data using the
604 ComBat function implemented in the *sva* R package[39]. We applied Pearson correlation to
605 evaluate linear relationships to age in the epigenetic clock analyses, while in all analyses we
606 applied Spearman correlation. Absolute β value differences of within EPIC version technical
607 replicates on each of the common probes were used to determine technical noise of β value per
608 probe. Absolute differences of within EPIC version technical replicates in DNA methylation-
609 based tool estimates (cell type deconvolution algorithms, epigenetic clocks, and inflammation
610 and lifestyle biomarkers) were used to indicate within EPIC version technical error. Technical

611 replicates were removed prior to calculating correlations and performing statistical tests
612 comparing EPICv1 and EPICv2.

613

614 Given that there are certain probes on EPICv2 having two or more replicates (replicate probes),
615 we characterized their distribution across the genome, and compared three strategies to collapse
616 them into a single β value (based on detection p -value, mean and median). Our analyses
617 identified that collapsed β values of EPICv2 replicate probes obtained using all three methods
618 were highly correlated to corresponding EPICv1 probes, therefore EPICv2 replicate probes with
619 lowest detection p -value were chosen as the representative probe based on previous
620 recommendation[6] (Supplementary Material), and this approach was used for all the reported
621 subsequent analyses.

622

623 **Estimation of immune cell type proportions using DNA methylation-based cell type** 624 **deconvolution**

625 Cellular composition in heterogeneous tissue such as whole blood is one of the key contributors
626 to the variation in DNA methylation profiles of bulk tissue[58,59]. In the absence of complete
627 cell count data for the study samples, we estimated proportions of twelve immune cell types,
628 basophils (Bas), naïve and memory B cells (Bnv, Bmem), naïve and memory CD4+ T cells
629 (CD4nv, CD4mem), naïve and memory CD8+ T cells (CD8nv, CD8mem), eosinophils (Eos),
630 monocytes (Mono), neutrophils (Neu), natural killer (NK), and T regulatory cells (Treg) from
631 matched venous blood samples measured on the two EPIC versions. We used two methods of
632 probe selection to estimate these cell type proportions: (i) the extended Identifying Optimal DNA

633 methylation Libraries reference (IDOL), with probes not represented on EPICv2 removed from
634 the reference before cell type proportions estimation in EPICv2 samples, and (ii) the auto method
635 which selects the top 100 probes with F-stat p -value $< 1E-8$ for each cell type with the greatest
636 magnitude of methylation difference, both implemented in the *FlowSorted.Blood.EPIC* R
637 package with noob corrected values as recommended[10].

638 **Estimation of epigenetic age and epigenetic age acceleration**

639 We compared the performance of eight commonly used epigenetic clocks between EPICv1 and
640 EPICv2 in VHAS, CLHNS, CALERIE, and the external validation cohort BeCOME. Epigenetic
641 clocks analyses on capillary blood samples in the VHAS cohort were also performed
642 (Supplementary material, Supplementary Figures 25-28). Epigenetic age of first generation
643 clocks including Horvath pan-tissue[11], Hannum[12], and Horvath skin and blood clocks[13],
644 and second generation clocks including PhenoAge[14], and GrimAge[15] were obtained from
645 the online DNA Methylation Age Calculator (<https://dnamage.genetics.ucla.edu/new>). Missing
646 clock CpG β value imputation was performed by the clock algorithms. For these clocks, we
647 calculated epigenetic age acceleration (EAA), a measure of rate of aging commonly used in
648 epigenetic clock investigations, by employing three approaches independently for each cohort.

- 649 1. **EPIC version separate:** we separated epigenetic ages of EPICv1 and EPICv2 samples
650 and then calculated EAA independently on EPICv1 and EPICv2 samples by extracting
651 residuals from the linear regression model: Epigenetic age \sim chronological age.
- 652 2. **EPIC versions combined:** we first combined epigenetic ages of EPICv1 and EPICv2
653 samples and then calculated EAA by extracting residuals from the linear regression
654 model: Epigenetic age \sim chronological age.

655 3. **EPIC versions combined and version adjusted:** we first combined epigenetic ages of
656 EPICv1 and EPICv2 samples and calculated EAA by extracting residuals from the linear
657 regression model: Epigenetic age \sim chronological age + EPIC version.

658 To evaluate if there are significant differences in principal components (PC) clock[36] estimates,
659 which are more robust to technical noise, by EPIC version, we first estimated epigenetic ages by
660 the R script provided (<https://github.com/MorganLevineLab/PC-Clocks>) and then calculated
661 EAAs using the approaches mentioned above.

662
663 DunedinPACE, a rate-based clock, was calculated using the DunedinPACE R package[17], and
664 the two other clocks, epiTOC and DNA methylation-based estimator of telomere length
665 (DNAmTL)[16] were obtained using the *getEpiTOC* function in the *cgageR* R package[18] and
666 the online DNA Methylation Age Calculator (<https://dnamage.genetics.ucla.edu/new>),
667 respectively. Missing clock CpG β value imputation was performed by the clock algorithms.
668 Unlike EAA calculation, there were no secondary measures calculated from these three clock
669 estimates in our analyses. Estimates remained the same when calculated by the EPIC versions
670 separate or combined approach, therefore, we employed only two approaches for each cohort:

- 671 1. **EPIC version separate:** rate-based and other clock estimates were calculated for
672 EPICv1 and EPICv2 samples without EPIC version adjustment.
- 673 2. **EPIC versions combined and version adjusted:** rate-based and other clock estimates
674 were first calculated for EPICv1 and EPICv2 samples, and were subsequently adjusted
675 for EPIC versions by regressing out EPIC versions using linear regression model: Rate
676 estimate \sim EPIC version.

677 Using paired *t*-tests and applying a Bonferroni multiple test correction, we evaluated differences
678 in epigenetic clock estimations and EAAs (as well as biomarker predictor scores and cell type
679 proportions described below) between matched samples assessed on EPICv1 and EPICv2 in a
680 cohort-specific manner. Statistical significance was defined as Bonferroni adjusted *p*-value <
681 0.05. Effect sizes were measured by Cohen's *d*, and classified as “small” (*d* = 0.2-0.49),
682 “medium” (*d* = 0.5-0.79), and “large” (*d* ≥ 0.8) based on recommended benchmarks[60].

683 **Estimation of DNA methylation-based inflammation, smoking, and alcohol scores**

684 Among other DNA methylation-based tools are inflammation, smoking and alcohol score
685 predictors, which provide biomarker measures that correlate with levels of inflammatory markers
686 (IL-6, CRP), smoking and alcohol use, respectively. DNA methylation-derived scores of IL-6,
687 CRP, smoking and alcohol use were calculated as a weighted sum of coefficients derived from
688 published lists of predictive CpGs[19–21]. Being that these biomarkers were trained on previous
689 Illumina arrays, we sought out to determine the correlation of derived DNA methylation-based
690 scores between EPICv1 and EPICv2, and compare these scores without version adjustment
691 (EPIC version separate) and with version adjustment (EPIC versions combined and adjusted)
692 using approaches similar to the rate-based and other epigenetic clocks.

693 **References**

694 1. Battram T, Yousefi P, Crawford G, Prince C, Shekhali Babaei M, Sharp G, et al. The EWAS
695 Catalog: a database of epigenome-wide association studies. *Wellcome Open Res.* 2022;7:41.

- 696 2. Kuzawa CW, Ryan CP, Adair LS, Lee NR, Carba DB, MacIsaac JL, et al. Birth weight and
697 maternal energy status during pregnancy as predictors of epigenetic age acceleration in young
698 adults from metropolitan Cebu, Philippines. *Epigenetics*. 2022;17:1535–45.
- 699 3. Li M, Zou D, Li Z, Gao R, Sang J, Zhang Y, et al. EWAS Atlas: a curated knowledgebase of
700 epigenome-wide association studies. *Nucleic Acids Res*. 2019;47:D983–8.
- 701 4. Infinium MethylationEPIC v2.0 BeadChip. Infinium MethylationEPIC v2.0 BeadChip. 2023;
- 702 5. Peters TJ, Meyer B, Ryan L, Achinger-Kawecka J, Song J, Campbell EM, et al.
703 Characterisation and reproducibility of the HumanMethylationEPIC v2.0 BeadChip for DNA
704 methylation profiling. *BMC Genomics*. 2024;25:251.
- 705 6. Kaur D, Lee SM, Goldberg D, Spix NJ, Hinoue T, Li H-T, et al. Comprehensive evaluation of
706 the Infinium human MethylationEPIC v2 BeadChip. *Epigenetics Commun*. 2023;3:6.
- 707 7. Noguera-Castells A, García-Prieto CA, Álvarez-Errico D, Esteller M. Validation of the new
708 EPIC DNA methylation microarray (900K EPIC v2) for high-throughput profiling of the human
709 DNA methylome. *Epigenetics*. 2023;18:2185742.
- 710 8. Houseman EA, Molitor J, Marsit CJ. Reference-free cell mixture adjustments in analysis of
711 DNA methylation data. *Bioinforma Oxf Engl*. 2014;
- 712 9. Salas LA, Koestler DC, Butler RA, Hansen HM, Wiencke JK, Kelsey KT, et al. An optimized
713 library for reference-based deconvolution of whole-blood biospecimens assayed using the
714 Illumina HumanMethylationEPIC BeadArray. *Genome Biol*. 2018;19:64.

- 715 10. Salas LA, Zhang Z, Koestler DC, Butler RA, Hansen HM, Molinaro AM, et al. Enhanced
716 cell deconvolution of peripheral blood using DNA methylation for high-resolution immune
717 profiling. *Nat Commun.* 2022;13:761.
- 718 11. Horvath S. DNA methylation age of human tissues and cell types. *Genome Biol.*
719 2013;14:R115.
- 720 12. Hannum G, Guinney J, Zhao L, Zhang L, Hughes G, Sada S, et al. Genome-wide
721 Methylation Profiles Reveal Quantitative Views of Human Aging Rates. *Mol Cell.* 2013;49:359–
722 67.
- 723 13. Horvath S, Oshima J, Martin GM, Lu AT, Quach A, Cohen H, et al. Epigenetic clock for skin
724 and blood cells applied to Hutchinson Gilford Progeria Syndrome and *ex vivo* studies. *Aging.*
725 2018;10:1758–75.
- 726 14. Levine ME, Lu AT, Quach A, Chen BH, Assimes TL, Bandinelli S, et al. An epigenetic
727 biomarker of aging for lifespan and healthspan. *Aging.* 2018;10:573–91.
- 728 15. Lu AT, Quach A, Wilson JG, Reiner AP, Aviv A, Raj K, et al. DNA methylation GrimAge
729 strongly predicts lifespan and healthspan. *Aging.* 2019;11:303–27.
- 730 16. Lu AT, Seeboth A, Tsai P-C, Sun D, Quach A, Reiner AP, et al. DNA methylation-based
731 estimator of telomere length. *Aging.* 2019;11:5895–923.
- 732 17. Belsky DW, Caspi A, Corcoran DL, Sugden K, Poulton R, Arseneault L, et al.
733 DunedinPACE, a DNA methylation biomarker of the pace of aging. Deelen J, Tyler JK,
734 Suderman M, Deelen J, editors. *eLife.* 2022;11:e73420.

- 735 18. Yang Z, Wong A, Kuh D, Paul DS, Rakyan VK, Leslie RD, et al. Correlation of an
736 epigenetic mitotic clock with cancer risk. *Genome Biol.* 2016;17:205.
- 737 19. Stevenson AJ, Gadd DA, Hillary RF, McCartney DL, Campbell A, Walker RM, et al.
738 Creating and Validating a DNA Methylation-Based Proxy for Interleukin-6. *J Gerontol A Biol*
739 *Sci Med Sci.* 2021;76:2284–92.
- 740 20. Wielscher M, Mandaviya PR, Kuehnel B, Joehanes R, Mustafa R, Robinson O, et al. DNA
741 methylation signature of chronic low-grade inflammation and its role in cardio-respiratory
742 diseases. *Nat Commun.* 2022;13:2408.
- 743 21. McCartney DL, Hillary RF, Stevenson AJ, Ritchie SJ, Walker RM, Zhang Q, et al.
744 Epigenetic prediction of complex traits and death. *Genome Biol.* 2018;19:136.
- 745 22. Solomon O, MacIsaac J, Quach H, Tindula G, Kobor MS, Huen K, et al. Comparison of
746 DNA methylation measured by Illumina 450K and EPIC BeadChips in blood of newborns and
747 14-year-old children. *Epigenetics.* 2018;13:655–64.
- 748 23. McEwen LM, Jones MJ, Lin DTS, Edgar RD, Husquin LT, MacIsaac JL, et al. Systematic
749 evaluation of DNA methylation age estimation with common preprocessing methods and the
750 Infinium MethylationEPIC BeadChip array. *Clin Epigenetics.* 2018;10:123.
- 751 24. Dhingra R, Kwee LC, Diaz-Sanchez D, Devlin RB, Cascio W, Hauser ER, et al. Evaluating
752 DNA methylation age on the Illumina MethylationEPIC Bead Chip. *PLOS ONE.*
753 2019;14:e0207834.

- 754 25. Korinek K, Teerawichitchainan B, Zimmer Z, Brindle E, Nguyen TKC, Nguyen HM, et al.
755 Design and measurement in a study of war exposure, health, and aging: protocol for the Vietnam
756 health and aging study. *BMC Public Health*. 2019;19:1351.
- 757 26. Adair LS, Popkin BM, Akin JS, Guilkey DK, Gultiano S, Borja J, et al. Cohort Profile: The
758 Cebu Longitudinal Health and Nutrition Survey. *Int J Epidemiol*. 2011;40:619–25.
- 759 27. Rochon J, Bales CW, Ravussin E, Redman LM, Holloszy JO, Racette SB, et al. Design and
760 conduct of the CALERIE study: comprehensive assessment of the long-term effects of reducing
761 intake of energy. *J Gerontol A Biol Sci Med Sci*. 2011;66:97–108.
- 762 28. Brückl TM, Spoomaker VI, Sämann PG, Brem A-K, Henco L, Czamara D, et al. The
763 biological classification of mental disorders (BeCOME) study: a protocol for an observational
764 deep-phenotyping study for the identification of biological subtypes. *BMC Psychiatry*.
765 2020;20:213.
- 766 29. Pidsley R, Zotenko E, Peters TJ, Lawrence MG, Risbridger GP, Molloy P, et al. Critical
767 evaluation of the Illumina MethylationEPIC BeadChip microarray for whole-genome DNA
768 methylation profiling. *Genome Biol*. 2016;17:208.
- 769 30. Price EM, Cotton AM, Lam LL, Farré P, Emberly E, Brown CJ, et al. Additional annotation
770 enhances potential for biologically-relevant analysis of the Illumina Infinium
771 HumanMethylation450 BeadChip array. *Epigenetics Chromatin*. 2013;6:4.
- 772 31. McCartney DL, Walker RM, Morris SW, McIntosh AM, Porteous DJ, Evans KL.
773 Identification of polymorphic and off-target probe binding sites on the Illumina Infinium
774 MethylationEPIC BeadChip. *Genomics Data*. 2016;9:22–4.

- 775 32. Chen BH, Zhou W. mLiftOver: harmonizing data across Infinium DNA methylation
776 platforms. *Bioinformatics*. 2024;40:btac423.
- 777 33. Merrill SM, Gladish N, Fu MP, Moore SR, Konwar C, Giesbrecht GF, et al. Associations of
778 peripheral blood DNA methylation and estimated monocyte proportion differences during
779 infancy with toddler attachment style. *Attach Hum Dev*. 2023;25:132–61.
- 780 34. Ryan CP, Jones MJ, Edgar RD, Lee NR, Kobor MS, McDade TW, et al. Immune cell type
781 and DNA methylation vary with reproductive status in women: possible pathways for costs of
782 reproduction. *Evol Med Public Health*. 2022;10:47–58.
- 783 35. Kong Y, Rastogi D, Seoighe C, Grealley JM, Suzuki M. Insights from deconvolution of cell
784 subtype proportions enhance the interpretation of functional genomic data. *PLOS ONE*.
785 2019;14:e0215987.
- 786 36. Higgins-Chen AT, Thrush KL, Wang Y, Minter CJ, Kuo P-L, Wang M, et al. A
787 computational solution for bolstering reliability of epigenetic clocks: Implications for clinical
788 trials and longitudinal tracking. *Nat Aging*. 2022;2:644–61.
- 789 37. Engelbrecht H-R, Merrill SM, Gladish N, MacIsaac JL, Lin DTS, Ecker S, et al. Sex
790 differences in epigenetic age in Mediterranean high longevity regions. *Front Aging*.
791 2022;3:1007098.
- 792 38. Ori APS, Lu AT, Horvath S, Ophoff RA. Significant variation in the performance of DNA
793 methylation predictors across data preprocessing and normalization strategies. *Genome Biol*.
794 2022;23:225.

- 795 39. Leek JT, Johnson WE, Parker HS, Jaffe AE, Storey JD. The sva package for removing batch
796 effects and other unwanted variation in high-throughput experiments. *Bioinforma Oxf Engl.*
797 2012;28:882–3.
- 798 40. Sugden K, Hannon EJ, Arseneault L, Belsky DW, Corcoran DL, Fisher HL, et al. Patterns of
799 Reliability: Assessing the Reproducibility and Integrity of DNA Methylation Measurement.
800 *Patterns.* 2020;1:100014.
- 801 41. Olstad EW, Nordeng HME, Sandve GK, Lyle R, Gervin K. Low reliability of DNA
802 methylation across Illumina Infinium platforms in cord blood: implications for replication
803 studies and meta-analyses of prenatal exposures. *Clin Epigenetics.* 2022;14:80.
- 804 42. Price EM, Robinson WP. Adjusting for Batch Effects in DNA Methylation Microarray Data,
805 a Lesson Learned. *Front Genet.* 2018;9:83.
- 806 43. Buhule OD, Minster RL, Hawley NL, Medvedovic M, Sun G, Viali S, et al. Stratified
807 randomization controls better for batch effects in 450K methylation analysis: a cautionary tale.
808 *Front Genet.* 2014;5:354.
- 809 44. Nygaard V, Rødland EA, Hovig E. Methods that remove batch effects while retaining group
810 differences may lead to exaggerated confidence in downstream analyses. *Biostat Oxf Engl.*
811 2016;17:29–39.
- 812 45. Zindler T, Frieling H, Neyazi A, Bleich S, Friedel E. Simulating ComBat: how batch
813 correction can lead to the systematic introduction of false positive results in DNA methylation
814 microarray studies. *BMC Bioinformatics.* 2020;21:271.

- 815 46. Lin W-Y. Epigenetic clocks derived from western samples differentially reflect Taiwanese
816 health outcomes. *Front Genet.* 2023;14:1089819.
- 817 47. Horvath S, Gurven M, Levine ME, Trumble BC, Kaplan H, Allayee H, et al. An epigenetic
818 clock analysis of race/ethnicity, sex, and coronary heart disease. *Genome Biol.* 2016;17:171.
- 819 48. Cronjé HT, Nienaber-Rousseau C, Min JL, Green FR, Elliott HR, Pieters M. Comparison of
820 DNA methylation clocks in Black South African men. *Epigenomics.* 2021;13:437–49.
- 821 49. Konwar C, Asiimwe R, Inkster AM, Merrill SM, Negri GL, Aristizabal MJ, et al. Risk-
822 focused differences in molecular processes implicated in SARS-CoV-2 infection: corollaries in
823 DNA methylation and gene expression. *Epigenetics Chromatin.* 2021;14:54.
- 824 50. Murat K, Grüning B, Poterlowicz PW, Westgate G, Tobin DJ, Poterlowicz K. Ewastools:
825 Infinium Human Methylation BeadChip pipeline for population epigenetics integrated into
826 Galaxy. *GigaScience.* 2020;9:giaa049.
- 827 51. Illumina Inc. BeadArray Controls Reporter Software Guide. 2015;
- 828 52. R Core Team. R: A language and environment for statistical computing. R Foundation for
829 Statistical Computing. 2022; Available from: <https://www.R-project.org/>
- 830 53. Kolde R. pheatmap: Pretty Heatmaps. 2019;
- 831 54. Fortin J-P, Labbe A, Lemire M, Zanke BW, Hudson TJ, Fertig EJ, et al. Functional
832 normalization of 450k methylation array data improves replication in large cancer studies.
833 *Genome Biol.* 2014;15:503.

834 55. Triche TJ, Weisenberger DJ, Van Den Berg D, Laird PW, Siegmund KD. Low-level
835 processing of Illumina Infinium DNA Methylation BeadArrays. *Nucleic Acids Res.*
836 2013;41:e90.

837 56. Koo TK, Li MY. A Guideline of Selecting and Reporting Intraclass Correlation Coefficients
838 for Reliability Research. *J Chiropr Med.* 2016;15:155–63.

839 57. Teschendorff AE, Marabita F, Lechner M, Bartlett T, Tegner J, Gomez-Cabrero D, et al. A
840 beta-mixture quantile normalization method for correcting probe design bias in Illumina
841 Infinium 450 k DNA methylation data. *Bioinformatics.* 2013;29:189–96.

842 58. Jones MJ, Moore SR, Kobor MS. Principles and Challenges of Applying Epigenetic
843 Epidemiology to Psychology. 2017;30.

844 59. Zheng SC, Beck S, Jaffe AE, Koestler DC, Hansen KD, Houseman AE, et al. Correcting for
845 cell-type heterogeneity in epigenome-wide association studies: revisiting previous analyses. *Nat*
846 *Methods.* 2017;14:216–7.

847 60. Cohen J. *Statistical Power Analysis for the Behavioral Sciences.* 2nd ed. New York:
848 Routledge; 1988.

849

850

851 **Declarations**

852 **Ethics approval and consent to participate**

853 This study was approved by the University of British Columbia Research Ethics Boards (H18-
854 03136) and the University of Utah Institutional Review Board (IRB 00098861).

855

856 **Consent for publication**

857 Not applicable.

858 **Availability of data and materials**

859 The datasets generated and/or analyzed during the current study are not publicly available but are
860 available from the corresponding author or cohort owners/custodians upon reasonable request.

861 The EPICv2 preprocessing pipeline and analysis scripts in R are available on GitHub

862 https://github.com/kobor-lab/EPICv2_QC_preprocessing, and [https://github.com/kobor-](https://github.com/kobor-lab/EPICv1v2_comparison_manuscript)

863 [lab/EPICv1v2_comparison_manuscript](https://github.com/kobor-lab/EPICv1v2_comparison_manuscript).

864

865 **Competing interests**

866 D.W.B. is listed as an inventor of the Duke University and University of Otago invention

867 DunedinPACE, which is licensed to TruDiagnostic. The other authors declare that they have no

868 competing interests.

869 **Funding**

870 This work received supported from the Canadian Institutes of Health Research (CIHR) / Project
871 Grant (Sponsor Reference Number: PJT-175309), National Institute on Aging of the National
872 Institutes of Health under Award Number R01AG052537, National Institutes of Health /
873 Research Project Grant (R01) (Sponsor Reference Number: 5R01AG061006-05), US National
874 Institute on Aging Grants R01AG061378, Alexander von Humboldt Foundation for the German
875 Chancellor Fellowship, the National Institute of General Medical Sciences (Award Number
876 T32GM144273), BC Children's Hospital Research Investigator Grant Award Program, BC
877 Children's Hospital Research Institute Establishment Award, and Edwin S.H. Leong Centre for
878 Healthy Aging.

879

880 **Authors' contributions**

881 Conceptualization: B.C.Z., M.S.J., C.K., K.Korthauer, M.S.K.; biological data
882 collection/generation: T.K.T., K.Korinek, K.M.H., N.R.L., E.B.B., T.W.M., C.W.K., Z.Z.,
883 D.W.B., M.S.K.; DNA methylation data generation: J.L.M., K.D., M.S.K. (Kobor Lab facility),
884 E.B.B. (MPIP); DNA methylation data curation and processing: B.C.Z., M.S.J., N.Y., H-R.E.,
885 A.A.H., D.C. J.W.; Phenotypic data curation: T.K.T., K. Korinek, K.M.H., N.R.L., E.B.B.,
886 T.W.M., C.W.K., Z.Z., D.W.B.; Data analysis: B.C.Z., M.S.J.; Interpretation of results: M.S.J.,
887 C.K., B.C.Z., K.Korthauer, M.S.K.; Manuscript writing: M.S.J., C.K., B.C.Z., M.S.K.;
888 Figures/visualization: B.C.Z., M.S.J.; Manuscript review: all authors; Cohort
889 Owners/Custodians: T.K.T., K. Korinek, K.M.H., N.R.L., E.B.B., T.W.M., C.W.K., Z.Z.,
890 D.W.B.

891

892 **Acknowledgements**

893 We thank Dr. Sarah Merrill, Maggie Fu, and Dr. Kimberly Schmidt for their helpful feedback
894 during manuscript preparation. We would also like to thank all cohort participants for their
895 involvement and providing biological samples for research, and cohort study teams for their
896 efforts. We wish to thank Monika Rex-Haffner and the whole BeCOME study team for their
897 technical assistance. This research utilized the *FlowSorted.BloodExtended.EPIC* software
898 packages developed at Dartmouth College, which are governed by the licensing terms provided
899 by Dartmouth Technology Transfer. D.W.B. and M.S.K. are fellows of the CIFAR CBD
900 Network.

901


902

903

904

905

906

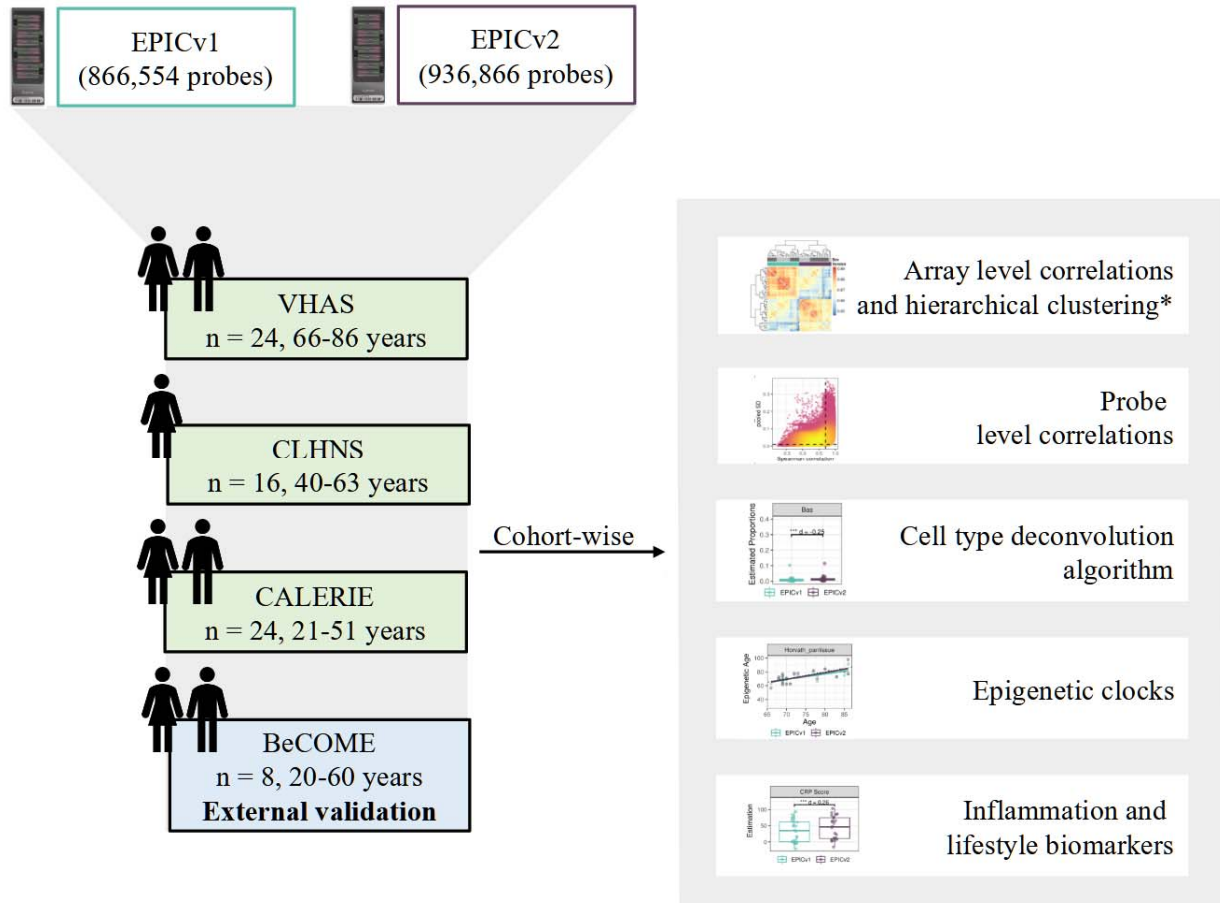

907


908 **Figure 1.** Overview of study design and analyses.

909 *Array level correlations and hierarchical clustering were also performed by combining cohorts.


910

911

912

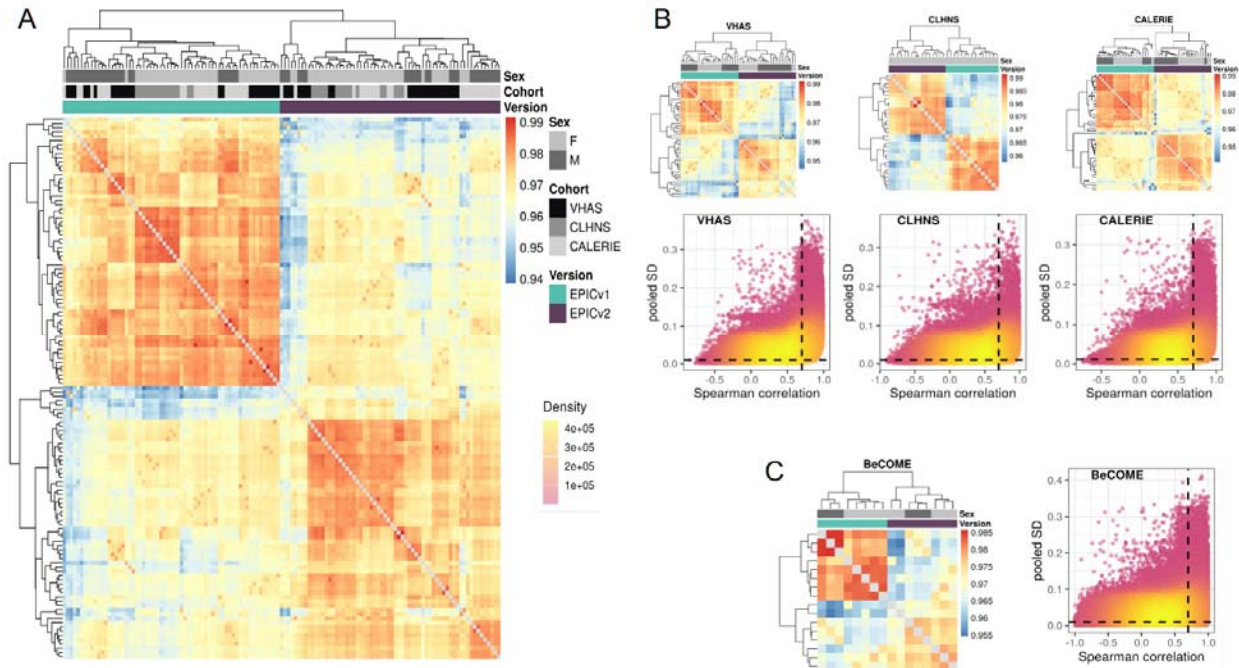

913
914 **Figure 2.** (A) Unsupervised hierarchical clustering of array level Spearman correlations between
915 matched VHAS, CLHNS, and CALERIE samples on EPICv1 and EPICv2 across 721,378 shared
916 probes; blue to red color range denotes Spearman correlation from 0.94-1.00. (B) Top: Cohort-
917 wise hierarchical clustering of sample-to-sample Spearman correlations across 721,378 probes
918 common between EPICv1 and EPICv2; Bottom: Cohort-wise Spearman correlation and pooled
919 standard deviation (SD) of common probes. The X-axis represents the Spearman correlation and
920 Y-axis represents the pooled SD of probes common to both arrays. Dashed horizontal line
921 indicates the pooled SD threshold set at lower quartile pooled SD for each cohort, and the
922 vertical dashed line indicates the correlation threshold set at 0.70. The colors indicate the density
923 of points, such that pink is low density and yellow is high density. Probes unique to either array
924 are not shown. (C) Hierarchical clustering of Spearman correlations between matched BeCOME
925 (external validation cohort) samples on EPICv1 and EPICv2 across 721,378 shared probes and
926 Spearman correlation and pooled SD of common probes.

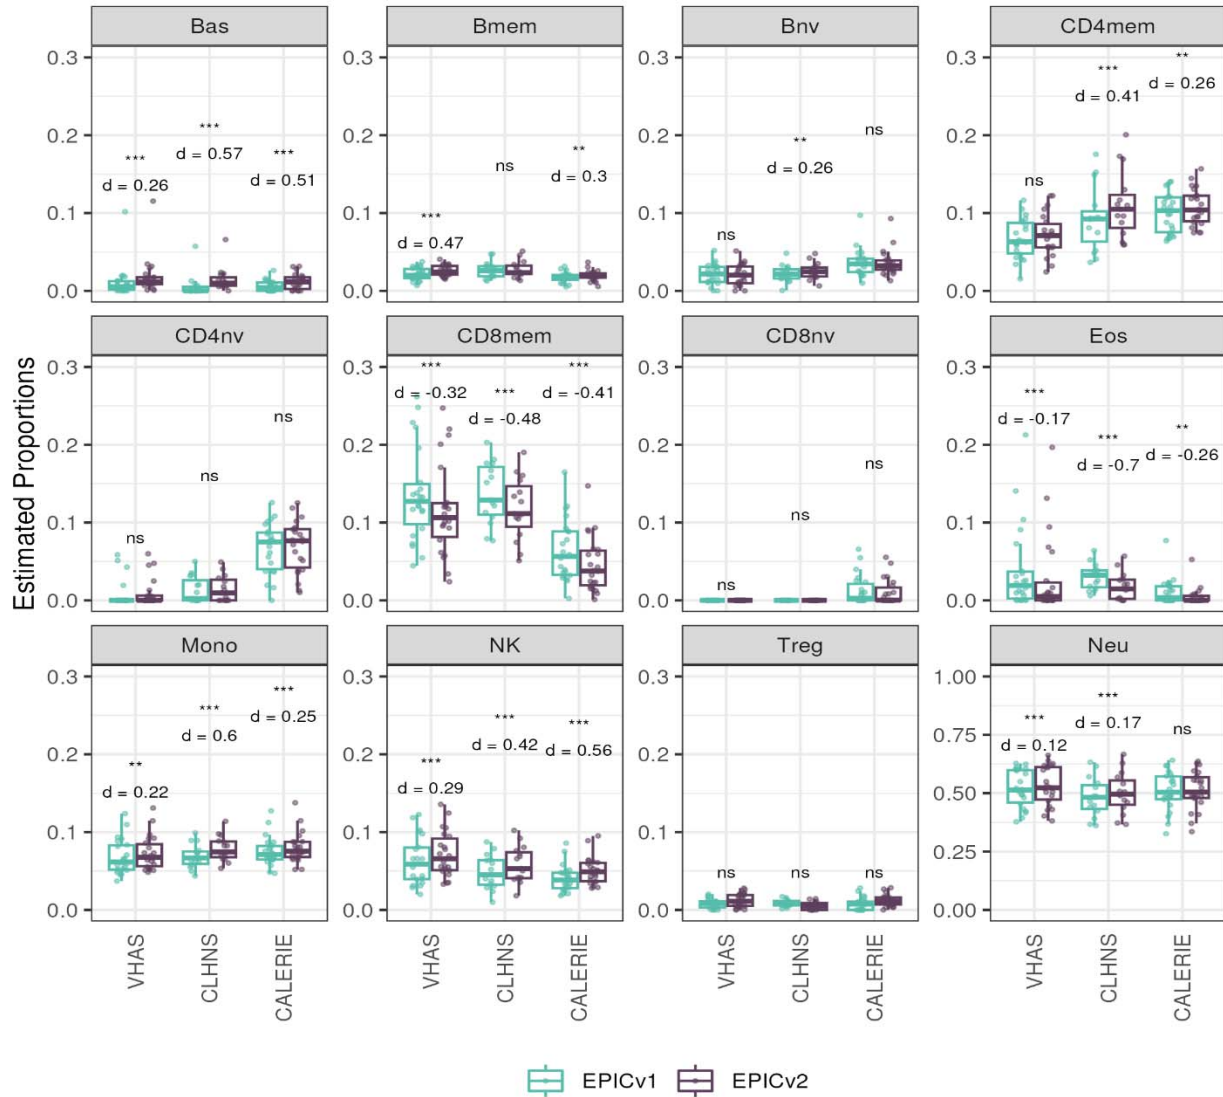


927

928 **Figure 3.** Differences in DNA methylation-based immune cell type proportions estimated using
 929 the IDOL reference on matched samples assessed on EPICv1 and EPICv2 in VHAS, CLHNS,
 930 and CALERIE. Statistical significance was defined as Bonferroni adjusted p -value < 0.05 . **
 931 denotes Bonferroni $p < 0.05$, *** denotes Bonferroni $p < 0.001$, “ns” denotes “not significant”,
 932 and “d” denotes effect size measured using Cohen’s d. A positive Cohen’s d indicates higher
 933 estimates in EPICv2 compared to EPICv1.

934

935

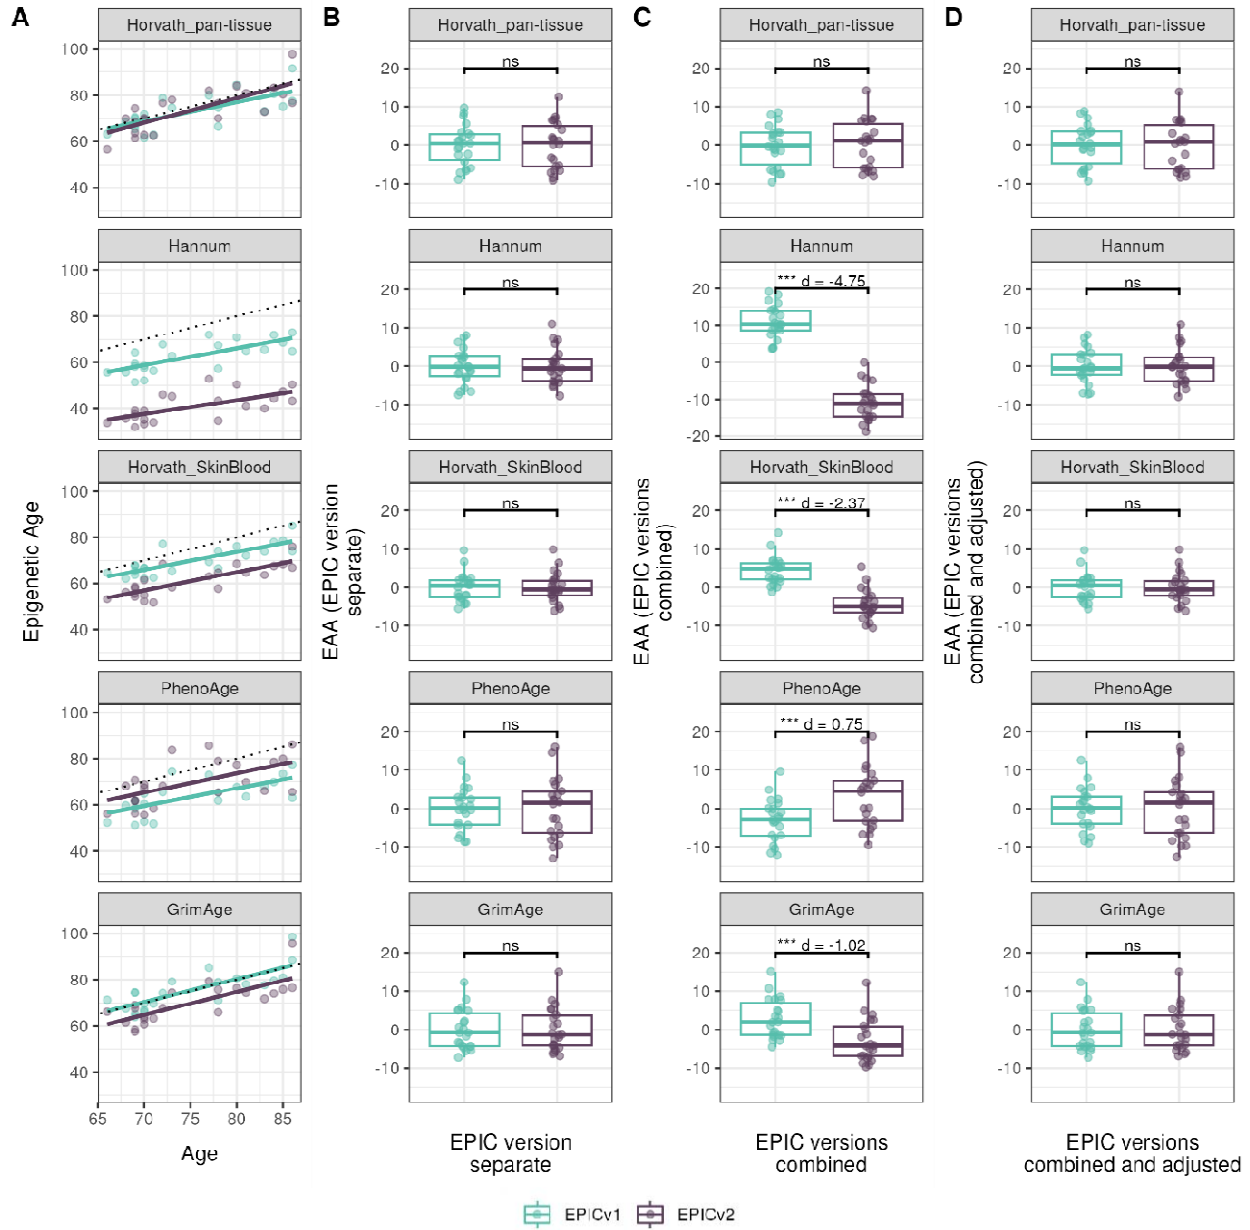


936

937 **Figure 4.** Epigenetic ages on matched samples assessed on EPICv1 and EPICv2 in VHAS. (A)
 938 Scatter plot of Horvath pan-tissue, Hannum, Horvath skin and blood, PhenoAge, and GrimAge
 939 clock ages (Y axis) and chronological age (X axis) with dotted line indicating $x=y$, coloured by
 940 EPIC version. (B-D) Boxplots comparing EPICv1 and EPICv2 EAAs calculated by considering
 941 (B) EPIC versions separately, (C) combined, and (D) combined and EPIC version adjusted.
 942 Statistical significance was defined as Bonferroni adjusted p -value <0.05 . ** denotes Bonferroni
 943 $p <0.05$, *** denotes Bonferroni $p <0.001$, “ns” denotes “not significant”, and “d” denotes effect
 944 size measured using Cohen’s d. A positive Cohen’s d indicates higher estimates in EPICv2
 945 compared to EPICv1.

946

947

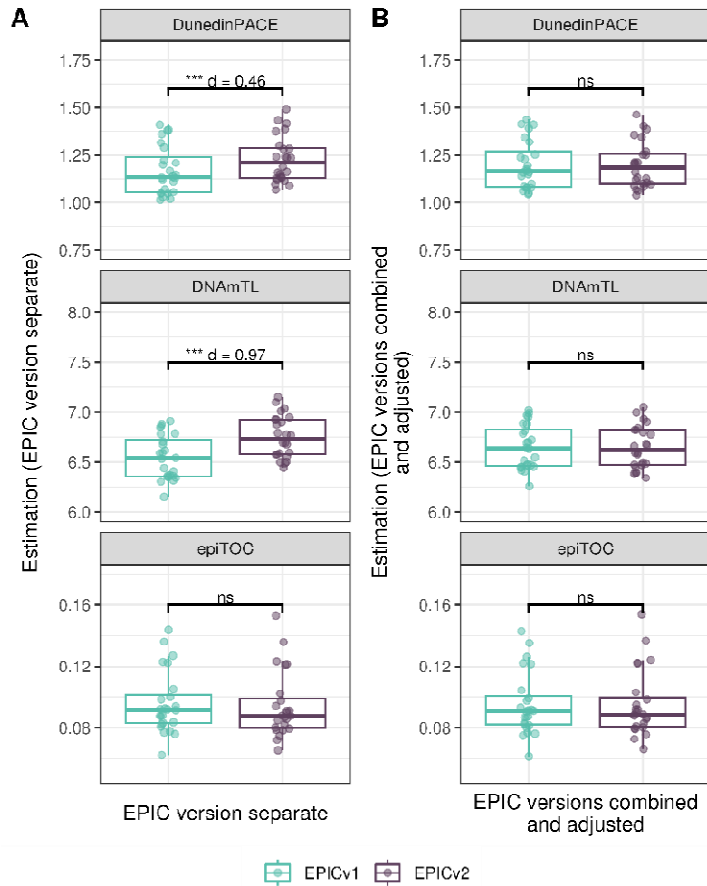

948

949 **Figure 5.** Rate-based and other clock estimates on matched samples assessed on EPICv1 and
950 EPICv2 in VHAS. Boxplots comparing DunedinPACE, DNAmTL and epiTOC estimates
951 calculated by considering EPIC versions separately (**A**) and combined and EPIC version adjusted
952 (**B**), between EPICv1 and EPICv2. Statistical significance was defined as Bonferroni adjusted p -
953 value <0.05 . ** denotes Bonferroni $p <0.05$, *** denotes Bonferroni $p <0.001$, “ns” denotes “not
954 significant”, and “d” denotes effect size measured using Cohen’s d . A positive Cohen’s d
955 indicates estimates in EPICv2 compared to EPICv1.

956

957

958

959

960

961

962

963

964 **Table 1.** Demographics of the three in-house cohorts and external validation cohort.

965

	VHAS	CLHNS	CALERIE	External validation cohort: BeCOME
Samples (n)	48 (24 matched venous and capillary samples)	16	24	8
Country of origin	Vietnam	Philippines	United States of America	Germany
Biological sex (% Female)	36.4%	100%	54.2%	62.5%
Average age in years \pm standard deviation	74.6 \pm 6.7	48.4 \pm 6.1	36.7 \pm 8.1	40.0 \pm 16.9

966
967
968
969
970
971
972
973
974
975
976
977
978
979
980
981
982
983
984

985 **Table 2.** Summary of predictive CpGs of DNA methylation-based clocks, biomarker predictors,
 986 and cell type deconvolution in EPICv1, EPICv2, Infinium Methylation Screening Array (MSA),
 987 and 450K.

Tools	CpGs	EPICv1 absent CpGs	EPICv2 absent CpGs	EPICv2 replicate probes	MSA absent CpGs	450K absent CpGs	Training arrays (sample size, age in years)
Horvath pan-tissue*	353	19 (5.38%)	13 (3.68%)	4 (1.13%)	6 (1.7%)	0	27K, 450K (n=7844, 0-100)
Hannum*	71	6 (8.45%)	7 (9.86%)	5 (7.04%)	3 (4.23%)	0	450K (n=656, 9-101)
Horvath Skin and Blood	391	0	17 (4.35%)	9 (2.3%)	3 (0.77%)	0	450K, EPICv1 (n=896, 0-94)
PhenoAge	513	0	18 (3.51%)	7 (1.36%)	3 (0.58%)	0	27K, 450K, EPICv1 (n=9926, 18-100)
GrimAge**	1030	NA	NA	NA	NA	NA	450K, EPICv1 (n=1731, mean 66)
PC Clocks***	78464	0	5801 (7.39%)	650 (0.83%)	51108 (65.14%)	0	450K, EPICv1 (n=NA, 0-101)
DunedinPACE	173	0	29 (16.76%)	2 (1.16%)	2 (1.16%)	0	EPICv1 (n=1037, 38 and 45)
DNAmTL	140	0	31 (22.14%)	3 (2.14%)	2 (1.43%)	0	450K, EPICv1 (n=2256, 22-93)
epiTOC*	385	31 (8.05%)	26 (6.75%)	0	13 (3.38%)	0	450K (n=656, 19-101)
IL-6 score	35	0	3 (8.57%)	1 (2.86%)	12 (34.29%)	0	450K, EPICv1 (n=875, 67-78)
CRP score*	1765	104 (5.89%)	96 (5.44%)	41 (2.32%)	357 (20.23%)	0	27K, 450K, EPICv1 (n=22774, 16-75)
Smoking score	233	0	23 (9.87%)	2 (0.86%)	27 (11.59%)	0	EPICv1 (n=5087, 18-99)
Alcohol score	450	0	49 (10.89%)	6 (1.33%)	47 (10.44%)	0	EPICv1 (n=5087, 18-99)
IDOL	1200	0	8 (0.67%)	48 (4%)	20 (1.67%)	741 (61.75%)	EPICv1 (n=56, 19-58)

988 * There are CpGs commonly absent in both EPICv1 and EPICv2 in these clocks: Horvath pan-
 989 tissue: 3 CpGs; Hannum: 2 CpGs; epiTOC: 6 CpGs; CRP score: 20 CpGs. There are probes
 990 absent in EPICv1 and are reintroduced in EPICv2 in these clocks: Horvath pan-tissue: 14 CpGs;
 991 Hannum: 4 CpGs; epiTOC: 25 CpGs; CRP score: 83 CpGs.

992 ** Clock CpGs for GrimAge are not publicly available.

993 *** PC Clocks CpGs include the total CpGs required to calculate PC versions of Horvath pan-
 994 tissue, Hannum, Horvath SkinBlood, PhenoAge, and GrimAge.