



Accuracy of lung ultrasound performed with handheld ultrasound device in internal medicine: an observational study

Anna Lo Cricchio¹ · Andrea Storelli¹ · Iacopo Bertoletti¹ · Gabriele Ciuti¹ · Alessia Fabbri¹ · Elisa Martinelli¹ · Maria Cristina De Santis¹ · Paolo Mercatelli¹ · Khadija El Aoufy² · Silvia Bellando Randone³ · Alberto Moggi Pignone¹ · Esterita Accogli⁴ · Giulia Bandini¹

Received: 14 June 2024 / Accepted: 27 June 2024 / Published online: 3 August 2024
© The Author(s) 2024

Abstract

Aims Lung ultrasound (LUS) is increasingly used in Internal Medicine to complement medical examination, documenting pleural and lung conditions. This study aimed to compare the accuracy of handheld ultrasound device (HHUSD) with high-end ultrasound device (HEUSD) in patients with heart failure or pneumonia, also including the assessment of costs and time-savings.

Methods In this observational study 72 patients (aged ≥ 18) admitted to Internal Medicine Unit for heart failure or pneumonia underwent LUS plus evaluation of inferior cava vein (ICV) when indicated, using both HHUSD and HEUSD. Each evaluation, independently performed by 2 different experienced operators, included B-lines number, pleural effusion, lung consolidations, ICV ectasia and its respiratory excursions.

Results Concordance between HHUSD and HEUSD findings was $79.3\% \pm 17.7$ (mean \pm SD) for B-lines, 88.6% for pleural effusion, 82.3% for consolidations and 88.7% and 84.9% for ICV ectasia and its respiratory excursions respectively. BMI didn't significantly influence concordance between the two methods. Moreover, examination time (as mean \pm SD) was shorter with HHUSD (8 ± 1.5 min) compared to HEUSD (10 ± 2.5 min).

Conclusions HHUSD demonstrated high accuracy in detecting B-lines, pleural effusions, lung consolidations and ICV evaluation when compared to HEUSD. Thus, HHUSD, not only is characterized by accessibility, portability, and easy handling due to its small size, but it also offers advantages in terms of saving costs and time, ultimately contributing to faster patient assessment compared to HEUSD.

Keywords Lung ultrasound · Point of care ultrasound · Handheld ultrasound device · Pocket-sized ultrasound · Heart failure · pneumonia

Introduction

In recent years, lung ultrasound (LUS) has emerged as a reliable and rapid tool for the evaluation of patients with pulmonary diseases [1]. LUS, plus the inferior cava vein (ICV) assessment, can improve the diagnosis of many cardiopulmonary conditions such as pleural effusion, interstitial lung disease and pneumonia; moreover, LUS can guide procedures (i.e. thoracentesis), drive therapeutic timing and dosage (i.e. diuretic therapy) and it is a valid instrument for monitoring and prognosis of patients with heart failure [2–5].

In the last few years, the development and spread of knowledge in the field of LUS and the expansion of inexpensive and handy tablet or smartphone/tablet format devices,

✉ Anna Lo Cricchio
anna.locricchio@unifi.it; anna.locricchio9@gmail.com

¹ Department of Experimental and Clinical Medicine, University of Florence, Careggi Hospital, Florence, Italy

² Department of Health Science, University of Florence, Florence, Italy

³ Department of Experimental and Clinical Medicine, Division of Rheumatology, University of Florence, Florence, Italy

⁴ Department of Internal Medicine, Centre of Research and Learning in Ultrasound, Maggiore Hospital, Bologna, Italy

have made the point-of-care ultrasound (POCUS) approach become a cornerstone in the evaluation of patients with respiratory symptoms. Nowadays, LUS is a fundamental supplement to the medical examination. Indeed, pocket-sized devices are frequently used in the bedside evaluation of hospitalized patients, however, their use is rapidly increasing even in ambulatory settings to answer simple clinical questions especially thanks to their low cost and good performance profiles [6–8].

These days, ultrasound is considered an essential aspect of bedside examination since it can help to rapidly frame the patient [9] and accelerate the diagnostic therapeutic pathway.

However, despite the widespread of pocket-sized devices thanks to new technologies, with a major boost for their development during the SARS-CoV2 pandemic, to date there are no solid data to support the interchangeable use between high-end ultrasound devices (HEUSDs) and hand-held ultrasound devices (HHUSDs), except for few papers comparing the two methods [10–12].

Despite technological advancements enabling the development of increasingly efficient pocket-sized ultrasound machines, the literature still reports lower performance of these devices in terms of image quality compared to HEUSDs. This discrepancy is attributed to various factors, including lower spatial resolution, reduced contrast and higher levels of noise. Specifically, the literature highlights a reduced penetration depth of the ultrasound beams produced by these devices [13, 14].

Thus, the aim of our work was to evaluate the accuracy of LUS performed with HHUSD compared to HEUSD in patients admitted to our ward for heart failure or pneumonia and to determine if the pocket-sized ultrasound approach has advantages in terms of saving costs and time. Then, we considered whether obesity may be a limiting condition for HHUSDs due to increased fat layer and reduced penetration depth of the sound beams of these machines.

Materials and methods

We conducted in a single center an observational study involving adults hospitalized in the Department of Internal Medicine 4 of the Careggi University Hospital in Florence.

Over 6 months, 72 patients were enrolled. For each patient demographic, clinical and laboratory data were recorded.

The enrolled patients underwent LUS plus the evaluation of ICV, when indicated, both performed with the HHUSD Vscan Extend Dual probe (GE Healthcare) with a phased array transducer (1.7–3.8 MHz) and a linear (3.3–8 MHz) transducer. and the HEUSD Vivid T8 (GE Healthcare) with a convex transducer (3.5–7 MHz). Ultrasound evaluations were performed independently by two different operators

experienced in LUS, at closely spaced times (a maximum of 15 min apart) using a standardized imaging protocol [15].

Every patient was scanned in the supine and sitting position and, for each of the 58 areas examined, the following data were registered: number of B-lines, quantified as suggested by the literature [16, 17], the total number of B-lines resulting from the evaluation of each of the spaces explored for the antero-lateral chest and for the posterior chest, the presence of pleural effusion and/or lung consolidation. Moreover, in patients with heart failure, inferior cava vein ectasia (diameter > 20 mm) and its respiratory excursions, defined as maintained if greater than 50% of the diameter, were recorded.

Finally, the duration of each examination was registered.

The data obtained by the two types of ultrasounds were then compared, and it was assessed whether there was overlap between the findings identified by the two different methods. The number of B-lines for each field explored was judged to be overlapping if there was a numerical difference ≤ 2 .

Statistical analysis

Continuous normal variables have been expressed as mean and standard deviation (SD), and non-normal variables as median (minimum value–maximum value). Categorical variables have been expressed as number and percentage. Comparison between groups have been performed with the chi-square test for dichotomous variables. Wilcoxon test have been performed for paired continuous variables for comparison of HEUSD and HHUSD. A *p*-value < 0.05 have been considered statistically significant. All statistical analyses have been performed using SPSS software version 20.0 (IBM, Armonk, New York, USA).

Results

Seventy-two patients with a median age of 80 years (range 28–99), among which 39 males (54%), were enrolled in the study. Admission diagnosis to our ward were heart failure (68%) or pneumonia (32%). The principal comorbidities were hypertension (72%), atrial fibrillation (40%), type II diabetes (24%), dyslipidemia (38%), chronic obstructive pulmonary disease (24%), chronic kidney failure (22%) and coronary heart disease (20%) (Fig. 1).

94% of patients had at least one of the following cardiovascular risk factors: obesity, smoking, hypertension, diabetes, dyslipidemia.

The most frequently prescribed medications upon admission to the ward were: diuretics (60%), beta-blockers (54%), calcium-antagonists (28%), direct anticoagulants (28%),

Fig. 1 Main comorbidities of enrolled patients

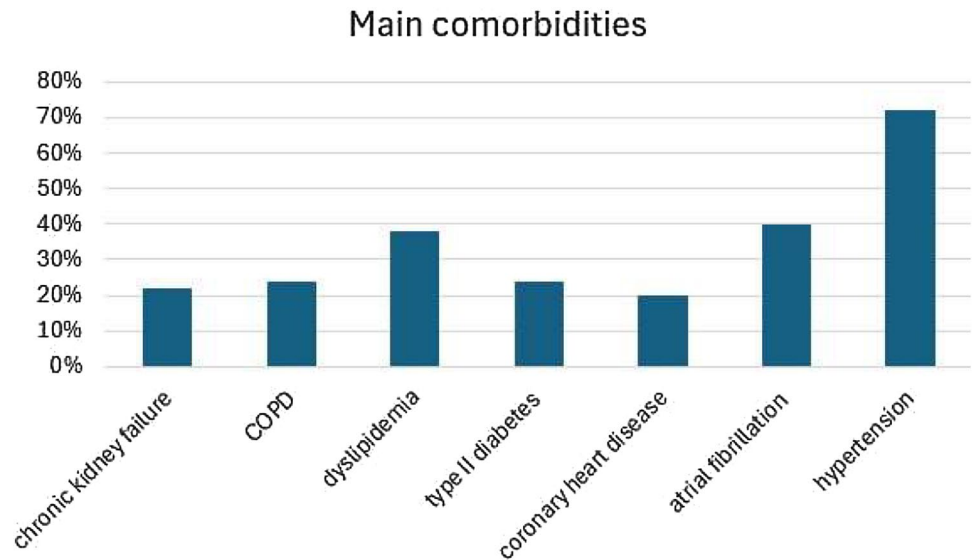


Table 1 Laboratory tests of enrolled patients available at the admission (↑ increased values, ↓ decreased values)

	Patients analyzed <i>n</i> (%)	Patients with abnormal values <i>n</i> (%)
NT-proBNP (n.v. 1–125 pg/mL)	57 (79.2%)	↑ 52 (97.1%)
Creatinine (n.v. 0.70–1.20 mg/dL)	72 (100%)	↑ 25 (34.7%)
Troponin T (n.v. < 14 pg/mL)	50 (69.4%)	↑ 43 (86%)
CRP (n.v. < 5 mg/L)	67 (93.1%)	↑ 62 (92.5%)
PCT (n.v. < 0.5 ng/mL)	65 (90.3%)	↑ 6 (9.2%)
Hb (n.v. 14.0–18.0 g/dL)	72 (100%)	↓ 59 (82%)
WBC (n.v. 4.00–10.00 × 10 ⁹ /L)	72 (100%)	↑ 20 (28%)
Hypokaliemia (K ⁺ < 3.5 mEq/L)	72 (100%)	9 (12.5%)
Hyperkaliemia (K ⁺ > 5.1 mEq/L)	72 (100%)	2 (2.8%)
Hyponatremia (Na ⁺ < 135 mEq/L)	72 (100%)	12 (16.7%)
Hypernatremia (Na ⁺ > 145 mEq/L)	72 (100%)	6 (8.3%)
AST (n.v. 10–50 U/L)	44 (61.1%)	↑ 10 (22.7%)
ALT (n.v. 10–50 U/L)	70 (97.2%)	↑ 9 (12.9%)

NT-proBNP N-terminal prohormone of brain natriuretic peptide, *CRP* C-reactive protein, *PCT* procalcitonin, *Hb* hemoglobin, *WBC* white blood cells, *K⁺* potassium, *Na⁺* sodium, *AST* aspartate transaminase, *ALT* alanine transaminase, *n.v.* normal value

angiotensin converting enzyme (ACE) inhibitors (20%), sartans (16%), and warfarin (4%).

In 70% of the cases, physical examination revealed the presence of wet sounds upon chest auscultation, while in the remaining 30% bronchial obstruction sounds; moreover, 55% of patients had swollen limbs or feet.

The main laboratory alterations upon admission to the ward were an increase in NT-proBNP, troponin, and C-reactive protein (Table 1).

The comparison between the HHUS and the HEUS evaluation showed a concordance rate of 79.3% ± 17.7 (mean ± SD) for the detection of B-lines, 88.6% for pleural effusion and 82.3% for lung consolidations.

Concordance rate between the two methods in the evaluation of ICV ectasia and its respiratory excursions were 88.7% and 84.9%, respectively.

BMI was available for 69 out of the 72 patients, in which 20% had BMI > 30 kg/m². In this subgroup of patients, the concordance rate between the 2 methods was 78.9% ± 12.6 for the detection of B-lines, 86.5% for pleural effusion, 79.5% for consolidations, 86.3% and 85.8% for the evaluation of ICV ectasia and its respiratory excursions respectively. Between the two groups (patients with BMI > 30 kg/m² and patients with BMI < 30 kg/m²), there were no statistically significant differences (*p* = 0,643) in LUS and ICV evaluation.

Data about concordance rates between the HHUSD and the HEUSD evaluation are reported in Table 2.

The average time taken to perform the evaluations (expressed as mean ± SD) was 8 ± 1.5 min with the HHUSD and 10 ± 2.5 min with the HEUSD, with a statistically significant difference (*p* < 0.0001).

Discussion

Bedside ultrasound has become a fundamental diagnostic tool in Internal Medicine care setting, and it has profoundly changed the clinical practice and the approach to patients' evaluation and management. In particular, LUS is an essential part of POCUS which is increasingly considered as an extension of the physical examination, leading to the modern concept of ultrasound-assisted patients examination [9].

Table 2 Concordance rate between handheld ultrasound device (HHUSD) and high-end ultrasound device (HEUSD) in B-lines detection was expressed in mean \pm standard deviation. Concordance rates between the two devices for the detection of pleural effusion and lung consolidations and for inferior cava vein (ICV) assessment were expressed as number and their percentages

Ultrasound findings detected	Concordance between HHUSD and HEUSD	
	Total enrolled population	Patients with BMI > 30 kg/m ²
B-lines	79.3% \pm 17.7	78.9% \pm 12.6
Pleural effusion	88.6%	86.5%
Lung consolidations	82.3%	79.5%
Presence/absence of ICV ectasia	88.7%	86.3%
Respiratory excursions of the ICV (> or < 50% of the diameter)	84.9%	85.8%

POCUS is, indeed, able to accelerate the diagnostic and therapeutic process and to guide the management of inpatients in Internal Medicine settings.

In recent years, pocket-sized ultrasound devices are increasingly used in many different clinical settings given their low cost and technological evolution. HHUSDs present several advantages such as their low costs and rapid use, their feasibility and the possibility of always having them at hand due to their small size, that have contributed to their widespread use in numerous hospital and non-hospital settings [10, 18]. Moreover, the use of a pocket-sized, lightweight, and handy device in everyday clinical practice can provide the operator with greater ergonomics due to the smaller spatial footprint, and this may contribute to making healthcare professionals' movements more comfortable [19, 20].

The use of a pocket-sized device, in daily clinical-assistance activities, can then help reducing physical stress for sonographers by reducing repetitive strain injuries that, to date, are becoming a perceived, and sometimes, disabling issue for physicians performing numerous ultrasound evaluations due to having non-ergonomic positions in environments where space is often limited.

However, the performance of HHUSDs in everyday clinical practice and their role in the evaluation of patients with heart failure and pneumonia hasn't still been clearly defined.

Our data show that the accuracy of LUS performed with HHUSD is high when compared with HEUSD in the evaluation of patients with heart failure/lung disease. In particular, pocket-sized device confirms its accuracy in the evaluation of B-lines and pleural effusion [21] (Fig. 2). Moreover, in

our study even the evaluation of ICV ectasia and its respiratory excursions is accurate with HHUSD compared to HEUSD. ICV evaluation, together with LUS, is fundamental in the management of patients with heart failure for diagnosis, monitoring and even during the follow up and to adjust diuretic therapy. To the best of our knowledge, this is the first study in which both LUS and ICV findings with pocket-sized ultrasound device are evaluated in comparison with a HEUSD. The substantial overlap, in the reported data, highlights the validity of the assessments performed with the pocket-sized ultrasound devices, thus confirming the reliability of this technique in the management of patients with heart failure. Moreover, there was a substantial correspondence even in the evaluation of lung consolidations; indeed, despite the limits of LUS for the assessment of consolidations [22], HHUSD can be a valid option for the management of patients with pneumonia.

In addition, the average time to perform the examination with the pocket-sized device is less than the time taken with the high-end machine, which can contribute to faster and more efficient ultrasound assessment at the patient's bedside.

Finally, our study shows that the accuracy of pocket-sized ultrasound devices is still relevant in the evaluation of patients with higher BMIs, making these portable instruments reliable also in this subgroup of patients.

Our findings support the interchangeable use of HHUSD and HEUSD in the management of inpatients with heart failure and pneumonia.

Our study has some limitations; indeed, all the ultrasound examinations were performed by expert lung ultrasound operators, and this may have contributed to increasing the accuracy of ultrasound examinations performed with the HHUSD. Then, our study has been conducted in a single center and the sample size is small, thus further studies will be needed to confirm the interchangeability of the two methods in larger populations.

Conclusions

In conclusion, this study shows that LUS, performed with a pocket-sized ultrasound device has high accuracy with regard to the detection of B-lines, pleural effusion and lung consolidations. Moreover, it allows adequate assessments of inferior cava vein. The accuracy remains high also in obese patients. Handheld ultrasound devices can be confidently used for the management of inpatients with heart failure and/or pneumonia. Given the usefulness of these tools, specific operators' training should be developed and encouraged to spread the HHUS devices use in clinical practice.

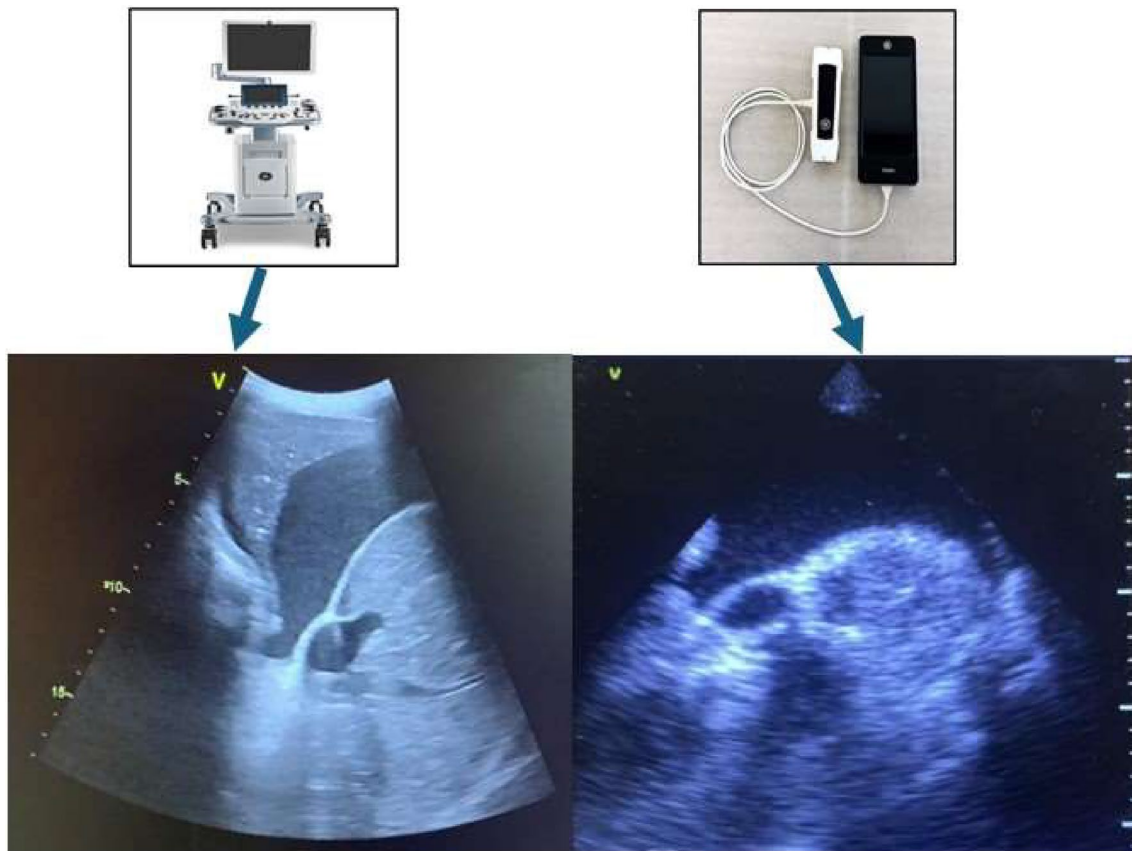


Fig. 2 On the left, a pleural effusion detected using the high-end ultrasound machine; on the right, a pleural effusion highlighted with the hand-held ultrasound device

Author contributions Study conception and design and material preparation were performed by ALC and GB. Data collection was performed by ALC, GB, AS, IB, AF, MCDS, PM and EM. Data analysis was performed by GC and KEA. The first draft of the manuscript was written by ALC and revised by AMP, EA and SBR; all authors commented on previous versions of the manuscript. All authors read and approved the final manuscript.

Funding Open access funding provided by Università degli Studi di Firenze within the CRUI-CARE Agreement. The authors declare that no funds, grants, or other support were received during the preparation of this manuscript.

Data availability All datasets generated or analysed during the current study are available from the corresponding author on reasonable request.

Declarations

Conflict of interest All authors declare no conflict of interest to disclose.

Ethics approval The study complies with the Declaration of Helsinki and was performed according to local ethics committee approval (Comitato Etico Regione Toscana – area vasta centro); approval code: Cod.26179_DM.

Consent to participate Informed consent was obtained from all individual participants included in the study.

Consent to publish The authors affirm that human research participants provided informed consent for publication of the images in Fig. 2.

Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

References

- Laursen CB, Clive A, Hallifax R, Pietersen PI, Asciak R, David-
sen JR et al (2021) European respiratory society statement on
thoracic ultrasound. *Eur Respir J* 57:2001519. <https://doi.org/10.1183/13993003.01519-2020>
- Soni NJ, Franco R, Velez MI, Schnobrich D, Dancel R, Restrepo
MI et al (2015) Ultrasound in the diagnosis & management of
pleural effusions. *J Hosp Med* 10:811–816. <https://doi.org/10.1002/jhm.2434>
- Gargani L (2019) Ultrasound of the lungs: more than a room with
a view. *Heart Fail Clin* 15:297–303. <https://doi.org/10.1016/j.hfc.2018.12.010>
- Pugliese NR, Mazzola M, Bandini G, Barbieri G, Spinelli S, De
Biase N et al (2023) Prognostic role of sonographic decongestion
in patients with acute heart failure with reduced and preserved
ejection fraction: a multicentre study. *J Clin Med* 12:773. <https://doi.org/10.3390/jcm12030773>
- Kajimoto K, Madeen K, Nakayama T, Tsudo H, Kuroda T, Abe T
(2012) Rapid evaluation by lung-cardiac-inferior vena cava (LCI)
integrated ultrasound for differentiating heart failure from pul-
monary disease as the cause of acute dyspnea in the emergency
setting. *Cardiovasc Ultrasound* 10:49. <https://doi.org/10.1186/1476-7120-10-49>
- Galderisi M, Santoro A, Versiero M, Lomoriello VS, Esposito R,
Raia R et al (2010) Improved cardiovascular diagnostic accuracy
by pocket size imaging device in non-cardiologic outpatients:
the NaUSiCa (Naples Ultrasound Stethoscope in Cardiology)
study. *Cardiovasc Ultrasound* 8:51. <https://doi.org/10.1186/1476-7120-8-51>
- Schleder S, Dendl L-M, Ernstberger A, Nerlich M, Hoffstetter P,
Jung E-M et al (2013) Diagnostic value of a hand-carried ultra-
sound device for free intra-abdominal fluid and organ lacerations
in major trauma patients. *Emerg Med J* 30:e20–e20. <https://doi.org/10.1136/emermed-2012-201258>
- Razi R, Estrada JR, Doll J, Spencer KT (2011) Bedside hand-car-
ried ultrasound by internal medicine residents versus traditional
clinical assessment for the identification of systolic dysfunction in
patients admitted with Decompensated Heart failure. *J Am Soc
Echocardiogr* 24:1319–1324. <https://doi.org/10.1016/j.echo.2011.07.013>
- Narula J, Chandrashekar Y, Braunwald E (2018) Time to add
a fifth pillar to bedside physical examination: inspection, palpa-
tion, percussion, auscultation, and insonation. *JAMA Cardiol*
3:346–350. <https://doi.org/10.1001/jamacardio.2018.0001>
- Rykkje A, Carlsen JF, Nielsen MB (2019) Hand-held ultrasound
devices compared with high-end ultrasound systems: a systematic
review. *Diagnostics (Basel)* 9:61. [https://doi.org/10.3390/diagnos-
tics9020061](https://doi.org/10.3390/diagnos-
tics9020061)
- Haji-Hassan M, Lenghel LM, Bolboacă SD (2021) Hand-held
ultrasound of the lung: a systematic review. *Diagnostics (Basel)*
11:1381. <https://doi.org/10.3390/diagnostics11081381>
- Nielsen MB, Cantisani V, Sidhu PS, Badea R, Batko T, Carlsen J
et al (2019) The use of handheld ultrasound devices - an EFSUMB
position paper. *Ultraschall Med* 40:30–39. <https://doi.org/10.1055/a-0783-2303>
- Wang R, Fang Z, Gu J, Guo Y, Zhou S, Wang Y et al (2019) High-
resolution image reconstruction for portable ultrasound imaging
devices. *EURASIP J Adv Signal Process* 2019:56. <https://doi.org/10.1186/s13634-019-0649-x>
- Fröhlich E, Beller K, Muller R, Herrmann M, Debove I, Klinger C
et al (2020) Point of care ultrasound in geriatric patients: prospec-
tive evaluation of a portable handheld ultrasound device. *Ultra-
schall Med* 41:308–316. <https://doi.org/10.1055/a-0889-8070>
- Gargani L, Romei C, Bruni C, Lepri G, El-Aoufy K, Orlandi M,
et al (2022) Lung ultrasound B-lines in systemic sclerosis: cut-off
values and methodological indications for interstitial lung disease
screening. *Rheumatology* 61:SI56–64. <https://doi.org/10.1093/rheumatology/keab801>
- Pellicori P, Platz E, Dauw J, ter Maaten JM, Martens P, Pivetta
E et al (2021) Ultrasound imaging of congestion in heart fail-
ure: examinations beyond the heart. *Eur J Heart Fail* 23:703–712. <https://doi.org/10.1002/ejhf.2032>
- Volpicelli G, Elbarbary M, Blaivas M, Lichtenstein DA, Mathis G,
Kirkpatrick AW et al (2012) International evidence-based recom-
mendations for point-of-care lung ultrasound. *Intensive Care Med*
38:577–591. <https://doi.org/10.1007/s00134-012-2513-4>
- Ault MJ, Rosen BT (2010) Portable ultrasound: the next genera-
tion arrives. *Crit Ultrasound J* 2:39–42. <https://doi.org/10.1007/s13089-010-0031-6>
- Coffin CT (2014) Work-related musculoskeletal disorders in
sonographers: a review of causes and types of injury and best
practices for reducing injury risk. *Rep Med Imag* 7:15–26. <https://doi.org/10.2147/RMI.S34724>
- Wilkinson JN, Saxhaug LM (2021) Handheld ultrasound in train-
ing - The future is getting smaller! *J Intensive Care Soc* 22:220–
229. <https://doi.org/10.1177/1751143720914216>
- Schleder S, Dornia C, Poschenrieder F, Dendl L, Cojocaru L,
Bein T, Schmid C, Stroszczyński C, Jung EM, Heiss P (2012)
Bedside diagnosis of pleural effusion with a latest generation
hand-carried ultrasound device in intensive care patients. *Acta
Radiol* 53(5):556–560. <https://doi.org/10.1258/ar.2012.110676>
- Reissig A, Görg C, Mathis G (2009) Transthoracic sonography
in the diagnosis of pulmonary diseases: a systematic approach.
Ultraschall Med 30:438–54; quiz 455–6. <https://doi.org/10.1055/s-0028-1109703>

Publisher's Note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.