



HHS Public Access

Author manuscript

J Neural Eng. Author manuscript; available in PMC 2007 August 13.

Published in final edited form as:

J Neural Eng. 2004 September ; 1(3): 135–141. doi:10.1088/1741-2560/1/3/002.

Motor Imagery Classification by Means of Source Analysis for Brain Computer Interface Applications

Lei Qin,

Lei Ding,

Bin He*

The University of Minnesota

Abstract

We report a pilot study of performing classification of motor imagery for Brain Computer Interface applications, by means of source analysis of scalp-recorded EEGs. Independent component analysis (ICA) was used as a spatio-temporal filter extracting signal components relevant to left or right motor imagery (MI) tasks. Source analysis methods including equivalent dipole analysis and cortical current density imaging were applied to reconstruct equivalent neural sources corresponding to MI, and classification was performed based on the inverse solutions. The classification was considered correct if the equivalent source was found over the motor cortex in the corresponding hemisphere. A classification rate of about 80% was achieved in the human subject studied using both the equivalent dipole analysis and the cortical current density imaging analysis. The present promising results suggest that the source analysis approach could manifest a clearer picture on the cortical activity, and thus facilitate the classification of MI tasks from scalp EEGs.

Keywords

Brain Computer Interface; Motor Imagery; Source Analysis; Inverse Solution; EEG; Independent Component Analysis; Event-related Desynchronization

I. INTRODUCTION

People suffering from severe motor disabilities but being cognitively intact need an alternative method to interact with environment. Over the past decades, the development of the technology of Brain Computer Interface (BCI) (see Wolpaw et al 2002 for review) provides a novel and promising communication channel for these patients. It reads out the intents of the patients and translates them into physical commands which control the output devices. Both noninvasive and invasive approaches have been used to acquire data for BCI. The noninvasive methods include the use of electroencephalography (EEG), magnetoencephalography (MEG), positron emission tomography (PET), functional magnetic resonance imaging (fMRI), and optical imaging. Among them, because EEG

*Correspondence: Bin He, Ph.D., University of Minnesota, Department of Biomedical Engineering, 7-105 BSBE, 312 Church Street, Minneapolis, MN 55455, e-mail: binhe@umn.edu.

has relatively short time constants, which can function in most environments, and EEG acquisition systems are relatively simple and inexpensive, EEG based BCI systems are currently widely used (Wolpaw et al 1991, 2002; Pfurtscheller et al 1994, 1997; Birbaumer 1999; Babiloni et al 2000, 2001; Wang & He, 2004; Vallabhaneni & He, 2004; Vallabhaneni et al, 2004). On the other hand, intracranial recording methods, such as electrocorticograms and single-neuron recordings, are invasive (Donoghue 2002; Nicoletis 2001, 2003; Rohde et al 2002) although these methods take advantage of better signal quality. For obvious reasons, it would be desirable if one can fully develop noninvasive methods to control BCI devices, thus avoiding brain implants in human subjects.

Present-day EEG-based BCIs use different signals to encode the subjects' intent, such as slow cortical potentials, P300 potentials, and mu or beta rhythms (Wolpaw et al 1991, 2002; Pfurtscheller et al 1994, 1997, 1999; McFarland et al 1997; Birbaumer 1999; Babiloni et al 2000, 2001; Wang & He, 2004; Vallabhaneni & He, 2004). In the present study, we focus on mu rhythms caused by motor imagination, i.e. left and right hand imagination. Mu rhythm, a part in alpha band, is traditionally defined as an 8–12Hz rhythm recorded over sensorimotor cortex that decreases, or desynchronizes with movement, while it has recently been demonstrated that it also occurs with motor imagery (Pfurtscheller 1999). During unilateral hand movement imagery, an event-related desynchronization (ERD) appears on the contralateral hemisphere. So the difference in the scalp EEG with the different hand imagination can be used to generate different control signals for BCI systems (Pfurtscheller et al 1997; Babiloni et al 2000, 2001; Wang & He 2004; Vallabhaneni & He, 2004).

The source analysis methods, which solve the inverse problem of EEG from noninvasively recorded scalp potentials, allow analysis of brain signals in the source space (He 1999; He and Lian, 2004). The reconstructed source distribution over certain physical regions, e.g. brain cortex, within the human brain can be regarded as an alternative representation of intracranial recordings, which compensates the distortion and smearing effect caused by low conductive skull (He et al., 2002; He, 2004). From this point of view, the EEG-based source analysis methods would convert the signal space of noninvasive EEG measurement from the smeared scalp potential into the source distribution within the human brain, which is believed to have improved quality. In the present study, we test the hypothesis that the source analysis methods will aid the classification of motor imagination by revealing the activity of the brain, thus facilitating BCI from the scalp EEG.

II. METHODS

1) Data Description

The EEG data consisting of the synchronized imaginary movement experiments were made available by Dr. Allen Osman of University of Pennsylvania (Osman & Robert 2001; Sajda et al 2003).

Scalp EEG data were recorded from 59 electrodes placed according to the International 10/20 System with sampling rate of 100 Hz. The subjects were asked to imagine either right or left hand movement (180 trials, 90 left and 90 right) according to a highly predictable time cue.

Each trial (6 second) began with a blank screen. Two important timing cues that should be mentioned here are that at 3.75 seconds of a trial epoch, a cue (*preparation cue*, lasting 250 ms) of one letter ("L" or "R") appeared on the screen indicating which hand movement should be imagined; and at 5.0 seconds another cue 'X' (*execution cue*, lasting 50 ms) appeared, indicating that it was time to make the requested response as is shown in Fig. 1. However, an important thing should be mentioned here that even though the execution cue is set as the start point of imagination, subjects would begin imagining right after the preparation cue.

2) Data Pre-processing

Data preprocessing consisted Laplacian spatial filtering, time-frequency analysis, bandpass temporal filtering, and independent component analysis. The raw EEG data were processed using each of these procedures, as described in detail below.

A) Laplacian Spatial Filtering—The surface Laplacian filter is a sort of spatial high pass filter, and it attempts to enhance neuronal activity which is close to the recording electrode (Hjorth 1975; Babiloni et al, 1996; He 1999; He et al 2001), thus accentuating localized activity and reducing diffused activity (McFarland et al 1997). It could be approximately calculated by using the five-point approximation method (Hjorth 1975).

$$M_j^{Lap} = M_j - \frac{1}{4} \sum_{k \in N_j} M_k \quad (1)$$

where M_j is the scalp potential EEG of the j -th channel, and N_j is an index set of the four neighboring channels.

B) Time-Frequency Analysis

The time range of one trial is 6s, while we cannot use the whole time range for source analysis since not all points during this period contain information of the difference between left and right hand movement imagination. Also, the correct frequency band should be chosen as event-related (de)synchronization (ERD/ERS) is highly frequency related. In the present study, the Time-Frequency (TF) representation was used to select the time window and frequency band for source analysis.

The TF representation provides a time-varying energy of the signal in each frequency band (Tallon-Baudry et al 1997). In the present study, the signal was convoluted by complex Morlet's wavelets $w(t, f_0)$:

$$w(t, f_0) = A \cdot \exp(-t^2/2\sigma_t^2) \exp(2i\pi f_0 t) \quad (2)$$

with $\sigma_f = 1/2\pi\sigma_t$, $A = (\sigma_t\sqrt{\pi})^{-1/2}$. The trade-off ratio (f_0/σ_f) was chosen as 7 to create a wavelet family. This constant was used to determine the compromise between time and frequency localization.

The time-varying energy $[E(t, f_0)]$ of the signal at a specific frequency band is the squared norm of the convolution of a complex wavelet with the signal:

$$E(t, f_0) = |w(t, f_0) * M(t)|^2 \quad (3)$$

where M refers to Laplacian-filtered scalp-recorded EEG data. The convolution of the signal by a family of wavelets constructs a TF representation of the signal as shown in Fig. 2. Fig. 2 shows the averaged TF representation of all trials. The left column is TF representation for EEG signals recorded at electrode C3 (on the left hemisphere), while the right for channel C4 (on the right hemisphere). The upper row corresponds to left hand movement imagination, and the lower right hand movement imagination.

From Fig. 2, we can see that the mu rhythm has a clear energy decrease or ERD on the contralateral hemisphere starting from 4s to 5.75s, which also suggests that the subject would begin to imagine right after the preparation cue instead of the execution cue. With the help of TF representation, we chose the time window from 4.5 to 5s and frequency band from 11–12Hz for source analysis due to the observation of largest difference as appeared during this time window and the frequency band.

C) Bandpass Temporal Filtering—The Laplacian-filtered EEG data were then band-pass filtered in the alpha band (11–12Hz) using fifth order butterworth temporal filter. As previously reported, mu rhythm ERD emerges over the contralateral central region from the start of the movement imagination (Pfurtscheller 1994, 1997, 1999), which means the mu rhythm is blocked on the contralateral side, we can anticipate that using source analysis methods, the equivalent sources estimated using dipole localization method or cortical current density imaging should be stronger on the ipsilateral side of the brain.

D) Noise Estimation—The 20% time points with lowest mean global field/potential power (MGFP) were selected as noise.

After getting the noise covariance matrix C , the original data were transformed to SNR values by

$$\tilde{M} = \frac{1}{\text{diag}\sqrt{C}} M \quad (4)$$

where M is the spatial and temporally filtered EEG data and only the diagonal value in matrix C was used.

E) Independent Components Analysis (ICA)—The ICA method is a statistical method for transforming an observed multidimensional vector into components that are statistically as independent from each other as possible (Jutten & Herault, 1991; Comon 1994; Hyvärinen & Oja, 1997). The goal is to find a coordinate system in which the data are maximally statistically independent:

$$\tilde{M} = A \cdot S \quad (5)$$

where \tilde{M} is the SNR value of n (channel number) by t (time points), A is the mixing matrix and S is a matrix whose components are mutually independent.

Solving the ICA problem is to find a matrix W iteratively so that the linear transformation of the data \tilde{M} yields components that are as mutually independent as possible.

$$S = W \cdot \tilde{M} \quad (6)$$

In the present study, the fixed-point algorithm was used for ICA (Hyvärinen & Oja, 1997). Before implementing ICA, Singular value decomposition (SVD) was used for decorrelation. This procedure can speed up the iteration process of ICA by setting all singular values to zero which are below a certain threshold. It was realized as

$$\tilde{M} = U \cdot \Sigma \cdot V^T \quad (7)$$

where Σ is a diagonal matrix containing singular values of \tilde{M} . U contains the orthogonal, normalized spatial patterns and V^T contains the normalized time courses.

After noise estimation, we have changed our signal data to SNR values, all the time courses with singular value less than a certain value were regarded as noise subspace and discarded. Assuming that V_c is the subset of time courses from V^T corresponding to singular values above threshold, which is regarded as signal subspace, ICA can be computed and realized only on this signal subspace. Then, equation (6) can be changed to

$$\tilde{S} = \tilde{W} \cdot V_c \quad (8)$$

Replacing V^T in equation (7) by V_c from equation (8), the mixing matrix A in equation (5) can be obtained by following equation

$$A = U \Sigma \tilde{W}^{-1} \quad (9)$$

Sorting mixing matrix A by its column norm, independent components can be obtained from equation (5) in non-decreasing order.

3) Source Analysis

Source analysis is a widely used technique to estimate the source signals from scalp recorded EEG data. Such approach has been used extensively to localize neural sources that generate the scalp EEG (He 1999; He & Lian, 2004). It's necessary to assume a model of the source and a model of the head volume conductor for estimation of the neural sources. In the present study, both the equivalent dipole analysis and cortical current density (CCD) imaging approaches were used. The equivalent dipole model assumes that the neural sources

corresponding to a particular event or task can be approximated by one or few current dipoles that are movable within the brain (He et al., 1987; He & Lian, 2004). The cortical current density model assumes that neural sources can be approximated by a layer of current dipoles distributed over the cortex (Dale & Sereno, 1993). The 3-concentric sphere head model (Rush and Driscoll, 1968) contains three concentric layers with different electrical conductivities, which represent the cortex, skull and scalp, respectively.

Because we are only interested in the activity in motor cortex, channels on the frontal and occipital parts were removed -- only the electrodes around sensorimotor cortex (FC3, FC1, FCz, FC2, FC4, C3, C1, Cz, C2, C4, CP3, CP1, CPz, CP2, CP4) were chosen for source analysis. In the present study, only the first component of ICA was used for source reconstruction, by setting all but the first column of A to zero. The time point with the largest amplitude in this first component of ICA was used for source reconstruction, which consists of 15 data points over the corresponding sites of the scalp.

In the equivalent dipole analysis, to find the location and moment of the dipole is to minimize the residual error (He et al., 1987):

$$\Delta^2 = \| Lj - \tilde{M} \|^2 \quad (10)$$

where L is the lead field matrix, j is the dipole moment and \tilde{M} represents the first component of ICA. The Simplex method (Kowalik & Osborne, 1968) was used to solve this problem.

CCD is defined as dipole moment per volume with the unit $\mu\text{Amm}/\text{mm}^3$. A CCD is discretized into a large number of elementary dipoles which are distributed over the cortical surface. The weighted minimum norm (MN) method was used to solve the inverse problem,

$$\Delta^2 = \| Lj - \tilde{M} \|^2 + \lambda \| Qj \|^2 \quad (11)$$

where L is the lead field, j is the cortical current density vector, \tilde{M} is the first component of ICA, Q is a weighting matrix with depth information, and λ is the regularization parameter, which was determined by the L-curve criterion (Hansen 1992).

III. RESULTS

The effect of source analysis is illustrated in Fig. 3. Fig. 3(a) depicts the scalp EEG map of one single trial, after Laplacian spatial filtering and bandpass temporal filtering, while Fig. 3(b) shows the equivalent dipole solution and cortical current density distribution (only those larger than 80% of the largest current strength are plotted.). From Fig. 3(a), it is hard to tell whether the activity is originated on the left or right hemisphere of the brain, while it is clear from the source space as shown in Fig. 3(b).

Figs. 4 and 5 show the equivalent dipole solutions and cortical current density distribution of five trials for both left and right hand movement imagination respectively. As we have mentioned above that in μ rhythm, an ERD appears at the contralateral side of the brain

during motor imagination, thus the equivalent dipole and CCD should appear or be stronger at the ipsilateral side. These two figures support this hypothesis.

Till now, a simple classification rule can be defined based on source analysis results.

- a. For equivalent dipole analysis, the classification is correct if the equivalent dipole is located at the ipsilateral side with the imaginary hand.
- b. For CCD, all currents larger than 80% of the largest sum up. If the summation is larger at the ipsilateral side than at the contralateral side, we judge the classification correct, otherwise wrong.

The classification accuracy was defined as the ratio of the number of trials the present source analysis method classified correctly the motor imagery over the total number of the trials. Based on these two criteria, we obtained 78.9% and 80.6% classification accuracy in the human subject studied. This result is quite promising because it is based on single trial, not averaged values. We also didn't use any training procedure and all data analysis was performed based on only one frequency component. So to use more frequency bands and a better classifier may further improve the results as obtained from the source analysis.

IV. DISCUSSION

In the present pilot study we have initially tested the hypothesis that source analysis methods such as dipole localization and cortical imaging can be applied to classification of motor imagery tasks for BCI applications. The promising results we have obtained in this pilot study suggest that the source analysis approach has the unique characteristics of detecting the activity within the human brain thus substantially reducing the distortion or smearing problem caused by the skull low conductivity and making the motor imagery classification easier.

We have performed the source analysis of the recorded scalp EEG signals in a human subject by means of two representative source reconstruction methods: equivalent dipole localization and cortical imaging. The classification was based on the phenomena that during motor imagination, contralateral mu rhythm ERD always appears, and thus the corresponding equivalent source distribution should show dominating phenomena on the ipsilateral side. By means of signal processing strategy we have developed and tested in the present study, our results show that reasonable classification rate can be achieved by this simple classification rule. Note that, not only the contralateral ERD can be found, a significant ipsilateral ERS has also been observed, which may make this classification more accurately. However, the classification rule we have adopted in the present study is totally based on the contralateral ERD. If some subjects have different topography of ERD, this rule may not be so effective. A better classifier with some training procedure could be introduced to further improve the approach (Babiloni et al 2000, 2001; Pfurtscheller 1997; Wang & He 2004; Vallabhaneni & He, 2004).

Previously reported methods showed about 80% classification accuracy for the 10-fold cross-validation protocol with training (Wang & He, 2004; Vallabhaneni & He, 2004), while the present method achieved about 80% classification accuracy using all trials without

training. The unique feature of not requiring training process appears to be one of the advantages of the present approach, where the physical relationships between the neural sources and scalp EEG are taken into consideration. The obtained source signals have better SNR than the scalp EEG data and can be well related to cortical regions that are involved in the motor imagery tasks. ICA appears to play an important role to extract the useful information, enabling effective source estimation to identify the imagined hand movements by revealing the origins of the brain activities so as to manifest the difference between mental tasks directly. The present 80% single trial based classification accuracy indicates that the use of source analysis methods in facilitating discrimination of left or right hand movement imagination is quite positive. It is worthy to point out that a full scale of human study in a large group of subjects should be conducted before the final conclusion can be drawn. However, the present results do suggest the feasibility of using source analysis for classifying motor imagery tasks.

In the present study, all the 180 trials that are provided by the UPenn database are used for testing without rejecting any “bad” trial. However, in the practical experiment, subjects could not always concentrate and perform well on every trial. Sometimes they might be distracted and thought nothing. The performance would be further improved if these “bad” trials could be rejected based on on-line feedback. Although we have tested the present approach in off-line data, the approach itself could be implemented in on-line BCI application with little alteration.

Note that the frequency band and time window are also essential for classification because we know for different subjects, the clearest ERD may occur at different frequency band and at different time points (Pfurtscheller 1997; Wang & He, 2004). In this study, we have selected the two parameters manually with the help of TF representation. How to find a better way to choose the suitable frequency band and time window for source analysis is another issue that should be further explored.

In summary, we have developed a source analysis approach in combination with signal preprocessing for classification of motor imagery, and tested the present approach in a human subject. The present results obtained in the pilot study suggest that the source analysis provides an alternative means of aiding the classification of motor imagery tasks by converting scalp EEGs onto the source signals.

Acknowledgments

The authors are grateful to Jie Deng for useful discussions, and Dr. Allen Osman of University of Pennsylvania for making his data available. This work was supported in part by NSF BES-0411898, NSF-BES-0218736, and NIH R01 EB00178.

References

- Babiloni F, Babiloni C, Carducci F, Fattorini L, Onorati P, Urbano A. Spline Laplacian estimate of EEG potentials over a realistic magnetic resonance-constructed scalp surface model. *Electroencephalogr Clin Neurophysiol.* 1996; 98 (4) 363–73. [PubMed: 8641156]
- Babiloni F, Cincotti F, Lazzarini L, Millan J, Mourino J, Varsta M, Heikkinen J, Bianchi L, Marciani MG. Linear classification of low-resolution EEG patterns produced by imagined hand movements. *IEEE Trans Rehabil Eng.* 2000; 8 (2) 186–188. [PubMed: 10896181]

- Babiloni F, Febo C, Luigi B. Recognition of imagined hand movements with low resolution surface Laplacian and linear classifiers. *Med Eng & Phys.* 2001; 23: 323–328. [PubMed: 11435146]
- Birbaumer N. A spelling device for the paralysed. *Nature.* 1999; 398: 297–298. [PubMed: 10192330]
- Comon P. Independent component analysis, a new concept? *Signal Processing.* 1994; 36: 287–314.
- Dale AM, Sereno M. Improved localization of cortical activity by combining EEG and MEG with MRI cortical surface reconstruction: a linear approach. *J Cognitive Neuroscience.* 1993; 5: 162–76.
- Donoghue JP. Connecting cortex to machines: recent advances in brain interfaces. *Nature Neurosci Suppl.* 2002; 5: 1085–1088.
- Hansen PC. Analysis of discrete ill-posed problems by means of the L-curve. *SIAM Rev.* 1992; 34: 561–580.
- He B, Musha T, Okamoto Y, Homma S, Nakajima Y, Sato T. Electric dipole tracing in the brain by means of the boundary element method and its solution accuracy. *IEEE Trans Biomed Eng.* 1987; 34: 406–414. [PubMed: 3610187]
- He B. Brain Electric Source Imaging: Scalp Laplacian Mapping and Cortical Imaging. *Critic Rev Biomed Eng.* 1999; 27: 149–188.
- He B, Lian J, Li G. High-Resolution EEG: A New Realistic Geometry Spline Laplacian Estimation Technique. *Clin Neurophysiol.* 2001; 112: 845–852. [PubMed: 11336900]
- He B, Zhang Z, Lian J, Sasaki H, Wu S, Towle VL. Boundary Element Method Based Cortical Potential Imaging of Somatosensory Evoked Potentials Using Subjects' Magnetic Resonance Images. *NeuroImage.* 2002; 16: 564–576. [PubMed: 12169243]
- He, B, editor. *Modeling and Imaging of Bioelectric Activity – Principles and Applications.* Kluwer Academic/Plenum Publishers; 2004.
- He, B, Lian, J. *Electrophysiological Neuroimaging.* In: He, B, editor. *Neural Engineering.* Kluwer Academic/Plenum Publishers; 2004. in press
- Hjorth B. An on-line transformation of EEG scalp potentials into orthogonal source derivations. *Electroencephalogr Clin Neurophysiol.* 1975; 39 (5) 526–530. [PubMed: 52448]
- Hyvärinen A, Oja E. A Fast Fixed-Point Algorithm for Independent Component Analysis. *Neural Computation.* 1997; 9: 1483–1492.
- Jutten C, Herault J. Blind separation of sources, I: An adaptive algorithm based on neuromimetic architecture. *Signal Processing.* 1991; 24: 1–10.
- Kowalik, J, Osborne, MR. *Methods for unconstrained optimization problems.* New York: Elsevier; 1968.
- McFarland DJ, McCane LM, David SV, Wolpaw JR. Spatial filter selection for EEG-based communication. *Electroencephalogr Clin Neurophysiol.* 1997; 103: 386–394. [PubMed: 9305287]
- Nicolelis MAL. Actions from thoughts. *Nature.* 2001; 409: 403–407. [PubMed: 11201755]
- Nicolelis MAL. Brain-machine interfaces to restore motor function and probe neural circuits. *Nature.* 2003; 4: 417–422.
- Osman, A; Robert, A. Time-course of cortical activation during overt and imagined movements; *Cognit Neurosci Annual Meeting; New York.* March 2001;
- Pfurtscheller G, Neuper C. Event-related synchronization of mu rhythm in the EEG over the cortical hand area in man. *Neurosci Lett.* 1994; 174: 93–96. [PubMed: 7970165]
- Pfurtscheller G, Neuper Ch, Flotzinger D, Pregenzer M. EEG-based discrimination between imagination of right and left hand movement. *Electroencephalogr Clin Neurophysiol.* 1997; 103: 642–651. [PubMed: 9546492]
- Pfurtscheller, G. *Event-related desynchronization.* Elsevier Publisher; 1999. 303–325.
- Rohde MM, Belmont SL, Huggins JE, Levine SP, Kushwaha RK, Schuh LA. Quality estimation of subdurally recorded, event-related potentials based on signal-to-noise ratio. *IEEE Trans Biomed Eng.* 2002; 49: 31–40. [PubMed: 11794769]
- Rush S, Driscoll D. Current distribution in the brain from surface electrodes. *Anesth & Analg.* 1968; 47: 717–723.
- Sajda P, Gerson A, Mueller KR, Blankertz B, Parra L. A data analysis competition to evaluate machine learning algorithms for use in brain-computer interfaces. *IEEE Trans Neural Syst Rehabil Eng.* 2003; 11: 184–185. [PubMed: 12899269]

- Tallon-Baudry C, Bertrand O, Delpuech C, Pernier J. Oscillatory γ -band activity induced by a visual search task in humans. *J Neurosci.* 1997; 17 (2) 722–734. [PubMed: 8987794]
- Vallabhaneni A, He B. Motor imagery task classification for brain computer interface applications using spatiotemporal principle component analysis. *Neurolog Res.* 2004; 26: 282–287.
- Vallabhaneni, A, Wang, T, He, B. Brain Computer Interface. In: He, B, editor. *Neural Engineering.* Kluwer Academic/Plenum Publishers; 2004. in press
- Wang T, He B. An efficient rhythmic component expression and weighting synthesis strategy for classifying motor imagery EEG in brain computer interface. *J Neural Eng.* 2004; 1: 1–7. [PubMed: 15876616]
- Wolpaw JR, McFarland DJ, Neat GW, Forneris CA. An EEG-based brain–computer interface for cursor control. *Electroencephalogr Clin Neurophysiol.* 1991; 78: 252–259. [PubMed: 1707798]
- Wolpaw JR, Birbaumer N, McFarland DJ, Pfurtscheller G, Vaughan TM. Brain–computer interfaces for communication and control. *Clin Neurophysiol.* 2002; 113: 767–791. [PubMed: 12048038]

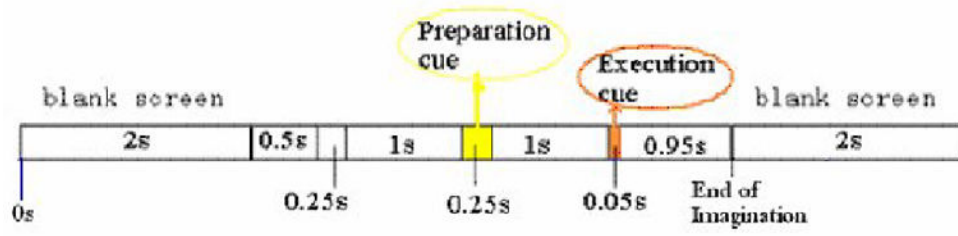


Fig. 1.
Time sequence of one trial epoch of the experiment.

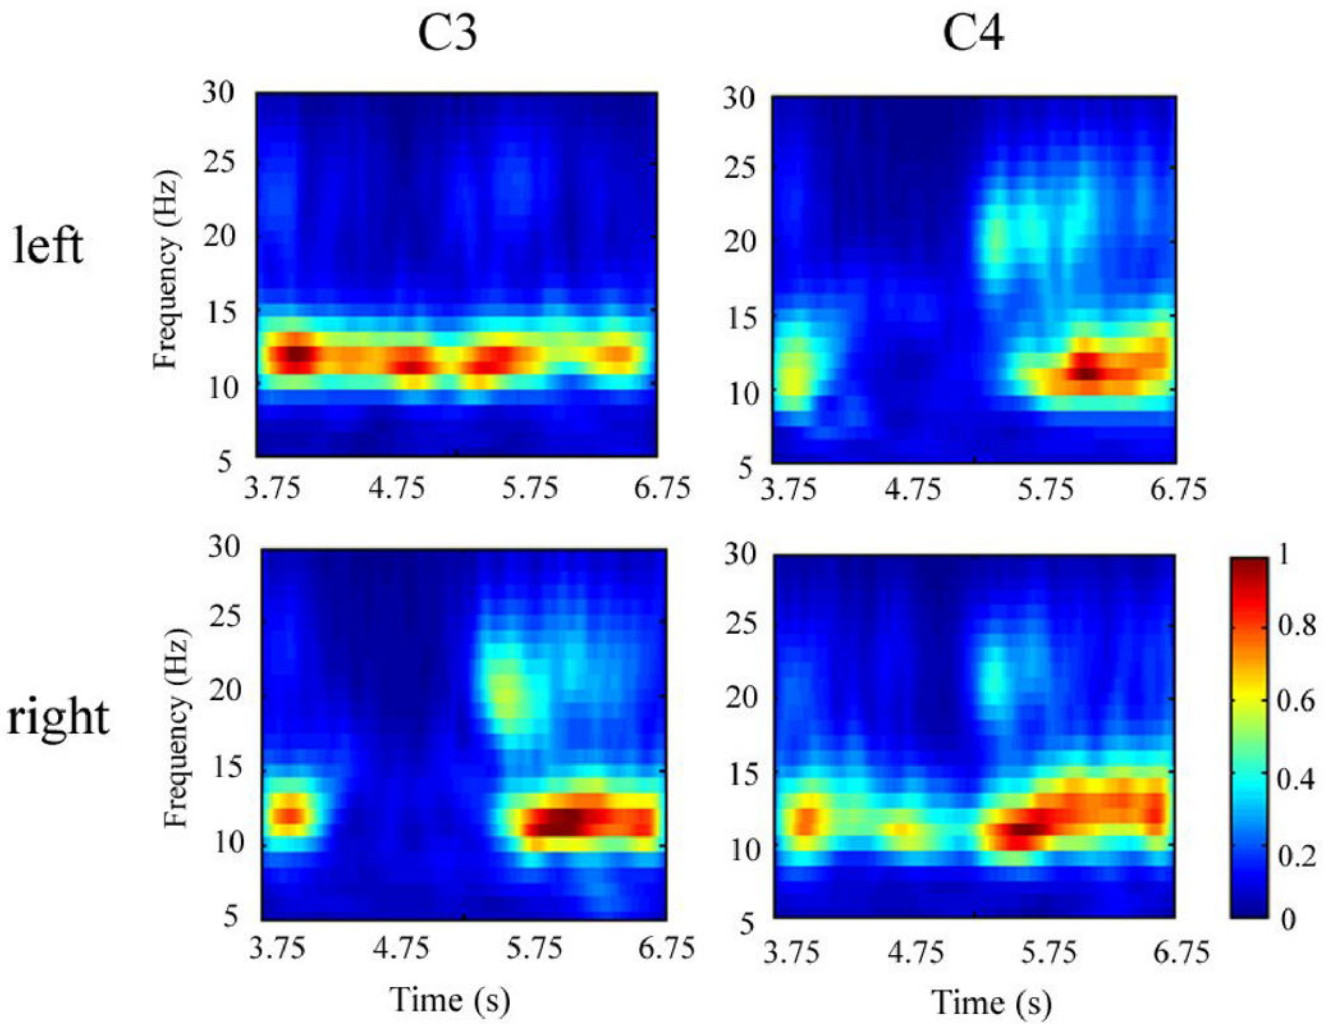


Fig. 2. Averaged Time-Frequency (TF) representation of channel C3 and C4 during motor imagery in a subject. Left column refers to TF representation for C3 and right column for C4. The upper row refers to the TF representation of left hand movement imagination and the lower refers to right hand movement imagination. The time period shown here is 3s from the preparation cue (3.75s) and frequency band is from 5 to 30 Hz.

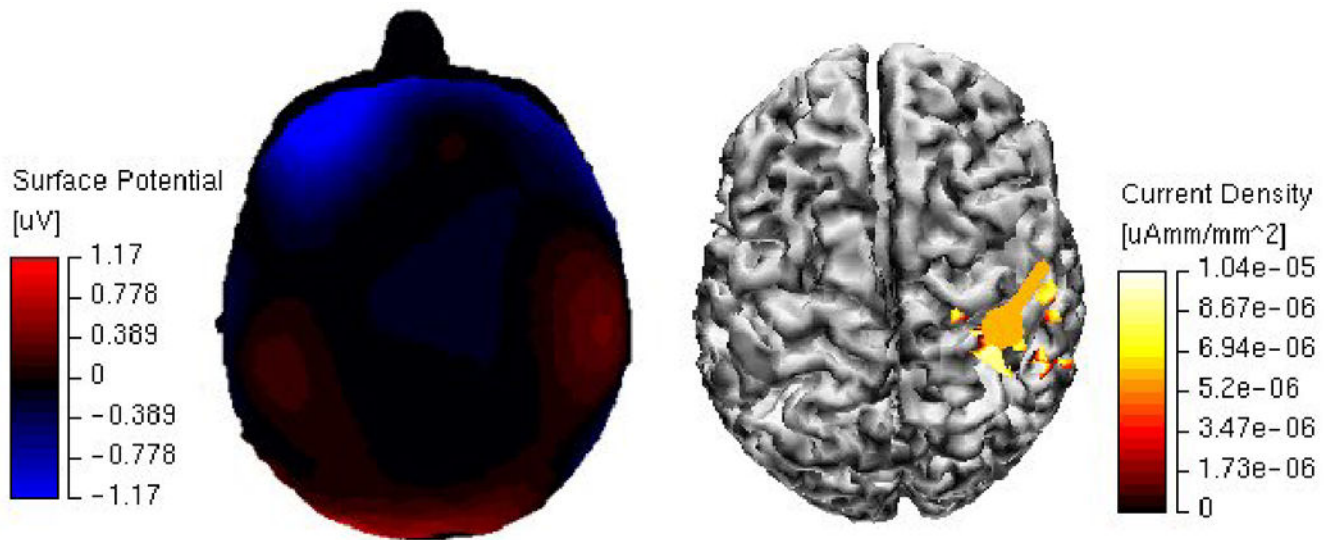


Fig. 3. Illustration of effect of source analysis. The left panel illustrates the surface Laplacian and temporal-bandpass filtered scalp EEG map of a single trial, and the right panel depicts the equivalent dipole solution and cortical current density distribution estimated from it.

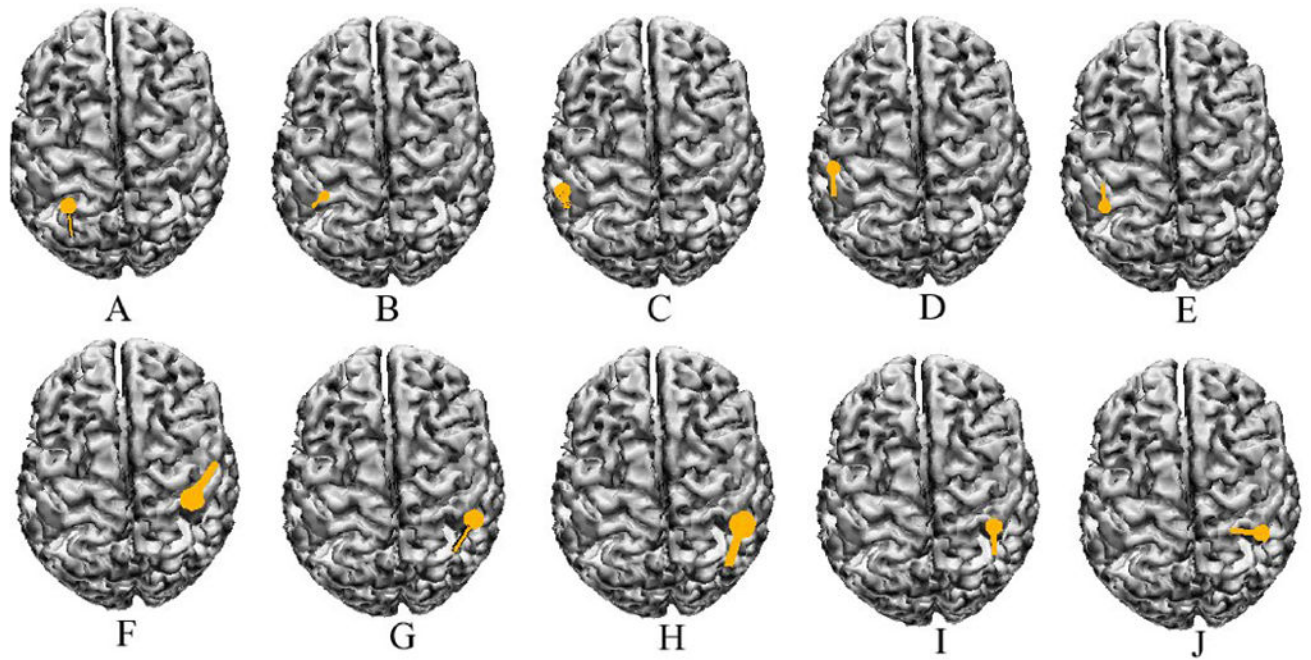


Fig. 4. Examples of equivalent dipole solutions of different trials in a human subject during imagination of left or right hand in alpha band. (A,B,C,D,E - left-hand movement imagery; F,G,H,I,J - right-hand movement imagery). Results were estimated from single trial scalp EEG data. See text for detailed procedures to obtain single trial inverse solutions.

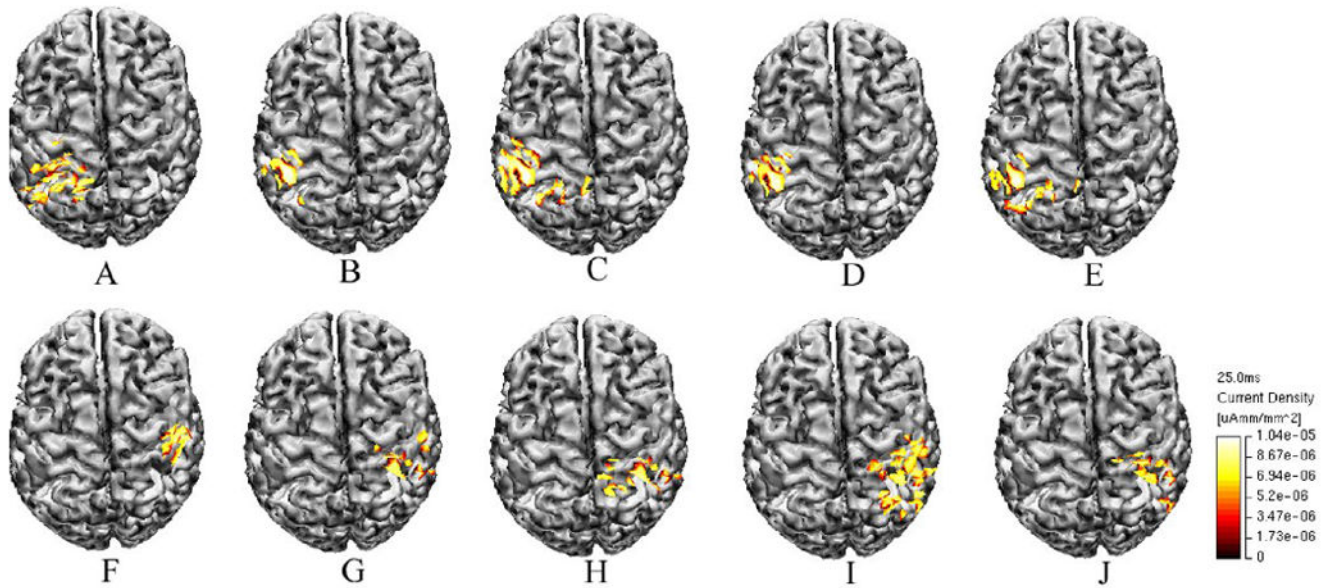


Fig. 5. Examples of cortical current density distributions of different trials in a human subject during motor imagination. (A,B,C,D,E - left-hand movement imagery; F,G,H,I,J – right-hand movement imagery). Results were estimated from single trial scalp EEG data. See text for detailed procedures to obtain single trial inverse solutions.