

Published in final edited form as:

J Am Chem Soc. 2007 January 31; 129(4): 728–729.

Proton Assisted Insensitive Nuclei Cross Polarization

Józef Lewandowski, Gaël De Paëpe, and Robert G. Griffin

Department of Chemistry and Francis Bitter Magnet Laboratory, Massachusetts Institute of Technology, Cambridge, MA 02139

Abstract

This communication presents a solid-state NMR ^{15}N - ^{13}C polarization transfer scheme applicable at high B_0 and high MAS frequencies, requiring moderate r.f. powers (~ 50 kHz $^{13}\text{C}/^{15}\text{N}$) and mixing time (1–6 ms). The sequence, PAIN-CP, involves the abundant nearby protons in the heteronuclear recoupling dynamics, and provides a new tool for obtaining long distance ^{15}N - ^{13}C contacts. It should be of major interest for biomolecular structural studies.

Polarization transfer^{1–15} between different nuclear species mediated by dipolar couplings is used extensively in magic angle spinning (MAS)¹⁶ experiments to perform chemical shift assignments, and to measure distances^{5–7, 11, 17–21} and torsion angles.^{22–25} Heteronuclear dipolar recoupling sequences can be classified into two categories depending on their behavior with respect to dipolar truncation. The first group includes the double CP sequence (DCP²⁶) and its variants (SPICP²⁷, RFDRCP⁴, *i*DCP⁹) which lead to non-commuting terms in the effective Hamiltonian, and thus are mainly used to perform one-bond transfers (NCO, NCA) sometimes followed by a homonuclear ^{13}C - ^{13}C recoupling period for obtaining ^{15}N - ^{13}C multiple-bond contacts.^{28, 29} The second group of sequences (REDOR⁵, TEDOR^{1/} REPT¹⁹, GATE¹⁷) yields a longitudinal effective Hamiltonian and enables measurement of long distances (< 4 Å).^{20, 21}

High magnetic fields (> 600 MHz) are an important experimental component for improving sensitivity and resolution in biomolecular MAS experiments involving ^{15}N - ^{13}C magnetization transfer, provided that experiments can be performed at high MAS frequencies (> 15 kHz) to compensate for increases in chemical shift anisotropies (CSA). Unfortunately, the application of the sequences mentioned above becomes problematic in this regime as the applied high r.f. powers lead to increased sample heating, jeopardize the integrity of the probe, but often do not provide sufficient ^1H decoupling.

Here we present an efficient ^{15}N - ^{13}C heteronuclear recoupling technique that involves nearby protons in the transfer and is applicable at high MAS frequency ($\omega_r/2\pi > 20$ kHz). This new scheme, Proton Assisted Insensitive Nuclei Cross Polarization (PAIN-CP), reduces dipolar truncation and therefore is particularly well suited for obtaining long distance contacts. PAIN-CP demonstrates that *the involvement of protons in the polarization transfer between low- γ nuclei does not have to be deleterious in nature; on the contrary ^1H 's can be used to enhance the rate and efficiency of the transfer.* The PAIN-CP experiment utilizes a mechanism which we refer to as Third Spin Assisted Recoupling (TSAR). Its extension to the homonuclear case is straightforward and will be discussed elsewhere. Note that the use of ^1H irradiation has been reported previously for ^{13}C - ^{13}C recoupling experiments,^{30–32} but that the underlying mechanism is different.

Even though PAIN-CP and DCP²⁶ have similar pulse sequences (see Figure 1 and Supporting Information Section 7–8 (S.I.-7, 8)), they rely on very different mechanisms. The PAIN-CP mechanism corresponds to a second order recoupling in an interaction frame defined by the three C.W. r.f. fields involving cross terms between heteronuclear N-H and C-H dipolar couplings (see S.I.-2). In this process, nearby ¹H's are used to create trilinear (N, C, H) terms in the effective Hamiltonian that can lead to ZQ and DQ ¹⁵N-¹³C polarization transfer. In this publication we explore only the ZQ transfer.

Figure 2 shows simulations comparing ¹⁵N-¹³C polarization transfer for the PAIN-CP, DCP, TEDOR and GATE sequences at $\omega_{1H}/2\pi=750$ MHz and $\omega_r/2\pi=20$ kHz. The model spin system consists of seven spins (¹⁵N, ¹³C _{α} , ¹³C _{β} , 4 ¹H's). Simulations were performed with SPINEVOLUTION³³ (see S.I.-1 for details).

DCP simulations utilized typical r.f. field strengths -- ($\omega_{1C}/2\pi$)=45 kHz, ($\omega_{1N}/2\pi$)=25 kHz, ($\omega_{1H}/2\pi$)=100 and 150 kHz of ¹H C.W. decoupling respectively, illustrating that r.f. power levels should satisfy the condition (ω_{1H}/ω_{1C}) ≥ 3 to ensure correct ¹H decoupling.³⁴ However, even for 150 kHz of ¹H decoupling, a challenge for most triple resonance probes, the two-bond transfer from ¹⁵N to C _{β} reaches only about 6.5% efficiency in 6.5 ms, a result of the dipolar truncation effect (see S.I.-4). Longitudinal recoupling sequences such as TEDOR or GATE, where there is no dipolar truncation, do not provide efficient two-bond transfer in the presence of strong one-bond coupling. For example, GATE reaches about 7% transfer in 2.3 ms for extremely demanding experimental settings. On the other hand, the PAIN-CP buildup obtained with a ¹³C and ¹⁵N fields set to the same value (n=0 Hartmann-Hahn)^{35, 36} reaches 16.5% transfer efficiency in 4 ms, an improvement of 3 to 8 times when compared to DCP with high power ¹H decoupling. In addition, contrary to TEDOR and GATE results, the transferred magnetization achieves an equilibrium value simplifying the choice of the mixing time in a correlation experiment.

In practice, it is possible to utilize the PAIN-CP mechanism provided that ¹H-¹⁵N and ¹H-¹³C Hartmann-Hahn (H.H.) as well as rotary resonance³ (R.R.) conditions are avoided. The ¹⁵N and ¹³C r.f. fields do not necessarily have to match n=0 H.H. condition (see S.I.-2, 6). Optimal PAIN-CP settings are a compromise between avoiding destructive H.H. or R.R. recoupling conditions and retaining significant second order scaling to ensure efficient polarization transfer. Accordingly, there are usually a few different ¹H r.f. levels that lead to an appreciable PAIN-CP effect (see S.I.-6).

Figure 3 is an experimental demonstration that PAIN-CP is an efficient technique for heteronuclear ¹⁵N-¹³C correlation experiments. The spectra were obtained with [^{U-¹³C, ¹⁵N}] N-*f*-MLF-OH using $\omega_r/2\pi=20$ kHz, $\omega_{1H}/2\pi=750$ MHz, and a 2.5 mm, triple-channel Bruker probe. Figure 3(a) shows a NCA DCP spectrum with 3 ms mixing (optimum for one-bond transfer) and 112 kHz ¹H decoupling. Long range cross peaks (more than 2 bonds) are completely absent from the spectrum at this mixing time and do not appear at longer mixing times (data not shown). Figure 3(b) depicts an n=0 H.H. PAIN-CP spectrum with 4 ms mixing, using r.f. fields of ~50 kHz for ¹³C, ¹⁵N and (a) 112 kHz and (b) 62 kHz respectively for ¹H. *We observe cross peaks for ¹⁵N-¹³C pairs separated by up to 6 Å in a uniformly ¹³C, ¹⁵N labeled compound.* Note that part of the long range transfer also involves a ¹³C homonuclear TSAR effect (see S.I.-2). In addition, in spite of distributing the initial ¹⁵N magnetization over a larger number of ¹³C sites, the one-bond cross peaks are much more intense than in the DCP case. This fact indicates that for this system a ~2.5 ratio for ($\omega_{1H}/\omega_{13C,15N}$) is not sufficient to provide efficient ¹H decoupling in the DCP case.

In summary, we present a new heteronuclear ¹⁵N-¹³C correlation mechanism, applicable at high $\omega_r/2\pi$, leading, in this regime, to superior recoupling performance compared to alternative

techniques. PAIN-CP can provide long ^{15}N - ^{13}C contacts, circumventing the usual dipolar truncation encountered with DCP-type sequences. The method provides a highly efficient alternative to NCX and NCXCY experiments, extends the range of applicability of heteronuclear recoupling techniques to high B_0 and $\omega_r/2\pi$, and should thus be of major interest for structure determination of biomolecules.

Supplementary Material

Refer to Web version on PubMed Central for supplementary material.

Acknowledgements

This work was supported by National Institutes of Health Grants EB-001960 and EB-002026. We would like to thank Dr Patrick van der Wel for stimulating discussions and to the reviewers for their constructive comments.

References

1. Hing AW, Vega S, Schaefer J. *J Magn Reson* 1992;96(1):205–209.
2. Baldus M, Petkova AT, Herzfeld J, Griffin RG. *Mol Phys* 1998;95(6):1197–1207.
3. Oas TG, Griffin RG, Levitt MH. *J Chem Phys* 1988;89(2):692–695.
4. Sun BQ, Costa PR, Griffin RG. *J Magn Reson A* 1995;112(2):191–198.
5. Gullion T, Schaefer J. *J Magn Reson* 1989;81(1):196–200.
6. Zhao X, Hoffbauer W, auf der Gunne JS, Levitt MH. *Solid State Nucl Magn Reson* 2004;26(2):57–64. [PubMed: 15276635]
7. van Rossum BJ, de Groot CP, Ladizhansky V, Vega S, de Groot HJM. *J Am Chem Soc* 2000;122(14):3465–3472.
8. Ladizhansky V, Vinogradov E, van Rossum BJ, de Groot HJM, Vega S. *J Chem Phys* 2003;118(12):5547–5557.
9. Bjerring M, Nielsen NC. *Chem Phys Lett* 2003;382(5–6):671–678.
10. Dvinskikh S, Chizhik V. *J Exp Theor Phys* 2006;102(1):91–101.
11. Bertani P, Raya K, Hirschinger K. *Comptes Rendus Chimie* 2004;7(3–4):363–369.
12. Ray S, Ladizhansky V, Vega S. *J Magn Reson* 1998;135(2):427–434. [PubMed: 9878470]
13. Chan JCC. *Chem Phys Lett* 2001;335(3–4):289–297.
14. Pines A, Gibby MG, Waugh JS. *J Chem Phys* 1973;59(2):569–590.
15. Baldus M, Geurts DG, Hediger S, Meier BH. *J Magn Reson A* 1996;118(1):140–144.
16. Lowe IJ. *Phys Rev Lett* 1959;2:285.
17. Bjerring M, Rasmussen JT, Krogshave RS, Nielsen NC. *J Chem Phys* 2003;119(17):8916–8926.
18. Hing AW, Vega S, Schaefer J. *J Magn Reson A* 1993;103(2):151–162.
19. Saalwachter K, Graf R, Spiess HW. *J Magn Reson* 2001;148(2):398–418. [PubMed: 11237647]
20. Jaroniec CP, Filip C, Griffin RG. *J Am Chem Soc* 2002;124(36):10728–10742. [PubMed: 12207528]
21. Jaroniec CP, Tounge BA, Rienstra CM, Herzfeld J, Griffin RG. *J Am Chem Soc* 1999;121(43):10237–10238.
22. Hong M, Gross JD, Hu W, Griffin RG. *J Magn Reson* 1998;135(1):169–177. [PubMed: 9799691]
23. Hong M, Gross JD, Rienstra CM, Griffin RG, Kumashiro KK, Schmidt-Rohr K. *J Magn Reson* 1997;129(1):85–92. [PubMed: 9405219]
24. Hong M, Gross JD, Griffin RG. *J Phys Chem B* 1997;101(30):5869–5874.
25. Sack I, Balazs YS, Rahimipour S, Vega S. *J Am Chem Soc* 2000;122(49):12263–12269.
26. Schaefer J, McKay RA, Stejskal EO. *J Magn Reson* 1979;34(2):443–447.
27. Wu XL, Zilm KW. *J Magn Reson A* 1993;104(2):154–165.
28. Pauli J, Baldus M, van Rossum B, de Groot H, Oschkinat H. *Chembiochem* 2001;2(4):272–281. [PubMed: 11828455]

29. Egorova-Zachernyuk TA, Hollander J, Fraser N, Gast P, Hoff AJ, Cogdell R, de Groot HJM, Baldus M. *J Biomol Nmr* 2001;19(3):243–253. [PubMed: 11330811]
30. Morcombe CR, Gaponenko V, Byrd RA, Zilm KW. *J Am Chem Soc* 2004;126(23):7196–7197. [PubMed: 15186155]
31. Takegoshi K, Nakamura S, Terao T. 2001;344(5–6):631–637.
32. Takegoshi K, Nakamura S, Terao T. *J Chem Phys* 2003;118(5):2325–2341.
33. Veshkort M, Griffin RG. *J Magn Reson* 2006;178(2):248–82. [PubMed: 16338152]
34. Ishii Y, Ashida J, Terao T. *Chem Phys Lett* 1995;246(4–5):439–445.
35. Hartmann SR, Hahn EL. *Phys Rev* 1962;128(5):2042–2053.
36. Stejskal EO, Schaefer J, Waugh JS. *J Magn Reson* 1977;28(1):105–112.

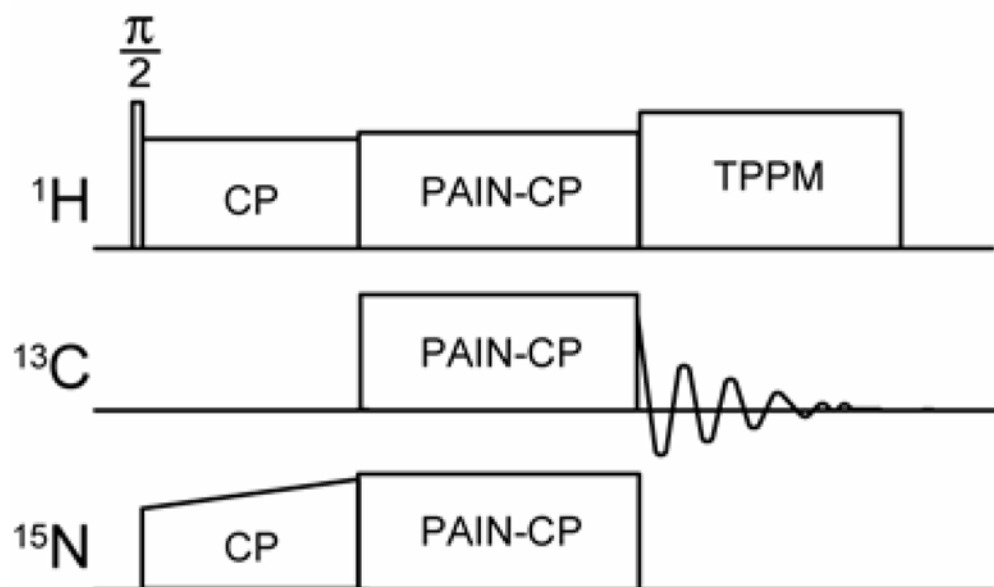


Figure 1. PAIN-CP ^{15}N - ^{13}C correlation pulse sequence. The proper combination of ^{15}N , ^{13}C and ^1H r.f. power results in enhanced rates and efficiency of ^1H mediated ^{15}N - ^{13}C polarization transfer.




Figure 2. Comparison of ^{15}N - ^{13}C two-bond polarization transfer for PAIN-CP, DCP, TEDOR, GATE AC sequences at $\omega_r/2\pi=20$ kHz. Note that variants of DCP such as RFDRCP, SPICP, and *i*DCP are not considered here as they mainly improve the recoupling bandwidth, which is not the major concern in this simulation.

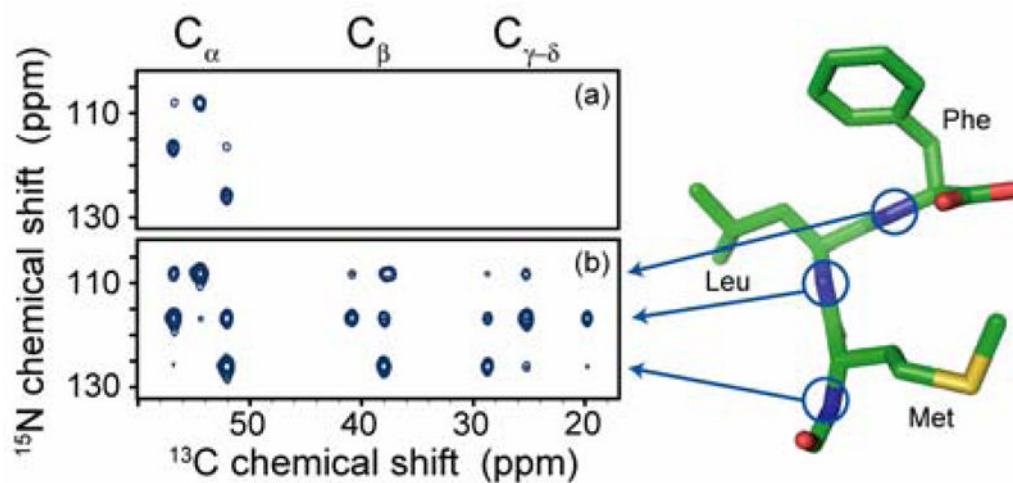


Figure 3. Aliphatic region of 2D ^{15}N - ^{13}C correlation spectra obtained at 750 MHz with 20 kHz MAS: (a) DCP with 3 ms mixing, (b) PAIN-CP with 4 ms mixing. The ^1H r.f. field strength was 112 and 62 kHz for (a) and (b) respectively. In (a) the $n=1$ ZQ Hartmann-Hahn condition was matched with 45 kHz ^{13}C r.f. and 25 kHz ^{15}N r.f.. In (b) $\omega_1/2\pi = 50$ kHz for both ^{13}C and ^{15}N . All spectra were acquired and processed in exactly the same manner. The contour levels are set to the same value.