

# The effect of ceramic thickness and number of firings on the color of a zirconium oxide based all ceramic system fabricated using CAD/CAM technology

Vinay Chila Bachhav\*, MDS, Meena Ajay Aras, MDS

Department of Prosthodontics, Goa Dental College and Hospital, Bambolim, Goa, India

**PURPOSE.** Ceramics have a long history in fixed prosthodontics for achieving optimal esthetics and various materials have been used to improve ceramic core strength. However, there is a lack of information on how color is affected by fabrication procedure. The purpose of this study was to evaluate the effects of various dentin ceramic thicknesses and repeated firings on the color of zirconium oxide all-ceramic system (Lava™) fabricated using CAD/CAM technology. **MATERIALS AND METHODS.** Thirty disc-shaped cores, 12 mm in diameter with a 1 mm thickness were fabricated from zirconium oxide based all ceramic systems (Lava™, 3M ESPE, St Paul, MN, USA) and divided into three groups (n = 10) according to veneering with dentin ceramic thicknesses: as 0.5, 1, or 1.5 mm. Repeated firings (3, 5, 7, or 9) were performed, and the color of the specimens was compared with the color after the initial firing. Color differences among ceramic specimens were measured using a spectrophotometer (VITA Easyshade, VITA Zahnfabrik, Bad Säckingen, Germany) and data were expressed in CIELAB system coordinates. A repeated measures ANOVA and Bonferroni post hoc test were used to analyze the data (n = 10,  $\alpha = .05$ ). **RESULTS.** L\*a\*b\* values of the ceramic systems were affected by the number of firings (3, 5, 7, or 9 firings) ( $P < .001$ ) and ceramic thickness (0.5, 1, or 1.5 mm) ( $P < .001$ ). Significant interactions were present in L\*a\*b\* values between the number of firings and ceramic thickness ( $P < .001$ ). An increase in number of firings resulted in significant increase in L\* values for both 0.5 mm and 1.5 mm thicknesses ( $P < .01$ ,  $P = .013$ ); however it decreased for 1 mm thickness ( $P < .01$ ). The a\* values increased for 1 mm and 1.5 mm thicknesses ( $P < .01$ ), while it decreased for 0.5 mm specimens. The b\* values increased significantly for all thicknesses ( $P < .01$ ,  $P = .022$ ). As the dentin ceramic thickness increased, significant reductions in L\* values ( $P < .01$ ) were recorded. There were significant increases in both a\* and b\* values ( $P < .01$ ) as the dentin ceramic thickness increased. **CONCLUSION.** The number of firings and dentin ceramic thickness have a definite effect on the final color of all ceramic system tested. The mean  $\Delta E$  value increased as the dentin ceramic thicknesses increased for zirconium-oxide based all ceramic specimens tested. However, the mean  $\Delta E$  values were less than 3.7  $\Delta E$  units which is rated as a match in the oral environment. [J Adv Prosthodont 2011;3:57-62]

**KEY WORDS.** Dental porcelain, Color, CAD/CAM

## INTRODUCTION

Ceramics have a long history in fixed prosthodontics for achieving optimal esthetics. Yttria-stabilized tetragonal zirconia (Y-TZP) is gaining use in dentistry due to its good mechanical properties and superior biocompatibility.<sup>1</sup> It is currently used as core material in all ceramic dental restorations,<sup>2,3</sup> implant superstructures,<sup>4</sup> and orthodontic brackets.<sup>5</sup> Its superior mechanical properties compared to other dental ceramics, such as higher strength and fracture toughness,<sup>2,6,7</sup> which are due to the transformation toughening mechanism, are similar to that observed in quenched steel.

Color assessment is regarded as a complex psychophysiological process subject to numerous variables. Dentin is considered to

be the primary source of color for teeth, which is modified by the thickness and translucency of overlying enamel. The perceived color of natural teeth is a result of light reflected from the enamel surface, in addition to the effect of light scattering within enamel and dentin before it is ultimately reflected back.<sup>8</sup> Clinically, it is important that ceramic restorations reproduce the translucency and color of the natural teeth. There are many factors affecting the match, such as translucency, opalescence, fluorescence, surface texture, and shape.<sup>9,10</sup>

Most all ceramic systems require the combination of 2 layers of ceramic material, such as a strong ceramic core and a weak veneering porcelain,<sup>11</sup> with different opacity, shade, and thickness, to provide a natural appearance.<sup>12,13</sup> All ceramic restorations without a metal substructure allow for greater light

Corresponding author: Vinay C. Bachhav.

Department of Prosthodontics, Goa Dental College and Hospital, Rajiv Gandhi Medical Complex, Bambolim, Goa 403202, India

Tel. 91 9422783856; e-mail, vinaybachhav@gmail.com.

Received March 1, 2011 / Last Revision April 30, 2011 / Accepted May 9, 2011

© 2011 The Korean Academy of Prosthodontics

This is an Open Access article distributed under the terms of the Creative Commons Attribution Non-Commercial License (<http://creativecommons.org/licenses/by-nc/3.0>) which permits unrestricted non-commercial use, distribution, and reproduction in any medium, provided the original work is properly cited.

\*The zirconium oxide blocks used in this study were partly supported by 3M ESPE, India.

transmission within the restoration, thereby improving the color and translucency of the restoration; however, a perfect esthetic tooth-colored restoration cannot be ensured.<sup>14</sup> If the majority of light passing through a ceramic restoration is diffusely transmitted and only part of it is scattered, the material will appear translucent.<sup>15</sup> The amount of light that is absorbed, reflected, and transmitted depends on the quantity of crystals within the core matrix, their chemical nature, and the size of the particles compared to the incident light wavelength.<sup>16</sup> Core translucency was also identified as a primary factor in controlling esthetics and a critical consideration in the selection of the materials.<sup>17</sup> Some all ceramic core materials have high *in vitro* strength values.<sup>18,19</sup> However, an increase in crystalline content to achieve greater strength generally results in greater opacity.<sup>17,20</sup>

Clinical perceptibility of color differences has been the subject of numerous investigations. The Commission Internationale de l'Éclairage (CIE) recommended calculating color difference ( $\Delta E$ ) based on CIELAB color parameters.<sup>21</sup> The  $\Delta E$  values are used to describe whether the changes in the overall shade are perceivable to the human observer. This magnitude of the color difference is based on the human perception of color; color differences greater than 1  $\Delta E$  unit are visually detectable by 50% of human observers.<sup>22</sup> However, under uncontrolled clinical conditions, such small differences in color would be unnoticeable because average color differences below 3.7 have been rated as a match in the oral environment.<sup>23,24</sup>

Instrumental measurements can quantify color and allow communication to be more uniform and precise. In addition to the opacity and shade of the ceramic that determine the definitive shade of an esthetic restoration, other factors, including porcelain brand,<sup>8,25,26</sup> batches,<sup>25</sup> condensation techniques,<sup>25</sup> firing temperatures,<sup>26</sup> dentin thickness,<sup>27-29</sup> and number of porcelain firings,<sup>28,30</sup> can have an effect. Specific contributions of core and veneer thickness to the appearance of layered ceramics were determined,<sup>29</sup> and it was concluded that there was a significant correlation between the thickness ratio of core and veneer ceramics and the color of the restoration. Even when adequate ceramic thickness exists, clinical shade matches are difficult to achieve<sup>31</sup> because there is a wide range of translucency among the core materials of all ceramic systems at clinically relevant core thicknesses.<sup>16</sup> The thickness and the combination of ceramic layers, such as the core, veneer, and other specialty ceramic materials, have been shown to control the appearance of all ceramic materials.<sup>15,23,32</sup> Antonson and Anusavice<sup>32</sup> found that it was important to determine the translucency of a layered core-veneering ceramic as a function of thickness. Moreover, Heffernan *et al.*<sup>10,16</sup> investigated the influence of core and core-veneering ceramic thickness on overall translucency. Lee *et al.*<sup>33</sup> showed that the layered color of varied all ceramic and veneer combinations was different depending on the type of all ceramic core material, even though the thickness of the layered specimen was set to 1.5 mm. These studies, however,

did not address the particular contribution of each variable: the difference in core substructure, the changes in veneer thickness, or the number of firings.

The effect of multiple firings has been investigated in previous studies, and it has been reported that repeated firings did not noticeably affect the color of dental ceramics.<sup>28,30,34,35</sup> However, O'Brien *et al.*<sup>25</sup> found perceivable differences ( $\Delta E = 1$ ) between the color of ceramic specimens that were fired 3 and 6 times. Uludag *et al.*<sup>36</sup> and Ozturk *et al.*<sup>37</sup> reported perceptual color changes in L\*a\*b\* color parameters as the number of firings increase. The purpose of this study was to evaluate the effects of various dentin ceramic thicknesses (0.5, 1, or 1.5 mm) and number of firings (3, 5, 7, or 9) on the color of zirconium oxide all ceramic system fabricated using CAD/CAM technology. The research hypothesis was that the color difference would be determined relative to the firing times and dentin ceramic thicknesses.

## MATERIALS AND METHODS

The zirconia-based ceramic used in this study; the Lava™ All-ceramic system (3M ESPE Dental Products, St Paul MN, USA) utilizes CAD/CAM technology to produce a densely sintered and high strength zirconia framework with a 3% mol partially yttria-stabilized zirconia polycrystal content.

Thirty disc-shaped cores, 12 mm in diameter and 1 mm thick were fabricated from zirconia based all ceramic system using CAD/CAM technology. These cores were divided into three groups (n = 10) for veneering with dentin ceramic with thicknesses of 0.5, 1 and 1.5 mm. The cores were veneered with A1 (according to the VITA Shade Guide) dentin ceramic (LavaCeram, 3M ESPE, St Paul, MN, USA) with the use of the similar molds described by others<sup>25,28,32</sup> which allowed standardization of the dentin thicknesses for each of group to be studied. Specimens were then fired in a dental ceramic furnace (Lava Furnace 200, 3M ESPE, St Paul, MN, USA). The thickness of each group of specimens was then measured with a digital caliper (Dial Caliper D, Aura Dental, Aura an der Saale, Germany) with an accuracy of 0.02 mm, and corrected with diamond rotary cutting instruments (ISO 173/016, Mani. Inc, Utsunomiya, Tochigi, Japan) until the desired thickness of dentin ceramic was achieved (0.5, 1, or 1.5 mm).

The color of each specimen was measured with a spectrophotometer (VITA Easyshade; VITA Zahnfabrik, Bad Säckingen, Germany). The spectrophotometer's CIE L\*a\*b\* output is based on D65 illuminant and a 2-degree standard observer. Three measurements were made, and the average reading was calculated for each specimen. Instrument was recalibrated after measurement of each group (n = 10). The CIELAB measurements make it possible to evaluate the amount of perceptible color change in each specimen. The CIELAB color space is a uniform 3-dimensional color order

system. Equal changes in any of the 3 coordinates can be perceived as visually similar. Total color differences were calculated with use of the following equation.<sup>38</sup>

$$\Delta E^* = [(\Delta L^*)^2 + (\Delta a^*)^2 + (\Delta b^*)^2]^{1/2}$$

The L\* coordinate is a measure of the lightness-darkness of the specimen. The greater the L\* is, the lighter the specimen. The a\* coordinate is a measure of the chroma along the red-green axis. A positive a\* relates to the amount of redness, and a negative a\* relates to greenness of a specimen. The b\* coordinate is a measure of the chroma along the yellow-blue axis; that is, a positive b\* relates to the amount of yellowness, while a negative b\* relates to the blueness of the specimen.  $\Delta L^*$ ,  $\Delta a^*$ , and  $\Delta b^*$  are the differences in the CIE color-space parameters of the 2 colors.<sup>38</sup>

The results of the testing were analyzed with statistical software (SPSS, PC, Version 17.0; SPSS, Inc, Chicago, IL, USA). Repeated measurements of the data (number of firings and ceramic thicknesses) were analyzed with analysis of variance (ANOVA) for significant differences. Bonferroni post hoc test was used to perform pairwise comparisons ( $\alpha=.05$ ).

## RESULTS

The analysis revealed that L\*a\*b\* values of ceramic system (Table 1) were affected by number of firings [3, 5, 7 or 9] ( $P<.001$ ) and dentin ceramic thickness [0.5 mm, 1 mm or 1.5 mm] ( $P<.001$ ).

Significant interactions were present in L\*, a\* and b\* values within each group of dentin ceramic thickness i.e. 0.5 mm, 1 mm or 1.5 mm. An increase in number of firings resulted in significant increase in L\* values for both 0.5 mm and 1.5 mm thicknesses ( $P<.01$ ,  $P=.013$ ); however it decreased for 1 mm thickness ( $P<.01$ ). The a\* values increased for 1 mm and 1.5 mm thicknesses ( $P<.01$ ), while it decreased for 0.5 mm specimens. The b\* values increased significantly for all thicknesses-0.5 mm, 1 mm and 1.5 mm as the number of firings increased ( $P<.01$ ,  $P<.01$ ,  $P=.022$ ).

Significant interactions were also present in all color co-ordi-

nates i.e. L\*, a\* and b\* values among all three groups of dentin ceramic thicknesses and number of firings. As the dentin ceramic thickness increased (0.5 mm - 1 mm - 1.5 mm), significant reductions in L\* values ( $P<.01$ ) were recorded (Fig. 1). There were significant increases in both a\* and b\* values ( $P<.01$ ) as the dentin ceramic thickness increased (Fig. 2, 3).

Mean color difference ( $\Delta E$ ) values were calculated for each group of thickness. The mean  $\Delta E$  value increased as the thicknesses increased. Mean  $\Delta E$  values were less than 3 when ceramic thickness increased from 0.5 mm to 1 mm ( $\Delta E = 1.43$ ) and from 1 mm to 1.5 mm ( $\Delta E = 2.38$ ). It was higher than 3 ( $\Delta E = 3.37$ ) when ceramic thickness increased from 0.5 mm to 1.5 mm.

The  $\Delta E$  values were calculated for each specimen within each group to determine mean color differences ( $\Delta E$ ), depending on repeated firings (Table 2). The  $\Delta E$  value was smaller than 1 between firing 5 and 7, firing 5 and 9, and firing 7 and 9 for 0.5 mm thickness and between firing 3 and 9 for 1 mm thickness. The  $\Delta E$  value was higher than 1 between all firings for 1.5 mm specimens.

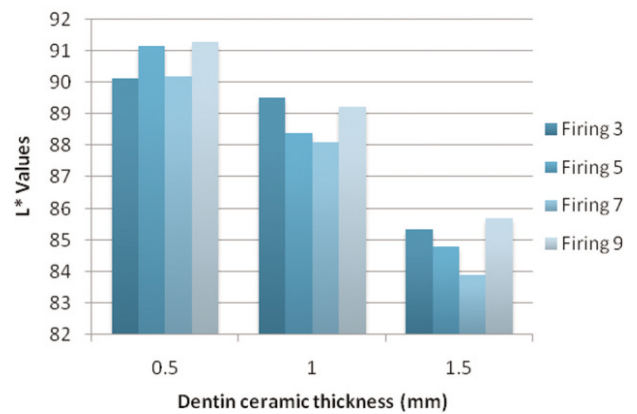


Fig. 1. Means of L\* for number of firings and dentin ceramic thicknesses.

Table 1. Multivariate test results based on a repeated measures ANOVA for changes in color coordinates after repeated firings of ceramic

Effect		Pillai's value	F	Hypothesis df	Error df	Sig.
$\Delta L^*$	Thickness	.970	131.241 <sup>a</sup>	2	8	<.001
	Number of firings	.955	49.557 <sup>a</sup>	3	7	<.001
	Number of firings × thickness	.981	33.537 <sup>a</sup>	6	4	<.001
$\Delta a^*$	Thickness	.993	557.185 <sup>a</sup>	2	8	<.001
	Number of firings	.955	49.988 <sup>a</sup>	3	7	<.001
	Number of firings × thickness	.999	1247.562 <sup>a</sup>	6	4	<.001
$\Delta b^*$	Thickness	.938	60.507 <sup>a</sup>	2	8	<.001
	Number of firings	.868	15.289 <sup>a</sup>	3	7	<.001
	Number of firings × thickness	.988	56.342 <sup>a</sup>	6	4	<.001

( $P<.05$  indicates significant difference; <sup>a</sup>: Exact statistics)

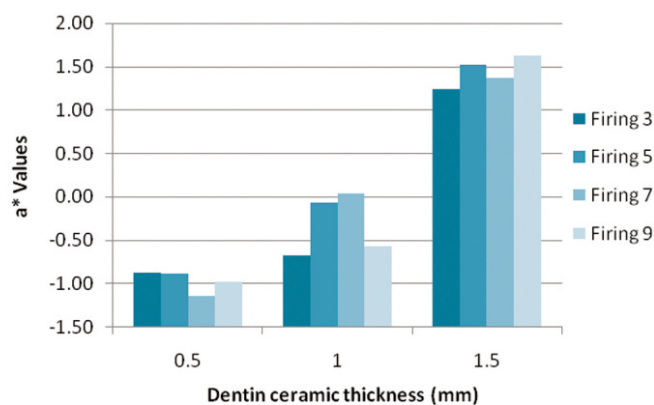


Fig. 2. Means of a\* for number of firings and dentin ceramic thicknesses.

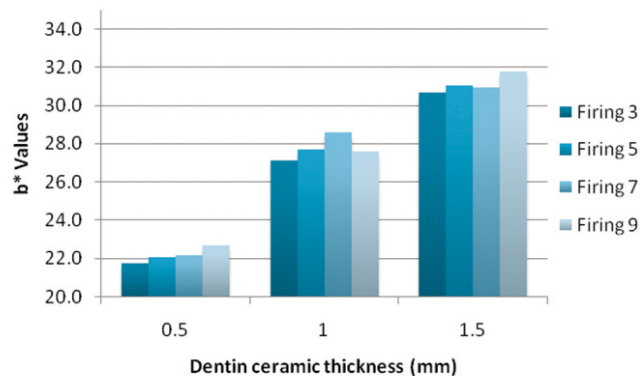


Fig. 3. Means of b\* for number of firings and dentin ceramic thicknesses.

Table 2. Mean ΔE\*ab values (SD) of Lava™ all ceramic specimens with different thicknesses

Number of firings	Mean ΔE (SD)		
	0.5 mm	1 mm	1.5 mm
3 - 5	1.10 (0.57)	1.44 (0.46)	1.61 (1.47)
3 - 7	1.00 (0.42)	2.19 (0.89)	1.68 (1.40)
3 - 9	1.59 (0.44)	0.78 (0.33)	1.97 (1.06)
5 - 7	0.75 (0.26)	1.19 (0.75)	1.13 (0.35)
5 - 9	0.82 (0.42)	1.11 (0.44)	1.25 (0.47)
7 - 9	0.99 (0.44)	1.64 (0.74)	2.04 (0.16)

## DISCUSSION

This *in vitro* study measured the color changes of ceramic specimens prepared at different thicknesses and fired different numbers of times. The results of this study support the hypothesis that the color difference varies with respect to the firing times and dentin ceramic thicknesses. There were significant differences in color change within groups.

Most all ceramic systems consist of a ceramic core with a thickness of 0.5 to 1.0 mm and approximately 1.0 to 1.5 mm of space available for veneering ceramic.<sup>16</sup> In the current study, the specimens had ceramic thicknesses of 0.5, 1, or 1.5 mm, with a core thickness of 1 mm. L\* values, which reflect the brightness of the specimens, decreased for both systems as the total thickness of the specimens increased. Antonson and Anusavice<sup>22</sup> studied the effect of change in the thickness of ceramics on the contrast ratio of dental core and veneering ceramic, and concluded that the contrast ratio was dependent on the type of the material tested. Heffernan *et al.*<sup>10,16</sup> described the influence of core material thickness on its translucency and the influence of core plus ceramic veneer thickness on the overall translucency of specimens. Shokry *et al.*<sup>29</sup> demonstrated that L\* values decreased for leucite reinforced and spinell ceramics as

the total thickness increased. The results of the present study are in agreement with the previous studies<sup>12,29,31,36,37</sup> since the thickness of the layered ceramic influenced the final shade, partially due to the translucency, as the thicker ceramic disks were less translucent.

As the dentin ceramic thickness increased, significant reductions in L\* values were recorded. There were significant increases in both a\* and b\* values as the dentin ceramic thickness increased. These changes in L\*, a\* and b\* values are consistent with a study by Ozturk *et al.*<sup>37</sup>. An increase in the number of firings resulted in an appreciable increase in L\* values that resulted in darker specimens for 0.5 mm and 1.5 mm thicknesses used in the present study. However it decreased for 1 mm thickness specimens. The a\* color values of 1 mm and 1.5 mm thicknesses increased after repeated firings which resulted in redder specimens. However, the a\* values decreased for 0.5 mm thickness specimens. The b\* values increased appreciably by the number of firings in all specimens of 0.5, 1 and 1.5 mm thicknesses. This resulted in yellower specimens.

The mean ΔE values increased as the dentin ceramic thickness was increased. The ΔE value was smaller than 1 between firing 5 and 7, firing 5 and 9 and firing 7 and 9 for 0.5 mm thickness and between firing 3 and 9 for 1 mm thickness. The ΔE value was higher than 1 between all firings for 1.5 mm specimens. Color changes following repeated firings may also be attributed to the color stability of metal oxides during firing which can affect the resulting color of ceramic. Several studies have suggested that certain metal oxides are not color stable after they are subjected to firing temperatures, and color changes of surface colorants after firing have demonstrated pigment breakdown at firing temperatures.<sup>39-41</sup>

In the current study, mean color differences caused by various dentin thicknesses and repeated firings were below 3.7 ΔE units, which is rated as a match in the oral environment.<sup>23,24</sup> Ceramic systems in the present study exhibited visual color changes during firing and demonstrated that changes in the thick-

ness and repeated firings of ceramic have an effect on the final shade.

The results of this study suggest that dentin ceramic thickness and the number of firings of the all ceramic system tested significantly affect the final color of the all ceramic restorations. These are important factors for the definitive color of the restoration, and should be considered during shade selection and fabrication. The limitations of this study include the *in vitro* use of a spectrophotometer to evaluate shade differences of only 1 type of all ceramic material. Furthermore, the specimens were disc shaped rather than shaped like crowns. Further study of the clinical implications of the color and translucency of consistent layers for all ceramic restorations, such as core and veneer ceramics, luting cements, and abutment, on the final shade of restorations after repeated firings, should be performed.

## CONCLUSION

Within the limitations of this *in vitro* study, the following conclusions were drawn:

1. The number of firings and dentin ceramic thickness have a definite effect on the final color of all ceramic system tested and these factors should be considered during shade selection and fabrication of the restoration.
2. As the ceramic thickness increased, significant reductions in L\* values and significant increases in both a\* and b\* values were recorded. This resulted in darker, redder and yellow lower specimens.
3. The mean  $\Delta E$  value increased as the dentin ceramic thicknesses increased for zirconium oxide based all-ceramic specimens tested. However, the mean  $\Delta E$  values were less than 3.7  $\Delta E$  units which is rated as a match in the oral environment.

## REFERENCES

1. Piconi C, Maccauro G. Zirconia as a ceramic biomaterial. *Biomaterials* 1999;20:1-25.
2. Meyenberg KH, Lüthy H, Schärer P. Zirconia posts: a new all-ceramic concept for nonvital abutment teeth. *J Esthet Dent* 1995;7:73-80.
3. Derand T, Molin M, Kvam K. Bond strength of composite luting cement to zirconia ceramic surfaces. *Dent Mater* 2005;21:1158-62.
4. Wohlwend A, Studer S, Schärer P. The zirconium oxide abutment: an all-ceramic abutment for the esthetic improvement of implant superstructures. *Quintessence Dent Technol* 1997;1:63-74.
5. Keith O, Kusy RP, Whitley JQ. Zirconia brackets: an evaluation of morphology and coefficients of friction. *Am J Orthod Dentofacial Orthop* 1994;106:605-14.
6. Christel P, Meunier A, Heller M, Torre JP, Peille CN. Mechanical properties and short-term in-vivo evaluation of yttrium-oxide-partially-stabilized zirconia. *J Biomed Mater Res* 1989;23:45-61.
7. Luthardt RG, Sandkuhl O, Reitz B. Zirconia-TZP and alumina-advanced technologies for the manufacturing of single crowns. *Eur J Prosthodont Restor Dent* 1999;7:113-9.
8. Seghi RR, Johnston WM, O'Brien WJ. Spectrophotometric analysis of color differences between porcelain systems. *J Prosthet Dent* 1986;56:35-40.
9. Judd DB, Wyszecki G. *Color in business, science and industry*. 3<sup>rd</sup> ed. New York; John Wiley & Sons; 1975. p. 105-22.
10. Heffernan MJ, Aquilino SA, Diaz-Arnold AM, Haselton DR, Stanford CM, Vargas MA. Relative translucency of six all-ceramic systems. Part II: core and veneer materials. *J Prosthet Dent* 2002;88:10-5.
11. Isgro G, Pallav P, van der Zel JM, Feilzer AJ. The influence of the veneering porcelain and different surface treatments on the biaxial flexural strength of a heat-pressed ceramic. *J Prosthet Dent* 2003;90:465-73.
12. Dozić A, Kleverlaan CJ, Meegdes M, van der Zel J, Feilzer AJ. The influence of porcelain layer thickness on the final shade of ceramic restorations. *J Prosthet Dent* 2003;90:563-70.
13. Mclean JW. *New dental ceramics and esthetics*. *J Esthet Dent* 1995;7:141-9.
14. Wee AG, Monaghan P, Johnston WM. Variation in color between intended matched shade and fabricated shade of dental porcelain. *J Prosthet Dent* 2002;87:657-66.
15. Kingery WD, Bowen HK, Uhlmann DR. *Introduction to ceramics*. 2<sup>nd</sup> ed. New York; John Wiley & Sons; 1976. p. 646-89.
16. Heffernan MJ, Aquilino SA, Diaz-Arnold AM, Haselton DR, Stanford CM, Vargas MA. Relative translucency of six all-ceramic systems. Part I: core materials. *J Prosthet Dent* 2002;88:4-9.
17. Kelly JR, Nishimura I, Campbell SD. *Ceramics in dentistry: historical roots and current perspectives*. *J Prosthet Dent* 1996;75:18-32.
18. Seghi RR, Sorensen JA. Relative flexural strength of six new ceramic materials. *Int J Prosthodont* 1995;8:239-46.
19. Wagner WC, Chu TM. Biaxial flexural strength and indentation fracture toughness of three new dental core ceramics. *J Prosthet Dent* 1996;76:140-4.
20. Giordano RA. Dental ceramic restorative systems. *Compend Contin Educ Dent* 1996;17:779-82, 784-6.
21. CIE (Commission Internationale de l'Éclairage). *Colorimetry-technical report*. 3rd ed. Vienna: Bureau Central de la CIE. CIE Publication No. 15; 2004.
22. Seghi RR, Hewlett ER, Kim J. Visual and instrumental colorimetric assessments of small color differences on translucent dental porcelain. *J Dent Res* 1989;68:1760-4.
23. Johnston WM, Kao EC. Assessment of appearance match by visual observation and clinical colorimetry. *J Dent Res* 1989;68:819-22.
24. Ruyter IE, Nilner K, Moller B. Color stability of dental composite resin materials for crown and bridge veneers. *Dent Mater* 1987;3:246-51.
25. O'Brien WJ, Kay KS, Boenke KM, Groh CL. Sources of color variation on firing porcelain. *Dent Mater* 1991;7:170-3.
26. Hammad IA, Stein RS. A qualitative study for the bond and color of ceramometals. Part II. *J Prosthet Dent* 1991;65:169-79.
27. Jacobs SH, Goodacre CJ, Moore BK, Dykema RW. Effect of porcelain thickness and type of metal-ceramic alloy on color. *J Prosthet Dent* 1987;57:138-45.
28. Barghi N, Lorenzana RE. Optimum thickness of opaque and body porcelain. *J Prosthet Dent* 1982;48:429-31.
29. Shokry TE, Shen C, Elhosary MM, Elkhodary AM. Effect of core and veneer thicknesses on the color parameters of two all-ceramic systems. *J Prosthet Dent* 2006;95:124-9.
30. Jorgenson MW, Goodkind RJ. Spectrophotometric study of five porcelain shades relative to the dimensions of color, porcelain thickness, and repeated firings. *J Prosthet Dent* 1979;42:96-105.
31. Douglas RD, Przybylska M. Predicting porcelain thickness

- required for dental shade matches. *J Prosthet Dent* 1999;82:143-9.
32. Antonson SA, Anusavice KJ. Contrast ratio of veneering and core ceramics as a function of thickness. *Int J Prosthodont* 2001;14: 316-20.
  33. Lee YK, Cha HS, Ahn JS. Layered color of all-ceramic core and veneer ceramics. *J Prosthet Dent* 2007;97:279-86.
  34. Barghi N, Goldberg. Porcelain shade stability after repeated firing. *J Prosthet Dent* 1977;37:173-5.
  35. Barghi N, Richardson JT. A study of various factors influencing shade of bonded porcelain. *J Prosthet Dent* 1978;39:282-4.
  36. Uludag B, Usumez A, Sahin V, Eser K, Ercoban E. The effect of ceramic thickness and number of firings on the color of ceramic systems: an in vitro study. *J Prosthet Dent* 2007;97: 25-31.
  37. Ozturk O, Uludag B, Usumez A, Sahin V, Celik G. The effect of ceramic thickness and number of firings on the color of two all-ceramic systems. *J Prosthet Dent* 2008;100:99-106.
  38. Knispel G. Factors affecting the process of color matching restorative materials to natural teeth. *Quintessence Int* 1991;22: 525-31.
  39. Crispin BJ, Seghi RR, Globe H. Effect of different metal ceramic alloys on the color of opaque and dentin porcelain. *J Prosthet Dent* 1991;65:351-6.
  40. Mulla FA, Weiner S. Effects of temperature on color stability of porcelain stains. *J Prosthet Dent* 1991;65:507-12.
  41. Lund PS, Piotrowski TJ. Color changes of porcelain surface colorants resulting from firing. *Int J Prosthodont* 1992;5:22-7.