

An Aptamer-Based Biosensor for Colorimetric Detection of *Escherichia coli* O157:H7

Wenhe Wu¹*, Jie Zhang¹*, Meiqin Zheng²*, Yuhong Zhong¹, Jie Yang¹, Yuhong Zhao¹, Wenping Wu¹, Wei Ye¹, Jie Wen¹, Qi Wang³*, Jianxin Lu¹*

1 Key Laboratory of Laboratory Medicine, Ministry of Education, Zhejiang Provincial Key Laboratory of Medical Genetics, Wenzhou Medical College, Wenzhou, Zhejiang, People's Republic of China, **2** Department of Clinical Laboratory Medicine, The Affiliated Eye Hospital of Wenzhou Medical College, Wenzhou, People's Republic of China, **3** Department of Respiratory Medicine, The Second Hospital Affiliated to Dalian Medical University, Dalian, People's Republic of China

Abstract

Background: An aptamer based biosensor (aptasensor) was developed and evaluated for rapid colorimetric detection of *Escherichia coli* (*E. coli*) O157:H7.

Methodology/Principal Findings: The aptasensor was assembled by modifying the truncated lipopolysaccharides (LPS)-binding aptamer on the surface of nanoscale polydiacetylene (PDA) vesicle using peptide bonding between the carboxyl group of the vesicle and the amine group of the aptamer. Molecular recognition between *E. coli* O157:H7 and aptamer at the interface of the vesicle lead to blue-red transition of PDA which was readily visible to the naked eyes and could be quantified by colorimetric responses (CR). Confocal laser scanning microscope (CLSM) and transmission electron microscopy (TEM) was used to confirm the specific interactions between the truncated aptamer and *E. coli* O157:H7. The aptasensor could detect cellular concentrations in a range of $10^4 \sim 10^8$ colony-forming units (CFU)/ml within 2 hours and its specificity was 100% for detection of *E. coli* O157:H7. Compared with the standard culture method, the correspondent rate was 98.5% for the detection of *E. coli* O157:H7 on 203 clinical fecal specimens with our aptasensor.

Conclusions: The new aptasensor represents a significant advancement in detection capabilities based on the combination of nucleic acid aptamer with PDA vesicle, and offers a specific and convenient screening method for the detection of pathogenic bacteria. This technic could also be applied in areas from clinical analysis to biological terrorism defense, especially in low-resource settings.

Citation: Wu W, Zhang J, Zheng M, Zhong Y, Yang J, et al. (2012) An Aptamer-Based Biosensor for Colorimetric Detection of *Escherichia coli* O157:H7. PLoS ONE 7(11): e48999. doi:10.1371/journal.pone.0048999

Editor: Richard C. Willson, University of Houston, United States of America

Received: May 15, 2012; **Accepted:** October 3, 2012; **Published:** November 7, 2012

Copyright: © 2012 Wu et al. This is an open-access article distributed under the terms of the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original author and source are credited.

Funding: This study was supported by National Science and Technology Major Project of China (2008ZX10003-003), the National High Technology Research and Development Program of China (863) (2007AA022008), Zhejiang Provincial Program for the Cultivation of High-level Innovative Health talents and Key Laboratory of Laboratory Medicine, Ministry of Education, Key Science and Technology Innovation Team of Zhejiang (2010R50048), Major Project of Wenzhou Science and Technology Foundation (Y20080080). The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Competing Interests: The authors have declared that no competing interests exist.

* E-mail: wqdmu@yahoo.com.cn (QW); jxlu313@163.com (JXL)

† These authors contributed equally to this work.

Introduction

In recent years, outbreaks of foodborne diseases associated with pathogenic *Escherichia coli* (*E. coli*) have been widely spread and grown as *public health problems*. Most of what we know about pathogenic *E. coli* comes from the outbreak studies of *E. coli* O157:H7 infection, which was first identified as a pathogen in 1982 [1]. According to the Centers for Disease Control and Prevention (CDC), *E. coli* O157:H7 infections accounted for 32 outbreaks between 2003 and 2008 in United States [2] including large outbreaks related to contaminated spinach, iceberg and romaine lettuce [3,4]. The *E. coli* O157:H7 is a specific serotype of *E. coli*, which can cause watery diarrhea, hemorrhagic colitis, hemolytic-uremia syndrome (HUS) and thrombotic thrombocytopenic purpura (TTP), especially in young children and the elderly. The conventional assays to detect *E. coli* O157:H7 are specimen culture and colony counting which are sensitive and selective enough. But, these methods are labor intensive, time consuming

(requiring 5 to 7 days) and professional operation limited. Many types of *E. coli* O157:H7 rapid detection tests have been developed during the last decades, involving nucleic acid-based polymerase chain reaction (PCR) technology [5,6], enzyme-linked immunosorbent assay (ELISA) [7] and immunomagnetic separation method [8] and microarray technology [9]. However, PCR-based assay and microarray technology has high risk of false result owing to inhibition by components of the sample matrix, and ELISA requires extra labeled antibodies, while immunomagnetic separation method often requires a combination of other methods.

Various kinds of biosensors have been also developed to detect the *E. coli* O157:H7, including microarray biosensor [10,11], immunosensor [12,13], surface plasmon resonance (SPR) biosensor [14,15], waveguide biosensor [16] and so on. But these test results can not be easily seen by naked eyes due to professional instrument and operation limited. Additionally, *the antibody disadvantages associated with their production, stability and cross-*

reaction have prompted us to seek alternatives of molecular recognition component. Other biosensors, which are based on oligonucleotide [17], have been also proposed. But they often require short enrichment or DNA extraction. Thus, the developments of improved and easy methods are emergent, especially those primary screening tests of the outbreak of the foodborne diseases.

Due to their unique optical properties, polydiacetylene (PDA) and its derivatives have been widely exploited for biosensing applications [18,19]. Our research group and others [20,21] have found that diacetylenes could undergo polymerization via 1, 4-addition reaction and form alternating eneyne polymer chains by ultraviolet (UV) irradiation at room temperature. The resulting polymer showed a maximum absorbance around 640 nm (blue form) in the visible region of the spectrum. Particularly, the maximum absorbance changed from 640 nm to 540 nm and the color changed through violet from blue to red in response to external stimuli, such as temperature [22], pH change [23], surface pressure [24] and molecular recognition [25,26].

Nucleic acid aptamers are relatively short single-stranded DNA or RNA oligonucleotides that have been engineered through repeated rounds of *in vitro* selection referred to as systematic evolution of ligands by exponential enrichment (SELEX) [27,28]. They are created to bind to specific targets such as small molecules, proteins, nucleic acids, and even cells, tissues and organisms [29]. Owing to their *in vitro* selection, high affinity and specificity, aptamers are beginning to emerge as new molecular recognition components that rival antibodies in biosensing applications [30].

In this paper, an aptamer based biosensor (aptasensor) was developed and evaluated for rapid colorimetric detection of *E. coli* O157:H7. 10, 12-pentacosadiynoic acid (PCDA), one of the well-known diacetylene monomers, was used to prepare PDA vesicles. It consists of hydrophilic head group and hydrophobic tail, can be easily self-assembled into vesicles in solution. The free carboxyl of nanoscale PDA vesicle was activated with N-hydroxysuccinimide (NHS) and 1-Ethyl-3-(3-dimethylaminopropyl)carbodiimide (EDC), and formed reactive intermediate. The aptasensor was obtained by modifying the truncated 5'-amino-aptamer on the surface of nanoscale PDA vesicle using peptide bonding between the carboxyl group of the vesicle and the amine group of the aptamer (Figure 1). Molecular recognition between *E. coli* O157:H7 and aptamer at the interface of the vesicle lead to blue-red transition of PDA vesicle which was readily visible to the naked eyes and could be quantified by colorimetric responses (CR).

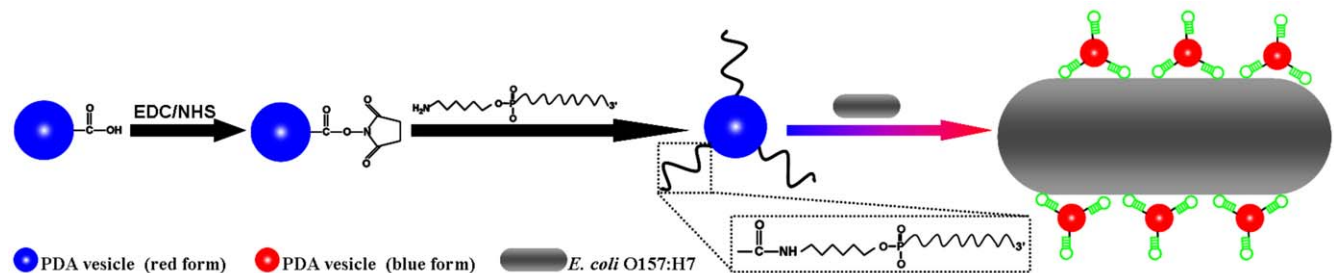


Figure 1. Principle of *E. coli* O157:H7 detection using aptasensor.
doi:10.1371/journal.pone.0048999.g001

Results and Discussion

Aptamers Modified and Conjugation

Unpolymerized vesicles were made by using PCDA, DMPC/PCDA or LPS/DMPC/PCDA in the dark room. Then the PDA vesicles were polymerized via 1, 4-addition reaction to form alternating polymer chains under UV light irradiation at 254 nm. The resulting polymers appeared deeply blue which is directly visible to the unaided eye and can be characterized by the UV-vis spectrum showing an absorption peak at 640 nm (Figure 2, blue curve). After binding the aptamers (E17F-37 and E18R-42) to the PDA vesicles, the absorption peak at 640 nm did not change, and an additional absorption peak appeared at 260 nm (characteristic absorption peak of the nucleotide), which meant that the aptamers had been modified to PDA vesicles (Figure 2, black and red curve). By detecting the optical absorbance of the samples at 260 nm before and after dialysis, the efficiency of conjugation was about 85%. It was estimated that aptamer conjugated on pure PCDA vesicle of 50 nmol (18.73 mg) could reach 4.25 nmol. The pure PCDA vesicles, aptamer/PCDA vesicles, DMPC/PCDA vesicles and LPS/DMPC/PCDA vesicles, confirmed by transmission electron microscopy (TEM), were produced successfully. Four kinds of PDA vesicles appeared to be nearly monodispersed, with diameters of 30–100 nm (shown in Figure S1).

CLSM Images of Affinity Tests

To address the effect of affinity between aptamers and *E. coli* O157:H7, we prepared fluorescein isothiocyanate (FITC) labeled

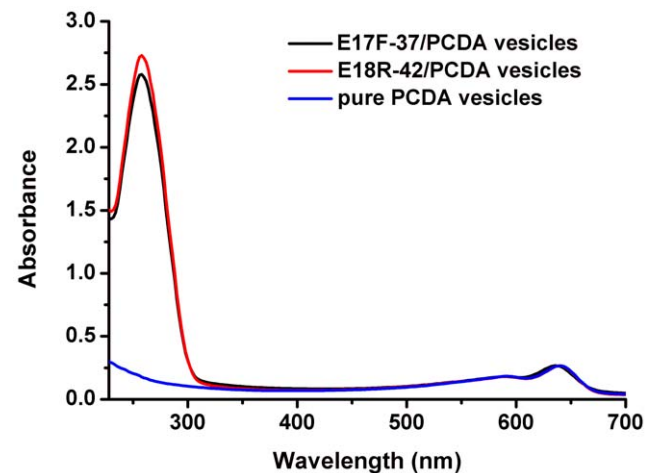


Figure 2. UV-vis absorbance spectra of pure PCDA vesicles before (blue curve) and after binding aptamers (red and black curve).

doi:10.1371/journal.pone.0048999.g002

aptamers before and after truncated. Positive controls were investigated with FITC labeled E17F-72 (or E18R-72) instead of FITC labeled E17F-37 (or E18R-42). Further, *Salmonella typhimurium* was used instead of *E. coli* O157:H7 in the experiment as negative controls. Figure S2a, b, d and e shows representative CLSM images of *E. coli* O157:H7 after incubating of FITC labeled E17F-37, E18R-42, E17F-72 and E18R-72 separately. Green fluorescence was detected on *E. coli* O157:H7 with all four kinds of FITC labeled aptamers. It was well known that the recognition and binding between the aptamers and target molecules were depended on their structures, like the interactions between antigen and antibody, the results also might indicate that the aptamers before and after truncated had the same loops structures and similar functions. Moreover, no green fluorescence was detected on *Salmonella typhimurium* with FITC labeled E17F-37, E18R-42 (Figure S2c and f). It provided preliminary evidence of specificity of aptamers after truncated.

TEM Images of Affinity Tests

In order to elucidate the mechanism behind the aptasensors in recognition, we generated the LPS/DMPC/PCDA vesicles to simulate the *E. coli* O157:H7. Because of high hydrophobicity of the lipid A in LPS, LPS could insert into vesicles easily by the hydrophobic interaction between DMPC and lipid A, leaving the polysaccharide free on the surface of vesicles. The aptamer/PCDA vesicles were added to the LPS/DMPC/PCDA vesicles and the DMPC/PCDA vesicles, the results were observed by TEM. As shown in Figure 3, after adding the aptamer/PCDA vesicles to the DMPC/PCDA vesicles, we observed that all the aptasensors were spherical in shape with an approximate diameter of less than 100 nm, with no change in the morphology and being separated well. However, after adding the aptamer/PCDA vesicles to the LPS/DMPC/PCDA vesicles, there were dramatic changes in their morphology, leading to the formation of aggregate clusters with size that over 100 nm. These results also confirmed that the aptasensors could specifically recognize the LPS of *E. coli* O157:H7, suggesting that the aptasensors might respond to LPS in *E. coli* O157:H7 and could be used for detecting *Escherichia coli* as well.

Colorimetric Detection of *E. coli* O157:H7 with the Aptasensor

The aptasensors appeared deeply blue and showed an absorption maximum at 640 nm. After being incubated with *E. coli* O157:H7 solution ($50 \mu\text{l}$ 10^8 colony-forming units (CFU)/ml) at 37°C temperature under stirring, the color of aptasensors turned from deeply blue to red, which could be easily seen by naked eyes. In contrast to pure PCDA vesicles (Figure 4, blue curve) and random/PCDA vesicles (Figure 4, green curve), the absorption maximum shifted from 640 to 540 nm, and a new absorption (500 nm) appeared after the aptasensors (E17F-37/PCDA vesicles, E18R-42/PCDA vesicles) were exposed to *E. coli* O157:H7 (Figure 4, black curve and red curve). All this indicated that the color changes might be caused by the reaction between aptamers and *E. coli* O157:H7. In order to further validate whether the color change was resulted from the conjugation of the aptasensor and the bacterium, we added the *E. coli* O157:H7 with a concentration of 10^7 CFU/ml to the aptasensors (E17F-37/PCDA vesicles, E18R-42/PCDA vesicles) and pure PCDA vesicles, and drew the CR%-time curve. As shown in Figure 5, as the time went on, the CR% values gradually increased. Both aptasensors reacted with bacteria quickly (Figure 5, black curve and red curve). In 15 minutes, both CR%s were almost 15%, and reached saturation in almost 120 min. However, for the control

(Figure 5, blue curve), no color change was observed by naked eye and the CR% was less than 7%. Thus, these results suggested that the color changes were resulted from the reaction between aptamers and *E. coli* O157:H7.

Sensitivity Analysis and Linear Range

To quantify the sensitivity of the aptasensors, we challenged with an increasing concentration of bacteria and generated a calibration curve. As shown in Figure 6, when the concentration of bacteria increased, the value of CR% enhanced as well, which meant, with the increasing of the concentration of bacteria, the tendency of the color changed from blue to red, and the CR% increased gradually.

Also, a good linear relationship was shown when the concentrations of bacteria was in the range of $10^4 \sim 10^8$ CFU/ml. Figure 6 (A) showed the linear equation for the reaction between the E17F-42/PCDA vesicles and the *E. coli* O157:H7 was $Y = 6.0163X - 10.5468$ ($R^2 = 0.99087$), the detect limitation was 10^4 CFU/ml (three times the standard deviation of blank). The Figure 6 (B) showed the linear equation for the reaction between the E18R-42/PCDA vesicles and the *E. coli* O157:H7: the linear equation was $Y = 6.1055X - 13.8503$ ($R^2 = 0.98982$) and the detect limitation was 10^4 CFU/ml too. These detection limits were 10^4 -fold lower than previously reported PDA-based approach [31] and 10^2 -fold lower [12] than or comparable [11,15] to the presently available immunosensor (see performance comparison in Table 1).

Specificity Analysis

The recognition of aptamer to target molecule was highly specific which could identify the target accurately from similar molecules with subtle difference. In order to confirm that the color shift was specifically caused by *E. coli* O157:H7, the aptasensors were challenged with other types of bacteria including *E. coli* (ATCC 25922, CMCC44825, CMCC44155, CMCC44151), *Salmonella typhimurium*, *Salmonella typhi*, *Salmonella paratyphi* A, *Salmonella paratyphi* B, *Shigella sonnei*, *Shigella flexneri*, *Proteus vulgaris*, *Enterobacter aerogenes*, *Citrobacter freundii*, *Staphylococcus aureus* and *Monilia albican*.

E. coli O157:H7 was diluted to the concentration of 10^7 CFU/ml while other bacteria were diluted to the concentration of 10^8 CFU/ml by deionized water, and then be incubated with aptasensors for 2 hours. The values of CR%s were calculated as previously mentioned. As shown in Figure 7, only the *E. coli* O157:H7 could be recognized by the aptasensors, which means our biosensors could only specially detect the *E. coli* O157:H7. Importantly, this selectivity can be visualized with the naked eye.

Indeed, only the aptasensors containing *E. coli* O157:H7 were red, whereas all others (10-fold higher than *E. coli* O157:H7) have remained blue. This clearly illustrated that the aptasensors was only specific to the *E. coli* O157:H7 and did not respond to the wide range of background bacteria even to other *E. coli*.

Detection of *E. coli* O157:H7 in Fecal Samples

The 100 fecal samples artificially contaminated were exposed to E18R-42/PCDA vesicles and pure PCDA vesicles for 2 hours. As shown in Figure 8, group A (E18R-42/PCDA vesicles with artificially contaminated fecal samples) produced 3 times the CR% of group B (E18R-42/PCDA vesicles with uncontaminated fecal samples) and group C (pure PCDA vesicles with artificially contaminated fecal samples). The CR%s difference between these groups demonstrated that this sensor could determine *E. coli* O157:H7 in artificially contaminated fecal samples and it is feasible to separate *E. coli* O157:H7 as pretreatment process.

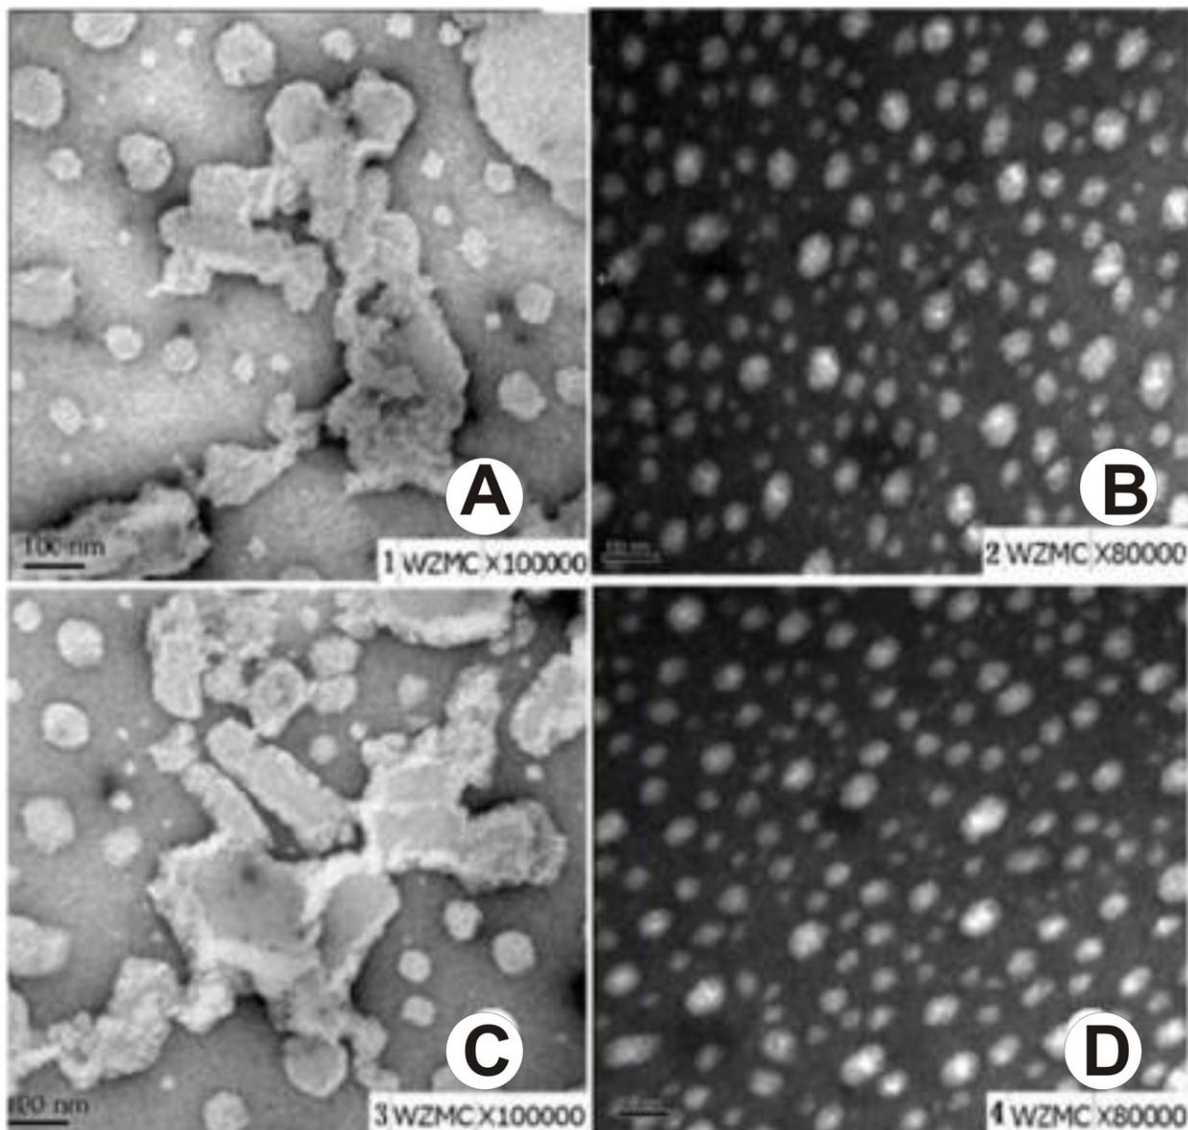


Figure 3. Negative-stained TEM images. (A) E17F-37/PCDA vesicles with LPS/DMPC/PCDA. (B) E17F-37/PCDA vesicles with DMPC/PCDA. (C) E18R-42/PCDA vesicles with LPS/DMPC/PCDA. (D) E18R-42/PCDA vesicles with DMPC/PCDA. Scale bar is 100 nm. doi:10.1371/journal.pone.0048999.g003

However, the pretreatment process inevitably decreased the concentration of *E. coli* O157:H7 and the CR% of group A were less than those of E18R-42/PCDA vesicles with *E. coli* O157:H7 (10^8 CFU/ml). Furthermore, in order to quantitatively compare the difference responses of E18R-42/PCDA vesicles to the artificially contaminated and uncontaminated fecal samples, a Student's t-test was conducted. Based on Figure 8, the responses of the E18R-42/PCDA vesicles to the 100 artificially contaminated and uncontaminated fecal samples showed a statistically significant difference.

In addition, the clinical fecal specimens ($n = 203$) were tested for detecting *E. coli* O157:H7 by standard culture method and our E18R-42/PCDA vesicles. Samples were deemed to be aptasensor – positive if CR% were equal or greater than 10%. All samples resulted in 98.5% (200 to 203) agreement of *E. coli* O157:H7 detection between standard culture method and our E18R-42/PCDA vesicles. The agreement rate was the proportion of all samples diagnosed correctly by E18R-42/PCDA vesicles. It was

computed from the proportion diagnosed correctly by E18R-42/PCDA vesicles of the fourfold table given in Table 2. Chi-square test indicated that, there was no statistically significant difference ($p > 0.05$) for the detection of *E. coli* O157:H7 with the standard culture method and our E18R-42/PCDA vesicles. It was thus clear that our aptasensor was feasible and reliable for primary screening *E. coli* O157:H7 in clinical fecal samples.

In conclusion, we present a new aptasensor for rapid colorimetric detection of *E. coli* O157:H7. Through the experimental evidence, the mechanism behind the color change via TEM were elucidated. All these meant the aptasensor acted as both the molecular recognition element and the signal transducer element of the biosensor. This direct *E. coli* O157:H7 detection methodology relied on unique properties of PDA and aptamer, offers advantages rather than the conventional *E. coli* O157:H7 detection assays or other rapid detection methods. First, PDA vesicles and aptamers can be readily synthesized chemically with large quantities. Second, the aptasensor exhibits high specificity

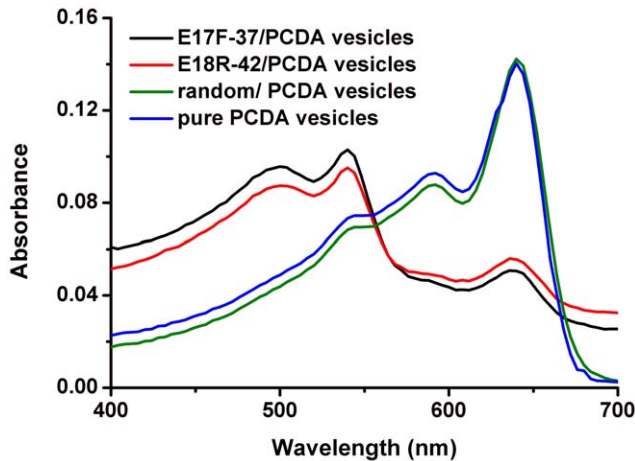


Figure 4. Representative spectrum for *E. coli* O157:H7 (10^8 CFU/ml) in presence of E17F-37/PCDA vesicles (black curve), E18R-42/PCDA vesicles (red curve), random/PCDA vesicles (green curve) and pure PCDA vesicles (blue curve).
doi:10.1371/journal.pone.0048999.g004

since aptamers could form complex secondary and tertiary structure for *E. coli* O157:H7. Also, the truncating on aptamers can cause them to increase their affinity to *E. coli* O157:H7 and reduce the cost for assays. Third, the assay took only 2 hours in time and 50 μ l in volume, which saved time and volume and was very important especially at the time of encountering the wide spread of the disease. Last, by using this novel sensor, the results could be read by naked eye and not require any power or instrumentation. We expect that the aptasensor presented here provides a promising approach for pathogenic bacteria detection, and this method could be used not only in clinical analysis but also in biological terrorism defense.

Materials and Methods

Apparatus Materials

Bacteria. *E. coli* O157: H7 was purchased from China Center of Industrial Culture Collection. *E. coli* (ATCC25922, CMCC44825, CMCC44155, CMCC44151), *Salmonella typhimurium* (CMCC50115), *Salmonella typhi* (CMCC50071), *Salmonella paratyphi* A (CMCC50433), *Salmonella paratyphi* B (CMCC50004), *Shigella sonnei* (ATCC25931), *Shigella flexneri* (CMCC51571), *Proteus vulgaris* (CMCC49072), *Enterobacter aerogenes* (ATCC 13048), *Citrobacter freundii* (ATCC8090), *Staphylococcus aureus* (ATCC25923) and *Monilia albican* (ATCC14053) were obtained from Wenzhou Medical College.

Reagent. PCDA was purchased from GFS chemicals. (Powell, OH, USA). 1,2-Dimyristoyl-sn-glycero-3-phosphocholine (DMPC), NHS and 1-Ethyl-3-(3-dimethylaminopropyl)carbodiimide, hydrochloride (EDC·HCl) were purchased from Sigma-Aldrich. (St Louis, MO). DNA oligonucleotides modified with amine group or FITC at the 5' end were obtained from Bioneer Co. Ltd. (Shanghai, China). All solvents used in this study were of analytical grade and were prepared by using deionized water of resistivity not less than 18.2 M Ω cm.

Apparatus. PURELAB Classic was purchased from ELGA Lab Water (High Wycombe, UK). Scientz-IID ultrasonic homogenizer and SCIENTZ03-II UV crosslinker were purchased from Ningbo Scientz Biotechnology Co.Ltd. (Ningbo, China). CLSM Fluoview FV1000 was purchased from Olympus (Tokyo, Japan). TEM H-7500 was purchased from Hitachi (Tokyo, Japan).

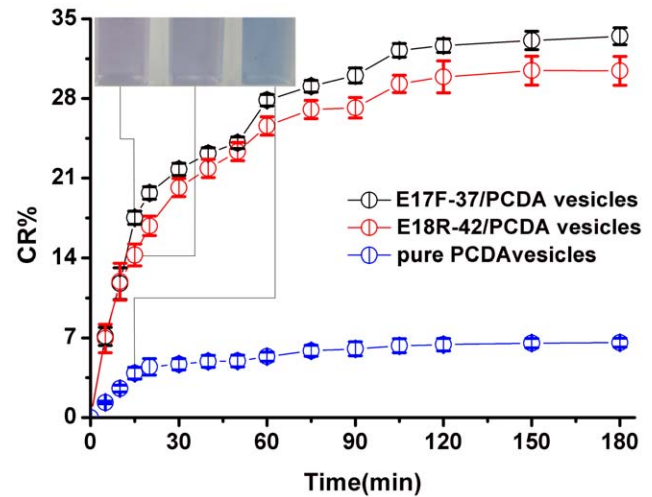


Figure 5. Kinetic study for the CR% change of *E. coli* O157:H7 with E17F-37/PCDA vesicles (black curve), E18R-42/PCDA vesicles (red curve) and pure PCDA vesicles (blue curve). Inset: Visual detection in 15 minutes.
doi:10.1371/journal.pone.0048999.g005

Varioskan Flash spectral scan multimode plate reader was purchased from Thermo Fisher Scientific (Waltham, MA, USA).

PDA Vesicles Preparation and Conjugation

PCDA monomers were dissolved in chloroform and the solvent was removed by purging with nitrogen to generate a thin lipid film on the glass surface, and continued to be dried by vacuum for 2 hours. After adding the deionized water (18.2 M Ω cm) to make the 1 mM lipids, the lipids were sonicated at 72°C for 15 min until it turned clarity. The lipids were cooled in the dark bottle at 4°C overnight. They were polymerized by using UV light irradiation at 254 nm until turning blue, and then the vesicle solution was obtained. The quality of vesicle solution was monitored with Varioskan Flash spectral scan multimode plate reader and TEM. Most of the procedures for preparing LPS/PCDA/DMPC vesicle or PCDA/DMPC vesicle were the same as pure PCDA vesicle's, excepting for replacing the PCDA monomer by a mixture containing PCDA monomer, DMPC and LPS (molar ratios as 6:2: 0.1), or a mixture containing PCDA monomer and DMPC (molar ratios as 6:2) to a total lipid concentration of 1 mM.

The aptamers were conjugated to the pure PCDA vesicles by using the carbodiimide method in the presence of the EDC and the NHS (Figure 1). Briefly, 6.25 μ l of NHS (4 mM), 6.25 μ l of EDC (4 mM) and 50 μ l of pure PCDA (1 mM) vesicle were mixed in 187.5 μ l of deionized water at room temperature. After stirring the mixtures for 2 h to active carboxy, 10 μ l (0.5 mM) DNA (E17F-37, E18R-42 or random DNA) were added into the mixed solution. After incubating the mixtures at the room temperature overnight, the aptamers or random DNA were conjugated to the pure PCDA vesicles. Unbound aptamers were removed by dialysis with excess deionized water. The final volume was adjusted to 0.5 ml by adding deionized water and PCDA concentration was approximately 0.1 mM.

Bacteria Preparation

Bacteria were cultured in the Luria Broth at 37°C overnight, and then washed 3 times with deionized water. Then appropriate 10-fold serial dilutions (10^{-1} , 10^{-2} , 10^{-3} , 10^{-4} , 10^{-5} , 10^{-6} , 10^{-7} and 10^{-8}) of the bacterial suspension were prepared in saline (0.9%). A 0.1 ml of each dilution was spread plated on to Luria

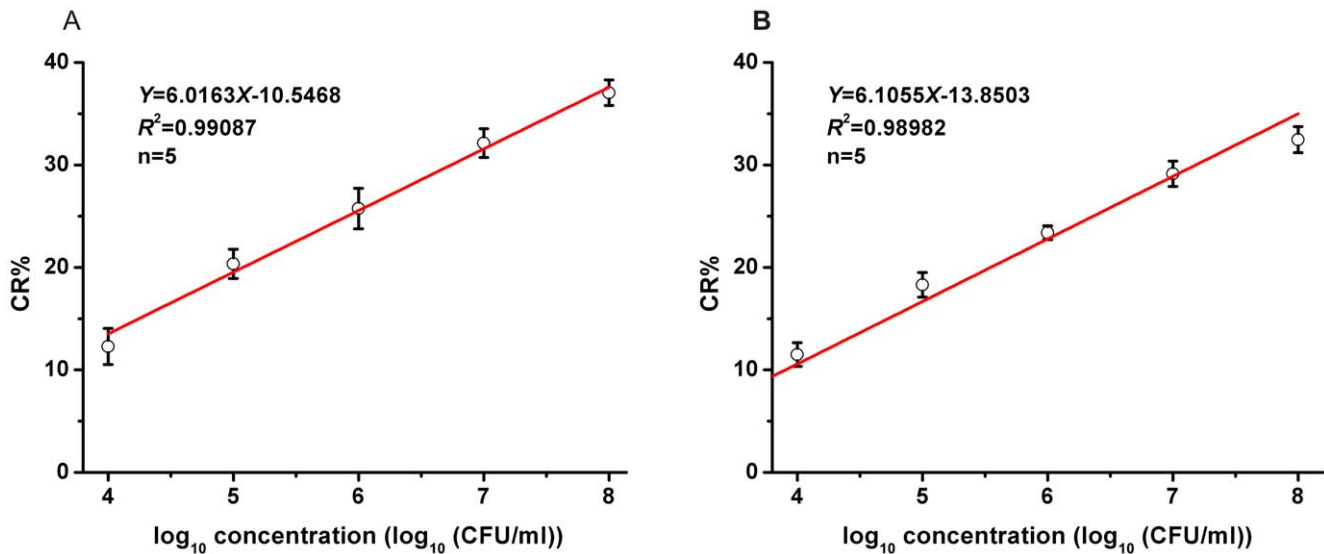


Figure 6. Calibration curve for CR% vs. concentration of *E. coli* O157:H7 using by different PDA vesicles. (A) CR% of E17F-37/PCDA vesicles with *E. coli* O157:H7. (B) CR% of E18R-42/PCDA vesicles with *E. coli* O157:H7. doi:10.1371/journal.pone.0048999.g006

Broth agar plate and the plates were incubated overnight at 37°C for 24 h. Finally, we got the *E. coli* O157:H7 samples of different concentrations from 10^3 to 10^8 CFU/ml via suspending bacteria with different volume deionized water.

LPS-binding Aptamers Truncating and Affinity Test

As shown in table 3, the chosen aptamers were based on the sequences of E17F-72 and E18R-72 which could specifically bind to LPS of the *E. coli* O157:H7 [32]. With the purposes of making the aptamers work better and reducing the cost, the E17F-72 and the E18R-72 were truncated by deleting some sequences to investigate the relationships between structure and function. We finally got two aptamers, named E17F-37 and E18R-42 (Table 3). The sequences of these two pairs were loaded to the software of RNAstructure 4.5 and website of RNAfold to predict the second structures. The results indicated that they have the same loop in the second structures, implying the similar functions of them. CLSM was used to verify this implication. 5 μ l (0.1 mM) different FITC-tagged aptamers (E17F-72, E17F-37, E18R-42 or E18R-72)

were incubated with *E. coli* O157:H7 in the dark bottle at room temperature overnight. Then, the mixtures were purified by centrifugation at 5000 rpm and 3–4 times washes with 1 ml of 10 mM PBS buffer (pH 7.2). The mixtures were redispersed finally in the same buffer (10 μ l) and placed onto a glass slide. After complete drying, the slides covered with coverslips were observed under CLSM equipped with an excitation wavelength of 488 nm and an emission wavelength of 520 nm.

And then, the E17F-37 and the E18R-42 were modified with the amide groups at the 5' region and were used to prepare for the aptamer/PCDA vesicles. We performed the affinity tests to verify the binding sites of the E17F-37 and the E18R-42 by mixing the aptamer/PCDA vesicles to the LPS/DMPC/PCDA vesicles and the DMPC/PCDA vesicles. The DMPC/PCDA vesicles were used as the negative control. The results were observed by transmission electron microscopy (TEM).

Table 1. Performance comparison between biosensors for the Detection of *E. coli* O157:H7.

| Type | LOD (CFU/ml) | Visible to the naked eyes | Enrichment or DNA extraction | Molecular recognition component | Ref |
|---|--------------------------|---------------------------|------------------------------|---------------------------------|-------------------|
| microelectrode array biosensor | 10^7 | No | No | antibody | [10] |
| electrochemical impedance immunosensor | 10^6 | No | No | antibody | [12] |
| SPR immunosensor | 3.0×10^4 | No | No | antibody | [15] |
| Chemiluminescence microarray readout system | 10^4 | No | No | antibody | [11] |
| piezoelectric immunosensor | 10^3 | No | No | antibody | [13] |
| SAM based SPR biosensor | 10^3 | No | No | antibody | [14] |
| waveguide biosensor | 10^3 | No | Yes | antibody | [16] |
| QCM DNA sensor | 2.67×10^2 | No | Yes | oligonucleotide | [17] |
| PDA-based aptasensor | 10^4 | Yes | No | oligonucleotide | This study |

doi:10.1371/journal.pone.0048999.t001

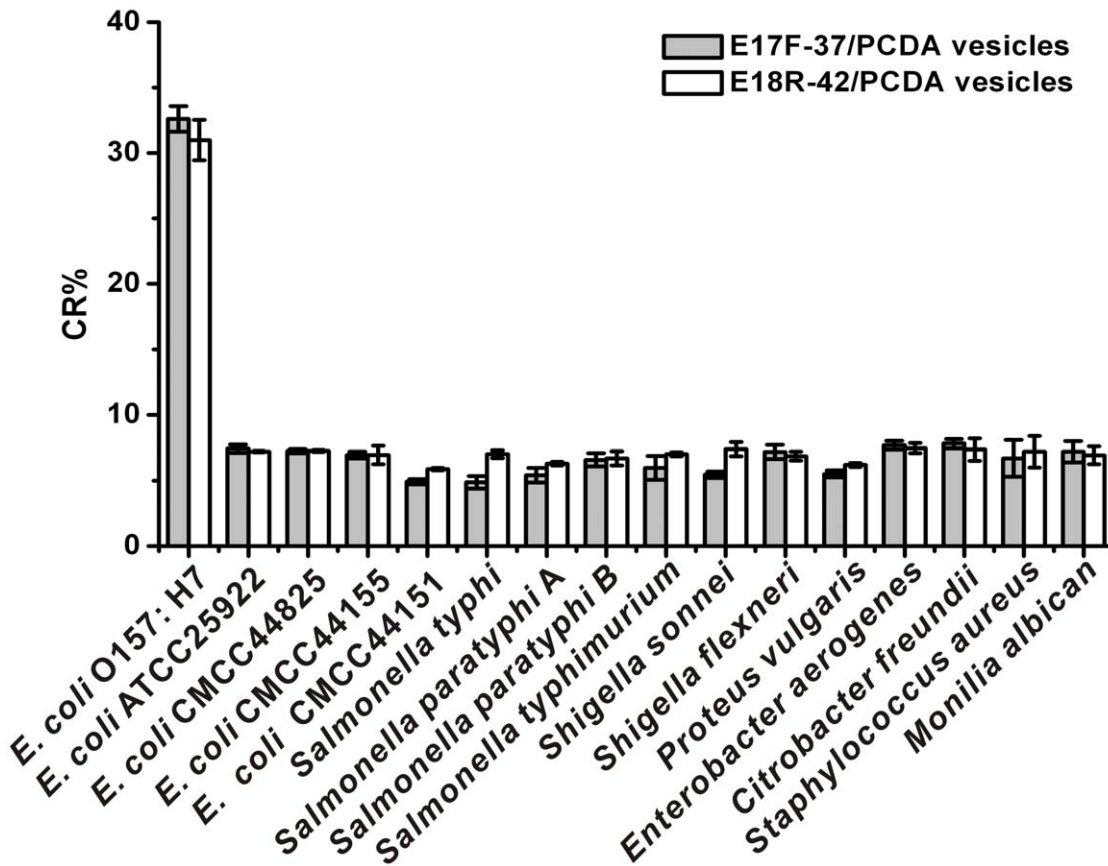


Figure 7. Specificity of aptamer-based biosensor detection *E. coli* O157: H7 (10^7 CFU/ml *E. coli* O157:H7, all other bacteria of 10^8 CFU/ml).
doi:10.1371/journal.pone.0048999.g007

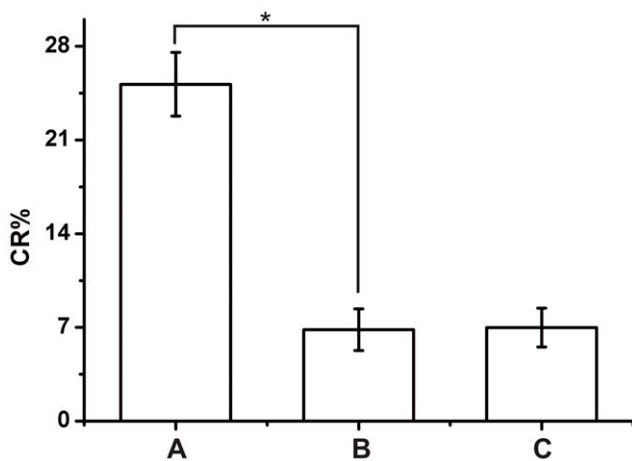


Figure 8. Application of E18R-42/PCDA vesicles in fecal samples contaminated artificially (10^8 CFU/ml initial concentration of *E. coli* O157:H7). (A) CR% of E18R-42/PCDA vesicles with artificially contaminated fecal samples. (B) CR% of E18R-42/PCDA vesicles with uncontaminated fecal samples. (C) CR% of pure PCDA vesicles with artificially contaminated fecal samples. *, $p < 0.05$ by Student's *t* test.
doi:10.1371/journal.pone.0048999.g008

Characteristic Absorption Spectrum of Vesicles

The absorbance was obtained by using the Varioskan Flash spectral scan multimode plate reader from 228 nm to 700 nm at room temperature.

Colorimetric Assays for *E. coli* O157: H7 and Sensitivity Test

Sensitivity test was performed as follows: the aptamer/PCDA vesicles were incubated with various concentrations of *E. coli* O157: H7 (10^3 to 10^8 CFU/ml) at 37°C for 2 hours. Absorbance measurements were performed at different time points using absorption spectroscopy from 400 nm to 700 nm. The aptamers of E17F-37 and E18R-42 automatically folded to capture the *E.*

Table 2. Detection of *E. coli* O157:H7 in fecal samples by aptasensor and standard culture method.

| E18R-42/PCDA vesicles | Standard culture method | | Total |
|-----------------------|-------------------------|-----|-------|
| | + | - | |
| + | 2 | 3 | 5 |
| - | 0 | 198 | 198 |
| Total | 2 | 201 | 203 |

+positive result;
-negative result.

doi:10.1371/journal.pone.0048999.t002

Table 3. The sequence of LPS-binding aptamers and random DNA.

| DNA | Sequences(5'-3') | Length | source |
|---------|--|--------|------------|
| E17F-72 | ATCCGTCACACCTGCTCTATCAAATGTGCAGATATCA AGACGATTGTACAAGATGGTGTGGCTCCCGTAT | 72 bp | [32] |
| E17F-37 | ATCAAATGTGCAGATATCAAGACGATTGTACAAGAT | 37 bp | This study |
| E18R-72 | ATACGGGAGCCAACACCATTCTATCGTTCGGACGCT TATGCCTTGCCATCTACAGAGCAGGTGTGACGGAT | 72 bp | [32] |
| E18R-42 | CCGACGCTTATGCCTTGCCATCTACAGAGCAGGTGT GACGG | 42 bp | This study |
| random | GCCGGCTCAGCATGACTAAGAAGGAAGTTATGTGGTGTGGC | 42 bp | This study |

doi:10.1371/journal.pone.0048999.t003

coli O157:H7, which would change the structure of PCDA backbone, and then induced the color turning blue to red. To quantify the degree of color change, we used the following formula [33,34]: $CR\% = [(PB_0 - PB_f)/PB_0] \times 100\%$. Where the $PB = A_{640\text{ nm}}/(A_{640\text{ nm}} + A_{540\text{ nm}})$; the PB_0 was in the absence of *E. coli* O157:H7, while the PB_f was in the presence of *E. coli* O157:H7. The higher CR% represents more efficient transition from the blue color to the red color. The data of A640 and A540 was collected before and after adding the O157:H7 from at least three independent experiments; the CR% values were then calculated.

Specificity Testing

Specificity test was performed as follows: the aptasensors were used to detect other different bacteria at the concentration of 10^8 CFU/ml but *E. coli* O157:H7 at the concentration of 10^7 CFU/ml. The bacteria were as follows: *E. coli* (ATCC 25922, CMCC44825, CMCC44155, CMCC44151), *Salmonella typhimurium*, *Salmonella typhi*, *Salmonella paratyphi* A, *Salmonella paratyphi* B, *Shigella sonnei*, *Shigella flexneri*, *Proteus vulgaris*, *Enterobacter aerogenes*, *Citrobacter freundii*, *Staphylococcus aureus*, *Monilia albican* and *E. coli* O157: H7.

Detection of *E. coli* O157:H7 in Fecal Samples

The clinical fecal specimens ($n=203$), that were used for detecting *E. coli* O157:H7 by standard culture method and our E18R-42/PCDA vesicles, were from patients from the First Affiliated Hospital of Wenzhou Medical College. For artificially contaminated fecal samples, 1 ml of 10^8 CFU/ml *E. coli* O157:H7 was added to each 1 g of fecal samples ($n=100$) that were culture negative for *E. coli* O157:H7. For uncontaminated fecal samples, 1 ml of 10 mM sterile PBS buffer (pH 7.2) was added to each 1 g of fecal samples ($n=100$) that were culture negative for *E. coli* O157:H7. All three kinds of samples need to be pretreated simply before application of E18R-42/PCDA vesicles. 1 g of fecal

samples was homogenized in 8 ml of 10 mM sterile PBS buffer (pH 7.2) and was centrifuged at 500 rpm for 10 min. Then the supernatant was filtered through a 0.45 μm filtration device. Agitate the filter membrane carefully with 8 ml of sterile water in order to resuspend any bacteria that were caught in the filter membrane. Finally, bacteria were centrifuged at 12000 rpm for 10 min and resuspended in 1 ml of sterile water.

Supporting Information

Figure S1 Negative-stained TEM images of PDA vesicles. (A) pure PCDA vesicles. (B) aptamer/PCDA vesicles. (C) DMPC/PCDA vesicles. (D) LPS/DMPC/PCDA vesicles. Scale bar is 100 nm.

(TIF)

Figure S2 CLSM images of affinity tests. (A) FITC labeled E17F-37 with *E. coli* O157:H7. (B) FITC labeled E18R-42 with *E. coli* O157:H7. (C) FITC labeled E17F-37 with *Salmonella typhimurium*. (D) FITC labeled E17F-72 with *E. coli* O157:H7. (E) FITC labeled E18R-72 with *E. coli* O157:H7. (F) FITC labeled E18R-42 with *Salmonella typhimurium*.

(TIF)

Acknowledgments

We thank Tieli Zhou, Aibing Zeng, Xiaolong Li, Zengqiang Chen and Jinhong Yang for their kind assistance in providing bacterial strains or samples.

Author Contributions

Conceived and designed the experiments: WHW JZ JXL QW. Performed the experiments: MQZ JZ Y. Zhong JY Y. Zhao WPW. Analyzed the data: Y. Zhong JY WPW WY JW. Contributed reagents/materials/analysis tools: JXL. Wrote the paper: WHW JZ QW JXL.

References

- Riley LW, Remis RS, Helgerson SD, McGee HB, Wells JG, et al. (1983) Hemorrhagic Colitis Associated with a Rare *Escherichia coli* Serotype. *N Engl J Med* 308: 681–685.
- CDC (2011) Surveillance for Foodborne Disease Outbreaks - United States, 2008. *Morb Mortal Wkly Rep* 60: 1197–1202.
- Kulasekara BR, Jacobs M, Zhou Y, Wu Z, Sims E, et al. (2009) Analysis of the Genome of the *Escherichia coli* O157:H7 2006 Spinach-Associated Outbreak Isolate Indicates Candidate Genes That May Enhance Virulence. *Infect Immun* 77: 3713–3721.
- Parker CT, Kyle JL, Huynh S, Carter MQ, Brandt MT, et al. (2012) Distinct transcriptional profiles and phenotypes exhibited by *Escherichia coli* O157: H7 isolates related to the 2006 spinach-associated outbreak. *Appl Environ Microbiol* 78: 455–463.
- Johnston LM, Elhanafi D, Drake M, Jaykus LA (2005) A simple method for the direct detection of *Salmonella* and *Escherichia coli* O157: H7 from raw alfalfa sprouts and spent irrigation water using PCR. *J Food Prot* 68: 2256–2263.
- Weagant SD, Jinneman KC, Yoshitomi KJ, Zapata R, Fedio WM (2011) Optimization and evaluation of a modified enrichment procedure combined with immunomagnetic separation for detection of *E. coli* O157: H7 from artificially contaminated alfalfa sprouts. *Int J Food Microbiol* 149: 209–217.
- Park CH, Vandel NM, Hixon DL (1996) Rapid Immunoassay for detection of *Escherichia coli* O157 directly from stool specimens. *J Clin Microbiol* 34: 988–990.
- Wang L, Li Y, Mustapha A (2007) Rapid and simultaneous quantitation of *Escherichia coli* O157: H7, *Salmonella*, and *Shigella* in ground beef by multiplex real-time PCR and immunomagnetic separation. *J Food Prot* 70: 1366–1372.
- Jin HY, Tao KH, Li YX, Li FQ, Li SQ (2005) Microarray analysis of *Escherichia coli* O157: H7. *World J Gastroenterol* 11: 5811–5815.
- Radke SM, Alcocilja EC (2005) A high density microelectrode array biosensor for detection of *E. coli* O157: H7. *Biosens Bioelectron* 20: 1662–1667.
- Wolter A, Niessner R, Seidel M (2008) Detection of *Escherichia coli* O157: H7, *Salmonella typhimurium*, and *Legionella pneumophila* in water using a flow-through chemiluminescence microarray readout system. *Anal Chem* 80: 5854–5863.
- Yang L, Li Y, Erf GF (2004) Interdigitated Array Microelectrode-Based Electrochemical Impedance Immunosensor for Detection of *Escherichia coli* O157: H7. *Anal Chem* 76: 1107–1113.

13. Su XL, Li Y (2004) A self-assembled monolayer-based piezoelectric immunosensor for rapid detection of *Escherichia coli* O157: H7. *Biosens Bioelectron* 19: 563–574.
14. Subramanian A, Irudayaraj J, Ryan T (2006) A mixed self-assembled monolayer-based surface plasmon immunosensor for detection of *E. coli* O157: H7. *Biosens Bioelectron* 21: 998–1006.
15. Wang Y, Ye Z, Si C, Ying Y (2011) Subtractive Inhibition Assay for the Detection of *E. coli* O157: H7 Using Surface Plasmon Resonance. *Sensors* 11: 2728–2739.
16. Tims TB, Lim DV (2003) Confirmation of viable *E. coli* O157: H7 by enrichment and PCR after rapid biosensor detection. *J Microbiol Methods* 55: 141–147.
17. Mao X, Yang L, Su XL, Li Y (2006) A nanoparticle amplification based quartz crystal microbalance DNA sensor for detection of *Escherichia coli* O157: H7. *Biosens Bioelectron* 21: 1178–1185.
18. Jelinek R, Kolusheva S (2007) Biomolecular sensing with colorimetric vesicles. *Top Curr Chem* 277: 155–180.
19. Chen Y, Nieg X, Cui X, Wu W, Zhang J, et al. (2011) Direct Colorimetric Biosensors from Polydiacetylenes. *Curr Org Chem* 15: 518–533.
20. Enkelmann V (1984) Structural aspects of the topochemical polymerization of diacetylenes. *Adv Polym Sci* 63: 91–136.
21. Lee J, Kim HJ, Kim J (2008) Polydiacetylene liposome arrays for selective potassium detection. *J Am Chem Soc* 130: 5010–5011.
22. Ahn DJ, Chae E-H, Lee GS, Shim H-Y, Chang T-E, et al. (2003) Colorimetric Reversibility of Polydiacetylene Supramolecules Having Enhanced Hydrogen-Bonding under Thermal and pH Stimuli. *J Am Chem Soc* 125: 8976–8977.
23. Jonas U, Shah K, Norvez S, Charych DH (1999) Reversible Color Switching and Unusual Solution Polymerization of Hydrazide-Modified Diacetylene Lipids. *J Am Chem Soc* 121: 4580–4588.
24. Tomioka Y, Tanaka N, Imazeki S (1989) Surface-pressure-induced reversible color change of a polydiacetylene monolayer at a gas-water interface. *J Chem Phys* 91: 5694.
25. Lee J, Jun H, Kim J (2009) Polydiacetylene-Liposome microarrays for selective and sensitive mercury (II) detection. *Adv Mater* 21: 3674–3677.
26. Jung YK, Kim TW, Park HG, Soh HT (2010) Specific Colorimetric Detection of Proteins Using Bidentate Aptamer-Conjugated Polydiacetylene (PDA) Liposomes. *Adv Funct Mater* 20: 3092–3097.
27. Ellington AD, Szostak J (1990) In vitro selection of RNA molecules that bind specific ligands. *Nature* 346: 818–822.
28. Tuerk C, Gold L (1990) Systematic evolution of ligands by exponential enrichment: RNA ligands to bacteriophage T4 DNA polymerase. *Science* 249: 505–510.
29. Hesselberth J, Robertson MP, Jhaveri S, Ellington AD (2000) In vitro selection of nucleic acids for diagnostic applications. *Rev Mol Biotechnol* 74: 15–25.
30. Jayasena SD (1999) Aptamers: An Emerging Class of Molecules That Rival Antibodies in Diagnostics. *Clin Chem* 45: 1628–1650.
31. Ma Z, Li J, Liu M, Cao J, Zou Z, et al. (1998) Colorimetric detection of *Escherichia coli* by polydiacetylene vesicles functionalized with glycolipid. *J Am Chem Soc* 120: 12678–12679.
32. Bruno JG, Chanpong J (2008) Methods of producing competitive aptamer fret reagents and assays. US Patent.
33. Jung YK, Kim TW, Park HG, Soh HT (2010) Specific Colorimetric Detection of Proteins Using Bidentate Aptamer-Conjugated Polydiacetylene (PDA) Liposomes. *Adv Funct Mater* 20: 3092–3097.
34. Reppy MA, Pindzola BA (2007) Biosensing with polydiacetylene materials: structures, optical properties and applications. *Chem Commun*: 4317–4338.