

# Oral pressure therapy for treatment of obstructive sleep apnea: clinical feasibility

Mehran Farid-Moayer<sup>1</sup>  
Lawrence C Siegel<sup>2,3</sup>  
Jed Black<sup>4</sup>

<sup>1</sup>Peninsula Sleep Center, Burlingame, CA, USA; <sup>2</sup>Department of Anesthesia, Stanford University School of Medicine, Stanford, CA, USA; <sup>3</sup>Department of Clinical Affairs, ApniCure, Inc, Redwood City, CA, USA; <sup>4</sup>Stanford Center for Sleep Research and Medicine, Stanford University School of Medicine, Stanford, CA, USA

**Purpose:** This feasibility study examined the initial-use safety and effectiveness of a new noninvasive oral pressure therapy (OPT) system developed to treat obstructive sleep apnea (OSA).

**Methods:** The OPT system consists of a console that connects with flexible tubing to a premanufactured polymer mouthpiece. Through the mouthpiece, a pump in the console creates oral vacuum intended to move the soft palate anteriorly to decrease obstruction of the airway during sleep. The mouthpiece was produced in ten different sizes to accommodate a range of oral dimensions. Subjects with OSA in this single-center, single-night study underwent a polysomnography (PSG) study at baseline, followed by PSG during use of OPT.

**Results:** Fifty-six men and 20 women, aged  $50.8 \pm 12.0$  years (mean  $\pm$  standard deviation [SD]), had OSA with apnea-hypopnea indices (AHI) greater than five events per hour at baseline. Body weight averaged  $98.0 \pm 18.2$  kg (mean  $\pm$  SD), body mass index ranged from  $22.6$  kg/m<sup>2</sup> to  $57.9$  kg/m<sup>2</sup> and averaged  $32.5 \pm 5.8$  kg/m<sup>2</sup> (mean  $\pm$  SD). OPT was generally well tolerated without any serious adverse events. Baseline AHI was  $38.7 \pm 27.5$  events/hour (mean  $\pm$  SD) and was reduced with treatment to  $24.6 \pm 25.7$  events/hour ( $P < 0.001$ , Cohen's  $d$  0.53). Treatment produced AHI less than or equal to ten events/hour in 38% of the subjects. Oxygen desaturation index was  $30.1 \pm 23.7$  events/hour at baseline versus  $15.8 \pm 19.1$  events/hour with treatment ( $P < 0.001$ , Cohen's  $d$  0.66). The minimum oxygen saturation increased with treatment from  $77.9 \pm 8.3$  to  $82.2 \pm 7.9$  ( $P < 0.001$ , Cohen's  $d$  0.53). Stage-N1 sleep shifts, total sleep-stage shifts, and awakenings were significantly reduced with treatment.

**Conclusion:** This single-center, single-night feasibility study demonstrates that OPT can improve OSA in certain subjects identifiable by PSG during systematic usage. In appropriately responsive patients, OPT shows potential as a clinically useful new alternative for treatment of OSA without the need for custom manufacture of an oral device component.

**Keywords:** apnea-hypopnea index, obstructive sleep apnea, oral pressure, therapy, treatment

## Introduction

Obstructive sleep apnea (OSA) is a common clinical problem characterized by periods of reduction and cessation of airflow during sleep. Desaturation of arterial blood oxygen occurs in connection with diminished ventilation. Chronic OSA is associated with important medical problems including hypertension, coronary artery disease, cardiac dysrhythmia, cerebral vascular accident, and diabetes.<sup>1-3</sup>

Various treatment methods are available for the management of OSA. Positive airway pressure (PAP) is the most commonly prescribed treatment. PAP is a noninvasive therapy that creates a pressure gradient between the posterior oropharynx and the anterior oropharynx to move tissues anteriorly and improve gas flow in

Correspondence: Mehran Farid-Moayer  
Peninsula Sleep Center,  
1720 El Camino Real, Suite 150,  
Burlingame, CA 94010, USA  
Tel +1 650 200 5288  
Fax +1 650 752 6976  
Email sleep9000@gmail.com

the airway. While the mechanism of action of PAP is well characterized and PAP is understood as an effective treatment, tolerability issues with PAP limit the use of this therapy by some patients.<sup>4</sup> Other noninvasive treatments less commonly employed include mandibular repositioning appliances, positional therapy, and weight loss.<sup>5-7</sup> A variety of surgical treatments are available as well.<sup>8,9</sup> Results with these alternative noninvasive and invasive treatments have been disappointing for some patients, especially those with severe sleep apnea. Some therapies require significant investment of effort and expense before effectiveness can be adequately established in an individual patient.

Recognizing that some patients remain untreated or undertreated despite these important current therapeutic options, oral pressure therapy (OPT) was developed recently. The OPT system consists of a bedside console containing a pump, a soft polymer mouthpiece, and a flexible tube connecting the mouthpiece to the console (Figure 1). The console creates vacuum in the oral cavity intended to pull the soft palate anteriorly to decrease airway obstruction during sleep. A



**Figure 1** © ApniCure, Inc. The oral pressure therapy system consists of a bedside console containing a pump, a soft polymer mouthpiece, and a flexible tube connecting the mouthpiece to the console.


previous study evaluated this approach using mouthpieces customized for each subject.<sup>10</sup> A new version of the OPT mouthpiece has been developed and is now available in ten standard sizes to accommodate a range of oral dimensions in individuals without requiring a custom production process for each patient. The system is designed to be easy to trial and evaluate before a decision is made about chronic therapy. This single-night-use feasibility study examined the safety and initial effectiveness of this new noninvasive OPT system with premanufactured mouthpieces.

## Methods

Study participants were recruited from the patient database of the Peninsula Sleep Center (Burlingame, CA, USA). Patients between the ages of 18 and 80 years with an untreated apnea-hypopnea index (AHI) of five events or more per hour were included. Subjects with the following conditions were excluded: oral or dental infection or a condition that would limit the use of the mouthpiece, night-shift work schedule, abnormal nasal patency, pregnancy or intention to become pregnant during the study, unstable medical conditions other than uncomplicated OSA, or clinically significant disease which might pose additional risk to the subject or confound study results.

The OPT system (ApniCure, Inc, Redwood City, CA, USA) has three components: a mouthpiece, a console containing a pump, and tubing connecting the mouthpiece to the console. The mouthpiece is available in ten different sizes. The pump in the console applies continuous negative pressure to the mouthpiece and the console controls the pump to maintain constant negative pressure in the mouth. The system provides negative pressure to the oral cavity moving the soft palate anteriorly into contact with the tongue to reduce obstruction and improve airflow during sleep (Figure 2). With the device in operation, the patient breathes normally through the nose. The negative pressure produced in the oral cavity is isolated from the nasal-pharyngeal airway by a natural seal that occurs between the soft palate and tongue. The lightweight mouthpiece is not affixed to the teeth and can be easily removed or inserted by the patient at any time.

The Western Institutional Review Board (Olympia, WA, USA) approved this study. For each participant, written informed consent was obtained, inclusion and exclusion criteria were confirmed, and a brief oral cavity examination was performed. An imprint of the teeth was obtained on a piece of wax and compared to a visual template to identify which one of the ten available mouthpiece sizes was most

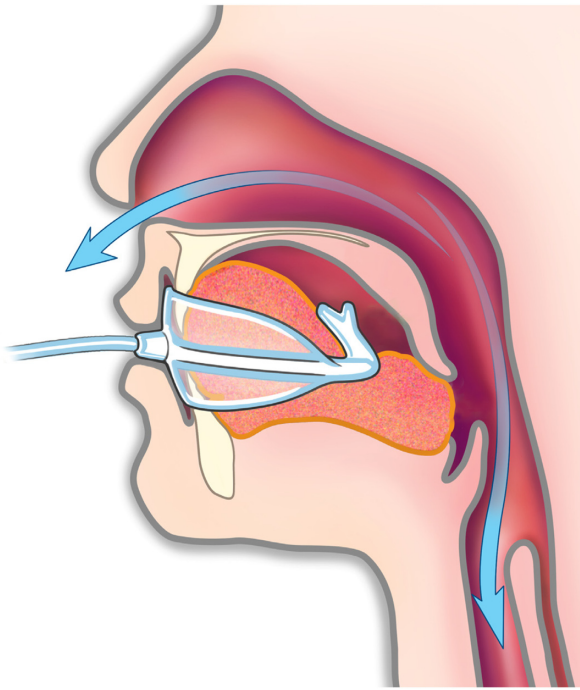


**Figure 2** © ApniCure, Inc. With the mouthpiece in place, gentle oral vacuum creates a pressure gradient intended to move the soft palate against the tongue to relieve airway obstruction during sleep.

**Notes:** The apposition of the soft palate against the tongue isolates the oral cavity from the airway. The patient breathes through the nose.

appropriate (Figure 3). After mouthpiece selection, the initial mouthpiece insertion provided an opportunity for the participant and technician to consider fit and comfort. Full-night polysomnography (PSG) without the device was performed to establish a baseline level of OSA severity without treatment and then another full-night PSG was performed with the device.

PSG data were collected using Sandman SD32 equipment and Sandman Elite software (Natus Medical, San Carlos, CA, USA). In accordance with the American Academy of Sleep Medicine 2007 protocol,<sup>11</sup> the following signals were collected on each night: electroencephalogram, electrooculogram, electromyogram (EMG), electrocardiogram, respiratory inductance plethysmograph, oxygen saturation, leg movement (EMG), nasal airflow (cannula), nasal and oral airflow (thermocouple), and body position (video). Subjects were encouraged to sleep in the supine position.

PSG data were scored manually according to American Academy of Sleep Medicine standard “recommended” criteria<sup>11</sup> by a single blinded professional scorer. In accordance with this scoring scheme, hypopneas were required to have at least a 30% airflow reduction and a 4% oxygen desaturation. The oxygen desaturation index (ODI) was calculated as the total number of events with 4% or more decrease in oxygen

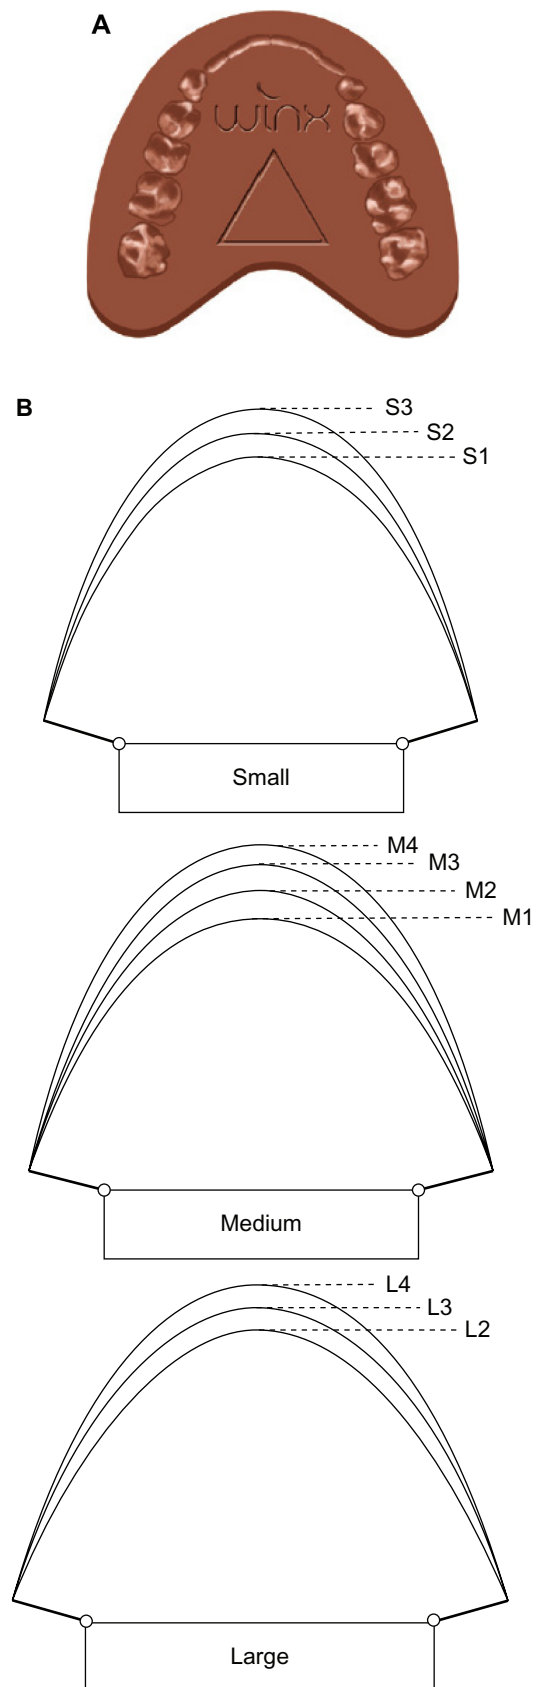

**Figure 3** © ApniCure, Inc. An imprint of the teeth is obtained on a piece of wax (A) and compared to a visual template (B) to identify which one of the ten available mouthpiece sizes is most appropriate.


saturation divided by the total sleep time (TST). Minimum oxygen saturation was determined. The percent of the night with oxygen saturation greater than or equal to 90% was calculated. AHI was calculated as the sum of the number of apnea events and hypopnea events divided by TST in hours. Measures of sleep architecture were scored.

Subjects were categorized into three OSA severity groups (mild OSA:  $\text{AHI} \geq 5$  events/hour and  $\text{AHI} < 15$  events/hour; moderate OSA:  $\text{AHI} \geq 15$  events/hour and  $\text{AHI} < 30$  events/hour; severe OSA:  $\text{AHI} \geq 30$  events/hour) based on the AHI measurement obtained from the baseline PSG. Measurements obtained at baseline and while on treatment were summarized by the baseline OSA severity. The change from baseline to treatment and percent change from baseline to treatment for all these measurements were calculated and summarized descriptively by the baseline OSA severity. A paired *t*-test was used for the test of change or percent change from baseline to treatment within each group with  $P < 0.05$  considered significant. SAS (version 9.1; SAS Institute Inc, Cary, NC, USA) and Prism 6.0 (GraphPad Software, La Jolla, CA, USA) software were used for statistical analysis.

## Results

Of the 76 subjects who were studied, 56 were male and 20 were female. The age ranged from 25 years to 75 years, averaging  $50.8 \pm 12.0$  years (mean  $\pm$  standard deviation [SD]) with ten subjects aged 65 years or older. Body weight averaged  $98.0 \pm 18.2$  kg (mean  $\pm$  SD), body mass index ranged from  $22.6 \text{ kg/m}^2$  to  $57.9 \text{ kg/m}^2$  and averaged  $32.5 \pm 5.8 \text{ kg/m}^2$  (mean  $\pm$  SD), and neck circumference was  $41.8 \pm 3.9$  cm (mean  $\pm$  SD).


AHI, ODI, and minimum oxygen saturation were significantly reduced by treatment. Baseline AHI was  $38.7 \pm 27.5$  events/hour (mean  $\pm$  SD) and was reduced with treatment to  $24.6 \pm 25.7$  events/hour ( $P < 0.001$ , Cohen's *d* 0.53). Individual responses are shown in Figure 4. ODI was  $30.1 \pm 23.7$  events/hour at baseline versus  $15.8 \pm 19.1$  events/hour with treatment ( $P < 0.001$ , Cohen's *d* 0.66). The minimum oxygen saturation increased with treatment from  $77.9 \pm 8.3$  to  $82.2 \pm 7.9$  ( $P < 0.001$ , Cohen's *d* 0.53). The percentage of the night with oxygen saturation of 90% or greater was not significantly different between baseline ( $90.8 \pm 12.5$ ) and treatment ( $93.2 \pm 12.2$ ;  $P = 0.11$ ). Figure 5 shows the extent to which treatment reduced the degree of OSA severity in the 76 subjects. Treatment produced AHI less than or equal to ten events/hour in 38% of the subjects. AHI was reduced by at least 50% with treatment as compared to baseline in 47%

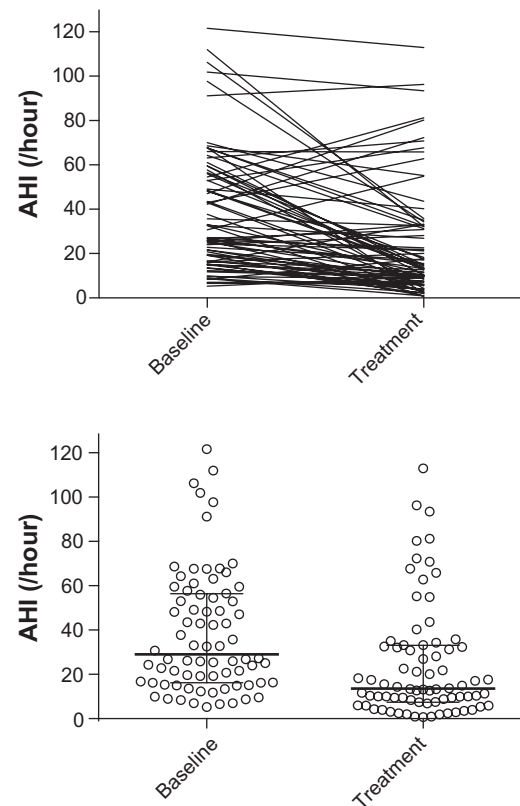

**Figure 4** Individual apnea-hypopnea index (AHI) measures are shown with the horizontal lines denoting median and quartile values.

of the subjects. Treatment produced the combined effect of AHI less than ten events per hour and reduction in AHI of at least 50% from baseline in 25% of the subjects. The alternate combined criteria of treatment AHI less than 20 events per hour and reduction in AHI of at least 50% from baseline has been suggested by a panel of advisors to the United States Food and Drug Administration<sup>12</sup> and was observed in 41% of subjects as follows: 5 of 14 subjects (36%) with mild OSA, 10 of 24 (42%) subjects with moderate OSA, and 16 of 38 (42%) subjects with severe OSA. AHI, ODI, and minimum oxygen saturation data are shown by baseline OSA severity in Figure 6.

TST was significantly reduced on the initial night of treatment from  $346.4 \pm 63.4$  minutes to  $303.0 \pm 81.5$  minutes. Sleep onset latency was not significantly altered with treatment. Total stage N1 shifts were significantly reduced with treatment from  $76.9 \pm 35.0$  to  $60.1 \pm 25.9$  ( $P < 0.001$ , Cohen's *d* 0.55). Similarly, total shifts of all sleep stages were reduced with treatment from  $198.7 \pm 74.3$  to  $158.5 \pm 56.4$  ( $P < 0.001$ , Cohen's *d* 0.61). Total awakenings were significantly reduced with treatment from  $48.4 \pm 25.7$  to  $39.0 \pm 16.5$  ( $P = 0.001$ , Cohen's *d* 0.44). Wakefulness after sleep onset was significantly increased with treatment from  $83.6 \pm 53.9$  minutes to  $103.1 \pm 57.8$  ( $P = 0.012$ , Cohen's *d* 0.35).

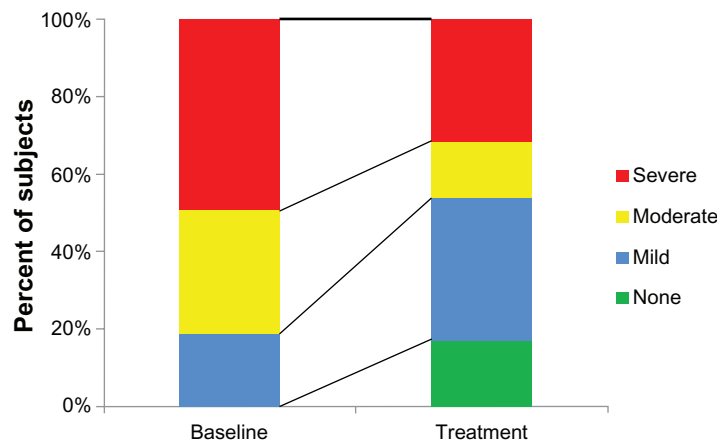

**Figure 5** Based on AHI measurements at baseline and with treatment, OSA severity was identified for each subject and the portion of the 76-subject population at each severity level is shown.

**Abbreviations:** AHI, apnea–hypopnea index; OSA, obstructive sleep apnea.

Device-related adverse events were reported by 30% of subjects and all were mild. The most common adverse events were oral tissue discomfort (12 subjects), oral tissue irritation (11 subjects), and dental discomfort (5 subjects).


## Discussion

In this acute treatment-feasibility evaluation, OPT improved sleep-related breathing disturbance in subjects with mild-to-severe OSA. Mean AHI was reduced from  $38.7 \pm 27.5$  events/hour (mean  $\pm$  SD) without treatment to  $24.6 \pm 25.7$  events/hour with treatment ( $P < 0.001$ ). Some subjects had a vigorous response to OPT while others did not respond. AHI reduction with OPT exceeded 72% in the upper quartile in this study. Since clinically relevant improvements were observed in some subjects, this study suggests that treatment with this noninvasive therapy could potentially be worthwhile for individuals who are evaluated and identified as having a clinically useful response. Improvements with OPT were notable even in some subjects with severe OSA. No significant safety issues were identified in this study. These results suggest that while OPT would not be appropriate for treating all patients, a subset of strong responders can be identified with PSG. Individual evaluation of OPT can be performed safely and rapidly without the need to customize equipment to patients, and without limiting the future use of other therapeutic options for those with an insufficient response to OPT.

As the present work was a feasibility study, there are important limitations that should be recognized in interpreting these results and in planning additional studies. With data from only a single night of treatment per subject, durability of treatment is not evaluated and chronic-treatment studies are needed. OPT was associated with significant

reductions in stage shifts and awakenings, consistent with the expectation that relief of airway obstruction during sleep should lead to improvements in sleep measures. However, as is expected with the first night of treatment with a new device, total sleep duration was reduced and wakefulness after sleep onset was increased. With chronic therapy, improvements in these measures and further improvements in stage-shifts and awakenings and in daytime symptoms such as excessive daytime sleepiness can be anticipated but should be confirmed directly by future studies. In each subject, the sequence of PSG studies was not randomized and the baseline study was completed before the PSG with OPT; however, order of PSG evaluation is unlikely to have any significant effect on respiratory parameters.<sup>13</sup> Moving beyond this feasibility study, in future studies, a randomized sequence of treatment conditions on PSG nights may be employed. Study designs with control conditions and blinding are desirable. In the present study, each subject served as his or her own control and the subjects were not blinded with regard to treatment condition. Blinding of subjects to treatment versus baseline condition or use of a sham condition are problematic to achieve due to the recognizable oral sensation that OPT produces. The mouthpiece also feels very differently in the presence and absence of the applied vacuum. Comparisons to other treatment methods using multiple treatment arms or parallel treatment groups might be considered in future study designs.

The response to therapy varied across subjects, raising the possibility that future studies might explore how the response could be predicted in individuals. Such insight would further guide the potential clinical application of OPT. Considerations for the etiology of lack of response in individuals may include

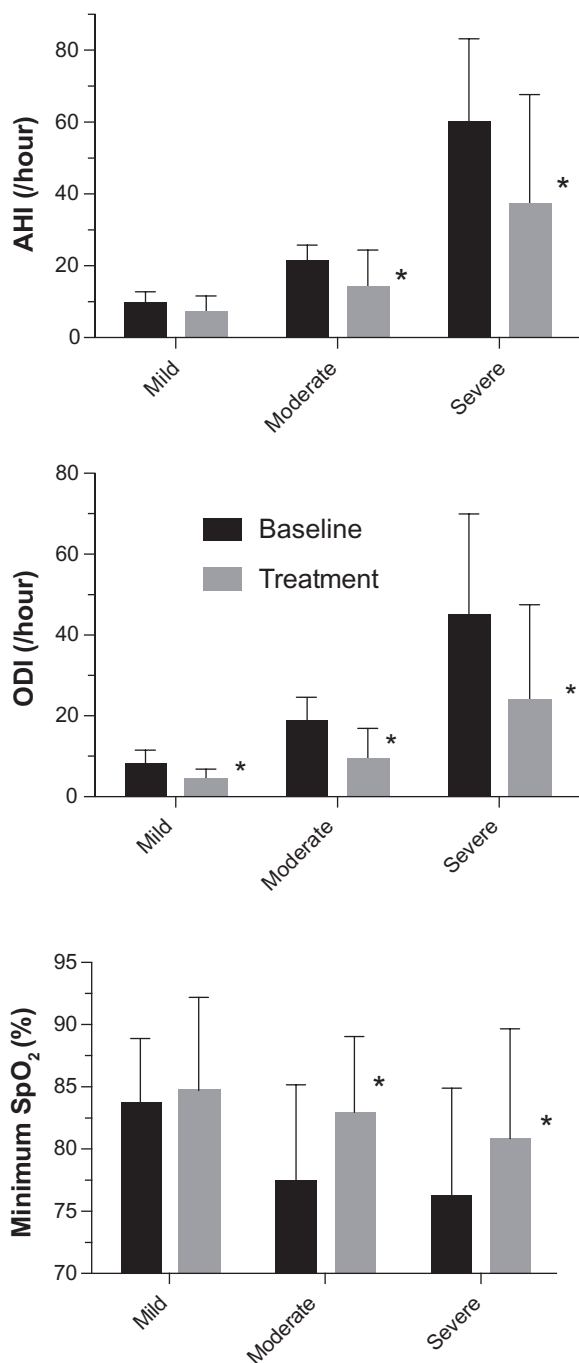

**Figure 6** AHI, ODI, and minimum oxygen saturation for baseline and treatment conditions are shown as mean  $\pm$  SD.

**Note:** \* $P < 0.01$ .

**Abbreviations:** AHI, apnea-hypopnea index; ODI, oxygen desaturation index; SD, standard deviation.

inadequate lip seal on the mouthpiece, opening of the mouth during sleep, or inadequate tissue movement with the tested device configuration. These factors, along with the night-to-night variability inherent in PSG measurement of AHI and the potential for unfavorable positioning of the mouthpiece in oral cavity relative to the tongue may explain the observation

that some subjects had treatment AHI in excess of the baseline measurement. Design improvements might lead to enhanced performance allowing OPT to become relevant for a broader portion of patients. OSA has multiple phenotypes and understanding the multiple anatomic and physiologic factors that are important in OSA is complex.<sup>14</sup> Evaluation of OPT using magnetic resonance imaging may provide insight into the mechanism of action and facilitate identifying clinical predictors. Such work may also stimulate new thinking about how the implementation of OPT can evolve to be suitable for more patients.<sup>15</sup> Ongoing research may also lead to refinement of the technology and to consideration of combinations of therapeutic methods.

Mild oral tissue discomfort was the most frequent adverse event noted. Evolution of mouthpiece shape and the materials used might help increase comfort. By way of comparison, the pressure change associated with OPT is less than that with denture seals<sup>16</sup> or breast-feeding.<sup>17</sup> Sleep architecture results may improve if comfort during OPT use can be increased. An acclimation period as typically occurs with other devices used to treat sleep apnea might enhance tolerability. The present safety results suggest that OPT is feasible for treatment of OSA. Following the demonstration of feasibility in this study, design improvements may be considered to make OPT easily applied in clinical practice. This study used mouthpieces in premanufactured sizes, which provided the potential for easier clinical application than custom production; however, optimizing the fitting procedure and identifying the most appropriate mouthpiece size for an individual patient may merit further consideration.

The results of this study confirm the feasibility of OPT for treatment of OSA as reported previously in a study of OPT in a different cohort of 71 subjects with OSA using individually customized mouthpieces.<sup>10</sup> The magnitude of AHI reduction in the present study was similar to the reduction from  $34.4 \pm 28.9$  (mean  $\pm$  SD) events per hour to  $20.7 \pm 23.3$  events per hour found in the prior study. OPT produced significant improvements in ODI in both studies. In addition, stage-N1 sleep shifts, total sleep-stage shifts, and awakenings were significantly reduced with treatment in both studies. There were no serious device-related adverse events in either study.

Patients who reject therapy with PAP or mandibular advancement devices might be candidates for treatment with OPT and should be studied to further define how their OSA can be managed successfully. Adherence to therapy is an important topic in the treatment of OSA and was not evaluated in this single-night comparison study.<sup>18</sup>

Effectiveness of response to OPT can be evaluated with PSG and the console can electronically record usage data to provide objective information regarding compliance with therapy. Trial usage of OPT may be pursued without limiting the future selection of alternative treatment methods. OPT offers promise as a noninvasive treatment approach for selected patients.

## Conclusion

This study demonstrates that OPT can improve OSA in certain subjects identifiable by PSG during systematic usage. In appropriately responsive patients, OPT shows potential as a clinically useful new alternative for treatment of OSA without the need for custom manufacture of an oral device component. Additional research evaluating sustained nightly treatment is needed to confirm and extend the findings of this study.

## Acknowledgments

Financial support for the conduct of this study was provided by ApniCure, Inc.

## Disclosure

Dr Farid-Moayer was the principal investigator. He has no conflicts of interest to disclose. Dr Siegel is employed by ApniCure and the USA Department of Veterans Affairs and is Clinical Associate Professor of Anesthesia (Affiliated), Stanford University School of Medicine. Dr Black is a consultant to ApniCure and is Consulting Associate Professor, Stanford Center for Sleep Research and Medicine, Stanford University School of Medicine.

## References

1. Young T, Finn L, Peppard PE, et al. Sleep disordered breathing and mortality: eighteen-year follow-up of the Wisconsin sleep cohort. *Sleep*. 2008;31(6):1071–1078.
2. Levy P, Pepin JL, Arnaud C, Baguet JP, Dematteis M, Mach F. Obstructive sleep apnea and atherosclerosis. *Prog Cardiovasc Dis*. 2009; 51(5):400–410.

3. Gharibeh T, Mehra R. Obstructive sleep apnea syndrome: natural history, diagnosis, and emerging treatment options. *Nat Sci Sleep*. 2010;2:233–255.
4. Shapiro GK, Shapiro CM. Factors that influence CPAP adherence: an overview. *Sleep Breath*. 2010;14(4):323–335.
5. Chan AS, Cistulli PA. Oral appliance treatment of obstructive sleep apnea: an update. *Curr Opin Pulm Med*. 2009;15(6):591–596.
6. Marklund M, Verbraecken J, Randerath W. Non-CPAP therapies in obstructive sleep apnoea: mandibular advancement device therapy. *Eur Respir J*. 2011;39(5):1241–1247.
7. van Maanen JP, Wietshe R, Van Kesteren ER, et al. Evaluation of a new simple treatment for positional sleep apnoea patients. *J Sleep Res*. 2011;21(3):322–329.
8. Holty JE, Guilleminault C. Surgical options for the treatment of obstructive sleep apnea. *Med Clin North Am*. 2010;94(3):479–515.
9. Kezerian EJ, Boudewyns A, Eisele DW, et al. Electrical stimulation of the hypoglossal nerve in the treatment of obstructive sleep apnea. *Sleep Med Rev*. 2010;14(5):299–305.
10. Farid-Moayer M, Siegel LC, Black J. A feasibility evaluation of oral pressure therapy for the treatment of obstructive sleep apnea. *Ther Adv Respir Dis*. 2013;7(1):3–12.
11. Iber C, Ancoli-Israel S, Chesson A, Quan SF. *The AASM Manual for the Scoring of Sleep and Associated Events*. Westchester, NY: American Academy of Sleep Medicine; 2007.
12. FDA Ear, Nose, and Throat Devices and Dental Products Joint Advisory Panel Meeting Open Session October 6, 2004 [Internet] Available from: [http://www.fda.gov/ohrms/dockets/ac/04/minutes/2004-4071m1\\_summary%20minutes.pdf](http://www.fda.gov/ohrms/dockets/ac/04/minutes/2004-4071m1_summary%20minutes.pdf). Accessed February 26, 2013.
13. Gouveris H, Selivanova O, Bausmer U, Goepel B, Mann W. First-night-effect on polysomnographic respiratory sleep parameters in patients with sleep-disordered breathing and upper airway pathology. *Eur Arch Otorhinolaryngol*. 2010;267(9):1449–1453.
14. Riha RL, Gislason T, Diefenbach K. The phenotype and genotype of adult obstructive sleep apnoea/hypopnoea syndrome. *Eur Respir J*. 2009;33(3):646–655.
15. Schwab R, Kim C, Siegel L, et al. Examining the mechanism of action of a new device using oral pressure therapy for treatment of obstructive sleep apnea [abstract]. *J Sleep Res*. 2012;21(Suppl 1):O310.
16. Grossman ES, Forbes ME. Studies related to reaction of supporting soft tissue to denture wear: the histological response of vervet monkey oral epithelium to a –80 mmHg vacuum. *J Oral Rehabil*. 1990;17(6): 587–597.
17. Geddes DT, Kent JC, Mitoulas LR, Hartmann PE. Tongue movement and intra-oral vacuum in breastfeeding infants. *Early Hum Dev*. 2008; 84(7):471–477.
18. Weaver TE, Grunstein RR. Adherence to continuous positive airway pressure therapy: the challenge to effective treatment. *Proc Am Thorac Soc*. 2008;5(2):173–178.

### Nature and Science of Sleep

### Publish your work in this journal

Nature and Science of Sleep is an international, peer-reviewed, open access journal covering all aspects of sleep science and sleep medicine, including the neurophysiology and functions of sleep, the genetics of sleep, sleep and society, biological rhythms, dreaming, sleep disorders and therapy, and strategies to optimize healthy sleep. The journal welcomes

Submit your manuscript here: <http://www.dovepress.com/nature-and-science-of-sleep-journal>

Dovepress

original research, clinical & epidemiological studies, reviews & evaluations, case reports and extended reports. The manuscript management system is completely online and includes a very quick and fair peer-review system, which is all easy to use. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.