

# Cytotoxic effect of a new endodontic cement and mineral trioxide aggregate on L929 line culture

Jamileh Ghoddusi<sup>1\*</sup>, Jalil Tavakkol Afshari<sup>2</sup>, Zakiyeh Donyavi<sup>3</sup>, Azam Brook<sup>4</sup>,

Reza Disfani<sup>3</sup>, Mohammad Esmaeelzadeh<sup>5</sup>

1. Department of Endodontics, Dental Research Center, Dental School, Mashad University of Medical Sciences, Mashad, Iran and Member of Iranian Center for Endodontic Research

2. Department of Bou Ali Research Institute, Mashad University of Medical Sciences, Mashad, Iran

3. Department of Endodontics, Dental School, Mashad University of Medical Sciences, Mashad, Iran

4. Technician of Bou Ali Research Institute, Mashad university of Medical Sciences, Mashad, Iran

5. Department of Pediatric Dentistry, Dental School, Shahid Beheshti University MC, Tehran, Iran

## Abstract

**Introduction:** The aim of this study was to compare the cytotoxicity of Mineral Trioxide Aggregate (MTA) and a New Endodontic Cement (NEC) on L929 mouse fibroblasts.

**Materials and Methods:** Different dilutions (Neat, 1/2, 1/10, 1/100) of fresh and set materials placed adjacent flasks of L929 in DMEM medium. Cellular viability was assessed using MTT assay in three time intervals (24, 48, and 72 h after mixing). Differences in mean cell viability values between materials were assessed by using the One-way ANOVA and Bonferoni post-test. Optical microscopic analysis of morphology of the untreated control and the cement-treated cell cultures were carried out in all experimental periods.

**Results:** It was indicated that there was not a significant difference in cytotoxicity among the materials of test and between them and the control group. However, there was a statistically significant difference between different time intervals within each group ( $P < 0.05$ ) and between different concentration of test materials ( $P < 0.05$ ). In all samples, set materials showed better viability than fresh ones.

**Conclusion:** According to results of this study, NEC and MTA have similar cytotoxic effect on L929 cell culture.

**Keywords:** Cytotoxicity test; Fibroblast; New material; Mineral trioxide aggregate

**Received:** 17 Jun 2007; **Revised:** 28 Oct 2007; **Accepted:** 09 Dec 2007

**\*Corresponding author at:** Jamileh Ghoddusi, Department of Endodontics, Mashad Dental School, P.O.Box: 984, Mashad, Iran. Tel: +98-9153161560. E-mail: ghoddusij@mums.ac.ir

## Introduction

Properties of a good root-end filling material include the ability to adhere and seal the root canal system. The material also should be easy to manipulate, radiopaque, dimensionally stable, non-absorbable, biocompatible with the periradicular tissue, and nontoxic (1).

MTA is an endodontic material that was developed at Loma Linda University in 1993 (2). This material was first used as a root-end filling, but it has also been used as a viable alternative for various clinical applications, such as capping of pulp tissue, root end closure and for repairing furcal perforations (3). Underlying these applications are the

properties of MTA that include biocompatibility, good sealing ability and capability of promoting dental pulp and periradicular tissues regeneration (2). Perez *et al.* reported that MTA might be an ideal material because it consistently induced the regeneration of periodontal ligament tissues, the apposition of a cementum like material and formation of bone (4). MTA has been reported to be biocompatible in many *in vivo* and *in vitro* studies. Koh *et al.* reported that MTA offered a biologically active substrate for bone and cells stimulating interleukin production (5). Mitchel *et al.* reported that MTA was biocompatible and suitable for clinical trials (6). Zhu *et al.* reported that

osteoblasts have a favorable response to MTA (7). Although MTA has superior biocompatibility in comparison with other materials, it has delayed setting time (8), poor handling characteristics (9), and is an expensive material.

Recently, a new endodontic cement (NEC) consisting of different calcium compounds was developed by Asgary (10). Clinical uses of this cement are similar to MTA. It has good handling characteristics and forms an effective seal when used as root-end filling material (11). NEC is also able to produce hydroxyapatite (12). The results of an in vivo study showed that as pulp capping materials, MTA and NEC showed similar favorable results. These results were better than calcium hydroxide (13).

So, the purpose of this study was to compare the cytotoxicity of MTA and NEC on L929 mouse fibroblasts

### Materials and Methods

Test materials used were ProRoot MTA (Dentsply, Tulsa Dental, OK, USA) and a Novel Endodontic Cement. Samples of the materials were prepared under aseptic conditions according to the manufacture and inventor's direction. The samples were divided into two groups. The first group included all materials in a freshly mixed state, whereas in the second group materials were allowed to set for 24 h at 37°C at 100% relative humidity.

Extracts of the materials were made as follows: 5 of complete Dulbecco's Modified Eagles Medium (DMEM) was added to 1gr of test material in every one state (fresh and set), and the tubes were incubated at 37°C at 100% relative humidity for 24h. The medium was then drawn off and sterilefiltered at 0.22 µm. To observe a dose-response relationship, the extracts were serially diluted with complete DMEM to achieve a total of four concentrations (Neat, 1/2, 1/10, and 1/100 V/V). 5-Fluorouracil was dissolved in complete DMEM and tested as positive control, complete DMEM placed into empty 96 well tissue culture plates for 24, 48, 72 h was tested as negative control.

L929 (ATCC CCL I, NCTC clone 929, mouse L Cells) mouse fibroblasts were grown

in Dulbecco's Modified Eagles Medium (Sigma chemical co, Germany), in a bicarbonate buffer system, supplemented with 10% (V/V) fetal bovine serum, 50 µg/streptomycin and 100 units/ mL Penicillin.

L929 cells were collected by washing with serum free DMEM before treatment with 5 trypsin (0.1%), 1 EDTA (0.1%) solution in phosphate buffered saline for 7-10 min. Cells from the fourth collection were plated in a 96 well plate at a density of  $5 \times 10^3$  cells per well and allowed to attach for 24 h to the DMEM plus supplements. The following protocol is adapted from Schweikl and Schmalz and Wataha *et al.* (14-15). Single cell suspensions of L929 fibroblasts were seeded in 96-well flat-bottomed plates,  $5 \times 10^3$  cells per well as determined by hemo-cytometer counting, in complete DMEM, and incubated in a humidified atmosphere of air and 5% CO<sub>2</sub> at 37°C for 24h. The culture medium then was replaced with 200 µl aliquots of the test extracts or control media.

Effects of the materials on mitochondrial function were measured by a colorimetric assay as described by Mossman (16). Upon incubation with viable cells, the tetrazolium ring of MTT (Plate yellow) is cleaved by cellular dehydrogenase enzymes to convert the yellow water-soluble tetrazolium salt MTT into dark blue formazan crystals. MTT Solution (0.5 mg/well) was added to each plate and they were incubated to be solubilized with dimethyl-sulphoxide and the absorbance determined at 570nm using an ELISA plate reader (Thermomax Microplate Reader: Molecular devices, Santo Monica, CA, USA). At each experimental time period (24, 48 and 72h), an MTT assay was conducted to measure cell viability. Optical microscopic analysis (Zeiss, Germany) of the morphology of the human untreated control and the cement-treated cell cultures were carried out in the five experimental periods (24, 48, 72, 96h, and 6d).

The mean absorbances of the three wells containing the same extract and their standard deviation were calculated. Original optical density values of test cultures were expressed as percentage of optical density obtained from the control medium. The absorption

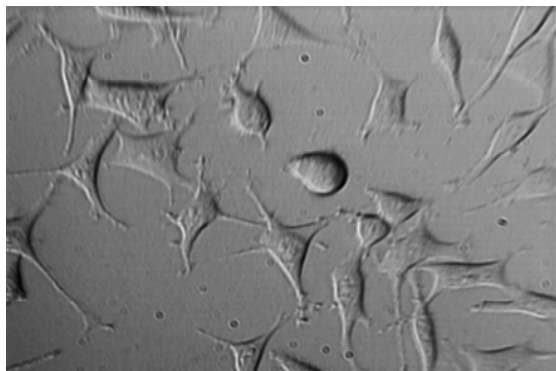


Figure1: L929 cells exposed to neat concentration of fresh MTA after 24 h. Mag×200

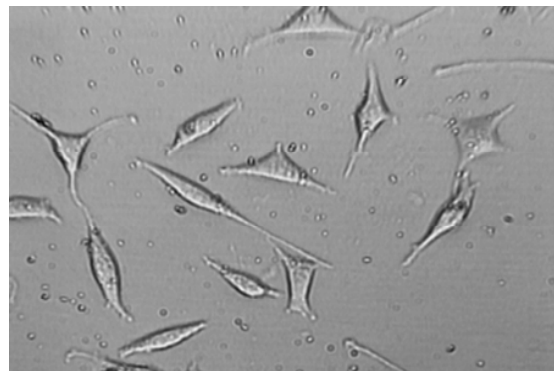


Figure2: L929 cells exposed to neat concentration of fresh NEC after 24 h. Mag×200

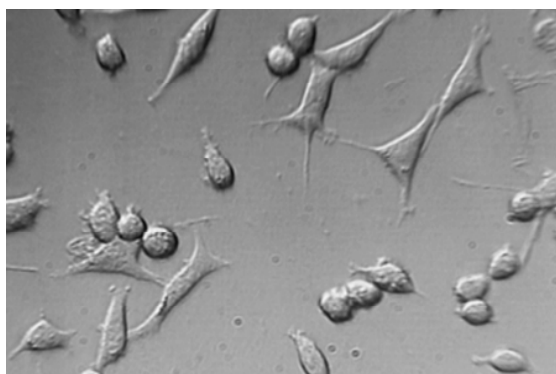


Figure3: L929 cells exposed to Neat concentration of set MTA after 24h. Mag×200



Figure4: L929 cells exposed to Neat concentration of set NEC after 24h. Mag×200

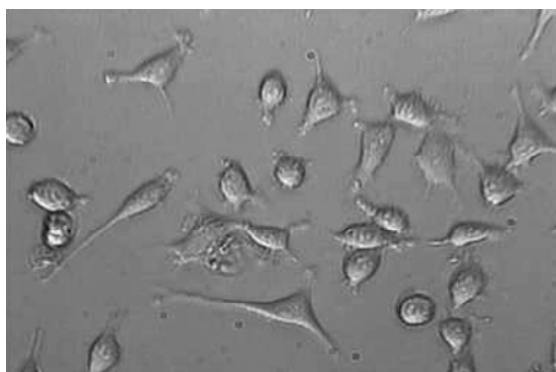


Figure5: L929 cells exposed to 5-FU in concentration of 16µg/ after 24h. Mag×200

value obtained with the control was considered as indicating 100% viability cytotoxicity. More than 90% cell viability was considered as non- cytotoxic, 60-90% as slightly cytotoxic, 30-59% as moderately cytotoxic and < 30% cell viability was also considered as strongly cytotoxic (16). All assays repeated three times to guarantee reproducibility. One-way analysis of variance and the Bonferoni post-test statistically analyzed the significance of the difference between the control and experimental groups. A  $P < 0.05$  was considered statically significant.

## Results

Findings of this study revealed that MTA and NEC do not induce cytotoxicity on L929 in both techniques including optical microscopy (Figures 1-5) and MTT assay. A confluent cell culture was observed in the negative control group maintained for the whole time of the experiment.

**In 24h, Fresh Materials:** There were statistically significant differences ( $P < 0.05$ ) between cell viability (CV) of neat MTA and their other concentrations. There was a statistically significant difference ( $P < 0.01$ ) between CV of NEC and MTA in concentration of 1/2 (Figure 6).

**In 24h, Set Materials:** There were statistically significant differences ( $P < 0.01$ ) between CV of neat NEC and their other concentrations. There was a statistically significant difference between CV of neat NEC and control group ( $P < 0.001$ ). There was a statistically significant difference ( $P = 0.001$ ) between CV of NEC and MTA in concentration of neat (Figure 7).

**In 48h, Fresh Materials:** There were statistically significant differences between CV of Neat, 1/10/, 1/100 concentration of both

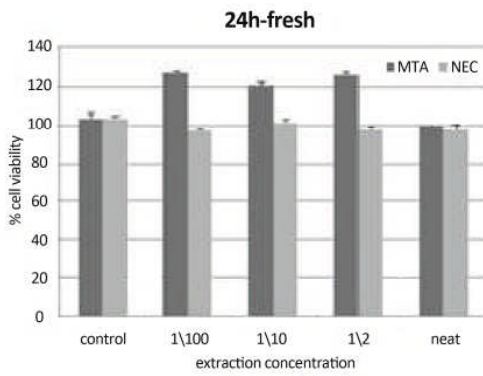


Figure6: Mean cell viability +SD at different concentration (0 concentration for control) using freshly mixed materials at 24h on L929 by MTT assay.

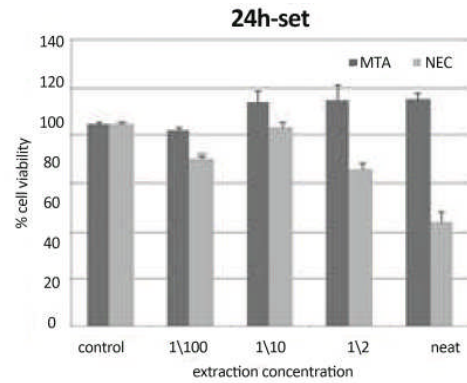


Figure7: Mean cell viability +SD at different concentration (0 concentration for control) using set materials at 24h on L929 by MTT assay.

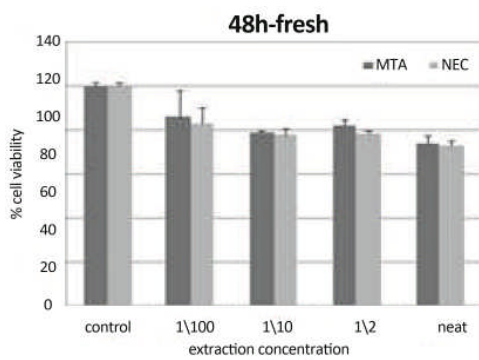


Figure8: Means cell viability +SD at different concentration (0 concentration for control) using freshly mixed materials at 48h on L929 by MTT assay.

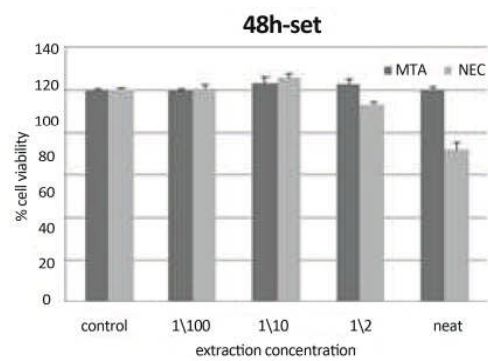


Figure9: Means cell viability +S at different concentration (0 concentration for control) using set materials at 48h on L929 by MTT assay.


materials and control group ( $P < 0.05$ ). There were statistically significant differences between CV of Neat of MTA and 1/2, 1/10, 1/100 of it ( $P < 0.05$ ). There was a statistically significant difference between CV of Neat of NEC and 1/2, 1/10 of it ( $P < 0.05$ ). There were statistically significant differences between CV of 1/2 of NEC and 1/10, 1/100 of it ( $P < 0.05$ ). There was a statistically significant difference ( $P < 0.01$ ) between CV of NEC and MTA in concentration of 1/2 ( $P = 0.033$ ) (Figure 8).

**In 48 h, Set Materials:** There were statistically significant differences between CV of neat NEC and their other concentrations ( $P < 0.05$ ). There were statistically significant differences between CV of neat of NEC and control group ( $P = 0.001$ ). There was a statistically significant difference between CV of NEC and MTA in concentration of neat ( $P < 0.001$ ). There was a statistically significant difference between CV of NEC and MTA in concentration of 1/2 ( $P = 0.02$ ) (Figure 9).

**In 72h, Fresh Materials:** There were

statistically significant differences ( $P < 0.001$ ) between CV of neat MTA and their other concentrations. There were statistically significant differences between CV of neat, 1/10, 1/100 concentration of both materials and control group ( $P < 0.05$ ). There were statistically significant differences ( $P < 0.001$ ) between CV of neat of NEC and their other concentrations. There were statistically significant differences ( $P < 0.001$ ) between CV of materials in concentration of 1/2 and 1/10 and 1/2 and 1/100. There was a statistically significant difference between CV of NEC and MTA in concentration of 1/100 ( $P = 0.003$ ) (Figure 10)

**In 72h, Set Materials:** There was a statistically significant difference between CV of NEC and MTA in concentration of neat ( $P < 0.001$ ). There were statistically significant differences between CV of 1/2 and 1/10 and 1/2 and 1/100 concentration of NEC ( $P = 0.02$ ). There were statistically significant differences between CV of NEC in concentration of neat and 1/10 ( $P = 0.002$ ). There were statistically significant

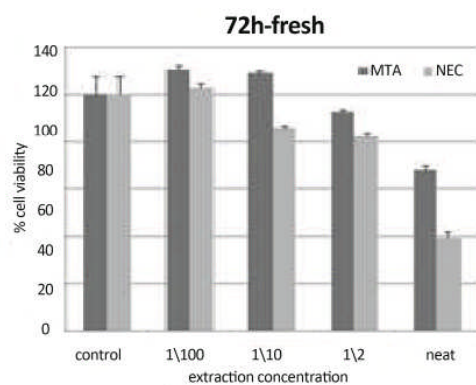

**Figure10: Means cell viability +SD at different concentration (0 concentration for control) using freshly mixed materials at 72h on L929 by MTT assay.**

differences between CV of NEC in concentration of neat and 1/100 ( $P=0.003$ ). There was a statistically significant difference between CV of neat NEC and control group ( $P=0.035$ ) (Figure11).


Comparison of fresh and set state of test materials showed at 24h: There was a statistically significant difference between CV of neat concentration of MTA ( $P=0.002$ ). There was a statistically significant difference between CV of neat concentration of NEC ( $P<0.001$ ). There was a statistically significant difference between CV of 1/100 concentration of NEC ( $P=0.034$ ).

Comparison of fresh and set state of test materials showed at 48h: There was a statistically significant difference between CV of 1/10 concentration of MTA ( $P=0.017$ ). There was a statistically significant difference between CV of 1/100 concentration of MTA ( $P=0.001$ ). There was a statistically significant difference between CV of 1/10 concentration of NEC ( $P=0.0049$ ). There was a statistically significant difference between CV of 1/100 concentration of NEC ( $P=0.012$ ).

Comparison of fresh and set state of test materials showed at 72h: There was a statistically significant difference between CV of neat concentration of MTA ( $P<0.001$ ). There was a statistically significant difference between CV of neat concentration of NEC ( $P=0.029$ ).

## Discussion

In this study cytotoxicity of Pro Root MTA and NEC were evaluated with comparison because these materials have been introduced as a root

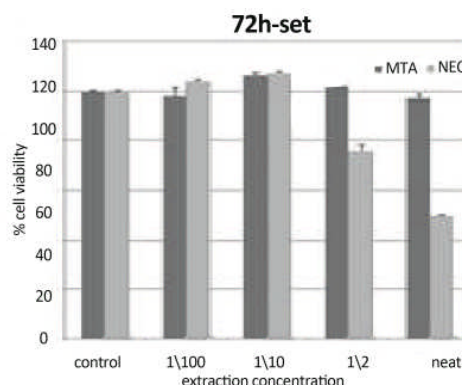

**Figure11: Means cell viability +SD at different concentration (0 concentration for control) using set materials at 72h on L929 by MTT assay.**

end filling material and in clinical application are in close contact with live tissue (17). The toxic effects of materials used for endodontic therapy are of particular concern, because damage or irritation could cause degeneration of the periapical tissue and delayed wound healing. In *in vivo* tests such as implantation and usage tests have an advantage in that they allow complex interaction between the host and the material to be examined. In *in vitro* tests such as cell culture enable experimental factors and variables to be controlled which often is a significant problem when performing experiments *in-vivo*. These *in vitro* model assays are increasingly being used for initial screening of new dental materials intended for clinical use (17). A variety of test systems are available to determine the cytotoxicity of dental materials in cultured mammalian cell populations. Permeability assays monitor the integrity of cell membranes by the inclusion or exclusion of vital dyes or by the release of radiolabeled chromium. Replication assays indirectly assess the ability of cells to proliferate by measuring the incorporation of nucleotide analogues that have been radiolabeled or are detectable by immunoassay during DNA synthesis. Changes in the cellular cytoskeleton or at the cell surface are observed by morphological studies. Finally, functional assays typically evaluate the cell's ability to provide the energy necessary for anabolic activities, or the end products of such activities. The assay used in the present study used the tetrazolium salt MTT to measure mitochondrial dehydrogenase activity. It is a plate yellow substrate that produces a dark blue formazan product when cleaved by active mitochondria. Therefore, the reaction only occurs in living

metabolically active cells. The decision to use a particular test system should be based on its consonance with the chemical nature of the material being tested. For example, if a material is not likely to cause a change in the permeability of cell membranes, a permeability assay is less apt to determine cytotoxicity in a valid manner. Because MTA is a hydrophilic substance, it is likely to release ionic components. It would be more apt to interfere with intracellular enzyme activities than influence membrane permeabilities (17). Therefore, the MTT assay was chosen for the present study.

After mixing materials, in order to achieve effective dilutions for performing the tests, serial dilution method was used, which is applied for evaluation of dose-response effect in material toxicity studies and was due to Keiser's method (18). Preparation of Neat concentration (1 gram of test sample with 5 mL of culture media) was due to Ossorio (19).

Eluates (extracts) of the test materials were used in the present investigation. They offer the advantages of being easily sterilized by filtration, and the ability to examine the effect of materials on cells that are both distant to and in contact with them. Sterilization of the test materials for direct contact testing, introduces the possibility of changing the properties of the materials. The use of eluates also simulates the immediate postsurgical root end environment in which toxic elements of the retrofilling material leach into the surrounding fluids in the bony crypt. Eluates can also be made in a series of concentrations to observe a possible dose-response relationship and determine the ideal concentration for the sensitivity of the cells tested (17).

For evaluating toxicity, Pro Root-MTA and NEC were tested in two states of freshly mixed and set. Generally freshly mixed materials as they release materials during chemical setting reactions, have more cytotoxicity. However, when the setting reactions complete, materials whole structure becomes chemically fixed and may have less cytotoxicity. This evaluation was performed according to the method of previous studies (8, 18, 19).

In this study, both qualitative assessment including morphologic evaluation applying optical microscopy and quantitative assessment with cell functional tests were accomplished.

Thus, according to quality and quantity assessment in this investigation, it possesses the privilege that what was observed in optical microscope qualitatively was also evaluated quantitatively using MTT assay test. While most of other studies were only based on whether quantitative or qualitative assessment, the histological investigations of Christopher *et al.* (20) on tissue response of dog's periapical, Torabinejad *et al.* (21) on tissue response of monkey's periapical incisor, Zhu *et al.* (7) on osteoblast cell response in contact with retrofill compounds, all were qualitative. While, the studies of, Ossorio *et al.* (19) evaluating MTT assay and crystal violet assay, Torabinejad *et al.* (22) based on two techniques of Agar over lay and Radiochromium Release method and Keisser (18) with MTT assay technique, represent quantitative assessment of materials' cytotoxicity.

NEC contains some constituents such as tricalcium phosphate, calcium sulfate, calcium silicate, calcium hydroxide, calcium oxide and some others, which have been added to NEC for improving histocompatibility and physicochemical properties. Calcium hydroxide can be produced by calcium oxide hydration. Based on the obtained results of this study, calcium hydroxide is not toxic for vital tissue. This finding is in accordance with Das (23) results, but has contradiction with Cox data (24), probability because of the produced calcium hydroxide concentration. No Study has been done on the amount of calcium hydroxide produced from NEC yet. Holland has suggested that MTA forms calcium hydroxide when is in contact with tissue fluid and triggers hard tissue precipitation (25). Findings of this study revealed that MTA and NEC do not induce cytotoxicity on L929 fibroblasts in both techniques including optical microscopy and MTT assay. The obtained result for MTA was in accordance with many other investigations.

### **Conclusion**

Results of this study encourage us using NEC as an alternative of MTA, but further studies needed to assessing other properties of this material.

### **Acknowledgement**

This research was financially supported by a

grant of the research council of Mashad University of Medical Sciences in Iran. The authors wish to thank Professor Saeed Asgary for supplying the experimental material used in this project and Dr. Esmaeeli for conducting statistical analysis.

*Conflict of Interest: 'None declared'.*

## References

1. Gartner AH, Dorn SO. Advances in endodontic surgery. *Dent Clin North Am.* 1992;36:357-78.
2. Abdullah D, Ford TR, Papaioannou S, Nicholson J, McDonald F. An evaluation of accelerated Portland cement as a restorative material. *Biomaterials.* 2002;23:4001-10.
3. Torabinejad M, Chivian N. Clinical application of mineral trioxide aggregate. *J Endod.* 1999;25:197-205.
4. Pérez AL, Spears R, Gutmann JL, Opperman LA. Osteoblasts and MG-63 osteosarcoma cells behave differently when in contact with ProRoot MTA and White MTA. *Int Endod J.* 2003;36:564-70.
5. Koh ET, McDonald F, Pitt Ford TR, Torabinejad M. Cellular response to Mineral Trioxide Aggregate. *J Endod.* 1998;24:543-7.
6. Mitchell PJ, Pitt Ford TR, Torabinejad M, McDonald F. Osteoblast biocompatibility of mineral trioxide aggregate. *Biomaterials.* 1999;20:167-73.
7. Zhu Q, Haglund R, Safavi KE, Spangberg LS. Adhesion of human osteoblasts on root-end filling materials. *J Endod.* 2000;26:404-6.
8. Torabinejad M, Hong CU, McDonald F, Pitt Ford TR. Physical and chemical properties of a new rootend filling material. *J Endod.* 1995;21:349-53.
9. Chng HK, Islam I, Yap AU, Tong YW, Koh ET. Properties of a new root-end filling material. *J Endod.* 2005;31:665-8.
10. Asgary S, Shahabi S, Jafarzadeh T, Amini S, Kheirieh S. The properties of a new endodontic material. *J Endod.* 2008;34:990-3.
11. Asgary S, Eghbal MJ, Parioikh M. Sealing ability of a novel endodontic cement as a root-end filling material. *J Biomed Mater Res A.* 2008 Jan 15; [Epub ahead of print].
12. Asgary S, Eghbal MJ, Parioikh M, Ghodduzi J. Effect of two storage solutions on surface topography of two root-end fillings. *Aust Endod J* (In press).
13. Asgary S, Eghbal MJ, Parioikh M, Ghanavati F, Rahimi H. A comparative study of histological response to different pulp capping materials and a novel endodontic cement. *Oral Surg Oral Med Oral Pathol Oral Radiol Endod.* 2008 Aug 19; [Epub ahead of print].
14. Schweickl H, Schmalz G. Toxicity parameters for cytotoxicity testing of dental materials in two different mammalian cell lines. *Eur J Oral Sci.* 1996;104:292-9.
15. Wataha JC, Craig RG, Hanks CT. Precision of and new methods for testing in vitro alloy cytotoxicity. *Dent Mater.* 1992;8:65-70.
16. Mosmann T. Rapid colorimetric assay for cellular growth and survival: application to proliferation and cytotoxicity assays. *J Immunol Methods.* 1983;65:55-63.
17. Dahl JE, Frangou-Polyzois MJ, Polyzois GL. In vitro biocompatibility of denture relining materials. *Gerodontology.* 2006;23:17-22.
18. Keiser K, Johnson CC, Tipton DA. Cytotoxicity of mineral trioxide aggregate using human periodontal ligament fibroblasts. *J Endod.* 2000;26:288-91.
19. Osorio RM, Hefti A, Vertucci FJ, Shawley AL. Cytotoxicity of endodontic materials. *J Endod.* 1998;24:91-6.
20. Bates CF, Carnes DL, del Rio CE. Longitudinal sealing ability of mineral trioxide aggregate as a rootend filling material. *J Endod.* 1996;22:575-8.
21. Torabinejad M, Pitt Ford TR, McKendry DJ, Abedi HR, Miller DA, Kariyawasam SP. Histologic assessment of mineral trioxide aggregate as a rootend filling in monkeys. *J Endod.* 1997;23:225-8.
22. Torabinejad M, Hong CU, Pitt Ford TR, Kettering JD. Cytotoxicity of four root end filling materials. *J Endod.* 1995;21:489-92.
23. Das S. Effect of certain dental materials on human pulp in tissue culture. *Oral Surg Oral Med Oral Pathol.* 1981;52:76-84.
24. Smith AJ. Dentin formation and repair. In: Hargreaves KM, Goodis HE. *Seltzer and Bender's Dental pulp.* 3 ed. Chicago: Quintessence Publishing Co; 2002. p.315.
25. Holland R, de Souza V, Nery MJ, Otoboni Filho JA, Bernabé PF, Dezan Júnior E. Reaction of dogs' teeth to root canal filling with mineral trioxide aggregate or a glass ionomer sealer. *J Endod.* 1999;25:728-30.