



Published in final edited form as:

Magn Reson Chem. 2012 April ; 50(4): . doi:10.1002/mrc.3800.

Broadband Excitation Pulses for High-Field Solid-State Nuclear Magnetic Resonance Spectroscopy

Nikolaus M. Loening^{a,b,*}, Barth-Jan van Rossum^b, and Hartmut Oschkinat^b

^aDepartment of Chemistry, Lewis & Clark College, 0615 SW Palatine Hill Road, Portland, OR 97219, USA

^bLeibniz-Institut für Molekulare Pharmakologie (FMP), Robert-Rössle-Strasse 10, 13125 Berlin, Germany

Abstract

In nuclear magnetic resonance spectroscopy, experimental limits due to the radiofrequency transmitter and/or coil means that conventional radiofrequency pulses (“hard pulses”) are sometimes not sufficiently powerful to excite magnetization uniformly over a desired range of frequencies. Effects due to non-uniform excitation are most frequently encountered at high magnetic fields for nuclei with a large range of chemical shifts. Using optimal control theory, we have designed broadband excitation pulses that are suitable for solid-state samples under magic-angle-spinning conditions. These pulses are easy to implement, robust to spinning frequency variations and radiofrequency inhomogeneities, and only four times as long as a corresponding hard-pulse. The utility of these pulses for uniformly exciting ¹³C nuclei is demonstrated on a 900 MHz (21.1 T) spectrometer.

Keywords

broadband excitation pulses; optimal control; solid-state NMR

1. Introduction

In this paper, we demonstrate the use of optimal control (OC) theory^[1–3] to design pulses for solid-state nuclear magnetic resonance (NMR) spectroscopy that uniformly excite magnetization across a broad range of frequency offsets. Excitation pulses (i.e., pulses that convert longitudinal magnetization into transverse magnetization) are one of the elementary building blocks of NMR pulse sequences. Unfortunately, uniform excitation of magnetization across a range of chemical shifts is constrained by limits to the amount of radiofrequency field strength that is experimentally accessible. Consequently, a number of pulse shapes have been explored for broadband excitation in solution-state NMR spectroscopy, including composite^[4,5], Gaussian cascade^[6], polychromatic^[7], adiabatic^[8,9], ABSTRUSE^[10], and BEBOP pulses^[11–13].

Achieving uniform excitation has not been as frequent a problem in solid-state NMR spectroscopy. This is primarily because the radiofrequency coils and amplifiers used for solid-state experiments are typically designed to operate at higher power levels than those

*Corresponding author. Fax: +1-503-768-7369. loening@lclark.edu (Nikolaus M. Loening).

6. Resources

SIMPSON scripts for generating and testing OC_{EX} pulses, as well as shape files (in Bruker format) for all pulses (OC_{EX} and OC_{FB}), are provided in the supplementary information and also at: <http://lclark.edu/~loening/pulses.html>

used for solution-state experiments. In addition, solid-state spectrometers have tended to use lower magnetic fields (due to the use of wide-bore magnets) than solution-state spectrometers with a corresponding reduction in the range of frequencies that need to be excited. As a result, the development of broadband excitation pulses for solid-state NMR has focused on quadrupolar nuclei^[14,15] where the range of frequencies to be excited can be orders of magnitude larger than for ^{13}C or ^{15}N . However, as solid-state NMR spectroscopy moves to using higher magnetic fields, there are now circumstances where it can be difficult to uniformly excite the spectrum for isotopes such as ^{13}C .

For conventional radiofrequency pulses, magnetization will not be uniformly excited once the chemical shift offset is on the same order of magnitude as the radiofrequency field strength. For relatively small offsets in simple experiments, the effects due to non-uniform excitation can be partially counteracted by applying a first-order phase correction to the resulting spectrum. For more complicated experiments, non-uniform excitation usually results in reduced signal-to-noise and can also lead to spectral artifacts. Although these effects can be reduced by increasing the radiofrequency field strength, in practice the extent to which this can be increased is always limited by saturation of the radiofrequency amplifier or arcing in the probehead. For example, on a 21.1 T spectrometer (900 MHz for ^1H), exciting the full 200 ppm ^{13}C spectrum requires covering a ± 23 kHz range of chemical shift offsets. A typical 3.2 or 4 mm solid-state MAS probe may only be able to generate ^{13}C radiofrequency fields of 50–75 kHz, so off-resonance effects will be apparent (particularly for methyl and carbonyl signals) as the radiofrequency field is not much larger than the maximum chemical shift offset.

In solid-state NMR spectroscopy, broadband excitation is usually not problematic in cross-polarization magic-angle-spinning (CP-MAS) experiments (Figure 1a), as the observed signal is due to magnetization transfer from the more easily excited ^1H spectrum (where a smaller range of offsets must be covered and the available pulse powers are typically higher) rather than by direct excitation of the ^{13}C nuclei (Figure 1b). However, broadband excitation pulses (which convert I_z magnetization to I_x magnetization), as well as “flip-back” pulses to restore magnetization to the longitudinal axis (I_x to I_z), are still needed for experiments such as PDSD^[16] and DARR^[17] (Figure 1c). Consequently, even in experiments where the magnetization begins on ^1H , excitation pulses designed using optimal control theory ($^{\text{OC}}\text{EX}$) can still be a useful addition. $^{\text{OC}}\text{EX}$ pulses can be turned into flip-back pulses ($^{\text{OC}}\text{FB}$) simply by time-reversing the pulse and adding a 180° phase shift, so it is not necessary to repeat the calculations to generate flip-back pulses.

2. Experimental

2.1. Pulse Design

All simulations and optimal control pulse calculations were performed using SIMPSON 3.0.1^[18,19]. The source code and compiled binaries for this program are freely available for download at <http://www.bionmr.chem.au.dk/bionmr/software/simpson.php>. Optimal control calculations used 20 REPULSION^[20] , crystallite angles and 5 angles for powder averaging, whereas simulations of calculated pulses used 168 REPULSION angles and 10 gamma angles. Calculations with larger sets of crystallites produced results that were essentially the same but at the expense of increased computation time.

The $^{\text{OC}}\text{EX}$ pulses were generated in an iterative procedure where the best results from each step of the calculation were used as input for the subsequent step. A smoothed random RF field was used as the initial input, and at all points in the calculation the RF amplitude was capped at 50 kHz. We performed the optimization in four steps, where the parameters included in the steps of the calculation were:

1. A narrow band optimization using a single carbon chemical shift offset. The chemical shift anisotropy was set to -76 ppm and asymmetry to 0.90 (values appropriate for carbonyl carbons).
2. Chemical shift offsets were added to ensure uniform excitation over the desired chemical shift range. Eleven chemical shifts that were evenly-spaced over a 50 kHz range of offsets (corresponding to 225 ppm for ^{13}C on a 21.1 T spectrometer) were used.
3. An RF inhomogeneity profile was added. The profile used was a 5% Lorentzian (full-width-half-height for the RF profile relative to the nominal RF field strength) with nine points (evenly spaced between 90% and 110% of the nominal field strength).
4. Optimization with the RF amplitude set to constant power (50 kHz).

The fourth step of the optimization was possible as the output from the third step was mostly phase-modulated with only slight variations in the amplitude. The advantage of including this fourth step is that the resulting $^{\text{OC}}\text{EX}$ pulses are of constant amplitude and, consequently, they do not depend on the linearity of the radiofrequency amplifier. This makes setting up the pulses easier. Simulations comparing pulses generated in the third and fourth step reveal that forcing the $^{\text{OC}}\text{EX}$ pulse to have a constant amplitude does not impact the pulse performance (data not shown).

The overall pulse length (10–100 μs), the spinning frequency (13 kHz), and the magnetic field (21.1 T, 900 MHz for ^1H) were all specified at the beginning of the calculation, as was the length of the steps within the pulse. The step length was set to 1 μs , so a 20 μs pulse ($^{\text{OC}}\text{EX}_{20}$) consists of 20 periods each with constant amplitude and phase. As will be seen in the next section, relatively short $^{\text{OC}}\text{EX}$ pulses (20 μs) are sufficiently broadband for our purposes and the pulses are not highly dependent on either the spinning frequency or the magnetic field. Five to ten $^{\text{OC}}\text{EX}$ pulses were calculated for each pulse length and then those with the best simulated performance were tested experimentally. Multiple calculations for each pulse length are necessary as, occasionally, the calculation procedure resulted in less optimal solutions (i.e., local minima) in comparison to other solutions.

2.2. Spectroscopy

The $^{\text{OC}}\text{EX}$ and $^{\text{OC}}\text{FB}$ pulses were tested on a Bruker (Karlsruhe, Germany) Avance 900 MHz (21.1 T) spectrometer using a 3.2 mm HXY MAS probe and the pulse sequences shown in Figure 1. The MAS frequency (ν_r) was set to 13.0 kHz. One-dimensional spectra were acquired with 32 scans and a recycle delay of 3 s. Spectra were acquired using SPINAL-64^[21] ^1H decoupling with a decoupling field strength of ~ 85 kHz.

The [1,3- ^{13}C , U- ^{15}N]-labeled OmpG sample was prepared as described previously^[22]. The sample consisted of ≈ 10 mg of OmpG and *E. coli* lipids packed into a 3.2 mm rotor. The sample temperature was maintained at 275 K for all experiments.

3. Results and Discussion

The theoretical excitation efficiencies (i.e., conversion of longitudinal (I_z) magnetization into transverse (I_x) magnetization) as a function of the chemical shift offset for 10–40 μs $^{\text{OC}}\text{EX}$ pulses are shown at the top of Figure 2. 50 and 100 μs $^{\text{OC}}\text{EX}$ pulses were also calculated but performed poorly, so only the shorter pulses are analyzed in the following. As seen in Figure 2, there is no significant improvement in the performance of the $^{\text{OC}}\text{EX}$ pulses for pulse lengths beyond 20 μs . This is because the $^{\text{OC}}\text{EX}$ pulses were designed to cover an

offset range of “only” 50 kHz; the $^{OC}EX_{20}$ pulse covers this bandwidth adequately so longer pulses are only needed for optimizations with a larger range of offsets.

The middle and bottom of Figure 2 compares the $^{OC}EX_{20}$ pulse to conventional 50 and 75 kHz excitation pulses (which have lengths of 5 and 3.33 μ s, respectively). Not only is the $^{OC}EX_{20}$ pulse more efficient at converting I_z magnetization into I_x over a broad range of offsets, but also less magnetization is converted to I_y magnetization. Consequently, whereas a 1D direct excitation spectrum taken using a conventional pulse may require a first-order phase correction, a similar spectrum taken using an ^{OC}EX pulse will usually not require such a correction. This behavior is shown at the top of Figure 3, which shows ^{13}C spectra taken with conventional excitation and ^{OC}EX pulses. The spectra were processed using only a zero-order phase correction to highlight the uniform phase behavior of the ^{OC}EX pulse. For experiments with multiple excitation and flip-back pulses, the phase behavior of the $^{OC}EX/^{OC}FB$ pulses not only makes processing easier but also improve the signal-to-noise ratio of the resulting spectra. For example, when implemented in a 2D DARR experiment, the use of ^{OC}EX and ^{OC}FB pulses resulted in a signal-to-noise gain of 5–10%. The results from the first increments of 2D DARR spectra are shown at the bottom of Figure 3.

Representative ^{OC}EX pulses are shown in Figure 4; only the phase is shown, as the amplitude is constant (50 kHz) for all the pulses. For short pulses the solutions look similar to composite pulses whereas longer pulses appear to be quasi-adiabatic (i.e., frequency-swept). For example, the $^{OC}EX_{10}$ pulse approximately corresponds to $54_{-y}^{\circ}126_y^{\circ}$ and the $^{OC}EX_{20}$ pulse approximately corresponds to $18_{-y}^{\circ}18_x^{\circ}72_y^{\circ}108_{-y}^{\circ}144_y^{\circ}$. The pulses that we calculated have similar shapes to the BEBOP pulses devised for solution-state NMR by Kobzar et al.^[11–13]. As the BEBOP pulses were also developed using optimal control theory and the physics for magnetization excitation are essentially the same for solution- and solid-state NMR (at least for spin-1/2 nuclei), the similarities in the resulting pulse shapes are not surprising. The main differences are that the ^{OC}EX pulses in this paper are optimized to account for RF inhomogeneity and use a constant RF amplitude in addition to having an overall pulse length and power that are appropriate for solid-state NMR under magic-angle-spinning conditions.

All ^{OC}EX pulses were optimized to include compensation for inhomogeneity of the RF field. Consequently, ^{OC}EX pulses should result in more signal than conventional pulses not only due to more uniform excitation but also because regions of the sample where the RF field is non-optimal can still contribute to the NMR signal. A calculation of the tolerance of the $^{OC}EX_{20}$ pulse to RF inhomogeneity as a function of chemical shift offset is shown in the top row of Figure 5, alongside simulations for conventional pulses. The $^{OC}EX_{20}$ pulse has transfer efficiencies in excess of 98% not only over the desired chemical shift range, but also over an approximately $\pm 10\%$ range in RF inhomogeneity. A side effect of this compensation for inhomogeneity is that the ^{OC}EX pulses are remarkably resilient to miscalibrated pulse power levels. Figure 6 illustrates the experimental excitation profile for the $^{OC}EX_{20}$ pulse with power attenuation levels between -2 dB and 1.5 dB (in 0.5 dB steps). This robustness with respect to RF inhomogeneity is advantageous in long measurements where the sample composition and/or tuning may vary during the course of the experiment, and also means that the ^{OC}EX pulses are less sensitive to calibration errors than conventional pulses.

The bottom row of Figure 5 illustrates how the offset performance of both conventional and optimal control excitation pulses varies with spinning frequency. The optimal control pulses that we have calculated are not very sensitive to the spinning frequency and are superior to conventional pulses for spinning frequencies of up to 20 kHz. At higher spinning frequencies, the optimal control pulses still have relatively uniform excitation properties, but

the transfer efficiency begins to decrease. That the ^{OC}EX and ^{OC}FB pulses are relatively insensitive to spinning frequency is a little unusual, as most solid-state pulses designed using optimal control are exquisitely sensitive to this parameter (and, consequently, need to be recalculated for every desired spinning frequency)^[23,24]. In the case of our ^{OC}EX and ^{OC}FB pulses, the relative insensitivity is probably due to their short length with respect to the rotor period and because they are not designed to recouple an interaction that varies with the rotor position.

We repeated the optimal control calculations with a spinning frequency of 24 kHz (instead of 13 kHz) to see if we could devise a pulse that had good offset performance over an even larger range of spinning frequencies. The transfer efficiency of one such pulse as a function of RF inhomogeneity, spinning frequency, and chemical shift offset is shown in the rightmost column of Figure 5. In comparison to ^{OC}EX pulses designed for a spinning frequency of 13 kHz, this pulse better covers the desired chemical shift range at spinning frequencies between 15–24 kHz but with the trade-off that it is less well compensated for RF inhomogeneity.

Designing ^{OC}EX pulses for spinning frequencies in excess of 24 kHz is not necessary, at least for ^{13}C on a 21.1 T spectrometer. This is because higher spinning frequencies can only be achieved in MAS probes with a sample diameter smaller than 3.2 mm. Such probes have smaller coils that allow for higher RF amplitudes, which means that conventional pulses are able to adequately cover the ^{13}C chemical shift range. However, for isotopes with larger chemical shift ranges (or for future spectrometers operating at even higher field strengths) excitation pulses calculated using optimal control may still be of use.

4. Conclusions

We have found that, at high fields, optimal control excitation and flip-back pulses result in improvements in experiments in which a large bandwidth needs to be efficiently excited or restored to the z -axis. In addition, the spectra that result from using these pulses have better phase properties. Although the signal improvement demonstrated in a DARR experiment is relatively modest ($\approx 10\%$), pulse sequences with additional excitation and flip-back pulses will typically show even greater improvements. The ^{OC}EX and ^{OC}FB pulses are very easy to implement as they are only phase-modulated, and are robust to variations in the power level due to the inclusion of compensation for radiofrequency field inhomogeneities in their design (which makes them relatively forgiving of mismatches in the probe tuning). Unlike most optimal control pulses for solid-state NMR spectroscopy, the ^{OC}EX pulses perform well over a wide range of spinning frequencies. Consequently, we feel that a large number of experiments could easily benefit from the use of these OC pulses as replacements for conventional excitation and flip-back pulses.


Acknowledgments

We thank Niels Chr. Nielsen (Aarhus University) for helpful conversations. N.M.L. was supported by Award Number R15GM085733 from the National Institute of General Medical Sciences.

References

1. Pontryagin, L.S.; Boltyanskii, V.G.; Gamkrelidze, R.V.; Mishchenko, E.F. *The Mathematical Theory of Optimal Processes*. Wiley-Interscience; New York: 1962.
2. Bryson, A.E., Jr; Ho, Y-C. *Applied Optimal Control: Optimization, Estimation, and Control*. Hemisphere; Washington, DC: 1975.

3. Nielsen, NC.; Kehlet, C.; Glaser, SJ.; Khaneja, N. Optimal control methods in NMR spectroscopy. In: Harris, RK.; Wasylshen, RE., editors. Encyclopedia of Magnetic Resonance. John Wiley & Sons, Ltd; Chichester: 2007.
4. Levitt MH. Composite pulses. Progress in NMR Spectroscopy. 1986; 18:61.
5. Levitt, MH. Composite pulses. In: Grant, DM.; Harris, RK., editors. Encyclopedia of Magnetic Resonance. John Wiley & Sons, Ltd; Chichester: 1996.
6. Emsley L, Bodenhausen G. Gaussian pulse cascades: New analytical functions for rectangular selective inversion and in-phase excitation in NMR. Chemical Physics Letters. 1990; 165:469–476.
7. Kupce E, Freeman R. Wideband excitation with polychromatic pulses. Journal of Magnetic Resonance, Series A. 1994; 108:268–273.
8. Bohlen JM, Rey M, Bodenhausen G. Refocusing with chirped pulses for broadband excitation without phase dispersion. Journal of Magnetic Resonance. 1989; 84:191–197.
9. Ermakov VL, Bodenhausen G. Broadband excitation in magnetic resonance by self-refocusing doubly frequency-modulated pulses. Chemical Physics Letters. 1993; 204:375–380.
10. Cano KE, Smith MA, Shaka A. Adjustable, broadband, selective excitation with uniform phase. Journal of Magnetic Resonance. 2002; 155:131–139. [PubMed: 11945042]
11. Kobzar K, Skinner TE, Khaneja N, Glaser SJ, Luy B. Exploring the limits of broadband excitation and inversion pulses. Journal of Magnetic Resonance. 2004; 170:236–243. [PubMed: 15388086]
12. Kobzar K, Skinner TE, Khaneja N, Glaser SJ, Luy B. Exploring the limits of broadband excitation and inversion: Ii. Rf-power optimized pulses. Journal of Magnetic Resonance. 2008; 194:58–66. [PubMed: 18586540]
13. Skinner TE, Kobzar K, Luy B, Bendall MR, Bermel W, Khaneja N, Glaser SJ. Optimal control design of constant amplitude phase-modulated pulses: Application to calibration-free broadband excitation. Journal of Magnetic Resonance. 2006; 179:241–249. [PubMed: 16413802]
14. Lee DK, Ramamoorthy A. A composite pulse sequence for the broadband excitation in overtone ^{14}N NMR spectroscopy. Chemical Physics Letters. 1997; 280:501–506.
15. Vitzthum V, Caporini MA, Ulzega S, Bodenhausen G. Broadband excitation and indirect detection of nitrogen-14 in rotating solids using delays alternating with nutation (DANTE). Journal of Magnetic Resonance. 2011; 212:234–239. [PubMed: 21764341]
16. Szeverenyi NM, Sullivan MJ, Maciel GE. Observation of spin exchange by two-dimensional fourier transform ^{13}C cross polarization-magic-angle spinning. Journal of Magnetic Resonance. 1982; 47:462–475.
17. Takegoshi K, Nakamura S, Terao T. ^{13}C - ^1H dipolar-assisted rotational resonance in magic-angle spinning NMR. Chemical Physics Letters. 2001; 344:631–637.
18. Bak M, Rasmussen JT, Nielsen NC. SIMPSON: A general simulation program for solid-state NMR spectroscopy. Journal of Magnetic Resonance. 2000; 147:296–330. [PubMed: 11097821]
19. Tosner Z, Vosegaard T, Kehlet C, Khaneja N, Glaser SJ, Nielsen NC. Optimal control in NMR spectroscopy: Numerical implementation in SIMPSON. Journal of Magnetic Resonance. 2009; 197:120–134. [PubMed: 19119034]
20. Bak M, Nielsen NC. REPULSION, a novel approach to efficient powder averaging in solid-state NMR. Journal of Magnetic Resonance. 1997; 125:132–139. [PubMed: 9245368]
21. Fung BM, Khitritin AK, Ermolaev K. An improved broadband decoupling sequence for liquid crystals and solids. Journal of Magnetic Resonance. 2000; 142:97–101. [PubMed: 10617439]
22. Hiller M, Higman VA, Jehle S, van Rossum BJ, Kühlbrandt W, Oschkinat H. [2,3- ^{13}C]-labeling of aromatic residues—getting a head start in the magic-angle-spinning NMR assignment of membrane proteins. Journal of the American Chemical Society. 2008; 130:408–409. [PubMed: 18092784]
23. Kehlet C, Bjerring M, Sivertsen AC, Kristensen T, Enghild JJ, Glaser SJ, Khaneja N, Nielsen NC. Optimal control based NCO and NCA experiments for spectral assignment in biological solid-state NMR spectroscopy. Journal of Magnetic Resonance. 2007; 188:216–230. [PubMed: 17681479]
24. Loening NM, Bjerring M, Nielsen NC, Oschkinat H. A comparison of NCO and NCA transfer methods for biological solid-state NMR spectroscopy. Journal of Magnetic Resonance. 2012; 214:81–90. [PubMed: 22116035]

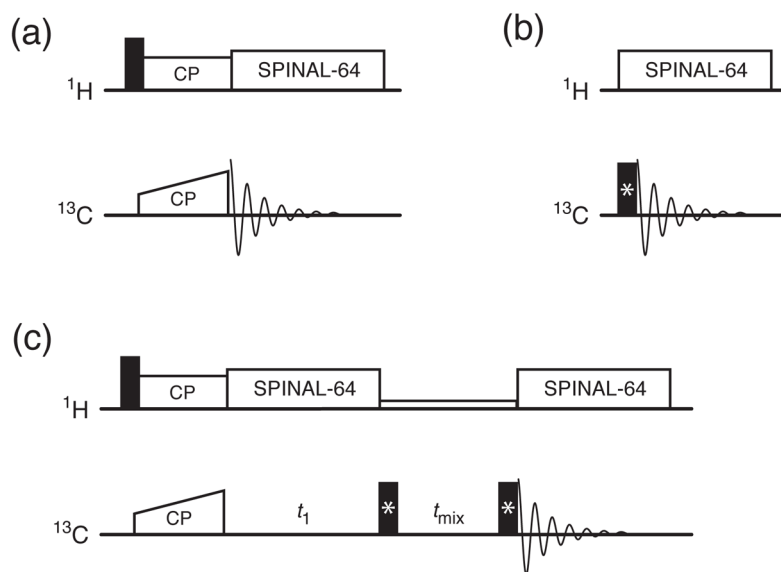**Figure 1.**

Pulse sequences mentioned in the text. Filled rectangles represent excitation or flip-back pulses. The ^1H - ^{13}C CP-MAS experiment (a) does not benefit significantly from $^{\text{OC}}\text{EX}$ pulses as the excitation pulse is on the ^1H channel. For the ^{13}C -direction excitation (b) and PDS/DARR (c) experiments, the pulses replaced with $^{\text{OC}}\text{EX}$ and $^{\text{OC}}\text{FB}$ pulses are indicated with an asterisk (*).

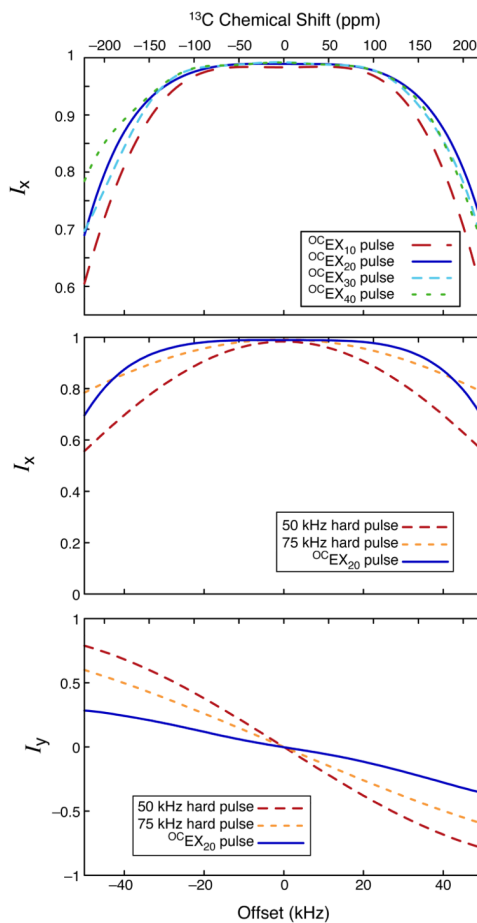


Figure 2. Conversion of longitudinal (I_z) magnetization into transverse (I_x and I_y) magnetization as a function of chemical shift offset for ^{13}C OCEX pulses and conventional hard radiofrequency pulses. The chemical shift scale corresponds to ^{13}C on a 21.1 T (900 MHz) spectrometer and $\tau = 13$ kHz.

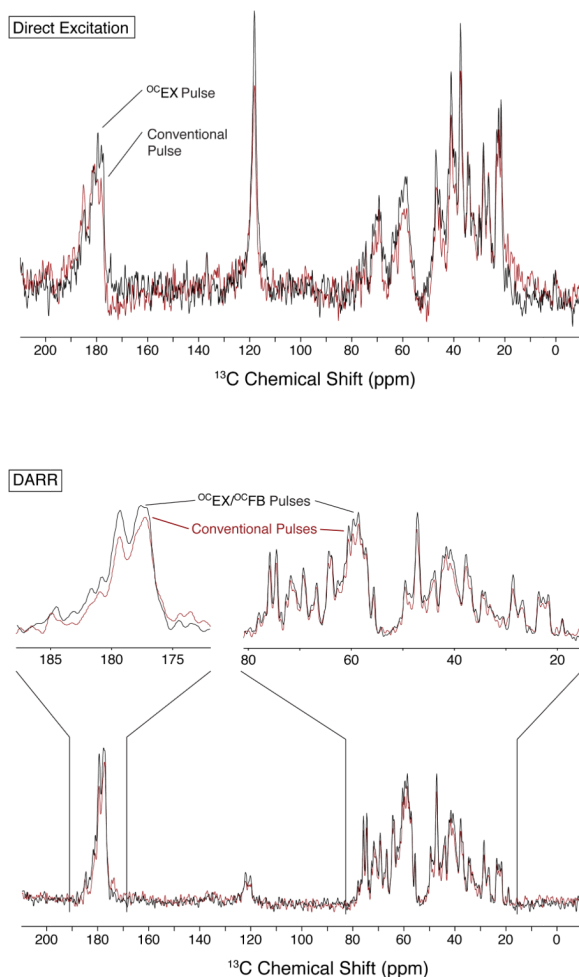


Figure 3. Comparison of 1D ^{13}C direction excitation NMR spectra (top) and the first increment from ^{13}C DARR spectra (bottom) acquired using $[1,3\text{-}^{13}\text{C}, \text{U-}^{15}\text{N}]$ OmpG at 900 MHz for ^1H and with $\nu_r=13$ kHz. The black spectra are from using OCEX and OCFB pulses, whereas the red spectra are from using conventional 50 kHz pulses. No first-order phase correction was applied to the direction excitation spectra. The prominent feature in the middle of the direction excitation spectra (at 120 ppm) is from aromatic resonances that are usually attenuated in $^1\text{H}\text{-}^{13}\text{C}$ CP-MAS spectra.

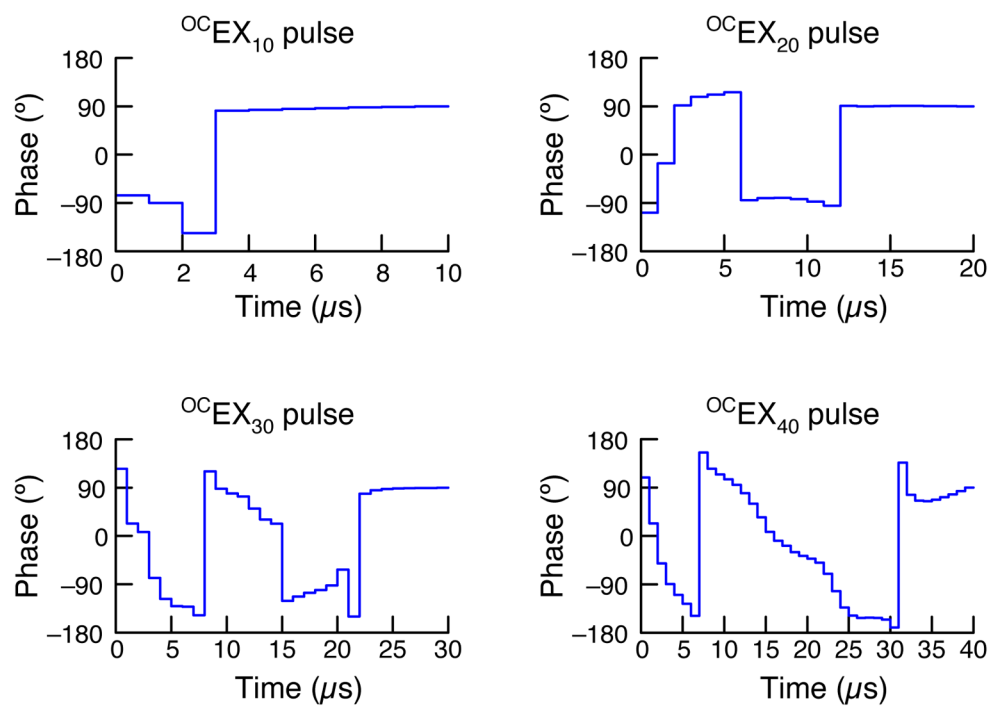


Figure 4. Phase profiles of the 10, 20, 30, and 40 μs OC EX pulses.

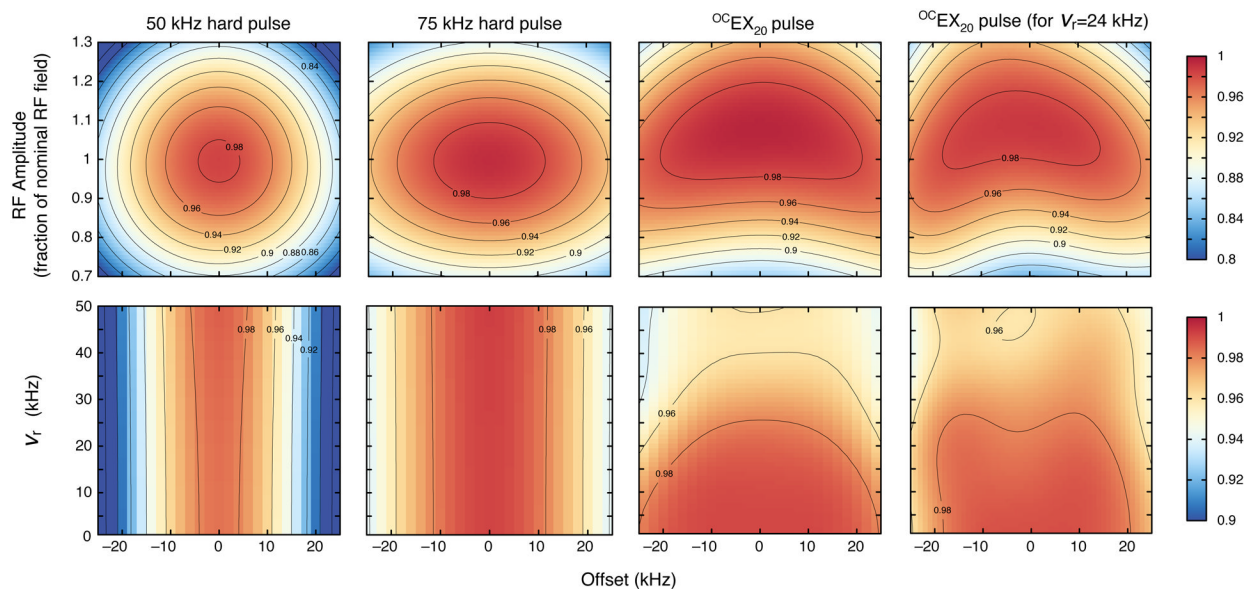


Figure 5.

Excitation efficiency as a function of RF inhomogeneity and chemical shift offset (top row) and as a function of spinning frequency (ν_r) and chemical shift offset (bottom) for 50 and 75 kHz conventional RF excitation pulses and $^{OC}EX_{20}$ pulses designed for 13 and 24 kHz spinning frequencies. In the top row, the first three graphs were calculated for $\nu_r=13$ kHz and the fourth for $\nu_r=24$ kHz. The color scale represents the transfer efficiency from I_z to I_x and runs from 80–100% (top row) and 90–100% (bottom row).

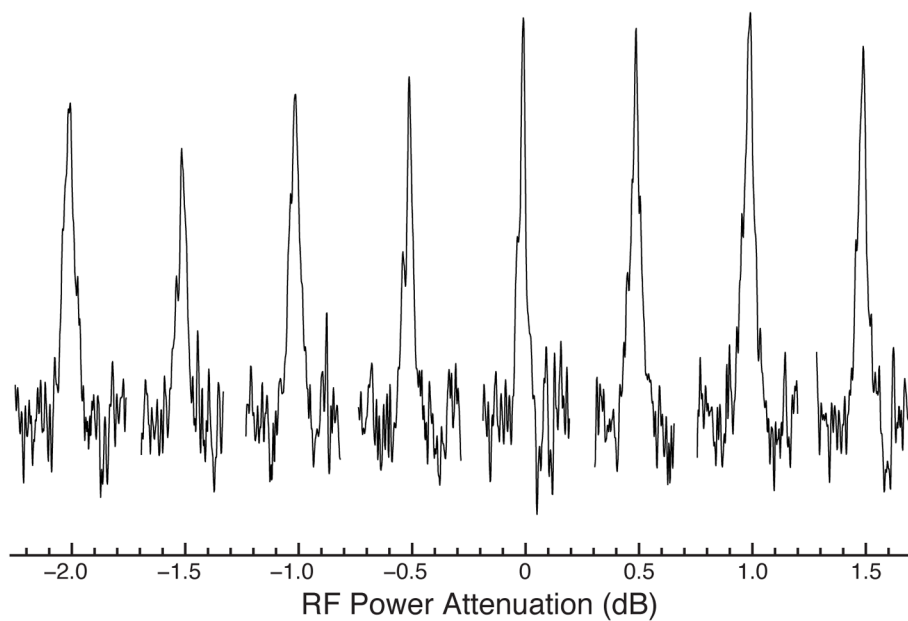


Figure 6. RF power dependence for the $OC EX_{20}$ pulse at 900 MHz for 1H and with $r = 13$ kHz. The horizontal axis corresponds to RF power attenuation (more positive values correspond to smaller RF amplitudes). The individual spectra show the aromatic region from a 1D ^{13}C direction excitation experiment using $[1,3-^{13}C, U-^{15}N]$ OmpG.