

Published in final edited form as:

*Nat Protoc.* 2010 March ; 5(3): . doi:10.1038/nprot.2009.236.

## RNA-Seq analysis to capture the transcriptome landscape of a single cell

Fuchou Tang<sup>1</sup>, Catalin Barbacioru<sup>2</sup>, Ellen Nordman<sup>2</sup>, Nanlan Xu<sup>2</sup>, Vladimir I Bashkirov<sup>2</sup>, Kaiqin Lao<sup>2</sup>, and M. Azim Surani<sup>1</sup>

<sup>1</sup>Wellcome Trust/Cancer Research UK Gurdon Institute of Cancer and Developmental Biology, University of Cambridge, Tennis Court Road, Cambridge, CB2 1QN, UK

<sup>2</sup>Genetic Systems, Applied Biosystems, part of Life Technologies, 850 Lincoln Centre Drive, Foster City, CA 94404, USA

### Abstract

We describe here a protocol for digital transcriptome analysis in a single mouse blastomere using a deep sequencing approach. An individual blastomere was first isolated and put into lysate buffer by mouth pipette. Reverse transcription was then performed directly on the whole cell lysate. After this, the free primers were removed by Exonuclease I and a poly(A) tail was added to the 3' end of the first-strand cDNA by Terminal Deoxynucleotidyl Transferase. Then the single cell cDNAs were amplified by 20 plus 9 cycles of PCR. Then 100-200 ng of these amplified cDNAs were used to construct a sequencing library. The sequencing library can be used for deep sequencing using the SOLiD system. Compared with the cDNA microarray technique, our assay can capture up to 75% more genes expressed in early embryos. The protocol can generate deep sequencing libraries within 6 days for 16 single cell samples.

### INTRODUCTION

The identity and function of a cell is determined by its entire RNA component, which is called the transcriptome of a cell<sup>1,2</sup>. The transcriptome is the functional readout of the genome and epigenome. In an organism, essentially every cell has the same genome, while every cell type and potentially each individual cell has a unique transcriptome. Ideally, the transcriptome analysis should capture the exact quantity of all full length RNAs of all classes at single-base resolution in the smallest functional unit of an organism—an individual cell<sup>2</sup>. Eventually the transcriptome analysis may even become non-invasive, allowing us to read the sequences of every RNA molecule of a living cell without destroying the cell. During the past decade, the most successful and most widely used transcriptome analysis method has been the cDNA microarray<sup>3-8</sup>. Due to the development of the genome project, the cDNA microarray technique became available for most of the model organisms with a known genome. It is a powerful way to capture the expression pattern of tens of thousands of known genes by hybridization onto a tiny chip. However, it has significant drawbacks and limitations<sup>1,2</sup>, including (1) cross reactions between genes of similar sequences that occur due to the nature of hybridization on microarrays, (2) detection of expression levels only in the range of hundreds of folds, or three orders, despite the real dynamic range of gene expression in a cell being hundreds of thousands of folds, or six orders, (3) the exact length and sequence of the mRNAs analyzed is unknown, and (4) novel transcripts cannot be detected.

Using a tiling array can resolve some of these problems. The recently developed deep sequencing based transcriptome analysis, or RNA-Seq, can potentially overcome all of these problems<sup>1,9-12</sup>. RNA-Seq is sequencing based and can achieve single base resolution. The

dynamic range of gene expression level that it can capture is theoretically unlimited, depending only on the depth of sequencing. More importantly, with the help of complete genome information, the exact length and sequence of all the RNAs analyzed can be captured accurately. During the past two years, people in the field have already witnessed the astonishingly fast development of the RNA-Seq technique and the deepening of our understanding of the complexity of the eukaryotic transcriptome, from yeast to human, from adult tissues to embryonic development<sup>13-21</sup>. However, due to the sensitivity of the method, it usually needs  $\mu\text{g}$  amounts of total RNAs, and most of the RNA-Seq studies used tissue, a mixture of different types of cells, or a cell line, which is at least a mixture of cells at different stages of the cell cycle. Also, recent progress on the stochastic nature of transcription and gene expression showed that even in the same cell type at the same cell cycle stage, the copy number of the mRNA of an expressed gene can be affected by both the microenvironment and the intrinsic noise of the transcription process<sup>22-27</sup>. Ideally the RNA-seq transcriptome analysis should be done using individual cells, or even the sub-compartment of a cell, such as the cytoplasm or nucleus. Also, for early embryonic development or stem cells *in vivo*, it is extremely difficult or even practically impossible to isolate millions of cells of a single type. RNA-Seq at single cell resolution will greatly promote the development of these fields by permitting comprehensive capture of the expression dynamics of all genes at all developmental stages.

During the past few years, people have already developed cDNA microarrays capable of using a small amount of starting material, or even a single cell through either *in vitro* transcription (IVT) based linear amplification, PCR-based exponential amplification, or a combination of the two methods<sup>28-38</sup>. However, these microarrays have inherited the limitations of the microarray technique. We improved a widely used single cell cDNA amplification strategy and combined it with SOLiD deep sequencing system to set up a digital transcriptome analysis method: single cell RNA-Seq<sup>38-40</sup>. By comparing the accuracy of single cell cDNA microarrays to our single cell RNA-Seq, we demonstrated that single cell RNA-Seq has greater accuracy. There are two reasons for this: (1) due to the higher sensitivity of the deep sequencing compared with the cDNA microarray, the IVT step is unnecessary to further amplify single cell cDNAs. This removes the amplification bias introduced by the IVT step. (2) With the better dynamic range of the deep sequencing method, the level of gene expression is more accurately captured by RNA-Seq. Using this method, we captured 5270 (75%) more genes than the cDNA microarray, expanding the transcriptome of a blastomere of a four-cell stage embryo from 7,050 expressed genes to 11,920 expressed genes. Around 10% of genes with multiple known transcript isoforms expressing more than two different transcript isoforms were detected in the same blastomere at the same time point, which has never been achieved by the single cell cDNA microarray. We also identified thousands of previously unknown splicing junctions from already known genes, indicating how limited our previous appreciation of the complexity of the eukaryotic transcriptome was based on the cDNA microarray.

This strategy has many possible future applications. It creates the possibility of isolating one or several cells from any of the organs or tumors of a patient and analyzing the transcriptome by RNA-seq, reducing the invasiveness of biopsies and clarifying the diagnosis of diseases. Potentially the sub-cellular distribution of mRNAs could be explored by comparing, for example, the axon and cell body of a neuron.

Current limitations of the single cell RNA-Seq include<sup>40</sup>:

1. The assay can only capture mRNAs with a poly(A) tail. Those mRNAs without poly(A) tails or other classes of RNAs such as small non-coding RNAs will not be detected.

2. The assay can not ascertain the strandedness of the transcript—that is, the sense or antisense transcripts can not be discriminated.
3. The assay can only capture about 3kb cDNA fragments from the 3' end of a mRNA. For the genes with mRNAs longer than 3 kb, which constitute about 36% of all known genes, the 5' end part of the mRNA can not be detected. We are currently improving the method to overcome these limitations.

## MATERIALS

### REAGENTS

- Ac-BSA (Sigma, cat. no. B8894)
- Acidic Tyrode's solution (Sigma, cat. no. T1788)
- 1× PBS (pH 7.2) (Gibco, cat. no. 14249-95)
- 10× PCR Buffer II and 25 mM MgCl<sub>2</sub> (Applied Biosystems, cat. no. 4379878)
- Nonidet P-40 SP (Roche, cat. no. 11332473001)
- SuperScript III Reverse Transcriptase with 0.1 M DTT (Invitrogen, cat. no. 18080-044 or 18080-085)
- RNase Inhibitor (Cloned) (40 U μl<sup>-1</sup>) (Applied Biosystems, cat. no. AM2682)
- SUPERase-In™ (20 U μl<sup>-1</sup>) (Applied Biosystems, cat. no. AM2694)
- T4 gene 32 Protein (Roche, cat. no. 972983)
- Exonuclease I (New England Biolabs, cat. no. M0293S)
- Terminal Transferase (TdT) (Invitrogen, cat. no. 10533-065 or 10533-073)
- 100 mM dATP (Promega, cat. no. U1201)
- Nuclease-free Water, 1 L (Applied Biosystems, cat. no. AM9932)
- RNase H (Invitrogen, cat. no. 18021-014 or 18021-071)
- TaKaRa Ex Taq™ HS (Includes: 10× ExTaq Buffer (mg<sup>2+</sup> plus) and dNTP mixture) (Takara Bio Inc, cat. no. RR006A or RR006B)
- QIAquick PCR Purification Kit (250) (Qiagen, cat. no. 28106)
- QIAquick Gel Extraction Kit (250) (Qiagen, cat. no. 28706)
- RNeasy Mini Kit (50) (Qiagen, cat. no. 74104)
- PCR tubes, 0.5 ml (Eppendorf, cat. no. 951010057)
- PCR tubes, 0.2 ml thin-wall (MLS)
- Filtered pipettor tips (MLS)
- SYBR Green PCR Mastermix (Applied Biosystems, cat. no. 4334973)

GeneAmp® dNTP Blend (100 mM) (Applied Biosystems, cat. no. N8080261)

3 M sodium acetate (pH 5.5) (Applied Biosystems/Ambion, cat. no. AM9740)

1 M Tris, pH 8.0 (100 ml) (Applied Biosystems/Ambion, AM9855G)

Nuclease-free Water (1 L) (Applied Biosystems/Ambion, cat. no. AM9932)

10× NEBuffer2 (New England BioLabs® Inc., B7002S)

Ethanol (Sigma-Aldrich®, cat. no. E7023)

Ethylene glycol (American Bioanalytical, cat. no. AB00455-01000)

Covaris microTUBE with AFA fiber and Snap-Cap with pre-slit Teflon/silicone/Teflon septa (Covaris™ Inc., cat. no. 520045)

End-It™ DNA End-Repair Kit (Epicentre®, cat. no. ER0720)

DNA Polymerase I (E. coli), (10U  $\mu\text{l}^{-1}$ ) (New England BioLabs® Inc., cat. no. M0209L)

Quick Ligation™ kit (New England Biolabs, cat. no. M2200L)

SYBR GreenER® qPCR SuperMix Universal (Invitrogen™ Corporation, cat. no. 11762-100) OR SYBR Green PCR Master Mix (Applied Biosystems, cat. no. 4309155)

Agilent DNA 1000 Kit (Agilent Technologies, cat. no. 5067-1504)

Agencourt® AMPure® 60 ml kit (Agencourt, cat. no. 000130)

AmpliTaq® DNA Polymerase, LD with Buffer I (Applied Biosystems, cat. no. N8080157)

Cloned Pfu polymerase (2.5 U  $\mu\text{l}^{-1}$ ) (Stratagene, cat. no. 600153)

Invitrogen Platinum® PCR SuperMix (Invitrogen™ Corporation, cat. no. 11306-016)

Quant-iT™ dsDNA HS Assay Kit, 100 assays (Invitrogen™ Corporation, cat. no. Q32854)

SOLiD™ Fragment Library Oligos Kit (Applied Biosystems, cat. no. 4401151)

## EQUIPMENT

Brown-flaming micropipette puller (Sutter Instrument Co., Model P-80)

Covaris™ S2 System, (for system materials summary, see “Covaris™ S2 System Materials Summary,” *SOLiD™ System 2.0 Site Preparation Guide.*)

Microcentrifuge 5417R, refrigerated, without rotor 120 V//60 Hz (Eppendorf, cat. no. 022621807)

96-Well GeneAmp® PCR System 9700 (thermal cycler) (Applied Biosystems, cat. no. N8050200)

Real-time PCR System with 96-well block (ABI PRISM 7000 real-time PCR system (Applied Biosystems)

NanoDrop ND1000 Spectrophotometer (computer required) (NanoDrop (Thermo Sci), cat. no. ND-1000)

Labquake Rotisserie Rotator (Barnstead/Thermolyne, cat. no. VWR 56264-312)

Qubit™ fluorometer (Invitrogen, cat. no. Q32857)

6 Tube Magnetic Stand (Applied Biosystems, cat. no. AM10055)

Agilent 2100 Bioanalyzer (Agilent Technologies, cat. no. G2938C)

## REAGENT SETUP

**PBS-BSA** (1 mg ml<sup>-1</sup>) Dissolve Ac-BSA (20 mg ml<sup>-1</sup>) in PBS at 1mg ml<sup>-1</sup> and aliquot into 1.5ml Eppendorf tubes. Store the solution at -20 °C.

## PROCEDURE

### Single cell lysis

1. Dilute the UP1 Primer to 0.5 μM by adding 1 μl of 100 μM UP1 Primer and 199 μl of nuclease-free water to a tube and mix well. (All of primer sequences are listed in Table 1).
2. Prepare the Cell Lysis Buffer (4.45 μl per sample) in a 0.5 ml thin-wall PCR tube by combining and mixing the following components:

Component	Stock concentration	Final concentration in RT (5 μl)	×1 volume	×12 volume
10X PCR Buffer II (without MgCl <sub>2</sub> )	10×	0.9×	0.45 μl	5.4 μl
25 mM MgCl <sub>2</sub>	25 mM	1.35 mM	0.27 μl	3.24 μl
10% NP40	10%	0.45%	0.225 μl	2.7 μl
0.1 M DTT	100 mM	4.5 mM	0.225 μl	2.7 μl
SUPERase-In (Ambion)	20 U μl <sup>-1</sup>	0.18 U μl <sup>-1</sup>	0.045 μl	0.54 μl
RNase Inhibitor (Ambion)	40 U μl <sup>-1</sup>	0.36 U μl <sup>-1</sup>	0.045 μl	0.54 μl
0.5 μM UP1 Primer	500 nM	12.5 nM	0.125 μl	1.5 μl
2.5 mM each dNTP	2.5 mM	0.045 mM (each)	0.09 μl	1.08 μl
Nuclease-free water	—	—	2.975 μl	35.7 μl
Total volume	—	—	4.45 μl	53.4 μl

**CRITICAL STEP** Prepare master mix based on the number of the samples (here we show processing 10 samples as an example). To minimize pipetting error, prepare at least 12× worth of lysis buffer if the total number of samples is 10. The final volume of RT reaction is 5 μl per tube including 4.45 μl lysis buffer, about 0.1 μl PBS-BSA carryover (when picking single cells), and 0.45 μl RT mix. All final concentrations were calculated based on the volume of the 5 μl RT reaction.

3. For picking up and transferring individual cells, we usually use a mouth tube to control a micropipette attached to it under a dissection microscope (also described in Ref. 39 & 41). First isolate four-cell stage embryos from the oviduct (see Ref. 42). Transfer them by micropipette to a drop of Acidic Tyrode's solution to remove the zona pellucida. Then transfer the embryos into

calcium free medium and gently pipette until the individual blastomeres separate. Transfer the blastomeres into three drops of PBS-BSA sequentially to wash them. Finally transfer the blastomeres into a final drop of PBS-BSA for picking.

**CRITICAL STEP** Be careful during all the transfer steps to make sure no bubbles are made in the drops by the micropipette.

4. Seed a single cell (with PBS-BSA carryover) into each 0.5 ml thin-wall PCR tube containing 4.45  $\mu$ l of Cell Lysis Buffer.

**CRITICAL STEP** Make sure the part of the micropipette outside the mouse tube is long enough (longer than 4 cm) to permit the tip of it to dip into the lysis buffer at the bottom of the 0.5 ml PCR tube with the mouse tube part not touching the lid and rim of the PCR tube to avoid any potential contamination. Also, during picking single cells using the micropipette gloves should be worn to avoid potential contaminations of the PCR tubes.

**CRITICAL STEP** First suck a small volume of PBS-BSA using the mouse pipette, then gently suck the single cell into the micropipette to keep the cell already inside the micropipette, but still near the tip of the micropipette. When pushing the cell out of the micropipette into the lysis, push out all the carryover PBS-BSA.

**CRITICAL STEP** It is crucial to make sure that the individual cell to be analyzed has actually been transferred into the lysis buffer from the drop of PBS-BSA by a micropipette. At this starting point the operator can practice transferring an individual cell into a drop of 4 - 5  $\mu$ l PBS-BSA instead of lysis buffer on a 6 cm cell culture dish, and then recover it to ascertain if they can accurately transfer an individual cell into a small drop of the solution.

**CRITICAL STEP** Each micropipette can be used only once for an individual cell when picking the cell into the lysis buffer in the PCR tube. Never use the same micropipette repeatedly for transferring single cells into lysis buffer.

**CRITICAL STEP** It is essential to include a negative control sample without picking a single cell into it, but only pick a PBS-BSA solution equivalent to the carryover volume when picking a single cell into the lysis buffer tube. This negative control will ensure that all the steps from the start to the end of the whole procedure are not contaminated.

5. Centrifuge for 30 sec at 7,500 g at 4 °C and put on ice immediately.
6. Incubate at 70 °C for 90 sec and put on ice immediately.

**CRITICAL STEP** Use a thermal cycler with heated lid for all incubations throughout this protocol.

**CRITICAL STEP** The protocol also allows use of purified total RNA instead of single cells. If using total RNA, simply use total RNA to replace the single cell and keep the final volume of the reverse transcription reaction at 5  $\mu$ l (although the volume of water in the lysis buffer should be adjusted). 20 pg to 1 ng of total RNA for each sample should work.

7. Centrifuge the tubes for 30 sec at 7,500 g at 4 °C and put them on ice immediately for 1 min.

**CRITICAL STEP** After this step, all mRNAs from the single cell are released.

### Reverse transcription

8. Prepare the Reverse Transcriptase (RT) mix (0.45  $\mu$ l per sample) by combining and mixing the following components:

Component	Stock concentration	Final concentration	×1 volume	×12 volume
SuperScript III Reverse Transcriptase	200 U $\mu\text{l}^{-1}$	13.2 U $\mu\text{l}^{-1}$	0.33 $\mu\text{l}$	3.96 $\mu\text{l}$
RNase Inhibitor (Ambion)	40 U $\mu\text{l}^{-1}$	0.4 U $\mu\text{l}^{-1}$	0.05 $\mu\text{l}$	0.6 $\mu\text{l}$
T4 gene 32 protein	1-10 U $\mu\text{l}^{-1}$ (5 U $\mu\text{l}^{-1}$ in average)	0.07 U $\mu\text{l}^{-1}$	0.07 $\mu\text{l}$	0.84 $\mu\text{l}$
Total volume	—	—	0.45 $\mu\text{l}$	5.4 $\mu\text{l}$

**CRITICAL STEP** Prepare master mix based on the number of the samples. To minimize pipetting error, prepare at least 12× worth of reaction mix if the total number of samples is 10.

9. Add 0.45  $\mu\text{l}$  RT mix to each tube. The total volume is now 5.0  $\mu\text{l}$ .
10. Incubate at 50 °C for 30 min.
11. Inactivate the reverse transcriptase at 70 °C for 10 min.
12. Centrifuge tubes for 30 sec at 7,500 g at 4 °C and immediately place on ice for 1 min.

**CRITICAL STEP** After this step, first strand cDNAs for all mRNAs are synthesized.

#### Free primer removal

13. Prepare the Exonuclease I mix by combining and mixing the following components:

Component	Stock concentration	Final concentration in Cut (1 $\mu\text{L}$ )	×1 volume	×12 volume
10X Exonuclease I Buffer	10×	1×	0.1 $\mu\text{l}$	1.2 $\mu\text{l}$
Nuclease-free water	—	—	0.8 $\mu\text{l}$	9.6 $\mu\text{l}$
Exonuclease I	5 U $\mu\text{l}^{-1}$	0.5 U $\mu\text{l}^{-1}$	0.1 $\mu\text{l}$	1.2 $\mu\text{l}$
Total volume	—	—	1 $\mu\text{l}$	12 $\mu\text{l}$

**CRITICAL STEP** Prepare master mix based on the number of the samples. To minimize pipetting error, prepare at least 12× worth of reaction mix if the total number of samples is 10.

14. Add 1.0  $\mu\text{l}$  of Exonuclease I mix to each reaction. Total volume in the tube is now 6  $\mu\text{l}$ .
15. Incubate at 37 °C for 30 min.
16. Inactivate the Exonuclease I at 80 °C for 25 min.
17. Centrifuge tubes for 30 sec at 7,500 g at 4 °C and immediately place on ice for 1 min.

**CRITICAL STEP** After this step, all free UP1 primers are destroyed and the 3'-end of cDNAs are shortened about 50 bp. The 5'-end of cDNAs (UP1 sequence) are intact.



### 3'-Poly-A tailing

18. Prepare terminal deoxynucleotidyl transferase (TdT) reaction mix by combining and mixing the following components:

Component	Stock concentration	Final concentration	×1 volume	×11 volume
10X PCR Buffer II (without MgCl <sub>2</sub> )	10×	1×	0.6 μl	6.6 μl
25 mM MgCl <sub>2</sub>	25 mM	1.5 mM	0.36 μl	3.96 μl
100 mM dATP	100 mM	3 mM	0.18 μl	1.98 μl
Nuclease-free water	—	—	4.26 μl	46.86 μl
Terminal Transferase	15 U μl <sup>-1</sup>	0.75 U μl <sup>-1</sup>	0.3 μl	3.3 μl
RNase H	2 U μl <sup>-1</sup>	0.1 U μl <sup>-1</sup>	0.3 μl	3.3 μl
Total volume	—	—	6 μl	66 μl

**CRITICAL STEP** Prepare master mix based on the number of the samples. To minimize pipetting error, prepare at least 11× worth of reaction mix if the total number of samples is 10.

19. Add 6.0 μl of TdT mixture to each reaction. Total volume is now 12.0 μl per tube.
20. Incubate at 37 °C for 15 min.
21. Inactivate the terminal deoxynucleotidyl transferase at 70 °C for 10 min.
22. Centrifuge tubes for 30 sec at 7,500 g at 4 °C and immediately place on ice for 1 min.

**CRITICAL STEP** After this step, 3'-end of the first-stranded cDNAs has a poly(A) tail.

### Second strand cDNA synthesis

23. Prepare 76 μl PCR Mix 1 for each reaction by combining and mixing the following components:

Component	Stock concentration	Final concentration	×1 volume	×11 volume
10X Ex Taq Buffer (with MgCl <sub>2</sub> )	10×	1×	7.6 μl	83.6 μl
2.5 mM each dNTP	2.5 mM	0.25 mM	7.6 μl	83.6 μl
UP2 primer (100 μM)	100 μM	1 μM	0.76 μl	8.36 μl
Nuclease-free water	—	—	59.28 μl	652.08 μl
TaKaRa Ex Taq™ HS	5 U μl <sup>-1</sup>	0.05 U μl <sup>-1</sup>	0.76 μl	8.36 μl
Total volume	—	—	76 μl	836 μl

24. Divide the poly(A) tailed RT product (12 μl) into four empty 0.2ml thin wall PCR tubes (3 μl for each tube).
25. Add 19 μl PCR Mix 1 (primer UP2) to each tube (final concentration of UP2 Primer is 0.86 μM). The total volume in the tube is 22 μl.



26. Perform the following PCR program: one cycle of 95 °C for 3 min, 50 °C for 2 min, and 72 °C for 10 min.
27. Put tubes on ice for 1 min.
28. Centrifuge tubes for 30 sec at 7,500 g at 4 °C and immediately place on ice.

**CRITICAL STEP** After this step, the second-strand cDNAs are 5'-UP2-(T)<sub>n</sub>-cDNA-(A)<sub>n</sub>-UP1-3'

### PCR amplification

29. Prepare 76 µl PCR Mix 2 for each reaction by combining and mixing the following components:

Component	Stock Concentration	Final Concentration	×1 Volume	×11 Volume
10X Ex Taq Buffer (with MgCl <sub>2</sub> )	10X	1 X	7.6 µl	83.6 µl
2.5 mM each dNTP	2.5 mM	0.25 mM	7.6 µl	83.6 µl
100 µM UP1 primer	100 µM	1 µM	0.76 µl	8.36 µl
Nuclease-free water	—	—	59.28 µl	652.08 µl
TaKaRa Ex Taq™ HS	5 U µl <sup>-1</sup>	0.05 U µl <sup>-1</sup>	0.76 µl	8.36 µl
Total volume	—	—	76 µl	836 µl

30. Add 19 µl of the PCR Mix 2 to each tube (the final concentration of UP1 and UP2 is 0.46 µM each). The total volume in the tube is 41 µl.
31. Perform the following PCR program: 95 °C for 3 min, then 20 cycles of 95 °C for 30 sec, 67 °C for 1 min, and 72 °C for 6 min (+ 6 sec each cycle).

**PAUSE POINT** The single cell cDNA PCR product can be saved at -80 °C for 6 months.

**CRITICAL STEP** The PCR amplification cycles can be adjusted according to the size (or mRNA content) of the single cell. For a blastomere from a four-cell stage embryo, we use 20 cycles of PCR. For a mature oocyte, we use 18 cycles of PCR.

**CRITICAL STEP** 1<sup>st</sup> cycle = 6 minutes and 6 seconds, 2<sup>nd</sup> cycle = 6 minutes and 12 seconds, 3<sup>rd</sup> cycle = 6 minutes and 18 seconds, etc.

**CRITICAL STEP** After this step, all cDNAs have been amplified.

### Optional DNA purification step—

32. Mix the divided PCR product together (41 µl × 4 = 164 µl for each sample).
33. Take 10 µl of single cell PCR products, add 90 µl Nuclease-free water to dilute ten folds. Take 1 µl (or 2 µl) as template to run a 20 µl SYBR Green real-time PCR reaction to check the expression of house-keeping genes (such as GAPDH, HPRT, β-actin) or specific marker genes (such as H1foo, oog1 for mature oocytes).
34. Purify the remaining 154 µl PCR product with QIAquick PCR Purification Kit, and elute with 50 µl EB buffer.
35. Store at -80 °C.

**PAUSE POINT** The purified PCR product can be saved at  $-80^{\circ}\text{C}$  for 6 months.

### 2nd round of PCR and QC steps—

36. 2<sup>nd</sup> PCR amplification – Set up 4 of the following 90  $\mu\text{l}$  PCR reactions per sample. (Adjust the number of reactions according to the final yield of the cDNA after gel purification.)

Component	Stock Concentration	Final Concentration	$\times 1$ Volume
Purified 1st PCR products	—	—	1.2 $\mu\text{l}$
10X Ex Taq Buffer	10X	1X	9 $\mu\text{l}$
2.5 mM each dNTP	2.5 mM (each)	0.25 mM (each)	9 $\mu\text{l}$
Amine-blocked Universal Primer 1 (AUP1)	100 $\mu\text{M}$	1 $\mu\text{M}$	0.9 $\mu\text{l}$
Amine-blocked Universal Primer 2 (AUP2)	100 $\mu\text{M}$	1 $\mu\text{M}$	0.9 $\mu\text{l}$
Nuclease-free water	—	—	68.1 $\mu\text{l}$
Ex Taq HS	5 $\text{U } \mu\text{l}^{-1}$	0.05 $\text{U } \mu\text{l}^{-1}$	0.9 $\mu\text{l}$
Total volume	—	—	90 $\mu\text{l}$

**CRITICAL STEP** In our experience, with one blastomere of four-cell stage embryo (or 20 pg of input total RNA), four reactions at this step will produce at least 100 ng of gel purified cDNA in the next step.

37. Run the following PCR program:  $95^{\circ}\text{C}$  for 3 min, then 9 cycles of  $95^{\circ}\text{C}$  for 30 sec,  $67^{\circ}\text{C}$  for 1 min, and  $72^{\circ}\text{C}$  for 6 min (+ 6 sec each cycle).

**PAUSE POINT** The 2<sup>nd</sup> round PCR product can be saved at  $-80^{\circ}\text{C}$  for 6 months.

**CRITICAL STEP** The template amount for the 2<sup>nd</sup> round of PCR can be flexible. 1  $\mu\text{l}$  to 4  $\mu\text{l}$  of the purified 1<sup>st</sup> round PCR product can be used for each 90  $\mu\text{l}$  PCR reaction. The PCR amplification cycles can also be adjusted according to the final amount of cDNA needed. The PCR cycles can be between 6 to 12. And cycles of PCR should be minimized to reduce bias. Also, the combined cycles of PCR from the 1<sup>st</sup> and 2<sup>nd</sup> rounds of PCR should be less than 30 cycles.

38. Optional quality check: Combine the four 90  $\mu\text{l}$  PCR reactions. Take 20  $\mu\text{l}$  of the 2<sup>nd</sup> round PCR product to run electrophoresis on a 2% E-Gel.
39. For the remaining 340  $\mu\text{l}$  PCR product, purify the cDNA using Qiaquick PCR purification kit. Elute in 30  $\mu\text{l}$  EB buffer.
40. Store at  $-80^{\circ}\text{C}$ .

**PAUSE POINT** The purified PCR product can be saved at  $-80^{\circ}\text{C}$  for 6 months.

### Gel purification

41. Load the cDNA on 1% agarose gel. Run the gel until the BPB dye is 2 cm from the well. Excise the cDNA from 0.5 kb to 3 kb. Purify the cDNA using Qiaquick gel extraction kit. Elute the cDNA in 30  $\mu\text{l}$  EB buffer. Store at  $-80^{\circ}\text{C}$ . Quantify the cDNA using Qubit and Quant-it HS dsDNA kit.

**PAUSE POINT** The gel purified PCR product can be saved at  $-80^{\circ}\text{C}$  for 6 months.

**CRITICAL STEP** The cDNA is weakly stained because the primer dimer band saturates the ethidium bromide. If this happens, simply cut the gel between 0.5 kb to 3 kb and proceed to gel extraction. Or the operator can stain the gel with ethidium bromide to see the cDNA smear.

**CRITICAL STEP** The AUP1 and AUP2 primers have a NH<sub>2</sub> modification at their 5'-ends that prevents the ligation of the 5'-end fragments of the double-stranded cDNA (after the shearing) to the SOLiD™ library P1/P2 adaptors. Because of this, any undesired small amplification products that may have been formed will not be carried into the library being generated.

42. Optional quality check: If you have enough cDNA to spare and want to check the quality of the gel purified cDNA, run 50 – 100 ng of the purified cDNA on a 2% agarose gel (see Fig. 1).

### SOLiD System *Express* Library Preparation for Fragment Libraries and Multiplexed Fragment Libraries

Workflow (see Fig. 2).

#### Fragment Library Construction Oligonucleotides

**CRITICAL STEP** All library construction oligonucleotides needed for fragment library construction are included in the SOLiD™ Fragment Library Oligo Kit. All multiplexed oligonucleotides must be ordered and hybridized to create double-stranded adaptors (see Table 1).

**CRITICAL STEP** Adjust microcentrifuge speeds and times according to the g-forces specified in the protocols. Applied Biosystems recommends the Eppendorf 5417R tabletop microcentrifuge.

**CRITICAL STEP** All steps requiring the use of 1.5-ml tubes should be done with the 1.5-ml Lo-Bind tubes (Eppendorf, catalog number 022431021).

#### Hybridization of Oligonucleotides

43. Prepare 1 mM stock of individual oligonucleotides.
44. Mix equal volumes of 1 mM oligonucleotide A and B. Add enough 5X Ligase buffer for a final concentration of 1X Ligase buffer.
45. Hybridize the oligonucleotides by running the following program on a PCR machine:

Temperature	Time
95 °C	5 min
72 °C	5 min
60 °C	5 min
50 °C	3 min
40 °C	3 min
30 °C	3 min
20 °C	3 min
10 °C	3 min

Temperature	Time
4 °C	Forever

46. After hybridization, store hybridized oligonucleotides at  $-20\text{ }^{\circ}\text{C}$  until ready for use.

### DNA Shearing using the Covaris™ S2 System

**CRITICAL STEP** Fine tuning the shearing protocol may be necessary for certain DNA samples. However, the following procedures can be used as a guideline when using Covaris™ S2 System. These conditions have been tested for shearing 50 ng- 10  $\mu\text{g}$  of DNA in a total volume of 100  $\mu\text{l}$  in a Covaris™ S2 System. Be sure to use the appropriate tube holder, and program the instrument correspondingly.

**CRITICAL STEP** Set the chiller temperature to between 2-5  $^{\circ}\text{C}$  to ensure the temperature reading in the water bath displays 5  $^{\circ}\text{C}$ . The circulated water chiller should be supplemented with 20% ethylene glycol.

### Shear the DNA

The sonication protocol generates DNA fragments with mean size 100-110 bp (see Fig. 3)

47. In borosilicate glass microTUBE dilute desired number of micrograms of DNA in 100  $\mu\text{l}$  of 10 mM Tris, pH 7.5.

Component	Volume
1-2 $\mu\text{g}$ DNA	x $\mu\text{l}$
1M Tris, pH 7.5	1 $\mu\text{l}$
Nuclease-free water	Variable
Total volume	100 $\mu\text{l}$

48. Shear the DNA using the Covaris™ S2 System shearing program described below:

No. of cycles: 15

Bath Temperature: 5  $^{\circ}\text{C}$

Bath temp limit: 30  $^{\circ}\text{C}$

Mode: Frequency sweeping

Water Quality Testing Function: Off

Treatment 1:

Duty Cycle: 20%

Intensity: 5

Cycles/burst: 200

Time: 60 sec

49. Transfer the sheared DNA into a clean 1.5 ml LoBind tube.

50. For quality control, 2  $\mu\text{l}$  of the reaction should be saved and used to confirm that shearing has created the desired range of fragment sizes using the Agilent 2100 Bioanalyzer.

### Repair the DNA Ends

51. Add to the tube containing sheared DNA the following components:

Component	Volume
Sheared DNA	98 $\mu\text{l}$
10 $\times$ End-it Buffer	14 $\mu\text{l}$
End-it ATP (10 mM)	7 $\mu\text{l}$
End-it dNTPs (2.5 mM)	14 $\mu\text{l}$
End-it Enzyme Mix	2 $\mu\text{l}$
Nuclease-free water	5 $\mu\text{l}$
Total volume	140 $\mu\text{l}$

52. Incubate at room temperature for 30 min.
53. Inactivate End-it Enzymes by transferring tube to the heating block and incubating for 20 min at 65  $^{\circ}\text{C}$ . Centrifuge the tube for 5 sec at 7,500 g at 4  $^{\circ}\text{C}$ .

### Ligate P1 (ds) and P2 (ds) Adapters to End-Repaired DNA

54. Thaw the adapters on ice or at room temperature.
55. Use the information below to calculate the pmoles of adapter needed for the reaction.
- $$1 \mu\text{g DNA} \times 10^6 \text{ pg } \mu\text{g}^{-1} \times 1 \text{ pmol } 660\text{pg}^{-1} \times 1/(\text{average insert fragment size}) = X \text{ pmoles}$$
- $$(\# \mu\text{g DNA}) \times (X \text{ pmoles DNA}) = (\# \text{ pmoles DNA for adapter ligation})$$
- $$(\# \text{ pmoles DNA for adapter ligation}) \times (30) = (\# \text{ pmoles adapters needed})$$
- $$(\# \text{ pmoles adapters needed}) / (\# \text{ pmoles}/\mu\text{l stock}) = (\# \mu\text{l adapter needed})$$
56. In a tube containing the end-repaired DNA from the previous step combine and mix the components below. For DNA inputs higher than 2  $\mu\text{g}$ , scale-up the total volume of the reaction and amount of components (buffer, adaptors, ATP, ligase) correspondingly. Add 1  $\mu\text{l}$  of Quick Ligase per 20  $\mu\text{l}$  of reaction volume. Use one adapter set per sample.

Component	Volume	i.e. Volume for 2 $\mu\text{g}$ input DNA
P1 (ds) Adapter (500 pmol $\mu\text{l}^{-1}$ )	As determined above	1.8 $\mu\text{l}$
P2 (ds) Adapter (500 pmol $\mu\text{l}^{-1}$ )	As determined above	1.8 $\mu\text{l}$
10 $\times$ End-it Buffer	2 $\mu\text{l}$	2 $\mu\text{l}$
End-it ATP (10 mM)	2 $\mu\text{l}$	2 $\mu\text{l}$
Quick Ligase Enzyme (NEB)	8 $\mu\text{l}$	8 $\mu\text{l}$

Component	Volume	i.e. Volume for 2 µg input DNA
End-repaired DNA	140 µl	140 µl
Nuclease-Free Water	Variable	4.4 µl
Total volume	160 µl	160 µl

57. Incubate at room temperature for 10-15min.

### Purification of ligated DNA using Agencourt's Solid Phase Reversible Immobilization (SPRI) purification system

**CRITICAL STEP** Sample purification at the post-ligation step is recommended with the Agencourt® AMPure® Kit. The Agencourt® AMPure® PCR purification system utilizes solid-phase paramagnetic bead technology to purify DNA. The reaction conditions are optimized to selectively bind DNA 100 bp and larger. Excess oligonucleotides, nucleotides, salts and enzymes can be removed by a simple washing procedure. Agencourt® AMPure® purification will remove the 68-bp primer-dimer contamination and reduce carryover of this product into the fragment libraries.

58. Purify ligated DNA using the Agencourt® AMPure® Kit.
- a) Add 1.8× volumes of Agencourt® AMPure® beads to the sample (~160 µl) and incubate for 5 min at room temperature on a rotator
  - b) Prepare 70% ethanol (~650 µl per sample).

**CRITICAL STEP** Using freshly prepared and precisely 70% ethanol is critical, as a higher percentage will result in inefficient washing of smaller-sized molecules and using lower than 70% ethanol could cause loss of sample.

- c) Place the tube of beads in the magnetic rack to separate beads from solution. Wait for the solution to clear before proceeding to the next step.
- d) Remove the supernatant and discard.
- e) Dispense 200 µl of freshly prepared 70% ethanol, vortex the tube thoroughly, and incubate for 30 sec at room temperature.
- f) Place the tube of beads in the magnetic rack to separate beads from solution. Wait for the solution to clear before proceeding to the next step.
- g) Aspirate out the ethanol and discard.
- h) Repeat steps d–g **two** more times.
- i) Place the tube of beads in the magnetic rack and remove the supernatant and pulse-spin to remove the residual ethanol.
- j) Repeat step i **2-3 more times** to remove the residual ethanol.
- k) Dry the beads at room temperature for approximately 5 min.
- l) Elute the DNA by adding 36 µl 10 mM Tris pH 8, vortexing for 10 sec and ensuring homogeneity by pipetting the solution up and down several times.
- m) Place the tube of beads in the magnetic rack to separate beads from solution. Wait for the solution to clear before proceeding to the next step.
- n) Save the eluant in a 1.5 ml LoBind tube.

- o) Place the eluted sample in the magnetic rack again to separate any remaining beads from solution. Wait for the solution to clear before proceeding to the next step.
- p) Save the eluted sample in a new 1.5 ml LoBind tube.
- q) Repeat steps p-q **once**.
- r) Store DNA in a 1.5 ml LoBind tube.
- s) Save 2  $\mu\text{l}$  of the AMPure®-purified ligated library DNA. The aliquot can be used for running a library QC for troubleshooting purposes.

**PAUSE POINT** The sample(s) may be stored at  $-20^{\circ}\text{C}$ .

### For Multiplexed Samples

**CRITICAL STEP** Using Qubit (following manufacturer's protocol) or qPCR (see Steps 66-71) determine the concentration of each of the multiplexed samples. Pool equal concentrations of the samples and purify with AMPure beads as above, eluting with 34  $\mu\text{l}$  of 10 mM Tris, pH 8 solution and continue with nick translation. If necessary, after nick translation PCR amplification can be performed on individual samples, or on pooled samples, as long as the pooled samples are equal in concentration to each other.

**CRITICAL STEP** For fragment libraries or multiplexed libraries that are not yet pooled, the operator may skip quantitation and go directly on to nick translation—pooling before nick translation is primarily to conserve reagents.

### Nick-Translation of the DNA

59. Combine and mix the following components in a LoBind tube:

Component	Volume
P1 (ds) and P2 (ds) adapter ligated fragment DNA	34 $\mu\text{l}$
10 $\times$ NEBuffer 2	4 $\mu\text{l}$
GeneAmp® dNTP Blend (100mM)	0.8 $\mu\text{l}$
DNA Polymerase I (10 U $\mu\text{l}^{-1}$ )	1.0 $\mu\text{l}$
Nuclease-free water	Variable
Total volume	40 $\mu\text{l}$

60. Incubate at 16  $^{\circ}\text{C}$  for 30 min.
61. Stop the reaction by adding 0.5 $\mu\text{l}$  0.5 M EDTA pH8.0
62. Purify the nick-translated DNA with the the Agencourt® AMPure® Kit as before, eluting with 40  $\mu\text{l}$  of a 10 mM Tris, pH 8.0 solution.

**CRITICAL STEP** Save 2  $\mu\text{l}$  of the AMPure®-purified ligated library DNA. The aliquot can be used for running a library QC for troubleshooting purposes.

**PAUSE POINT** The sample(s) may be stored at  $-20^{\circ}\text{C}$ .

**CRITICAL STEP** Proceed to qPCR to quantify library molecules bearing P1 and P2 adaptors. If the library concentration is too low for emulsion PCR (it should be above 1 ng  $\mu\text{l}^{-1}$ ) continue with PCR, otherwise begin emulsion PCR.



### Quantification of library by qPCR

**CRITICAL STEP** Quantitative PCR is performed using real-time SYBR Green assay. For multiplexed samples that need to be pooled, normalize the Ct values and pool accordingly. For determining relative concentrations of the samples, two titration points are adequate per multiplexed sample.

**CRITICAL STEP** For the final pooled multiplexed library, Qubit may be used to determine the final concentration of the pooled samples, following the manufacturers' protocol. For a fragment library sample, either Qubit or qPCR may be used to determine the final concentration. For qPCR of fragment libraries, a Standard Library is used to generate a standard curve.

**CRITICAL STEP** For quantitating samples for pooling, make sure all samples are done on the same plate to avoid variation that can occur between plates and instruments.

63. Prepare serial 10-fold dilutions of the library eluted in EB:
  - $10^{-1}$ : 3  $\mu$ l of eluted library + 27  $\mu$ l H<sub>2</sub>O,
  - $10^{-2}$ : 5  $\mu$ l of  $10^{-1}$  + 45  $\mu$ l H<sub>2</sub>O,
  - etc. down to  $10^{-6}$
64. Prepare Standard samples containing 390 fg, 39 fg, 3.9 fg, 0.39 fg, and 0.039 fg of Standard Library (*E.coli* DH10B fragment library, 150 bp mean fragment size) in 5  $\mu$ l H<sub>2</sub>O. These values should be used for absolute quantification when programming the 7900HT Fast Real-Time PCR System to generate a Standard Curve.

**CRITICAL STEP** Both AB's and Invitrogen's SYBR Green Mixes work well. Assay is performed in a standard 96-well plate from Applied Biosystems.

qPCR Assay Pre-Mix using SYBR Green PCR Master Mix (AB, Cat. No 4309155)\*

For one reaction:

	Final concentration	$\times 1$ volume
2 $\times$ SYBR Green Master Mix (ABI)	1 $\times$	15 $\mu$ l
qPCR primer Fw (50 $\mu$ M)	0.9 $\mu$ M	0.54 $\mu$ l
qPCR primer Rev (50 $\mu$ M)	0.9 $\mu$ M	0.54 $\mu$ l
H <sub>2</sub> O		8.92 $\mu$ l
Total volume		25 $\mu$ l

\* ROX already pre-mixed in Master Mix

65. Distribute 25  $\mu$ l Pre-Mix in corresponding wells. Then add 5  $\mu$ l of template DNA (or H<sub>2</sub>O for NTC). Seal the plate with adhesive optical cover. The total volume of PCR reaction is 30  $\mu$ l.
66. When using Absolute Quantification with 7900HT Fast Real-Time PCR System, set up the following thermal profile:

95°C	2min	
95°C	15sec	40 cycles
62°C	15 sec	
70°C	1min	

Also set:

Thermal Cycler Protocol Mode: Standard

Data Collection: at 70 °C (extension step)

67. Run qPCR and quantify the amount of library DNA/number of P1-insert-P2 molecules. Typical Standard curve and Amplification plots for Standards and Library samples are shown in Fig. 4.
68. Proceed to emulsion PCR step if sample concentration(s) adequate. Otherwise continue with PCR amplification, steps 69-71.

#### (Optional) PCR Amplification

69. Perform minimal cycles of PCR as follows below. 25 µl of a sample, either a multiplexed pool of samples or a single multiplexed sample, is amplified using the following protocol:

Component	Volume
Multiplexed sample	25 µl
Invitrogen™ SuperMix	75 µl
16Barcode Library PCR Primer 1	1.5 µl
16Barcode Library PCR Primer 2	1.5 µl
Pfu polymerase	0.25 µl
AmpliTaq	0.2 µl
Total volume	103.45 µl

Temperature	Time	Condition/note
95 °C	5 min	Hold
95 °C	15 sec	8-16 cycles
62 °C	15 sec	
70 °C	1 min	
70 °C	5 min	Hold
4 °C	Forever	Hold

**CRITICAL STEP** The number of cycles should be decided based on the amount of starting material used for shearing. Minimal cycling is desirable for avoiding over-amplification. Use the table below as a guideline to determine the number of PCR cycles based on the amount of input DNA:

Starting Amount of DNA	Number of PCR Cycles
1 µg to 2 µg	8-10
100 ng to 1 µg	10-12
20 ng to 100 ng	13-16

- 70.** To determine if amplification was adequate, load and run 4 µl of sample on a 2.2% Lonza FlashGel® cassette for 6 min at 275 V to ensure amplification after a minimal number of cycles as described above.
- 71.** If fairly robust amplification products are visible, proceed with Step 72. If little or no amplification products are observed at this point, return the tubes to the thermal cycler and run the PCR cycling program below:

Temperature	Time	Condition
95 °C	5 min	Hold
95 °C	15 sec	X 2-3 cycles
62 °C	15 sec	
70 °C	1 min	
70 °C	5 min	Hold
4 °C	Forever	Hold

- 72.** Repeat AMPure purification as in step 58.
- 73.** Quantify sample(s) with either Qubit quantitation or qPCR.

## TIMING

- Day 1: Step 1 - 2: 1 h  
 Step 3 - 11: 1 h  
 Step 12 - 16: 1.5 h  
 Step 17 - 21: 1 h  
 Step 22 - 27: 0.5h  
 Step 28 - 30: 5h
- Day 2: Step 31 - 34: 3 - 7 h
- Day 3: Step 35 - 36: 3 h  
 Step 37 - 39: 3h
- Day 4: Step 40: 5h  
 Step 41: 1.5h
- Day 5:  
 Step 43-46: 0.5 h  
 Step 47-50: 0.5-1 h if Bioanalyzer used

Step 51-53: 1 h

Step 54-57: 0.3 h

Step 58: Time depends on sample numbers. For 16 samples, about 1 h

Step 59-61: 0.5 h

Step 62: Time depends on sample numbers. For 16 samples, about 1 h

Step 63-68: 2 h

Day 6:

Step 69-71 (optional): 1 h

Step 72: Time depends on sample numbers. For 16 samples, about 1 h

Step 73: 2 h if using qPCR

## TROUBLESHOOTING

Problem	Possible reason	Solution
Cell not transferred into lysis tube	Cell stuck to the inside wall of the glass capillary (micropipette)	First suck a small volume of PBS-BSA using the mouse pipette, then suck the single cell into the glass capillary gently to keep the cell already inside the capillary but still near the tip of the capillary. When pushing the cell out of the capillary into the lysis, push all the carryover PBS-BSA until a bubble is visible from the capillary into the lysis buffer.
Picking buffer only control shows positive signal when using real-time PCR to check expression of house-keeping genes	PBS-BSA drop is contaminated by lysed cells	Make sure the PBS-BSA drop for holding single cells is not contaminated by lysed cells. Wash the single cells through several PBS-BSA drops before picking them. Aliquot all reagents for lysis, RT, cutting, tailing, and PCR steps in small batches. Each aliquot is only used once and the remainder is discarded. Also only load the exact number of single cells that will be picked into the final PBS-BSA drop. After picking each of them, check the number of remaining single cells to make sure every cell is correctly picked and no cell is by chance lysed or incorrectly picked.
The expression level of house-keeping genes is much lower than expected in some single cell cDNA samples.	Some dead or partially damaged single cells were picked	Before picking, try to check the quality of the single cells by either morphology or trypan blue staining. Only pick healthy single cells.
	RNase contamination during the lysate and reverse transcription step	Keep the bench and surrounding area very clean. Wear a dust mask to avoid breathing contaminants into reaction reagents. Change gloves regularly during these steps. Try to do all manipulations in a clean hood.
Low recovery of gel purification	Loss of activity of some enzymes and reagents	Some of the reagents are not very stable, such as dATP, dNTP, or primers at low concentrations. Aliquot them into small batches. Avoid repeated freeze/thaws. Make sure reagents are not expired.
	Gel fragment recovered more than the kit requested	Try to cut the gel fragment containing the cDNA smear more accurately. If too much gel is already cut, split them into two gel purification columns and finally combine the purified cDNAs. Each QIAGEN column can hold up to 400 mg of gel.
Primer dimers present on Lonza Gel in step 70	Too many cycles of PCR were done, or the amount of adaptors added was too large relative to sample size	Gel purification must be done to remove primer dimers. SOLiD Fragment Library protocol recommends the use of 3% or 4% agarose gel run in 1X TAE, using a 25 bp Track-It ladder as reference. Cut the gel between 125 bp and 200 bp and purify using QIAGEN MinElute Gel Extraction Kit following manufacturer's instructions.
Size distribution of fragment after	Sonication protocol was not calibrated correctly for the sample	Readjust shearing protocol and redo shearing. Make sure the Covaris S2 System is properly set up.

Problem	Possible reason	Solution
shearing is not in the desired range		
Low yield after AMPure purification	Ethanol was not freshly prepared, and/or was not at 70%	If there is adequate sample remaining, PCR can be done to increase the quantity, see steps 69-72. If not, protocol must be redone, using freshly prepared 70% ethanol.
Overall yield is low	Sample quality was poor	Confirm quality of sample before beginning Express protocol using a housekeeping gene assay, or use Qubit to confirm that the sample's concentration is adequate for input.
	Sample loss occurred during AMPure purification	See above. Check QC aliquots using Qubit or NanoDrop to determine where loss occurred.
	Loss of sample can occur during steps when sample is transferred or purified	Take care to transfer the entire volume during purification steps and minimize transferring of samples. Sample input may need to be increased if initial input was low and loss occurs.

## ANTICIPATED RESULTS

We first used relatively small cells—mouse embryonic stem (ES) cells—to show that the method is sensitive and reproducible, and we picked into each tube either one individual ES cell or ten ES cells together (Fig. 5). Then we ran the single cell cDNA amplification procedure and ran real-time PCR to analyze the expression of house-keeping genes, GAPDH. (Fig. 6).

Then we confirmed the accuracy of the method by analyzing the correlation efficiency between two separately processed biological replicates. Based on our previous single cell cDNA microarray results (unpublished) and results from other labs, undifferentiated ES cells have strong subpopulations with dramatic differences in gene expression<sup>43-45</sup>. So we analyzed biological replicates of mature oocytes, as we know that mature oocytes are a much more homogeneous population<sup>40</sup>. We can achieve correlation coefficients as high as 0.986 (Fig. 7). The coverage plots<sup>40</sup> of several individual genes are shown in Fig. 8. The top 20 most abundant genes<sup>40</sup> in the mature oocyte and the blastomere of a 4-cell stage embryo respectively are shown in Table 2.


## References

1. Wang Z, Gerstein M, Snyder M. RNA-Seq: a revolutionary tool for transcriptomics. *Nat. Rev. Genet.* 2009; 10:57–63. [PubMed: 19015660]
2. Cloonan N, Grimmond SM. Transcriptome content and dynamics at single-nucleotide resolution. *Genome Biol.* 2008; 9:234. [PubMed: 18828881]
3. Schena M, Shalon D, Davis RW, Brown PO. Quantitative monitoring of gene expression patterns with a complementary DNA microarray. *Science.* 1995; 270:467–470. [PubMed: 7569999]
4. DeRisi J, et al. Use of a cDNA microarray to analyse gene expression patterns in human cancer. *Nat. Genet.* 1996; 14:457–460. [PubMed: 8944026]
5. Lockhart DJ, et al. Expression monitoring by hybridization to high-density oligonucleotide arrays. *Nat. Biotechnol.* 1996; 14:1675–1680. [PubMed: 9634850]
6. Duggan DJ, Bittner M, Chen Y, Meltzer P, Trent JM. Expression profiling using cDNA microarrays. *Nat. Genet.* 1999; 21:10–14. [PubMed: 9915494]
7. Lipshutz RJ, Fodor SP, Gingeras TR, Lockhart DJ. High density synthetic oligonucleotide arrays. *Nat. Genet.* 1999; 21:20–24. [PubMed: 9915496]
8. Blackshaw S, Livesey R. Applying genomics technologies to neural development. *Curr. Opin. Neurobiol.* 2002; 12:110–114. [PubMed: 11861173]
9. Mardis ER. The impact of next-generation sequencing technology on genetics. *Trends Genet.* 2008; 24:133–141. [PubMed: 18262675]


10. Wold B, Myers RM. Sequence census methods for functional genomics. *Nat. Methods*. 2008; 5:19–21. [PubMed: 18165803]
11. Schuster SC. Next-generation sequencing transforms today's biology. *Nat. Methods*. 2008; 5:16–18. [PubMed: 18165802]
12. Shendure J. The beginning of the end for microarrays? *Nat. Methods*. 2008; 5:585–587. [PubMed: 18587314]
13. Wilhelm BT, et al. Dynamic repertoire of a eukaryotic transcriptome surveyed at single-nucleotide resolution. *Nature*. 2008; 453:1239–1243. [PubMed: 18488015]
14. Nagalakshmi U, et al. The transcriptional landscape of the yeast genome defined by RNA sequencing. *Science*. 2008; 320:1344–1349. [PubMed: 18451266]
15. Sultan M, et al. A global view of gene activity and alternative splicing by deep sequencing of the human transcriptome. *Science*. 2008; 321:956–960. [PubMed: 18599741]
16. Wang ET, et al. Alternative isoform regulation in human tissue transcriptomes. *Nature*. 2008; 456:470–476. [PubMed: 18978772]
17. Cloonan N, et al. Stem cell transcriptome profiling via massive-scale mRNA sequencing. *Nat. Methods*. 2008; 5:613–619. [PubMed: 18516046]
18. Mortazavi A, Williams BA, McCue K, Schaeffer L, Wold B. Mapping and quantifying mammalian transcriptomes by RNA-Seq. *Nat. Methods*. 2008; 5:621–628. [PubMed: 18516045]
19. Marioni JC, Mason CE, Mane SM, Stephens M, Gilad Y. RNA-seq: an assessment of technical reproducibility and comparison with gene expression arrays. *Genome Res*. 2008; 18:1509–1517. [PubMed: 18550803]
20. Pan Q, Shai O, Lee LJ, Frey BJ, Blencowe BJ. Deep surveying of alternative splicing complexity in the human transcriptome by high-throughput sequencing. *Nat. Genet*. 2008; 40:1413–1415. [PubMed: 18978789]
21. Li H, et al. Determination of tag density required for digital transcriptome analysis: application to an androgen-sensitive prostate cancer model. *Proc. Natl. Acad. Sci. USA*. 2008; 105:20179–20184. [PubMed: 19088194]
22. Blake WJ, KAern M, Cantor CR, Collins JJ. Noise in eukaryotic gene expression. *Nature*. 2003; 422:633–637. [PubMed: 12687005]
23. Raser JM, O'Shea EK. Noise in gene expression: origins, consequences, and control. *Science*. 2005; 309:2010–2013. [PubMed: 16179466]
24. Arias AM, Hayward P. Filtering transcriptional noise during development: concepts and mechanisms. *Nat. Rev. Genet*. 2006; 7:34–44. [PubMed: 16369570]
25. Raj A, van Oudenaarden A. Nature, nurture, or chance: stochastic gene expression and its consequences. *Cell*. 2008; 135:216–226. [PubMed: 18957198]
26. Losick R, Desplan C. Stochasticity and cell fate. *Science*. 2008; 320:65–68. [PubMed: 18388284]
27. Shahrezaei V, Swain PS. The stochastic nature of biochemical networks. *Curr. Opin. Biotechnol*. 2008; 19:369–374. [PubMed: 18662776]
28. Kawasaki ES. Microarrays and the gene expression profile of a single cell. *Ann. N Y Acad. Sci*. 2004; 1020:92–100. [PubMed: 15208186]
29. Livesey FJ. Strategies for microarray analysis of limiting amounts of RNA. *Brief. Funct. Genomic Proteomic*. 2003; 2:31–36. [PubMed: 15239941]
30. Iscove NN, et al. Representation is faithfully preserved in global cDNA amplified exponentially from sub-picogram quantities of mRNA. *Nat. Biotechnol*. 2002; 20:940–943. [PubMed: 12172558]
31. Klein CA, et al. Combined transcriptome and genome analysis of single micrometastatic cells. *Nat. Biotechnol*. 2002; 20:387–392. [PubMed: 11923846]
32. Hamatani T, Carter MG, Sharov AA, Ko MS. Dynamics of global gene expression changes during mouse preimplantation development. *Dev. Cell*. 2004; 6:117–131. [PubMed: 14723852]
33. Wang QT, et al. A genome-wide study of gene activity reveals developmental signaling pathways in the preimplantation mouse embryo. *Dev. Cell*. 2004; 6:133–144. [PubMed: 14723853]
34. Zeng F, Baldwin DA, Schultz RM. Transcript profiling during preimplantation mouse development. *Dev. Biol*. 2004; 272:483–96. [PubMed: 15282163]

35. Hartmann CH, Klein CA. Gene expression profiling of single cells on large-scale oligonucleotide arrays. *Nucleic Acids Res.* 2006; 34:e143. [PubMed: 17071717]
36. Jensen KB, Watt FM. Single-cell expression profiling of human epidermal stem and transit-amplifying cells: *Lrig1* is a regulator of stem cell quiescence. *Proc. Natl. Acad. Sci. U S A.* 2006; 103:11958–11963. [PubMed: 16877544]
37. Bontoux N, et al. Integrating whole transcriptome assays on a lab-on-a-chip for single cell gene profiling. *Lab Chip.* 2008; 8:443–450. [PubMed: 18305863]
38. Kurimoto K, et al. An improved single-cell cDNA amplification method for efficient high-density oligonucleotide microarray analysis. *Nucleic Acids Res.* 2006; 34:e42. [PubMed: 16547197]
39. Kurimoto K, Yabuta Y, Ohinata Y, Saitou M. Global single-cell cDNA amplification to provide a template for representative high-density oligonucleotide microarray analysis. *Nat Protoc.* 2007; 2:739–752. [PubMed: 17406636]
40. Tang F, et al. mRNA-Seq whole-transcriptome analysis of a single cell. *Nat. Methods.* 2009; 6:377–382. [PubMed: 19349980]
41. Tang F, et al. 220-plex microRNA expression profile of a single cell. *Nat. Protoc.* 2006; 1:1154–1159. [PubMed: 17406397]
42. Nagy, A.; Gertsenstein, M.; Vintersten, K.; Behringer, R. *Manipulating the mouse embryo.* 3rd ed. Cold Spring Harbor Laboratory Press; Cold Spring Harbor, NY: 2003. p. 194-200.
43. Chambers I, et al. Nanog safeguards pluripotency and mediates germline development. *Nature.* 2007; 450:1230–1234. [PubMed: 18097409]
44. Toyooka Y, Shimosato D, Murakami K, Takahashi K, Niwa H. Identification and characterization of subpopulations in undifferentiated ES cell culture. *Development.* 2008; 135:909–918. [PubMed: 18263842]
45. Hayashi K, Lopes SM, Tang F, Surani MA. Dynamic equilibrium and heterogeneity of mouse pluripotent stem cells with distinct functional and epigenetic states. *Cell Stem Cell.* 2008; 3:391–401. [PubMed: 18940731]




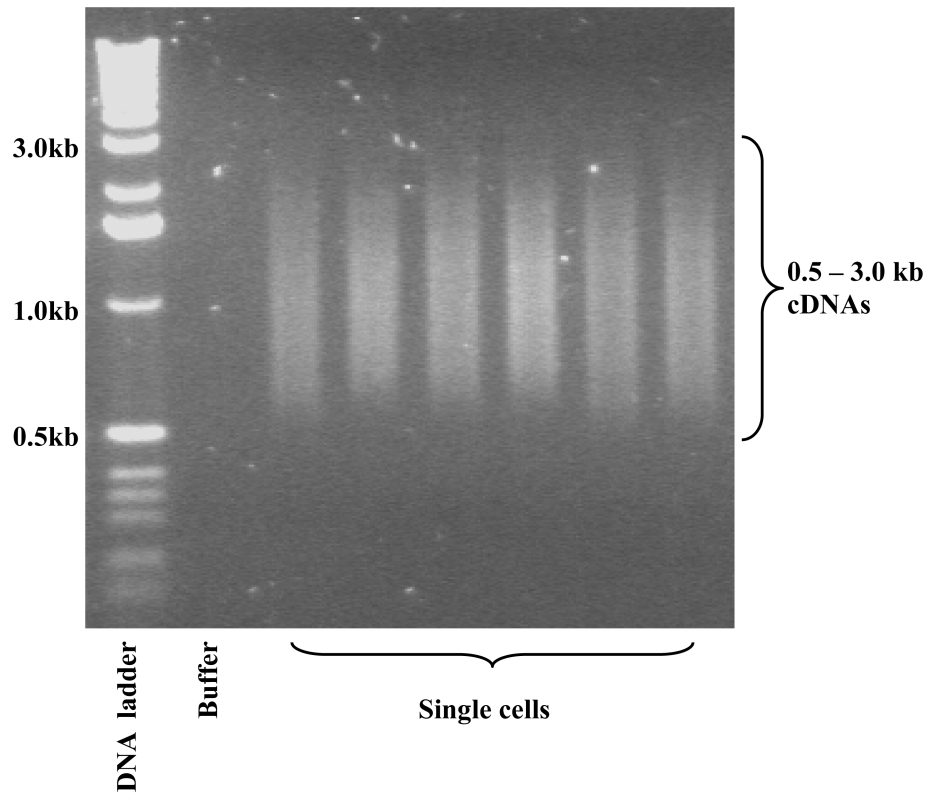


**Figure 1.** Typical agarose gel electrophoresis for single cell cDNAs after 20 + 9 cycles of PCR and gel purification.

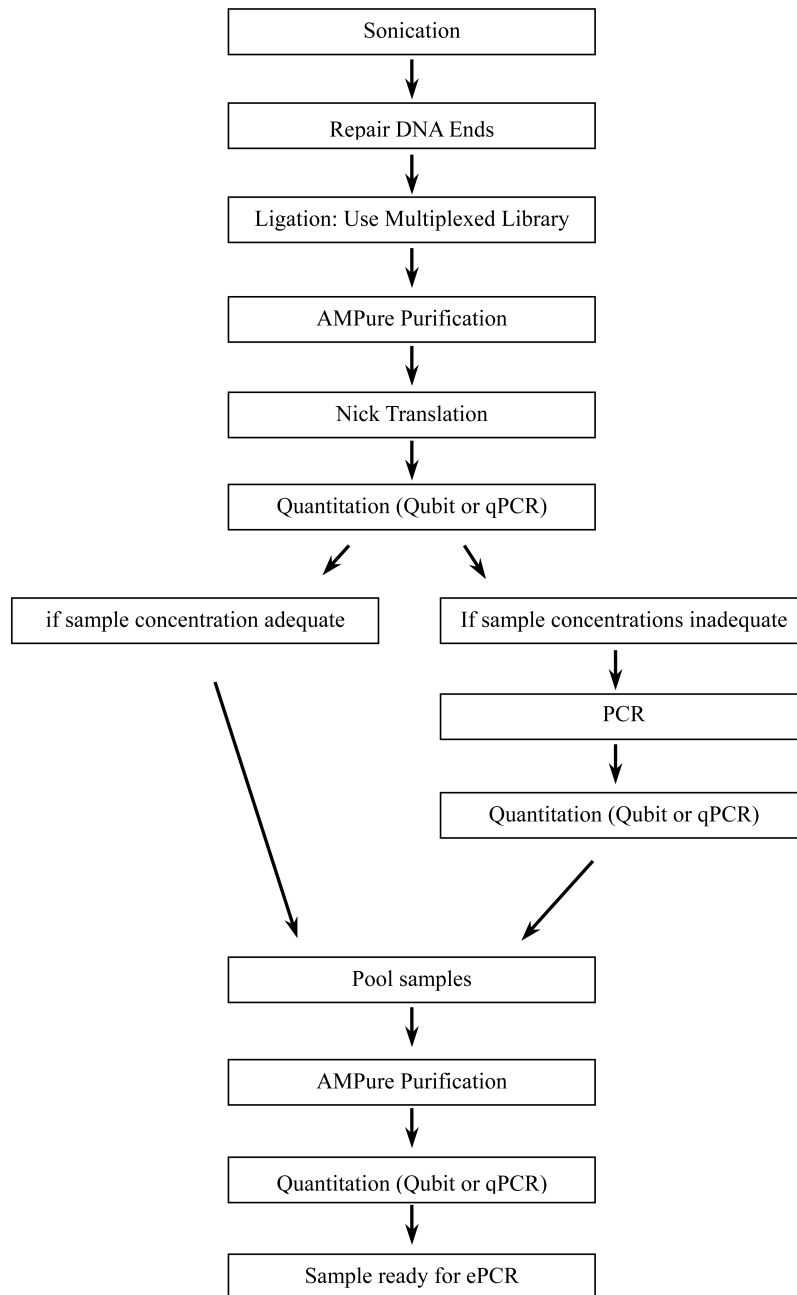

**Figure 2. Workflow of the SOLiD System Express Library Preparation for Fragment Libraries and Multiplexed Fragment Libraries.**

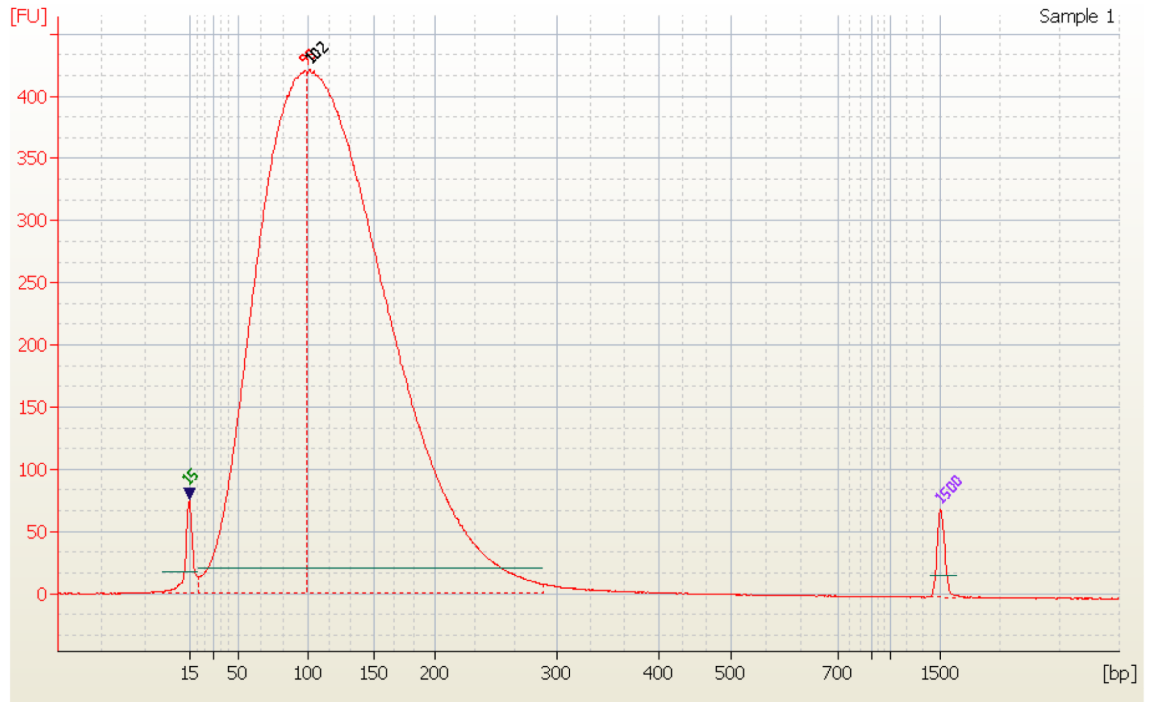


**Figure 3. Electropherogram of DNA sheared in C4011-10 tubes generated using Bioanalyzer (Agilent Technologies, Inc.)**

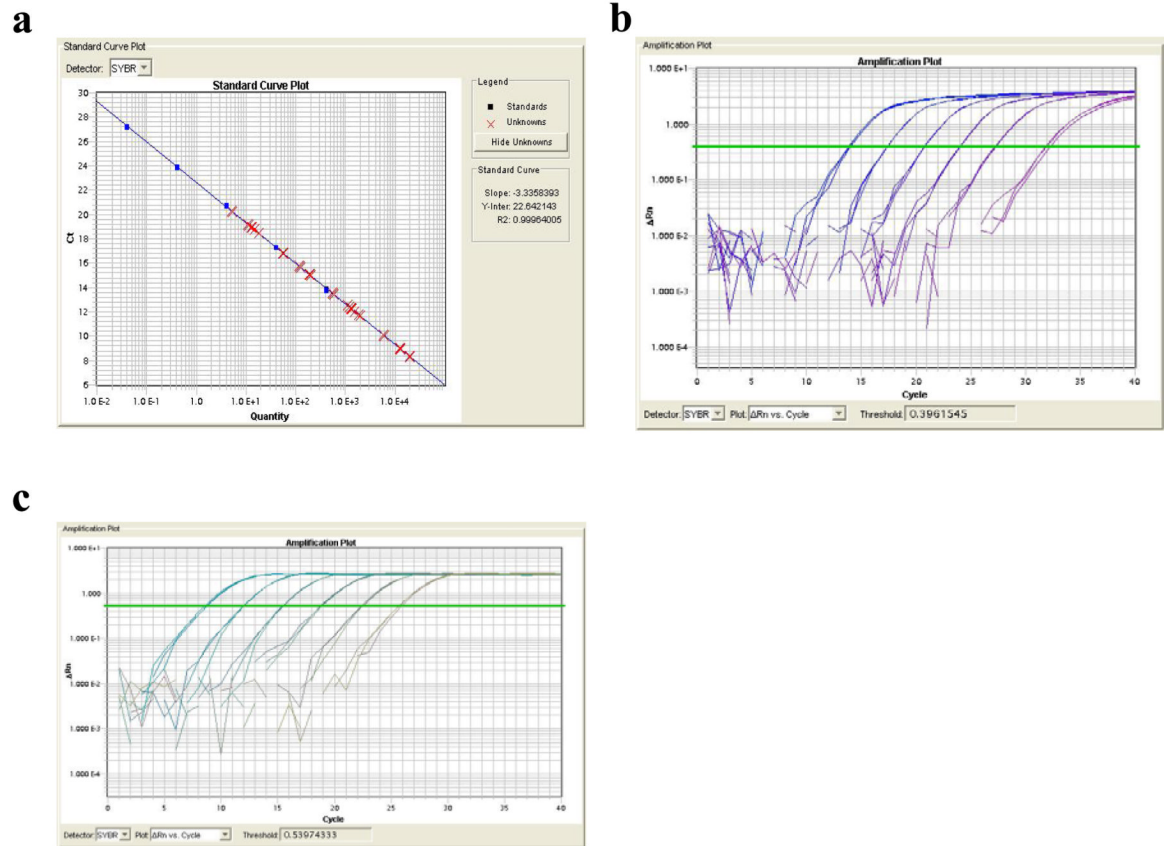


**Figure 4. Standard curve of the cDNAs.**

(a) Standard curve. (b) Standard plot. (c) Library plot.

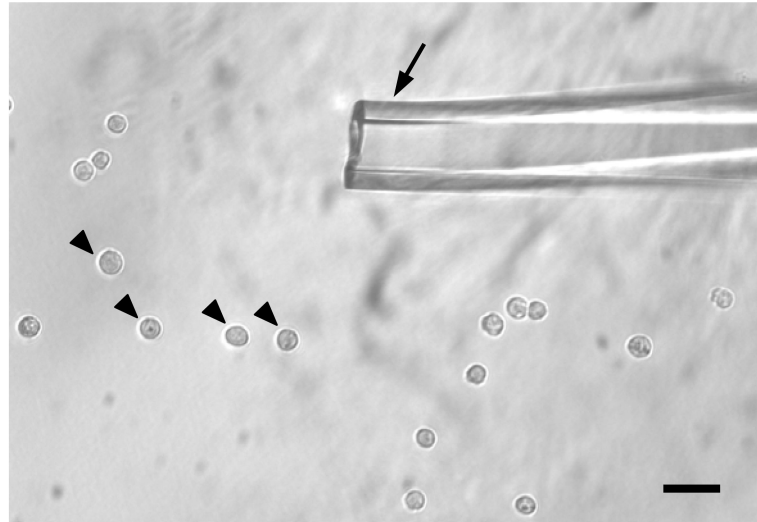


**Figure 5. The single ES cells in PBS-BSA drop.**

Black arrowheads indicate individual ES cells. Black arrow indicates the tip of micropipette for picking single cells. The inner diameter of the micropipette is about 2 – 3 fold of the diameter of an individual ES cell. Scale bar: 30um.

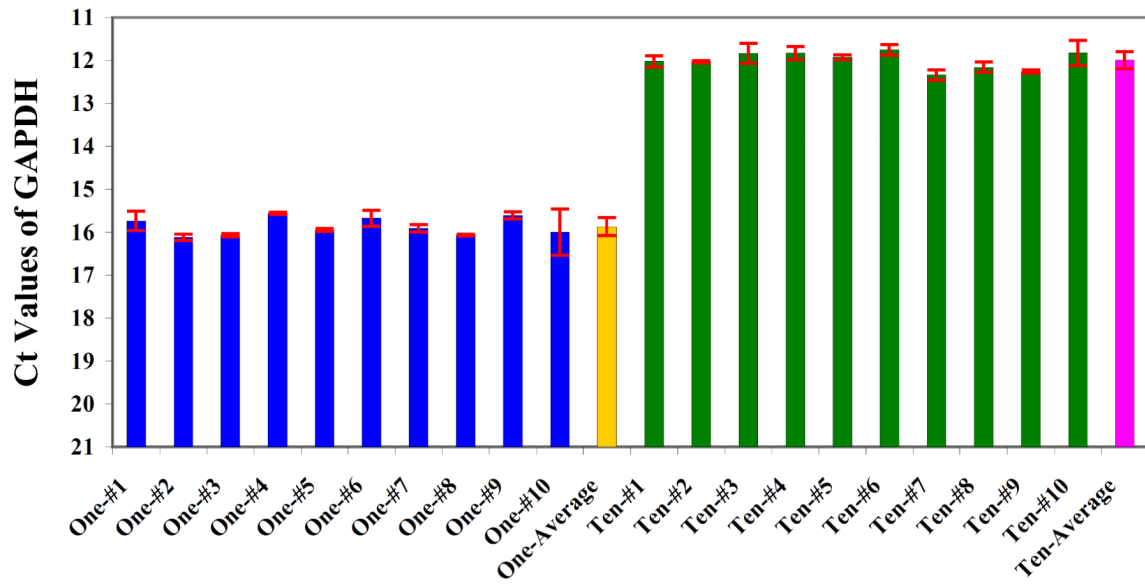


**Figure 6. GAPDH expression in single and ten mouse ES cells measured by real-time PCR.** One or ten ES cells were picked into each tube to amplify cDNAs by 20 cycles of PCR. Then the PCR product was diluted 10 fold (20ul into 200ul) and take 2ul as template for a 20ul real-time PCR reaction.

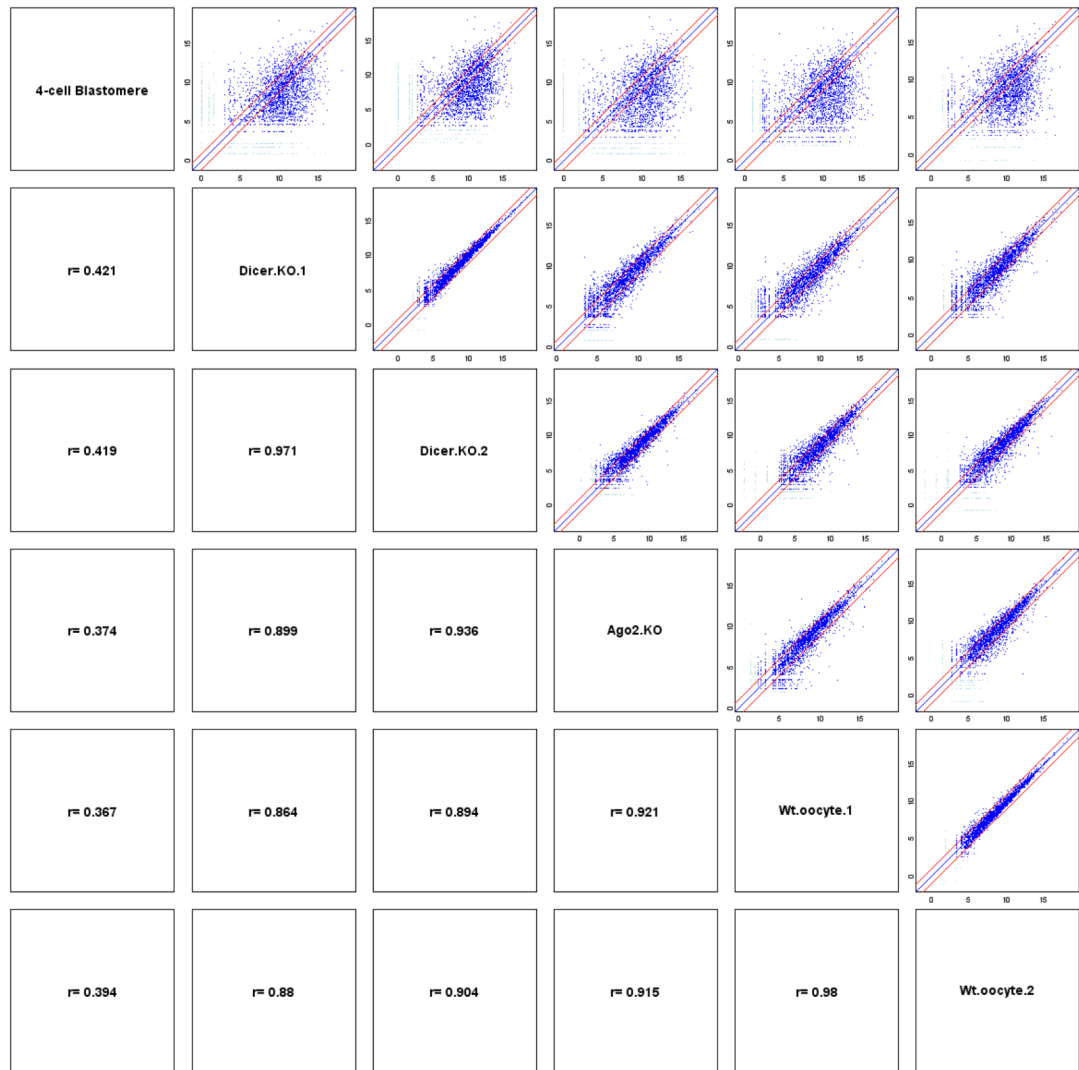

**Figure 7. Pearson coefficient plots for single cell RNA-Seq of one blastomere of a 4-cell stage embryo, two wildtype mature oocytes, two Dicer knockout mature oocytes, and one Ago2 knockout mature oocyte.**



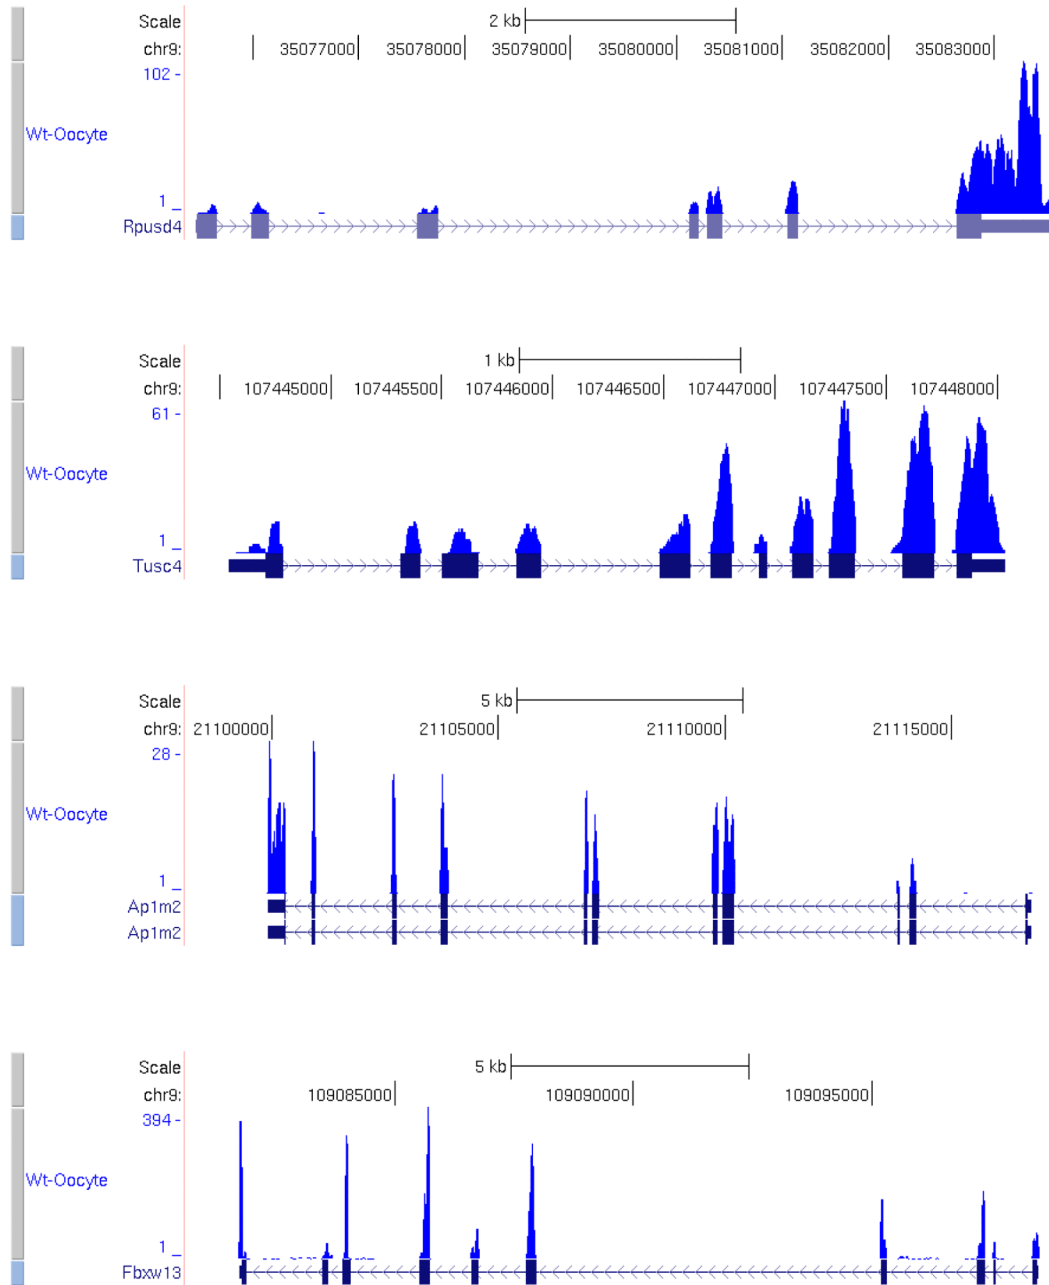

**Figure 8. Coverage plots of RNA-Seq reads in a single wildtype mature oocyte.**

**Table 1**  
**All oligos needed for the single cell RNA-Seq protocol.**

Oligo Name	Oligo Sequence (all oligos sequence read 5'-->3')
UP1	ATATGGATCCGGCGCGCCGTCGACTTTTTTTTTTTTTTTTTTTTTT
UP2	ATATCTCGAGGGCGCGCCGATCCTTTTTTTTTTTTTTTTTTTTTT
AUP1	(NH2)ATATGGATCCGGCGCGCCGTCGACTTTTTTTTTTTTTTTTTTTT
AUP2	(NH2)ATATCTCGAGGGCGCGCCGATCCTTTTTTTTTTTTTTTTTTTTTT
Fragment Library P1 PCR Primer	CCACTACGCCTCCGCTTTCCTCTCTATG
Fragment Library P2 PCR Primer	
Fragment Library P1 Adaptor -5'end	CCACTACGCCTCCGCTTTCCTCTCTATGGGCAGTCGGTGAT
Fragment Library P1 Adaptor 3' end	ATCACCGACTGCCCATAGAGAGAAAGCGGAGGCGTAGTGGTT
Fragment Library P2 Adaptor 5' end	AGAGAATGAGGAACCCGGGGCAGTT
Fragment Library P2 Adaptor 3' end	CTGCCCCGGGTTCTCATTCTCT
P1-Adaptor-5-end	ATCACCGACTGCCCATAGAGAGTT
P1-Adaptor-3-end	CCTCTCTATGGGCAGTCGGTGAT
P2-Bar-1-5-end	CGCCTTGGCCGTACAGCAGGGCTTAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-1-3-end	CTGCCCCGGGTTCTCATTCTCTAAGCCCTGCTGTACGGCCAAGGCG
P2-Bar-2-5-end	CGCCTTGGCCGTACAGCAGGGTGTGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-2-3-end	CTGCCCCGGGTTCTCATTCTCTCACACCTGCTGTACGGCCAAGGCG
P2-Bar-3-5-end	CGCCTTGGCCGTACAGCAGAAGGGGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-3-3-end	CTGCCCCGGGTTCTCATTCTCTCCCCTTCTGCTGTACGGCCAAGGCG
P2-Bar-4-5-end	CGCCTTGGCCGTACAGCAGCCGATGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-4-3-end	CTGCCCCGGGTTCTCATTCTCTCATCGGCTGCTGTACGGCCAAGGCG
P2-Bar-5-5-end	CGCCTTGGCCGTACAGCAGCAACGAAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-5-3-end	CTGCCCCGGGTTCTCATTCTCTTCGTTGCTGTGTACGGCCAAGGCG
P2-Bar-6-5-end	CGCCTTGGCCGTACAGCAGGTGCCAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-6-3-end	CTGCCCCGGGTTCTCATTCTCTGGGCACCTGCTGTACGGCCAAGGCG
P2-Bar-7-5-end	CGCCTTGGCCGTACAGCAGGTCTGGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-7-3-end	CTGCCCCGGGTTCTCATTCTCTCCAGACCTGCTGTACGGCCAAGGCG
P2-Bar-8-5-end	CGCCTTGGCCGTACAGCAGACGGAGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-8-3-end	CTGCCCCGGGTTCTCATTCTCTCCGTCTGCTGTACGGCCAAGGCG
P2-Bar-9-5-end	CGCCTTGGCCGTACAGCAGGAAGGGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-9-3-end	CTGCCCCGGGTTCTCATTCTCTCCCTTCTGCTGTACGGCCAAGGCG
P2-Bar-10-5-end	CGCCTTGGCCGTACAGCAGGACCGCAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-10-3-end	CTGCCCCGGGTTCTCATTCTCTGCGGTCCTGCTGTACGGCCAAGGCG
P2-Bar-11-5-end	CGCCTTGGCCGTACAGCAGCTCAGGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-11-3-end	CTGCCCCGGGTTCTCATTCTCTCCTGAGCTGCTGTACGGCCAAGGCG
P2-Bar-12-5-end	CGCCTTGGCCGTACAGCAGAGCGTTAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-12-3-end	CTGCCCCGGGTTCTCATTCTCTAACGCTCTGCTGTACGGCCAAGGCG
P2-Bar-13-5-end	CGCCTTGGCCGTACAGCAGCGGTCAGAGAATGAGGAACCCGGGGCAGTT

Oligo Name	Oligo Sequence (all oligos sequence read 5'-->3')
P2-Bar-13-3-end	CTGCCCCGGGTTCTCATTCTCTGACCCGCTGCTGTACGGCCAAGGCG
P2-Bar-14-5-end	CGCCTGGCCGTACAGCAGCGTCTGAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-14-3-end	CTGCCCCGGGTTCTCATTCTCTCAGACGCTGCTGTACGGCCAAGGCG
P2-Bar-15-5-end	CGCCTGGCCGTACAGCAGTAGCGTAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-15-3-end	CTGCCCCGGGTTCTCATTCTCTACGCTACTGCTGTACGGCCAAGGCG
P2-Bar-16-5-end	CGCCTGGCCGTACAGCAGGCGTTTAGAGAATGAGGAACCCGGGGCAGTT
P2-Bar-16-3-end	CTGCCCCGGGTTCTCATTCTCTAAACGCCTGCTGTACGGCCAAGGCG
16Barcode Library PCR Primer-1	CCACTACGCCTCCGCTTTCCTCTCTATGGGCAGTCGGTGAT
16Barcode Library PCR Primer-2	CTGCCCCGGGTTCTCATTCT

Please refer to the web version for colour-coding.

Red – indicates barcode sequence

Green – 16Barcode Library PCR Primer-2 sequence for amplification during emulsion PCR

Blue – segment of 16Barcode Library PCR Primer-1 that matches P1 adapter

**Table 2**  
**Top 20 most abundant genes in the mature oocyte and the blastomere of 4-cell stage embryos, respectively.**

Gene name	RefSeq ID	Relative counts in mature oocyte	Relative counts in 4-cell Blastomere
H1foo	NM_138311	209,872	2,117
Bcl2l10	NM_013479	205,060	1,027
Spin1	NM_011462	200,333	23,757
Gdf9	NM_008110	165,482	14,100
Obox1	NM_027802	149,944	2,247
Oog1	NM_178657	136,086	100,086
Tel1b2	NM_013775	131,326	76,552
Tel1	NM_009337	129,237	22,122
Omt2b	NM_205822	122,678	258,088
Tel1b1	NM_013773	118,580	74,377
Omt2a	NM_001111286	113,360	243,955
Obox5	NM_145709	110,924	2,669
E330034G19Rik	NM_001033214	106,956	1,162
Zbed3	NM_028106	106,540	3,005
Slc45a3	NM_145977	98,658	14,813
Tel1b5	NM_013776	95,977	68,387
Khdc1b	NM_001113187	95,938	23,715
Oosp1	NM_133353	93,718	14,502
Bpgm	NM_007563	86,249	4,611
EG194588	NM_001038676	84,998	2,979
Map1lc3b	NM_026160	984	279,836
Omt2b	NM_205822	12,2678	258,088
Omt2a	NM_001111286	113,360	243,955
Oaz1	NM_008753	30,967	165,822
Rplp0	NM_007475	1,844	151,774
Pdxk	NM_172134	0	126,122
Akp5	NM_007433	17	121,700
Ubb	NM_011664	21,871	118,549
Sp110	NM_175397	1,238	115,350
Klf17	NM_029416	24,531	112,781
H3f3b	NM_008211	47,128	112,188
Dppa3	NM_139218	29,844	106,509
Rps5	NM_009095	129	105,279
Tubb2c	NM_146116	3,013	101,600
Oog1	NM_178657	136,086	100,086

<b>Gene name</b>	<b>RefSeq ID</b>	<b>Relative counts in mature oocyte</b>	<b>Relative counts in 4-cell Blastomere</b>
EG547109	NM_001034906	0	98,682
Serf2	NM_011354	17,828	95,696
Impdh2	NM_011830	27	90,365
Prps1	NM_021463	20	88,663
Ccnb1	NM_172301	35,328	87,846