

## Video Article

# Multiplexed Fluorescent Microarray for Human Salivary Protein Analysis Using Polymer Microspheres and Fiber-optic Bundles

Shuai Nie<sup>1</sup>, Elena Benito-Peña<sup>1,2</sup>, Huaibin Zhang<sup>1</sup>, Yue Wu<sup>3</sup>, David R. Walt<sup>1</sup><sup>1</sup>Department of Chemistry, Tufts University<sup>2</sup>Department of Analytical Chemistry, Complutense University (Spain)<sup>3</sup>Department of Electrical and Computer Engineering, Tufts UniversityCorrespondence to: David R. Walt at [david.walt@tufts.edu](mailto:david.walt@tufts.edu)URL: <http://www.jove.com/video/50726>DOI: [doi:10.3791/50726](https://doi.org/10.3791/50726)

Keywords: Chemistry, Issue 80, protein sensing, microarray, multiplexed fluorescent quantification, fiber-optic biosensor, microsphere-based immunoassays, saliva analysis, microsphere encoding

Date Published: 10/10/2013

Citation: Nie, S., Benito-Peña, E., Zhang, H., Wu, Y., Walt, D.R. Multiplexed Fluorescent Microarray for Human Salivary Protein Analysis Using Polymer Microspheres and Fiber-optic Bundles. *J. Vis. Exp.* (80), e50726, doi:10.3791/50726 (2013).

## Abstract

Herein, we describe a protocol for simultaneously measuring six proteins in saliva using a fiber-optic microsphere-based antibody array. The immuno-array technology employed combines the advantages of microsphere-based suspension array fabrication with the use of fluorescence microscopy. As described in the video protocol, commercially available 4.5  $\mu\text{m}$  polymer microspheres were encoded into seven different types, differentiated by the concentration of two fluorescent dyes physically trapped inside the microspheres. The encoded microspheres containing surface carboxyl groups were modified with monoclonal capture antibodies through EDC/NHS coupling chemistry. To assemble the protein microarray, the different types of encoded and functionalized microspheres were mixed and randomly deposited in 4.5  $\mu\text{m}$  microwells, which were chemically etched at the proximal end of a fiber-optic bundle. The fiber-optic bundle was used as both a carrier and for imaging the microspheres. Once assembled, the microarray was used to capture proteins in the saliva supernatant collected from the clinic. The detection was based on a sandwich immunoassay using a mixture of biotinylated detection antibodies for different analytes with a streptavidin-conjugated fluorescent probe, R-phycoerythrin. The microarray was imaged by fluorescence microscopy in three different channels, two for microsphere registration and one for the assay signal. The fluorescence micrographs were then decoded and analyzed using a homemade algorithm in MATLAB.

## Video Link


The video component of this article can be found at <http://www.jove.com/video/50726/>

## Introduction

Since the first microarray reported by Mark Schena and coworkers in the mid-1990s, this powerful tool has been utilized in many fields of biological research<sup>1</sup>. Antibody microarrays capable of simultaneously detecting multiple proteins in diagnostic fluids, such as blood, have important applications in clinical diagnostics and biomarker screening<sup>2-10</sup>. Saliva, containing many of the same analytes as blood, has been considered as a preferable alternative to blood because saliva collection is safe, noninvasive, and can be carried out by minimally-trained medical personnel<sup>11-13</sup>. Currently, multiplexed protein analysis using saliva samples is limited by several important factors, including the low concentration of target analyte<sup>14</sup> and the wide concentration range of different biomarkers<sup>15</sup>.

Herein, we demonstrate the analysis of six proteins: human vascular endothelial growth factor (VEGF), interferon gamma-induced protein 10 (IP-10), interleukin-8 (IL-8), epidermal growth factor (EGF), matrix metalloproteinase 9 (MMP-9), and interleukin-1 beta (IL-1 $\beta$ ). The performance of the method was initially verified using standard solutions constituting recombinant analyte proteins and blocking buffer. Real saliva samples collected from patients of different chronic respiratory diseases as well as healthy controls were also tested with satisfactory performance. The protocol should be applicable to other protein analytes and other microsphere-based assays. This platform offers considerable advantages to the Analytical Chemistry field as it enables fast, accurate, and reproducible simultaneous analysis of low concentrations of several proteins with a broad dynamic range, minimal non-specific interactions, reduced sample consumption, and low cost in comparison to an analogous Enzyme-Linked Immunosorbent Assay (ELISA).

Protocol

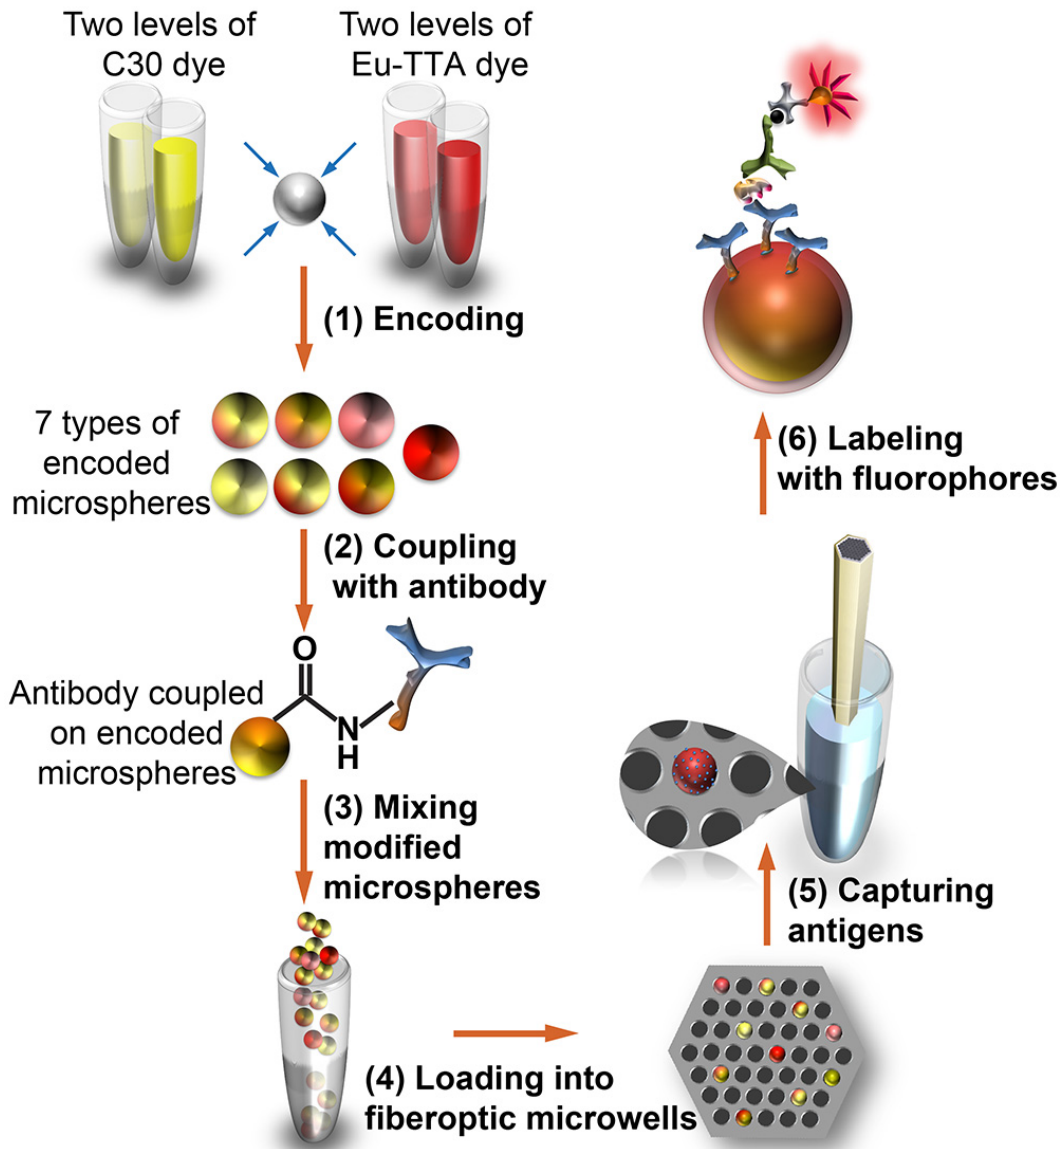

**Figure 1. Workflow for applying fiber-optic microsphere antibody array to saliva profiling.** (1) Microspheres are internally encoded with two fluorescent dyes; (2) the encoded microspheres are externally modified with protein-specific monoclonal antibodies; (3) the multiplexed microspheres are mixed, and (4) randomly deposited in microwells etched at the proximal end of a fiber-optic bundle; (5) salivary proteins are captured by microspheres through sandwich immunoassay, and (6) quantified using fluorescence microscopy.

## 1. Microspheres Encoding

1. Weigh sodium europium (III) thenoyltrifluoroacetate trihydrate (Eu-TTA, MW = 869.54 g/mol) in an amber glass vial and prepare a 200 mM stock solution in tetrahydrofuran (THF). Mix gently by pipetting; visually verify the dye is completely dissolved.
2. Weigh coumarin 30 (C30, MW = 347.41 g/mol) in an amber glass vial and prepare a 12 mM stock solution in THF. Mix gently by pipetting; visually verify the dye is completely dissolved.
3. Prepare 700  $\mu$ l of working solution for each microsphere type using the stock solutions and THF to reach final concentration listed in **Table 1**.
4. Ensure microspheres (10% w/v) are well suspended by vortexing, and then transfer 60  $\mu$ l suspension to a 1.5 ml microcentrifuge tube.
5. Add 600  $\mu$ l PBS to microsphere suspension and mix by pipetting 20x. Centrifuge the tube at 10,000 rpm for 3 min and carefully remove the supernatant. Repeat this process another 2x to wash the microspheres.
6. Wash the microsphere pellet 3x with THF using a similar procedure as step 1.5.
7. Centrifuge the microsphere/THF suspension at 10,000 rpm for 3 min, remove the supernatant, and re-suspend the pellet in 600  $\mu$ l working solution listed in **Table 1**. Transfer the mixture to a new 1.5 ml microcentrifuge tube.

8. Seal the microcentrifuge tube with Parafilm and place it on a shaker. Shake at 3,000 rpm and incubate for 24 hr, protect from light by covering the setup using a box covered with aluminum foil.
9. Centrifuge the microsphere suspension at 10,000 rpm for 3 min to form a pellet.
10. Remove the supernatant dye solution, wash the microspheres 6x with 600 µl methanol and then with 600 µl PBS containing 0.01% Tween-20 another 6x, as described in step 1.5.
11. Store the encoded microspheres in 600 µl PBS containing 0.01% Tween-20 at 4 °C until use, protect from light.

Microsphere type name:	1	2	3	4	5	6	7
Eu-TTA (mM)	100	100	10	100	10		
C30 (mM)		1	1	6	6	1	6

Table 1. Concentrations of Eu-TTA and C30 working solutions.

## 2. Preparation of Protein-capture Microspheres

1. Prepare MES buffer [2-(N-morpholino)ethanesulfonic acid (MES) 0.1 M, NaCl 0.9%, SDS 0.01%, pH 5.7] and PBS/SDS buffer (Sodium Phosphate 0.01 M, NaCl 0.154 M, SDS 0.01%, pH 7.4) in advance at room temperature.
2. Add 200 µl encoded microsphere suspension (containing ~2 mg microspheres) into a Safe-Lock 1.5 ml microcentrifuge tube. It is important to use this type of microcentrifuge tube to avoid spillage during the incubation in step 2.6.
3. Wash the microspheres with 600 µl MES buffer 3x as described in step 1.5. Add 700 µl MES to the microsphere pellet and mix well by pipetting.
4. Prepare 0.105 g/ml 1-ethyl-3-[3-dimethylaminopropyl] carbodiimide hydrochloride (EDC, MW = 191.7 g/mol) and 0.163 g/ml sulfo-N-hydroxysulfosuccinimide (sulfo-NHS, MW = 217.13 g/mol) solutions in MES buffer in separate tubes.
5. Add 150 µl freshly prepared EDC solution **drop by drop** into the microsphere suspension. The EDC hydrolyzes very quickly, thus it is essential to use freshly made solution to ensure the immobilization efficiency. Immediately after the addition of the EDC, add 150 µl sulfo-NHS solution to the microspheres, mix well by pipetting and verify the suspension is homogenous.
6. Cap the tube, seal it with Parafilm, and place it on a shaker. Shake at 1,500 rpm for 4 hr, protect from light using a box covered with aluminum foil.
7. Centrifuge the microsphere suspension at 10,000 rpm for 3 min to form a pellet and remove the supernatant. Wash the microspheres with 500 µl PBS/SDS buffer 3x as described in the step 1.5.
8. Add 200 µl PBS/SDS buffer to the pellet, mix the microspheres well and transfer the solution to 300 µl PBS/SDS buffer containing 60 µg capture antibodies. It is important to suspend the microsphere pellet first and then add the microsphere suspension into the antibody solution.
9. Incubate the antibody-microspheres mixture by shaking at 1,500 rpm for 4 hr on a shaker, protect from light using a box covered with aluminum foil.
10. Centrifuge the microsphere suspension at 10,000 rpm for 3 min to form a pellet and remove the supernatant. Wash the microspheres with 500 µl StartingBlock (TBS) blocking buffer 3x, as described in step 1.5.
11. Mix microspheres with 1 ml of TBS blocking buffer and incubate microspheres at 1,500 rpm for 1 hr on a shaker, protect from light using a box covered with aluminum foil.
12. Centrifuge the microsphere suspension at 7,000 rpm for 3 min to form a pellet and remove the supernatant. Wash the pellet 3x with 500 µl TBS blocking buffer, as described in step 1.5.
13. Centrifuge the microsphere solution at 7,000 rpm for 3 min to form a pellet and remove the supernatant. Add 500 µl TBS blocking buffer and mix by pipetting.
14. Store the modified microsphere suspension at 4 °C until use, protect from light.
15. Repeat this procedure to make other types of microspheres using corresponding antibodies.

## 3. Fiber-optic Microarray Assembly

1. Mix 50 µl of each type of protein-capture microspheres into a new autoclaved microcentrifuge tube. Centrifuge the stock microspheres pool at 7,000 rpm for 3 min, and remove the supernatant so that the remaining volume is approximately 100 µl.
2. Hand-cut fiber-optic bundles to approximately 5 cm in length and sequentially polish both ends on a polishing machine using 30, 15, 9, 6, 3, 1, 0.5, and 0.05 µm-sized diamond lapping films. Sonicate the polished bundle in deionized water for 2 min to remove any particles.
3. Put a small magnetic stirring bar into a 0.5 ml microcentrifuge tube, add 400 µl of protein-free PBS buffer and stir on a magnetic stirring plate for 30 min to remove air bubbles.
4. Etch one end of the polished fiber bundle in a 0.025 N HCl solution for 150 sec<sup>10,16</sup>. Immediately submerge and sonicate the etched end in deionized water for 1 min. Dry the fiber bundles with compressed air.
5. Mount the fiber bundle on a fiber holder and block the etched end in the bubble-free, Protein-free PBS buffer for 1 hr.
6. Deposit 1 µl aliquot of the stored microsphere suspension on the etched end of the fiber-optic bundle. Protect the setup from light with a box with aluminum foil, and wait for 15 min. The volume of the suspension will decrease by evaporation and force the microspheres into the etched microwells. Repeat this loading step one more time.
7. Use a swab saturated with sample solution to remove microspheres that are not trapped in the microwells. The protein microarray is now ready to use. Go immediately to step 4.1 for saliva analysis.

## 4. Saliva Sample Analysis Using Microspheres Microarray


1. Add 200  $\mu$ l sample solution (100  $\mu$ l saliva supernatant diluted with equal volume of StartingBlock T20 (PBS) blocking buffer. The collection protocol for saliva supernatant has been published previously<sup>10</sup>). into a 0.5 ml autoclaved microcentrifuge tube. Dip the protein microarray loaded on the fiber into the solution and incubate on the shaker at 600 rpm for 2 hr, protect from light using a box covered with aluminum foil.
2. Prepare 20 ml wash buffer by adding 200  $\mu$ l 10 % BSA solution and 200  $\mu$ l 10% Tween-20 into 19.6 ml PBS, mix well by gently shaking.
3. Dip the protein microarray into a new autoclaved microcentrifuge tube containing 200  $\mu$ l wash buffer and shake at 600 rpm for 2 min. Repeat this wash 3x.
4. Incubate the microarray in 100  $\mu$ l solution of a detection antibody cocktail containing 5  $\mu$ g/ml of anti-VEGF, IP-10, IL-8, EGF, MMP-9, IL-1 $\beta$  biotinylated detection antibodies in StartingBlock T20 (PBS) blocking buffer for 30 min at room temperature on the shaker at 600 rpm, protect from light using a box covered with aluminum foil.
5. Wash the microarray 3x with wash buffer as described in step 4.3.
6. Incubate the microarray in 200  $\mu$ l of 20  $\mu$ g/ml streptavidin R-phycoerythrin conjugate (SAPE) solution in PBS at 600 rpm on the shaker for 10 min, protect from light using a box covered with aluminum foil.
7. Wash the microarray 5x with wash buffer as described in step 4.3.
8. Clean the distal end of the fiber (*i.e.*, the end away from the microspheres) bundle with a swab saturated with absolute ethanol.
9. Dry both ends of the fiber with compressed air. Mount the fiber on an epifluorescent microscope and image through the distal end of the fiber.
10. Acquire microsphere images corresponding to Eu-TTA, C30, and SAPE fluorescence emission intensities. Optical filters setup and exposure times for fluorescence imaging of Eu-TTA, C30, and SAPE are depicted in **Table 2**.

Channel	Eu-TTA	C30	SAPE
Exciter	365/10x	350/50x	546/10x
Beamsplitter	525DCLP	400DCLP	560LP
Emitter	620/60m	460/50m	580/30m
Exposure time	1 sec	0.3 sec	1 sec

**Table 2. Parameters for the three fluorescent images of the microarray.**

### Representative Results

Fluorescence images from three channels showing a small section of the fiber-optic bundle are shown in **Figures 2A-C**. These images were analyzed using an algorithm written in MATLAB (as described in more detail in the Discussion section). The analysis employs both information from the Eu-TTA encoding image (**Figure 2A**) and the C30 encoding image (**Figure 2B**) to decode the microspheres, and the fluorescence intensities of different microspheres in the signal image (**Figure 2C**) were calculated. With the calibration curves obtained from correlated protein standards, the concentrations of proteins in saliva samples were calculated.

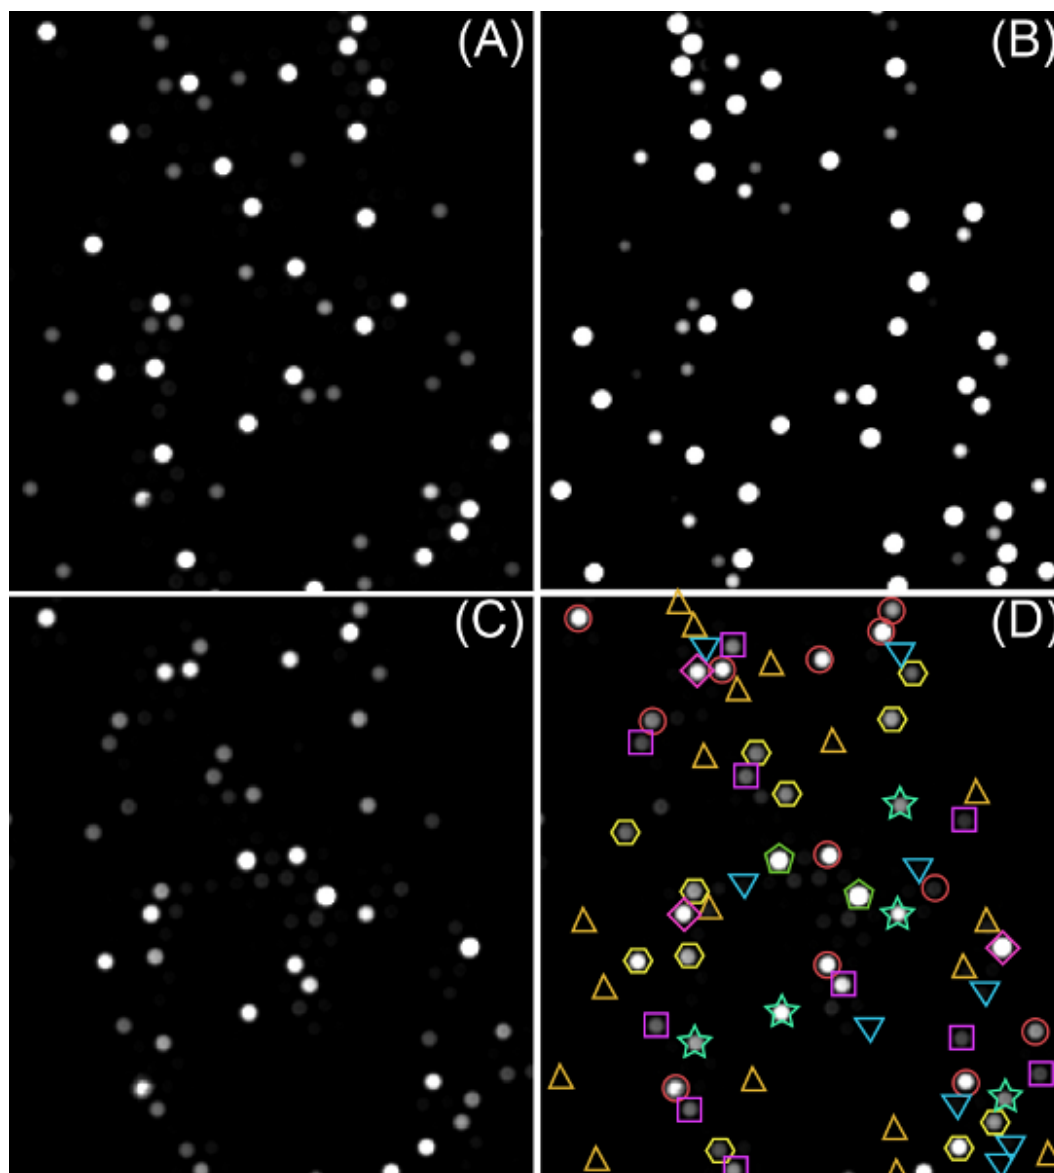

**Figure 2.** (A) Eu-TTA encoding image, (B) C30 encoding image, (C) SAPE signal image, (D) decoding results overlapped on the signal image; different types of microspheres were labeled with different colors and shapes.

## Discussion

Researchers should pay extra attention to the following steps: for better decoding accuracy, it is necessary to verify the microspheres were homogeneously suspended in all incubation and wash steps during the microspheres encoding procedure. In addition, the encoded microspheres need to be protected from light throughout the entire experiment. Following proper encoding and storage procedures, we found that overall decoding accuracy was above 99%. The encoded microspheres should be stored at 4 °C. **Avoid freezing and protect from light.** Under proper storage conditions, the encoded microspheres are stable for more than six months. Extreme care is required during the encoding and modification steps to reduce the loss of microspheres. For example, do not disturb the microsphere pellet when removing supernatant. In addition, including Tween-20 and SDS in the buffers is essential for better microsphere pelleting.

Some of the common troubleshooting procedures are: (1) use only freshly prepared EDC solution and the EDC solution should be added dropwise, (2) autoclaved tubes should be used and the microsphere solution should be transferred into a new tube before each incubation step, (3) during each wash step, try to remove the supernatant as much as possible, (4) the modified microspheres should be stored at 4 °C, **avoid freezing and protect from light.** Under proper storage conditions, the modified microspheres may be stored for more than 3 months with no detectable signal loss.

The MATLAB algorithm used to analyze the fluorescence images is briefly described below. The relevant code can be found in supplemental materials. Pixels within a user-defined intensity range for the Eu-TTA image are filtered first. Different areas were checked with a size-filter, areas containing a "hollow" center caused by light attenuation were removed and areas where microspheres are present were sorted into a watch

list for future processing. All microspheres from the watch list were further filtered with responses in the corresponding C30 image. The signals for all the pixels of a particular microsphere were averaged. The signal strength of this microsphere of interest was calculated by averaging the intensities of all microspheres in the watch list. To make the results statistically more representative, a minimum of 25 microspheres of each type was required. To minimize the nonspecific signal and decrease the variation between different experiments, signals for all microsphere types were normalized by subtracting the signal from the control microspheres.

The signal response of the microspheres can be adjusted by the amount of antibodies immobilized on the surface of microspheres, which is ideal for multiplexed detection of proteins with wide ranges of concentrations. Based on different diameters of the microspheres, the amount of antibody required to form a monolayer on the microspheres can be estimated by the equation from the manufacturer<sup>17</sup>. For microspheres with a diameter of 4.5 μm, 3 μg of antibody is needed per 1 mg of microspheres. We have tested different antibody amounts in the coupling solution in step 2.8 from 3 μg (0.5x) to 60 μg (10x) of antibody. Increased signals were observed when more antibody was used in the solution. Optimal antibody amounts for different antibodies and applications must be experimentally determined. The "control microspheres" were coupled with the mouse isotype IgG antibody, which is supplied by the manufacturer as the negative control in direct ELISA and has shown no cross-reactivity with up to 40 recombinant human proteins<sup>18</sup>. To evaluate the reproducibility of the coupling method, two batches of MMP-9 microspheres were coupled on different days. The performance of the microspheres was tested by using multiplexed detection of 10 ng/ml MMP-9. The results showed no significant differences among different batches of microspheres (detailed results are shown in **Table 3**).

No	Date	Test 1	Test 2	Test 3	Average	Std
1	01/12/2011	773.8	690.1	756.8	740.2	44.2
2	01/26/2011	791.9	721.8	867.0	793.6	72.6

**Table 3. Reproducibility of the coupling methods (results shown in arbitrary units).**

The multiplexed method presented here enables fast, accurate, and reproducible analysis of different proteins over a wide concentration range (results listed in **Table 4**). The potential cross-reactivity for the six antibody pairs we used in this study was also tested. All signals from cross-reactivity were found to be negligible (less than 3%). Other advantages of this method, when compared to a conventional Enzyme-Linked Immunosorbent Assay (ELISA), include a broad dynamic range, minimal non-specific interactions, reduced sample consumption and low cost<sup>10</sup>. The required volume of saliva sample is as low as 100 μl and the assay can be completed within 3.5 hr. When compared with other suspension arrays, one limitation of this approach is that once the microarray was assembled, the detection needs to be started in less than 15 min. The method described here has been used in our lab to analyze human saliva samples collected from patients with inflammatory diseases and healthy controls (unpublished data). The method should be applicable for protein analysis of other complex fluid specimens. A similar microsphere-based protein array can be used on other platforms such as microfluidic devices. The encoding and immobilized methods could also be applied to microspheres made with other materials<sup>9</sup>.

	VEGF	IP-10	IL-8	EGF	MMP-9	IL-1β
Test 1	5365.9	2578.4	6508.7	2584.0	515.5	1147.4
Test 2	5787.8	2577.9	7238.9	2919.2	375.7	1099.2
Test 3	4944.6	2883.3	6726.3	3619.3	406.8	1084.1
<b>Average</b>	5366.1	2679.9	6824.6	3040.8	432.7	1110.2
<b>Std. Dev</b>	421.6	176.2	374.9	528.3	73.4	33.1

**Table 4. Results for the three independent tests on the same saliva sample (results shown in arbitrary units).**

## Disclosures

The authors declare that they have no competing financial interests.

## Acknowledgements

This work was supported by the National Institutes of Health (grant 08UDE017788-05). E.B.P. also acknowledges support from the Spanish Foundation for Science and Technology (FECYT). The authors thank Shonda T. Gaylord and Pratyusha Mogalsetti for critical reading of the manuscript.

## References

- Schena, M., Shalon, D., Davis, R.W., & Brown, P.O. Quantitative monitoring of gene-expression patterns with a complementary-DNA microarray. *Science*. **270**, 467-470, doi:10.1126/science.270.5235.467 (1995).
- Schena, M. *Protein Microarray*. Jones and Bartlett Publishers (2004).
- Tam, S.W., Wiese, R., Lee, S., Gilmore, J., & Kumble, K.D. Simultaneous analysis of eight human Th1/Th2 cytokines using microarrays. *J. Immunol. Methods*. **261**, 157-165, doi:Pii s0022-1759(01)00572-5.1016/s0022-1759(01)00572-5 (2002).
- Wang, C.C., et al. Array-based multiplexed screening and quantitation of human cytokines and chemokines. *J. Proteome Res.* **1**, 337-343, doi:10.1021/pr0255203 (2002).



5. de Jager, W., te Velthuis, H., Prakken, B.J., Kuis, W., & Rijkers, G.T. Simultaneous detection of 15 human cytokines in a single sample of stimulated peripheral blood mononuclear cells. *Clin. Diagn. Lab. Immunol.* **10**, 133-139, doi:10.1128/cdli.10.1.133-139.2003 (2003).
6. Lee, H.J., Nedelkov, D., & Corn, R.M. Surface plasmon resonance imaging measurements of antibody arrays for the multiplexed detection of low molecular weight protein biomarkers. *Anal. Chem.* **78**, 6504-6510, doi:10.1021/ac060881d (2006).
7. Vignali, D.A.A. Multiplexed particle-based flow cytometric assays. *J. Immunol. Methods.* **243**, 243-255, doi:10.1016/s0022-1759(00)00238-6 (2000).
8. Rissin, D.M., *et al.* Single-molecule enzyme-linked immunosorbent assay detects serum proteins at subfemtomolar concentrations. *Nat. Biotechnol.* **28**, 595-599, doi:10.1038/nbt.1641 (2010).
9. Zhang, H., Nie, S., Etson, C.M., Wang, R.M., & Walt, D.R. Oil-sealed femtoliter fiber-optic arrays for single molecule analysis. *Lab Chip.* **12**, 2229-2239, doi:10.1039/c2lc21113k (2012).
10. Blicharz, T.M., *et al.* Fiber-Optic Microsphere-Based Antibody Array for the Analysis of Inflammatory Cytokines in Saliva. *Anal. Chem.* **81**, 2106-2114, doi:10.1021/ac802181j (2009).
11. Mukhopadhyay, R. Devices to drool for. *Anal. Chem.* **78**, 4255-4259, doi:10.1021/ac069420i (2006).
12. Wong, D.T. Salivary diagnostics powered by nanotechnologies, proteomics and genomics. *J. Am. Dent. Assoc.* **137**, 313-321 (2006).
13. Segal, A. & Wong, D.T. Salivary diagnostics: enhancing disease detection and making medicine better. *Eur. J. Dent. Educ.* **12**, 22-29 (2008).
14. St John, M.A.R., *et al.* Interleukin 6 and interleukin 8 as potential biomarkers for oral cavity and oropharyngeal squamous cell carcinoma. *Arch. Otolaryngol. Head Neck Surg.* **130**, 929-935, doi:10.1001/archotol.130.8.929 (2004).
15. Herr, A.E., *et al.* Microfluidic immunoassays as rapid saliva-based clinical diagnostics. *Proc. Natl. Acad. Sci. U.S.A.* **104**, 5268-5273, doi:10.1073/pnas.0607254104 (2007).
16. Pantano, P. & Walt, D.R. Ordered nanowell arrays. *Chem. Mater.* **8**, 2832-2835, doi:10.1021/cm9603314 (1996).
17. Schena, M. *Protein Microarrays*. Jones and Bartlett Publishers (2005).
18. <http://www.mdsystems.com/Products/MAB002> (2013).