


Correction

J Voigt, M Mosier. A powered bone marrow biopsy system versus manual methods: a systematic review and meta-analysis of randomised trials. *J Clin Pathol* 2013;66:9 792–796. Figure 5 in this paper was incorrect. It depicted adverse events identified and did not represent the overall trephine length analysis. The correct Figure 5 is shown below.

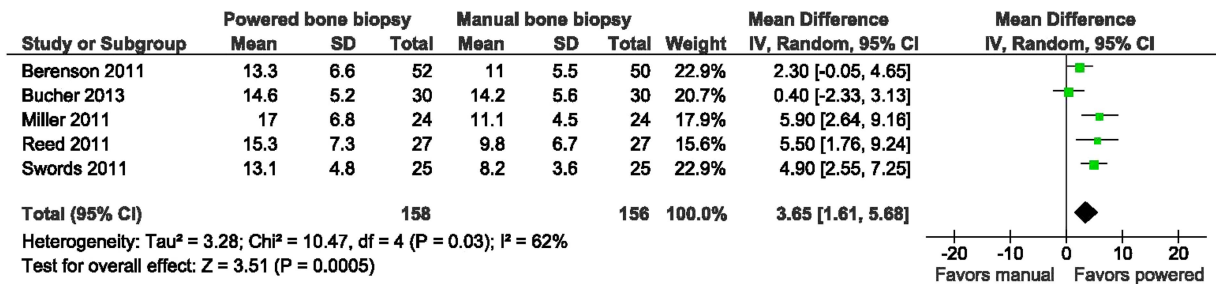

J Clin Pathol 2013;66:1004. doi:10.1136/jclinpath-2013-201605corr1