

Research

Open Access

## Assessment of body composition by air-displacement plethysmography: influence of body temperature and moisture

David A Fields\*<sup>1</sup>, Paul B Higgins<sup>2</sup> and Gary R Hunter<sup>3</sup>

Address: <sup>1</sup>Department of Health and Exercise Sciences, University of Oklahoma, Norman, OK, USA, <sup>2</sup>Division of Physiology and Metabolism, Department of Nutrition Sciences, University of Alabama at Birmingham, Birmingham, AL, USA and <sup>3</sup>Department of Human Studies University of Alabama at Birmingham, Birmingham, AL, USA

Email: David A Fields\* - [dafiels@ou.edu](mailto:dafiels@ou.edu); Paul B Higgins - [higginsp@uab.edu](mailto:higginsp@uab.edu); Gary R Hunter - [ghunter@uab.edu](mailto:ghunter@uab.edu)

\* Corresponding author

Published: 01 April 2004

Received: 06 February 2004

*Dynamic Medicine* 2004, **3**:3

Accepted: 01 April 2004

This article is available from: <http://www.dynamic-med.com/content/3/1/3>

© 2004 Fields et al; licensee BioMed Central Ltd. This is an Open Access article: verbatim copying and redistribution of this article are permitted in all media for any purpose, provided this notice is preserved along with the article's original URL.

### Abstract

**Background:** To investigate the effect of body temperature and moisture on body fat (%fat), volume and density by air-displacement plethysmography (BOD POD).

**Methods:** %fat, body volume and density by the BOD POD before (BOD POD<sub>BH</sub>) and immediately following hydrostatic weighing (BOD POD<sub>FH</sub>) were performed in 32 healthy females (age (yr) 33 ± 11, weight (kg) 64 ± 14, height (cm) 167 ± 7). Body temperature and moisture were measured prior to BOD POD<sub>BH</sub> and prior to BOD POD<sub>FH</sub> with body moisture defined as the difference in body weight (kg) between the BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub> measurements.


**Results:** BOD POD<sub>FH</sub> %fat (27.1%) and body volume (61.5 L) were significantly lower ( $P \leq 0.001$ ) and body density (1.0379 g/cm<sup>3</sup>) significantly higher ( $P \leq 0.001$ ) than BOD POD<sub>BH</sub> %fat (28.9%), body volume (61.7 L), and body density (1.0341 g/cm<sup>3</sup>). A significant increase in body temperature (~0.6°C;  $P \leq 0.001$ ) and body moisture (0.08 kg;  $P \leq 0.01$ ) were observed between BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub>. Body surface area was positively associated with the difference in %fat independent of changes in body temperature and moisture,  $r = 0.30$ ,  $P < 0.05$ .

**Conclusion:** These data demonstrate for the first time that increases in body heat and moisture result in an underestimation of body fat when using the BOD POD, however, the precise mechanism remains unidentified.

### Background

Air-displacement plethysmography (i.e. BOD POD) has gained popularity among body composition researchers since its introduction in 1995. This is mainly attributable to the non-invasive test-procedure and the lack of technical expertise required compared to the traditional hydrostatic weighing procedure.

The BOD POD is a single fiberglass unit composed of two chambers. The test chamber accommodates the subject during testing and the reference chamber contains instrumentation for measuring changes in pressure between the two chambers [1]. The operating principles of the BOD POD are detailed elsewhere [1-3]. Briefly, the volume of the test chamber is determined by pressure changes precipitated between the test chamber and reference chamber

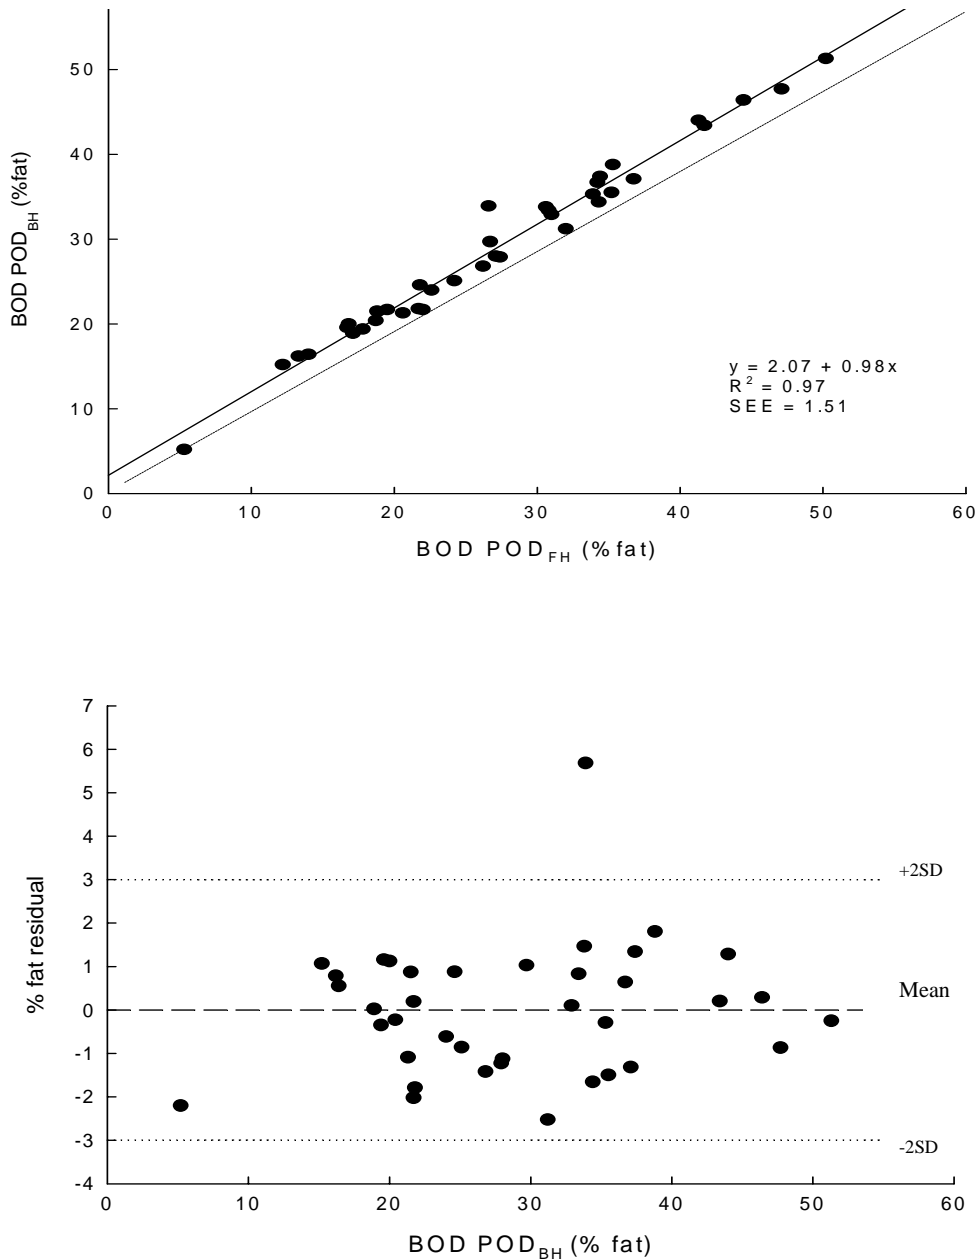

**Figure 1**

Panel A is the regression of percent fat determined by BOD POD<sub>BH</sub> before hydrostatic weighing against percent fat determined by BOD POD<sub>FH</sub> following hydrostatic weighing. The dotted line is the line of identity (regression slope = 1 and regression intercept = 0). The regression line significantly deviated from the line of identity. Panel B are the residuals from linear regressions of the percent fat from the BOD POD<sub>BH</sub> on percent fat from the BOD POD<sub>FH</sub>. The middle line represents the mean difference while the upper and lower dashed lines represent  $\pm 2$  SD from the mean. No bias was observed as indicated by the non-significant *P* value.

**Table 1: Subject characteristics and body composition variables before and immediately following hydrostatic weighing.**

Variable	BOD POD <sub>BH</sub>	BOD POD <sub>FH</sub>	P value
Body weight (kg)	63.58 ± 13.7	63.66 ± 13.7	P ≤ 0.05
Body temperature (°C)	36.3 ± 0.97	36.9 ± 1.00	P ≤ 0.001
Body surface area <sup>§</sup> (cm <sup>2</sup> )	17090 ± 1714	17090 ± 1714	
SAA (L)	-0.7976 ± 0.01	-0.7976 ± 0.01	
TGV (L)	3.46 ± 0.11	3.37 ± 0.11	NS
Raw Body Volume (L)	61.1 ± 2.4	60.9 ± 2.4	P ≤ 0.001
Corrected Body Volume* (L)	61.7 ± 14.5	61.5 ± 14.5	P ≤ 0.001
Body density (g/cm <sup>3</sup> )	1.0341 ± 0.022	1.0379 ± 0.023	P ≤ 0.001
Percentage body fat	28.91 ± 10.3	27.12 ± 10.3	P ≤ 0.001

§ 71.84 × weight<sup>0.425</sup> × height<sup>0.725</sup> \* Corrected for TGV and surface area artifact (raw body volume - SAA + 40%TGV) SAA: surface area artifact  
 BOD POD<sub>BH</sub>: BOD POD measures before hydrostatic weighing. BOD POD<sub>FH</sub>: BOD POD measures following hydrostatic weighing. Data are mean ± SD

by a moving diaphragm mounted on the common wall between the chambers. The pressure ratio relationships between the chambers are inversely related and are characterized by Boyle's Law:

$$P_1/P_2 = V_2/V_1$$

where V<sub>1</sub> and P<sub>1</sub> are the volume and pressure prior to subject entry into the test chamber and V<sub>2</sub> and P<sub>2</sub> are the volume and pressure while the subject is in the test chamber. Therefore, subject body volume will equal the volume of the test chamber before subject entry less the test chamber volume with the subject present.

Because of difficulty maintaining isothermal conditions in the enclosed environment of the test chamber, the BOD POD functions under adiabatic conditions (i.e. air temperature is gaining/loosing heat), thus Poisson's Law more accurately characterizes the pressure volume relationship in the testing chamber:

$$P_1/P_2 = (V_2/V_1)^\gamma$$

where V<sub>1</sub> and P<sub>1</sub> are the volume and pressure prior to subject entry into the test chamber, V<sub>2</sub> and P<sub>2</sub> are the volume and pressure while the subject is in the test chamber, and γ is the ratio of the specific heat of a gas at constant pressure to constant volume (1.4 for air) [4,5]. Moreover, isothermal air present in the test chamber during a body volume measurement will result in an underestimation of body volume because isothermal air is more easily compressed (40%) than an equivalent volume of adiabatic air, resulting in a lower pressure output signal for a given body volume [1]. There is one source of isothermal air (i.e. air in the lungs) and several sources that are "isothermal-like" (air trapped within the fabric of clothing and air

trapped within hair on the head and body). Instructions and procedures have been recommended by the manufacturers to correct and control for these sources of error [1,6].

To avoid erroneous data the BOD POD manufacturers recommend that testing be conducted prior to exercise, that the subject be dry, and that the testing environments temperature remain stable [7]. Strict adherence to these conditions can sometimes prove difficult when testing large numbers of subjects in a short period of time and when testing people who are perspiring or have an elevated temperature due to illness. In one study, BOD POD measurements were performed following hydrostatic weighing, which resulted in a regression that significantly deviated from the line of identity [8]. However, other studies have reported significant differences when the BOD POD preceded hydrostatic weighing [9,10]. Thus, the specific effect of elevated body temperature and body moisture (resulting from hydrostatic weighing) on BOD POD measurements needs clarification. An increase in body temperature and moisture could increase the quantity of isothermal-like air surrounding the skin. Therefore, the purpose of this study was to determine the effect of increased body temperature and moisture on BOD POD estimates of %fat, body volume, and body density. We hypothesized that an increase in body temperature and moisture would result in an underestimation of %fat. We also speculated that the increase in temperature, the increase in moisture, and total body surface area (BSA) would be positively associated with the magnitude of this underestimation.

**Methods**

**Subjects**

Thirty-two adult females (33 ± 11 yr., 64 ± 14 kg., 167 ± 7 cm) representing a wide range of BMI (19 – 36 kg/m<sup>2</sup>)

gave their informed consent to participate in the study. Approval for the use of human subjects was obtained from the Institutional Human Subject Review Board from the University of Alabama at Birmingham.

### Protocol

Subjects arrived for testing after an overnight fast. Height was measured using a wall mounted stadiometer while body weight was measured to the nearest 0.01 kg using the BOD POD system electronic scale, as previously described and was calibrated prior to each BOD POD test [2]. Body temperature was measured in the right ear using a Thermoscan IRT 3520 orbital thermometer (Braun, San Diego, CA). The repeat measures, between multiple measurements for body temperature in eight healthy subjects had an intra-class correlation of  $r = 0.98$  and a SEE =  $0.03^{\circ}\text{C}$ . After body temperature was determined and before hydrostatic weighing, the first BOD POD (BOD POD<sub>BH</sub>) test was performed, subjects were then asked to shower (this was done to keep the tank free of debris, wash off excess lotion, and sweat from the subjects) and prepare for hydrostatic weighing. Hydrostatic weighing was performed as part of an alternative study objective, (data not presented). Immediately following hydrostatic weighing subjects dried off thoroughly using towels provided by the laboratory. A second body temperature was determined and the second BOD POD test was performed (BOD POD<sub>FH</sub>). The moisture trapped in body hair and the fabric of the swimsuit was defined as the difference in body weight (kg) prior to hydrostatic weighing and upon completion of hydrostatic weighing (after towel dry). All testing was undertaken by the same investigator (DAF).

### BOD POD instrumentation

Whole body air-displacement was evaluated with the BOD POD version 1.69 (Body Composition System; Life Measurement, Incorporated, Concord, CA) as previously described [2]. Each subject was tested in a one - piece swimsuit and Lycra® swim cap. Thoracic gas volume (TGV) was measured in all subjects and BOD POD conditions (i.e. BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub>) according to the procedures described in the manual, while %fat was determined by the Siri equation [11]. In the calculation of body density for each testing condition, the body weight obtained in the dry state was used; this was done to investigate the effect of moisture and temperature increases on estimates of %fat independent of effects caused by increases in body weight. BSA was calculated according to the Dubois formula [12]:  $\text{BSA} = 71.84 \times \text{Weight (kg)}^{0.425} \times \text{Height (cm)}^{0.725}$ . Same-day repeat measures of body density by the BOD POD in our laboratory had an intra-class correlation of  $r = 0.98$  and an SEE of  $0.00365 \text{ (g/cm}^3\text{)}$  [6]. The room that housed the BOD POD was well ventilated between tests.

### Data analysis

Group mean estimates of %fat, body volume, and body density, by the BOD POD were compared using paired t-tests. Linear regression analysis and residuals from the regressions (percent fat and body density) were used to assess the agreement between BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub> for body density and %fat. Estimates were not considered different if the regression slope did not differ from one or the intercept from zero (line of identity). BOD POD<sub>FH</sub> %fat, body volume and density estimates were calculated using dry body weight to control for the effect of weight gain (due to moisture). Pearson correlation coefficients were used to examine the relation between the changes in body temperature, moisture, %fat, body volume and BSA before hydrostatic weighing (BOD POD<sub>BH</sub>) and following hydrostatic weighing (BOD POD<sub>FH</sub>). The independent relationships of  $\Delta$  temperature (difference in BOD POD<sub>BH</sub> temperature and BOD POD<sub>FH</sub> temperature), moisture, and BSA with  $\Delta$  %fat (difference in BOD POD<sub>BH</sub> %fat and BOD POD<sub>FH</sub> %fat) were determined using partial correlations. Statistical significance was set at  $P \leq 0.05$ . All statistics were derived using SPSS statistical software (version 10.0; SPSS Inc., Chicago, IL).


### Results

The %fat (28.9 vs. 27.1), raw body volume (61.1 L vs. 60.9 L), and corrected body volume (61.7 vs. 61.5 L) were significantly higher for the BOD POD<sub>BH</sub> vs. BOD POD<sub>FH</sub> (Table 1).

Linear regression analysis revealed that the regression of BOD POD<sub>BH</sub> %fat vs. BOD POD<sub>FH</sub> %fat significantly deviated from the line of identity,  $P \leq 0.005$  (Figure 1 panel A), though no bias was found across the range of body fatness  $P = 0.66$  (Figure 1 panel B). However, BOD POD<sub>BH</sub> body density versus BOD POD<sub>FH</sub> body density did not significantly deviate from the line of identity (Figure 2 panel A) and no significant bias was observed between body density estimates across the range of fatness  $P = 0.36$  (Figure 2 panel B).


Following hydrostatic weighing (i.e. BOD POD<sub>FH</sub>) subjects demonstrated a significant increase in body temperature ( $36.9^{\circ}\text{C}$  vs.  $36.3^{\circ}\text{C}$ ;  $P \leq 0.001$ ) and body weight ( $63.66$  vs.  $63.58$  kg;  $P \leq 0.05$ ) as compared to BOD POD<sub>BH</sub> (Table 1 and Figure 3).

$\Delta$ %fat was not associated with  $\Delta$  temperature after controlling for BSA and moisture gain, similarly  $\Delta$ %fat was not associated with moisture gain after controlling for BSA and  $\Delta$  temperature (Table 2). However, BSA was positively correlated ( $r = 0.30$ ,  $P < 0.05$ ) with  $\Delta$  %fat after controlling for moisture gain and  $\Delta$  temperature (Table 2).

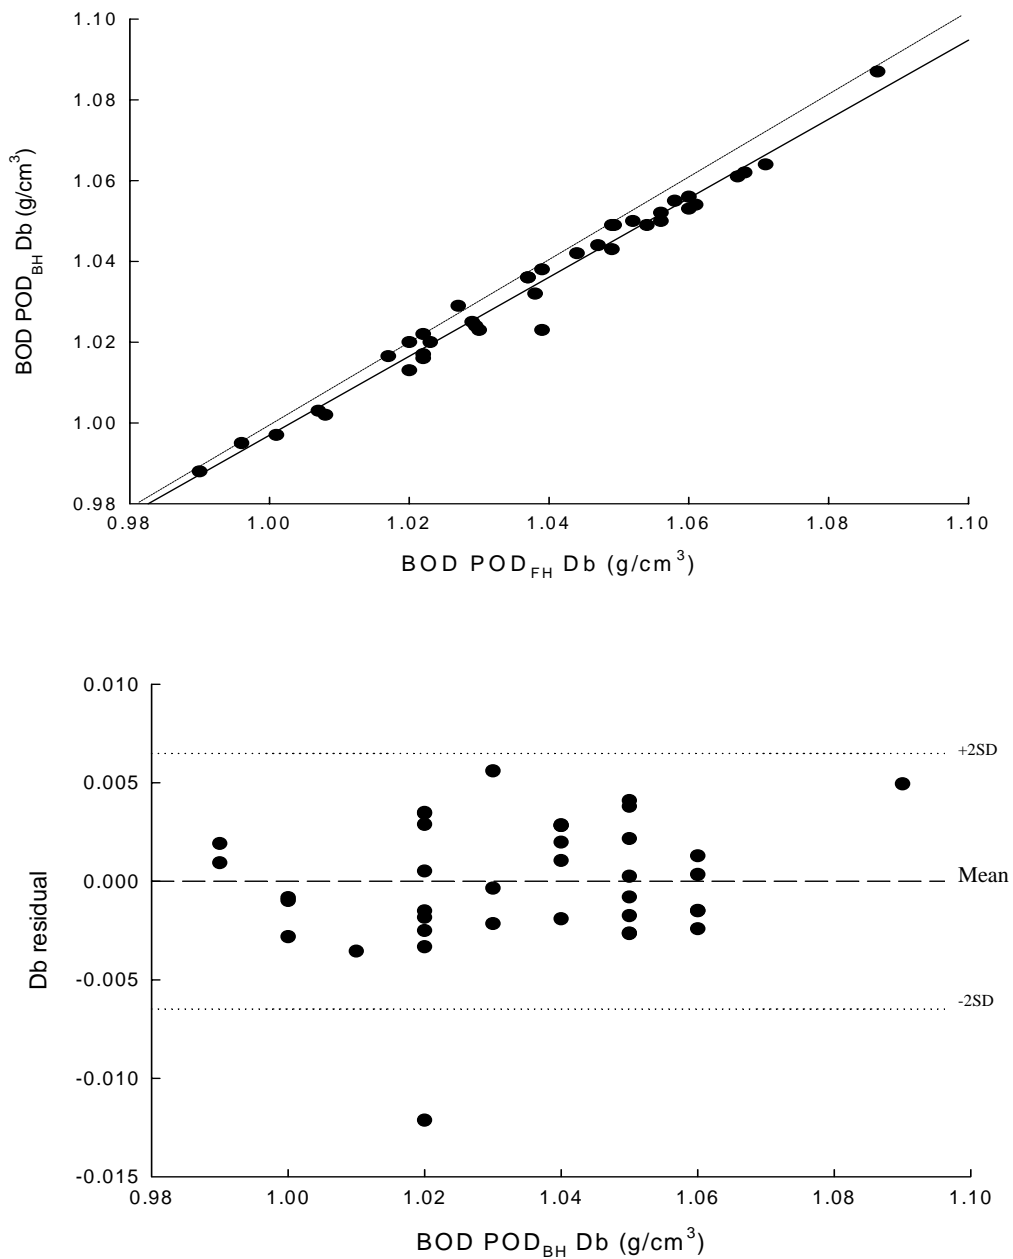

**Figure 2**

Panel A is the regression of body density ( $g/cm^3$ ) determined by  $BOD\ POD_{BH}$  before hydrostatic weighing against body density determined by  $BOD\ POD_{FH}$  following hydrostatic weighing. The dotted line is the line of identity (regression slope = 1 and regression intercept = 0). The regression line did not significantly deviate from the line of identity. Panel B are the residuals from linear regressions of body density  $BOD\ POD_{BH}$  on body density from the  $BOD\ POD_{FH}$ . The middle line represents the mean difference while the upper and lower dashed lines represent  $\pm 2\ SD$  from the mean. No bias was observed as indicated by the non-significant  $P$  value.

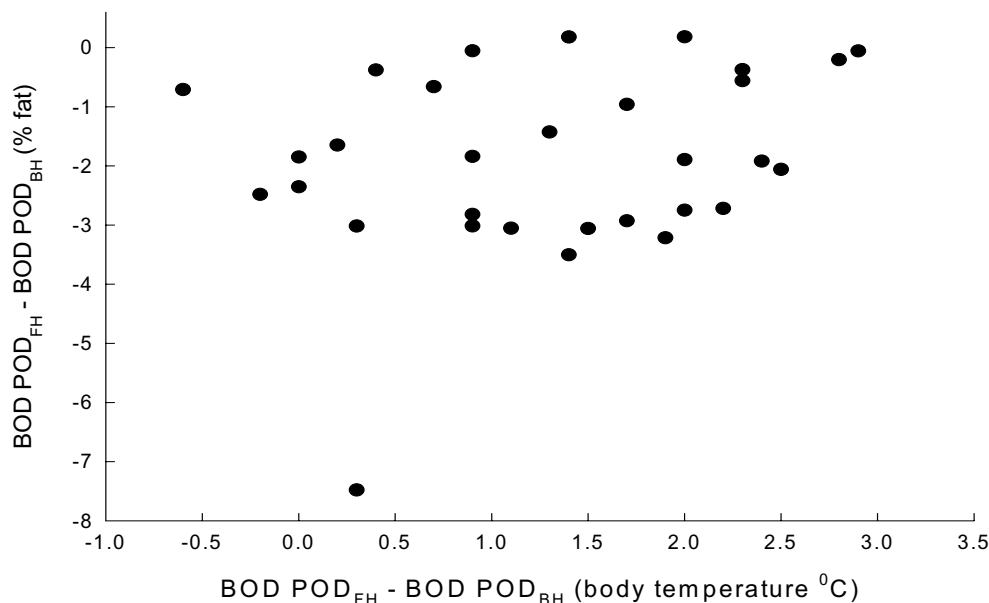

**Figure 3**  
Scatter plot between the difference in %fat (BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub>) and the difference in body temperature (BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub>).

**Table 2: Partial correlations to test the independent effect of temperature, moisture and BSA on %fat.**

	Δ Temperature (moisture, BSA, BMI)	Moisture (Δ temperature, BSA,)	BSA (moisture, Δ temperature,)
Δ %fat	0.21	0.28	0.30*

Δ %fat: BOD POD<sub>BH</sub> %fat – BOD POD<sub>FH</sub> %fat\*P < 0.05 BSA:Body surface area Δ Temperature: BOD POD Moisture: BOD POD<sub>BH</sub> weight – BOD POD<sub>FH</sub> weight

**Discussion**

The effect of body temperature and moisture on %fat, body volume, and body density using the BOD POD was addressed in the present study. Subjects underwent hydrostatic weighing between BOD POD tests, analogous to spending 30 minutes in a bath of 40°C water. Consequently, body temperature and body moisture were significantly elevated for the BOD POD<sub>FH</sub> measurement. Since subjects had not consumed any liquids or food, nor were they allowed to void between BOD POD<sub>BH</sub> and BOD POD<sub>FH</sub> measurements, it was assumed that the net body weight gain was due to water trapped on the skin, in the hair follicles, or within the fabric of the swimsuit. As a result of body volume being underestimated (0.210 L), the estimation in %fat by the BOD POD<sub>FH</sub> was signifi-

cantly lower (1.8 %fat) than the estimation of %fat by BOD POD<sub>BH</sub>, independent of the weight gain due to moisture retention.

The precise mechanism by which elevated body temperature and moisture affect BOD POD measures is unclear. The BOD POD operates under adiabatic conditions and therefore can accommodate changes in air temperature due to the presence of the test subject (1). Isothermal air present in the thoracic cavity is corrected for using measures of TGV during testing. The isothermal like air surrounding the skin is adjusted for using the surface area artifact, which is a correction factor calculated from BSA (1). However, under the present aberrant conditions the changes in the internal environment may have been too

rapid to be controlled. Furthermore, the isothermal-like air surrounding the skin may have increased in quantity and the usual correction (SAA) may have been inadequate. In addition, the release of water vapor from the skin surface, swimsuit, or hair may have altered the composition of the chamber air such that the correction constant  $\gamma$  (1.4) was no longer appropriate to control for the adiabatic conditions.

There was a significant relation between BSA and the reduction in %fat. The reduction in % fat was not related to the change in body temperature or to the gain in body moisture. This suggests that a larger BSA facilitates a greater dissipation of heat and/or water vapor into the BOD POD testing chamber resulting in a greater underestimation of body volume. We emphasize that the independent effects of body temperature and moisture on body volume measurement could not be assessed with the present study design. The lack of correlation between temperature and %fat might be related to the small variability in the average change in temperature from the first and second BOD POD measurements ( $\sim 0.6^\circ\text{C}$  with range of  $0.1 - 1.6^\circ\text{C}$ ). Since the variability in the temperature change was truncated, a relationship may have been undetectable. In addition, it is likely that the effects of moisture within the test chamber were not readily quantifiable by weight gain alone. Moisture on the skin and body hair was likely to be the variable of interest; this could not be quantified independent of moisture in the swimsuit.

In conclusion, the presence of excess heat and moisture in the BOD POD testing chamber leads to a small but significant underestimation in estimates of %fat. These findings are similar to those reported for the effects of clothing and body hair on BOD POD measures [6,13]. The specific mechanism(s) by which body heat and moisture effect estimates of body volume remain to be elucidated. The results from this study lead to the following recommendation: the BOD POD should always precede hydrostatic weighing or a bout of exercise. In addition, caution should be practiced when testing subjects with elevated body temperatures.

### Authors' contributions

DAF participated in study design, participated in data collection data analysis and writing the manuscript.

PBH participated in data analysis and editing the manuscript, and making all tables and figures.

GRH participated in study design, data analysis, and writing the manuscript.

### Acknowledgements

We thank the Division of Physiology and Metabolism at the University of Alabama in Birmingham for laboratory supplies and equipment.

### References

1. Dempster P, Aitkens S: **A new air displacement method for the determination of human body composition.** *Med Sci Sports Exerc* 1995, **27**:1692-1697.
2. McCrory MA, Gomez TD, Bernauer EM, Molé PA: **Evaluation of a new air displacement plethysmograph for measuring human body composition.** *Med Sci Sports Exerc* 1995, **27**:1686-1691.
3. Fields DA, Goran MI, McCrory MA: **Body-composition assessment via air-displacement plethysmography in adults and children: a review.** *Am J Clin Nutr* 2002, **75**:453-467.
4. Sly PD, Lanteri C, Bates JHT: **Effect of the thermodynamics of an infant plethysmograph on the measurement of thoracic gas volume.** *Pediatr Pulmonol* 1990, **8**:203-208.
5. Daniels F, Alberty RA: **Physical Chemistry.** John Wiley and Sons., Inc.; 1967:40-44.
6. Higgins PB, Fields DA, Gower BA, Hunter GR: **The effect of scalp and facial hair on body fat estimates by the BOD POD.** *Obes Res* 2001, **9**:326-330.
7. **BOD POD body composition system: Operator's manual.** Life Measurement, Inc. Concord, CA. 2000.
8. Levenhagen DK, Borel MJ, Welch D, C, Piasecki JH, Piasecki DP, Chen KY, Flakoll PJ: **A comparison of air displacement plethysmography with three other techniques to determine body fat in healthy adults.** *JPEN J Parenter Enteral Nutr* 1999, **23**:293-299.
9. Collins MA, Millard-Stafford ML, Sparling PB, Snow TK, Roszkopf LB, Webb SA, Omer J: **Evaluation of the BOD POD for assessing body fat in collegiate football players.** *Med Sci Sports Exerc* 1999, **31**:1350-1356.
10. Iwaoka H, Yokoyama T, Nakayama T, Matsumura Y, Yoshitake Y, Fuchi T, Yoshiike N, Tanaka H: **Determination of percent body fat by the newly developed sulfur hexafluoride dilution method and air displacement plethysmography.** *J Nutr Sci Vitaminol* 1998, **44**:561-568.
11. Siri WE: **Body composition from fluid spaces and density: analysis of methods.** *Techniques for Measuring Body Composition* Edited by: Brozek J and Henschel A. Washington, D.C., Natl Acad Sciences/Natl Res Council; 1961:223-224.
12. DuBois D, DuBois EF: **A formula to estimate the approximate surface area if height and weight be known.** *Arch Intern Med* 1916, **17**:863-871.
13. Fields DA, Hunter GR, Goran MI: **Validation of the BOD POD with hydrostatic weighing: Influence of body clothing.** *Int J Obes* 2000, **24**:200-205.

Publish with **BioMed Central** and every scientist can read your work free of charge

"BioMed Central will be the most significant development for disseminating the results of biomedical research in our lifetime."

Sir Paul Nurse, Cancer Research UK

Your research papers will be:

- available free of charge to the entire biomedical community
- peer reviewed and published immediately upon acceptance
- cited in PubMed and archived on PubMed Central
- yours — you keep the copyright

Submit your manuscript here:  
http://www.biomedcentral.com/info/publishing\_adv.asp

