

SHORT REPORT

Open Access



# Development and usefulness of an immunochromatographic device to detect antibodies for rapid diagnosis of human gnathostomiasis

Penchom Janwan<sup>1,2</sup>, Pewpan M. Intapan<sup>1,3\*</sup>, Hiroshi Yamasaki<sup>4</sup>, Rutchanee Rodpai<sup>1,3</sup>, Porntip Laummaunwai<sup>1,3</sup>, Tongjit Thanchomnang<sup>1,5</sup>, Oranuch Sanpool<sup>1,3,5</sup>, Kaoru Kobayashi<sup>6</sup>, Katsuyoshi Takayama<sup>6</sup>, Yukuharu Kobayashi<sup>6</sup> and Wanchai Maleewong<sup>1,3</sup>

## Abstract

**Background:** Human gnathostomiasis is a serious tropical disease, which is often overlooked. There is an urgent need to improve tools to aid the potential diagnosis of the disease in endemic regions. To overcome this, we produced the immunochromatographic test (ICT) kit for a rapid and simple diagnosis of human gnathostomiasis.

**Findings:** The recombinant protein (named rGslc18) was applied to ICT kit as the antigen. The diagnostic value of ICT kit was evaluated using serum samples from parasitologically proven and clinically suspected gnathostomiasis patients, healthy volunteers and patients with other parasitic diseases. The ICT kit exhibited quite high sensitivity (93.75 %) and specificity (97.01 %).

**Conclusions:** The ICT kit is simple, convenient and easy to implement and expected to provide reliable diagnostic results for human gnathostomiasis. It also will be a promising diagnostic tool not only for large-scale epidemiological surveys in endemic or remote areas where diagnostic facilities are poor but also for a rapid clinical diagnosis in the bedside laboratory.

**Keywords:** *Gnathostoma spinigerum*, Human gnathostomiasis, Immunochromatographic test kit, Serodiagnosis, Recombinant protein

## Background

Human gnathostomiasis is a serious food-borne parasitic zoonosis caused by infections with larval spirurid nematodes *Gnathostoma* spp. and the disease is regularly found in Asia and the Americas [1]. It is also common in travelers returning from visits to areas endemic to this harmful parasite [1]. Definitive diagnosis for human gnathostomiasis can be made by detecting the larvae migrating out from the human body. However, since direct detection of the parasite is difficult and often unsuccessful, diagnosis of human gnathostomiasis is primarily

made by relying upon clinical features, history of eating parasite-contaminated food, elevated blood eosinophilia, and serological outcomes [1]. Here, a recombinant protein produced from a *Gnathostoma spinigerum* clone (named Gslc18) isolated from *G. spinigerum* cDNA library, was used as an alternative antigen for the immunochromatographic test (ICT) kit development. The result was analysed and compared with specific IgG antibody detection against the native 24/21 kDa *G. spinigerum* larval antigen using immunoblotting [2]. This study demonstrated the effectiveness of the ICT kit as a convenient and rapid platform in the diagnosis of human gnathostomiasis that had not yet been reported elsewhere.

\* Correspondence: pewpan@kku.ac.th

<sup>1</sup>Research and Diagnostic Center for Emerging Infectious Diseases, Faculty of Medicine, Khon Kaen University, Khon Kaen 40002, Thailand

<sup>3</sup>Department of Parasitology, Faculty of Medicine, Khon Kaen University, Khon Kaen 40002, Thailand

Full list of author information is available at the end of the article




**Table 1** Types of human sera examined and diagnostic results of the ICT kit and the immunoblotting using the 24/21 kDa *G. spinigerum* antigen

Type of serum samples	Number of positive/Total number	
	ICT kit	Immunoblotting
Healthy control	0/20	0/20
Confirmed gnathostomiasis	9/9	9/9
Suspected gnathostomiasis	21/23	23/23
Cysticercosis	1/4	0/4
Taeniasis	0/10	0/10
Opisthorchiasis viverrini	0/15	0/15
Fascioliasis	1/5	0/5
Paragonimiasis	1/10	0/10
Angiostrongyliasis	1/10	0/10
Strongyloidiasis	0/10	0/10
Hookworm infection	0/10	0/10
Capillariasis	0/10	0/10
Ascariasis	0/10	0/10
Trichinellosis	0/3	0/3
Sparganosis	0/2	0/2
Malaria	0/10	0/10
Filariasis	0/5	0/5

**Methods**


*Gnathostoma spinigerum* advanced third-stage larvae RNA (920 ng) was used for cDNA synthesis. The cDNA library was constructed and colonies showing positive immunoscreening with serum samples from gnathostomiasis patients were selected for cloning procedure. A clone (named Gslic18) with a strong positive reaction to IgG antibodies in serum samples from gnathostomiasis patients, but not reactive to serum samples from patients with other parasitic infections or those in the negative control group, was selected through immunoscreening. The cDNA insert of Gslic18 was subcloned into a pQE-31 expression vector and transformed into *Escherichia coli* XL-1 Blue (Qiagen, Hilden, Germany) as the expression system. The recombinant Gslic18 (rGslic18) protein was expressed as insoluble protein and solubilised using urea solution (8 M urea, 0.1 M NaH<sub>2</sub>PO<sub>4</sub>, 0.01 M Tris-HCl, pH 8.0). Then, the rGslic18 carrying 6-Histidine (6-His)-tagged residues was purified using Ni-NTA His Bind Resin (Novagen, Darmstadt, Germany) according to the manufacturer’s protocol. The purified protein concentration was determined [3]. All human serum samples used for diagnostic values were supplied by the frozen bank (-70 °C). The samples were divided into three groups:

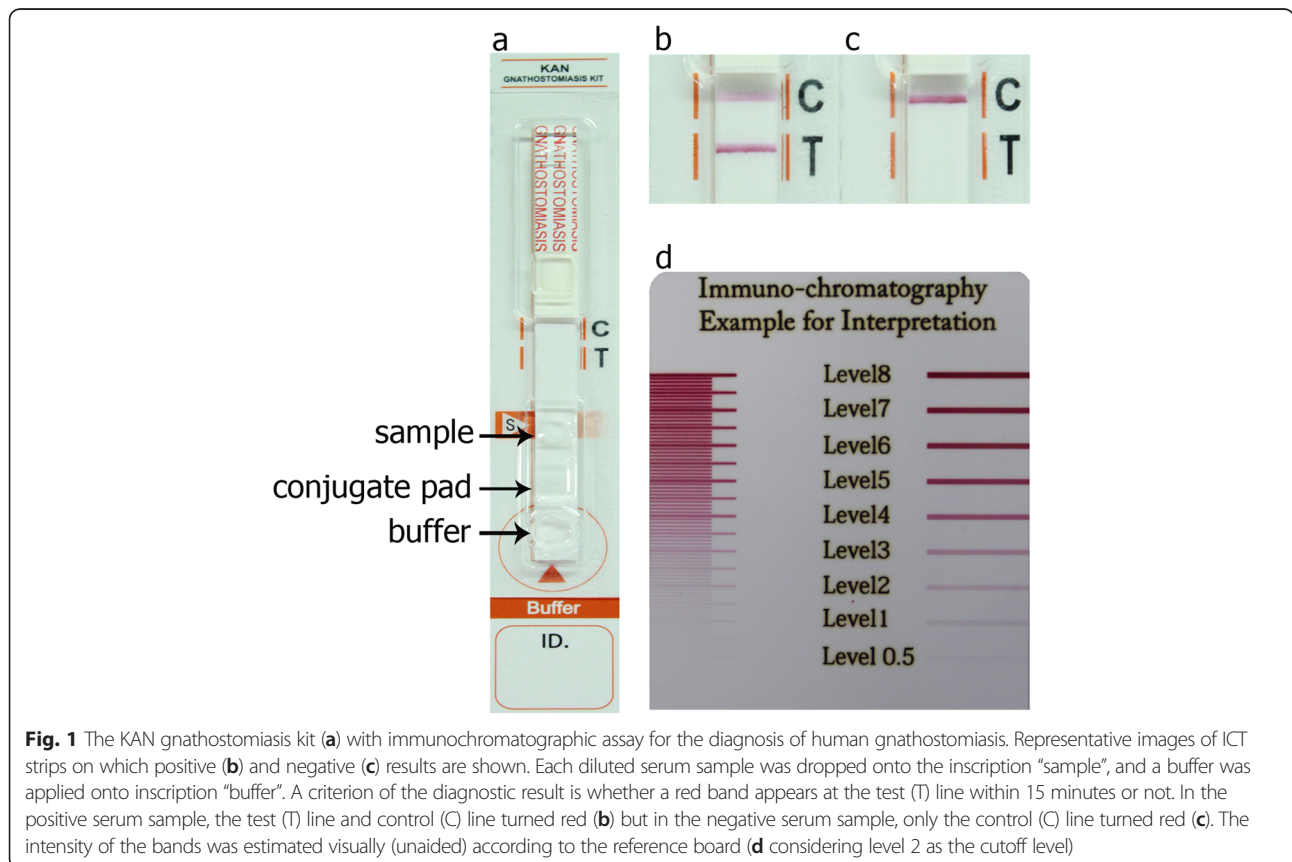

(i) the negative control group ( $n = 20$ ) comprised samples from healthy adult volunteers who underwent stool examination [4] and were found to be free from any intestinal parasitic infection at the time of blood collection (a pooled serum consisting of samples from the healthy individuals was also used as a negative control for each assay); (ii) the gnathostomiasis group ( $n = 32$ ), which included samples from parasitologically confirmed gnathostomiasis patients ( $n = 9$ ) and from patients showing clinical symptoms of suspected cutaneous and visceral gnathostomiasis, and neurognathostomiasis ( $n = 23$ ) [1] with a history of eating food possibly contaminated with *Gnathostoma* larvae and were positive 24/21 kDa *G. spinigerum* antigen by immunoblotting [2]; and (iii) the third group ( $n = 114$ ), which consisted of serum samples from patients with parasitic infections other than gnathostomiasis. Their infections were confirmed by parasitological methods except in cases of cysticercosis which were diagnosed by a computerised tomography scan and found positive by the immunological method [5] (Table 1).

The rapid ICT kit (named the “KAN gnathostomiasis kit, K, Khon Kaen University; A, Adtec Inc. Oita; N, National Institute of Infectious Diseases, Tokyo”) using the rGslc18 antigen was optimised based on the ELISA result using the same antigen at Adtec Inc., Oita, Japan. One mg/ml of anti-human IgG (H + L) (Medical and Biological Laboratories Co., Ltd., Nagoya, Japan) was absorbed at control line (C), 0.5 mg/ml of the rGslc18 antigen was absorbed at test line (T), and OD 1.0 of colloidal gold conjugated with anti-human IgG (Adtec Inc.) was sprayed on a piece of glass fiber (conjugate pad) (Fig. 1). The kit consists of an immunochromatographic device, sample buffer for diluting serum sample and buffer for chromatography. The diagnostic procedure is as follows: dilute serum samples with sample buffer in 1:50 and spot the aliquot (5  $\mu$ l) onto inscription “sample”, and apply buffer (60  $\mu$ l) onto inscription “buffer” (Fig. 1a). A criterion of the diagnostic result is whether a red band appears at the test line within 15 min or not. The intensity of the bands was estimated visually (unaided) according to the reference board (Fig. 1d, with level 2 as the cutoff level). Positive results were judged by the appearance of red band at the test (T) line and the control (C) line (Fig. 1b). Negative results were judged by the disappearance of a red band at test (T) line and appearance at control (C) line (Fig. 1c). The diagnostic parameters of sensitivity and specificity were computed as previously [6]. The diagnostic values of the ICT kit were evaluated with those of immunoblotting [2] and percentages of total concordance were computed (percent concordance (%) = (the number of concordances between ICT and the immunoblotting reference  $\times$  100)/the number of tested samples). Informed

consent was obtained from all human adult participants and from parents or legal guardians of minors. The study protocol was accepted by the Khon Kaen University Ethics Committee for Human Research (HE571438).

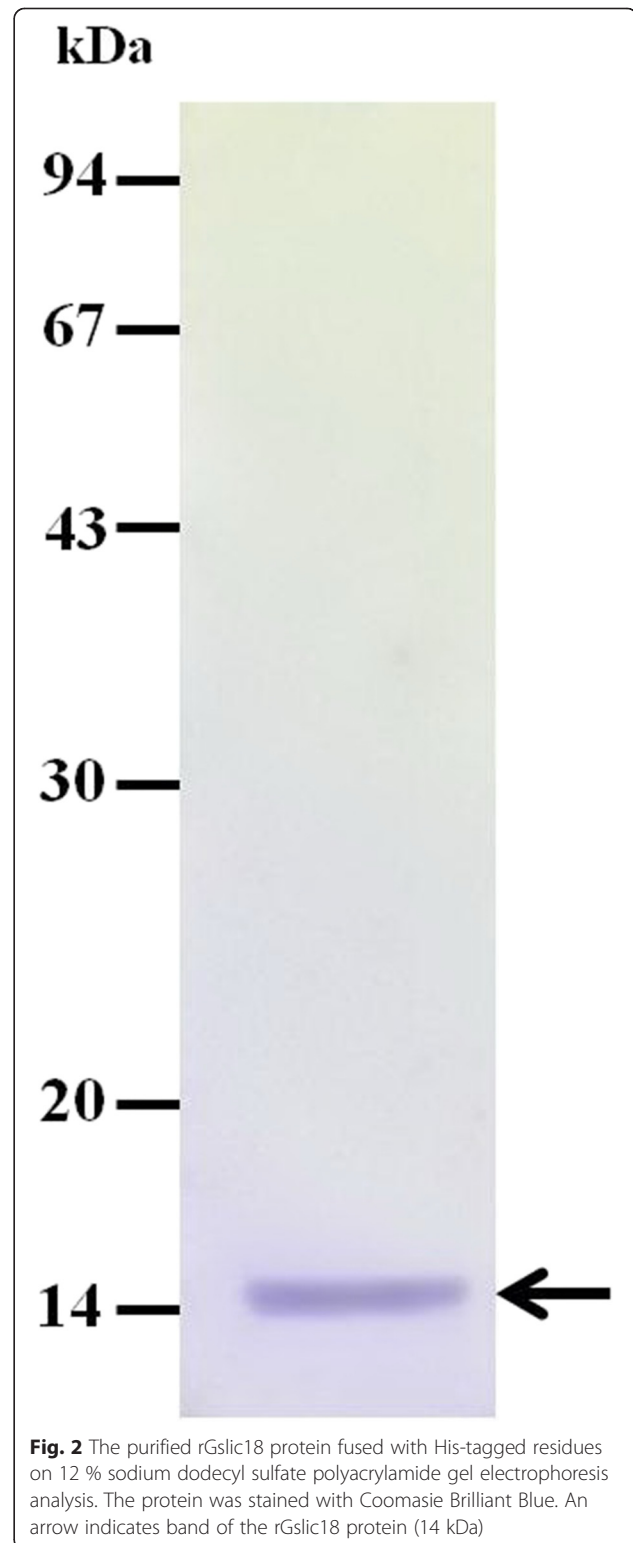

**Fig. 2** The purified rGslc18 protein fused with His-tagged residues on 12 % sodium dodecyl sulfate polyacrylamide gel electrophoresis analysis. The protein was stained with Coomassie Brilliant Blue. An arrow indicates band of the rGslc18 protein (14 kDa)

**Table 2** Comparison among ICT kit using rGslc18 and immunoblotting using 24/21 kDa *G. spinigerum* antigen

Test type and results	Immunoblotting		Total
	No. positive	No. negative	
ICT kit <sup>a</sup>			
No. positive	30	4	34
No. negative	2	130	132
Total	32	134	166

<sup>a</sup> There was no significant difference with immunoblotting ( $p > 0.05$ ; Exact McNemar's test)

## Results and discussion

The purified rGslc18 protein used as an antigen shown in Fig. 2 was used for preparation of immunochromatographic strips. The KAN gnathostomiasis kit, which employed the diagnostic values of the purified rGslc18 protein for human gnathostomiasis, was evaluated using serum from individuals among the gnathostomiasis patients, the healthy control, and the patients with other parasitic diseases (Table 1). All serum samples from the confirmed and suspected (except 2 cases) gnathostomiasis patients yielded positive results. In contrast, none of the 20 healthy control sera showed positive results. Some cross-reactivity was observed in serum samples of cysticercosis (1 of 4), fascioliasis (1 of 5), paragonimiasis (1 of 10), and angiostrongyliasis (1 of 10). The ICT kit exhibited high sensitivity (93.75 %) and specificity (97.01 %). Table 2 summarises the comparison of immunoblotting using immunodiagnostic 24/21 kDa *G. spinigerum* antigen and the ICT kit using the sera from the 166 subjects. Using the 24/21 kDa *G. spinigerum* antigen with immunoblotting as a standard test, both tests detected 30 positive cases and 130 negative cases. There were four false positive tests and two false negative tests detected by the KAN gnathostomiasis kit. The concordance of the ICT kit was determined to be 96.39 % (160/166 sera).

## Conclusions

This is the first time that the ICT kit with rGslc18 as an antigen was applied for the detection of anti-*Gnathostoma* antibodies in human sera and the results revealed high sensitivity and specificity. The ICT kit is a fast, simple, easy to implement and reliable as previous reports [7–9]. It has the potential to aid the development of a promising serodiagnostic kit for human gnathostomiasis as a stable mass production system, particularly for screening patients on a massive-scale in endemic areas or clinical diagnosis in the laboratory.

### Competing interests

The authors declare that they have no competing interests.

### Authors' contributions

PJ, PMI, HY, RR, PL, TT, OS, KK, YK and WM took part in the conception of this study and planned and designed the protocols. PJ, RR, OS, PL and TT performed the experiments and samples collection. PMI, HY, KK, KT, YK and

WM performed the experiments. PJ, PMI, HY and WM prepared the manuscript and reviewed the drafts of the manuscript for important intellectual content. All authors have seen and approved the final version of the manuscript.

### Acknowledgements

We wish to acknowledge the support of the English consultant Clinic, Research Affair, the Faculty of Medicine, Khon Kaen University and the Khon Kaen University Publication Clinic, Research and Technology Transfer Affairs, Khon Kaen University, for their assistance. This research was supported by a grant from the Higher Education Research Promotion and the National Research University Project of Thailand, Office of the Higher Education Commission, Thailand through the Health Cluster (SHeP-GMS) and the Faculty of Medicine, Khon Kaen University grant number RRU57201. RR was supported by the Thailand Research Fund through the Royal Golden Jubilee Ph.D. Program (grant no. PHD/0053/2556). OS was supported by the Postdoctoral Training Program Graduate School and Khon Kaen University (grant no. 58101), Khon Kaen University. PMI and WM were supported by the TRF Senior Research Scholar Grant, Thailand Research Fund grant number RTA5880001. HY was supported by Grants-in-Aid for Scientific Research from the Ministry of Health, Labour and Welfare, Japan (H25 ~ H26-Shinko-Ippan-009) and Research Program on Emerging and Re-emerging Infectious Diseases from Japan Agency for Medical Research and Development (No.15fk0108025h0502).

### Author details

<sup>1</sup>Research and Diagnostic Center for Emerging Infectious Diseases, Faculty of Medicine, Khon Kaen University, Khon Kaen 40002, Thailand. <sup>2</sup>Department of Medical Technology, School of Allied Health Sciences and Public Health, Walailak University, Nakhon Si Thammarat 80161, Thailand. <sup>3</sup>Department of Parasitology, Faculty of Medicine, Khon Kaen University, Khon Kaen 40002, Thailand. <sup>4</sup>Department of Parasitology, National Institute of Infectious Diseases, Tokyo 162-8640, Japan. <sup>5</sup>Faculty of Medicine, Mahasarakham University, Mahasarakham 44000, Thailand. <sup>6</sup>Division of Research and Development, Adtec Inc., Oita 879-0471, Japan.

Received: 24 December 2015 Accepted: 30 December 2015

Published online: 12 January 2016

### References

- Nawa Y, Maleewong W, Intapan MP, Diaz Camacho SP. *Gnathostoma*. In: Xiao L, Ryan U, Feng Y, editors. Food Microbiology Series: Biology of Foodborne Parasites. New York: CRC Press; 2015. p. 405–26.
- Intapan PM, Khotsri P, Kanpittaya J, Chotmongkol V, Sawanyawisuth K, Maleewong W. Immunoblot diagnostic test for neurognathostomiasis. *Am J Trop Med Hyg*. 2010;83:927–9.
- Bradford MM. A rapid and sensitive method for the quantitation of microgram quantities of protein utilizing the principle of protein-dye binding. *Anal Biochem*. 1976;72:248–54.
- Elkins DB, Haswell-Elkins M, Anderson RM. The epidemiology and control of intestinal helminths in the Pulicat Lake region of Southern India. I. Study design and pre- and posttreatment observations on *Ascaris lumbricoides* infection. *Trans R Soc Trop Med Hyg*. 1986;80:774–92.
- Intapan PM, Khotsri P, Kanpittaya J, Chotmongkol V, Maleewong W, Morakote N. Evaluation of IgG4 and total IgG antibodies against cysticerci and peptide antigens for the diagnosis of human neurocysticercosis by ELISA. *Asian Pac J Allergy Immunol*. 2008;26:237–44.
- Galen RS. Predictive value and efficiency of laboratory testing. *Pediatr Clin North Am*. 1980;27:861–9.
- Schnyder M, Stebler K, Naucke TJ, Lorentz S, Deplazes P. Evaluation of a rapid device for serological in-clinic diagnosis of canine angiostrongylosis. *Parasit Vectors*. 2014;7:72.
- Ghosh P, Hasnain MG, Ghosh D, Hossain F, Baker J, Boelaert M, et al. A comparative evaluation of the performance of commercially available rapid immunochromatographic tests for the diagnosis of visceral leishmaniasis in Bangladesh. *Parasit Vectors*. 2015;8:331.
- Lu Y, Guan G, Jiang T, Li Y, Yang J, Liu G, et al. Development of an immunochromatographic strip for the serodiagnosis of *Theileria* infection in sheep. *Parasit Vectors*. 2015;8:621.