



Published in final edited form as:

Int J Ion Mobil Spectrom. 2016 September ; 19(2): 69–76. doi:10.1007/s12127-016-0198-z.

Isomer Separation of Polybrominated Diphenyl Ether Metabolites using nanoESI-TIMS-MS

Kendra J. Adams¹, Dennise Montero¹, Diana Aga², and Francisco Fernandez-Lima^{1,3,*}

¹Department of Chemistry & Biochemistry, Florida International University, Miami, FL 33199, USA

²Department of Chemistry, University at Buffalo, The State University of New York, Buffalo, NY 14260, USA

³Biomolecular Science Institute, Florida International University, Miami, FL 33199, USA

Abstract

In this paper, high-resolution nano-electrospray ionization-trapped ion mobility spectrometry coupled to mass spectrometry (nESI-TIMS-MS) is used for the study of hydroxylated polybrominated diphenyl ether (OH-PBDE) metabolites. In particular, experimental ion-neutral collision cross sections (CCS) were measured for five structural OH-PBDE isomers using TIMS-MS. Candidate structures were proposed for each IMS band observed in good agreement with the experimental CCS measurements (5% error). The analytical power of TIMS-MS to baseline and partially separate structural isomers of OH-BDE in binary and ternary mixtures is shown for single charge species with a mobility resolving power of $R_{IMS} \sim 400$. This work provides the proof of concept for the analysis of low concentration OH-PBDE in environmental samples based on accurate collision cross section and mass measurements without the need for derivatization and pre-fractionation protocols, thus significantly reducing the cost and analysis time.

Introduction

Polybrominated diphenyl ethers (PBDEs) are members of the brominated flame retardant family (BFR), which have been frequently added since the 1970s to commercial products (e.g., plastics and textiles) (Darnerud et al. 2001). PBDEs are not chemically bound to the products and are easily released and accumulated in the environment, wildlife and humans (Darnerud et al. 2001; Eriksson et al. 2001; Siddiqi et al. 2003). There are three major classes of PBDEs; PBDEs, methoxylated PBDEs (MeO-PBDEs) and hydroxylated PBDEs (OH-PBDEs). The former class is anthropogenically created and released into the environment from commercial production. Previous research has shown that both MeO- and OH-PBDEs are formed from two sources: they are naturally occurring and produced by alga or they are metabolites from commercially produced PBDEs that have been released into the environment (Malmvärn et al. 2005; Malmvärn et al. 2008; Marsh et al. 2004). Studies have shown that PBDE metabolites such as OH-PBDEs are more toxic than their PBDE

*Corresponding Author: Phone: 305-348-2037. Fax: 305-348-3772. fernandf@fiu.edu.

Notes

The authors declare no competing financial interest.

counterparts (Feo et al. 2013a; Feo et al. 2013b; Wiseman et al. 2011; Zhao et al. 2015). Differences in toxicity/activity of PBDEs and their metabolites have been noted based on the location of hydroxyl group and bromine atoms on the diphenyl rings (Kim et al. 2010; Mercado-Feliciano and Bigsby 2008; Qiu et al. 2007; Su et al. 2014; Wiseman et al. 2011; Zhao et al. 2015). The variation in toxicity makes separation and identification of isomeric OH-PBDEs important for exposome profiling in the environment, humans and wildlife.

Traditional methods such as gas chromatography-mass spectrometry (GC-MS) and liquid chromatography-mass spectrometry (LC-MS) have allowed for separation and identification of PBDEs and their metabolites. For example, previous studies have utilized GC-MS for profiling of PBDEs, OH-PBDEs and MeO-PBDEs in human breast milk and serum (Butryn et al. 2015; Lacorte et al. 2010; Qiu et al. 2009). In addition, GC-MS has been utilized for PBDE analysis in wildlife and environmental samples (e.g., different species of fish and various river sediment samples) (Lacorte et al. 2010; Mackintosh et al. 2012). The use of GC-MS for analysis of OH-PBDEs requires derivatization of the molecules to more volatile metabolites such as MeO-BDEs (Butryn et al. 2015; Lacorte et al. 2010; Simpson et al. 2015). Previously, Simpson *et al.* analyzed hydroxylated PBDE metabolites via GC-MS and Conductor-like Screening Model for Realistic Solvents (COSMO-RS) to determine experimental retention times and theoretical boiling points of the compounds (Simpson et al. 2015). In COSMO-RS chemical potentials are calculated in liquids using the screening charge density (Klamt 1995; Klamt et al. 2010; Lei et al. 2008). Thermodynamic properties of molecules, such as boiling points, were predicted using COSMO-RS, converted to relative retention times and compared to experimental retention time values from GC-MS studies (Klamt et al. 2010; Lei et al. 2008; Simpson et al. 2015). This research proved that OH-PBDE isomers could be separated via retention on a GC-MS column and unknown metabolites could be identified by the combination of theoretically calculated boiling points and experimentally determined retention times after derivatization of the hydroxylated compounds (Simpson et al. 2015). In addition, four out of the five OH-PBDE metabolites analyzed in this research have previously been extracted and identified from human serum based on GC-MS analysis (Butryn et al. 2015).

Liquid chromatography-mass spectrometry (LC-MS) has also been used for both identification and quantification of PBDE metabolites within various matrices. Lacorte *et al.* developed an LC-ISP-MS/MS methodology in which eight different OH-PBDEs were identified and quantified from soil, fish and sludge (Mas et al. 2007). In these analyses, no sample derivatization was required, saving time and resources as well as allowing for the simultaneous analysis of both OH-PBDEs and MeO-PBDEs metabolites (Kato et al. 2009; Lupton et al. 2010; Mas et al. 2007). LC-MS techniques have also been used to successfully analyze for similar metabolites such as the chromatographic separation of 3-OH-BDE-47, 5-OH-BDE-47, and 6-OH-BDE-47 and the subsequent identification and confirmation via tandem mass spectrometry (Lupton et al. 2010). Although both GC-MS and LC-MS have proven valid methods for analysis and quantification of OH-PBDEs as standards and within biological matrices, the analyses still requires a significant amount of time (i.e., chromatographic separations typically lasting 40 minutes) and derivatizing agents for GC-MS.

Recent progress in gas-phase, post-ionization separations has been focused on the development of hyphenated techniques in order to achieve higher sensitivity, better separation and reduction of the chemical noise. Different variants of ion mobility spectrometry have been successfully coupled to mass spectrometry (e.g., periodic focusing DC ion guide (Gillig et al. 2004; Gillig and Russell 2001; Silveira et al. 2010), segmented quadrupole drift cell (Guo et al. 2004), multistage IMS (Glaskin et al. 2010; Koeniger et al. 2006; Kurulugama et al. 2009), field asymmetric waveform IMS (Kolakowski and Mester 2007; Purves and Guevremont 1999), travelling wave IMS (Shvartsburg and Smith 2008), trapped ion mobility spectrometry (Fernandez-Lima et al. 2011a; Fernandez-Lima et al. 2011b; Hernandez et al. 2014), and cyclic drift tube mobility spectrometry (Glaskin et al. 2013; Merenbloom et al. 2009). In particular, TIMS-MS has proved to provide high mobility resolution separations ($R \sim 150\text{--}300$) (Hernandez et al. 2014; Silveira et al. 2014) and the measurement of accurate mobility values using first principles (Hernandez et al. 2014). TIMS-MS provides complementary information separating samples in two dimensions: size-to-charge and mass-to-charge separation on a very limited time scale of analysis (hundreds of milliseconds) (Fernandez-Lima et al. 2011a; Hernandez et al. 2014). We have previously used TIMS-MS for detection of small molecules within complex matrices (McKenzie-Coe et al. 2015), the separation of polyaromatic hydrocarbons (Benigni et al. 2015a; Castellanos et al. 2014), targeted analysis of endocrine disruptors (Benigni et al. 2015b) and the analysis of the conformational dynamics of small molecules and biomolecules (Frost et al. 2015; Gonzalez et al. 2016; Molano-Arevalo et al. 2014; Schenk et al. 2015a; Schenk et al. 2014a; Schenk et al. 2015b; Schenk et al. 2014b; Silveira et al. 2014).

In this paper, we explore the potential of TIMS-MS for the analysis of isomeric metabolites of PBDEs. Five OH-tetra-brominated diphenyl ethers are studied: 3-OH-BDE-47, 5-OH-BDE-47, 6-OH-BDE-47, 4'-OH-BDE-49 and 2'-OH-BDE-68. Accurate mobility and ion-neutral CCSs were measured using nESI-TIMS-MS. Candidate structures were proposed for each IMS band observed of the individual OH-BDE. The capability of TIMS to separate structural isomers was evaluated for binary and ternary mixtures of OH-BDE. This is the first time resolving powers of $\sim 350\text{--}400$ are reported for single charge species using TIMS-MS.

Experimental Methods

Material and reagents

Hydroxylated tetra-brominated diphenyl ether standards were purchased from Accustandard Inc. (New Haven, CT, USA) and used as received. Five OH-PBDEs were analyzed in this study: 3-OH-BDE-47, 5-OH-BDE-47, 6-OH-BDE-47, 4'-OH-BDE-49 and 2'-OH-BDE-68. Binary and ternary mixtures were created by mixing equal volumes of individual standards and diluted to a final concentration of 200 nM. An aliquot (15 μL) of each sample was deposited into a pulled glass capillary tip for nESI-TIMS-MS analysis. All solvents used in these studies were analytical grade or better and purchased from Fisher Scientific (Pittsburg, PA).

TIMS-MS Analysis

TIMS-MS is a technique that combines ion mobility separation based on size with ion identification allowed by mass-to-charge ratios (Fernandez-Lima et al. 2011a; Fernandez-Lima et al. 2011b; Hernandez et al. 2014). Briefly, this separation technique is built on the utilization of an electric field to hold ions against a flow of moving gas ; allowing for the differentiation of ions based on their size-to-charge ratio (Fernandez-Lima et al. 2011a; Fernandez-Lima et al. 2011b; Hernandez et al. 2014). The mobility separation in a TIMS cell depends on the velocity of the bath gas (N_2), ion confinement and ion elution parameters (Fernandez-Lima et al. 2011a; Fernandez-Lima et al. 2011b; Hernandez et al. 2014). A voltage gradient along the TIMS tunnel provides parameters to trap geometric isomers simultaneously; the isomers are successively eluted from the tunnel by decreasing the electric field in stepwise increments (referred as the “ramp”). The eluted ions are further separated by mass in a time of flight (TOF) mass spectrometer. The results provide both a mass spectrum of the sample and mobility values which are correlated to collisional cross sections to determine the size of the molecules (Bush et al. 2010; Fernandez-Lima et al. 2011a; Fernandez-Lima et al. 2009a; Fernandez-Lima et al. 2010; Fernandez-Lima et al. 2011b; Fernandez-Lima et al. 2009b; Hernandez et al. 2014; May et al. 2014). The mobility in a TIMS analyzer can be described as:

$$K_i = v_g / E_x(i) = A(1 / (V_{out} - V_{elu}(i))) \quad (1)$$

where v_g is the velocity of the bath gas in the mobility cell and $E_x(i)$ is the electric field at which the specific packet of ions elute. These parameters can be related to the voltage the ions elute at ($V_{elu}(i)$) and the voltage of the mobility region exit. The A value is a calibration constant that is experimentally determined using a standard of known mobility. From the K or mobility value, the collisional cross section (CCS) can be related by the following equation:

$$CCS = \frac{(18\pi)^{\frac{1}{2}}}{16} \frac{z}{(k_b T)^{\frac{1}{2}}} \left[\frac{1}{m_1} + \frac{1}{m_b} \right]^{\frac{1}{2}} \frac{1}{K} \frac{760}{P} \frac{T}{273.15} \frac{1}{N^*} \quad (2)$$

The charge of the ion is represented by z , k_b represents the Boltzman constant, m_1 and m_b are the masses of molecular ion and the bath gas and N^* is the number density.

The mobility resolving power for the analysis considered was calculated as

$$R = CCS / \Delta CCS \quad (3)$$

Collisional cross sections were calculated using TuneMix as a calibration standard. Details on the Tunemix structures (e.g., $m/z = 322$ $K_0 = 1.376 \text{ cm}^2 \text{ V}^{-1} \text{ s}^{-1}$ and $m/z = 622$ $K_0 = 1.013 \text{ cm}^2 \text{ V}^{-1} \text{ s}^{-1}$) can be found elsewhere (Flanagan 1999; Hernandez et al. 2014).

TIMS-MS Operation Parameters—The instrument was operated in wide and narrow mobility selection modes, depending on the analytical challenge. For a wide range mobility analysis, a wide voltage ramp of $V_{\text{ramp}} = 200 \text{ V}$ with respect to $V_{\text{out}} = 60 \text{ V}$ was used with a typical ramp step of up to 500ms. For a narrow mobility selection (higher resolving power), a narrow voltage ramp of $V_{\text{ramp}} = 10 \text{ V}$ with respect to $V_{\text{out}} = 60 \text{ V}$ was used with a typical ramp step of up to 500ms. Notice that, TIMS mobility resolution depends on the ramp speed; the lower the speed the higher the mobility resolution. (Fernandez-Lima et al. 2011a; Fernandez-Lima et al. 2011b; Hernandez et al. 2014) In addition to the ramp speed, the velocity of the gas also defines the mobility resolution and trapping efficiency of the TIMS analyzer. Increasing the velocity of the gas, by changing the pressure difference between the front ($P_1 = 1.6 - 3.2 \text{ mbar}$) and the end ($P_2 = 0.6 - 1.4 \text{ mbar}$) of the analyzer region also increases the mobility resolution; the higher the velocity of the gas, the higher the drift force and the higher the electric field required to trap the ions. A constant radiofrequency is applied to the entrance, analyzer and exit region of the TIMS analyzer. Each funnel electrode is divided into four electrically insulated segments, which are used to create a dipole field in the entrance and exit section to focus the ions downstream and a quadrupolar field in the separation region to radially confine the ions during the ion trapping and analysis. That is, in the entrance and exit region the RF between adjacent plates are 180° out phase, while in the analyzer region the RF phase only alternates between adjacent segments. Only the inner diameter and electrode spacing varies between the three sections from 20 to 8 to 1 mm in the entrance, analyzer, and exit region respectively. The radiofrequency was kept constant for all the experiments (frequency of 880kHz with 300 V peak-to-peak)

A custom-built, pulled capillary nanoESI source was utilized for all the experiments. Quartz glass capillaries (O.D.: 1.0 mm and I.D.: 0.70 mm) were pulled utilizing a P-2000 micropipette laser puller (Sutter Instruments, Novato, CA) and loaded with 10 μL aliquot of the sample solution. Sample solutions consisted single, binary and ternary mixtures of OH-BDEs. A typical nESI source voltage of - 600–1200 V was applied between the pulled capillary tips and the TIMS-MS instrument inlet. Ions were introduced via a stainless steel tube ($1/16 \times 0.020''$, IDEX Health Science, Oak Harbor, WA) held at room temperature into the TIMS cell.

Theoretical Calculations

A pool of candidate structures were proposed for each OH-BDE standard analyzed in the TIMS-MS experiments. Final structures were optimized at the DFT/B3LYP/6-311G(d,p) level using Gaussian software (Frisch et al. 2004). Vibrational frequencies were calculated to guarantee that the optimized structures correspond to actual minima in the energy space and zero-point energy corrections were applied to calculate the relative stability between the structures. Theoretical ion-neutral collision cross sections were calculated using MOBCAL (Campuzano et al. 2011; Kim et al. 2009) software for nitrogen as a bath gas at ca. 300K. Partial atomic charges were calculated using the Merz-Singh-Kollman scheme constrained to the molecular dipole moment (Besler et al. 1990; Singh and Kollman 1984).

Results and Discussion

TIMS-MS analyses of individual OH-BDE standards including 3-OH-BDE-47, 5-OH-BDE-47, 6-OH-BDE-47, 4'-OH-BDE-49 and 2'-OH-BDE-68 resulted in a single IMS band for each structural isomer. Analysis of the mass spectra revealed the expected isotopic pattern of a tetra-brominated compound for the deprotonated molecular ion $[M-H]^-$ (Figure 1). Analysis of the IMS projections showed that all individual compounds have very similar experimental CCS values, ranging from 194.5–197.3 \AA^2 (Figure 1 and Table 1). In particular, 2'-OH-BDE-68 has the smallest CCS (194.5 \AA^2) while 4'-OH-BDE-49 has the largest CCS (197.3 \AA^2). The 6'-OH-BDE-47 and 2'-OH-BDE-68 have very similar CCSs (194.7 \AA^2 and 194.5 \AA^2 , respectively). In addition, 3-OH-BDE-47 and 5-OH-BDE-47 also have very similar experimental CCS (196.0 and 196.6 \AA^2 , respectively).

Candidate structures were proposed for each IMS band observed (see Figure 1). Inspection of the optimized structures at the DFT/B3LYP/6-311G(d,p) shows that OH-BDE are near planar conformations, with a slight twist around the central oxygen atom, depending on the position of the Br atoms (ortho *vs* para positions) (Figure 1). A small error was observed between the theoretical and experimental CCS values (less than $\pm 5\%$). This small error can be attributed to the fact that the MOBCAL program does not properly describe bromine atoms for the CCS calculations (Campuzano et al. 2011; Kim et al. 2009).

Following analysis of individual OH-PBDE compounds, binary and ternary mixtures of OH-PBDE standards were analyzed in order to evaluate the potential of nESI-TIMS-MS for the separation of isomeric mixtures of these compounds. The analysis of a binary mixture containing 2'-OH-BDE-68 and 3-OH-BDE-47 shows that these two isomers can be baseline resolved with a mobility resolving power of ~ 350 (Figure 2). Closer inspection shows that 3-OH-BDE-47 elutes from the mobility cell at a voltage of 143 V and 2'-OH-BDE-68 elutes at a voltage of 141 V while the same isotopic pattern was observed in the m/z domain (Figure 2a). Conversion of the trapping voltage to CCS shows that the 3-OH-BDE-47 peak is centered at 196.0 \AA^2 while 2'-OH-BDE-68 is centered at 194.7 \AA^2 (Figure 2b), which are in good agreement with the analysis of individual compounds (Figure 1). A binary mixture of 4'-OH-BDE-49 and 6-OH-BDE-47 was analyzed using the same instrumental conditions. The 2D-IMS-MS contour plot shows two mobility bands eluting from the cell at trapping voltages of 144 V and 142 V respectively with the same m/z profile corresponding to the isotopic distribution of tetra-brominated OH-BDEs (Figure 2c). Conversion of the trapping voltage to the CCS shows baseline separation of 4'-OH-BDE-49 centered at 197.3 \AA^2 and 6-OH-BDE-47 centered at 194.7 \AA^2 with a resolving power of ~ 320 –350 (Figure 2d). It should be noted that in both analyses the narrow range of the ramp voltage (10 V), the higher gas flow velocity, and the slow ramp speed permitted the achievement of high resolving power. In addition, the rigidity of the OH-PBDE molecules in contrast with previously studied systems (e.g., peptides and proteins) utilizing TIMS allows for the observation of narrower IMS bands.

Ternary mixtures of OH-BDE compounds were also created and subsequently analyzed via nESI-TIMS-MS. A mixture of 3-OH-BDE-47, 5-OH-BDE-47 and 2'-OH-BDE-68 showed baseline separation between 2'-OH-BDE-68 and 3-OH-BDE-47 (CCS=194.5 \AA^2 and 196.0

\AA^2) with a resolving power of 320–400. The two BDE-47 compounds in the mixture (3-OH-BDE-47 and 5-OH-BDE47) were only partially resolved; however, the IMS peak clearly shows a bimodal peak with two well defined centers that correlate to the CCS of the single standards (Figure 3a). A second ternary mixture containing 6-OH-BDE-47, 5-OH-BDE-47 and 4'-OH-BDE-49 was analyzed to further evaluate TIMS-MS as a method to separate isomeric mixtures (Figure 3b). In this mixture the two metabolites from BDE-47 were baseline separated with a resolving power in the order of 350–400; however, the 4'-OH-BDE-49 and 5-OH-BDE-47 were only partially resolved with centers that correlate to the CCS of the single standards (197.4 \AA^2 and 196.6 \AA^2 , respectively).

Conclusions

In this work we provide the framework for rapid isomer separation of hydroxylated polybrominated diphenyl ethers using nESI-TIMS-MS. During the analysis of five OH-BDE standards, experimental CCS values were calculated using TuneMix as a mobility standard. Candidate structures were proposed for all the IMS bands observed in good agreement with the experimental CCS (within $\pm 5\%$). Analysis of binary mixtures showed that baseline separation is possible between 2'-OH-BDE-68 and 3-OH-BDE-47, 6-OH-BDE-47 and 4'-OH-BDE-49, and 6-OH-BDE-47 and 5-OH-BDE-47 with a resolving power of 350–400. Moreover, 3-OH-BDE-47 and 5-OH-BDE-47, and 5-OH-BDE-47 and 4'-OH-BDE-49 isomers were only partially resolved. This work provides the foundation for the analysis of OH-BDE from complex mixtures utilizing small volumes (15 μL), significantly decreasing the amount of material necessary for the analysis without the need for derivatization or chromatographic separation. In addition, separation in the TIMS cell occurred on the millisecond range and experiments typically take less than 5 minutes per sample significantly decreasing the amount of analysis time when compared to GC-MS and LC-MS analyses. It should be noted that the TIMS-MS operation (as low as 50ms analysis time (Hernandez et al. 2014)) can be easily coupled to GC and LC pre-separation as a way to diminish the matrix effects during nESI for the analysis of complex mixtures.

Acknowledgments

This work was supported by the National Institute of Health (Grant No. R00GM106414). The authors wish to acknowledge Paolo Benigni for helpful discussions during the theoretical calculations. The authors also acknowledge computing resources provided by the Instructional & Research Computing Center (IRCC) at Florida International University.

References

- Benigni P, Marin R, Fernandez-Lima F. Towards unsupervised polyaromatic hydrocarbons structural assignment from SA-TIMS –FTMS data. *International Journal for Ion Mobility Spectrometry*. 2015a; :1–7. DOI: 10.1007/s12127-015-0175-y
- Benigni P, Thompson CJ, Ridgeway ME, Park MA, Fernandez-Lima F. Targeted high-resolution ion mobility separation coupled to ultrahigh-resolution mass spectrometry of endocrine disruptors in complex mixtures. *Analytical chemistry*. 2015b; 87:4321–4325. [PubMed: 25818070]
- Besler BH, Merz KM, Kollman PA. Atomic charges derived from semiempirical methods. *Journal of Computational Chemistry*. 1990; 11:431–439. DOI: 10.1002/jcc.540110404

- Bush MF, Hall Z, Giles K, Hoyes J, Robinson CV, Ruotolo BT. Collision Cross Sections of Proteins and Their Complexes: A Calibration Framework and Database for Gas-Phase Structural Biology. *Analytical Chemistry*. 2010; 82:9557–9565. DOI: 10.1021/ac1022953 [PubMed: 20979392]
- Butryn DM, Gross MS, Chi L-H, Schecter A, Olson JR, Aga DS. “One-shot” analysis of polybrominated diphenyl ethers and their hydroxylated and methoxylated analogs in human breast milk and serum using gas chromatography-tandem mass spectrometry. *Analytica Chimica Acta*. 2015
- Campuzano I, Bush MF, Robinson CV, Beaumont C, Richardson K, Kim H, Kim HI. Structural characterization of drug-like compounds by ion mobility mass spectrometry: comparison of theoretical and experimentally derived nitrogen collision cross sections. *Analytical chemistry*. 2011; 84:1026–1033. [PubMed: 22141445]
- Castellanos A, Benigni P, Hernandez DR, DeBord JD, Ridgeway ME, Park MA, Fernandez-Lima F. Fast screening of polycyclic aromatic hydrocarbons using trapped ion mobility spectrometry–mass spectrometry. *Anal Methods*. 2014; 6:9328–9332. [PubMed: 25558291]
- Darnerud PO, Eriksen GS, Jóhannesson T, Larsen PB, Viluksela M. Polybrominated diphenyl ethers: occurrence, dietary exposure, and toxicology. *Environmental Health Perspectives*. 2001; 109:49. [PubMed: 11250805]
- Eriksson P, Jakobsson E, Fredriksson A. Brominated flame retardants: a novel class of developmental neurotoxicants in our environment? *Environmental health perspectives*. 2001; 109:903. [PubMed: 11673118]
- Feo ML, Barón E, Aga DS, Eljarrat E, Barceló D. Development of a liquid chromatography–electrospray chemical ionization tandem mass spectrometry analytical method for analysis of eleven hydroxylated polybrominated diphenyl ethers. *Journal of Chromatography A*. 2013a; 1301:80–87. [PubMed: 23791149]
- Feo ML, Gross MS, McGarrigle BP, Eljarrat E, Barceló D, Aga DS, Olson JR. Biotransformation of BDE-47 to potentially toxic metabolites is predominantly mediated by human CYP2B6. *Environmental Health Perspectives (Online)*. 2013b; 121:440.
- Fernandez-Lima F, Kaplan DA, Suetering J, Park MA. Gas-phase separation using a trapped ion mobility spectrometer. *International Journal for Ion Mobility Spectrometry*. 2011a; 14:93–98.
- Fernandez-Lima FA, Becker C, McKenna AM, Rodgers RP, Marshall AG, Russell DH. Petroleum Crude Oil Characterization by IMS-MS and FTICR MS. *Analytical Chemistry*. 2009a; 81:9941–9947. DOI: 10.1021/ac901594f [PubMed: 19904990]
- Fernandez-Lima FA, Blase RC, Russell DH. A study of ion-neutral collision cross-section values for low charge states of peptides, proteins, and peptide/protein complexes. *International Journal of Mass Spectrometry*. 2010; 298:111–118. DOI: 10.1016/j.ijms.2009.10.009 [PubMed: 21503273]
- Fernandez-Lima FA, Kaplan DA, Park MA. Note: Integration of trapped ion mobility spectrometry with mass spectrometry. *Rev Sci Instr*. 2011b; 82:126106.
- Fernandez-Lima FA, Wei H, Gao YQ, Russell DH. On the structure elucidation using IMS and Molecular Dynamics. *J Phys Chem A*. 2009b; 113:8221–8234. [PubMed: 19569657]
- Flanagan LA. Mass Spectrometry Calibration Using Homogeneously substituted fluorinated triazatriphosphorines. United States Patent. 1999
- Frisch, MJ., et al. Gaussian 03, Revision C.02. Wallingford CT: 2004.
- Frost L, Baez MAM, Harrilal C, Garabedian A, Fernandez-Lima F, Leng F. The Dimerization State of the Mammalian High Mobility Group Protein AT-Hook 2 (HMGA2). *Plos One*. 2015; 10:e0130478.doi: 10.1371/journal.pone.0130478 [PubMed: 26114780]
- Gillig KJ, Ruotolo BT, Stone EG, Russell DH. An electrostatic focusing ion guide for ion mobility-mass spectrometry. *Int J Mass Spectrom*. 2004; 239:43–49.
- Gillig KJ, Russell DH. A periodic field focusing ion mobility spectrometer. 2001 2001-US6398 2001065589, 20010907.
- Glaskin RS, Ewing MA, Clemmer DE. Ion trapping for ion mobility spectrometry measurements in a cyclical drift tube. *Analytical chemistry*. 2013; 85:7003–7008. [PubMed: 23855480]
- Glaskin RS, Valentine SJ, Clemmer DE. A Scanning Frequency Mode for Ion Cyclotron Mobility Spectrometry. *Analytical Chemistry*. 2010; 82:8266–8271. DOI: 10.1021/ac1017474 [PubMed: 20809629]

- Gonzalez WG, Ramos V, Diaz M, Garabedian A, Molano-Arevalo JC, Fernandez-Lima F, Miksovska J. Characterization of the Photophysical, Thermodynamic, and Structural Properties of the Terbium(III)–DREAM Complex. *Biochemistry*. 2016; 55:1873–1886. DOI: 10.1021/acs.biochem.6b00067 [PubMed: 26901070]
- Guo Y, Wang J, Javahery G, Thomson BA, Siu KWM. Ion Mobility Spectrometer with Radial Collisional Focusing. *Analytical Chemistry*. 2004; 77:266–275. DOI: 10.1021/ac048974n [PubMed: 15623305]
- Hernandez DR, DeBord JD, Ridgeway ME, Kaplan DA, Park MA, Fernandez-Lima F. Ion dynamics in a trapped ion mobility spectrometer. *Analyst*. 2014; 139:1913–1921. DOI: 10.1039/C3AN02174B [PubMed: 24571000]
- Kato Y, Okada S, Atobe K, Endo T, Matsubara F, Oguma T, Haraguchi K. Simultaneous determination by APCI-LC/MS/MS of hydroxylated and methoxylated polybrominated diphenyl ethers found in marine biota. *Analytical chemistry*. 2009; 81:5942–5948. [PubMed: 19530686]
- Kim HI, et al. Structural characterization of unsaturated phosphatidylcholines using traveling wave ion mobility spectrometry. *Analytical chemistry*. 2009; 81:8289–8297. [PubMed: 19764704]
- Kim KH, et al. Para- and Ortho-Substitutions Are Key Determinants of Polybrominated Diphenyl Ether Activity toward Ryanodine Receptors and Neurotoxicity. *Environmental health perspectives*. 2010; 119:519–526. [PubMed: 21106467]
- Klamt A. Conductor-like screening model for real solvents: a new approach to the quantitative calculation of solvation phenomena. *The Journal of Physical Chemistry*. 1995; 99:2224–2235.
- Klamt A, Eckert F, Arlt W. COSMO-RS: an alternative to simulation for calculating thermodynamic properties of liquid mixtures. *Annual review of chemical and biomolecular engineering*. 2010; 1:101–122.
- Koeniger SL, Merenbloom SI, Valentine SJ, Jarrold MF, Udseth HR, Smith RD, Clemmer DE. An IMS-IMS Analogue of MS-MS. *Anal Chem*. 2006; 78:4161–4174. [PubMed: 16771547]
- Kolakowski BM, Mester Z. Review of applications of high-field asymmetric waveform ion mobility spectrometry (FAIMS) and differential mobility spectrometry (DMS). *Analyst*. 2007; 132:842–864. [PubMed: 17710259]
- Kurulugama RT, Nachtigall FM, Lee S, Valentine SJ, Clemmer DE. Overtone mobility spectrometry: Part I. Experimental observations. *Journal of the American Society for Mass Spectrometry*. 2009; 20:729–737. [PubMed: 19195909]
- Lacorte S, Ikonomidou MG, Fischer M. A comprehensive gas chromatography coupled to high resolution mass spectrometry based method for the determination of polybrominated diphenyl ethers and their hydroxylated and methoxylated metabolites in environmental samples. *Journal of Chromatography A*. 2010; 1217:337–347. [PubMed: 19945713]
- Lei Z, Chen B, Li C, Liu H. Predictive molecular thermodynamic models for liquid solvents, solid salts, polymers, and ionic liquids. *Chemical reviews*. 2008; 108:1419–1455. [PubMed: 18336046]
- Lupton SJ, McGarrigle BP, Olson JR, Wood TD, Aga DS. Analysis of hydroxylated polybrominated diphenyl ether metabolites by liquid chromatography/atmospheric pressure chemical ionization tandem mass spectrometry. *Rapid Communications in Mass Spectrometry*. 2010; 24:2227–2235. [PubMed: 20623478]
- Mackintosh SA, Pérez-Fuentetaja A, Zimmerman LR, Pacepavicius G, Clapsadl M, Alaei M, Aga DS. Analytical performance of a triple quadrupole mass spectrometer compared to a high resolution mass spectrometer for the analysis of polybrominated diphenyl ethers in fish. *Analytica chimica acta*. 2012; 747:67–75. [PubMed: 22986137]
- Malmvärn A, Marsh G, Kautsky L, Athanasiadou M, Bergman Å, Asplund L. Hydroxylated and methoxylated brominated diphenyl ethers in the red algae *Ceramium tenuicorne* and blue mussels from the Baltic Sea. *Environmental science & technology*. 2005; 39:2990–2997. [PubMed: 15926543]
- Malmvärn A, Zebühr Y, Kautsky L, Bergman Å, Asplund L. Hydroxylated and methoxylated polybrominated diphenyl ethers and polybrominated dibenzo-p-dioxins in red alga and cyanobacteria living in the Baltic Sea. *Chemosphere*. 2008; 72:910–916. [PubMed: 18457860]

- Marsh G, Athanasiadou M, Bergman Å, Asplund L. Identification of hydroxylated and methoxylated polybrominated diphenyl ethers in Baltic Sea salmon (*Salmo salar*) blood. *Environmental science & technology*. 2004; 38:10–18. [PubMed: 14740711]
- Mas S, Jáuregui O, Rubio F, de Juan A, Tauler R, Lacorte S. Comprehensive liquid chromatography–ion – spray tandem mass spectrometry method for the identification and quantification of eight hydroxylated brominated diphenyl ethers in environmental matrices. *Journal of mass spectrometry*. 2007; 42:890–899. [PubMed: 17511022]
- May JC, et al. Conformational Ordering of Biomolecules in the Gas Phase: Nitrogen Collision Cross Sections Measured on a Prototype High Resolution Drift Tube Ion Mobility-Mass Spectrometer. *Analytical Chemistry*. 2014; 86:2107–2116. DOI: 10.1021/ac4038448 [PubMed: 24446877]
- McKenzie-Coe A, DeBord JD, Ridgeway M, Park M, Eiceman G, Fernandez-Lima F. Lifetimes and stabilities of familiar explosive molecular adduct complexes during ion mobility measurements. *Analyst*. 2015; 140:5692–5699. [PubMed: 26153567]
- Mercado-Feliciano M, Bigsby RM. Hydroxylated Metabolites of the Polybrominated Diphenyl Ether Mixture DE-71 Are Weak Estrogen Receptor-[alpha] Ligands. *Environmental health perspectives*. 2008; 116:1315. [PubMed: 18941571]
- Merenbloom SI, Glaskin RS, Henson ZB, Clemmer DE. High-resolution ion cyclotron mobility spectrometry. *Analytical chemistry*. 2009; 81:1482–1487. [PubMed: 19143495]
- Molano-Arevalo JC, Hernandez DR, Gonzalez WG, Miksovska J, Ridgeway ME, Park MA, Fernandez-Lima F. Flavin adenine dinucleotide structural motifs: from solution to gas phase. *Analytical chemistry*. 2014; 86:10223–10230. [PubMed: 25222439]
- Purves RW, Guevremont R. Electrospray ionization high-field asymmetric waveform ion mobility spectrometry-mass spectrometry. *Analytical chemistry*. 1999; 71:2346–2357. [PubMed: 21662783]
- Qiu X, Bigsby RM, Hites RA. Hydroxylated metabolites of polybrominated diphenyl ethers in human blood samples from the United States. *Environ Health Perspect*. 2009; 117:93–98. [PubMed: 19165393]
- Qiu X, Mercado-Feliciano M, Bigsby RM, Hites RA. Measurement of polybrominated diphenyl ethers and metabolites in mouse plasma after exposure to a commercial pentabromodiphenyl ether mixture. *Environmental health perspectives*. 2007:1052–1058. [PubMed: 17637922]
- Schenk ER, Almeida R, Miksovska J, Ridgeway ME, Park MA, Fernandez-Lima F. Kinetic Intermediates of Holo- and Apo-Myoglobin Studied Using HDX-TIMS-MS and Molecular Dynamic Simulations. *J Am Soc Mass Spectrom*. 2015a; 26:555–563. DOI: 10.1007/s13361-014-1067-9 [PubMed: 25690175]
- Schenk ER, Mendez V, Landrum JT, Ridgeway ME, Park MA, Fernandez-Lima F. Direct Observation of Differences of Carotenoid Polyene Chain cis/trans Isomers Resulting from Structural Topology. *Anal Chem*. 2014a; 86:2019–2024. DOI: 10.1021/ac403153m [PubMed: 24428664]
- Schenk ER, Nau F, Fernandez-Lima F. Theoretical predictor for candidate structure assignment from IMS data of biomolecule-related conformational space. *Int J Ion Mobility Spectrom*. 2015b; 18:23–29. DOI: 10.1007/s12127-015-0165-0
- Schenk ER, Ridgeway ME, Park MA, Leng F, Fernandez-Lima F. Isomerization kinetics of AT hook decapeptide solution structures. *Analytical chemistry*. 2014b; 86:1210–1214. [PubMed: 24364733]
- Shvartsburg AA, Smith RD. Fundamentals of traveling wave ion mobility spectrometry. *Analytical chemistry*. 2008; 80:9689–9699. [PubMed: 18986171]
- Siddiqi MA, Laessig RH, Reed KD. Polybrominated diphenyl ethers (PBDEs): new pollutants–old diseases. *Clinical Medicine & Research*. 2003; 1:281–290. [PubMed: 15931321]
- Silveira JA, Gamage CM, Blase RC, Russell DH. Gas-phase ion dynamics in a periodic-focusing DC ion guide. *International Journal of Mass Spectrometry*. 2010; 296:36–42. DOI: 10.1016/j.ijms.2010.07.019
- Silveira JA, Ridgeway ME, Park MA. High resolution trapped ion mobility spectrometry of peptides. *Analytical chemistry*. 2014; 86:5624–5627. [PubMed: 24862843]
- Simpson S, Gross MS, Olson JR, Zurek E, Aga DS. Identification of polybrominated diphenyl ether metabolites based on calculated boiling points from COSMO-RS, experimental retention times, and mass spectral fragmentation patterns. *Analytical chemistry*. 2015; 87:2299–2305. [PubMed: 25565148]

- Singh UC, Kollman PA. An approach to computing electrostatic charges for molecules. *Journal of Computational Chemistry*. 1984; 5:129–145. DOI: 10.1002/jcc.540050204
- Su G, Yu H, Lam MHW, Giesy JP, Zhang X. Mechanisms of toxicity of hydroxylated polybrominated diphenyl ethers (HO-PBDEs) determined by toxicogenomic analysis with a live cell array coupled with mutagenesis in *Escherichia coli*. *Environmental science & technology*. 2014; 48:5929–5937. [PubMed: 24717064]
- Wiseman SB, Wan Y, Chang H, Zhang X, Hecker M, Jones PD, Giesy JP. Polybrominated diphenyl ethers and their hydroxylated/methoxylated analogs: environmental sources, metabolic relationships, and relative toxicities. *Marine pollution bulletin*. 2011; 63:179–188. [PubMed: 21439595]
- Zhao J, Zhu X, Xu T, Yin D. Structure-dependent activities of polybrominated diphenyl ethers and hydroxylated metabolites on zebrafish retinoic acid receptor. *Environmental Science and Pollution Research*. 2015; 22:1723–1730. [PubMed: 25077655]

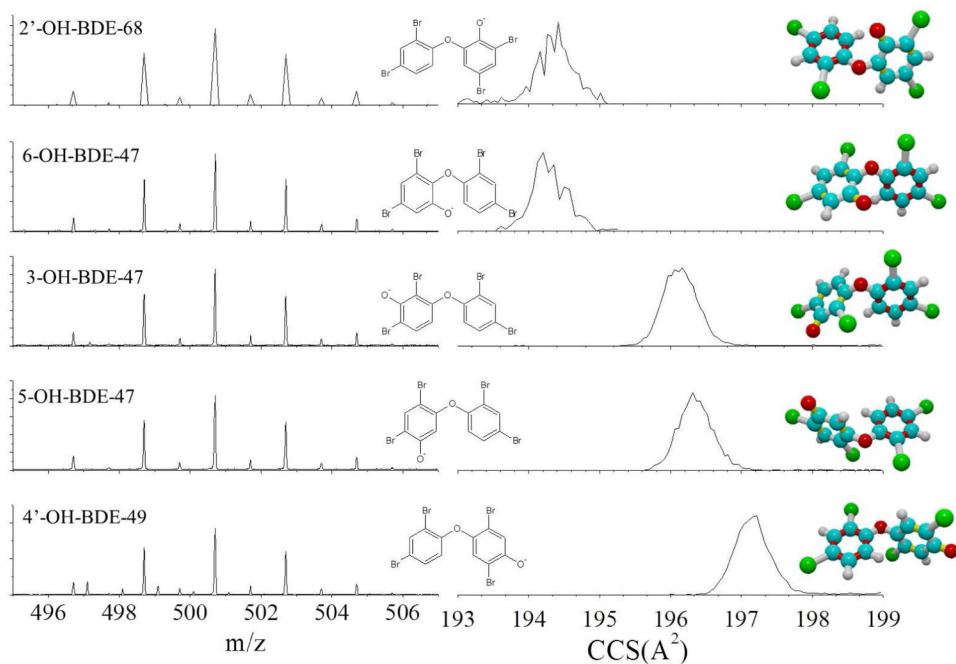


Figure 1. Typical mass spectra (left), IMS projections (middle) and candidate structures (right) of 2'-OH-BDE-68, 6-OH-BDE-47, 3-OH-BDE-47, 5-OH-BDE-47 and 4'-OH-BDE-49.

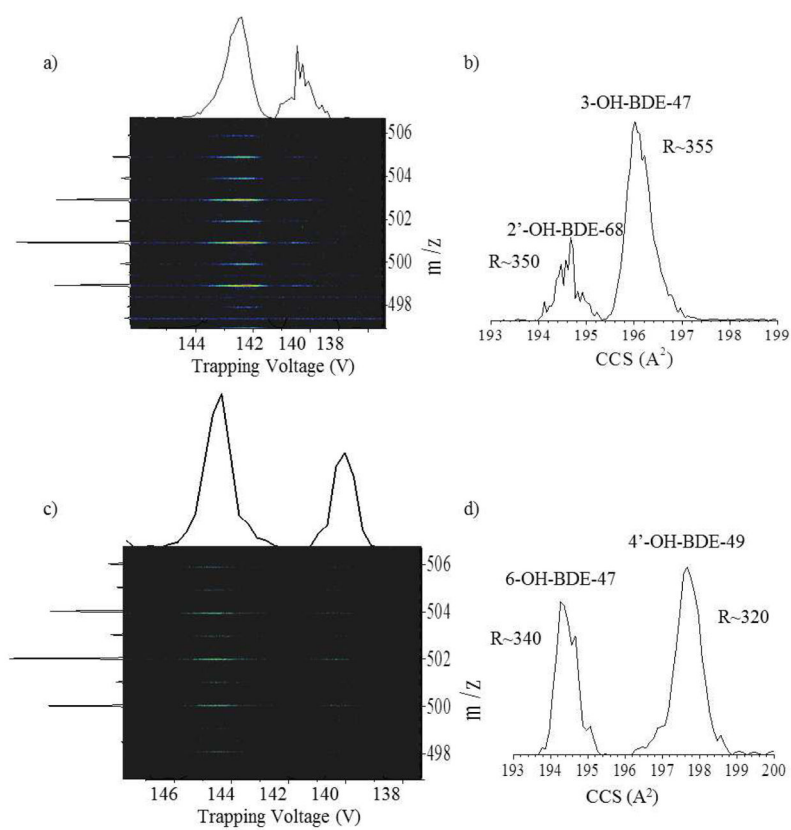


Figure 2. Typical 2D-IMS-MS contour and IMS projection plots for the binary mixture of 3-OH-BDE-47 and 2'-OH-BDE-68 (a) and b)) and the mixture of 6-OH-BDE-47 and 4'-OH-BDE-47 (c) and d)).

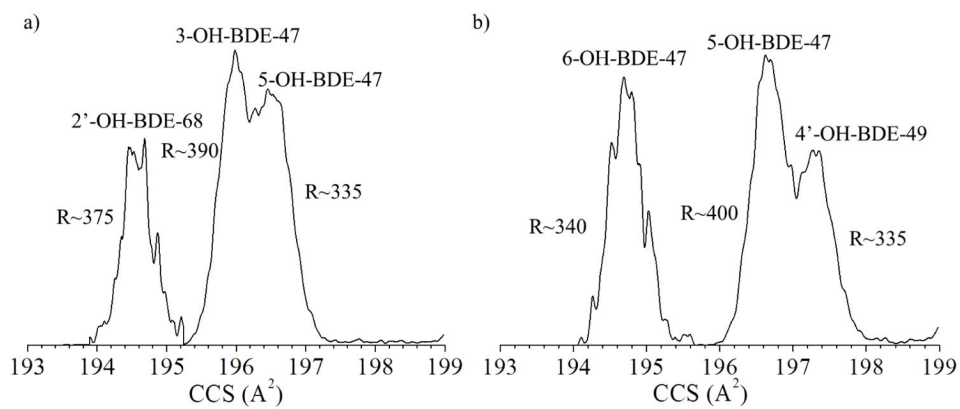


Figure 3. Typical IMS projection plots from the ternary mixture of 3-OH-BDE-47, 5-OH-BDE-47 and 2'-OH-BDE-68 (a) and the mixture of 4'-OH-BDE-49, 5-OH-BDE-47 and 6-OH-BDE-47 (b).

Table 1

Experimental and theoretical CCSs for of 2'-OH-BDE-68, 6-OH-BDE-47, 3-OH-BDE-47, 5-OH-BDE-47 and 4'-OH-BDE-4 isomers.

	[M-H] ⁻ m/z	Experimental	Theoretical
		TIMS (Å ²)	TM (Å ²)
2'-OH-BDE-68	500.7834	194.5	192
6-OH-BDE-47	500.7834	194.7	186
3-OH-BDE-47	500.7834	196.0	188
5-OH-BDE-47	500.7834	196.6	190
4'-OH-BDE-49	500.7834	197.3	193

Author Manuscript

Author Manuscript

Author Manuscript

Author Manuscript