



Published in final edited form as:

Bio Protoc. 2016 December 20; 6(24): . doi:10.21769/BioProtoc.2066.

Quantitative 3D Time Lapse Imaging of Muscle Progenitors in Skeletal Muscle of Live Mice

Micah T. Webster¹, Tyler Harvey^{1,2}, and Chen-Ming Fan^{1,*}

¹Department of Embryology, Carnegie Institution for Science, Baltimore, USA

²Department of Biology, Johns Hopkins University, Baltimore, USA

Abstract

For non-optically clear mammalian tissues, it is now possible to use multi-photon microscopy to penetrate deep into the tissue and obtain detailed single cell images in a live animal, *i.e.*, intravital imaging. This technique is in principle applicable to any fluorescently marked cell, and we have employed it to observe stem cells during the regenerative process. Stem cell-mediated skeletal muscle regeneration in the mouse model has been classically studied at specific time points by sacrificing the animal and harvesting the muscle tissue for downstream analyses. A method for direct visualization of muscle stem cells to gain real-time information over a long period in a live mammal has been lacking. Here we describe a step-by-step protocol adapted from Webster *et al.* (2016) to quantitatively measure the behaviors of fluorescently labeled (GFP, EYFP) muscle stem and progenitor cells during homeostasis as well as following muscle injury.

Keywords

Muscle stem cell; Muscle progenitor; Muscle regeneration; Ghost fiber; Live imaging; Multi-photon microscopy; Second harmonic generation

Background

Long-term *in vivo* imaging of stem and progenitor cells was first used for hair follicles during continuous physiological regeneration without surgical procedure (Rompolas *et al.*,

*For correspondence: fan@ciwemb.edu.

¹Obstructions to light transmission include hair, red blood cells, the epimysium, and adhesive. These can be avoided by removing all loose hair from the leg during step 3d, minimizing skin removal and damage to vasculature during steps 3e and 3f, removing all membrane covering the exposed TA in step 3f, and ensuring that adhesive does not cover the exposed tissue in step 3i.

²Mounting the fluorodish on the leg can be quite challenging and may require some practice. Fitting a P1000 pipette tip on the adhesive tube can allow for easier access and delivery of adhesive to the interface of skin and glass at the perimeter of the exposed TA.

³A shroud placed over the stage/microscope may be necessary to block ambient light from causing high background signal, especially when using very sensitive non-descanned detectors (Figure 6).

⁴For long duration imaging sessions, repeated applications of water are needed. To overcome the hassle of pausing the experiment and applying water to the objective lens, a water delivery objective lens ring cover and pump apparatus can be used (New Era Pump Systems, Inc.).

⁵This protocol can be adapted to other fluorescent proteins (*i.e.*, tdT, CFP) by adjusting MP wavelength and detection filters accordingly.

⁶All reagents used in this protocol were purchased and used directly without any dilution or mixing.

2012). By contrast, stem cells for skeletal muscles are largely quiescent and inactive during the normal homeostatic state. An injury to the muscle is necessary to activate muscle stem cells to mount a regenerative process. *In vitro* live imaging of muscle stem/progenitor cells has been widely used to study them in artificial settings. To understand muscle stem cell behavior during regeneration in their native environment, we developed a method to image them during skeletal muscle regeneration. Our method allows up to 8 h of continuous imaging per session daily following injury. This is the first time that skeletal muscle stem cells have been observed *in vivo* in an injured/regenerative environment (Webster *et al.*, 2016).

Materials and Reagents

1. Lab tape (VWR, catalog number: 89097)
2. Razor blades for shaving hair (VWR, catalog number: 55411-060)
3. Kimwipes (ULINE)
4. Transfer pipette (Globe Scientific, catalog number: 137038)
5. Cyanoacrylate based adhesive that bonds skin to glass (*i.e.*, Loctite glass glue; [Amazon.com](https://www.amazon.com); Scognamiglio *et al.*, 2016)
6. Mouse with GFP or YFP expression in Pax7-expressing muscle stem cells (or cell types of interest); GFP and YFP Cre-reporter mice and Pax7-Cre-ERT2 mouse strains are available at Jackson Laboratory (THE JACKSON LABORATORY, catalog numbers: 021847, 006148, and 012476, respectively)
7. Isoflurane (Patterson Veterinary Supply, IsoFlo[®], catalog number: 07-806-3204; To be applied directly into the vapor chamber of equipment list 4; indicated by arrow in Figure 2)
8. EtOH, 70% (Decon Labs, catalog number: V1401)
9. Distilled water (in house)

Equipment

1. An inverted Leica SP5 (or equivalent) equipped with a Leica 25×/0.95 water objective, a 35 mm culture dish holder attached to the stage, and nondescanned detectors with a dichroic mirror separating the detectable spectrum (430–550 nm) at 495 nm (Figure 1)
2. Chamelion Vision laser (Coherent)
3. Heating pad with enough area to cover the animal on the microscope stage (Sunbeam 756–500 Heating Pad from [Amazon.com](https://www.amazon.com))
4. Animal anesthesia system equipped with induction chamber as well as tubing with nose-cone (VetEquip, catalog number: 901806). Please consult with the operation manual prior to use
5. 35 mm fluorodish (World Precision Instruments, catalog number: FD35–100)

6. Metal spatula (VWR, catalog number: 82027-530)
7. Heat protective glove (VWR)
8. Bunsen burner (VWR, catalog number: 89038-528)
9. Laminar flow fume hood
10. Fine tip forceps (Dumont #5 forceps) (Fine Science Tools, catalog number: 11252-30)
11. Fine scissors for cutting skin (straight, 11.5 cm) (Fine Science Tools, catalog number: 14058-11)
12. Spring scissors for cutting fascia (8 mm blades) (Fine Science Tools, catalog number: 15009-08)

Software

1. Leica SP5 software
2. Fiji (Fiji is an updated version of ImageJ, an open source image processing software; Schindelin *et al.*, 2012)
3. Imaris (Bitplane, version 7.6.4 for Windows X64)

Procedure

Ethical statement: All procedures discussed here are in accordance with and were approved by the Carnegie Institution for Science Institutional Animal Care and Use Committee.

1. Intravital imaging setup
 - a. Turn on inverted confocal microscope and multi-photon (MP) laser. Set MP to 920 nm for GFP detection, or 940 nm for EYFP detection.
 - b. Start Leica imaging software.
 - c. Turn on heating pad and warm to 35 °C.
 - d. Begin oxygen flow to anesthesia machine and then begin filling induction chamber with 1.7% isoflurane (by adjusting the turn dial on top of the container to 1.7) and the flow-meter indicator ball to 1 (for 1 L/min flow rate) (See Figure 2).
 - e. Place mouse in induction chamber to begin anesthetization (Figure 2) and continue onto making modified fluorodish. The anesthetized mouse can stay in the induction chamber for this duration (~20 min). If the fluorodish preparation takes longer, the mouse can be left in the induction chamber without concern, as they will continue to be placed under similar anesthesia condition during imaging.
2. Prepare modified fluorodish for mounting on mouse's leg
 - a. Wearing a heat protective glove, heat metal spatula over Bunsen burner in a fume hood.

- modified fluorodish should run parallel with the length of the mouse's limb to be imaged.
- i.** While holding the dish in place, apply adhesive where the skin of the leg is in contact with the glass. Apply adhesive around the entire perimeter and let the adhesive set for 90 sec or more while holding the dish in place.
 - j.** Begin filling the induction chamber with 1.7% isoflurane at 1 L/min. Maintain flow to the nose-cone.
 - k.** Once adhesive has set, return mouse to induction chamber and stop flow to the nose-cone.
- 4.** Position mouse for intravital imaging
- a.** Tape the anesthesia tube with nose-cone to the microscope stage.
 - b.** If using a water immersion objective, apply water to the surface of the objective.
 - c.** Switch delivery of 1.7% isoflurane at 1 L/min to the nose-cone outlet.
 - d.** Remove mouse from induction chamber and place on microscope stage, placing the head of the mouse into the nose-cone. Secure the head to the nose-cone with tape. The mouse should be positioned on its abdomen. When placed on its back, lungs often collapse prematurely terminating imaging (~1–2 h).
 - e.** Place the fluorodish in the culture dish holder affixed to the stage (Figure 5I).
 - f.** Raise the objective lens into position and identify the imaging field using the epifluorescence function of the Leica SP5. A piece of tape may be placed across the lower portion of the mouse's body (attached on either side to the stage) to reduce movement from respiration.
 - g.** Place heating pad over mouse (Figure 5II).
 - h.** Reduce anesthesia to 1.3% isoflurane at 1 L/min.
- 5.** Image capture parameters and analyses
- a.** Capture serial optical sections at 3 μm steps to a total depth of 150–200 μm every 3 min for up to 8 h. Scan fields of 0.31 to 0.62 mm^2 at 400 Hz. Following imaging, the mouse is sacrificed. Due to the adhesive used, it is not possible to remove fluorodish without causing additional tissue damage for proper suture, and the fluorodish is too bulky to be left on the mouse without affecting mobility.
 - b.** Image sequence files (.lif) can be opened in Fiji and converted to .tiff stacks or image sequences for analysis.

Data analysis

Data storage, transfer, and processing:

1. A Leica generated .lif file can range from 3 to 8 GB.
2. A single .tiff image sequence (converted from .lif using Fiji) is about 3 GB (3D time lapse).
3. A single .tiff stack (3D time lapse) is 1 GB.
4. A single .tiff stack (2D time lapse) is 100 MB.
5. An .avi movie is 20 MB.
6. Image sequences can be aligned using the Fiji plugin, ImageJ 2.0.0 'Correct 3D drift'.
7. Drift-corrected image sequences can be analyzed further with Fiji (*e.g.*, long axes and division angle measurements of cells, as well as measurements of cell migration direction). Imaris 7.6.4 is used for 4D rendering, cell tracking, migration statistics, and 4D movies.
8. The processed data (images and videos) and statistical analyses are published in Webster *et al.* (2016), which can be found at: [http://www.cell.com/cell-stem-cell/fulltext/S1934-5909\(15\)00503-2](http://www.cell.com/cell-stem-cell/fulltext/S1934-5909(15)00503-2)

Acknowledgments

The protocol reported here was supported by the NIAMS of the NIH under award numbers F32AR065366 (to MTW) and RO1AR060042 (to C-MF), as well as by intramural funds of the Carnegie Institution (to TH). This protocol is a modified version derived from a previous publication in Cell Stem Cell (cited in the reference, Webster *et al.*, 2016).

References

1. Rompolas P, Deschene ER, Zito G, Gonzalez DG, Saotome I, Haberman AM, Greco V. Live imaging of stem cell and progeny behaviour in physiological hair-follicle regeneration. *Nature*. 2012; 487:496–499. [PubMed: 22763436]
2. Schindelin J, Arganda-Carreras I, Frise E, Kaynig V, Longair M, Pietzsch T, Preibisch S, Rueden C, Saalfeld S, Schmid B, Tinevez JY, White DJ, Hartenstein V, Eliceiri K, Tomancak P, Cardona A. Fiji: an open-source platform for biological-image analysis. *Nat Methods*. 2012; 9(7):676–682. [PubMed: 22743772]
3. Scognamiglio F, Travan A, Rustighi I, Tarchi P, Palmisano S, Marsich E, Borgogna M, Donati I, de Manzini N, Paoletti S. Adhesive and sealant interfaces for general surgery applications. *J Biomed Mater Res B Appl Biomater*. 2016; 104(3):626–639. [PubMed: 25891348]
4. Webster MT, Manor U, Lippincott-Schwartz J, Fan CM. Intravital imaging reveals ghost fibers as architectural units guiding myogenic progenitors during regeneration. *Cell Stem Cell*. 2016; 18(2): 243–252. [PubMed: 26686466]



Figure 1. Inverted Multi-photon setup

The imaging setup includes an inverted confocal microscope with 25× water objective fitted with a culture dish holder, multi-photon laser and computer.

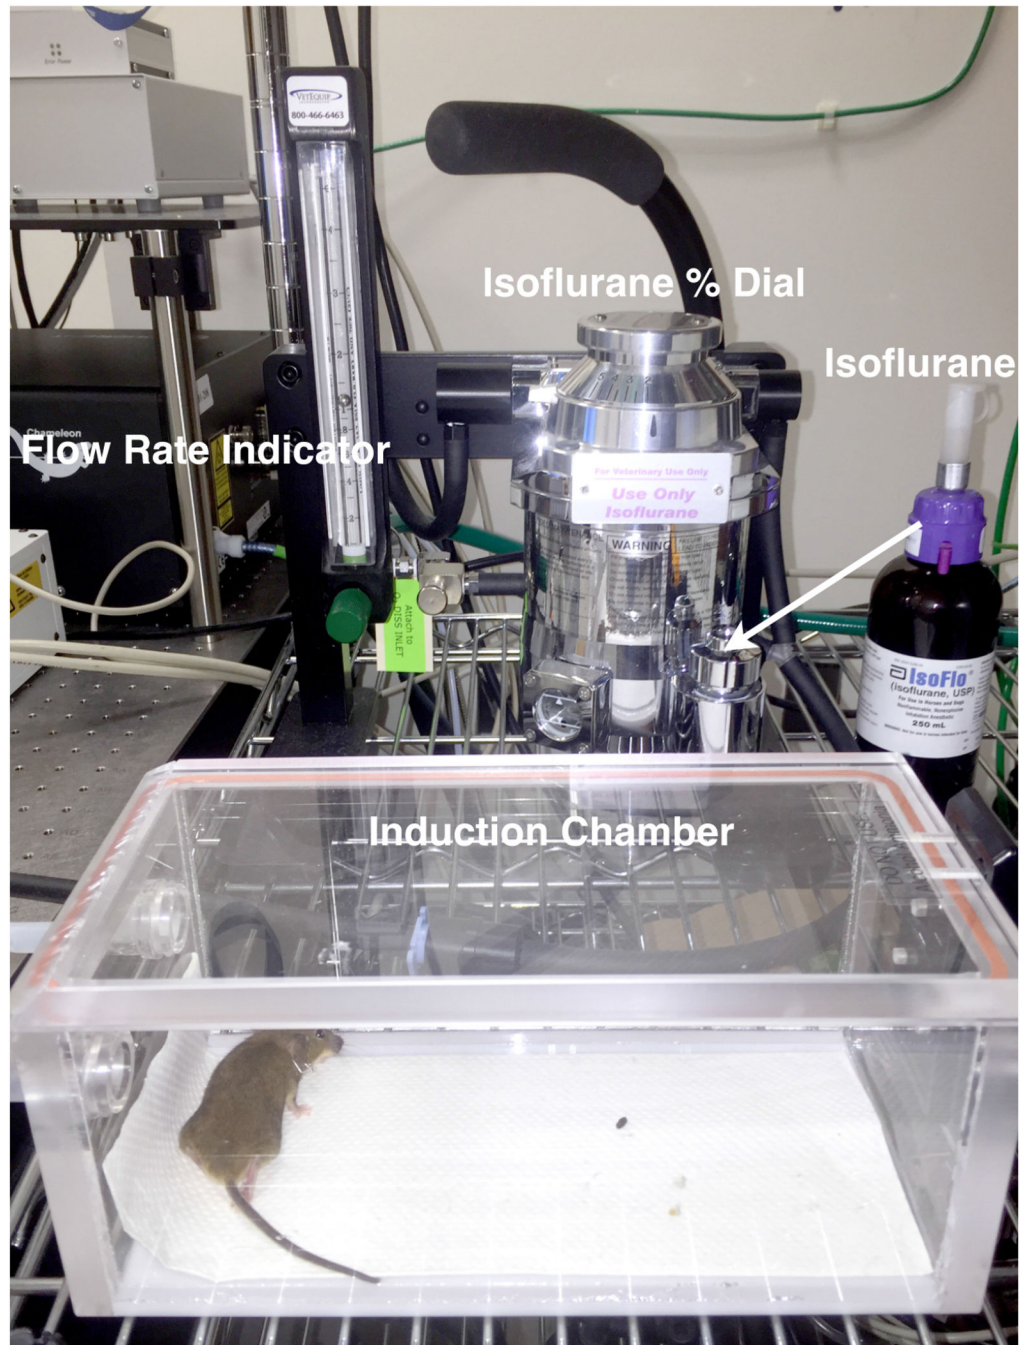


Figure 2. Anesthetization setup

This consists of anesthesia machine with regulator, induction chamber and nose-cone (pictured in Figure 4).

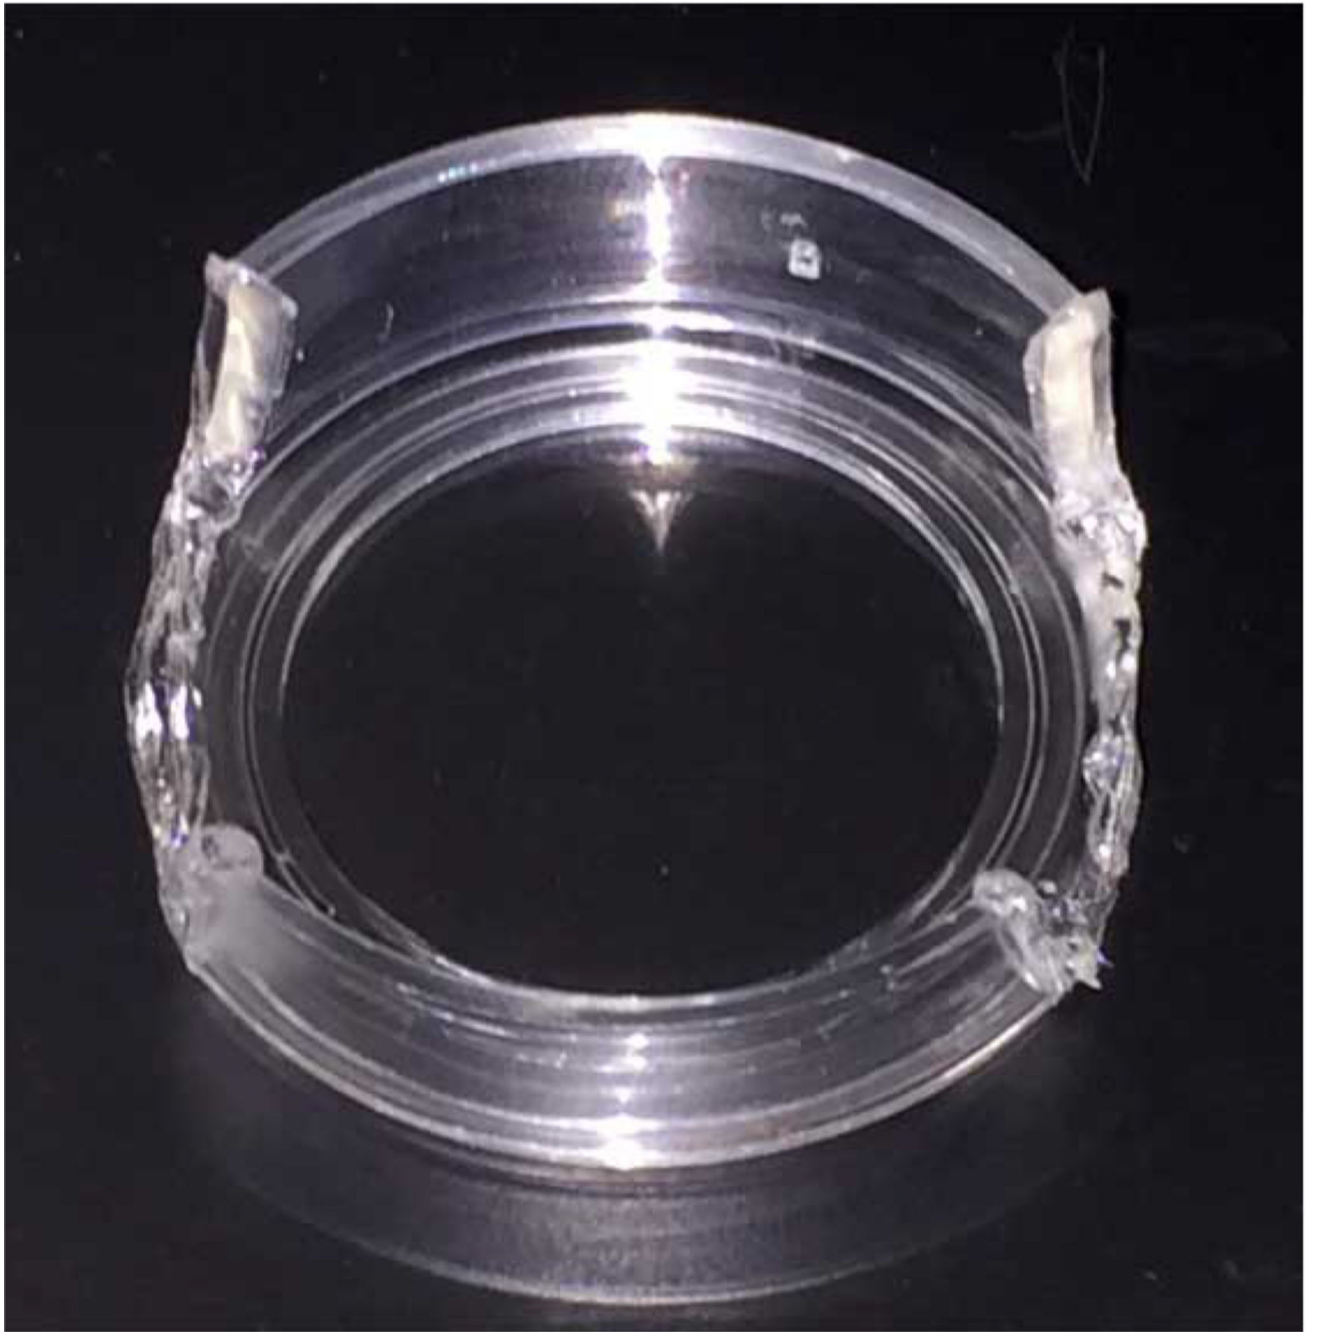


Figure 3. Modified fluorodish

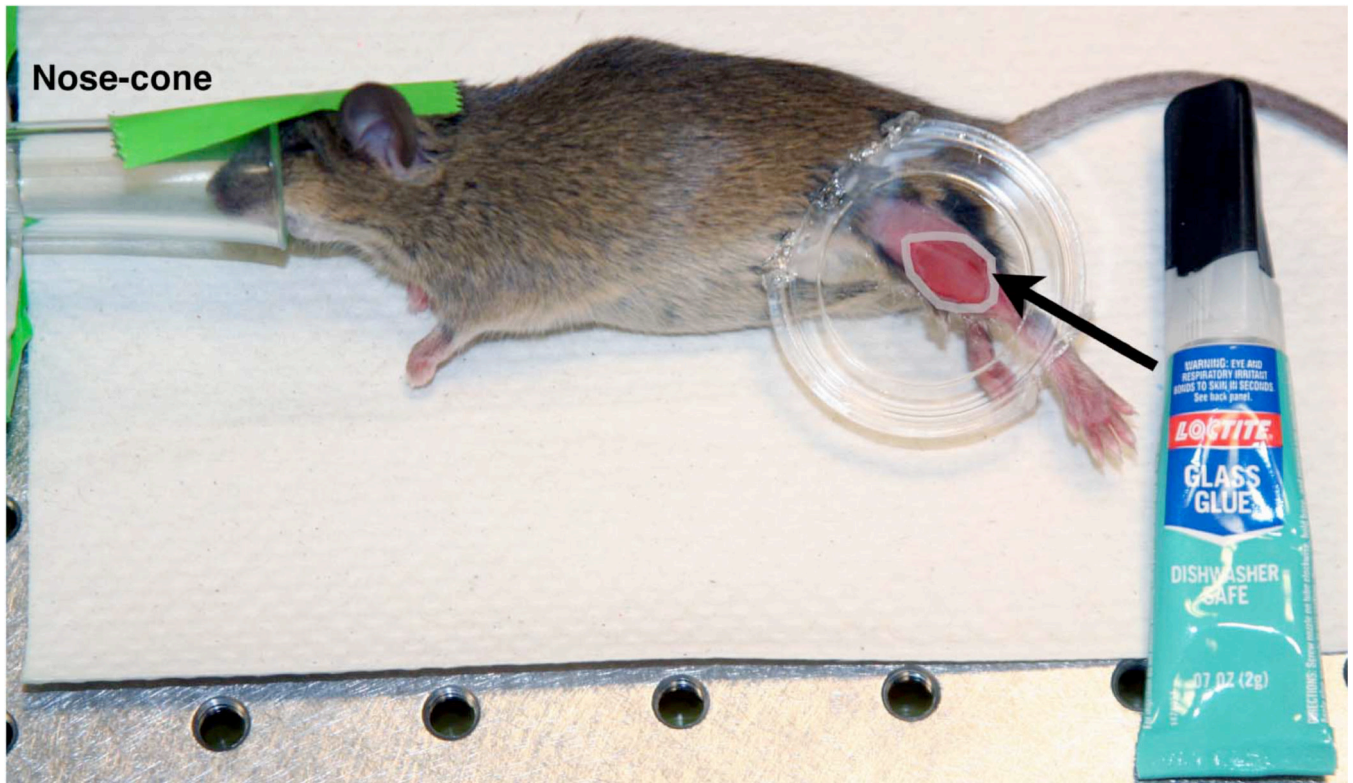


Figure 4. Fluorodish mounted on mouse
Pseudo-colored white ring indicates position to apply adhesive, performed using nose-cone anesthesia.

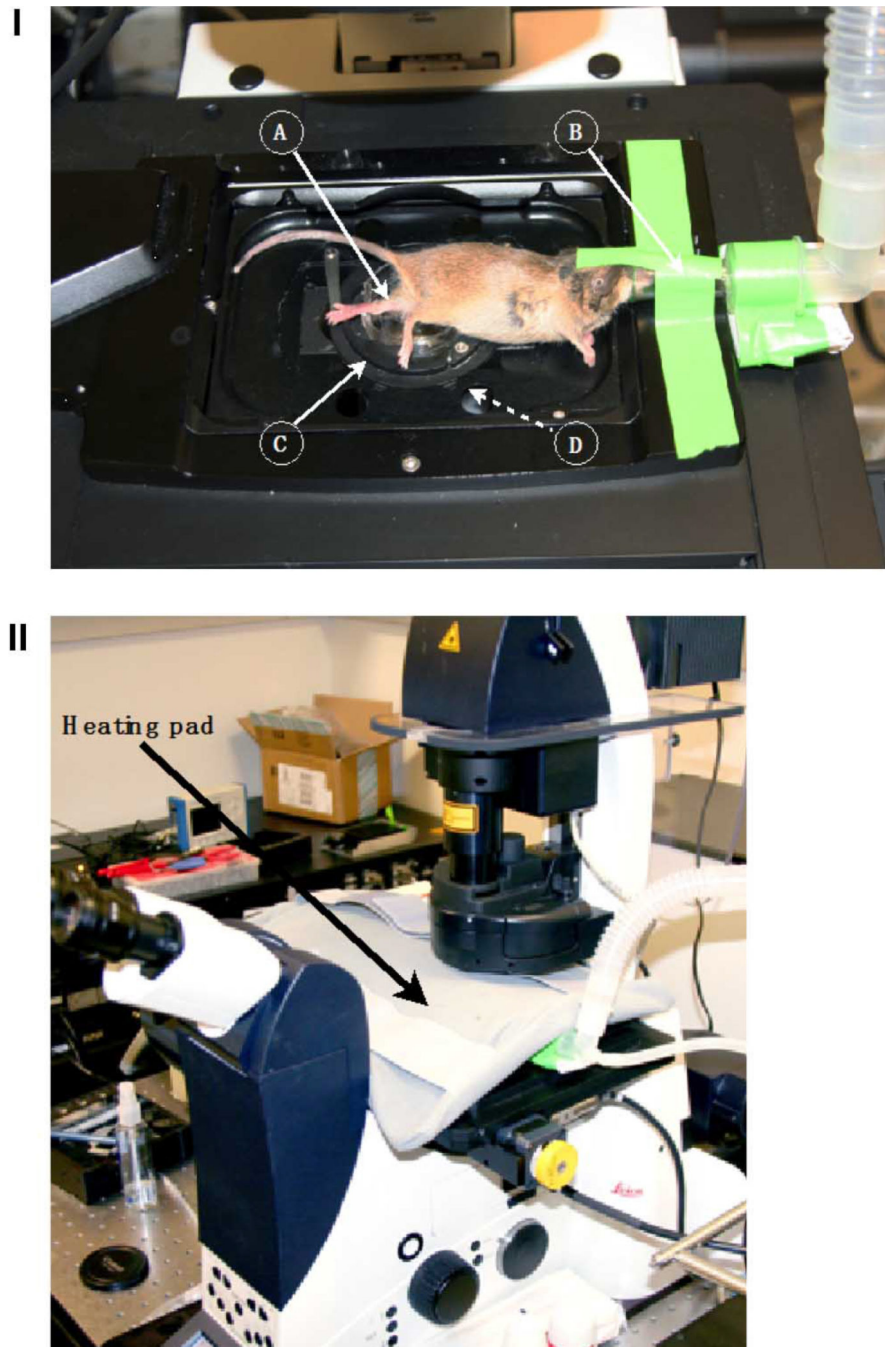


Figure 5. Mouse positioned for intravital imaging

I. Stage setup. A) Exposed TA muscle for imaging mounted to modified fluorodish. B) Nose-cone anesthesia apparatus adhered to stage. C) Culture dish holder. D) 25× water objective with H₂O (pictured below field of view). II. Microscope setup with positioned heating pad.

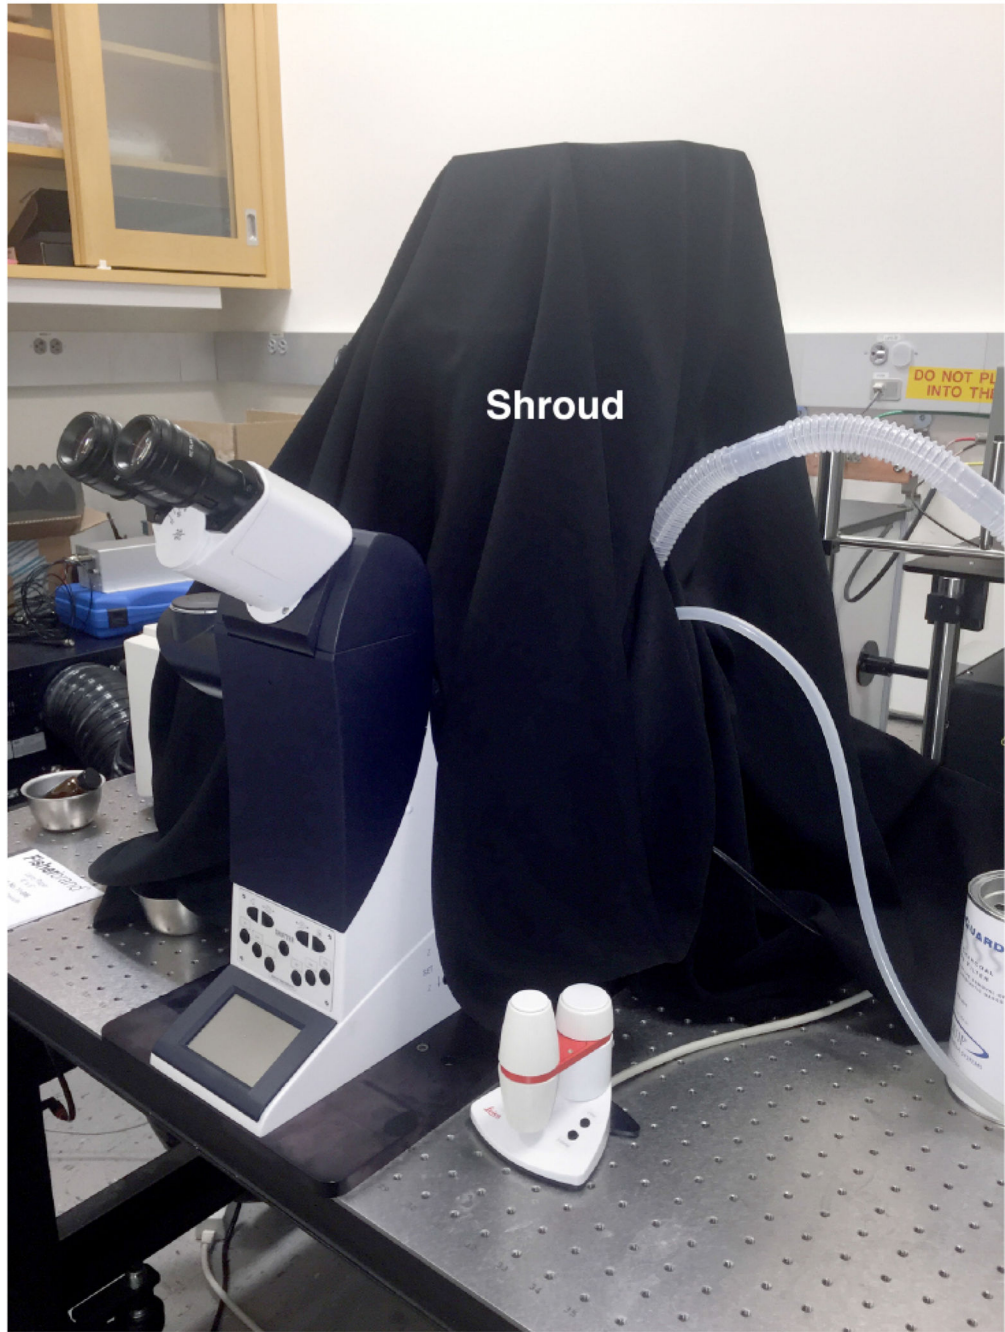


Figure 6. Imaging with shroud