

Case Report

A Case of Factitious Hyperglycemia in a Patient on Intravenous Ascorbic Acid

Eliza Sharma ¹, Christine Resta,² and Patricia Park²

¹Department of Internal Medicine, Maimonides Medical Center, Brooklyn, NY, USA

²Division of Endocrinology, Maimonides Medical Center, Brooklyn, NY, USA

Correspondence should be addressed to Eliza Sharma; Drelizasharma@gmail.com

Received 6 January 2018; Accepted 12 April 2018; Published 14 May 2018

Academic Editor: J. Paul Frindik

Copyright © 2018 Eliza Sharma et al. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Finger stick blood glucose meters are widely used in outpatient and inpatient settings. However, various factors can affect accuracy of readings from these meters. Here we present a patient who had spurious glucose elevation on these meters while being on intravenous ascorbic acid.

1. Introduction

Finger stick blood glucose (FSBG) meters are widely used to measure blood glucose levels in outpatient and inpatient settings; however, various factors can affect accuracy of glucose readings from these meters [1–4]. Here we present a case of marked interference with FSBG readings due to intravenous ascorbic acid.

2. Case Report

An 81-year-old female underwent coronary artery bypass graft surgery and replacement of mitral valve, with postoperative course complicated by dehiscence of sternal wound requiring wound vacuum assisted closure, sacral decubitus ulcer, multiple episodes of sepsis, and respiratory failure. Her past medical history was significant for prediabetes and end stage renal disease on hemodialysis. The patient's HbA1C at presentation was 6%, and her blood glucose was well-controlled during the first 45 days of admission with only 2 units total of sliding scale insulin required. She was started on intravenous ascorbic acid 10000 mg every 2 days to aid in sternal wound healing. Soon afterward, the patient had multiple high FSBG levels over 200 mg/dL, and she was treated with a total of 9 units of insulin in 24 hours. The FSBG levels remained high over the next few days with readings above 250 mg/dL. The patient was started on daily 10 units of glargine insulin, which was increased to 25 units over the

next few days. Of note, blood glucose in the metabolic panel (BGMP) ranged from 72 to 146 mg/dL, and a comparison of simultaneous FSBG and BGMP revealed a marked discrepancy of greater than 100 mg/dL between readings (Figure 1). These BGMP readings were obtained in the biochemistry laboratory of the hospital by the standard spectrophotometric technique. Given the suspicion for intravenous ascorbic acid causing falsely high FSBG readings in this individual without previous insulin requirements, it was discontinued. FSBG values decreased to normal. Fortunately, the patient did not have significant hypoglycemia while receiving the unnecessary insulin treatment.

3. Discussion

Measurement of serum glucose concentration by spectrophotometric technique using hexokinase method continues to be the gold standard and is used in clinical laboratories. However, monitoring of blood glucose using FSBG meters has greatly aided diabetes management. These FSBG meters make use of different enzymes including glucose oxidase, glucose dehydrogenase nicotinamide adenine dinucleotide (GDH-NAD), GDH flavin adenine dinucleotide (GDH-FAD), and GDH pyrroloquinolinequinone (GDH-PQQ). The enzymatic reaction of these enzymes with blood glucose generates an electrical current, the strength of which is proportional to the blood glucose level. FSBG meters relying on this analytic

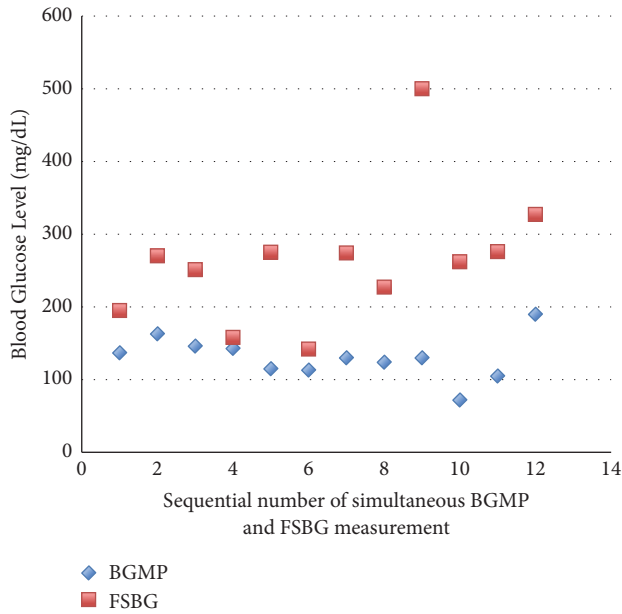


FIGURE 1: Discrepancy between simultaneous finger stick blood glucose (FSBG) and blood glucose in metabolic panel (BGMP).

method, known as amperometric detection, are widely used in outpatient and inpatient settings. However, they are subject to varying degrees of interference by different factors including hematocrit, blood oxygenation, presence of other sugars like maltose, and so on [1–4]. Furthermore, the Manufacturer And User Facility Device Experience (MAUDE) database maintained by the United States Food and Drug Administration links a large number of adverse events to improper use of these glucose meters in patients [5].

Ascorbic acid acts as an antioxidant and a cofactor and is required for different biological processes including synthesis of collagen and norepinephrine [6, 7]. High dose ascorbic acid is a nutraceutical used mainly by alternative medicine practitioners for various indications. It has long been used to aid in wound healing [8–10]. The benefit of ascorbic acid in cancer patients has been debated but continues to draw interest and wide use [11–14]. Patients with severe sepsis have a significantly depleted level of ascorbic acid, and its early supplementation has been shown to prevent morbidity and mortality in these patients [15, 16]. This has led to an increasing use of intravenous vitamin C in critical care setting. Physicians should, however, be aware of the potential for high dose intravenous ascorbic acid to cause erroneously high readings on FSBG meters [17–19]. This spurious glucose elevation results from glucose oxidase and glucose dehydrogenase oxidizing ascorbic acid with generation of electrical current measured as glucose. The error arises when the meter reads ascorbic acid as glucose, as the two molecules have similar molecular weights. In our patient, falsely high FSBG led to potentially harmful interventions while, in some other reported cases, patients developed life-threatening hypoglycemia [19]. Physicians must, therefore, understand the limitations of blood glucose meters. Most laboratories

measure serum glucose by spectrophotometric technique using the hexokinase method, which is specific for glucose and not affected by ascorbic acid. In this enzymatic method, hexokinase converts glucose to glucose-6-phosphate, which is then oxidized with concurrent reduction of nicotinamide adenine dinucleotide phosphate. The resulting increase in absorbance is measured. Furthermore, understanding the pharmacokinetics of ascorbic acid and waiting for at least 8–10 hours after intravenous ascorbic acid before reverting to FSBG meters to monitor blood glucose is preferred [20]. Blood glucose meters that utilize spectrophotometric methods are also available and may be used to avoid interferences in patients receiving intravenous ascorbic acid.

Conflicts of Interest

The authors declare that there are no conflicts of interest regarding the publication of this paper.

References

- [1] M. E. Lyon, L. B. Baskin, S. Braakman, S. Presti, J. Dubois, and T. Shirey, "Interference studies with two hospital-grade and two home-grade glucose meters," *Diabetes Technology & Therapeutics*, vol. 11, no. 10, pp. 641–647, 2009.
- [2] Z. Tang, R. F. Louie, J. H. Lee, D. M. Lee, E. E. Miller, and G. J. Kost, "Oxygen effects on glucose meter measurements with glucose dehydrogenase- and oxidase-based test strips for point-of-care testing," *Critical Care Medicine*, vol. 29, no. 5, pp. 1062–1070, 2001.
- [3] B. S. Karon, L. Griesmann, R. Scott et al., "Evaluation of the impact of hematocrit and other interference on the accuracy of hospital-based glucose meters," *Diabetes Technology & Therapeutics*, vol. 10, no. 2, pp. 111–120, 2008.
- [4] K. Dungan, J. Chapman, S. S. Braithwaite, and J. Buse, "Glucose measurement: Confounding issues in setting targets for inpatient management," *Diabetes Care*, vol. 30, no. 2, pp. 403–409, 2007.
- [5] United States Food and Drug Administration, "MAUDE - Manufacturer and User Facility Device Experience," <https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfMAUDE/Search.cfm>.
- [6] I. P. Ronchetti, D. Quagliano, and G. Bergamini, "Ascorbic Acid and Connective Tissue," in *Subcellular Biochemistry*, vol. 25 of *Subcellular Biochemistry*, pp. 249–264, Springer US, Boston, MA, 1996.
- [7] H. Katsuki, "Vitamin C and Nervous Tissue In Vivo and in Vitro Aspects," in *Subcellular Biochemistry*, vol. 25 of *Subcellular Biochemistry*, pp. 293–311, Springer US, Boston, MA, 1996.
- [8] T. V. Taylor, S. Rimmer, B. Day, J. Butcher, and I. W. Dymock, "ASCORBIC ACID SUPPLEMENTATION IN THE TREATMENT OF PRESSURE-SORES," *The Lancet*, vol. 304, no. 7880, pp. 544–546, 1974.
- [9] S. Ellinger and P. Stehle, "Efficacy of vitamin supplementation in situations with wound healing disorders: Results from clinical intervention studies," *Current Opinion in Clinical Nutrition & Metabolic Care*, vol. 12, no. 6, pp. 588–595, 2009.
- [10] W. M. Ringsdorf Jr. and E. Cheraskin, "Vitamin C and human wound healing," *Oral Surgery, Oral Medicine, Oral Pathology, Oral Radiology, and Endodontology*, vol. 53, no. 3, pp. 231–236, 1982.

- [11] E. Cameron and L. Pauling, "Supplemental ascorbate in the supportive treatment of cancer: prolongation of survival times in terminal human cancer," *Proceedings of the National Academy of Sciences of the United States of America*, vol. 73, no. 10, pp. 3685–3689, 1976.
- [12] A. Murata, F. Morishige, and H. Yamaguchi, "Prolongation of survival times of terminal cancer patients by administration of large doses of ascorbate," *International Journal for Vitamin and Nutrition Research*, vol. 23, pp. 103-13, 1982.
- [13] E. T. Creagan, C. G. Moertel, J. R. O'fallon et al., "Failure of High-Dose Vitamin C (Ascorbic Acid) Therapy to Benefit Patients with Advanced Cancer: A Controlled Trial," *The New England Journal of Medicine*, vol. 301, no. 13, pp. 687–690, 1979.
- [14] H. Fritz, G. Flower, L. Weeks et al., "Intravenous vitamin C and cancer: a systematic review," *Integrative Cancer Therapies*, vol. 13, no. 4, pp. 280–300, 2014.
- [15] A. C. Carr, P. C. Rosengrave, S. Bayer, S. Chambers, J. Mehrtens, and G. M. Shaw, "Hypovitaminosis C and vitamin C deficiency in critically ill patients despite recommended enteral and parenteral intakes," *Critical Care*, vol. 21, no. 1, article no. 300, 2017.
- [16] P. E. Marik, V. Khangoora, R. Rivera, M. H. Hooper, and J. Catravas, "Hydrocortisone, Vitamin C, and Thiamine for the Treatment of Severe Sepsis and Septic Shock: A Retrospective Before-After Study," *CHEST*, vol. 151, no. 6, pp. 1229–1238, 2017.
- [17] S. Vasudevan and I. B. Hirsch, "Interference of intravenous vitamin C with blood glucose testing," *Diabetes Care*, vol. 37, no. 5, pp. e93–e94, 2014.
- [18] Z. Sartor, J. Kesey, and S. Dissanaik, "The effects of intravenous vitamin C on point-of-care glucose monitoring," *Journal of Burn Care & Research*, vol. 36, no. 1, pp. 50–56, 2015.
- [19] S. K. Kim, J. R. Hahm, H.-S. Kim et al., "Spurious elevation of glucose concentration during administration of high dose of ascorbic acid in a patient with type 2 diabetes on hemodialysis," *Yonsei Medical Journal*, vol. 54, no. 5, pp. 1289–1292, 2013.
- [20] C. M. Stephenson, R. D. Levin, T. Spector, and C. G. Lis, "Phase i clinical trial to evaluate the safety, tolerability, and pharmacokinetics of high-dose intravenous ascorbic acid in patients with advanced cancer," *Cancer Chemotherapy and Pharmacology*, vol. 72, no. 1, pp. 139–146, 2013.