



Since January 2020 Elsevier has created a COVID-19 resource centre with free information in English and Mandarin on the novel coronavirus COVID-19. The COVID-19 resource centre is hosted on Elsevier Connect, the company's public news and information website.

Elsevier hereby grants permission to make all its COVID-19-related research that is available on the COVID-19 resource centre - including this research content - immediately available in PubMed Central and other publicly funded repositories, such as the WHO COVID database with rights for unrestricted research re-use and analyses in any form or by any means with acknowledgement of the original source. These permissions are granted for free by Elsevier for as long as the COVID-19 resource centre remains active.



## Serological immunochromatographic approach in diagnosis with SARS-CoV-2 infected COVID-19 patients

Yunbao Pan<sup>a,1</sup>, Xinran Li<sup>a,b,1</sup>, Gui Yang<sup>a</sup>, Junli Fan<sup>a</sup>, Yueting Tang<sup>a</sup>, Jin Zhao<sup>a</sup>, Xinghua Long<sup>a</sup>, Shuang Guo<sup>a</sup>, Ziwu Zhao<sup>a</sup>, Yinjuan Liu<sup>a</sup>, Hanning Hu<sup>a</sup>, Han Xue<sup>a,\*</sup>, Yirong Li<sup>a,\*</sup>

<sup>a</sup> Department of Laboratory Medicine, Zhongnan Hospital of Wuhan University, Wuhan University, No.169 Donghu Road, Wuhan, Hubei, China

<sup>b</sup> School of Biomedical Sciences, Li Ka Shing Faculty of Medicine, The University of Hong Kong, Hong Kong, China

### ARTICLE INFO

#### Article history:

Accepted 26 March 2020

Available online 10 April 2020

#### Keywords:

SARS-CoV-2

Covid-19

Real-time RT-PCR

Colloidal gold-based

Immunochromatographic strip

Serology

### SUMMARY

An outbreak of new coronavirus SARS-CoV-2 was occurred in Wuhan, China and rapidly spread to other cities and nations. The standard diagnostic approach that widely adopted in the clinic is nucleic acid detection by real-time RT-PCR. However, the false-negative rate of the technique is unneglectable and serological methods are urgently warranted. Here, we presented the colloidal gold-based immunochromatographic (ICG) strip targeting viral IgM or IgG antibody and compared it with real-time RT-PCR. The sensitivity of ICG assay with IgM and IgG combinatorial detection in nucleic acid confirmed cases were 11.1%, 92.9% and 96.8% at the early stage (1–7 days after onset), intermediate stage (8–14 days after onset), and late stage (more than 15 days), respectively. The ICG detection capacity in nucleic acid-negative suspected cases was 43.6%. In addition, the concordance of whole blood samples and plasma showed Cohen's kappa value of 0.93, which represented the almost perfect agreement between two types of samples. In conclusion, serological ICG strip assay in detecting SARS-CoV-2 infection is both sensitive and consistent, which is considered as an excellent supplementary approach in clinical application.

© 2020 The British Infection Association. Published by Elsevier Ltd. All rights reserved.

### Introduction

In December 2019, an outbreak of new coronavirus (SARS-CoV-2, also known as 2019-nCoV) infected pneumonia (COVID-19) was occurred in Wuhan, China and soon spread to other cities and countries. According to the epidemiological analysis conducted by the Chinese Center for Disease Control and Prevention (CCDC), 80.9% of the cases are mild/moderate pneumonia, and by February 11, the crude overall mortality rate is 2.3%.<sup>1</sup> As the epidemiological picture of COVID-19 is evolving daily, the global mortality rate of closed cases keeps rising ([www.worldometers.info/coronavirus/](http://www.worldometers.info/coronavirus/)). The clinical manifestations of most patients include fever, cough, shortness of breath and myalgia *etc.*, and radiographic evidence demonstrated pneumonia with multiple mottling and ground-glass opacity<sup>2</sup>. A fraction of patients in serious condition will proceed to complications including acute respiratory distress syndrome (ARDS) and cytokine storm, which may account for the reasons for COVID-19 caused death.<sup>3–5</sup> Despite the relatively low fatality, the transmissibility of COVID-19 is proved to be high. Basic


reproduction number ( $R_0$ ) of COVID-19 ranging from 1.4 to 6.47, while most of the modeling studies showed the  $R_0$  value greater than 3.<sup>6, 7</sup>

SARS-CoV-2 belongs to lineage B of the beta-coronavirus family, the zoonotic-origin single-strand RNA viruses that are transmitted between animals and people. The four prevalent viruses of seven coronavirus family members, 229E, OC43, NL63, and HKU1, cause only the mild upper respiratory diseases, while the other two highly pathogenic strains, SARS-CoV and MERS-CoV, together with the new identified SARS-CoV-2 are regarded to pose the global threats to public health. The full-genome sequencing data from two groups revealed that the SARS-CoV-2 comprises of six major open reading frames (ORFs) and shares approximately 80% of similarity with SARS-CoV, but 98.65% nucleotide identity to partial RdRp gene and 96.2% identity to RaTG13 of SARS-like bat coronavirus strain, respectively.<sup>8, 9</sup> Similar to SARS-CoV, SARS-CoV-2 recognizes the same cell entry receptor, angiotensin-converting enzyme II (ACE2). Real-time reverse-transcript Polymerase Chain Reaction (real-time RT-PCR) is regarded as the “gold-standard” in the diagnosis of SARS-CoV-2.<sup>10</sup> Designed primers targeting *ORF1ab*, envelope protein gene (E gene) or nucleocapsid protein gene (N gene) are proved to be both sensitive and specific toward the new SARS-CoV-2 virus and ruled out most of the other coronaviruses (229E,

\* Corresponding authors.

E-mail addresses: [58187532@qq.com](mailto:58187532@qq.com) (H. Xue), [93419136@qq.com](mailto:93419136@qq.com) (Y. Li).

<sup>1</sup> Equal contribution and co-first authors.

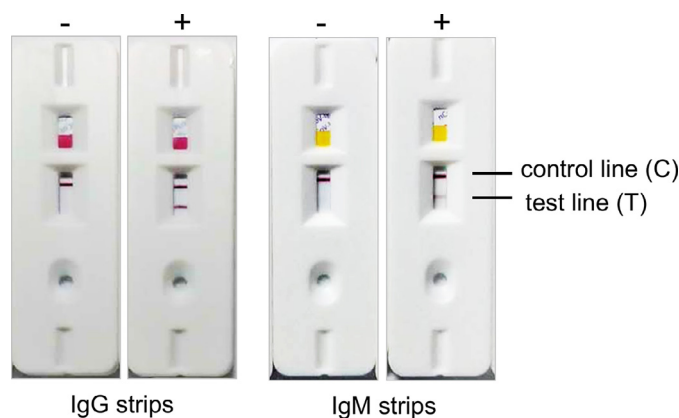

**Fig. 1.** Typical results of the ICG test strip for IgG (A) and IgM (B) antibodies against SARS-CoV-2. The representative results of negative (left) or positive (right) are shown. Upper line in each strip indicates control line (C), lower line in each strip indicates test line (T).

OC43 and MERS) and influenza viruses (H1N1, H3N2, H5N1, and H7N9 subtype).<sup>11, 12</sup>

Despite the real-time RT-PCR is widely adopted as the standard diagnostic method of SARS-CoV-2 in China and worldwide, the limitation of this technology is obvious. The patients that are positive to RT-PCR tests can be diagnosed as SARS-CoV-2 infection, while negative to the tests cannot rule out the possibility. The increasing number of reports from local authorities addressed the unneglectable false-negative rate in the diagnosis of suspected cases, which poses much threat to the community and adds an extra burden to the epidemic prevention. For example, the chest CT scanning from 5 suspected cases demonstrated ground-glass opacity and/or mixed consolidation, yet the initial real-time RT-PCR test showed to be negative. After a few days, all the 5 cases tested for the second or third examinations had eventually confirmed to be positive to SARS-CoV-2.<sup>13</sup> Complementary to RT-PCR, pneumonia radiography provides strong evidence for the diagnosis. Nevertheless, more specific measurements, such as serologic methods are urgently needed in the supplement to the current diagnosis. Here we present the newly developed serological detection methods targeting the viral antibody, colloidal gold-based immunochromatographic (ICG) strip, that conducted in Zhongnan Hospital of Wuhan University, hoping to provide supplementary diagnostic approaches for the SARS-CoV-2 infected patients.

## Methods

### Colloidal gold-based immunochromatographic (ICG) strip assay

The blood samples were collected, and blood serum, plasma or whole blood were subjected to ICG assay in accordant with the manufacturer's protocol (Zhuhai Livzon Diagnostic Inc.). In brief, 10  $\mu$ L of serum or plasma, or 20  $\mu$ L of whole blood samples were added onto the sample loading area followed by 100  $\mu$ L (2 drops) of sample dilution solution. After a short time (no longer than 15 min) of incubation, viral IgM- or IgG-containing positive samples (Fig. 1) could show up both the T line (test) and C line (control); the samples with only C line were regarded as negative (Fig. 1); the strips with no C line showed up should be considered as the invalid test.

### Real-time RT-PCR assay

Throat swab samples were collected and tested for SARS-CoV-2 with the Chinese Center for Disease Control and Prevention (CDC) recommended Kit (BioGerm, Shanghai, China), following

WHO guidelines for qRT-PCR. All samples were processed simultaneously at the Department of Laboratory Medicine of Zhongnan Hospital of Wuhan University. All patients were tested for SARS-CoV-2 by use of quantitative RT-PCR on samples from the respiratory tract. This study was reviewed and approved by the Ethical Committee of Zhongnan Hospital of Wuhan University. Written informed consent was waived by the Ethics Commission for emerging infectious diseases.

### Statistical analysis

In the ICG strip sensitivity assay with real-time RT-PCR confirmed cases and ICG detection capability with nucleic acid negative cases, the numbers of IgM positive, IgG positive and either IgM or IgG positive were counted, and the percentages and 95% confidence intervals were presented. In the ICG detection concordance analysis, the *Cohen's Kappa* test were calculated. *Kappa* values were shown in accompany with 95% confidence interval. *P* value of less than 0.05 is regarded as statistical significance.

### Data availability

The data that support the findings of this study are available from the corresponding author upon reasonable request.

## Results

### Information of COVID-19 confirmed or suspected patients

A total of 134 samples from 105 patients (48 male vs. 57 female), with a median age of 58 years (range from 20 to 96 years old) that hospitalized at Zhongnan hospital were enrolled in the study. Seventy-eight patients were collected the blood once, 25 patients were collected twice and 2 of the patients were collected three times. Among the samples, 95 of the samples from 76 patients were initially confirmed as SARS-CoV-2 infection by real-time RT-PCR, 8 of the patients were initially negative to nucleic acid detection but positive to the following tests; in total 39 nucleic acid negative samples from 37 of the patients were "clinically diagnosed" as SARS-CoV-2 infection according to the 5th edition of guideline on diagnosis and treatment of the novel coronavirus pneumonia. Specifically, the "clinical diagnosis" means the suspected cases were negative to the real-time RT-PCR test but presented viral pneumonia by radiography.

All the blood samples were collected between February 6 and February 21, and the ICG strip assay was performed between February 10 and 23. In total of 108 samples, including 86 of confirmed samples and 22 clinical diagnosed samples, were available for the symptom onset information (disease duration 0–34 days), which was range from January 7, 2020 to February 18, 2020, and subjected to the IgM or IgG sensitivity assay; the symptom onset information was not available for remaining 26 cases. Among all the samples, 39 "clinically diagnosed" samples from 37 patients were subjected to antibody detection capability in nucleic acid negative patients; 47 of the samples were used for the comparison of the consistency in plasma and whole blood samples, 13 of which were ruled out as the samples were expired.

### Sensitivity of IgM or IgG ICG strip assay

A total of 86 samples from 67 cases of real-time RT-PCR confirmed SARS-CoV-2 positive patients with disease duration information were subjected to the analysis. According to the disease progress stage calculated from the start of symptom onset, the disease was divided into early stage (1–7 days from onset), intermediate stage (8–14 days) and late stage (more than 15 days). As summarized in Table 1, the positive rates of IgM or IgG in the early

**Table 1**  
Sensitivity of IgM or IgG ICG strip assay in confirmed patients.

Disease duration	No. of sample	IgM+ No. (%; 95% CI)	IgG+No. (%; 95% CI)	IgM+ or IgG+ No. (%; 95% CI)
1–7 days	27	3 (11.1, 2.9–30.3)	1 (3.7, 0.2–20.9)	3 (11.1, 2.9–30.3)
8–14 days	28	22 (78.6, 58.5–91.0)	16 (57.1, 37.4–75.0)	26 (92.9, 75.0–98.8)
≥15 days	31	23 (74.2, 55.1–87.5)	30 (96.8, 81.5–99.8)	30 (96.8, 81.5–99.8)
In total	86	48 (55.8, 44.7–66.4)	47 (54.7, 43.6–65.3)	59 (68.6, 57.6–77.9)

The number of positive cases were shown here in accompany with percentages and 95% CI values. CI, confidence interval.

**Table 2**  
Detection capability of viral IgM or IgG in real-time RT-PCR negative patients.

Disease duration	No. of sample	IgM+ No. (%; 95% CI)	IgG+ No. (%; 95% CI)	IgM+ or IgG+ No. (%; 95% CI)
1–7 days	9	2 (22.2, 3.9–59.8)	4 (44.4, 15.3–77.3)	4 (44.4, 15.3–77.3)
8–14 days	6	2 (33.3, 6.0–75.9)	4 (66.7, 24.1–94.0)	5 (83.3, 36.5–99.1)
≥15 days	7	4 (57.1, 20.2–88.2)	5 (71.4, 30.3–94.9)	5 (71.4, 30.3–94.9)
In total	22	8 (36.4, 18.0–59.2)	13 (59.1, 36.7–78.5)	14 (63.6, 40.8–82.0)

The number of positive cases were shown here in accompany with percentages and 95% CI values. CI, confidence interval.

stage are relatively low, and gradually increase during the disease progression. The IgM positive rate rising from 11.1% of early stage to 78.6 and 74.2% in intermediate and late stage, respectively. The IgG positive rate in the confirmed patients is 3.6% in early, 57.1% in intermediate and 96.8% in late stage, respectively. Noteworthy, combining the result of IgM and IgG, i.e. patients with either IgM or IgG positive, would significantly increase the sensitivity of ICG assay, especially at the intermediate stage. While IgM and IgG positive rates at the intermediate stage are 78.6% and 57.1%, respectively, combining both parameters would bring a positive rate to 92.9%. Collectively, in response to the virus invade, the IgM was firstly produced against the virus; with the disease progression, IgG antibody start to produce and gradually become detectable. The sensitivity of ICG assays increase and peak at around 15 days. Combining both IgM and IgG would largely sensitize the result of ICG assay.

#### Antibody detection in nucleic acid-negative “clinically diagnosed” patients

According to the 5th edition of the guideline on diagnosis and treatment of the novel coronavirus pneumonia, highly suspected COVID-19 patients with real-time RT-PCR negative but with radiographic viral pneumonia were regarded as “clinically diagnosed” patients. Although the nucleic acid test is regarded as the “gold standard” of the diagnosis, due to certain limitations, the false-negative cases are not rare. Hence, the IgM and IgG anti-viral antibody were also examined in clinically diagnosed patients. In total 39 samples from 37 clinically diagnosed patients were included. Among these samples, 9 (23.1%) of them were positive to IgM and 15 (38.5%) of them were positive to IgG; when combine the IgG and IgM results in total 17 (43.6%) of samples were positive from 39 nucleic acid negative cases.

Considering the disease stage affects the detection of viral antibody, we also analyzed the clinically diagnosed patients in different stages. As shown in Table 2, 22 samples from clinical diagnosis patients with disease duration information were included. 9 cases were at early stage, 6 cases at the intermediate stage and 7 cases at late stage. The positive percentages of IgM at early, intermediate and late stages were 22.2%, 33.3% and 57.1%, respectively; the positive rate of IgG at early, intermediate and late stages were 44.4%, 66.7% and 71.4%, respectively. When it came to IgM and IgG combination, the positive rate boosted to 83.3% in cases at intermediate stage. Comparing with confirmed cases, the IgG and IgM positive rates were similar, albeit relatively lower. In accordant with nucleic acid positive cases, the IgG and IgM combinatorial detection strategy in clinically-diagnosed intermediate-stage patients

**Table 3**  
IgG detection concordance between whole blood and plasma samples.

	Serum/Plasma		In total
	+	-	
Whole Blood	23	0	23
In total	24	10	34
Cohen's kappa coefficient	0.93 (95% CI, 0.80–1.06; P-value, <0.000)		

CI, confidence interval.

demonstrated the maximal detection efficacy. In summary, IgM or IgG ICG strip detection in nucleic acid negative suspected patients showed promising detection capability, which would be an excellent supplementary approach in the clinically diagnostic application.

#### ICG assay concordance between whole blood and plasma samples

In order to test the concordance of whole blood samples with plasma, 34 paired whole blood and plasma samples were collected and subjected to IgM or IgG detection. Twenty-four of the plasma positive and 10 of the negative samples were used as a reference. Notably, all the IgM detection in whole blood samples showed 100% agreement with plasma samples. In the cases of IgG (shown in Table 3), 23 of the plasma positive samples were identified in whole blood samples, whereas 10 of the plasma negative samples were all negative in whole blood samples. To further address the consistency between whole blood and plasma, Cohen's kappa coefficient test was adopted for the analysis. The kappa coefficient value was 0.93 (95% CI, 0.80–1.06), which represented the almost perfect agreement between two types of the samples. Collectively, the whole blood antibody detection demonstrated strong agreements, which indicated that the whole blood samples showed excellent agreements with plasma samples.

#### Discussion

The late 2019 and early 2020 have witnessed the third and the largest coronavirus outbreak in recent two decades. Due to the limited knowledge related to the new virus SARS-CoV-2 at early stage of the outbreak and the capacity of virus with human-to-human transmissibility in the latent period, the infected cases were exponentially arising in Wuhan, the center of the epidemic, and rapidly spread to domestic and abroad areas. Scientific groups have quickly deciphered the viral whole-genome sequence and specific primers targeting SARS-CoV-2 were designed and tested preclin-



ically before massively diagnostic application in clinic. The viral whole-genome sequencing and viral nucleic acid detection by real-time RT-PCR are regarded as standard diagnostic approaches. While the whole-genome sequence is both time-consuming and labor-intensive, real-time RT-PCR is relatively fast and easy to carry out in hospital laboratories, which makes the latter technique as the “gold standard” of clinical diagnosis. However, the gold standard also has its limitations. Based on more than 3000 detected cases by real-time RT-PCR in the clinical laboratory of Zhongnan hospital, our previous review summarized several reasons for false-negative incidence, at both detection level and patients level.<sup>14</sup> From detection aspects, the quality and sensitivity of detection kits and viral preservation solutions from different companies may all affect the detection accuracy and result in the false-negative possibility. Besides, it is indicated that, during the disease progress, the heavy infection at the nasopharyngeal area of early stage would possibly become negative and the lower respiratory tract may severely be infected at late stage. Thus, the nasopharyngeal swab may not be the best sampling site for all patients at various disease stage. Moreover, patients with persistent anti-viral medication (such as anti-HIV drugs) may decrease the viral loading at the undetectable level. Therefore, additional detection techniques are urgently needed in the supplement to the current diagnostic shortages for the nucleic acid-negative suspected cases, whom would otherwise be ruled out.

In this study, we investigated the quick detection approach targeting viral IgM or IgG antibody, the colloidal gold-based immunochromatographic (ICG) strip assay, in comparison with real-time RT-PCR testing. The antibodies are produced and secreted by B lymphocytes of the adaptive immune system when the foreign pathogens invaded. IgM is usually the first responded antibody that eliminating pathogens before sufficient IgG is produced, while IgG serves as the most robust antibody-based immunity. From the retrospective study of immunoglobulins against SARS-CoV, IgM and IgG were started to be detected after 7 days of onset and persistent for 2–3 years.<sup>15, 16</sup> Similar to SARS-CoV, COVID-19 patients also showed similar characteristics. As demonstrated by Zhang et al., both IgM and IgG can be detected after 5 days of onset by anti-SARS-CoV-2 ELISA assay.<sup>17</sup> In accordant with Zhang et al., our study showed that both IgM and IgG were firstly detected on day 4 among the confirmed cohort and the positive rate of IgM and IgG were 11.1% and 3.6% in early stage patients, respectively. The positive rate of IgM remained approximately 75% in the intermediate and late stage patients, while IgG positive rate kept increasing during the disease progression and up to 96.8% of late-stage confirmed patients showed detectable IgG. Noteworthy, combining IgM and IgG detection results could reach the maximal testing efficacy, especially in intermediate stage. A similar trend could be captured in clinically diagnosed patients. In addition, the consistency rate of whole blood and plasma samples in IgM and IgG assays were 100% and 97.1%, respectively, demonstrating an excellent consistency between two types of samples. As the whole blood samples are capable of detecting antibody by ICG strip assay, the quick and massive viral detection in equipment-insufficient laboratories and communities is realizable.

The advantages of ICG strip viral antibody detection are obvious. First of all, the sensitivity of ICG strip is comparable, especially after 7 days of onset; the detection capacity in nucleic acid-negative “clinically diagnostic” patients is impressive. Therefore, ICG strip is highly recommended to be utilized as the supplementary diagnostic approach in clinical applications. The ICG strip can also be widely adopted in the areas where the diagnostic capacity is limited. Secondary, the ICG strip assay is operational as it is ready to use and time-saving. The assay can be finished within

15 min without specialized equipment. Thirdly, unlike oral swab sampling that may cause stimulated retching and coughing, which increases the exposure risk of laboratory technicians, the blood collection could avoid the unnecessary risk and reduce the operation steps that may cause aerosol. Fourthly, the detection of antibodies may also indicate the disease recovery, as immunoglobulins are among the most important soldiers in the battle of viruses. Patients that initially detected as virus-positive and gradually become negative but with detectable IgG or IgM during the disease progress may be considered as recovered from this battle. It is noteworthy that ICG strip can only provide qualitative results but the serological ELISA assay against viral antibody offered the quantitative antibody titer and regarded as the superior alternation at this point. Last but not least, ICG strip can be used for community surveillance. Some healthy people in epidemic areas may already get infected but without any symptoms, the detectable antibody from their blood is the evidence of infection. The surveillance detection in epidemic areas for both healthy members and patients could provide useful information for mapping the whole pictures of viral transmission, which would help us to better understand the real situation and establish optimal policies against the epidemic.

Although ICG strip assay is characterized as a rapid and sensitive complementary detection method against SARS-CoV-2, there are several limitations of our test. One is that the assay was carried out without specificity analysis. Our hospital is located in Wuhan, the center of the epidemic, and there are hundreds of, sometimes thousands of, confirmed or suspected COVID-19 cases each day. It is inoperable to select “uninfected” cases for the negative control of specificity analysis, as the patients received after the outbreak may possibly get infected with or without any symptoms. Such assay can be carried out in the areas where the epidemic is not severe and community transmission is at a low chance. Another limitation, as mentioned above, is that the ICG results are qualitative. Despite the positive bands on the strips may provide diverse gradations of color, i.e. deep or light red, the color itself doesn't correlate with the abundance of antibody. A more precise way of detecting antibody titer is by ELISA assay, though compromised the convenience.

Collectively, we provided a sensitive and consistent serology diagnostic approach in complementary to the current clinically used real-time RT-PCR testing in diagnosis with SARS-CoV-2 infected COVID-19 patients.

### Declaration of Competing Interest

The authors have no conflicts of interest to declare.

### CRediT authorship contribution statement

**Yunbao Pan:** Conceptualization, Data curation, Formal analysis, Methodology, Writing - review & editing. **Xinran Li:** Formal analysis, Writing - original draft. **Gui Yang:** Data curation. **Junli Fan:** Data curation. **Yueting Tang:** Data curation. **Jin Zhao:** Data curation. **Xinghua Long:** Data curation. **Shuang Guo:** Data curation. **Ziwu Zhao:** Data curation. **Yinjuan Liu:** Data curation. **Hanning Hu:** Data curation. **Han Xue:** Investigation. **Yirong Li:** Conceptualization, Funding acquisition, Investigation, Supervision.

### Acknowledgments

This work was supported by the National Key [Research and Development](#) Program of China (2018YFE0204500). We acknowledge all health-care workers involved in the diagnosis and treatment of patients in Wuhan.

## References

- Novel Coronavirus Pneumonia Emergency Response Epidemiology T [The epidemiological characteristics of an outbreak of 2019 novel coronavirus diseases (COVID-19) in China]. *Zhonghua Liu Xing Bing Xue Za Zhi* 2020;41:145–51.
- Chen N, Zhou M, Dong X, Qu J, Gong F, Han Y, Qiu Y, Wang J, Liu Y, Wei Y, Xia J, Yu T, Zhang X, Zhang L. Epidemiological and clinical characteristics of 99 cases of 2019 novel coronavirus pneumonia in Wuhan, China: a descriptive study. *Lancet* 2020;395:507–13.
- Wang D, Hu B, Hu C, Zhu F, Liu X, Zhang J, Wang B, Xiang H, Cheng Z, Xiong Y, Zhao Y, Li Y, Wang X, Peng Z. Clinical characteristics of 138 hospitalized patients with 2019 novel coronavirus-infected pneumonia in Wuhan, China. *JAMA* 2020. doi:10.1001/jama.2020.1585.
- Huang C, Wang Y, Li X, Ren L, Zhao J, Hu Y, Zhang L, Fan G, Xu J, Gu X, Cheng Z, Yu T, Xia J, Wei Y, Wu W, Xie X, Yin W, Li H, Liu M, Xiao Y, Gao H, Guo L, Xie J, Wang G, Jiang R, Gao Z, Jin Q, Wang J, Cao B. Clinical features of patients infected with 2019 novel coronavirus in Wuhan, China. *Lancet* 2020;395:497–506.
- Xu Z, Shi L, Wang Y, Zhang J, Huang L, Zhang C, Liu S, Zhao P, Liu H, Zhu L, Tai Y, Bai C, Gao T, Song J, Xia P, Dong J, Zhao J, Wang FS. Pathological findings of COVID-19 associated with acute respiratory distress syndrome. *Lancet Respir Med* 2020. doi:10.1016/S2213-2600(20)30076-X.
- Chen J. Pathogenicity and transmissibility of 2019-nCoV-A quick overview and comparison with other emerging viruses. *Microbes Infect* 2020. doi:10.1016/j.micinf.2020.01.004.
- Tang B, Wang X, Li Q, Bragazzi NL, Tang S, Xiao Y, Wu J. Estimation of the transmission risk of the 2019-nCoV and its implication for public health interventions. *J Clin Med* 2020;9.
- Chen L, Liu W, Zhang Q, Xu K, Ye G, Wu W, Sun Z, Liu F, Wu K, Zhong B, Mei Y, Zhang W, Chen Y, Li Y, Shi M, Lan K, Liu Y. RNA based mNGS approach identifies a novel human coronavirus from two individual pneumonia cases in 2019 Wuhan outbreak. *Emerg Microbes Infect* 2020;9:313–19.
- Zhou P, Yang XL, Wang XG, Hu B, Zhang L, Zhang W, Si HR, Zhu Y, Li B, Huang CL, Chen HD, Chen J, Luo Y, Guo H, Jiang RD, Liu MQ, Chen Y, Shen XR, Wang X, Zheng XS, Zhao K, Chen QJ, Deng F, Liu LL, Yan B, Zhan FX, Wang YY, Xiao GF, Shi ZL. A pneumonia outbreak associated with a new coronavirus of probable bat origin. *Nature* 2020. doi:10.1038/s41586-020-2012-7.
- Jin Y.H., Cai L., Cheng Z.S., Cheng H., Deng T., Fan Y.P., Fang C., Huang D., Huang L.Q., Huang Q., Han Y., Hu B., Hu F., Li B.H., Li Y.R., Liang K., Lin L.K., Luo L.S., Ma J., Ma L.L., Peng Z.Y., Pan Y.B., Pan Z.Y., Ren X.Q., Sun H.M., Wang Y., Wang Y.Y., Weng H., Wei C.J., Wu D.F., Xia J., Xiong Y., Xu H.B., Yao X.M., Yuan Y.F., Ye T.S., Zhang X.C., Zhang Y.W., Zhang Y.G., Zhang H.M., Zhao Y., Zhao M.J., Zi H., Zeng X.T., Wang Y.Y., Wang X.H., Management ftzHoWUNC, research team E-BMCoCIE, promotive association for M, health C. 2020. a rapid advice guideline for the diagnosis and treatment of 2019 novel coronavirus (2019-nCoV) infected pneumonia (standard version). *Mil Med Res* 7:4.
- Chu DKW, Pan Y, Cheng SMS, Hui KPY, Krishnan P, Liu Y, Ng DYM, Wan CKC, Yang P, Wang Q, Peiris M, Poon LLM. Molecular diagnosis of a novel coronavirus (2019-nCoV) causing an outbreak of pneumonia. *Clin Chem* 2020. doi:10.1093/clinchem/hvaa029.
- Corman VM, Landt O, Kaiser M, Molenkamp R, Meijer A, Chu DK, Bleicker T, Brunink S, Schneider J, Schmidt ML, Mulders DG, Haagmans BL, van der Veer B, van den Brink S, Wijsman L, Goderski G, Romette JL, Ellis J, Zambon M, Peiris M, Goossens H, Reusken C, Koopmans MP, Drosten C. Detection of 2019 novel coronavirus (2019-nCoV) by real-time RT-PCR. *Euro Surveill* 2020;25.
- Xie X, Zhong Z, Zhao W, Zheng C, Wang F, Liu J. Chest CT for typical 2019-nCoV pneumonia: relationship to negative RT-PCR testing. *Radiology* 2020. doi:10.1148/radiol.2020200343200343.
- Li J, Ye G, Chen L, Wang J, Li Y. Analysis of false-negative results for 2019 novel coronavirus nucleic acid test and related countermeasures. *Chinese J Laborat Med* 2020;43:E006.
- Wu LP, Wang NC, Chang YH, Tian XY, Na DY, Zhang LY, Zheng L, Lan T, Wang LF, Liang GD. Duration of antibody responses after severe acute respiratory syndrome. *Emerg Infect Dis* 2007;13:1562–4.
- Mo H, Zeng G, Ren X, Li H, Ke C, Tan Y, Cai C, Lai K, Chen R, Chan-Yeung M, Zhong N. Longitudinal profile of antibodies against SARS-coronavirus in sars patients and their clinical significance. *Respirology* 2006;11:49–53.
- Zhang W, Du RH, Li B, Zheng XS, Yang XL, Hu B, Wang YY, Xiao GF, Yan B, Shi ZL, Zhou P. Molecular and serological investigation of 2019-nCoV infected patients: Implication of multiple shedding routes. *Emerg Microbes Infect* 2020;9:386–9.