







Publisher Correction: Fast detection of SARS-CoV-2 RNA via the integration of plasmonic thermocycling and fluorescence detection in a portable device

Jiyong Cheong , Hojeong Yu, Chang Yeol Lee, Jung-uk Lee, Hyun-Jung Choi, Jae-Hyun Lee , Hakho Lee  and Jinwoo Cheon 

Correction to: *Nature Biomedical Engineering* <https://doi.org/10.1038/s41551-020-00654-0>, published online 3 December 2020.

In the version of this Article originally published, in Fig. 3f, in the first and third schematics of the synchronized Ferris wheel system shown in the bottom row, the labels of the samples were incorrect as '1' and '3'; in the first schematic these should have been '3' and '2', and in the third '2' and '1'. The original and corrected Fig. 3f is shown below. All versions of the Article have been amended.

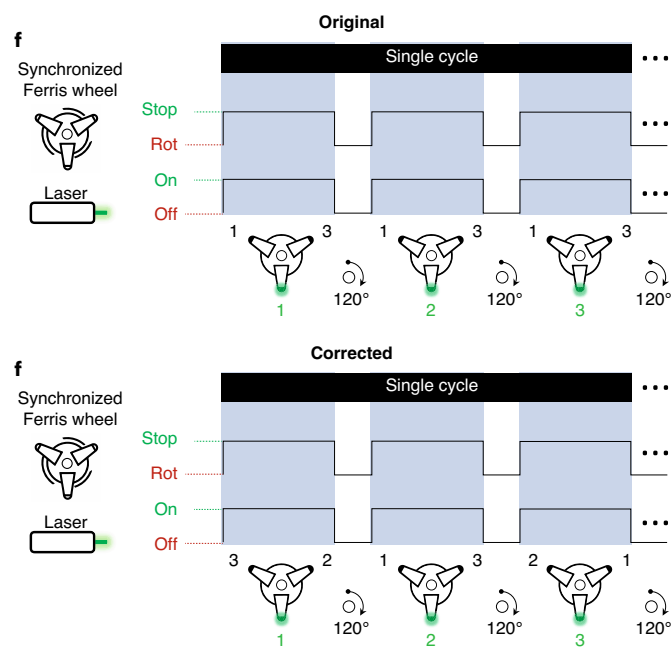


Fig. 3f | Original and corrected.

Published online: 17 December 2020

<https://doi.org/10.1038/s41551-020-00676-8>

© The Author(s), under exclusive licence to Springer Nature Limited 2020