



Since January 2020 Elsevier has created a COVID-19 resource centre with free information in English and Mandarin on the novel coronavirus COVID-19. The COVID-19 resource centre is hosted on Elsevier Connect, the company's public news and information website.

Elsevier hereby grants permission to make all its COVID-19-related research that is available on the COVID-19 resource centre - including this research content - immediately available in PubMed Central and other publicly funded repositories, such as the WHO COVID database with rights for unrestricted research re-use and analyses in any form or by any means with acknowledgement of the original source. These permissions are granted for free by Elsevier for as long as the COVID-19 resource centre remains active.

6. Ehrenfeld JM, Cassidy EA, Forbes VE, Mercaldo ND, Sandberg WS. Modified rapid sequence induction and intubation: a survey of United States current practice. *Anesth Analg* 2012; 115: 95–101
7. Casey JD, Janz DR, Russell DW. Bag-mask ventilation during tracheal intubation of critically ill adults. *N Engl J Med* 2019; 380: 811–21
8. Cook TM, El-Boghdady K, McGuire B, McNarry AF, Patel A, Higgs A. Consensus guidelines for managing the airway in patients with COVID-19: guidelines from the difficult airway society, the association of anaesthetists the intensive care society, the faculty of intensive care medicine and the royal college of anaesthetists. *Anaesthesia* 2020; 75: 785–99

doi: 10.1016/j.bja.2020.08.019

Advance Access Publication Date: 20 August 2020

© 2020 British Journal of Anaesthesia. Published by Elsevier Ltd. All rights reserved.

## Distanced-based dynamic behaviour of aerosol particles during aerosol-generating medical procedures

Ban C. H. Tsui\* and Stephanie Pan

Department of Anesthesiology, Perioperative, and Pain Medicine, Lucile Packard Children's Hospital at Stanford, Stanford, CA, USA

\*Corresponding author. E-mail: bantsui@stanford.edu


**Keywords:** aerosol-generating procedures; COVID-19; direct laryngoscopy; SARS-CoV-2; simulation; tracheal intubation; videolaryngoscopy

Editor—The coronavirus disease 2019 (COVID-19) pandemic caused by severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) has put the safety of healthcare providers at risk,<sup>1</sup> especially after aerosol-generating medical procedures such as tracheal intubation and extubation.<sup>2</sup> To improve the safety of healthcare providers, many aerosol-generating medical procedures have been modified and adapted in most clinical practices. For instance, recent guidelines for airway management in patients with COVID-19<sup>3</sup> recommend that all intubations be performed with videolaryngoscopy instead of direct laryngoscopy, not only to improve the success rate of a first-pass tracheal intubation, but also to distance healthcare providers from the airway and infectious aerosols. These recommendations are based on the assumption that increased distance from the patient's airway decreases the potential exposure to infectious droplets. However, the assumption that distance decreases infection risks remains unproved in the setting of aerosol-generating procedures. We therefore examined the relationship between distance and concentration of aerosols during simulated intubation of an airway manikin.

An aerosol nebuliser (Airlife Misty Max 10 Disposable Nebulizer, Carefusion, San Diego, CA, USA) introduced aerosolised saline into the trachea of an airway manikin to simulate passive breathing during intubation.<sup>4</sup> The particle concentrations ( $\mu\text{g m}^{-3}$ ) of particulate matter with diameter <1 mm ( $\text{PM}_1$ ), <2.5 mm ( $\text{PM}_{2.5}$ ), and <10 mm ( $\text{PM}_{10}$ ) were measured using a particle counter (Digital PM2.5 Air Quality Detector, Greekrit, Banggood, Guangzhou, China).<sup>4</sup> One particle counter was placed 30 cm above the manikin's head and the other was positioned 60 cm above the manikin's head to approximate the height of the healthcare provider performing an aerosol-generating procedure using direct laryngoscopy or

videolaryngoscopy. Measurements were taken every second for 5 min in the following sequence: (a) at time 0 min, the nebuliser was then activated for 3 min to simulate passive breathing during manual ventilation and intubation; (b) at time 3 min, the nebuliser was discontinued to simulate a secured airway; (c) measurements continued for an additional 2 min until particle concentrations reached baseline levels. The measurements were performed five times. The mean particle concentrations and their 95% confidence intervals are plotted (Fig. 1). All measurements were performed on a surgical bed at the centre of a standard operating room with laminar flow and an hourly air exchange rate of 27 with the door closed.

This study objectively measured and supports the assumption that increased distances decrease the particle concentrations for all particulate matter diameter sizes ( $\text{PM}_1$ ,  $\text{PM}_{2.5}$ , and  $\text{PM}_{10}$ ). However, this effect was limited to the first 30 s during an aerosol-generating procedure as seen in Figure 1. Beyond 30 s, the increased distance by 30 cm did not offer continued decreases in particle exposure. Particle concentrations became similar with multiple peaks between the two distances above the manikin's head. Although the mechanism of the observed multiple peaks is unclear, this may reflect the time required for redistribution and equilibration of aerosolised particles, especially those with smaller diameters, within the high dynamic airflow of a standard operating room. Because aerosolised SARS-CoV-2 droplets fall within two diameter sizes, between 0.25  $\mu\text{m}$  and 1  $\mu\text{m}$  and >2.5  $\mu\text{m}$ ,<sup>5</sup> we estimated the particle concentration of 'PM<sub>covid</sub>' by summing the particle concentrations of  $\text{PM}_1$  with the difference of  $\text{PM}_{10}$  minus  $\text{PM}_{2.5}$ .  $\text{PM}_{\text{covid}}$  mirrored the behaviour of the other particulate matter diameter sizes. Thus, although the benefit of decreased particle concentrations as a result of increased

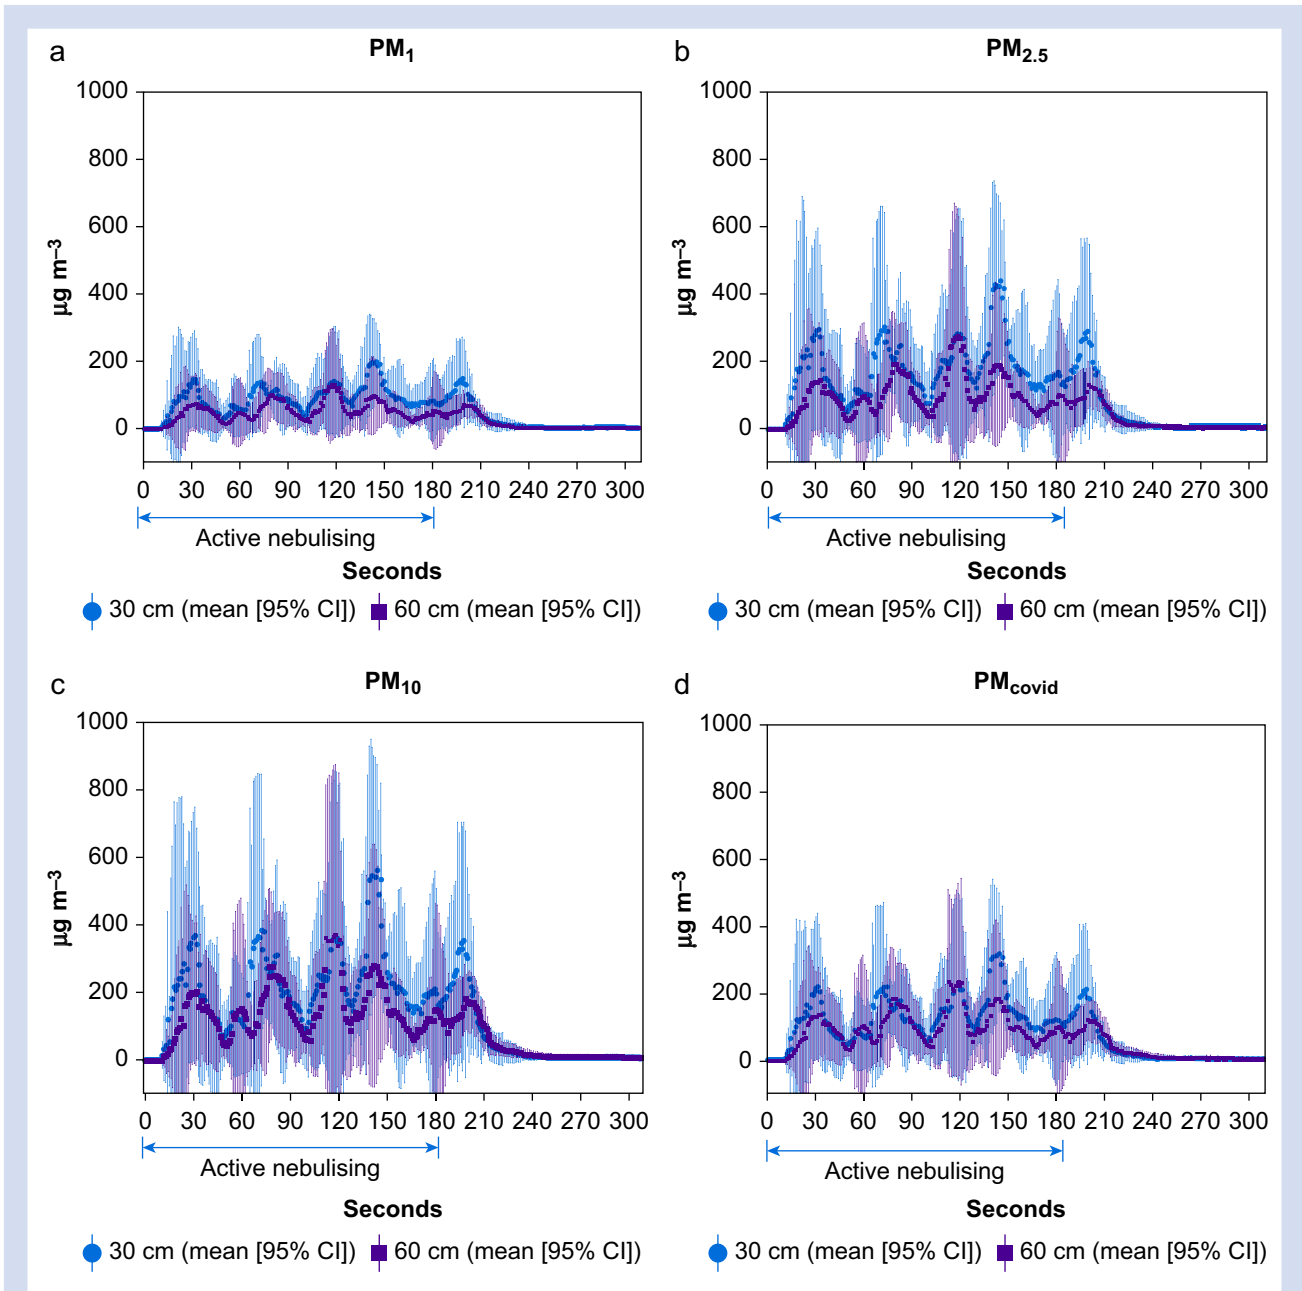

**Fig 1.** The mean of five measurements of particle concentrations ( $\mu\text{g m}^{-3}$ ) measured at 30 cm (red circle: mean [95% CI]) and 60 cm (blue solid square: mean [95% CI]) above the manikin’s head for particulate matter diameter sizes: (a)  $\text{PM}_1$ :  $<1 \mu\text{m}$ , (b)  $\text{PM}_{2.5}$ :  $<2.5 \mu\text{m}$ , (c)  $\text{PM}_{10}$ :  $<10 \mu\text{m}$ , and (d)  $\text{PM}_{\text{covid}}$ : sum of particulate matter diameter sizes  $<1 \mu\text{m}$  (i.e.  $\text{PM}_1$ ) and between 2.5 and  $10 \mu\text{m}$  to simulate severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) aerosols. CI, confidence interval.

distance is brief, it may be sufficient for most rapid intubations as the average intubation time is  $\sim 15 \text{ s}$ .<sup>5</sup>

Our study illustrates the potential benefits of increased distances in reducing aerosolised exposure during aerosol-generating procedures. However, the actual clinical benefit remains unknown. It is important to note that distances of 30 cm and 60 cm above the manikin’s head are greater than previously reported mean intubation distances of 15 cm during direct laryngoscopy and 35 cm during videolaryngoscopy,<sup>6</sup> although most healthcare providers have increased the

distance at which they perform aerosol-generating procedures during this pandemic. Thus, we decided to study distances of 30 cm and 60 cm as reflective of recent changes in clinical practice.

With experts bracing for a second wave of COVID-19 and the continued high incidence of infection from the first wave,<sup>7</sup> further studies are needed to refine our understanding of the behaviour of aerosolised particles and to better elucidate the assumptions we rely on to keep healthcare providers safe when performing aerosol-generating procedures. In addition

to distance, exposure to aerosolised particles is dependent on the duration of suspension, which is not only affected by particle size and concentration, but also by the surrounding air flow where the aerosol-generating procedure is performed. To prepare for a second wave and optimise safety, clinicians should assess the behaviour of aerosols and airflow dynamics within their individual clinical practices and operating rooms.

### Declarations of interest

The authors declare that they have no conflicts of interest.

### References

- Zhan M, Qin Y, Xue X, Zhu S. Death from Covid-19 of 23 health care workers in China. *N Engl J Med* 2020; **382**: 2267–8
- Heinzerling A, Stuckey MJ, Scheuer T, et al. Transmission of COVID-19 to health care personnel during exposures to a hospitalized patient - Solano County, California, February 2020. *MMWR Morb Mortal Wkly Rep* 2020; **69**: 472–6
- Yao W, Wang T, Jiang B, et al. Emergency tracheal intubation in 202 patients with COVID-19 in Wuhan, China: lessons learnt and international expert recommendations. *Br J Anaesth* 2020; **125**: e28–37
- Tsui BC-H, Deng A, Lin C, Okonski F, Pan S. Droplet evacuating strategy for simulated coughing during aerosol generating procedures in COVID-19 patients. *Br J Anaesth* 2020; **125**: e299–301
- Liu Y, Ning Z, Chen Y, et al. Aerodynamic analysis of SARS-CoV-2 in two Wuhan hospitals. *Nature* 2020; **582**: 557–60
- Hall D, Steel A, Heij R, Eley A, Young P. Videolaryngoscopy increases 'mouth-to-mouth' distance compared with direct laryngoscopy. *Anaesthesia* 2020; **75**: 822–3
- Xu S, Li Y. Beware of the second wave of COVID-19. *Lancet* 2020; **395**: 1321–2

doi: 10.1016/j.bja.2020.07.025

Advance Access Publication Date: 31 July 2020

© 2020 British Journal of Anaesthesia. Published by Elsevier Ltd. All rights reserved.

## Emergency schedule management for COVID-19

Benjamin Hardy\* and Chris Marshall

Worthing Hospital, Worthing, UK

\*Corresponding author. E-mail: [benjamin.hardy2@nhs.net](mailto:benjamin.hardy2@nhs.net)

**Keywords:** COVID-19; crisis management; intensive care; resource management; staff allocation

Editor—The coronavirus disease 2019 (COVID-19) pandemic brought a unique set of challenges to staff management owing to the need for the rapid redeployment of anaesthetists from theatres to cover the expansion of intensive care, while accommodating an increased absence rate because of sickness and self-isolation. As part of planning for the switch to an emergency rota, multiple options were considered by our management team, including adapting existing software and using free-to-use cloud-based collaborative tools offered by Google™. We decided to implement a new system that could be customised and adapted to crises more flexibly than our existing rota software (CLWRota, Rotamap Ltd., 3 Tottenham Street, London W1T 2AF, Registered in England No. 04551928, [info@rotamap.net](mailto:info@rotamap.net), +44 (0)20 7631 1555). A novel rota system was created using freely available online collaborative tools based on a system used in hospitals in London and Cambridge.<sup>1–3</sup> A perfect rota system would be free, easy to use by co-ordinators, and staff, able to record leave requests and alerts for self-isolation, individualised, and able to split the workforce into teams based on skill mix.<sup>4,5</sup> The new system was implemented in March 2020 and used to redeploy staff during the surge of COVID admissions until May 2020.

An online shared drive was created that contained the documents used to institute the emergency rota. The rota

management team could edit each file as it was being created. A spreadsheet was created with a rota template for the coming 4 months from implementation on March 30, 2020. The shift types were defined by their name and duration. All shifts were allocated on a centralised page that acted as a reference to other pages which displayed a personalised rota, a skills-based rota, and a daily on-call rota. In order to promote equality when allocating shifts, a live updated column next to each name included the mean number of hours per week as well as the number of night shifts and weekends.

The sheet was published as a PDF and on a website so staff members could access the rota at their leisure using their smartphone or desktop computer. A survey form was created that allowed individuals to report self-isolation, sickness, or request leave. This form triggered an email on completion sent to the rota co-ordination team to alert them to the new request. A document was created to contain links to each rota page for staff members that was published to the web in order to preserve the original document and sheet and protect them from being edited by staff members inadvertently. A dynamic shift pattern was used whereby reserve shifts were allocated to staff who were available to attend the hospital urgently to help with a sudden surge in demand. Shifts were colour co-ordinated in order to improve readability and highlight unallocated shifts. An automatic daily report was sent to senior