



## Research Article

# Establishment and Preliminary Application of a Rapid Fluorescent Focus Inhibition Test (RFFIT) for Rabies Virus

Pengcheng Yu, Xinjun Lv, Xinxin Shen, Qing Tang<sup>✉</sup> and Guodong Liang

*Key Laboratory of Medical Virology and Viral Diseases, Institute for Viral Disease Control and Prevention, Chinese Center for Disease Control and Prevention, Beijing 102206, China*

The World Health Organization (WHO) standard assay for determining levels of the rabies virus neutralization antibody (RVNA) is the rapid fluorescent focus inhibition test (RFFIT), which is used to evaluate the immunity effect after vaccination against rabies. For RFFIT, CVS-11 was used as the challenge virus, BSR cells as the adapted cells, and WHO rabies immunoglobulin (WHO STD) as the reference serum in this study. With reference to WHO and Pasteur RFFIT procedures, a micro-RFFIT procedure adapted to our laboratory was produced, and its specificity and reproducibility were tested. We tested levels of RVNA in human serum samples after immunization with different human rabies vaccines (domestic purified Vero cell rabies vaccine (PVRV) and imported purified chick embryo cell vaccine (PCECV)) using different regimens (Zagreb regimen and Essen regimen). We analyzed the levels of RVNA, and compared the immune efficacy of domestic PVRV and imported PCECV using different immunization regimens. The results showed that the immune efficacy of domestic PVRV using the Zagreb regimen was as good as that of the imported PCECV, but virus antibodies were generated more rapidly with the Zagreb regimen than with the Essen regimen. The RFFIT procedure established in our laboratory will enhance the comprehensive detection ability of institutions involved in rabies surveillance in China.

Rapid fluorescent focus inhibition test (RFFIT); RVNA; Rabies; Vaccination regimen

Rabies is one of the major zoonotic diseases caused by the rabies virus, and is almost always fatal in 100% of cases, once symptoms occur. Pre-exposure or post-exposure prophylaxis of rabies is the only effective way to prevent human rabies. In China, more than 1000 human rabies cases have occurred in recent years, and 87.5% of these cases were caused by dog bites (Yin C P, et al., 2011). Moreover, over 12 million people in China are inoculated every year with the rabies vaccine for pre-exposure and post-exposure prophylaxis.

The titer of the rabies virus-neutralizing antibody (RVNA) is an important parameter for evaluating the efficacy of the immunization vaccine for either pre-exposure or post-exposure prophylaxis for rabies. Detection of RVNA levels is also very important for laboratory diagnosis of

human rabies. The World Health Organization (WHO) recommends that booster immunizations should be carried out with reference to the titer of RVNA when it is <0.5 international units (IU) per mL (World Health Organization, 2005).

In October 2005, a WHO expert consultation on rabies recommended that evaluation of RVNA levels should be carried out using the rapid fluorescent focus inhibition test (RFFIT) or the fluorescent antibody virus neutralization test (FAVN) (World Health Organization, 2005). RFFIT is also one of the standard methods specified in the Pharmacopoeia of the People's Republic of China for evaluation of the efficacy of human rabies vaccines.

The RFFIT method is a neutralization test. When a fixed amount of rabies virus and serial dilutions of serum is neutralized, the remaining virus in each dilution is inoculated into cultured cells, and assessed using a specific anti-rabies nucleoprotein antibody labeled with fluorescein. The quantity of the remaining virus is calculated according to the number of infection foci produced by the remaining

Received: 2013-03-11, Accepted: 2013-07-24

Online First: 2013-07-25

Foundation item: National Department Public Benefit Research Foundation (201103032).

✉ Corresponding author.

Phone/Fax: +86-10-58900895, Email: qtang04@sina.com

virus. The titer of RVNA in the samples is calculated according to the number of virus infection foci and the quantity of the reference serum, and expressed as IU/mL.

In our laboratory, we established an RFFIT method according to the above procedure and preliminary work, in order to evaluate the efficacy of human rabies vaccination, and we present the results of this work below.

## MATERIALS AND METHODS

### Reagents

We used the WHO second international standard for rabies immunoglobulin (WHO STD), prepared by the WHO international laboratory, as the biological reference standard, with the titer of 30 IU/mL.

We also used an anti-rabies nucleoprotein antibody labeled with fluorescein (Rabies DFA Reagent; Millipore Corp., Billerica, MA, USA).

### Serum samples for specificity and repeatability

Two groups of human sera were used. Group A comprised 85 human sera (Guangzhou Center for Disease Control and Prevention (Guangzhou CDC), Guangzhou, China) which were used for testing the specificity of our RFFIT procedure: 40 human sera from individuals who had never been vaccinated with rabies vaccine, and 45 from individuals vaccinated by domestic PVRV using the Essen five-dose regimen. To test the repeatability of RFFIT, a second group of sera was used: group B comprised 15 human sera (Guangzhou CDC) from rabies-vaccinated individuals, which were tested triple using our RFFIT method.

### Experimental groups for different vaccines and regimens

We assessed whether different vaccination regimens would have an effect on efficacy. To evaluate the Zagreb 2-1-1 vaccination regimen and the Essen regimen, we recruited 112 healthy volunteers (sex and age were neglected) who were informed consent to receive post-exposure prophylaxis, and divided them into three groups. Group C comprised 50 subjects who received a domestic purified Vero cell rabies vaccine (SPEEDA PVRV) using the Zagreb 2-1-1 regimen; group D contained 32 subjects who received imported purified chick embryo cell rabies vaccine (PCECV) using the Zagreb 2-1-1 regimen; and group E consisted of 30 subjects who received PVRV (SPEEDA) using the Essen regimen (Table 1). From each subject, 5 mL of venous blood was collected on each of days 0 (before vaccination), 7, 14, and 45 (D0, D7, D14 and D45, respectively). The blood samples were centrifuged, and the isolated sera were frozen at -70 °C until tested.

Table 1. Comparison between different vaccines and regimens.

	Group C	Group D	Group E
Subjects, n	50	32	30
Vaccine	PVRV	PCECV	PVRV
Regimen	Zagreb	Zagreb	Essen
Injection	D0 (2 doses), D7, D21	D0 (2 doses), D7, D21	D0, D3, D7, D14, D28

D, day; PCECV, purified chick embryo cell vaccine; PVRV, purified Vero cell rabies vaccine. Group C: PVRV, Zagreb regimen; group D: PCECV, Zagreb regimen; group E: PVRV, Essen regimen.

### BSR cell culture

A BSR cell monolayer was grown for 3 days until it reached 100%. The monolayer was digested with trypsin, and suspended in DMEM-10 medium.  $1 \times 10^6$  cells/mL of BSR cell suspension was prepared and 2 mL suspension was inoculated into a 25 cm<sup>2</sup> flask, and cultured in 5% CO<sub>2</sub> in an incubator at 37 °C.

### Virus titration

The virus (CVS-11) was diluted in DMEM-10, using a set of five-fold serial dilutions (30 µL of virus added to 120 µL DMEM-10) in two adjacent lines in a 96-well plate. Then 50 µL virus suspension was removed from each well and transferred to the corresponding well of another 96-well plate, containing 100 µL DMEM-10 per well. After incubation at 37 °C for 1 hour, 50 µL BSR cell suspensions ( $1 \times 10^6$  cells/mL) were added to each well and incubated at 37 °C with 5% CO<sub>2</sub> for 24 hours.

Direct fluorescent assay (DFA) was conducted to calculate the foci of infection from CVS-11 using the Rabies DFA Reagent. The medium was removed and the cells were rinsed with PBS and fixed with 80% cold acetone at 4 °C for 30 minutes, then stained with the Rabies DFA Reagent solution. Finally, 60% glycerol-PBS was added, then the virus infection foci were counted under the microscope at 10× magnification, and the titer was calculated. This procedure was repeated for calculating the titer of the whole batch of virus, which was stored at -70 °C until required.

### Culturing of CVS-11

Prepared abundant of BSR cell suspension, CVS-11 virus at MOI = 0.1 was added to the BSR cell suspension and incubated at 37 °C with 5% CO<sub>2</sub> for 1 hour to adsorb adequately. The suspension was then transferred into cell culture flasks and incubated at 37 °C with 5% CO<sub>2</sub> for 72 hours. The virus-cell culture medium was mixed, divided into small tubes, labeled, and stored at -70 °C.

### RFFIT test procedure

The serum samples were denatured at 56°C for 30 minutes, each serum sample was diluted as a set of

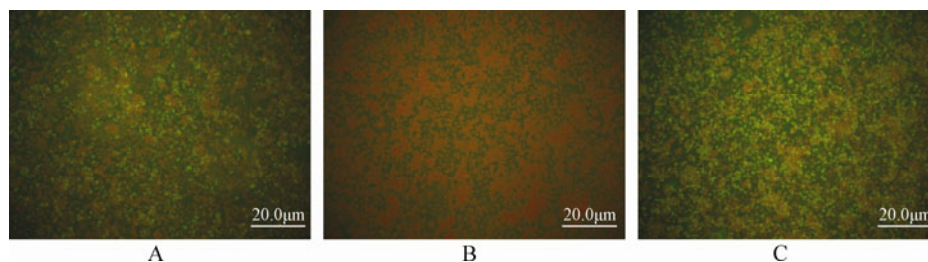


Fig. 1. Results for virus detection in control samples using the rapid fluorescent focus inhibition test. The red colors are the cells and the green are virus infections. (A) First well of negative serum control; (B) cell control; (C) virus control. Scale bar=20 μm.

three-fold serial dilutions using DMEM-10 in a 96-well plate. The control system included the WHO reference serum, negative serum control, virus control, and cell control. The WHO reference serum and negative serum were both diluted in the same way as the sample sera. A two-fold dilution for the virus control was also prepared. CVS-11 suspension (with sufficient quantity to infect 80% of cells in a single well) was added to each well with the exception of the virus and cell control wells. After neutralization at 37 °C for 1 hour, 50 μL BSR cell suspensions ( $1 \times 10^6$  cells/mL) were added to each well and incubated at 37 °C with 5% CO<sub>2</sub> for 24 hours.

DFA testing was conducted to measure the percentage of virus infection foci before and after 50% of cells infected, and these were used to calculate the titer of the serum samples.

## RESULTS

### Virus titration

Fluorescent foci were counted for the two wells in each line that first showed fluorescence (for example, in the first line N<sub>1</sub>, N<sub>2</sub> (N<sub>1</sub> > N<sub>2</sub>); the second line N<sub>1</sub>', N<sub>2</sub>' (N<sub>1</sub>' > N<sub>2</sub>')), then the virus titer was calculated as follows:

$$X(\text{FFU/mL}) = \frac{N \times \text{diluent fold} \times 1000}{\text{The virus volume added into the first well}}$$

$$N = (N_1 + N_2 \times 5 + N_1' + N_2' \times 5) / 4$$

5 means the dilution factor; diluent fold was the corresponding dilution of virus in N<sub>1</sub> and N<sub>1</sub>' wells; and the unit of virus titer was fluorescent focus units (FFU) per mL.

### Detection result of the controls

No fluorescent foci were found in the cell control wells, and >50% of cells were infected in the first well of the negative control, while the virus control wells had 80-90% fluorescent foci (Fig.1). Pictures were taken using a fluorescence microscope (IX51; Olympus, Tokyo, Japan).

### Calculation of the titer of anti-rabies neutralizing antibody

The neutralizing antibody titer was calculated (Excel software; Microsoft Corp., Redmond, WA, USA) using the Reed and Muench formula (see below), which measures the 50% end-point dilution of the standard serum (STD)

Table 2. Results of the specificity by RFFIT method.

	Unimmunized sera (n=40)	Immunized sera (n=45)
Negative	40 (0.01-0.1)	0
Positive	0	45 (0.63-461.67)

Data are given as mean (range) in IU/mL.

and the sample serum. The titer of the sample serum was calculated according to the following formula:

$$\begin{aligned} \text{Log (50\% end-point dilution)} &= \\ & \log(\text{starting point dilution}) - \text{difference between logarithms} \\ \text{Titer of the sample serum} &= \\ & \frac{50\% \text{ endpoint dilution of sample serum}}{d50\% \text{ endpoint dilution of STD}} \times \text{titer of STD} \end{aligned}$$

### Specificity and repeatability of RFFIT

Group A sera (40 never-immunized human sera and 45 human sera immunized with the Essen regimen) were tested using the RFFIT method. The results were summarized in Table 2. The specificity of RFFIT was 100%. A titer of >0.5 IU/mL was considered positive, and <0.5 IU/mL was considered negative.

In group B, 15 rabies-vaccinated sera were tested using the RFFIT test, by three independent researchers. The three sets of results (a, b, and c) and the coefficient of variance of the three result sets were calculated (Table 3). We used the same virus stock and same serum samples almost simultaneously. The results showed the RFFIT method had good repeatability (Fig. 2).

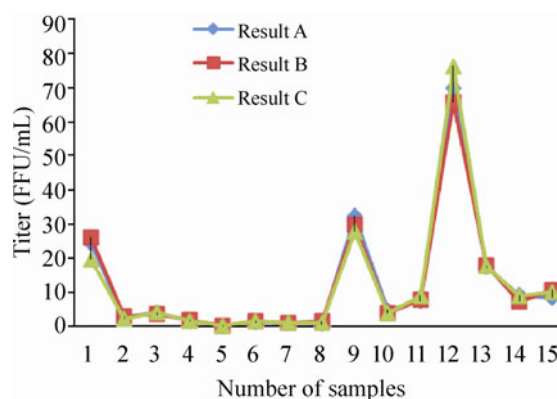


Fig. 2. Results for virus detection in experimental samples using the rapid fluorescent focus inhibition test, carried out by three independent researchers.

Table 3. Results of the repeatability of RFFIT method.

Sample number	Results, IU/mL			GMT, IU/mL	Standard deviation	CV
	a	b	c			
1	24.48	26.25	19.7	23.31	3.39	14.54
2	2.72	2.98	2.2	2.61	0.40	15.32
3	4.15	3.61	4.1	3.95	0.30	7.50
4	1.57	2.03	1.7	1.76	0.24	13.64
5	0.15	0.25	0.1	0.16	0.08	50
6	1.34	1.52	1.6	1.48	0.13	8.78
7	0.99	0.94	1	0.98	0.03	3.06
8	0.7	1.63	1.2	1.11	0.47	42.34
9	32.5	30	28	30.11	2.25	7.47
10	4.8	4	3.9	4.21	0.49	11.64
11	7.5	7.8	9	8.07	0.79	9.79
12	70	65.8	76.2	70.54	5.23	7.41
13	17.35	18	17.8	17.71	0.33	1.86
14	9.2	7.38	8.9	8.45	0.98	11.48
15	8.5	10.7	10.2	9.75	1.15	11.79

CV, coefficient of variation; GMT, geometric mean titer.

#### Amplification test of different vaccines and regimens

Using the RFFIT method, 433 serum samples collected from 112 volunteers by different vaccines and regimens (group C: PVRV-Zagreb, group D: PCECV-Zagreb and group E: PVRV-Essen) were tested and the results analyzed (Table 4).

Geometric mean titer (GMT) of all the subjects at D0 ranged from 0.01 to 0.06 IU/ml, confirming that these subjects were naive to rabies vaccination. At D7, seroconversion was higher for the PVRV-Zagreb than for the PVRV-Essen regimen, indicating that antibodies were generated more rapidly by the Zagreb 2-1-1 regimen than the Essen five-dose regimen for the same vaccine. Regardless of vaccine and regimen, all 112 subjects achieved RVNA titers >0.5 IU/mL on D14, and maintained this until D45. Interestingly, GMT was higher on D14 than D45 in the Zagreb regimen groups, indicating there was an increase in the antibody titer following the third vaccine dose on D7 than the increase after the fourth vaccine dose on D28. The rate of

positive seroconversion was 100% on D14 and D45 after vaccination in all groups, with no significant difference in GMT for the two regimens on D14 and D45 suggesting that both the Zagreb and Essen regimens had a similar good immunological response, but the RVNA generated more rapidly and achieved higher titers with the Zagreb regimen.

## DISCUSSION

Currently, the methods recommended by WHO and Office of International Epizootics (OIE) for detecting RVNA are the mouse neutralization test (MNT (mice)), RFFIT, and FAVN. MNT is the gold standard for the detection of RVNA internationally, but the test operation is cumbersome, time-consuming, and detrimental to animals. In 1992, the WHO Expert Committee on Rabies recommended use of RFFIT instead of MNT to detect RVNA. Compared with MNT, the RFFIT method is simpler and faster, has good repeatability, and does not use animals. Relative to the international RFFIT, our micro-RFFIT method is based on the Pasteur RFFIT procedure, conducted in 96-well plates rather than on 8-well cell culture slides, which can reduce the cost of experiments.

The results of our tests indicated that our RFFIT method has good specificity and repeatability. The amplification test also gave good results, which provided laboratory evidence for the formulation of a new immunization program. After the establishment of our RFFIT method, we also performed other amplifications, including comparison of the RFFIT test with different standard sera and test procedures using different reference sera. We obtained significantly different results using different reference sera in our RFFIT method, showing that there is a need to unify the reference sera used worldwide (Yu P C, et al., 2012).

Table 4. Results of different vaccines and different regimens.

Day	Group	Subjects, n	GMT, U/mL	Ranges	95% CI, IU/mL	N $\geq$ 0.5 IU/mL	Seroconversion, %
0	C	50	0.032	0.01-0.06	0.03-0.04	0	0
	D	32	0.029	0.01-0.06	0.03-0.04	0	0
	E	30	0.030	0.01-0.06	0.03-0.04	0	0
7	C	50	1.36	0.01-28.75	1.93-5.38	46	92
	D	31	0.55	0.01-62.96	1.18-10.75	22	70.97
	E	29	1.15	0.11-37.43	0.26-6.05	25	86.21
14	C	50	31.59	6.93-637.42	22.73-72.72	50	100
	D	29	34.63	6.90-452.20	28.93-102.86	29	100
	E	27	26.13	8.26-123.45	22.12-43.48	27	100
45	C	48	18.27	3.41-125.29	17.19-125.29	48	100
	D	31	12.67	2.30-243.75	11.49-47.98	31	100
	E	26	26.43	6.18-92.68	23.80-42.92	26	100

CV, coefficient of variation; GMT, geometric mean titer; PCECV, purified chick embryo cell vaccine; PVRV, purified Vero cell rabies vaccine. Group C: PVRV, Zagreb regimen; group D: PCECV, Zagreb regimen; group E: PVRV, Essen regimen.

In recent years, there have been various improvements made to the RFFIT method. In France, Péharpré *et al* conducted fluorescent foci counting using computer imaging techniques and fluorescence microscopy, and found that this gave more accurate RFFIT (Péharpré D, *et al.*, 1999), results, reducing the subjectivity of RFFIT identification. A Japanese study by Khawplod *et al.* using a recombinant rabies virus strain carrying a green fluorescent protein gene (rHEP-GFP) as the challenge virus for RFFIT showed that positivity could be observed directly without the need for a DFA test, which can reduce experimental expense and time.

In conclusion, we have established a new RFFIT protocol for RVNA, which can be used for detection of both human and animal RVNA. This test could be useful for investigations such as clinical diagnosis of rabies, detection of RVNA after rabies vaccination, preparation of immunoglobulin, evaluation of the effectiveness of new vaccines, and establishment of new immunization procedures. We hope it will enhance the comprehensive detection ability of institutions involved in rabies surveillance in China.

#### Acknowledgements

This work was supported by the National Department Public Benefit Research Foundation (201103032).

#### Author contributions

Conceived and designed the experiments: P Yu, Q Tang, and GD Liang; performed the experiments: P Yu; X Lv and X Shen helped with cell culture; P Yu and Q Tang wrote the paper.

#### References

- Yu P C, Noguchi A, Inoue S, Tang Q, Rayner S, Liang G D. 2012. **Comparison of RFFIT test with different standard sera and test procedures.** *Virol Sin.* 27(3):187-193.
- Ministry of Health of the People's Republic of China. 2009. **Situation of rabies prevention and control in China.**
- World Health Organization. 2005. **WHO Expert Consultation on Rabies.** WHO technical report series #931. World Health Organization, Geneva, Switzerland.
- World Health Organization. 1992. **WHO Expert Committee on Rabies. 8th Report.** World Health Organization Press, Geneva, Switzerland.
- Yin C P, Zhou H, Wu H, Shen X X, Wang L H, Yin W W, Wang S M, Tang Q. 2011. **Epidemiological analysis of rabies in 2010, China.** *Chin J Exp Clinic Virol.* 25: 434-436. (in Chinese)
- Péharpré D, Cliquet F, Sagné E, Renders C, Costy F, Aubert M.. 1999. **Comparison of visual microscopic and computer-automated fluorescence detection of rabies virus neutralizing antibodies.** *J Vet Diagn Invest.* 11(4): 330-333.
- Khawplod P, Inoue K, Shoji Y, Wilde H, Ubol S, Nishizono A, Kurane I, Morimoto K 2005. **A novel rapid fluorescent focus inhibition test for rabies virus using a recombinant rabies virus visualizing a green fluorescent protein.** *J Virol Methods.* 125(1): 35-40.