



OPEN

Author Correction: A new sensitizer DVDMS combined with multiple focused ultrasound treatments: an effective antitumor strategy

Wenli Xiong, Pan Wang, Jianmin Hu, Yali Jia, Lijie Wu, Xiyang Chen, Quanhong Liu & Xiaobing Wang

Correction to: *Scientific Reports* <https://doi.org/10.1038/srep17485>, published online 03 December 2015

This Article contains errors in Figure 7B.

As a result of an error during figure assembly, images corresponding to sample U-2 were used also for samples U-1 and S-1. The correct images for these samples are shown below as Figure 1 and Figure 2.

The quantification shown in Figure 7B was done at the time of data acquisition and is therefore unaffected by this error. The conclusions of the Article are not affected by this correction.

Published online: 23 August 2021

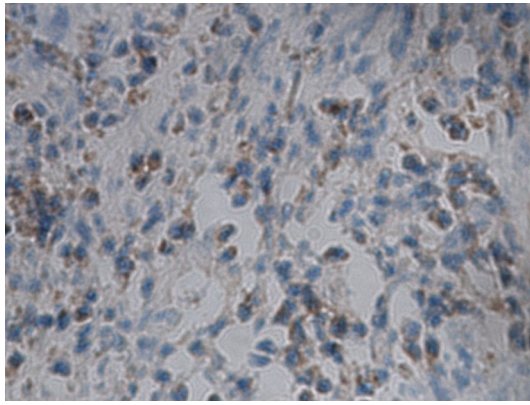


Figure 1. The VEGF level after treatment; sample U-1.

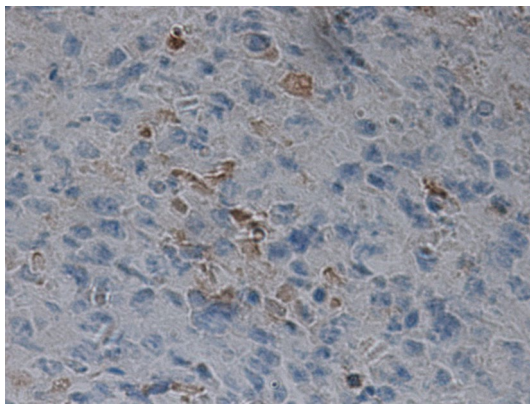


Figure 2. The VEGF level after treatment; sample S-1.



Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

© The Author(s) 2021