



RESEARCH ARTICLE

REVISED Fracture resistance and 3D finite element analysis of machined ceramic crowns bonded to endodontically treated molars with two planes versus flat occlusal preparation designs: an *in vitro* study [version 2; peer review: 2 approved, 1 approved with reservations]

Omnia Nabil , Carl Hany Halim, Ashraf Hassan Mokhtar

Department of Fixed Prosthodontics, Faculty of Dentistry, Cairo University, Cairo, 11553, Egypt

v2 First published: 08 Jul 2019, 8:1020
<https://doi.org/10.12688/f1000research.19455.1>
 Latest published: 11 Jun 2021, 8:1020
<https://doi.org/10.12688/f1000research.19455.2>

Abstract

Background: The flat occlusal preparation design (FOD) of posterior teeth offers promising results of fracture resistance and stress distribution, but its application in vital teeth is limited as there may be a danger of pulp injury. Although this danger is omitted in endodontically treated teeth, there is no research work assessing the impact of FOD on the fracture resistance and distribution of stresses among these teeth. The aim of this study was to assess the impact of FOD of endodontically treated molars on the fracture resistance and distribution of stresses among a ceramic crown-molar structure when compared to the two planes occlusal preparation design (TOD).




Methods: 20 human mandibular molars were endodontically treated and distributed equally to two groups: Group I (TOD) and Group II (FOD). Ceramic CAD/CAM milled lithium disilicate (IPS e.max CAD) crowns were produced for all preparations and adhered using self-adhesive resin cement. Using a universal testing machine, the fracture resistance test was performed. The fractured samples were examined using a stereomicroscope and scanning electron microscope to determine modes of failure. Stress distribution was evaluated by 3D finite element analysis, which was performed on digital models of endodontically treated mandibular molars (one model for each design).



Results: Group II recorded statistically non-significant higher fracture resistance mean values (3107.2 ± 604.9 N) than Group I mean values (2962.6 ± 524.27 N) as indicated by Student's t-test ($t=0.55$, $p=0.57$). Also, Group II resulted in more favorable failure mode as compared to Group I. Both preparation designs yielded low von-Mises stresses within the factor of safety. However, the stress distribution among

Open Peer Review

Approval Status



	1	2	3
version 2 (revision) 11 Jun 2021			 view
version 1 08 Jul 2019	 view	 view	

- Gürel Pekkan**, Tekirdag Namik Kemal University, Tekirdağ, Turkey
- Tarek Salah** , Ain Shams University, Cairo, Egypt
- Mostafa Aboushabha** , Future University in Egypt, Cairo, Egypt

Any reports and responses or comments on the article can be found at the end of the article.

different layers of the model differed.

Conclusions: FOD having comparable fracture strength to TOD and a more favorable fracture behavior can be used for the preparation of endodontically treated molars.

Keywords

Two planes occlusal preparation, Flat occlusal preparation, Endodontically treated molars, Ceramic-crown tooth structure, Fracture resistance, 3D Finite Element Analysis.

Corresponding author: Omnia Nabil (omnianabil@dentistry.cu.edu.eg)

Author roles: **Nabil O:** Conceptualization, Data Curation, Funding Acquisition, Investigation, Methodology, Project Administration, Writing – Original Draft Preparation; **Halim CH:** Conceptualization, Supervision, Validation, Writing – Review & Editing; **Mokhtar AH:** Conceptualization, Supervision, Validation, Writing – Review & Editing

Competing interests: No competing interests were disclosed.

Grant information: The author(s) declared that no grants were involved in supporting this work.

Copyright: © 2021 Nabil O *et al.* This is an open access article distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

How to cite this article: Nabil O, Halim CH and Mokhtar AH. **Fracture resistance and 3D finite element analysis of machined ceramic crowns bonded to endodontically treated molars with two planes versus flat occlusal preparation designs: an *in vitro* study [version 2; peer review: 2 approved, 1 approved with reservations]** F1000Research 2021, 8:1020
<https://doi.org/10.12688/f1000research.19455.2>

First published: 08 Jul 2019, 8:1020 <https://doi.org/10.12688/f1000research.19455.1>

REVISED Amendments from Version 1

In response to the reviewers' feedback, the following changes have been made to this article:

- In the introduction, added more info about the core build-up, the prosthetic materials, and the reasons for the choice of different restorative materials in endodontically treated teeth.
- In the methodology, added more details about teeth dimensions, access cavity preparation, master apical file, crown parameters, points of load application and a clarification of 3D scan in FEA.
- Also, in that section three figures have been added: diagram of tooth preparation, points of load application, and STL files showing components of crown-tooth structure as separate elements.
- The numbering of figures has been adjusted.
- Figure 6, caption has been changed to Column chart of fracture resistance mean values for both preparation designs.
- Figure 7, caption has been changed to Mode of Failure III: SEM image revealed the crack extension through the finish line (A: 70X, B: 250X).
- In the discussion, information regarding the load application has been added.

Any further responses from the reviewers can be found at the end of the article

Introduction

The best line of treatment to restore root canal treated teeth is one of the highly considered and debatable subjects¹. The liability to fracture of teeth increases after endodontic treatment. This can be attributed mainly to the loss of structure during preparation of access cavity. Accordingly, rebuilding the lost tooth structure requires a material with proper compensatory and high functional performance to support the overlying final restoration and sustain the falling occlusal loads². Ideally, the core build-up material should be consistent biologically and mechanically. It must have high sealing ability and durability³.

The breakthrough of adhesion in dentistry has enhanced the techniques of restoration of endodontically treated teeth. Adhesive composite resin and glass fiber posts have superseded the previously used non-bonded amalgam and metallic posts. Preservation of the remaining tooth structure without the need to create retentive means in the preparation is considered a great advantage, moreover, these tooth-colored materials support the esthetic demands⁴. Posts are not always used for a fact⁵. Earlier, using posts was considered to strengthen root canal treated teeth and prevent their fracture. However, this concept has changed, and they are mostly used when necessary to support the core¹.

The coverage of cusps of endodontically treated posterior teeth should not be undervalued to avoid the high risk of fracture⁶. These teeth are ought to be covered with crowns for their long-term survival⁷. The capability of these crowns to bear

load relies on the preparation of an appropriate design and the selection of a crown material with adequate fracture strength and thickness⁸.

Porcelain fused to metal crowns were commonly used to restore posterior teeth with the underlying metal substructure for the strength and overlying porcelain for the appearance. However, this type of restorations necessitated considerable amount of reduction and had limited esthetics. In a move towards improving the esthetics, porcelain fused to zirconia restorations were used. They enhanced the esthetics; however, they faced some adhesive failures⁹. The strength of junction between the substructure and overlying porcelain in multilayered ceramic restorations is of great concern due to their liability to chipping and failure¹⁰.

Nowadays, there is a shift towards monolithic restorations, especially in the posterior area. The well-known Lithium disilicate and the lately introduced monolithic zirconia ceramic materials together with the advancements in CAD/CAM technology offer strong reliable restorations with appropriate anatomy, improved cuspal contacts and acceptable esthetics^{9,10}.

In vital teeth, the anatomic occlusal preparation design is followed such that the occlusal surface is reduced uniformly, maintaining the cusps, fissures and normal inclined planes but at a reduced height. This aids in minimizing the risk of pulp injury. In contrast, in non-vital teeth, this design can be modified such that the occlusal surface is prepared in two planes (buccal and lingual planes)¹¹.

A flat prepared occlusal surface provides less quantitative and better qualitative stresses when compared to an anatomically prepared surface¹². Also, an anatomically prepared occlusal surface follows old preparation configurations for non-bonded crowns and more concern needs to be given to the functioning of bonded crowns, which can preserve tooth structure¹³.

The aim of our research was to assess the impact of a flat prepared occlusal surface (FOD) of endodontically treated molars on the fracture resistance and the distribution of stresses among the ceramic crown-molar structure when compared to a two planes prepared occlusal surface (TOD).

The hypothesis of our research was there would not be significant differences in both fracture resistance and developed stresses of the ceramic crown-molar structure of FOD when compared to TOD of endodontically treated molars (null hypothesis).

Methods

Ethical approval

This study was approved by the Research Ethics Committee of the Faculty of Dentistry, Cairo University. Approval number: 15636 (*Extended data*).

Extracted teeth were obtained from the outpatient clinic, Oral Surgery Department, Faculty of Dentistry, Cairo University.

Any researcher in the institute can obtain extracted teeth that meet the criteria of the research without requiring the researcher to contact the patients, since the patients give their consent for their extracted teeth to be used in future research when they are extracted.

Sample size calculation

Student’s t-test was performed to compare two groups (Group I: TOD; Group II: FOD), as per a previous study by Shahrabaf *et al.*¹³. The primary outcome of this study is the fracture resistance with an estimated mean value of 407.7±82.7 N for the control group (Group I) and 661.1±190 N for the test group (Group II) (effect size =1.7 with alpha 0.05 and power =0.8). Priori power showed that the required sample size should be above 14 (7 in each group) (calculated using G*power release 3.1.9.2). Accordingly, a total sample size of 20 (10 per group) was performed.

Sample fabrication

Teeth collection, endodontic treatment and coronal build up.

In total, 20 human mandibular molars free of caries, defects and cracks were chosen. The bucco-lingual dimension of crown as measured between the buccal and lingual maximum convexities was (10.5 ± 0.25 mm), while the mesio-distal dimension at cervix was (9 ± 0.25 mm) as measured using a digital caliber (Harbor Freight Tools, CA, USA). The teeth were kept in distilled water after ultrasonic scaling which was done to remove any remnants. In all teeth, the access cavity was prepared with a round diamond bur which was directed at center. The undercuts of dentin had been removed with long shafted round bur and finally finishing and flaring was carried out by safe ended diamond bur to allow straight-line access for instrumentation of the apical part of the canal¹⁴. The access cavity was triangular in case of single distal canal and trapezoidal in case of 2 distal canals, with the lesser base corresponding to the distal wall. Manual preparation and enlargement of root canals was performed until size # 25 (MANI, Japan)^{15,16}. Rotary root canal preparations were then performed with a series of ProTaper Ni-Ti rotary instruments (Dentsply Maillefer, Switzerland). The canals were prepared to F2 (D1 diameter 0.25 mm), while larger canals were shaped to F3 (D1 diameter 0.3 mm). The matched gutta percha points (Dentsply Maillefer, Switzerland) and resin based sealer (Adseal; META BIOMED Co, Korea) were used for obturation and the excess gutta percha was removed by a heated plugger¹⁷. Coronal cavities were then treated with 37% phosphoric acid Etch (Spident, USA) for 15 seconds, rinsed for 10 seconds and dried gently using a cotton pellet. A layer of light cure bonding agent (Adper Single Bond Plus Adhesive; 3M ESPE AG, Germany) was applied with gentle agitation and light cured for 10 seconds, then packable composite resin (3M Filtek Z250 XT Nano hybrid composite resin; 3M Deutschland GmbH, Germany) was incrementally added and light cured¹⁸.

Teeth mounting, grouping and preparation. A plastic ring (2.5 cm in diameter and 2 cm in length) was utilized to mount the teeth in epoxy resin (CMB, Egypt) and a custom made paralleling device (*Extended data*) was used to allow accurate

vertical centralization of the tooth in the ring. The mid-facial extent of the cemento-enamel junction was located 2 mm coronal to the resin top surface. The mounted teeth were randomly distributed into two equal groups as follows:

Group I (TOD): Prepared teeth with two planes occlusal surface.

Group II (FOD): Prepared teeth with flat occlusal surface.

A special milling machine (AF30 Nouvag, Switzerland) was used to prepare all the teeth by the same operator (Figure 1). The preparation parameters are detailed in Table 1, Figure 2.

Crown fabrication and cementation. A CAD/CAM system (CEREC AC; Sirona, Germany) was used for the fabrication of all crowns. Each prepared tooth was scanned using the CEREC Omnicam and design was carried out using CEREC Premium 4.4 software. With the purpose of standardization, the restoration parameters were fixed for all the restorations with the radial spacer set at 60 µm, minimal thickness occlusal 1500 µm and minimal thickness radial 1200 µm. The restoration’s position in 3D (buccolingually, mesiodistally and occlusocervically) was adjusted by rotation tools to follow the anatomy of the prepared tooth. The distance between central groove of restoration and the occlusal surface of tooth was standardized at 1.5 mm in all restorations. Milling of the crowns was done from Lithium disilicate blocks (IPS e.max CAD; Ivoclar

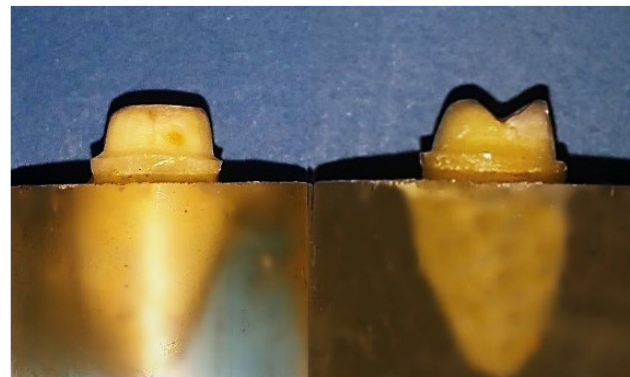


Figure 1. Flat occlusal preparation design (left) and two planes occlusal preparation design (right).

Table 1. Parameters of teeth preparation.

	Group I (TOD)	Group II (FOD)
Axial	1.5 mm	1.5 mm
Finish line	1 mm rounded shoulder	1 mm rounded shoulder
Taper	6°	6°
Occlusal surface	Two planes occlusal reduction (1.5 mm from occlusal center)	Flat occlusal reduction (1.5 mm from occlusal center)

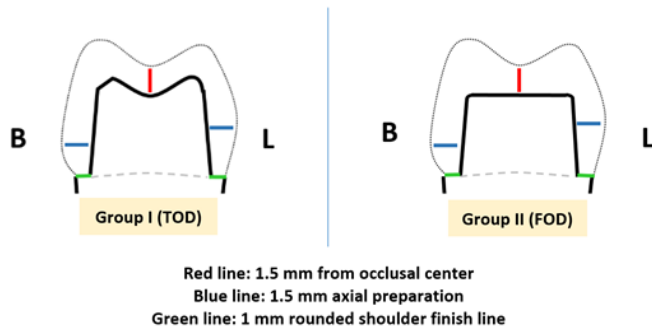


Figure 2. Diagram of teeth preparation.

Vivadent AG, Principality of Liechtenstein) in 4-axis milling machine CEREC MC XL. Finally, crowns were fully crystallized and glazed in Programat P510 furnace (Ivoclar Vivadent AG, Principality of Liechtenstein).

Surface treatment of the fitting surface of each crown was done as follows: Porcelain Etch (BISCO, USA) application for 20 seconds, followed by water rinsing and drying, then Silane (BISCO, USA) application for 60 seconds followed by air drying for 5 seconds. Self-adhesive resin cement (RelyX Unicem; 3M ESPE AG, Germany) was used for cementation.

Each crown was seated on its corresponding tooth and held with light pressure. The excess cement was cleared by an explorer after 2 seconds of tack-curing, then glycerine based gel (K-Y Jelly; Johnson & Johnson, USA) was applied at the margins of crown to prevent the oxygen inhibiting layer. A 5 kg load was applied parallel to the long axis of each tooth during cementation using a custom made loading device (*Extended data*)^{19,20}. The load was applied for 5 minutes to allow the cement to self-cure as recommended by the manufacturer. This was followed by final curing of axial and occlusal surfaces with light cure for 20 seconds.

Fracture resistance test

The test was carried out using a computer-controlled material testing machine (Instron, Model 3345; Instron industrial, USA). Each sample was tightened to the lower fixed compartment by screws. A compressive load was applied on the occlusal surface utilizing a metallic rod with round tip (5.8 mm diameter) attached to the upper movable compartment traveling at cross-head speed of 1mm/min with tin foil sheet in-between to achieve homogenous stress distribution and to minimize the transmission of local force peaks (Figure 3). The load to fracture was recorded in Newtons (N) using Instron Bluehill Lite Computer Software version 2 (Instron, USA). The fracture was manifested by an audible crack and confirmed by a sharp drop at load-deflection curve.

Statistical analysis

Data from the two groups were gathered, arranged and analyzed using SPSS (version 21; IBM, USA).

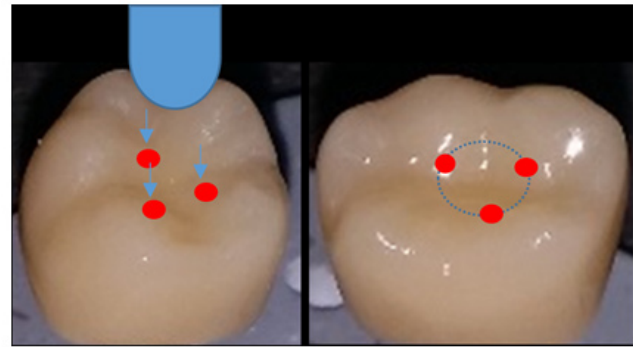


Figure 3. Three loading points on the inner inclines of the mesiobuccal, distobuccal and mesiolingual cusps.

Microscopic examination of fractured samples

High-performance Leica MZ6 Stereomicroscope (Meyer Instruments, USA) with 6.3:1 zoom was used to evaluate the fracture mode of the samples, indicating areas of interest for further examination under a scanning electron microscope (SEM; Model Quanta 250 Field Emission Gun; FEI Company, The Netherlands) attached with Energy Dispersive X-ray Analyses unit, with 30 KV accelerating voltage, 70X, 250X magnification and resolution of 1nm.

3D modeling and finite element analysis

3D designing of models

3D scanning. Two of the prepared samples (one for each group) and their corresponding crowns were scanned before cementation to produce models with real geometrical measures. 3D reconstruction from cone beam computed tomography (CBCT) data of the teeth scans was found had high linear, volumetric, and geometric accuracy²¹. A CBCT scanner (Next Generation iCAT scanner; ISI, USA) was used to obtain CBCT images in this research. After scanning, data were exported in DICOM format. **Mimics software** version 17 (Materialise, Belgium) was used^a for segmenting the scanned objects into separate elements. A definitive threshold level was set to most clearly show each element of the scanned samples with minimal interference from the surrounding structures, and once segmentation was completed the software automatically calculated the element's volume. The resulting STL files were opened separately on **Meshmixer software** version 3.3.15 (Autodesk Inc., USA) for the improvement of mesh quality and its refinement (Figure 4). Now we have the components of crown-tooth structure as separate elements of known volumes that can be assembled together in STL file format of improved quality.

Reverse engineering and assembly. Reverse engineering was performed by **NX software** version 10 (Siemens PLM, Texas, USA)^b. The refined STL files were imported into the software

^a Free alternative software that could be used for this analysis is **ITK-SNAP**.

^b Free alternative software that could be used for this analysis is **FreeCAD**.

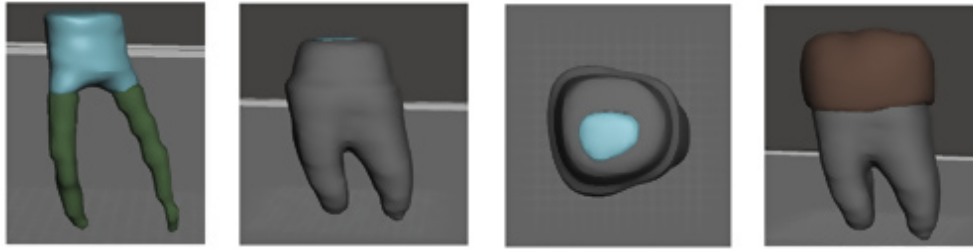


Figure 4. STL files: Core (blue), gutta percha (green), tooth structure (gray) and crown (brown).

and converted into solid parts. Then, cortical bone and cancellous bone were drawn as solid parts in cylindrical shapes followed by their superimposition together for Boolean subtraction. Finally, all the produced solid parts were superimposed together for Boolean subtraction and periodontal ligaments were modeled with 0.2 mm thickness to allow a fully defined simulation methodology. The generated 3D CAD geometry of all parts were then assembled using Solidworks software 2017 (Dassault Systèmes SolidWorks Corporation, France)^c to produce the 3D CAD models, one for each group (Figure 5).

Finite element analysis. Finite element analysis (FEA) was carried out by ANSYS R16.2 software (ANSYS, Canonsburg, USA)^d using the 3D CAD models. It included 3 phases:

Pre-processing phase. The type of element was defined as Solid 10 node 187. All the materials' properties were set as isotropic, homogenous and linear elastic. The modulus of elasticity and Poisson's ratio of each material were gathered and were uploaded to the software (Table 2). A perfect rigid bonding with no-slip condition between all the elements was simulated. Each model was divided into small parts called elements connected together at points called nodes forming a mesh structure. Parabolic tetrahedral solid elements were used to form a fine solid mesh. The overall number of elements and nodes was recorded (Table 3).

Processing phase. Following the creation of the 3D meshes, a zero displacement boundary condition was set at all nodes of the cortical bone that were confined in X, Y, and Z directions. Posterior fixed restorations ought to have the capability to tolerate a 500 N occlusal load^{22,23}. Accordingly a load of 500 N was applied by a ball model of diameter 5.8 mm equal to that of metallic rod ball of the universal testing machine used for fracture resistance test in this study. The occlusal surface of the crown was loaded at the inner inclines of the mesiobuccal, distobuccal and mesiolingual cusps.

Post-processing phase. The output of the processing phase was displayed as graphical output and numeric output.

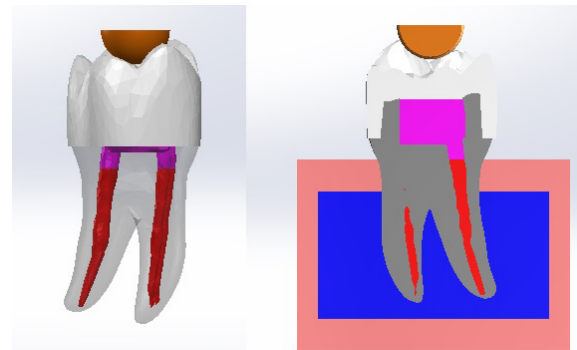


Figure 5. 3D CAD model (left). The model embedded in bone (right).

Table 2. Physical properties of each component of the model.

Material	Modulus of elasticity (GPa)	Poisson's ratio
Dentin	18.6 ²⁴	0.31 ²⁴
Periodontal ligaments	0.0000689 ²⁵	0.45 ²⁵
Cancellous bone	1.37 ²⁴	0.30 ²⁴
Cortical bone	13.7 ²⁴	0.30 ²⁴
IPS e.max CAD crown	96 ²⁶	0.23 ²⁶
Filtek Z250 composite	14 ²⁷	0.31 ²⁷
Gutta percha	0.14 ²⁵	0.45 ²⁵
Rely X Unicem cement	4.9 ²⁶	0.30 ²⁶

Results

Fracture resistance

Fracture resistance results as a function of preparation design are summarized in Table 4.

It was found that the fracture resistance mean \pm SD value recorded for Group I was 2962.6 \pm 524.2 N, with minimum

^c Free alternative software that could be used for this analysis is FreeCAD.

^d Free alternative software that could be used for this analysis is OpenFoam V6.

Table 3. The overall number of elements and nodes.

	Element	Node
Group I model	493788	706944
Group II model	439230	630975

Table 4. Descriptive statistics of fracture resistance results as a function of preparation design.

Variables		Group I	Group II
Mean		2962.6	3107.2
95% Confidence Interval for Mean	Lower Bound	2587.6	2674.5
	Upper Bound	3337.7	3539.9
Std. Deviation		524.2	604.94
Minimum		2206.01	2253.5
Maximum		4014.7	4153.4

value of 2206.01 N and maximum value of 4014.7 N. For Group II, the mean \pm SD value recorded was 3107.2 \pm 604.94 N, with minimum value of 2253.5 N and maximum value of 4153.4 N.

The difference between the mean fracture resistance between the two groups was non-statistically significant as indicated by Student's t-test ($p=0.57$) (Figure 6).

Fractographic analysis of fractured samples

The behavior of the samples upon fracture differed (Table 5). Five different modes were observed and categorized as restorable or non-restorable according to their relation to the cemento-enamel junction (CEJ). A fracture that ends before CEJ, implying that even after the occurrence of fracture, the tooth can be saved is a restorable one, while fractures that are non-restorable extend beyond CEJ and extraction of the tooth is expected²⁸. The extensions of the cracks were verified by SEM (Figure 7). The results are tabulated in Table 6 and classified as restorable and non-restorable.

3D FEA

In each model, FEA revealed stresses at every node. These results were presented as stress contours overlaid on the model. The numeric data of stress, deformation and safety factor in the models were calculated and transformed into color graphics.

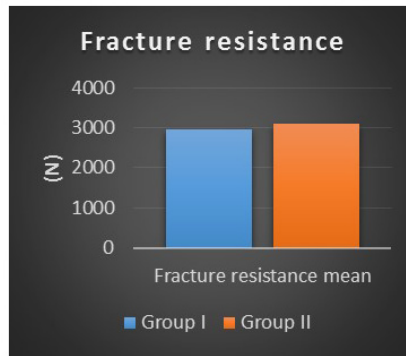







Figure 6. Column chart of fracture resistance mean values for both preparation designs.

Table 5. Classification of the modes of failure. Restorable remaining tooth structure: modes I, II and IV; non-restorable remaining tooth structure: modes III and V.

Mode of failure	I	II	III	IV	V
Descriptive form	Crack limited to occlusal half.	Crack extended to cervical half.	Crack extended through and beyond cervical finish line.	Fractured segment of coronal part of tooth.	Fractured segment of coronal part and root of the tooth.
Descriptive Stereomicroscopic photo					

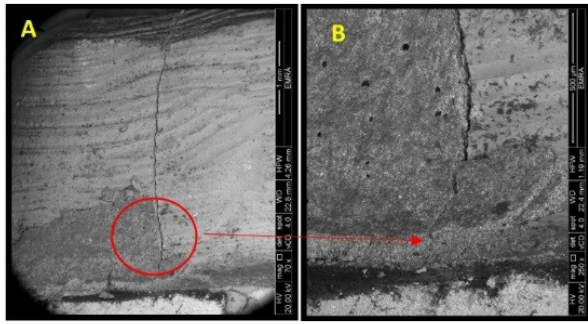


Figure 7. Mode of Failure III: SEM image revealed the crack extension through the finish line (A: 70X, B: 250X).

Table 6. Number of samples of Groups I and II relative to mode of failure, with restorability reported.

Behavior		Group I (N)	Group II (N)
Mode of failure	I	0	3
	II	2	2
	III	3	3
	IV	0	1
	V	5	1
Restorability	Restorable	2	6
	Non-restorable	8	4

Equivalent (von-Mises) stress. The “von-Mises Stress” at different areas were calculated and compared (Table 7). The stress distribution values were generally found to be low.

Total deformation. The maximum value of total deformation denoted by the red color in Group I was 0.0158 mm. It was concentrated on the mesial half of the coronal portion of model (Crown, dentin and core) and the root (neck of the tooth) at the mesial surface and the mesial half of the lingual surface (Figure 8). While in Group II the maximum value of total deformation was 0.01409 mm. It was located on middle and the lingual half of coronal portion of model and the lingual neck of the tooth with mesiolingual and distolingual line angles (Figure 9). When comparing both groups, Group II yielded less total deformation values than Group I.

Safety factor. Both groups had high safety factor where the maximum equivalent stress was less than the stress limit. In Group I: the lowest safety factor recorded was 1.5575 was

Table 7. The von-Mises stress values for each model. Red dot marks the higher value.

Area		Group I (Two planes) MPa	Group II (Flat) MPa	
Tooth (Dentin)	Occlusal Surface	Mesiobuccal cusp	4.10	6.36 •
		Mesiolingual cusp	5.15	6.01 •
		Mesial marginal ridge	4.57	8.66 •
		Distal marginal ridge	4.63 •	3.15
		Distobuccal cusp	4.27 •	3.96
		Distolingual cusp	4.30 •	3.03
		Distal cusp	3.92 •	2.32
	Axial walls	Mid buccal	0.26	1.86 •
		Mid distal	1.76	2.64 •
		Mid lingual	3.07	3.37 •
		Mid mesial	3.46 •	2.40
	Finish line	Mid buccal	4.66 •	3.64
		Mid distal	1.86	2.72 •
		Mid lingual	5.66 •	4.36
		Mid mesial	6.24 •	3.17
	Root (neck of the tooth)	Buccal	3.00	4.14 •
		Lingual	6.23	6.62 •
		Distal	2.36	2.57 •
		Mesial	5.87 •	4.76
		Furcation	5.37 •	5.24
	Crown center		22.60	36.50 •
Core center		22.60	36.50 •	
Gutta percha	Mesiobuccal	0.14640 •	0.13680	
	Mesiolingual	0.00736 •	0.00735	
	Distal	0.00653 •	0.00625	

at the mesial neck of the tooth denoted by the orange color (Figure 10). In Group II: the lowest safety factor recorded was 1.1571 was at the lingual neck of the tooth denoted by the orange color (Figure 11).

Correlation between fracture behavior and stress distribution

The stress distribution among different layers of the model differed as well as areas of total deformation. This was

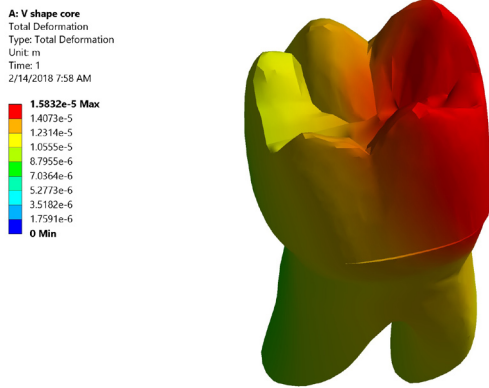


Figure 8. Color graphics showing total deformation of Group I.

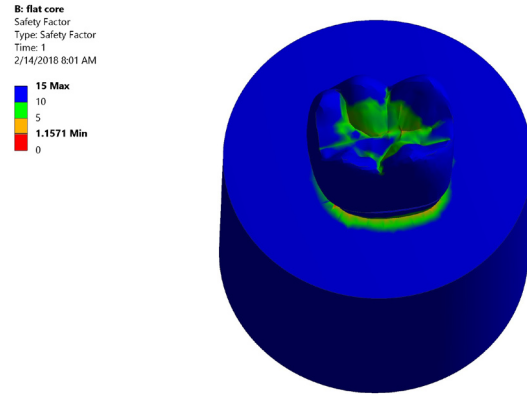


Figure 11. Color graphics showing safety factor of Group II.

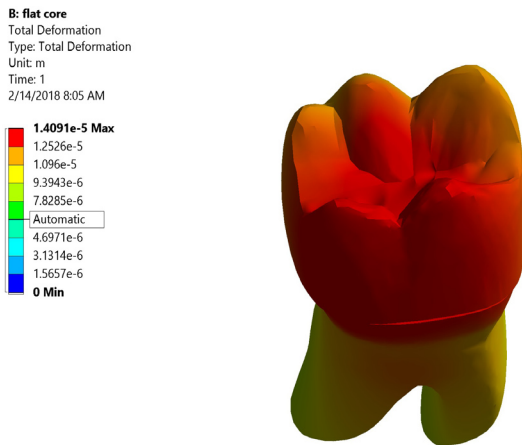


Figure 9. Color graphics showing total deformation of Group II.

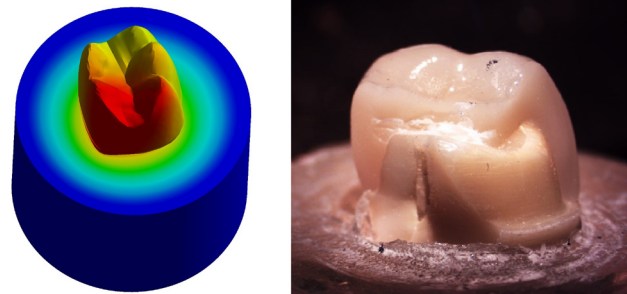


Figure 12. Correlation between total deformation (left) and fracture behavior (right) of Group I.

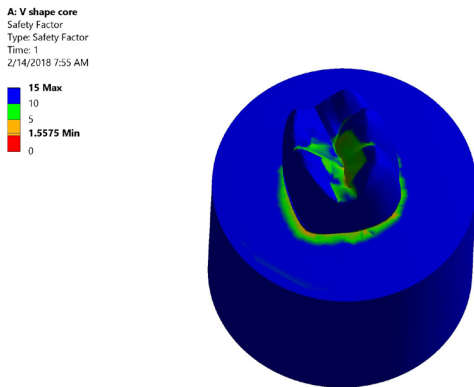


Figure 10. Color graphics showing safety factor of Group I.

correlated with the fracture behavior of samples of both groups as follows:

Group I (Figure 12). The stress values were high at mid-mesial and mid-lingual axial walls, mid-mesial and mid-lingual finish line, and root’s mesial surface. Maximum total deformation was

concentrated in the mesial half of the coronal portion of model (crown, dentin and core) and the neck of the tooth at the mesial surface and mesial half of the lingual surface.

Upon observation of fracture behavior of Group I samples of fracture resistance, the failure in most of the samples occurred at the mesial half of the crown-tooth structure including the finish line and the root (neck of the tooth).

Group II (Figure 13). The centers of the crown and the underlying core material generated high stress values upon load application. Also, at mesiobuccal cusp, mesiolingual cusp, mesial marginal ridge, and root’s lingual surface stresses were high. Maximum total deformation was located at the middle and the lingual half of coronal portion of model (crown, dentin, and core) and the lingual neck of the tooth with mesiolingual and distolingual line angles.

Upon observation of fracture behavior of Group II samples of fracture resistance, the failure in more than half of the samples occurred at the lingual half of the crown-tooth structure, not including the finish line and the root (neck of the tooth).

Discussion

Previous research has generally given minimal concern to the impact of the preparation configuration on the ability of the

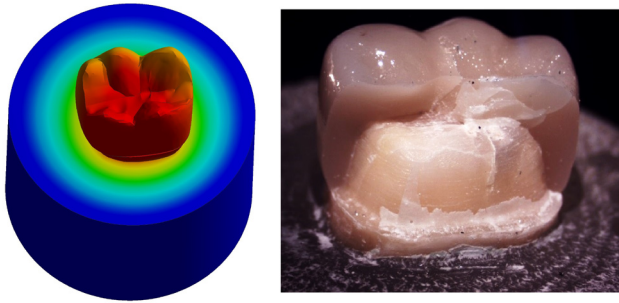


Figure 13. Correlation between total deformation (left) and fracture behavior (right) of Group II.

crown-tooth structure to resist fracture and distribute stresses, and instead has mainly targeted the crown material itself¹³. Thus, the focus of this study was to specifically address the impact of the prepared occlusal surface configuration comparing two planes occlusal preparation (TOD) versus flat occlusal preparation (FOD) of endodontically treated molars.

Mandibular molars were chosen due to their high incidence for developing caries, their subjection to strong occlusal loads and greater susceptibility to fracture²⁹. Single-cone obturation technique was followed to exclude the inordinate cutting of dentin needed to ease the entry of the endodontic plugger in vertical warm condensation technique and the wedge-acting stresses of the spreaders during lateral cold condensation technique³⁰. Lithium disilicate ceramic was chosen for crown fabrication. This ceramic material features appropriate mechanical and esthetic qualities for making monolithic restorations, allowing conservative tooth preparation and simplicity of production³¹. Self-adhesive resin cement was selected as it was revealed that the use of adhesive cement raised the fracture resistance by almost 26% when utilized with lithium disilicate glass ceramic as compared to non-adhesive cement³².

Periodontal ligament (PDL) was not simulated. Upon the application of a static load, no difference was anticipated in the resistance of teeth to fracture whether their roots were covered with a PDL simulating material or not. Moreover, the thickness of the silicone PDL simulating material used to cover the roots was found to be thicker than the normal PDL thickness. Also, with the difficulty to unify the thickness of this material, there was no control on the movability of the investigated teeth and more drawbacks were expected³³.

Static load fracture test was employed in an occluso-axial direction, which is viewed as the most well-known strategy for testing the integrity of a structure¹³. Molars tolerate well most of the forces of mastication that fall perpendicularly and generally, the anterior teeth protect them from eccentric loads via anterolateral guidance³⁴. Accordingly, the load was directed vertically at the center of the crown at three points on the inner

inclines of the mesiobuccal, distobuccal and mesiolingual cusps³⁵.

Checking the areas of stress is crucial as stress, regardless of if it is beneath the point of failure, is considered as a noteworthy reason for propagation of a crack and henceforth failure. 3D FEA has been used to investigate stress bearing and handling capabilities of various restoration materials and shapes in a safe and time saving method²².

FEA simulated the test of fracture resistance performed in this investigation to demonstrate the generated points of stress subsequent to load application. A good-bond interlayer condition was assumed between the distinctive layers in the model.

Our results failed to reject the null hypothesis that FOD of endodontically treated molars would not differ in both fracture resistance and the generated stresses of the ceramic crown-molar structure when compared to TOD.

The results of fracture resistance test displayed no significant difference statistically between both tested groups with an average > 2900 N, which surpasses the average and maximum biting force reported in the mouth (100-600 N)³⁶.

Also, these results exceeded those of other studies. According to Nordahl *et al.*³⁷ the mean fracture resistance of e.max lithium disilicate crowns of posterior molars of thickness 1.5 mm was 1,431 N while according to Yu *et al.*²⁸ it was 1827.3 N. This can be attributed to the exposure of crowns in both studies to artificial aging before loading until fracture. The exposure of the crowns to aging was stated in various investigations to diminish the resultant fracture loads significantly^{37,38}.

Regardless of the close and clinically satisfactory fracture resistance results of both investigated designs, the failure mode varied. It was found that 20% of Group I (TOD) had undergone restorable fractures, while in Group II (FOD) this was 60%. This denotes that FOD showed better stress distribution, thus more favorable fracture behavior.

The 3D FEA data recorded in this study showed that both preparation designs yielded low von-Mises stresses within the factor of safety of the model. In both groups, high stresses and deformation were induced in the lingual surface of molars. This was justified by the weakening effect of the hard tissue loss on the mandibular molars, which might predispose the lingual wall to fracture due to unfavorable distribution of stresses during chewing³⁹. This was confirmed by Oyar *et al.*⁸ who found high stress values were generated in the lingual dentin regions in both anatomic and non-anatomic occlusal preparation designs.

Upon observation of fracture behavior of samples of fracture resistance test and correlating it with the results of the FEA, the following were concluded: Group I (TOD) developed lower stresses in the center of the crown and the core, and the stresses

increased upon moving apically towards the root with greater influence on the mesial half of the model. This explained the failure pattern in most of the samples that occurred at the mesial portion of the crown-molar structure including the finish line and the root (neck of the tooth). While Group II (FOD) developed higher stresses in the center of the crown and the core, and the stresses decreased upon moving apically towards the root with greater influence on the lingual half of the model. This explained the failure pattern in more than half of the samples which occurred at the lingual portion of the crown-molar structure without the inclusion of finish line and root (neck of the tooth).

Our results differed than other studies regarding the stress distribution pattern. According to, Oyar *et al.*⁴⁰ the anatomically prepared design yielded better stress distribution in dentin while the non-anatomic design yielded better distribution and less amount of stresses in the porcelain structure. Their study was carried out on mandibular second premolars restored by metal-ceramic crowns.

While Shahrbafe *et al.*¹² concluded that the flat occlusal configuration presented lower stresses than the anatomic configuration in all layers and a more favorable distribution. Their study was carried out on maxillary first premolars with variable amount of occlusal reduction, such that 2 mm even reduction for the anatomic design and 1.2 mm reduction from the central groove for the flat one.

Oyar *et al.*⁸ found that different designs did not result in differences in the generated stresses in tooth (dentin, pulp) and bone. However, the anatomic design crown had the highest value of stresses and this was attributed to the crown thickness, which was less than that of the non-anatomic. Their study was conducted on mandibular second premolar teeth.

In the current researchers' opinion, the comparable results obtained among the two tested groups in the present study could be attributed to multiple factors: First, unifying the ceramic thickness at the fissure depth to 1.5 mm thickness, which is the most critical area for failure; second, selecting lithium disilicate monolithic crowns as the material of choice with its well-known high mechanical properties in terms of flexural strength and good bonding potential to tooth and composite resin; third, conducting adhesive bonding protocol using adhesive composite resin cement, which has a positive impact on overall fracture resistance of the ceramic-molar structure.

The fracture resistance test used in this research is considered a limitation, as it does not precisely mimic the load application inside patient's mouth, which is a cyclic loading process. Also, another limitation is the consideration of having a perfect bond between the crown and tooth in FEA method.

Conclusions

1. Flat and two planes occlusal preparation designs of endodontically treated molars had fracture resistance values surpassing the average and maximum biting force reported in the mouth.
2. Flat and two planes occlusal preparation designs of endodontically treated molars showed stress values within the safety factor when subjecting the models to the average biting force.
3. Flat occlusal preparation design showed more favorable mode of failure as compared to two planes occlusal preparation design based on the fractographic and 3D finite element analyses.
4. Flat occlusal preparation design can be used safely with endodontically treated molars.

Clinical significance

The occlusal reduction of endodontically treated molars can influence the functioning of the crown-molar structure. The occlusal surface preparation design has to strengthen the prepared tooth to sustain the forces being subjected to and, upon failure, it favors a restorable mode.

This study revealed that restorable fractures were higher in flat occlusal preparation design than two planes occlusal preparation design. Therefore, clinicians may choose the flat occlusal preparation design to improve the clinical performance and longevity of the restored endodontically treated molars.

Recommendations

1. Clinical studies comparing the behavior of the two tested designs.
2. Designing the same research using other contemporary metal free crown materials (hybrid materials, polycrystalline materials), which may yield different outcomes.

Data availability

Underlying data

Open Science Framework: Fracture Resistance and 3D Finite Element Analysis of Machined Ceramic Crowns Bonded to Endodontically Treated Molars with Two Planes versus Flat Occlusal Preparation Designs. "In-Vitro Study", <https://doi.org/10.17605/OSF.IO/WMRU441>.

This project contains the following underlying data:

- 3D FEA results (.xlsx files)
- Fracture resistance data (.xlsx file)
- SEM raw data (.doc file)
- FEA output (.mechdat files)
- Solidworks software 2017 files, 3D models (.x_t files)
- Instron Lab fracture resistance output report

Extended data

Open Science Framework: Fracture Resistance and 3D Finite Element Analysis of Machined Ceramic Crowns Bonded to Endodontically Treated Molars with Two Planes versus Flat Occlusal Preparation Designs. “*In-Vitro Study*”, <https://doi.org/10.17605/OSF.IO/WMRU4>¹.

This project contains the following extended data:

- Ethical approval document

- Custom made paralleling device

- Custom made loading device

Acknowledgements

We would like to express our thanks and appreciation to Mohamed Gamal Askar (MSc, Research Assistant, Mechanical Department, Faculty of Engineering, Helwan University) for his efforts, excellent work and beneficial remarks regarding 3D FEA.

References

- Faria ACL, Rodrigues RCS, de Almeida Antunes RP, et al.: **Endodontically treated teeth: characteristics and considerations to restore them.** *J Prosthodont Res.* 2011; **55**(2): 69–74.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Sharma A, Das S, Thomas MS, et al.: **Evaluation of fracture resistance of endodontically treated premolars restored by alkasite cement compared to various core build-up materials.** *Saudi Endod J.* 2019; **9**: 205–9.
[Reference Source](#)
- Reddy SN, Harika K, Manjula S, et al.: **Evaluation of occlusal fracture resistance of three different core materials using the Nayyar core technique.** *J Int Soc Prev Community Dent.* 2016; **6**(1): 40–43.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Mannocci F, Cowie J: **Restoration of endodontically treated teeth.** *Br Dent J.* 2014; **216**(6): 341–346.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Field C, Stone S, Whitworth J, et al.: **Core Build-Ups and Post Placement.** In: Wassell R., Nohl F., Steele J., Walls A. (eds) *Extra-Coronal Restorations*. BDJ Clinician's Guides. Springer, Cham, 2019.
[Publisher Full Text](#)
- Aquilino SA, Caplan DJ: **Relationship between crown placement and the survival of endodontically treated teeth.** *J Prosthet Dent.* 2002; **87**(3): 256–263.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Nagasiri R, Chitmongkolsuk S: **Long-term survival of endodontically treated molars without crown coverage: a retrospective cohort study.** *J Prosthet Dent.* 2005; **93**(2): 164–170.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Oyar P, Ulusoy M, Eskitaşçıoğlu G: **Finite element analysis of stress distribution in ceramic crowns fabricated with different tooth preparation designs.** *J Prosthet Dent.* 2014; **112**(4): 871–877.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Vallée J, Noble WH, Gupta S, et al.: **Selection Guidelines for All-Ceramic Restorations.** *Decisions in Dentistry.* 2017; **3**(3): 24–28.
[Reference Source](#)
- Warreth A, Elkareimi Y: **All-ceramic restorations: A review of the literature.** *Saudi Dent J.* 2020; **32**(8): 365–372.
[Publisher Full Text](#)
- Tylman SD: **Theory and Practice of Crown and Fixed Partial Prosthodontics (Bridge).** 6th Ed. St. Louis: C.V. Mosby Co.; 1970.
- Shahrbaf S, van Noort R, Mirzakouchaki B, et al.: **Effect of the crown design and interface lute parameters on the stress-state of a machined crown-tooth system: a finite element analysis.** *Dent Mater.* 2013; **29**(8): e123–31.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Shahrbaf S, van Noort R, Mirzakouchaki B, et al.: **Fracture strength of machined ceramic crowns as a function of tooth preparation design and the elastic modulus of the cement.** *Dent Mater.* 2014; **30**(2): 234–241.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Adams N, Tomson PL: **Access cavity preparation.** *Br Dent J.* 2014; **216**(6): 333–339.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Nazir SM, Abdallah AM, Mokhles NA: **Detection of Crack Formation Following Coronal Flaring With Three Different Instruments Using Two Evaluation Methods (in Vitro Study).** *Alexandria Dent J.* 2017; **42**(2): 135–140.
[Publisher Full Text](#)
- Nagaratna PJ, Shashikiran ND, Subbareddy VV: **In vitro comparison of NiTi rotary instruments and stainless steel hand instruments in root canal preparations of primary and permanent molar.** *J Indian Soc Pedod Prev Dent.* 2006; **24**(4): 186–91.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Capar ID, Ertas H, Ok E, et al.: **Comparison of single cone obturation performance of different novel nickel-titanium rotary systems.** *Acta Odontol Scand.* 2014; **72**(7): 537–542.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Ali SAM, Manoharan PS, Shekhawat KS, et al.: **Influence of Full Veneer Restoration on Fracture Resistance of Three Different Core Materials: An In Vitro Study.** *J Clin Diagn Res.* 2015; **9**(9): ZC12–ZC15.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Mobilio N, Fasiol A, Mollica F, et al.: **Effect of Different Luting Agents on the Retention of Lithium Disilicate Ceramic Crowns.** *Materials (Basel).* 2015; **8**(4): 1604–1611.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Abou-Madina M, Abdelaziz K: **Influence of Different Cementation Materials and Thermocycling on the Fracture Resistance of IPS e.max Press Posterior Crowns.** *Internet J Dent Sci.* 2008; **6**(2): 1–7.
[Reference Source](#)
- Sang YH, Hu HC, Lu SH, et al.: **Accuracy Assessment of Three-dimensional Surface Reconstructions of In vivo Teeth from Cone-beam Computed Tomography.** *Chin Med J (Engl).* 2016; **129**(12): 1464–70.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Alsadon O, Patrick D, Johnson A, et al.: **Fracture resistance of zirconia-composite veneered crowns in comparison with zirconia-porcelain crowns.** *Dent Mater J.* 2017; **36**(3): 289–295.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Saridag S, Ozyesil AG, Pekkan G: **Fracture strength and bending of all-ceramic and fiber-reinforced composites in inlay-retained fixed partial dentures.** *J Dent Sci.* 2012; **7**(2): 159–164.
[Publisher Full Text](#)
- D'souza KM, Aras MA: **Three-dimensional finite element analysis of the stress distribution pattern in a mandibular first molar tooth restored with five different restorative materials.** *J Indian Prosthodont Soc.* 2017; **17**(1): 53–60.
[PubMed Abstract](#) | [Free Full Text](#)
- Yikilgan I, Bala O: **How can stress be controlled in endodontically treated teeth? A 3D finite element analysis.** *ScientificWorldJournal.* 2013; **2013**: 426134.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- El-Anwar MI, Al-Azrag KE, Ghazy MH, et al.: **Influence of implant-abutment angulations and crown material on stress distribution on central incisor: A 3D FEA.** *Brazilian J Oral Sci.* 2015; **14**(4): 323–329.
[Publisher Full Text](#)
- Huang SH, Lin LS, Rudney J, et al.: **A novel dentin bond strength measurement technique using a composite disk in diametral compression.** *Acta Biomater.* 2012; **8**(4): 1597–1602.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Forster A, Sáry T, Braunitzer G, et al.: **In vitro fracture resistance of endodontically treated premolar teeth restored with a direct layered fiber-reinforced composite post and core.** *J Adhes Sci Technol.* 2017; **31**(13): 1454–1466.
[Publisher Full Text](#)
- Garlapati TG, Krithikadatta J, Natanasabapathy V: **Fracture resistance of endodontically treated teeth restored with short fiber composite used as a core material-An in vitro study.** *J Prosthodont Res.* 2017; **61**(4): 464–470.
[PubMed Abstract](#) | [Publisher Full Text](#)
- Celikten B, Uzuntas CF, Gulsahi K: **Resistance to fracture of dental roots obturated with different materials.** *Biomed Res Int.* 2015; **2015**: 591031.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
- Yu T, Wang F, Liu Y, et al.: **Fracture behaviors of monolithic lithium disilicate ceramic crowns with different thicknesses.** *RSC Adv.* 2017; **7**(41): 25542–25548.
[Publisher Full Text](#)

32. Lim MJ, Lee KW: **Effect of adhesive luting on the fracture resistance of zirconia compared to that of composite resin and lithium disilicate glass ceramic.** *Restor Dent Endod.* 2017; **42**(1): 1–8.
[PubMed Abstract](#) | [Publisher Full Text](#) | [Free Full Text](#)
33. Chang CY, Kuo JS, Lin YS, *et al.*: **Fracture resistance and failure modes of CEREC endo-crowns and conventional post and core-supported CEREC crowns.** *J Dent Sci.* 2009; **4**(3): 110–117.
[Publisher Full Text](#)
34. Peters OA: **The Guidebook to Molar Endodontics.** Springer, Berlin, Heidelberg; 2017.
[Publisher Full Text](#)
35. Ha SR, Kim SH, Lee JB, *et al.*: **Effects of coping designs on stress distributions in zirconia crowns: Finite element analysis.** *Ceram Int.* 2016; **42**(4): 4932–4940.
[Publisher Full Text](#)
36. Sadighpour L, Geramipناه F, Raeesi B: **In Vitro Mechanical Tests for Modern Dental Ceramics.** *J Dent.* 2006; **3**(3): 143–152.
[Reference Source](#)
37. Nordahl N, Vult von Steyern P, Larsson C: **Fracture strength of ceramic monolithic crown systems of different thickness.** *J Oral Sci.* 2015; **57**(3): 255–261.
[PubMed Abstract](#) | [Publisher Full Text](#)
38. Skouridou N, Pollington S, Rosentritt M, *et al.*: **Fracture strength of minimally prepared all-ceramic CEREC crowns after simulating 5 years of service.** *Dent Mater.* 2013; **29**(6): e70–e77.
[PubMed Abstract](#) | [Publisher Full Text](#)
39. Dejak B, Młotkowski A, Romanowicz M: **Finite element analysis of stresses in molars during clenching and mastication.** *J Prosthet Dent.* 2003; **90**(6): 591–597.
[PubMed Abstract](#) | [Publisher Full Text](#)
40. Oyar P, Ulusoy M, Eskitascioglu G: **Finite element analysis of stress distribution of 2 different tooth preparation designs in porcelain-fused-to-metal crowns.** *Int J Prosthodont.* 2006; **19**(1): 85–91.
[PubMed Abstract](#)
41. Nabil O: **Fracture Resistance and 3D Finite Element Analysis of Machined Ceramic Crowns Bonded to Endodontically Treated Molars with Two Planes versus Flat Occlusal Preparation Designs.** *"In-Vitro Study."* 2019.
<http://www.doi.org/10.17605/OSF.IO/WMRU4>

Open Peer Review

Current Peer Review Status: ? ✓ ✓

Version 2

Reviewer Report 28 November 2022

<https://doi.org/10.5256/f1000research.56912.r156322>

© 2022 **Aboushahba M.** This is an open access peer review report distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.



Mostafa Aboushahba 

Fixed Prosthodontics Faculty of Oral and Dental Medicine, Future University in Egypt, Cairo, Egypt

I am very pleased with the authors' work and the scientific content of the article. It is of great clinical value and gives preliminary answers to a long going question as to whether to prepare a flat occlusal surface or anatomical occ surface.

For the discussion:

- Can you add when to post or not to post; justify why didn't you use a post in your methodology.
- Can you also add that the flat occlusal surface had better results yet non-significant, that may be due to the structural durability of the material since the flat occlusal surface provides more restoration thickness than the anatomical.

Recommendations:

- Test cyclic loading as it resembles the oral environment more.
- Test the retention as I expect due to the reduction of occlusion-gingival height of the prep it might reduce the resistance and retention.

Is the work clearly and accurately presented and does it cite the current literature?

Yes

Is the study design appropriate and is the work technically sound?

Yes

Are sufficient details of methods and analysis provided to allow replication by others?

Yes

If applicable, is the statistical analysis and its interpretation appropriate?

Yes

Are all the source data underlying the results available to ensure full reproducibility?

Yes

Are the conclusions drawn adequately supported by the results?

Yes

Competing Interests: No competing interests were disclosed.

Reviewer Expertise: Associate Professor Fixed Prosthodontics Future University in Egypt FUE

I confirm that I have read this submission and believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.

Version 1

Reviewer Report 09 March 2020

<https://doi.org/10.5256/f1000research.21329.r50923>

© 2020 Salah T. This is an open access peer review report distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.



Tarek Salah 

Fixed Prosthodontics Department, Faculty Of Dentistry, Ain Shams University, Cairo, Egypt

This is a very interesting research and of high clinical interest and I really appreciate the work of the authors. It is definitely publishable material after some revisions.

Materials and Methods:

- Why didn't you consider doing mechanical cyclic loading before the fracture resistance testing? I think it would have been more clinically significant.
- More details are needed concerning teeth dimensions.
- Access cavity design and dimensions should be also described as all these details are important in behavior of the teeth during fracture resistance testing. And also, please mention the master apical file size.
- To which level were the teeth mounted in the epoxy resin?
- There should be more elaboration on specifics of teeth preparation designs, especially occlusal designs. A diagram would be highly beneficial. The photograph is not that descriptive.

- What were the details of crowns dimensions and standardization during designing?

Testing:

- Indicate the points of load application during fracture resistance testing?

Statistical analysis:

- There are no details. What type of tests or analysis did you perform?

FEA:

- The model designing step needs more description especially the role of CBCT and the correlation with the 3D scanning.

Fig 3:

- Just mention Bar chart or column chart.

Fig 4:

- Indicate which mode of failure that figure is.

Discussion:

- Paragraphs 2 to 6 are not necessary. Go straight for the interpretation after paragraph 1.
- Reference 33 has no journal.

Is the work clearly and accurately presented and does it cite the current literature?

Yes

Is the study design appropriate and is the work technically sound?

Yes

Are sufficient details of methods and analysis provided to allow replication by others?

Yes

If applicable, is the statistical analysis and its interpretation appropriate?

Partly

Are all the source data underlying the results available to ensure full reproducibility?

Yes

Are the conclusions drawn adequately supported by the results?

Yes

Competing Interests: No competing interests were disclosed.

Reviewer Expertise: Prosthodontics, Esthetic dentistry, Digital dentistry, Implantology

I confirm that I have read this submission and believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard.

Author Response 01 Jun 2021

Omnia Nabil, Cairo University, Cairo, Egypt

Thank you very much for your careful reading, useful comments and accepting our article. Your effort and time are much appreciated.

A second version of the article has been submitted, which has the following changes made in response:

Materials and Methods:

- *Why didn't you consider doing mechanical cyclic loading before the fracture resistance testing? I think it would have been more clinically significant.*

In our study we focused on the impact of the occlusal preparation design only on the fracture resistance and stress distribution among a ceramic crown-molar structure. A static load fracture test was preferred to avoid the addition of any variables that can be caused by fatigue testing.

- *More details concerning teeth dimensions.*

The bucco-lingual dimension of crown as measured between the buccal and lingual maximum convexities was (10.5 ± 0.25 mm), while the mesio-distal dimension at cervix was (9 ± 0.25 mm) as measured using a digital caliber (Harbor Freight Tools, CA, USA).

- *Access cavity design and dimensions should be also described as all these details are important in behavior of the teeth during fracture resistance testing. And also, please mention the master apical file size.*

In all teeth, the access cavity was prepared with a round diamond bur which was directed at center. The undercuts of dentin had been removed with long shafted round bur and finally finishing and flaring was carried out by safe ended diamond bur to allow straight-line access for instrumentation of the apical part of the canal. The access cavity was triangular in case of single distal canal and trapezoidal in case of 2 distal canals, with the lesser base corresponding to the distal wall.

Rotary root canal preparations were then performed with a series of ProTaper Ni-Ti rotary instruments (Dentsply Maillefer, Switzerland). The canals were prepared to F2 (D1 diameter 0.25 mm), while larger canals were shaped to F3 (D1 diameter 0.3 mm).

- *To which level were the teeth mounted in the epoxy resin?*

The mid-facial extent of the cemento-enamel junction was located 2 mm coronal to the resin top surface.

- *There should be more elaboration on specifics of teeth preparation designs, especially occlusal designs. A diagram would be highly beneficial. The photograph is not that descriptive.*

A diagram has been added.

- *What were the details of crowns dimensions and standardization during designing?*

With the purpose of standardization, the restoration parameters were fixed for all the restorations with the radial spacer set at 60 μm , minimal thickness occlusal 1500 μm and minimal thickness radial 1200 μm . The restoration's position in 3D (buccolingually, mesiodistally and occlusocervically) was adjusted by rotation tools to follow the anatomy of the prepared tooth. The distance between central groove of restoration and the occlusal surface of tooth was standardized at 1.5 mm in all restorations.

Testing:

- *Indicate the points of load application during fracture resistance testing?*

3 Loading points: 2 points on the inner inclines of the mesiobuccal and distobuccal cusps and 1 point on the inner incline of the mesiolingual cusp.

A figure has been added

Statistical analysis:

- *There are no details. What type of tests or analysis did you perform?*

Data analysis was performed using IBM SPSS, version 21 (SPSS, Chicago, IL, USA). Student t-test was used to detect significance between two groups which was set at 5% for all statistical analyses and confidence interval at 95% such that P values ≤ 0.05 were considered to be statistically significant

FEA:

- *The model designing step needs more description especially the role of CBCT and the correlation with the 3D scanning.*

CBCT 3D scanning of two of the prepared samples (one for each group) and their corresponding crowns was done before cementation.

After scanning, data were exported in DICOM format. Mimics software version 17 (Materialise, Belgium) was used for segmenting the scanned objects into separate elements.

A definitive threshold level was set to show each element of the scanned samples most clearly with minimal interference from the surrounding structures, and once segmentation was completed the software automatically calculated the element's volume.

The resulting STL files were opened separately on Meshmixer software version 3.3.15 (Autodesk Inc., USA) for the improvement of mesh quality and its refinement. Now we have the components of crown-tooth structure as separate elements of known volumes that can be assembled together in STL file format of improved quality.

A figure has been added to show components of STL files as separate elements

Fig 3: Just mention Bar chart or column chart.

- Column chart.

Fig 4: Indicate which mode of failure that figure is.

- Mode of failure III

Discussion:

- *Paragraphs 2 to 6 are not necessary. Go straight for the interpretation after paragraph 1.*

We think that justifying the important steps in the methodology would be beneficial for other readers to justify our choices.

References: *Reference 33 has no journal.*

It is a reference to our article account on Open Science Framework to access all the extended data of our work.

Competing Interests: No competing interests were disclosed.

Reviewer Report 05 December 2019

<https://doi.org/10.5256/f1000research.21329.r57384>

© 2019 Pekkan G. This is an open access peer review report distributed under the terms of the [Creative Commons Attribution License](#), which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.



Gürel Pekkan

Department of Prosthodontics, Faculty of Dentistry, Tekirdag Namik Kemal University, Tekirdağ, Turkey

The manuscript is well organised and well written. However, it needs more literature review in the introduction as well as discussion of some points that are listed below:

1. In the introduction, give more literature review about the core build-up materials and techniques.
2. Give more info about the prosthetic materials and the reasons for the choice of different restorative materials in endodontically treated teeth.
3. Please discuss the ball-contact points and localization in the test configuration that would affect the force distribution in the tooth.

Is the work clearly and accurately presented and does it cite the current literature?

Yes

Is the study design appropriate and is the work technically sound?

Yes

Are sufficient details of methods and analysis provided to allow replication by others?

Yes

If applicable, is the statistical analysis and its interpretation appropriate?

Yes

Are all the source data underlying the results available to ensure full reproducibility?

Yes

Are the conclusions drawn adequately supported by the results?

Yes

Competing Interests: No competing interests were disclosed.

I confirm that I have read this submission and believe that I have an appropriate level of expertise to confirm that it is of an acceptable scientific standard, however I have significant reservations, as outlined above.

Author Response 01 Jun 2021

Omnia Nabil, Cairo University, Cairo, Egypt

Thank you very much for your careful reading and useful comments.
Your effort and time are much appreciated.

A second version of the article has been submitted, which has the following changes made in response:

1. In the introduction, more literature review has been given about the core build-up materials and techniques. (Paragraphs 1 and 2)
2. In the introduction, more info about the prosthetic materials and the reasons for the choice of different restorative materials in endodontically treated teeth has been added. (Paragraphs 3, 4 and 5)
3. In the discussion, the ball-contact points and direction of load have been addressed. (Paragraph 4)

Competing Interests: No competing interests were disclosed.

The benefits of publishing with F1000Research:

- Your article is published within days, with no editorial bias
- You can publish traditional articles, null/negative results, case reports, data notes and more
- The peer review process is transparent and collaborative
- Your article is indexed in PubMed after passing peer review
- Dedicated customer support at every stage

For pre-submission enquiries, contact research@f1000.com

F1000Research