

Fig 1C

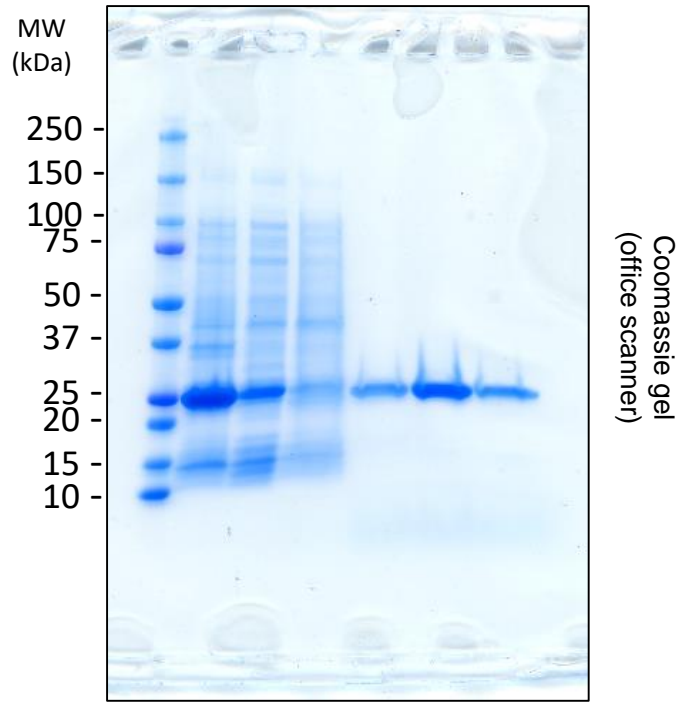


Fig 4A






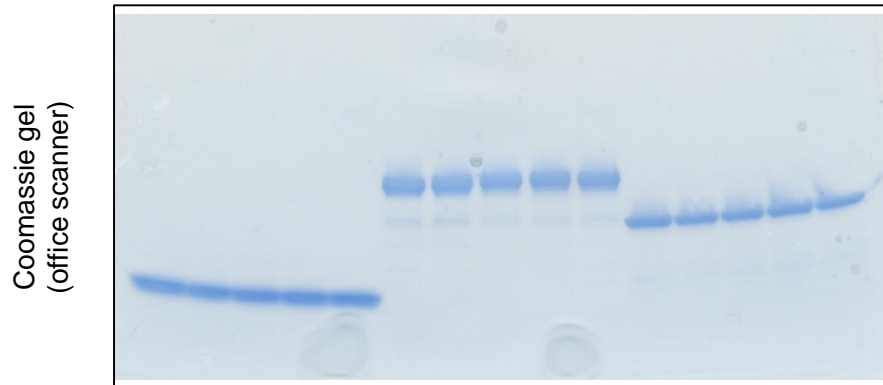


Fig 4B


S13 Fig panel C

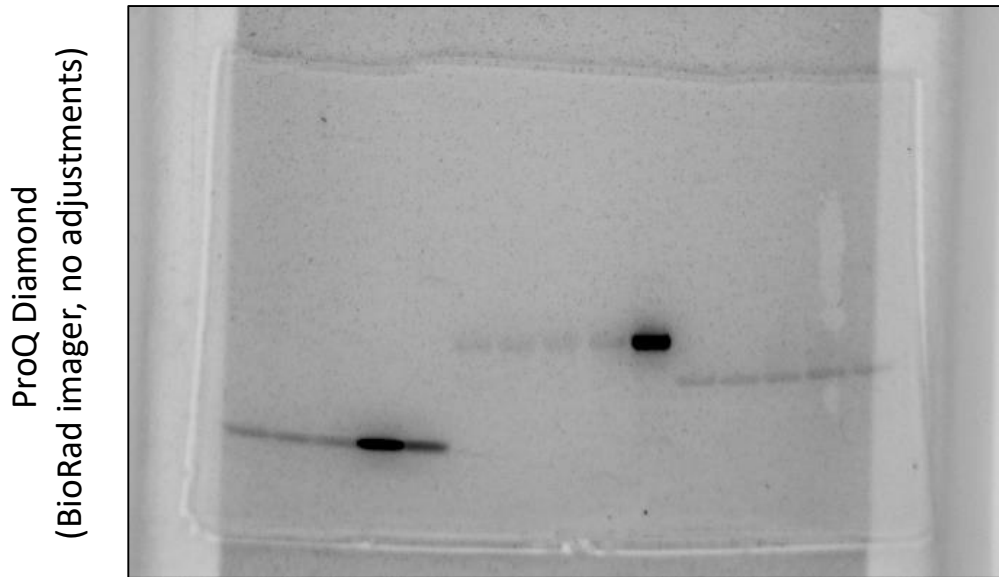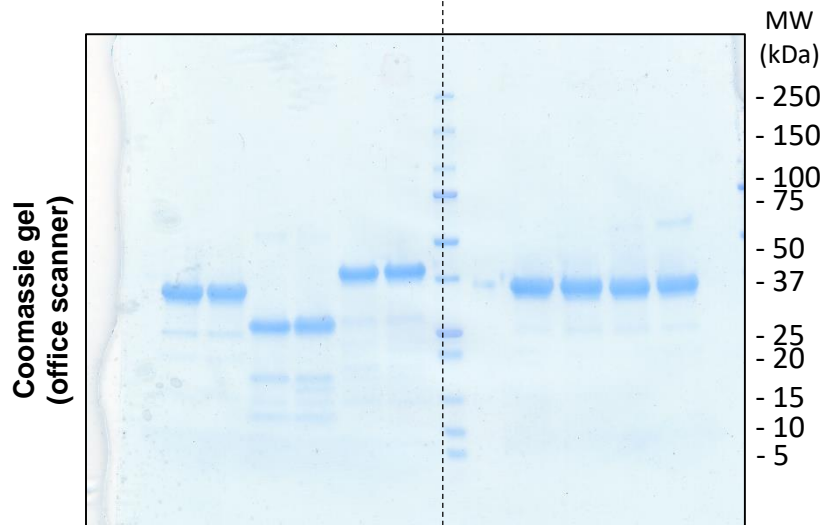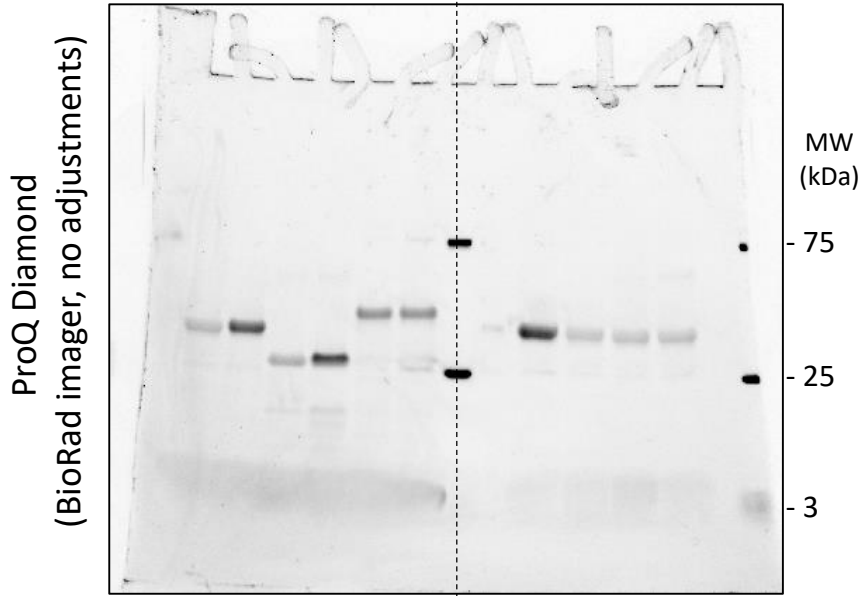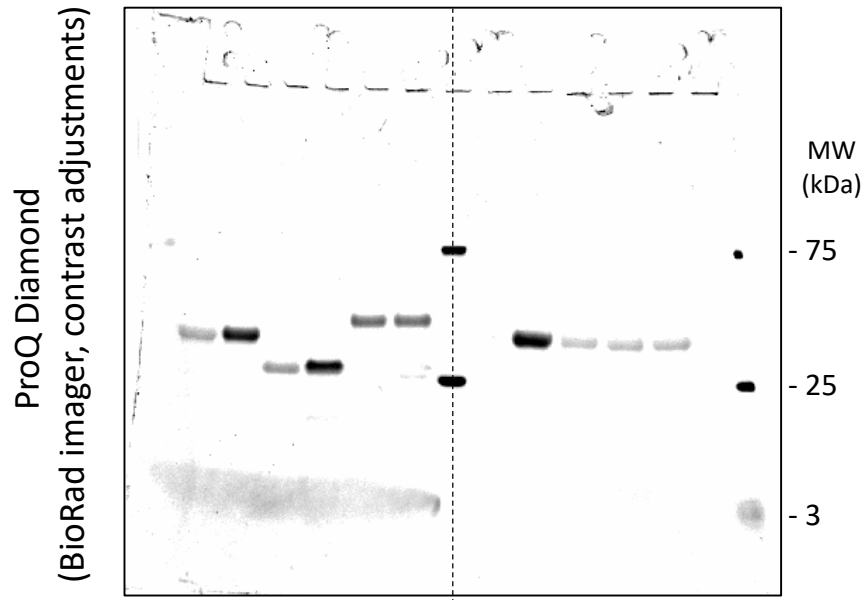


S1 Fig

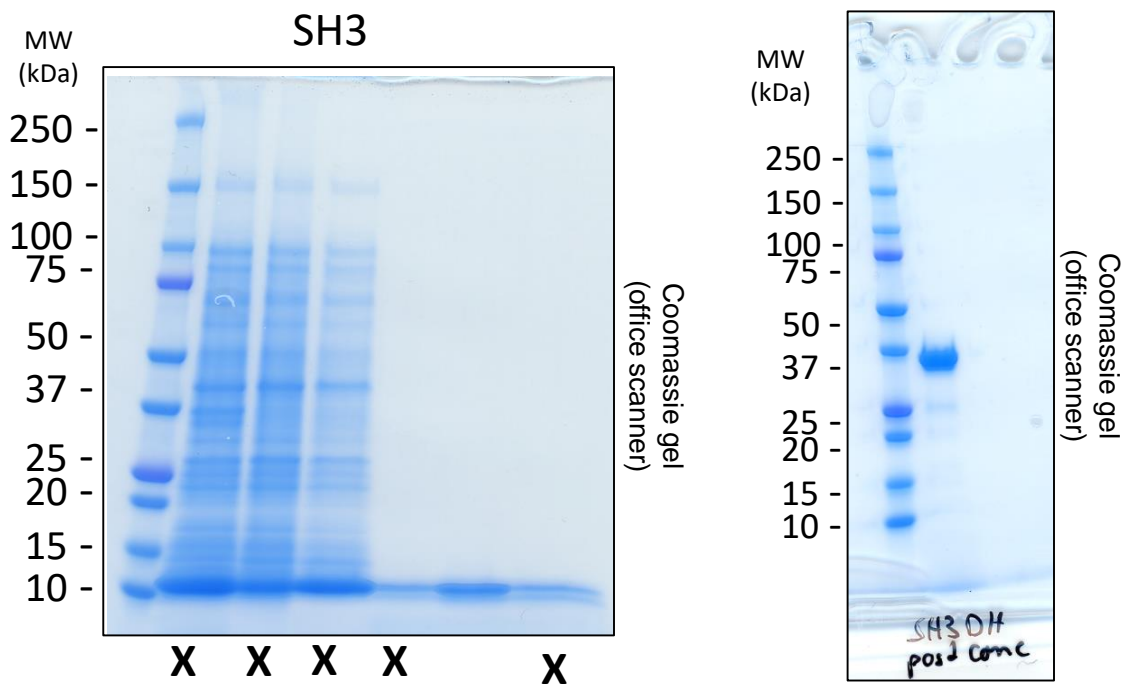

S4 Fig

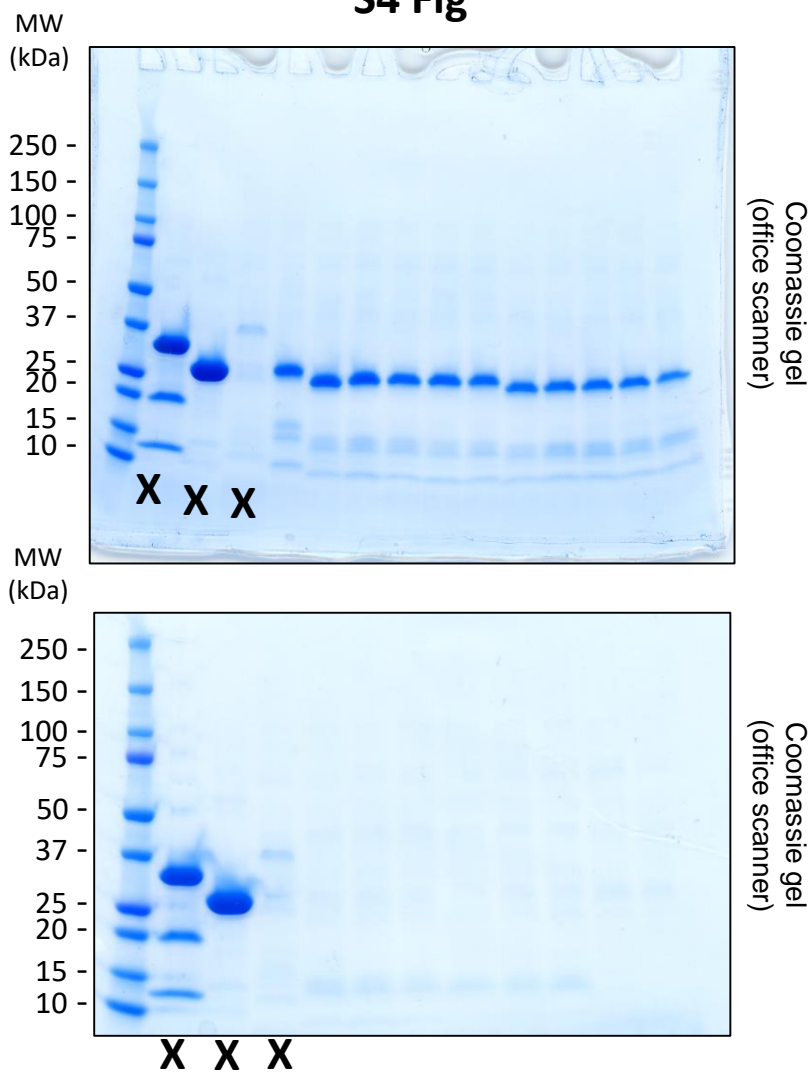


S5 Fig

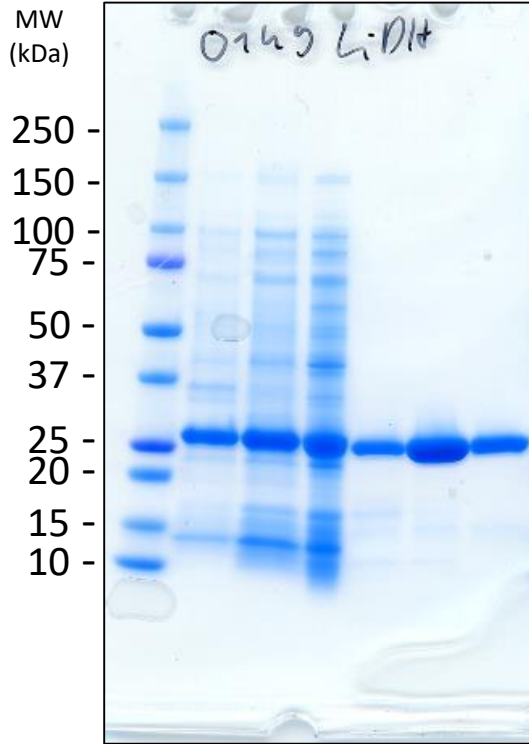


Coomassie gel
(office scanner)

S7 Fig

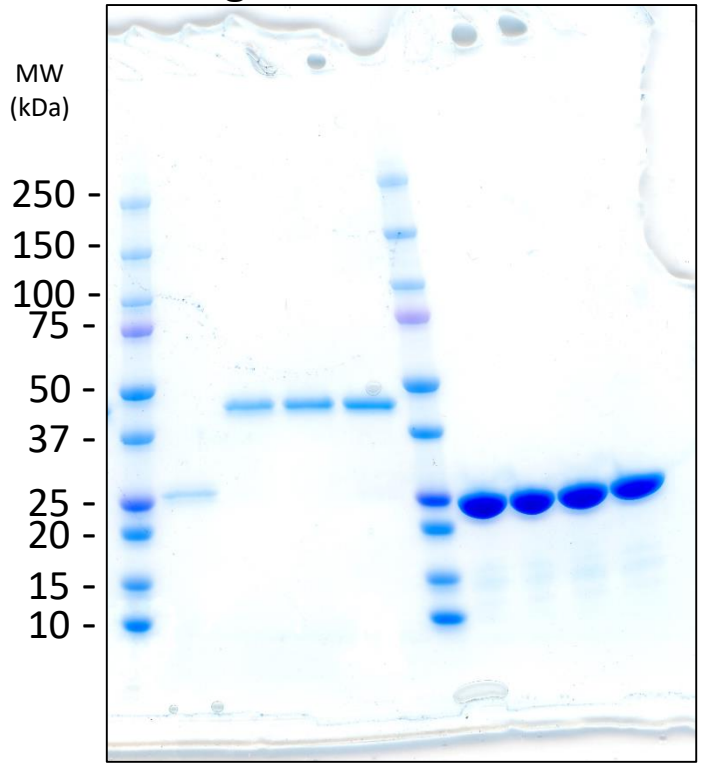


Coomassie gel
(office scanner)

S10 Fig, panel B

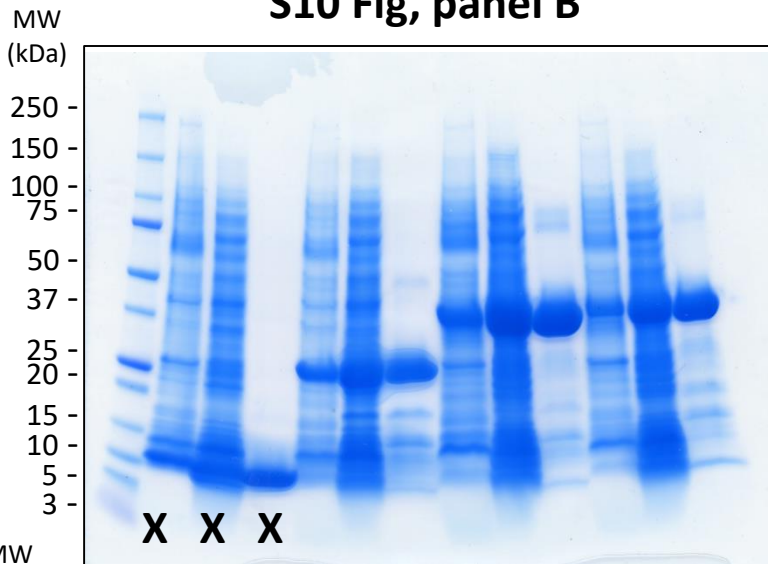


Coomassie gel
(office scanner)

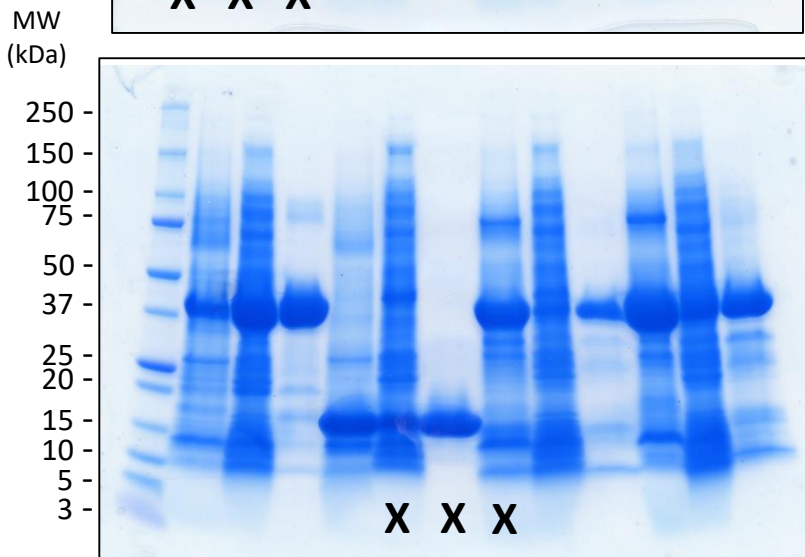


Coomassie gel
(office scanner)

S14 Fig, panel A


WB (BioRad imager)

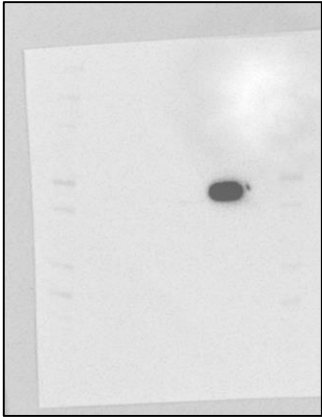


WB (BioRad imager)

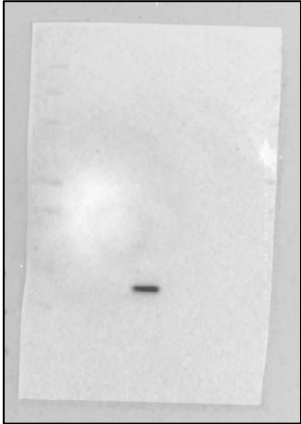

MW (kDa) Ponceau (BioRad imager)

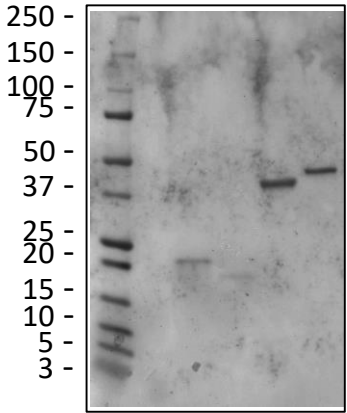


MW (kDa) Ponceau (BioRad imager)

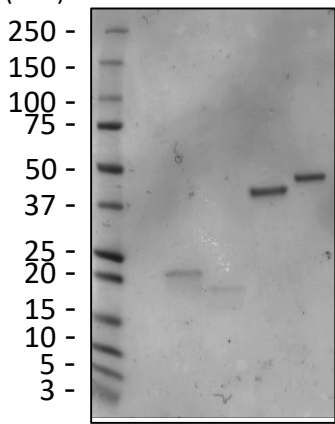

S14 Fig, panel B

WB (BioRad imager)

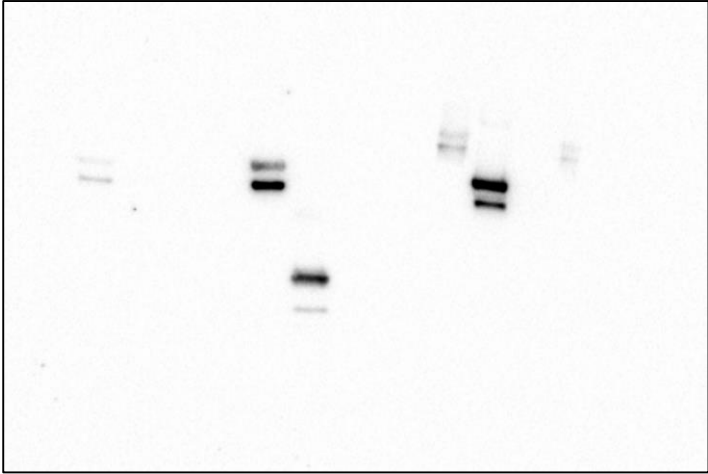

Ponceau (office scanner)

