

Supplementary

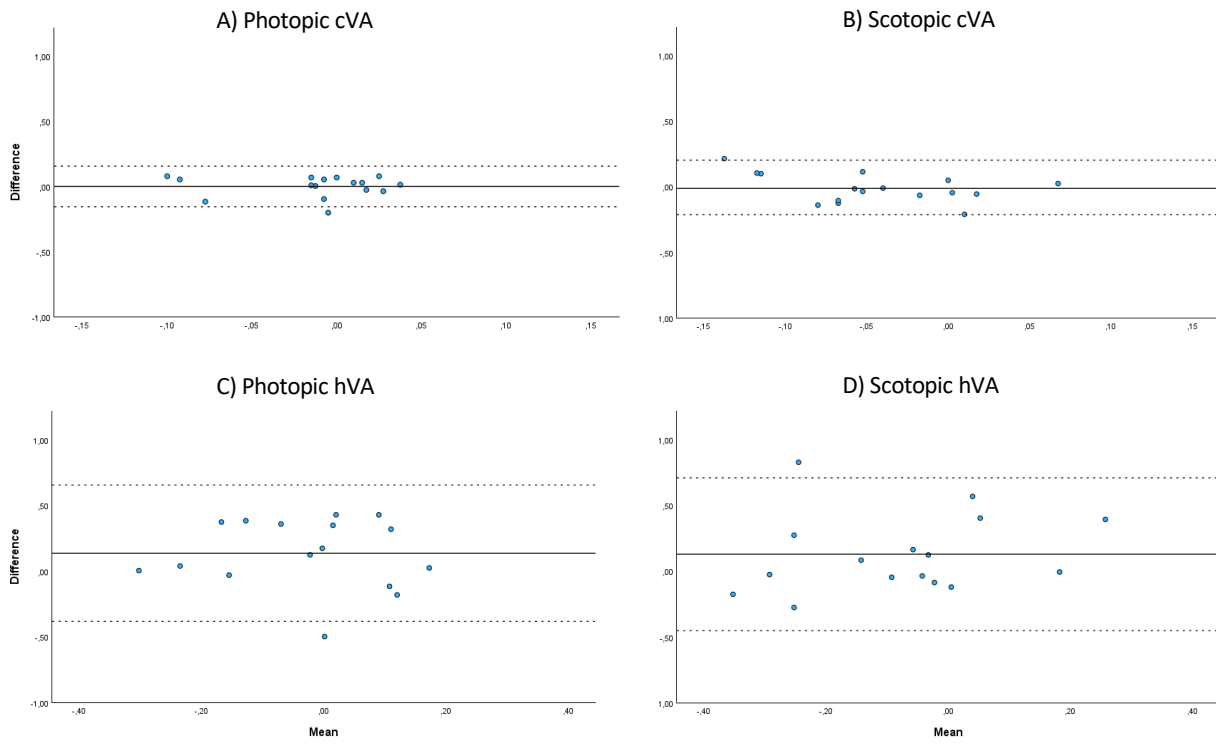


Figure 1 supplementary. Bland-Altman analysis for conventional (cVA) and hyperacuity (hVA) visual acuity values [logMAR] for the measurement between 2 days.