


Supplementary Figure S18. TRADITIOM LSC barcode statistics at single cell level and quality checks

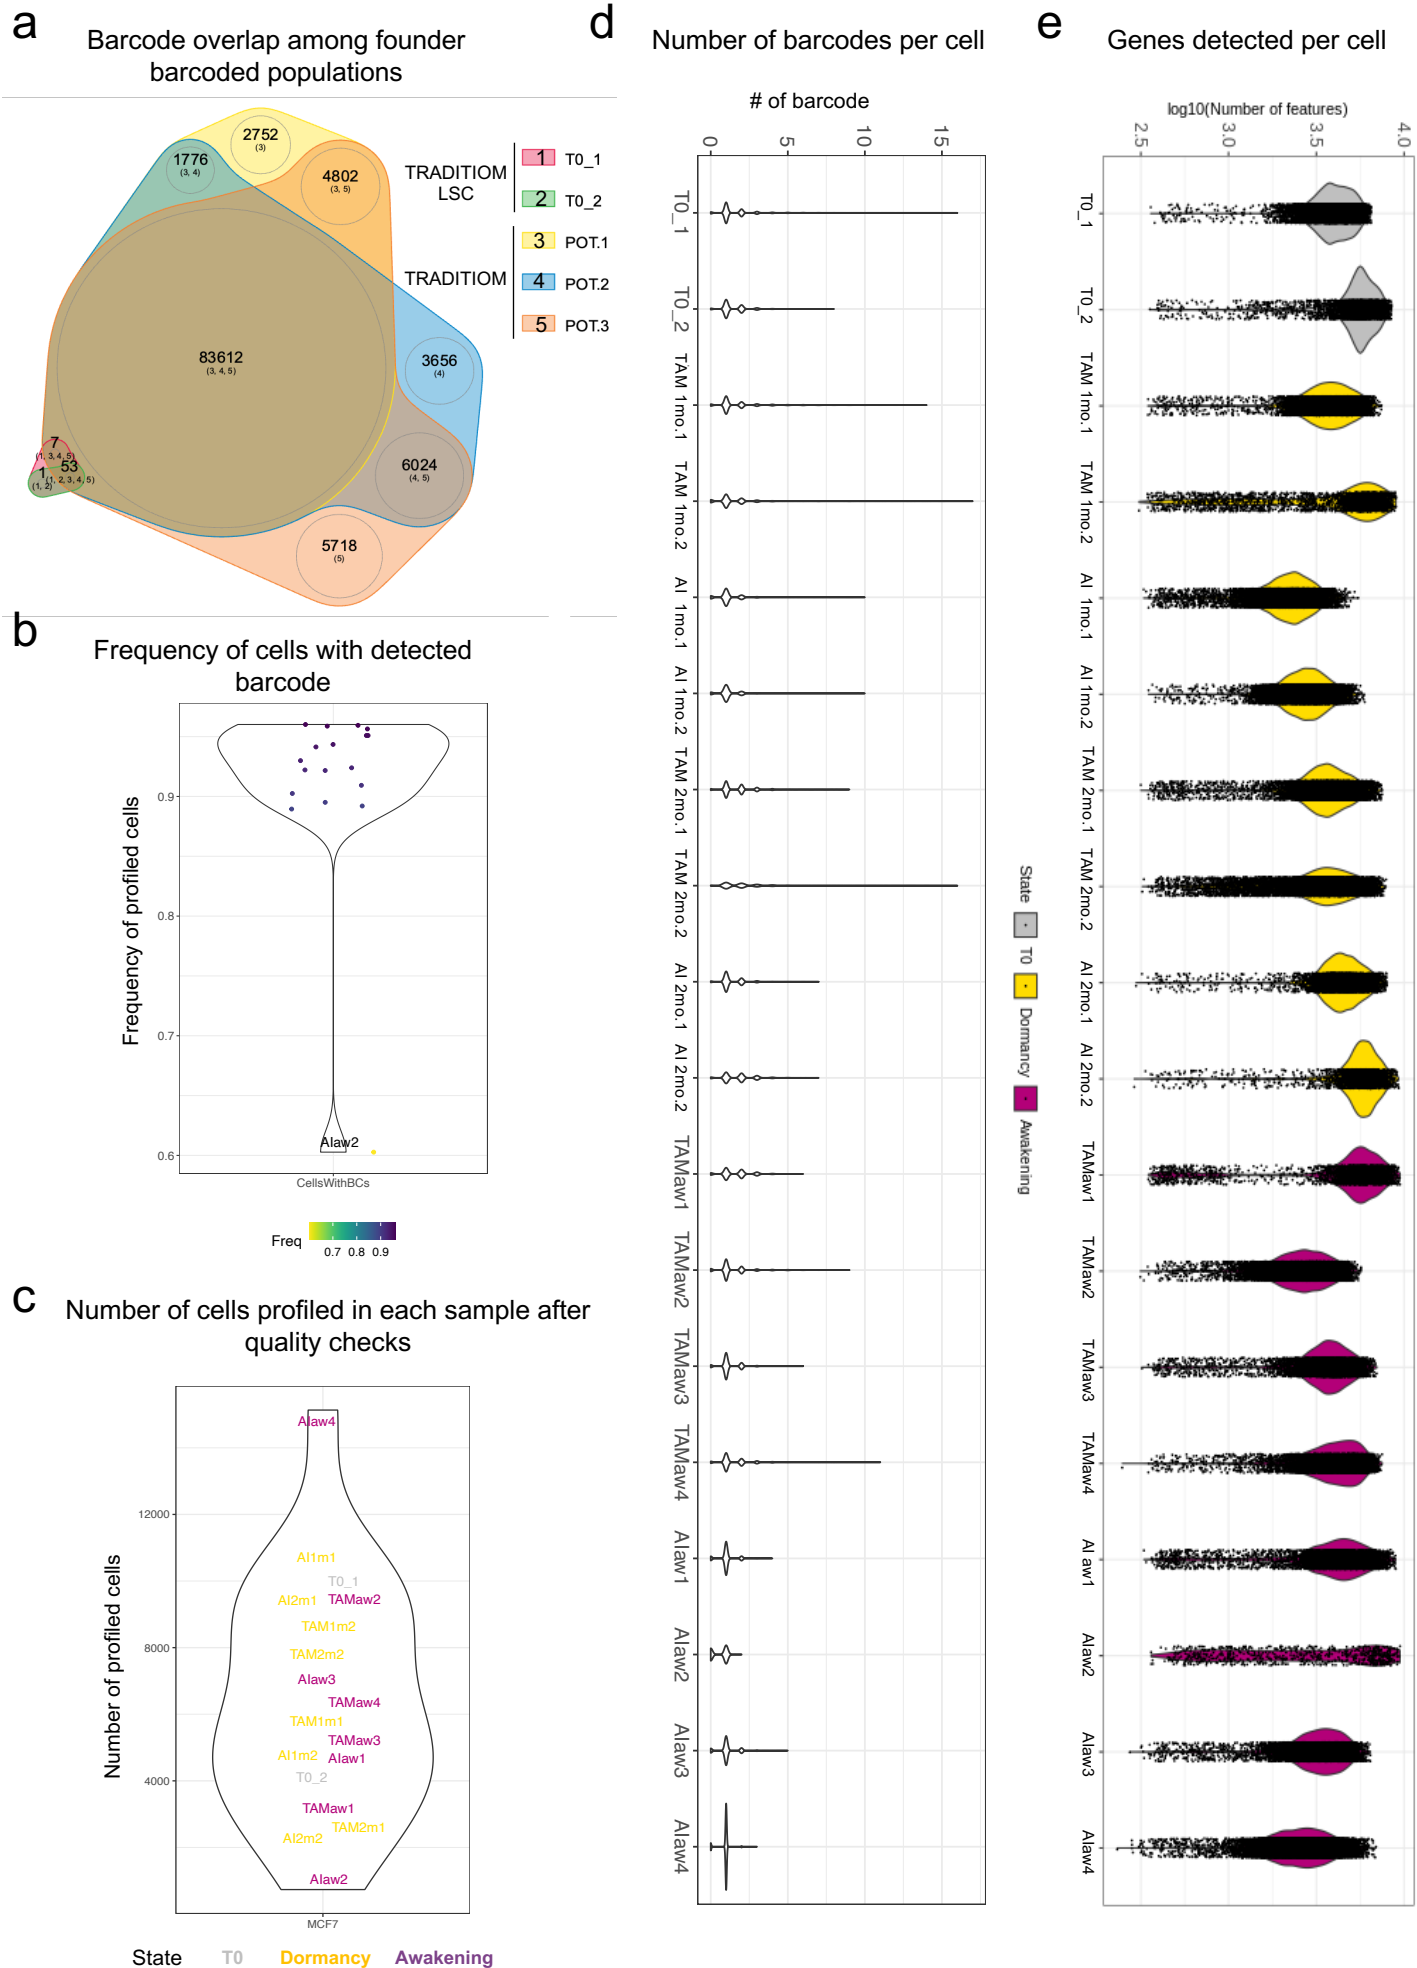

Supplementary Figure S18. TRADITIOM LSC barcode statistics at single cell level and quality checks. **a)** Barcode overlap between MCF7 TRADITIOM POTs (pre-treatment) (100K barcodes) and MCF7 TRADITIOM Live Single Cell (LSC) T0 (Time zero) samples (100 barcodes subsampled from TRADITIOM POT). **b)** Frequency of cells with detected barcodes. Barcodes could be detected in more than 85% of the cells for all the samples other than Alaw2 (-E2 arm, awakening sample 2). **c)** Number of cells profiled in each MCF7 TRADITIOM LSC (live single cell) sample after quality checks. **d)** Number of detected barcodes per cell along TRADITIOM LSC for MCF7 cells. **e)** Number of genes detected per cell in MCF7 TRADITIOM dataset.