



Bias of publication

Figura S1 – Funnel plot for discontinuation due to adverse events

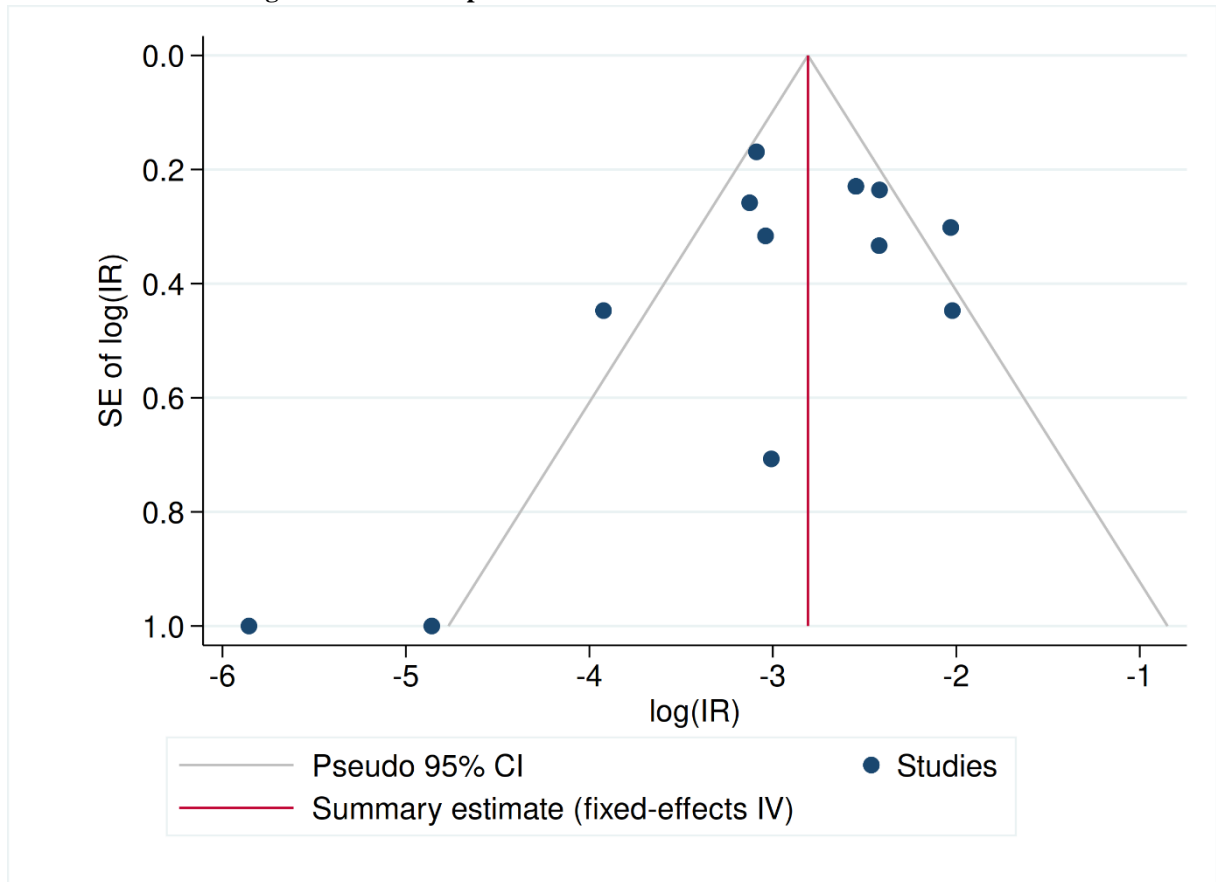

IR = incidence rate.

Figura S2 – Funnel plot for clinical and laboratory serious adverse events

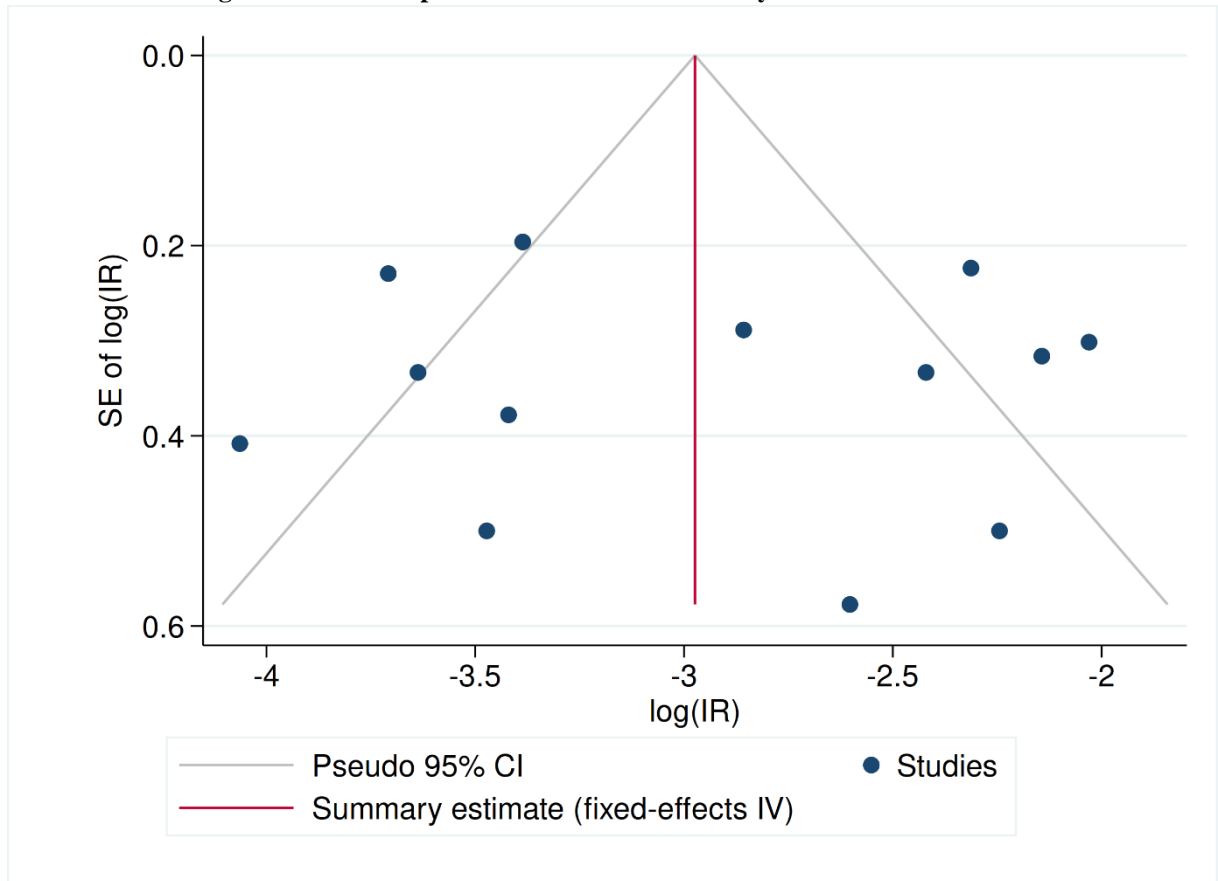

IR = incidence rate.