

Figure E1


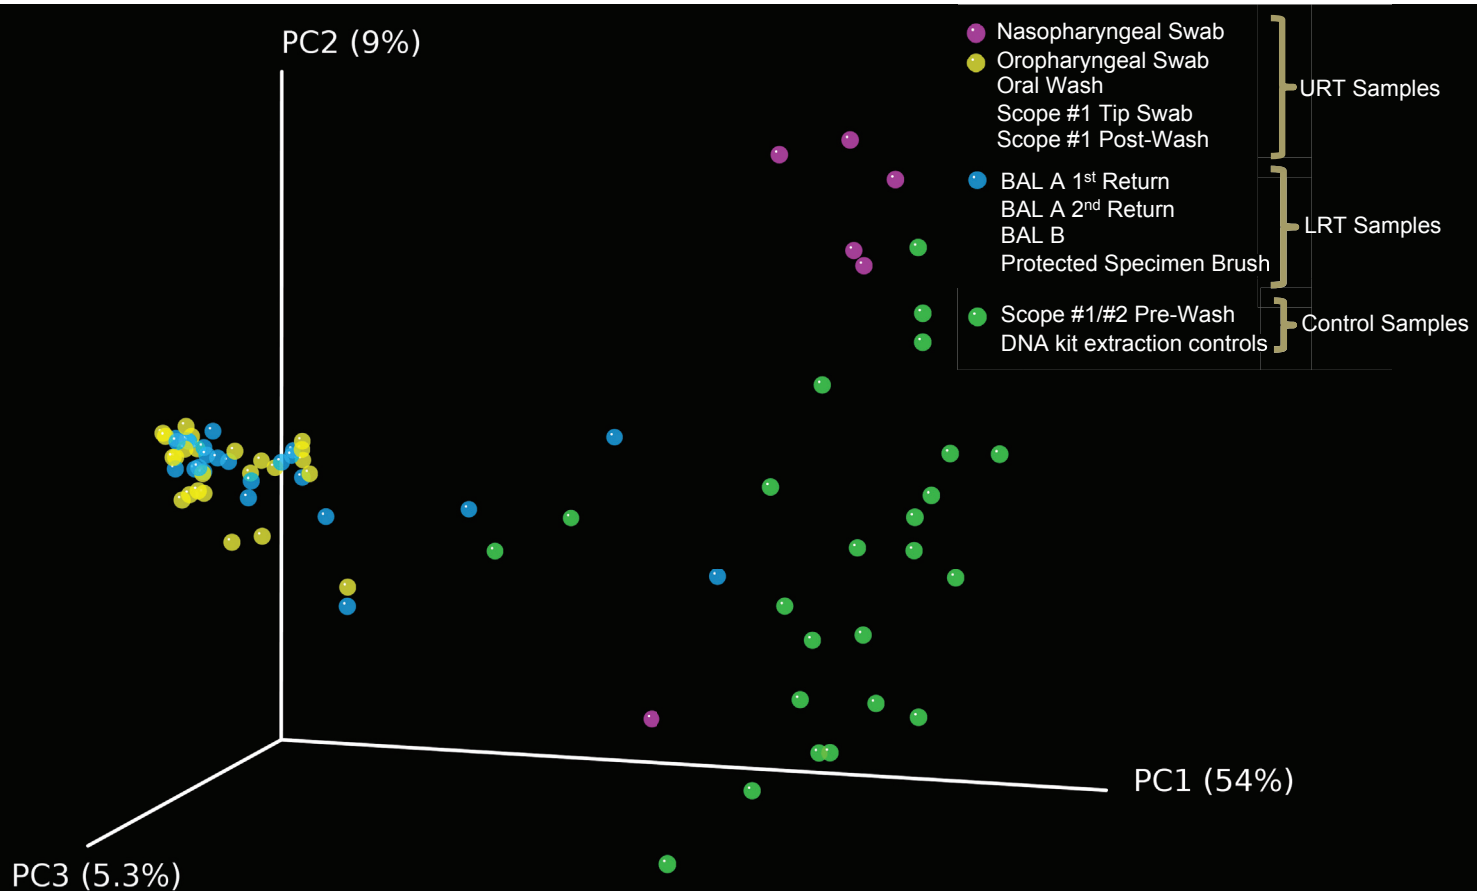


Figure E2

(A)

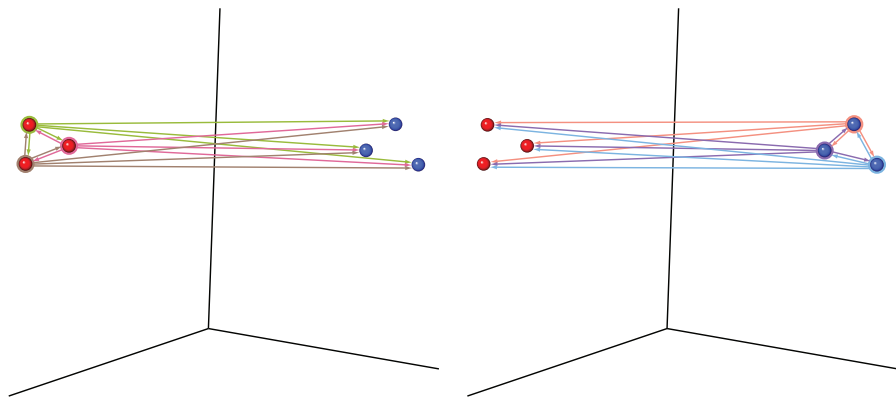

(B)

	Extraction Control	Scope 1 Pre-Wash	Scope 2 Pre-Wash	NP Swab	OP Swab	OW	Scope 1 Tip-Swab	Scope 1 Post-Wash	BAL A 1st Return	BAL A 2nd Return	BAL B	PSB
Extraction Control	NA	8.67E-01	7.55E-01	1.95E-01	1.34E-08	6.78E-07	1.99E-04	3.73E-08	3.77E-04	2.65E-03	7.67E-04	4.82E-08
Scope 1 Pre-Wash	4.75E-01	NA	6.22E-01	5.14E-01	1.19E-03	4.40E-03	4.81E-03	1.87E-03	5.28E-03	1.28E-02	5.72E-07	1.89E-03
Scope 2 Pre-Wash	5.75E-01	7.02E-01	NA	6.51E-01	1.19E-03	3.73E-03	2.97E-03	2.07E-03	5.28E-03	1.28E-02	6.16E-03	2.44E-03
NP Swab	2.14E-01	1.82E-01	6.07E-01	NA	1.39E-03	2.49E-03	3.78E-03	1.84E-03	6.16E-03	1.14E-02	4.94E-03	2.03E-03
OP Swab	1.00E-15	5.84E-11	1.42E-09	1.99E-11	NA	7.31E-01	3.77E-01	6.88E-01	4.89E-01	1.51E-01	2.49E-01	4.29E-01
OW	3.90E-14	1.15E-10	1.86E-09	4.42E-11	7.90E-01	NA	6.41E-01	6.45E-01	5.31E-01	1.33E-01	2.56E-01	7.13E-01
Scope 1 Tip-Swab	7.72E-12	3.22E-11	2.31E-10	7.29E-12	6.76E-01	9.58E-01	NA	6.85E-01	8.43E-01	2.96E-01	3.53E-01	4.69E-01
Scope 1 Post-Wash	0.00	9.92E-13	4.43E-11	1.07E-13	8.45E-01	7.97E-01	2.91E-01	NA	4.31E-01	9.36E-02	1.68E-01	5.18E-01
BAL A 1st Return	5.73E-06	9.37E-06	6.95E-06	5.63E-06	7.55E-01	7.28E-01	6.93E-01	5.05E-01	NA	9.65E-01	8.61E-01	4.07E-01
BAL A 2nd Return	7.84E-04	8.87E-04	4.82E-04	3.63E-04	5.32E-01	5.10E-01	4.27E-01	3.76E-01	4.09E-01	NA	4.85E-01	3.22E-01
BAL B	2.74E-07	5.54E-07	5.72E-07	1.13E-07	5.64E-01	5.71E-01	5.77E-01	2.83E-01	4.87E-01	8.57E-01	NA	2.51E-01
PSB	0.00	1.49E-12	1.24E-10	3.02E-13	8.80E-01	4.52E-01	2.80E-01	8.81E-01	4.32E-01	8.05E-02	1.09E-01	NA

Figure E3

