
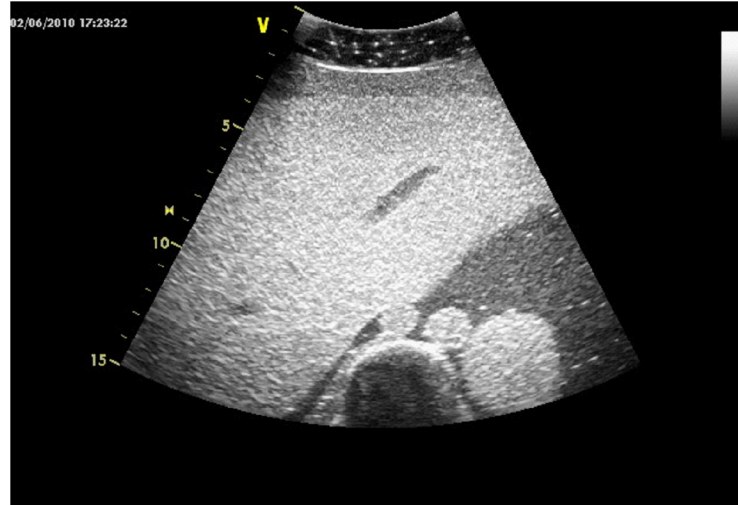
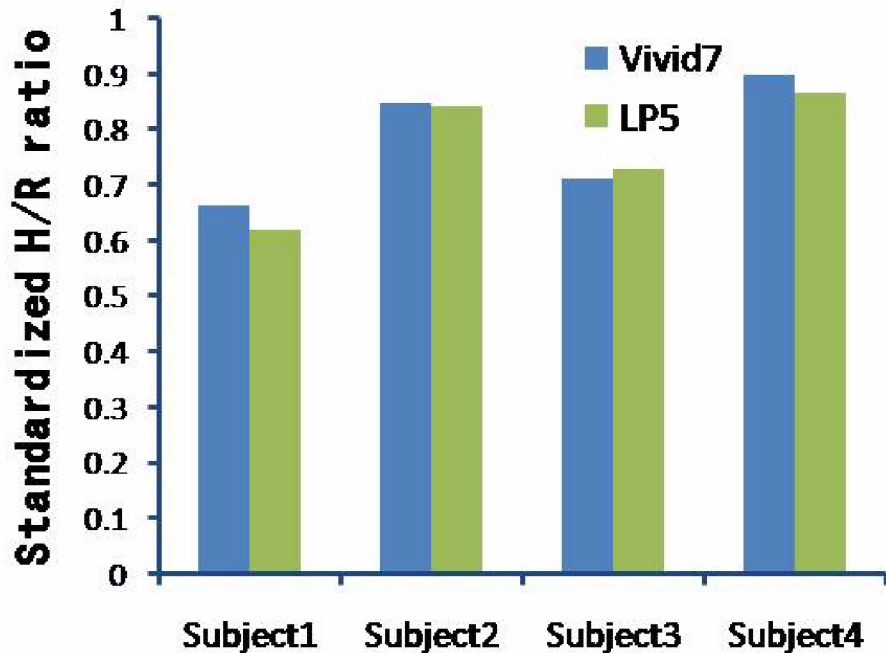


A**B****C****D**

ICC:0.985(0.768-0.999)

**E**

ICC:0.957(0.337-0.997)

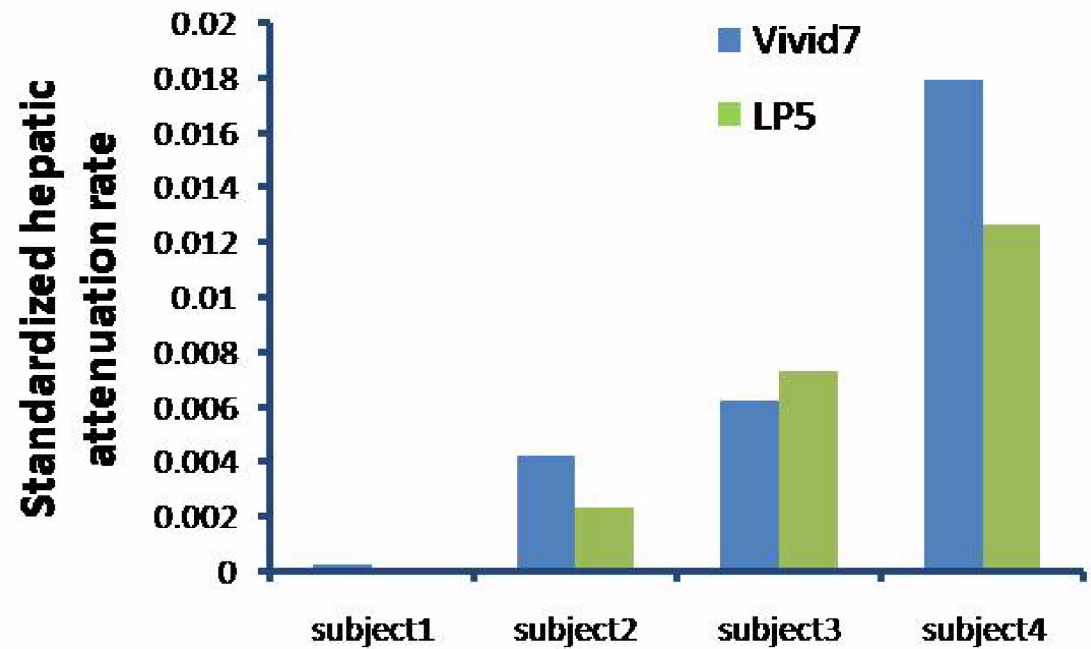

Supplement 1: A, Photograph of the tissue-mimicking phantom; B, ultrasound image of the phantom under Vivid 7 ultrasound machine; C, Ultrasound image of the phantom under LP5 ultrasound machine; D,E, Agreement of standardized H/R ratio and hepatic attenuation rate in four patients. ICC=0.985 and 0.957, respectively.