



Additional file 2 – The non-normalized raw Cq-values for PAXgene vs Tempus tubes

- A) The non-normalized raw Cq-values for adult blood samples collected in the PAXgene tubes;
 B) The non-normalized raw Cq-values for adult blood samples collected in the Tempus tubes; C)
 The non-normalized raw Cq-values for cord blood samples collected in the PAXgene and in the
 Tempus tubes. Each bar represents the average *Cq*-values and the error bar indicates \pm SE.

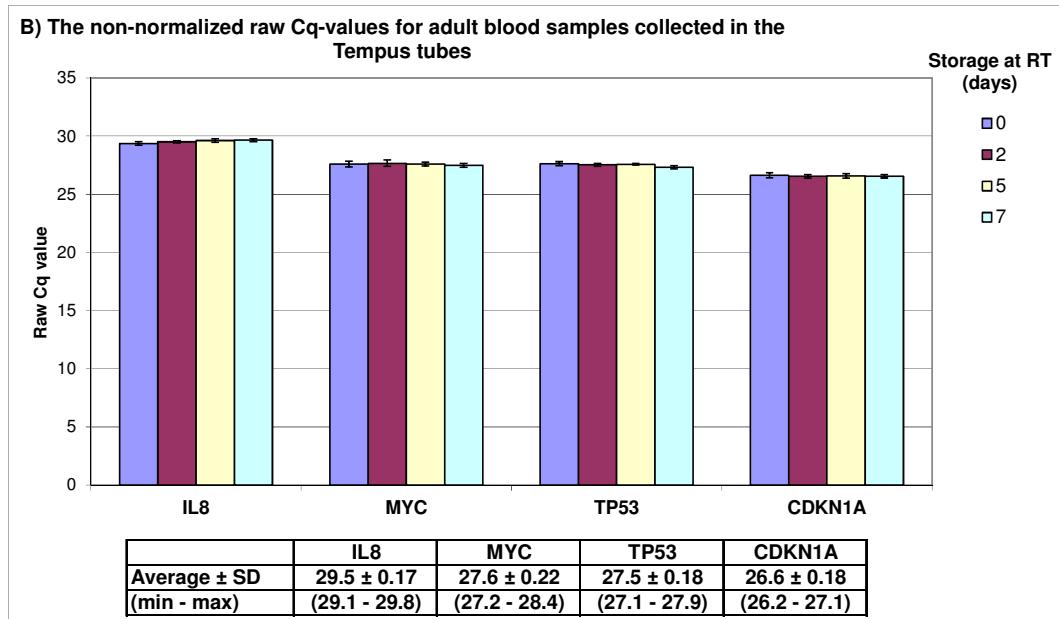

C) The non-normalized raw Cq-values for cord blood samples collected in the PAXgene and in the Tempus tubes

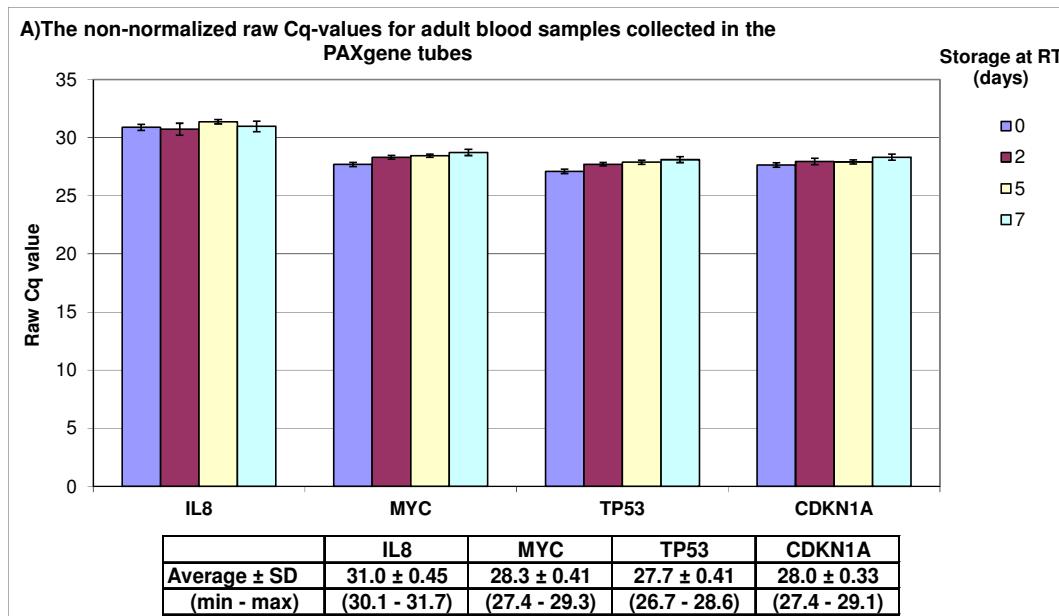