# Figure S1

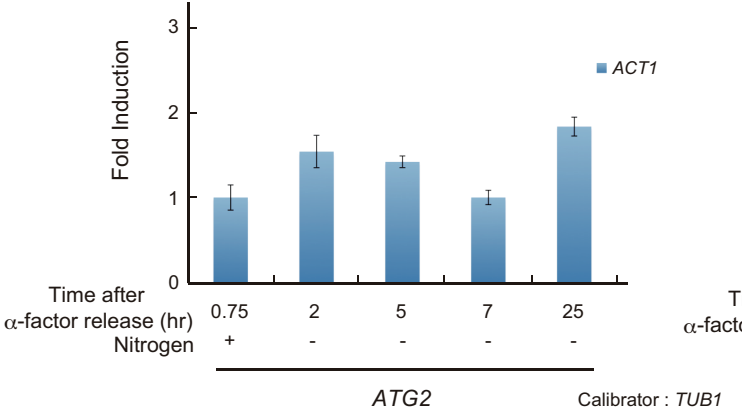
Fold Induction
3
2
1
0
ACT1
Time after
α-factor release (hr)
0.75
2
5
7
25
Nitrogen
+
-
-
-
-
ATG2
Calibrator : TUB1

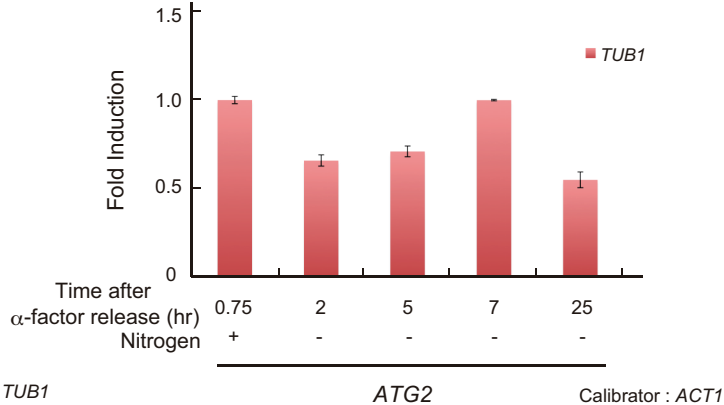
Fold Induction
1.5
1.0
0.5
0
TUB1
Time after
α-factor release (hr)
0.75
2
5
7
25
Nitrogen
+
-
-
-
-
ATG2
Calibrator : ACT1