


## Supplementary Information

**Figure S1.** Comparison between mir-30e and mir-16 stability in plasma samples from the 2 analyzed groups. *T* test *p* value = 0.1436 (mir-30e) vs. 0.002 (mir-16). Differences between means:  $0.119 \pm 0.080$  (mir-30e) vs.  $(-0.175) \pm 0.055$  (mir-16). \*\* *p* < 0.01 (*T* test).

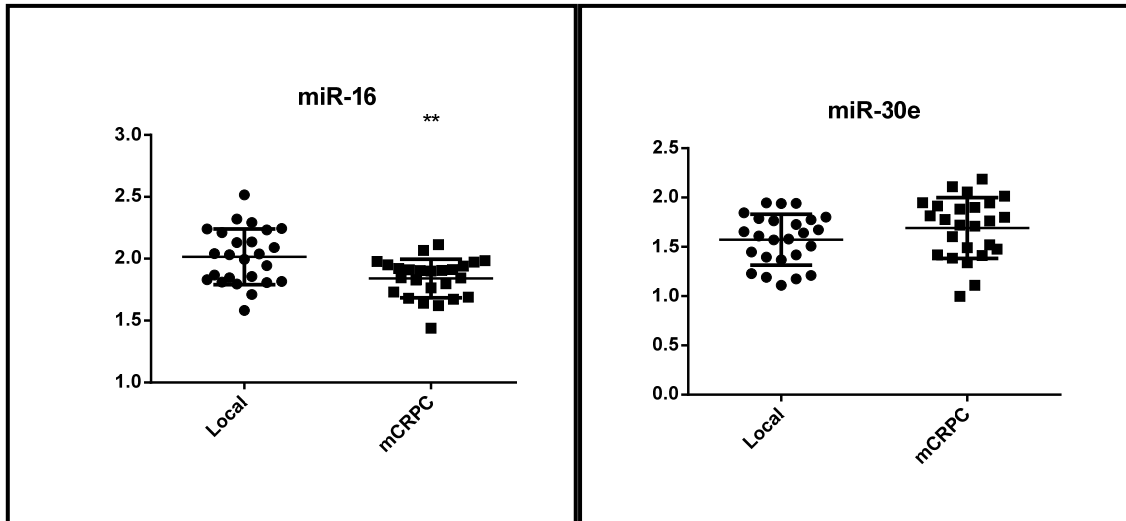

© 2013 by the authors; licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution license (<http://creativecommons.org/licenses/by/3.0/>).