


Supplemental File: Figure S5

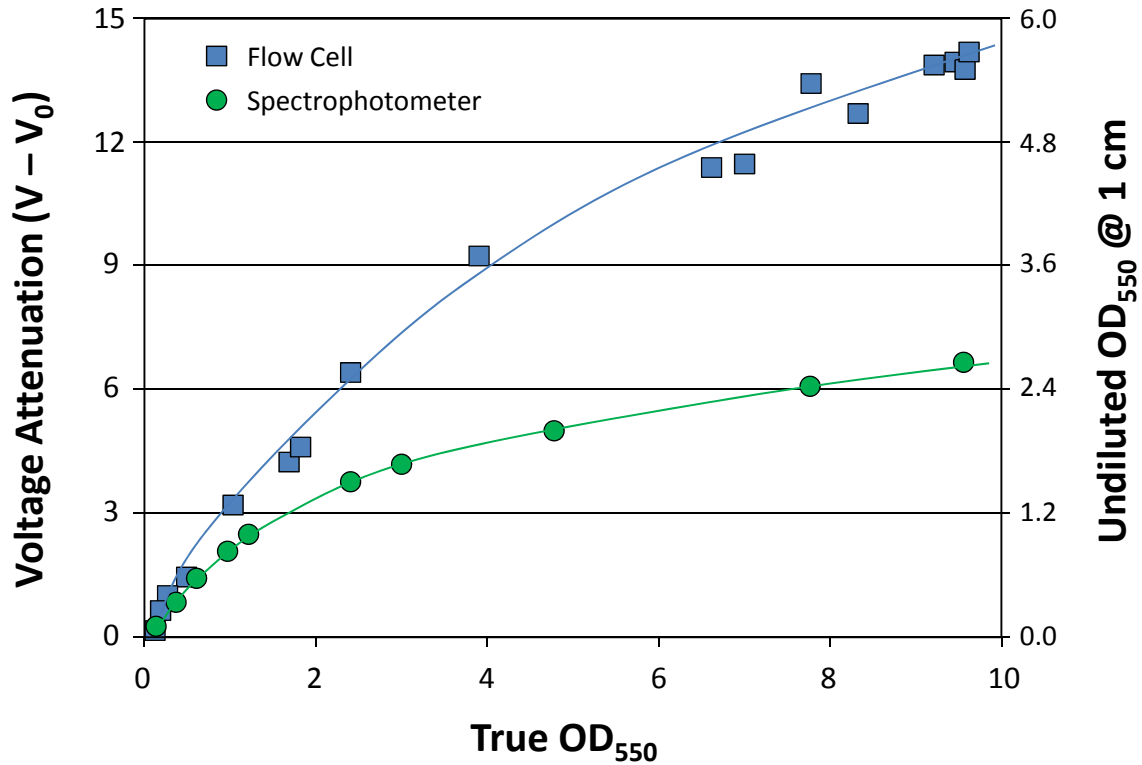

Additional file 5. Figure S5 – Algae OD measurements in OD flow cell.

Ability of a short path-length flow cell to extend the range of OD measurements. *Chlorella vulgaris* cultures grown photosynthetically were resuspended at various cell concentrations and run through the flow cell as compared to undiluted OD₅₅₀ measurements (Spectramax photometer).