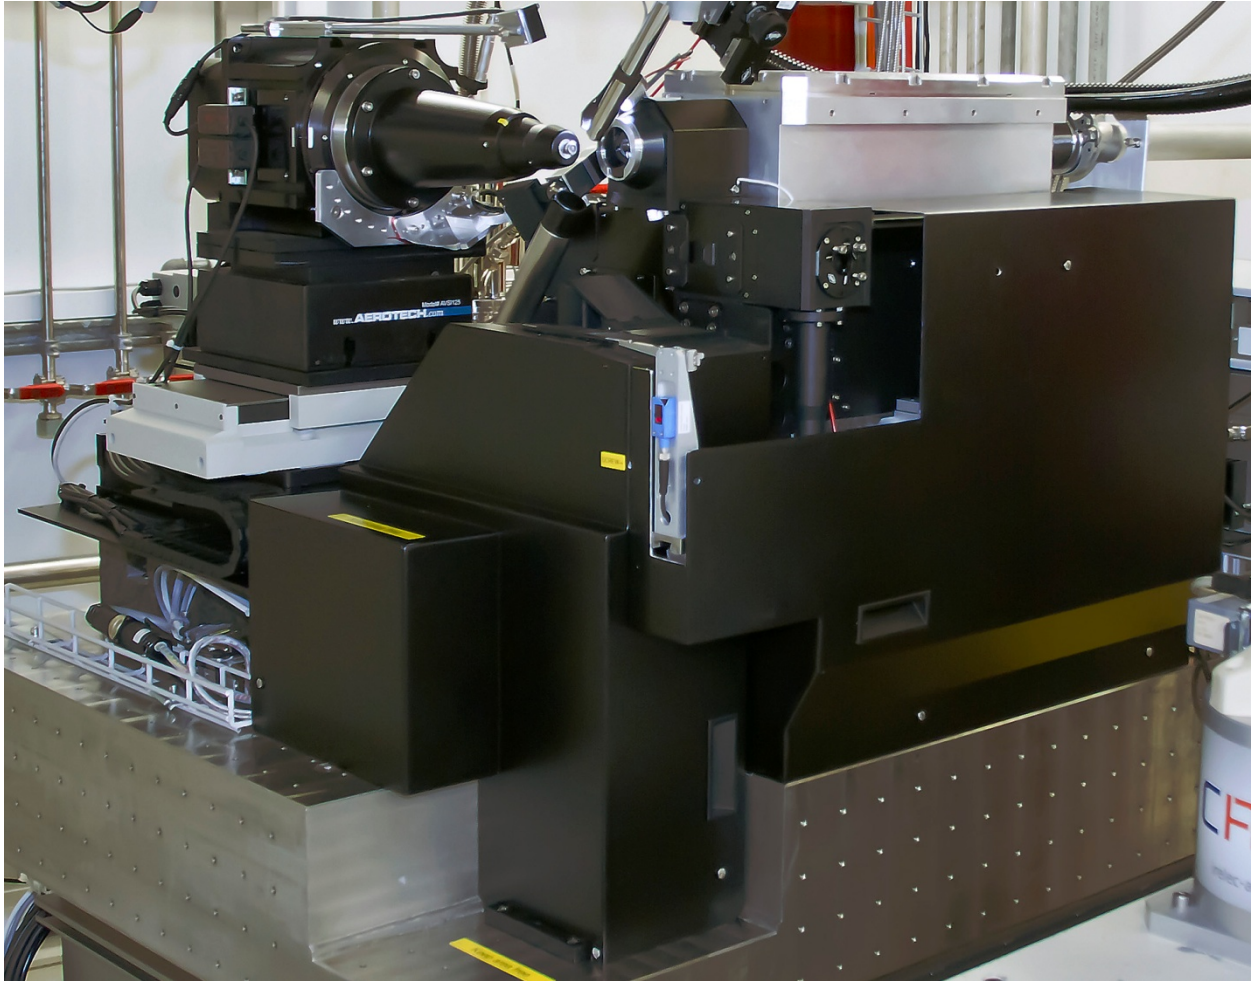


## Supplementary material



**Figure 3** Diffractometer cover close to sample. A two-piece Al-cover protects all cabling and actuators of the diffractometer with the exception of the goniometer at left.