

Analytical and Bioanalytical Chemistry

Electronic Supplementary Material

Measurement of bisphenol A, bisphenol A β -D-glucuronide, genistein, and genistein 4'- β -D-glucuronide via SPE and HPLC-MS/MS

Janis L. Coughlin, Bozena Winnik, and Brian Buckley

Figure S1: BPA calibration curve. (Y-axis: integrated area)

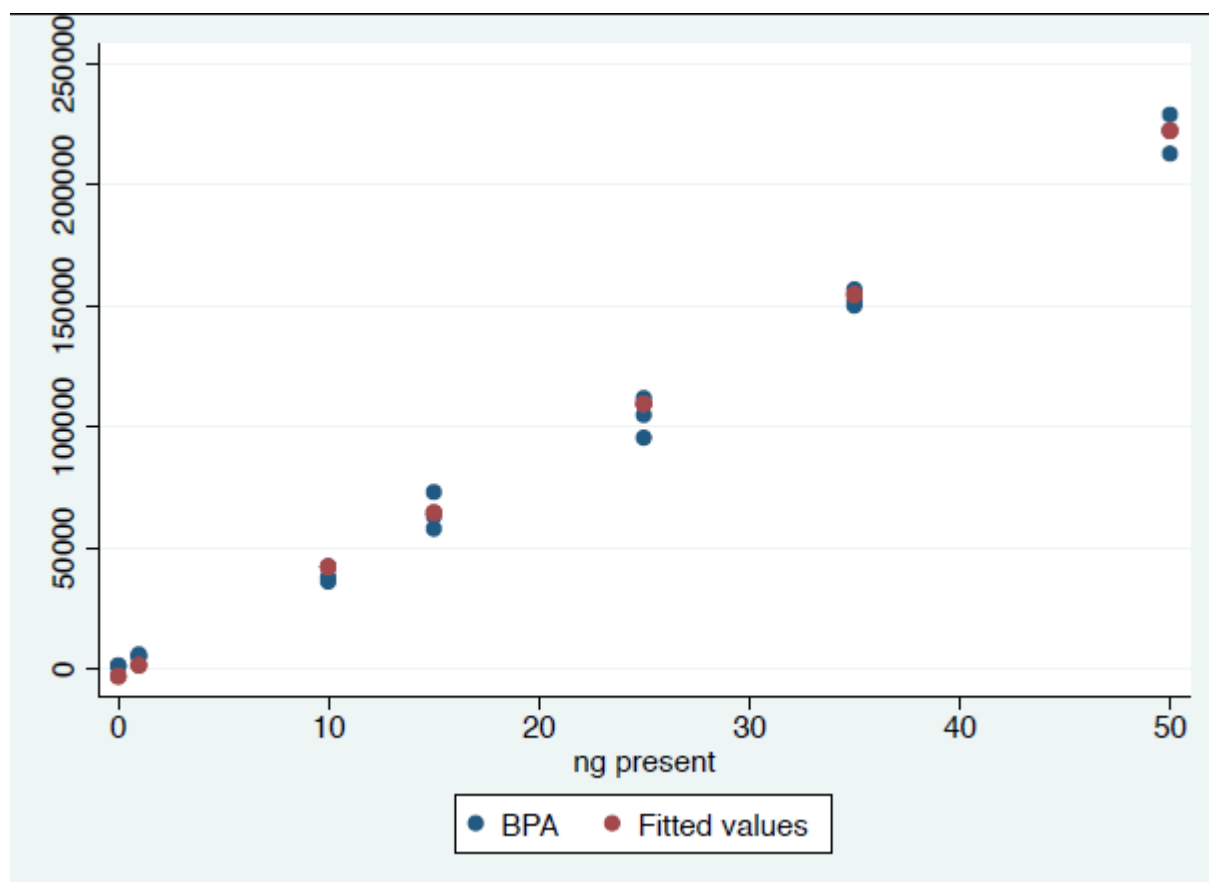


Figure S2: BPA glucuronide calibration curve. (Y-axis: integrated area)

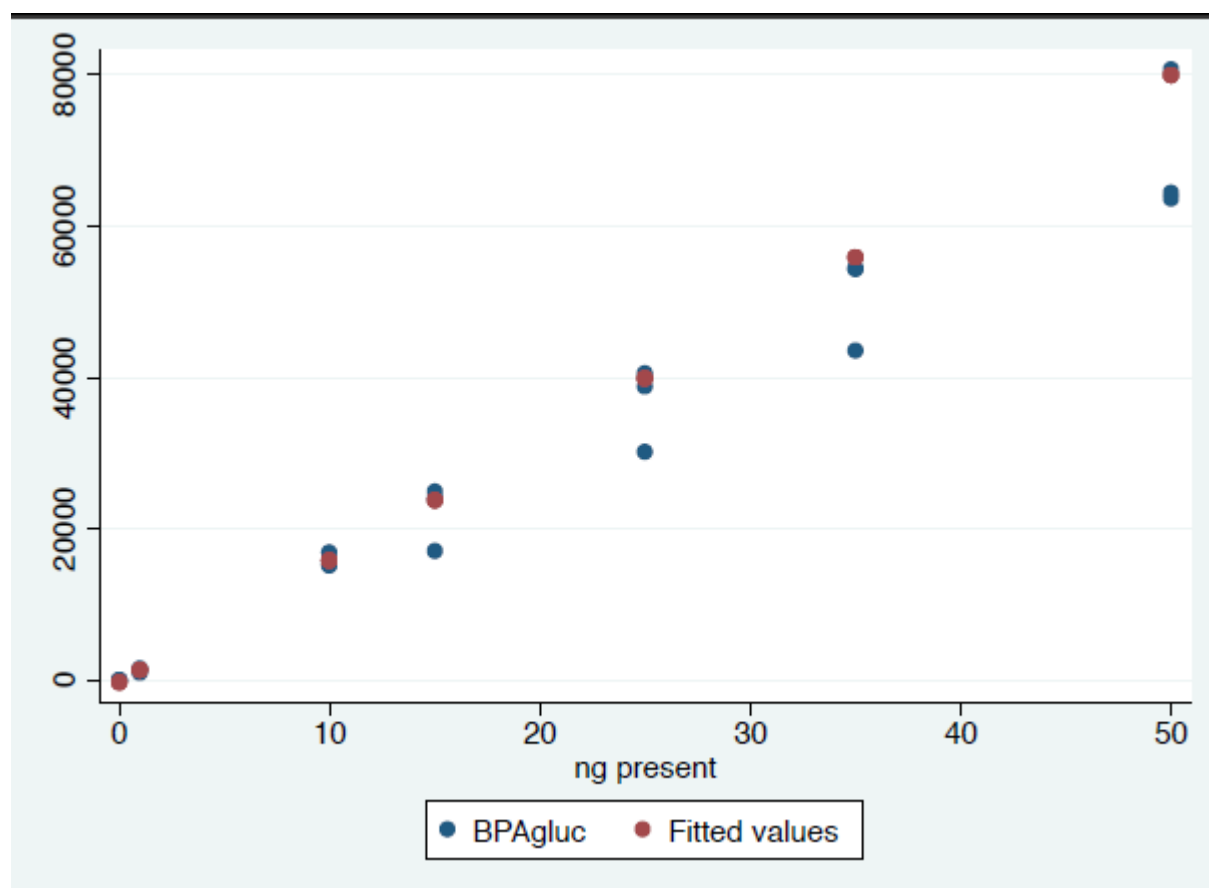


Figure S3: Genistein calibration curve. (Y-axis: integrated area)

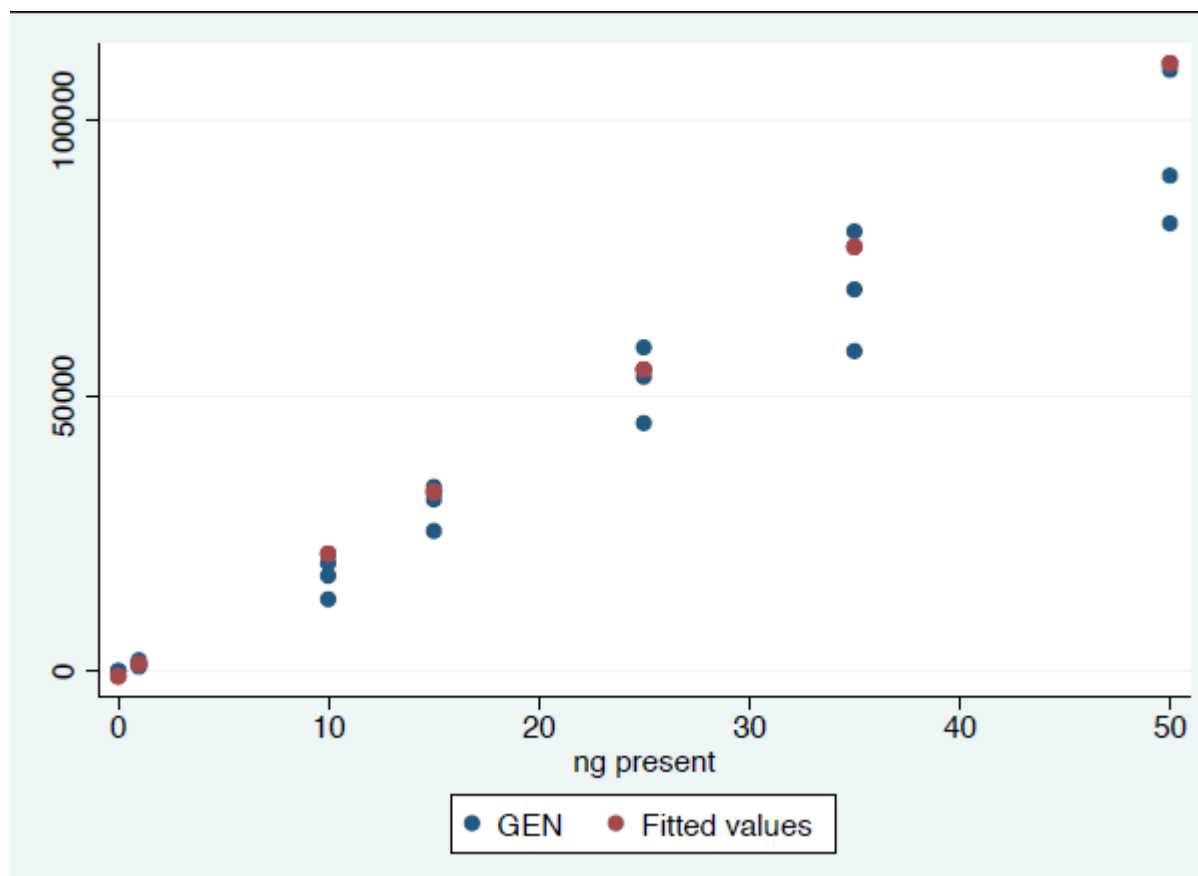


Figure S4: Genistein glucuronide calibration curve. (Y-axis: integrated area)

