


**PERCENT OF PATIENTS WITH PRIMARY PCI DONE WITHIN 90 MINUTES
(JUNE - NOVEMBER 2011)**

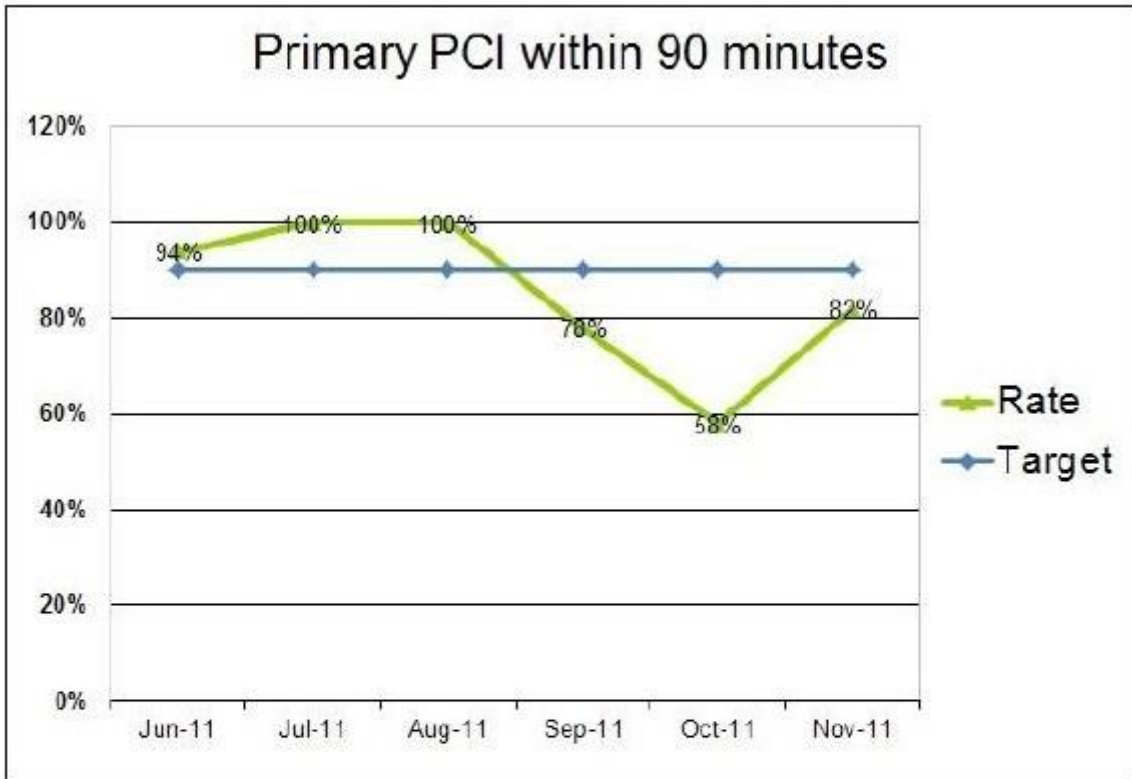

AVERAGE TIMES FOR PATIENTS NOT MEETING THE 90-MINUTE TARGET

DOOR-TO-BALLOON PHASE	AVERAGE MEASURED TIME (minutes)	RECOMMENDED TIME (minutes)
Door to ECG	24	<10
ECG to STEMI Confirmation / Activation	31	10
STEMI Confirmation to CathLab Activation	25	15
CathLab Activation to Device Deployment	82	50-60