


Figure S2. Distribution of programming parameters within 10 days of implant, across the entire analysis population.

Panel A.

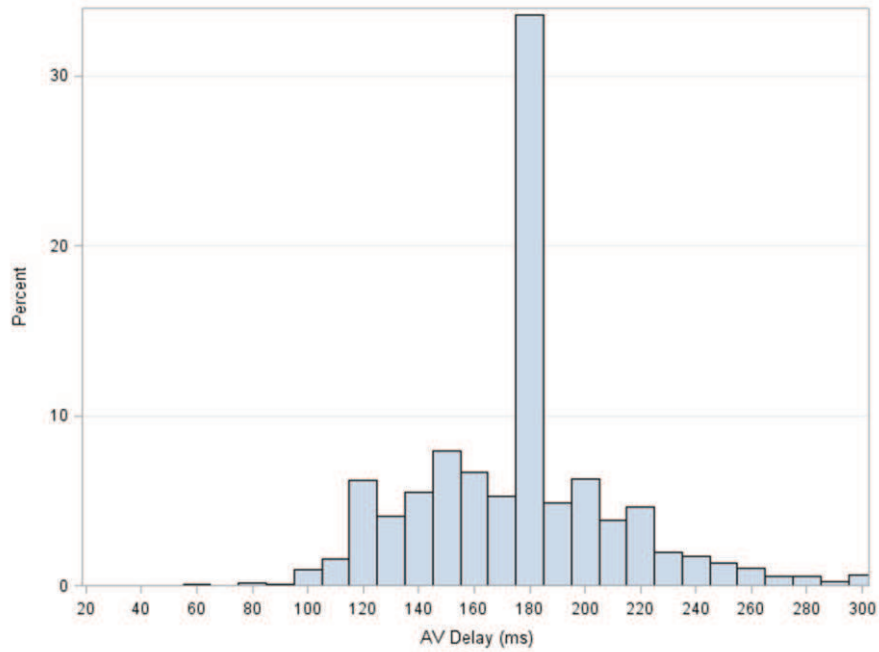

AV: atrioventricular timing (paced); VV: ventricular-to-ventricular timing.

Panel B.

