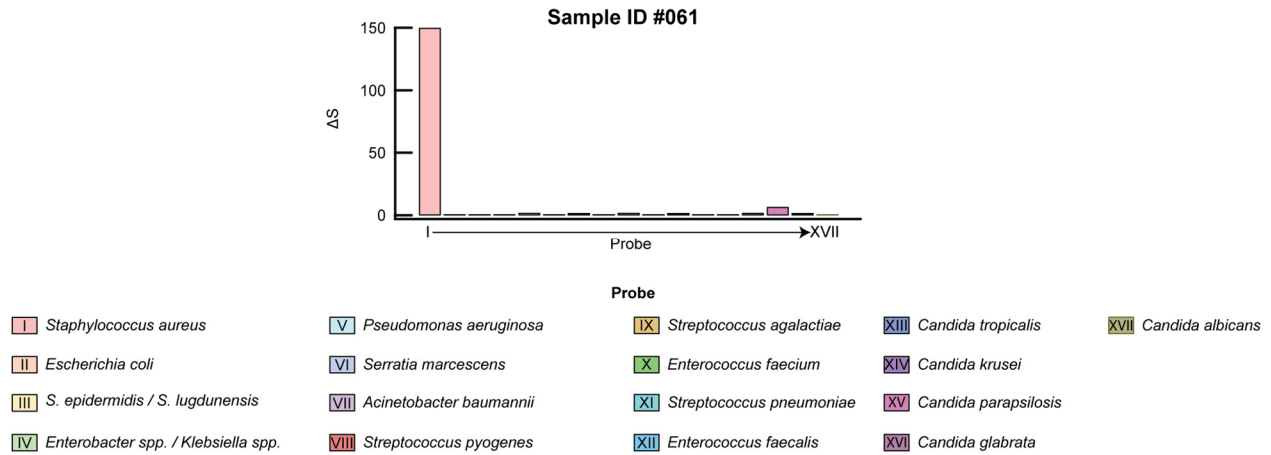


## PID assay / Culture positive concordant results



**Figure S4** - Performance of PID assay with concordant culture positive clinical specimens. Sample number refers to patient specimen listed in Tables 1 and S3. Sample ID #061 was deemed positive for *S. aureus*.