



Supplementary Figure S1

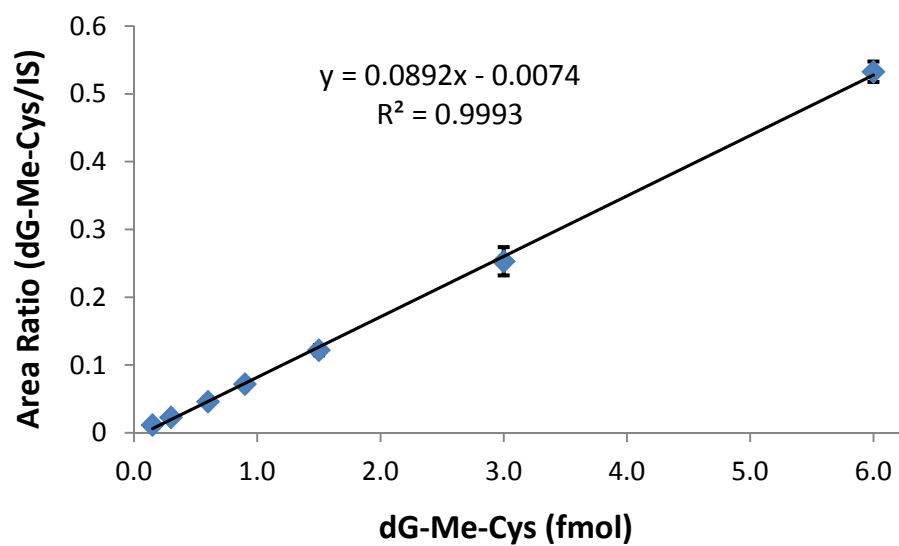


Supplementary Figure S1. Typical calibration curve used for the quantification of dG-Me-Cys with the linearity from 0.15 to 6.0 fmol. The data represent the mean value \pm standard deviation from three individual experiments.

Supplementary Figure S2

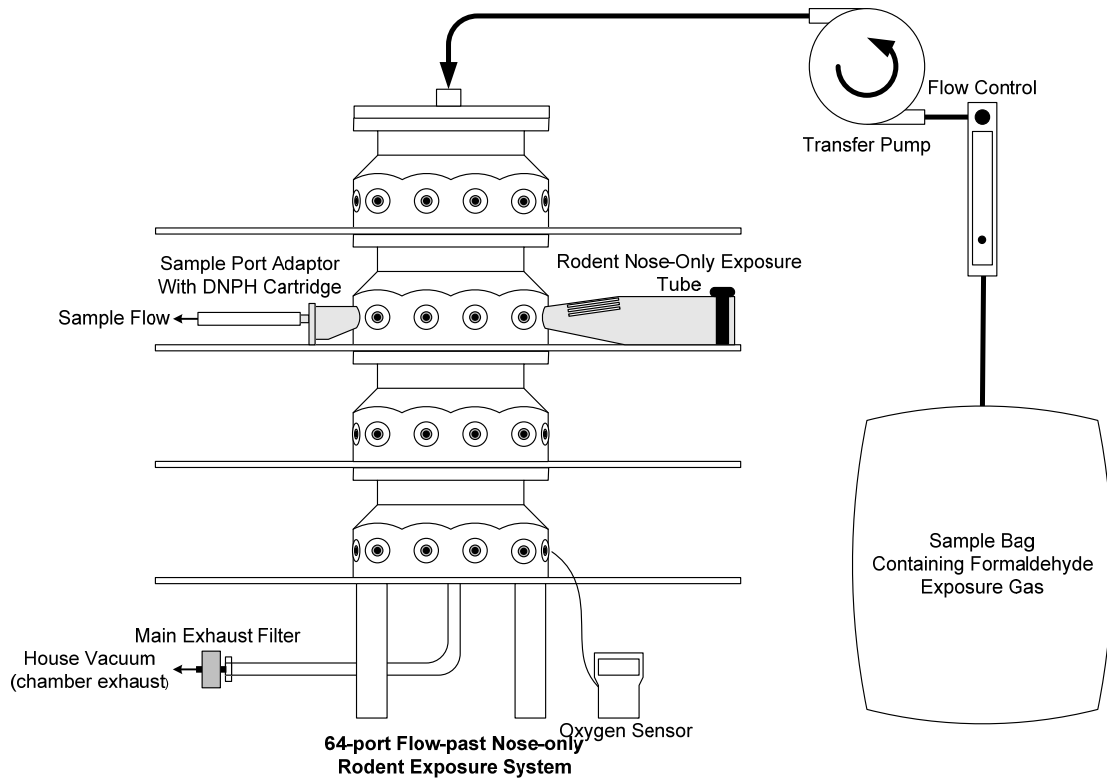

Supplementary Figure S2. Schematic of rat nose only inhalation chamber.

Supplementary Figure S3

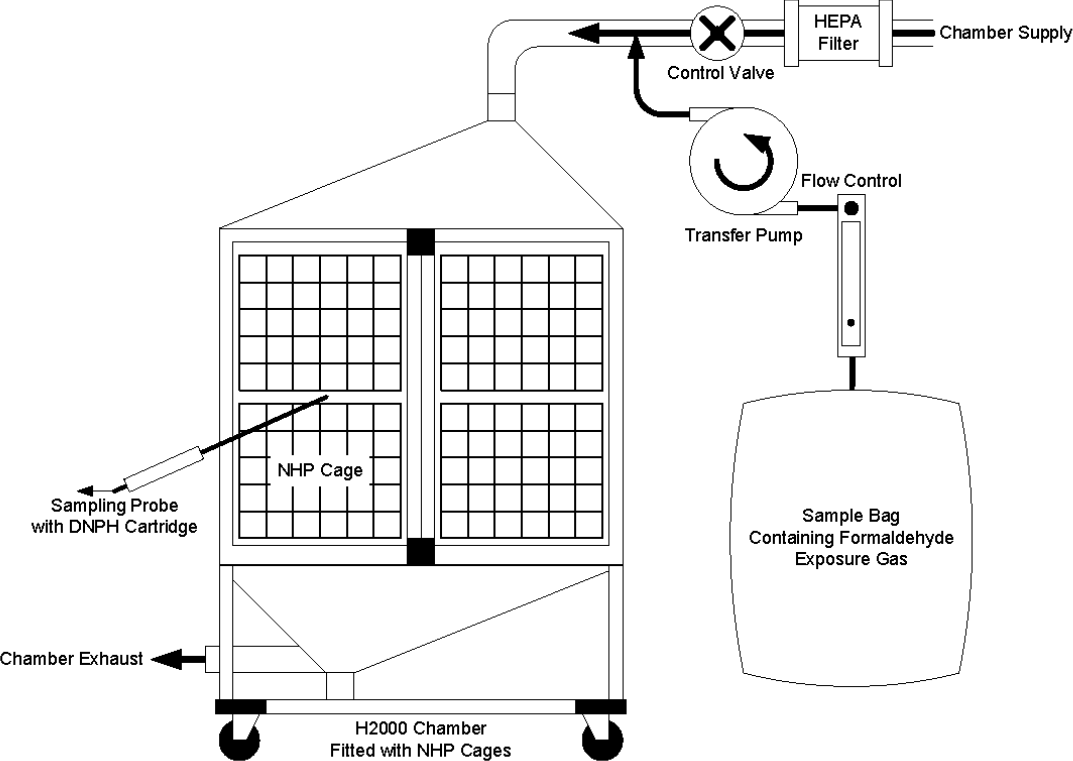

Supplementary Figure S3. Schematic of primate whole-body inhalation chamber.