


BEAD ASSAY FOR BIOFILMS



↓ place in container (+ 2 wet paper towels)

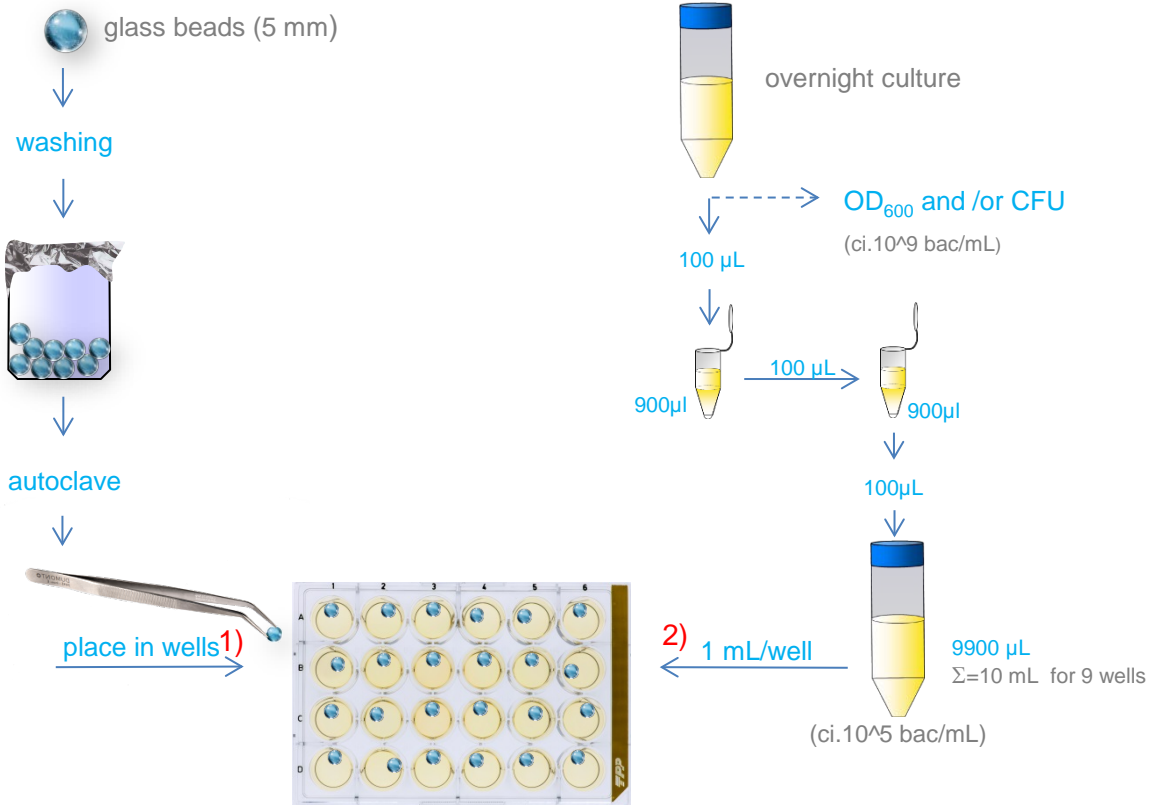

↓ place on orbital shaker



24 h, 37° C, 150 rpm



