


S5 Fig

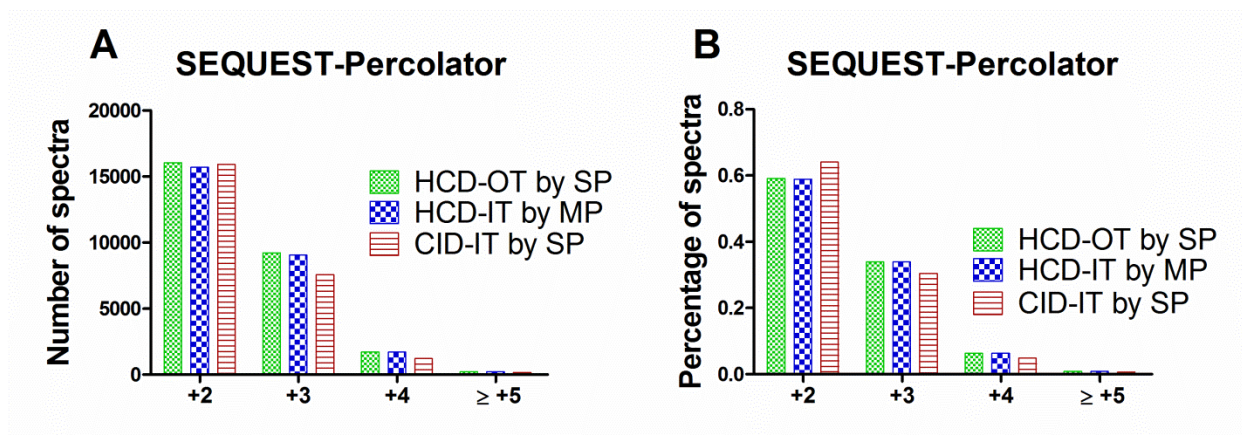

S5 Fig. The comparison of HCD-OT by SP, HCD-IT by MP, and CID-IT by SP for separate LC-MS/MS analyses. (A) Number of spectra for +2, +3, +4 and  $\geq 5$  charged; (B) Percentage of spectra for for +2, +3, +4 and  $\geq 5$  charged ions from these three MS2 acquisition methods. SP: SEQUEST-Percolator; MP: Mascot-Percolator.