

Supplementary Information for

TOF-SIMS imaging of biological samples with delayed extraction for high mass and high spatial resolutions

Quentin P. Vanbellingen,^{†,‡} Nicolas Elie,^{†,‡} Michael J. Eller,[§] Serge Della-Negra,[§] David Touboul,[†] and Alain Brunelle^{*,†}

[†] Institut de Chimie des Substances Naturelles, CNRS-ICSN UPR2301, Université Paris-Sud, Avenue de la Terrasse, 91198 Gif-sur-Yvette, France

[§] Institut de Physique Nucléaire, UMR8608, IN2P3-CNRS, Université Paris-Sud, 91406 Orsay, France

TABLE OF CONTENTS

Figure S-1: Peak width FWHM (ns) as a function of the extraction delay (a) negative ion mode, m/z 255.2 ([C16:0-H] ⁻ , blue) and m/z 385.4 (cholesterol [M-H] ⁻ , green) (b) positive ion mode, m/z 369.4 (cholesterol [M-H ₂ O+H] ⁺ , blue) and m/z 430.4 (Vitamin E [M] ⁺ , green).....	2
Figure S-2: Primary ion beam profiles (b,d,f) measured on a grid (a,c,e, pitch 25 μ m, hole width 19 μ m, wire width 6 μ m), for HCBU; BA; and BA+DE setting modes.....	2
Figure S-3: Part of TOF-SIMS negative ion mass spectra showing H ⁻ ion for different extraction delays. Vertical red line is to guide the eye and show the extraction delay for which the ions start shifting.	3
Figure S-4: Calculated arrival positions of secondary ions (m/z 400) on the surface of the MCP obtained by simulation for different kinetic energies: 0.1 eV (red); 0.2 eV (blue); 0.5 eV (orange) and 1.0 eV (green) with an extraction delay equal to the pulse duration (100 ns).....	3
Figure S-5: Calculated dispersion of secondary ion arrival positions (energy 0.1 eV) on the surface of the MCP obtained by simulation for different mass-to-charge ratios: m/z 1; 6; 12; 14; 23; 48 and 100 with an extraction delay equal to the pulse duration (100 ns).	4
Figure S-6: Parts of TOF-SIMS negative ion mass spectra recorded on the surface of a rat brain section, using HCBU, BA, and BA+DE setting modes and showing three deprotonated fatty acids: C16:0; C18:1 and C18:0.....	4
Figure S-7: Parts of TOF-SIMS positive ion mass spectra recorded on the surface of a rat brain section, using HCBU, BA, and BA+DE setting modes and showing two ion species of cholesterol (a,c,e) and the vitamin E isotopic distribution (b,d,f).	5

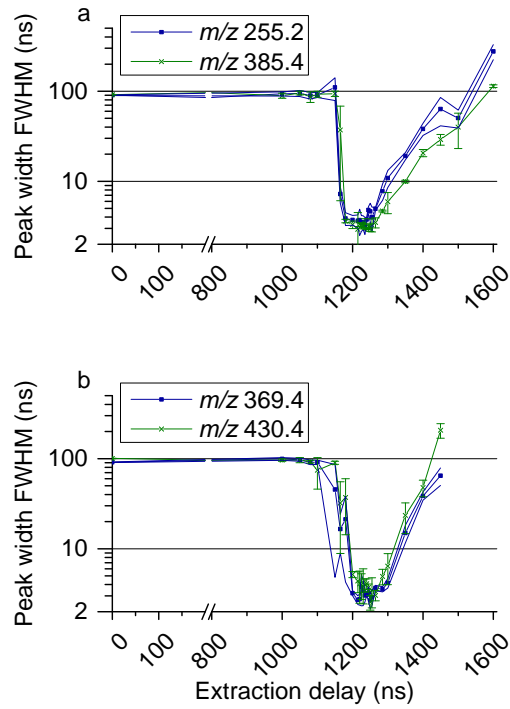


Figure S-1: Peak width FWHM (ns) as a function of the extraction delay (a) negative ion mode, m/z 255.2 ($[C_{16:0-H}]^-$, blue) and m/z 385.4 (cholesterol $[M-H]^-$, green) (b) positive ion mode, m/z 369.4 (cholesterol $[M-H_2O+H]^+$, blue) and m/z 430.4 (Vitamin E $[M]^+$, green).

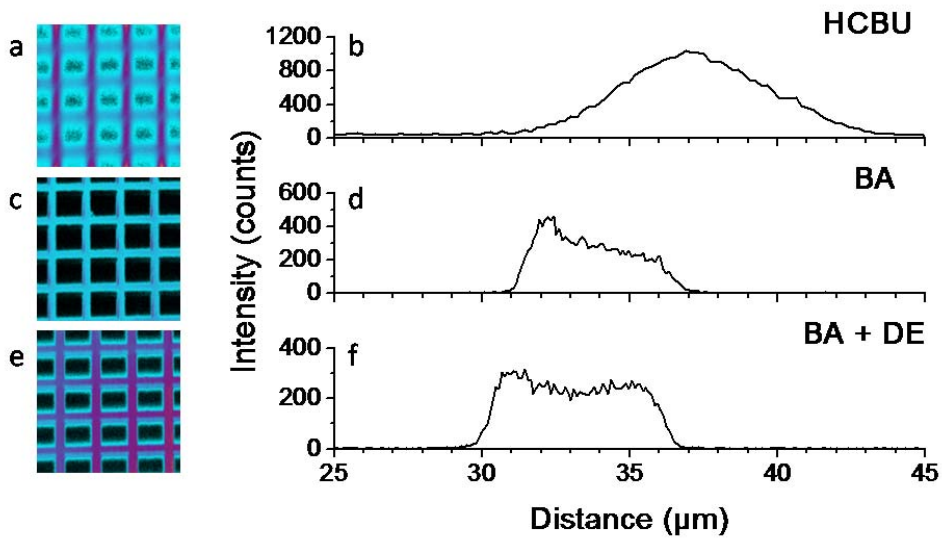


Figure S-2: Primary ion beam profiles (b,d,f) measured on a grid (a,c,e, pitch 25 μm , hole width 19 μm , wire width 6 μm), for HCBU; BA; and BA+DE setting modes.

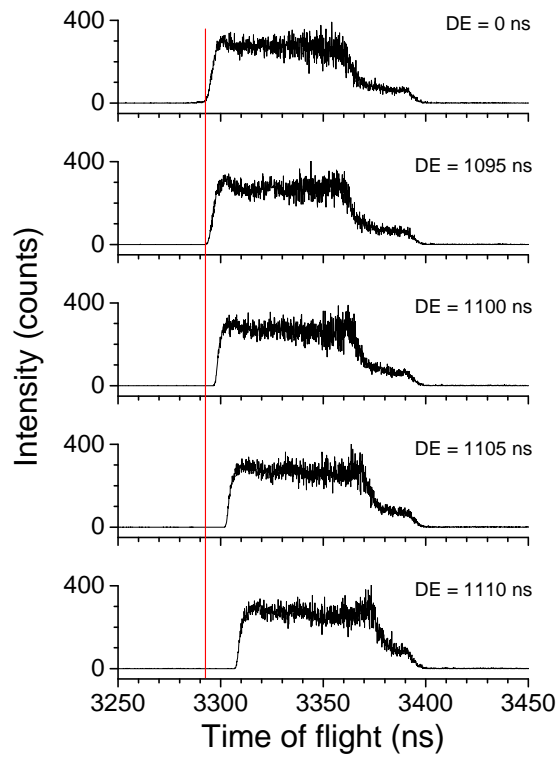


Figure S-3: Part of TOF-SIMS negative ion mass spectra showing H⁻ ion for different extraction delays. Vertical red line is to guide the eye and show the extraction delay for which the ions start shifting.

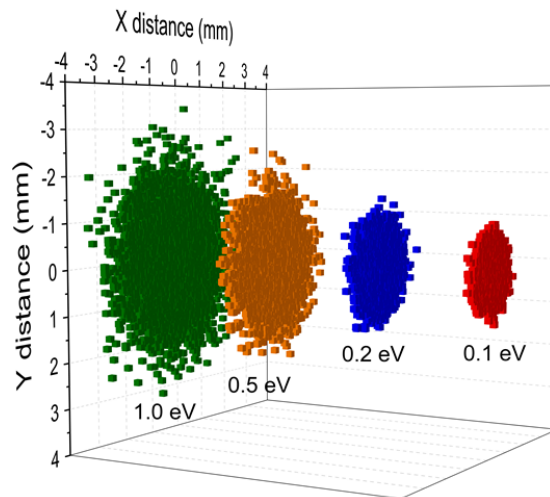


Figure S-4: Calculated arrival positions of secondary ions (m/z 400) on the surface of the MCP obtained by simulation for different kinetic energies: 0.1 eV (red); 0.2 eV (blue); 0.5 eV (orange) and 1.0 eV (green) with an extraction delay equal to the pulse duration (100 ns).

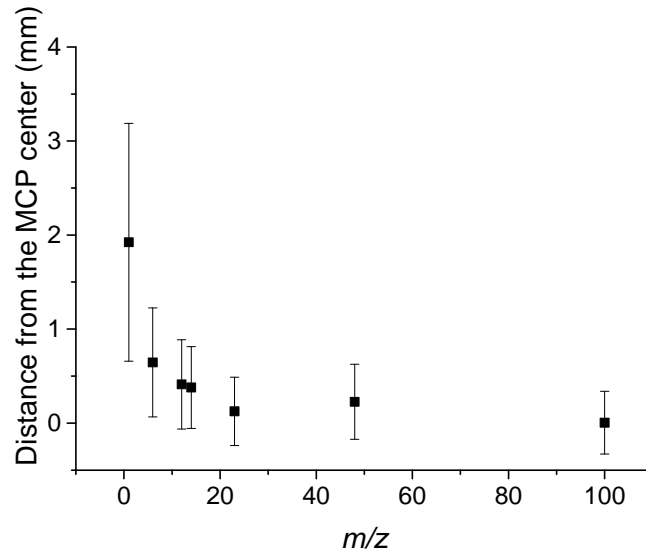


Figure S-5: Calculated dispersion of secondary ion arrival positions (energy 0.1 eV) on the surface of the MCP obtained by simulation for different mass-to-charge ratios: m/z 1; 6; 12; 14; 23; 48 and 100 with an extraction delay equal to the pulse duration (100 ns).

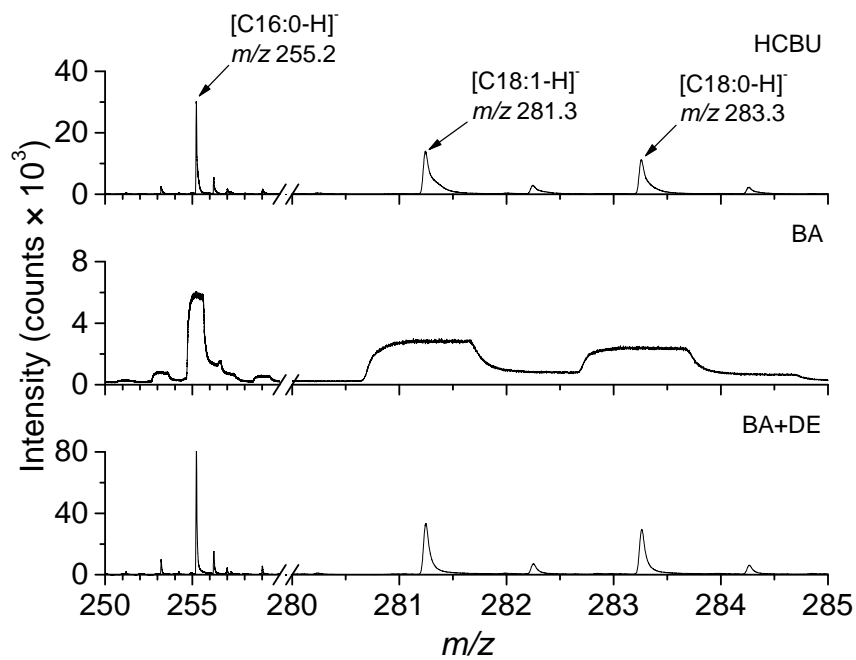


Figure S-6: Parts of TOF-SIMS negative ion mass spectra recorded on the surface of a rat brain section, using HCBU, BA, and BA+DE setting modes and showing three deprotonated fatty acids: C16:0; C18:1 and C18:0.

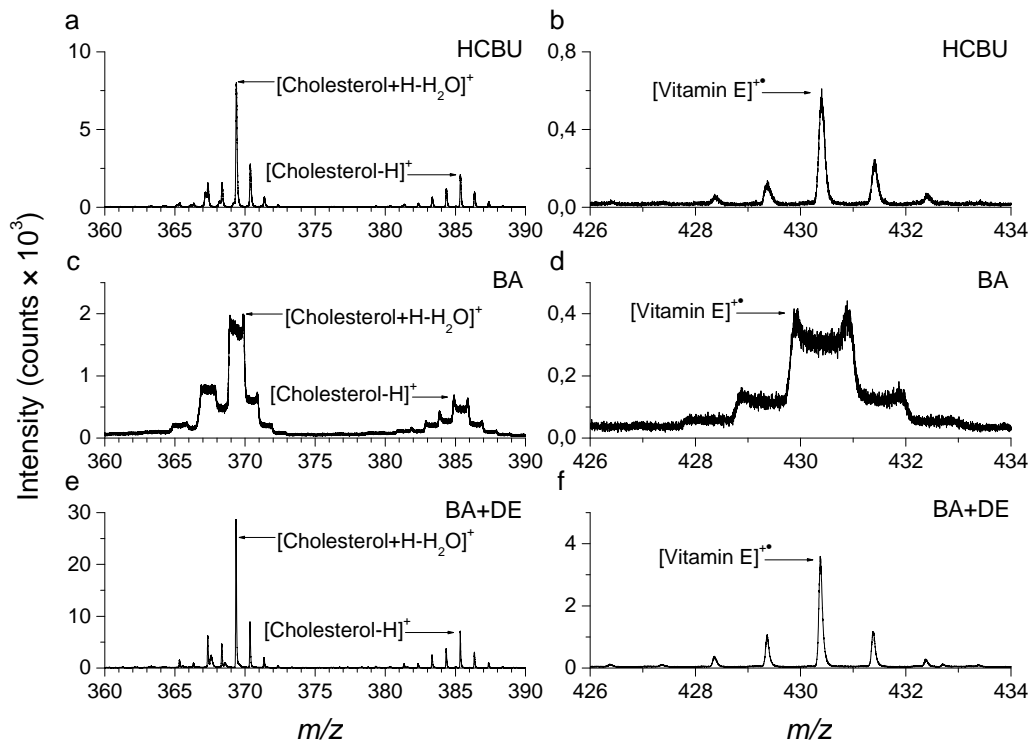


Figure S-7: Parts of TOF-SIMS positive ion mass spectra recorded on the surface of a rat brain section, using HCBU, BA, and BA+DE setting modes and showing two ion species of cholesterol (a,c,e) and the vitamin E isotopic distribution (b,d,f).