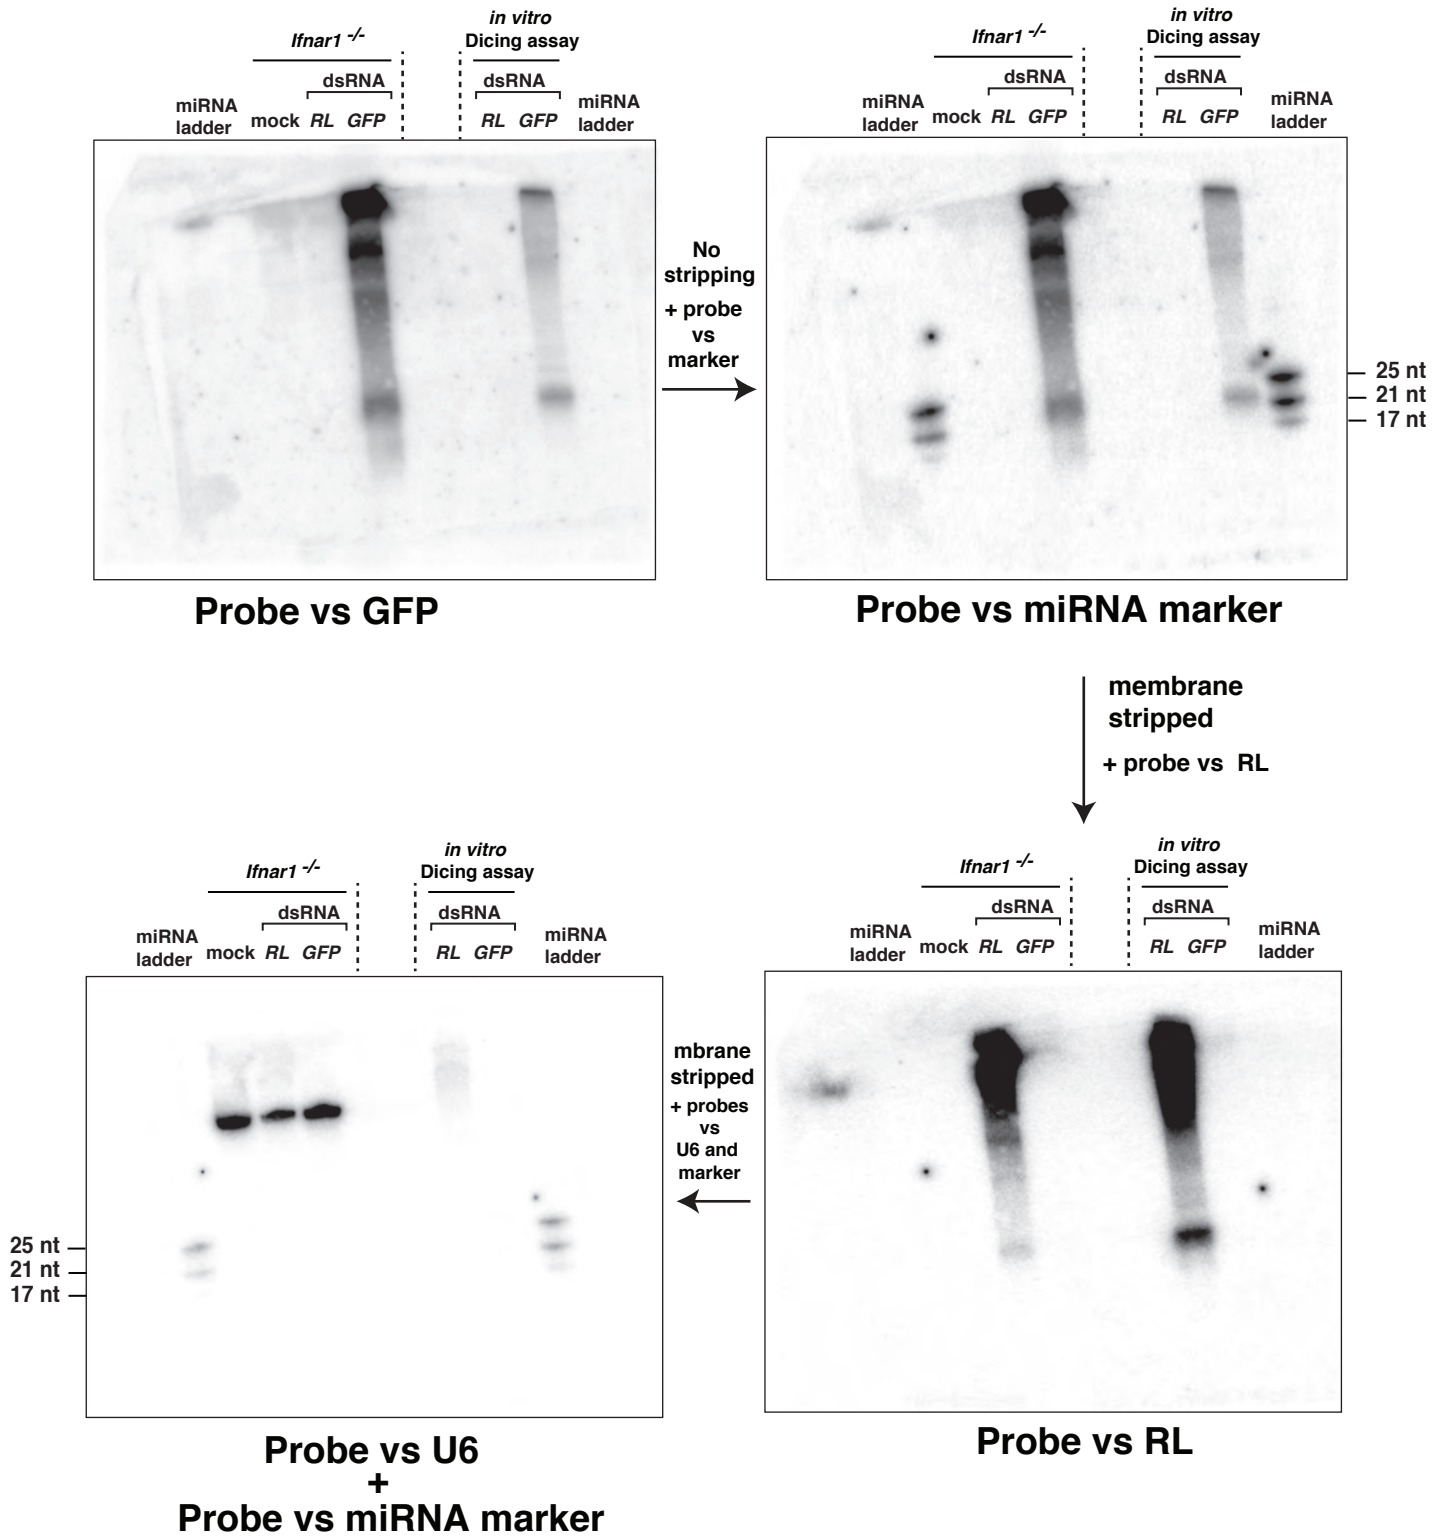
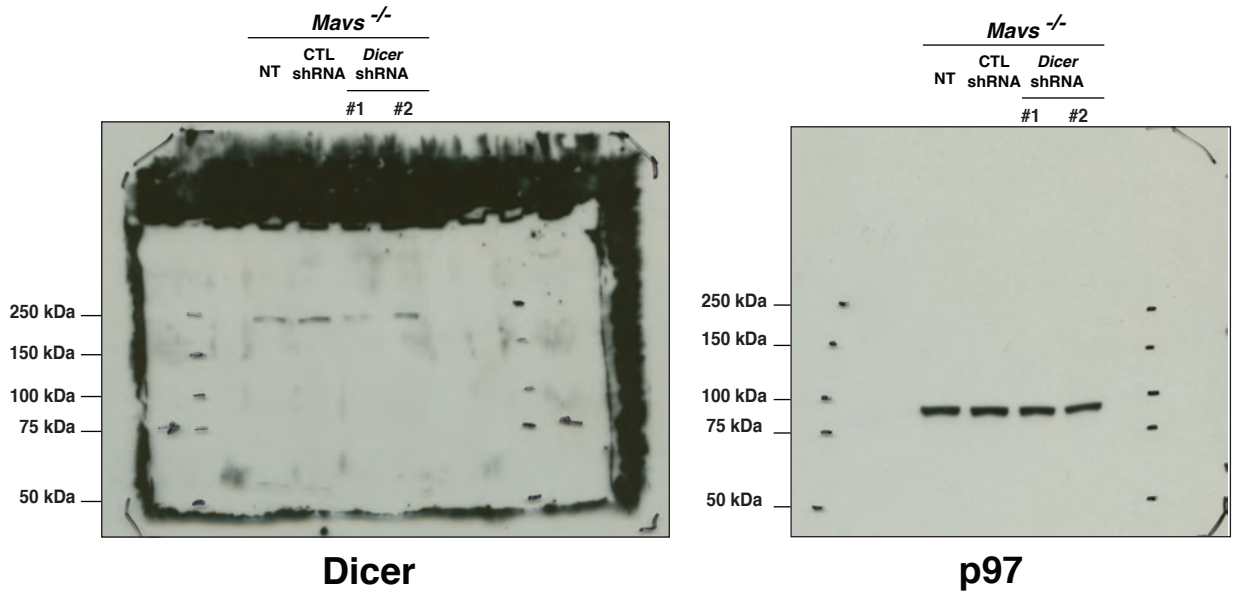
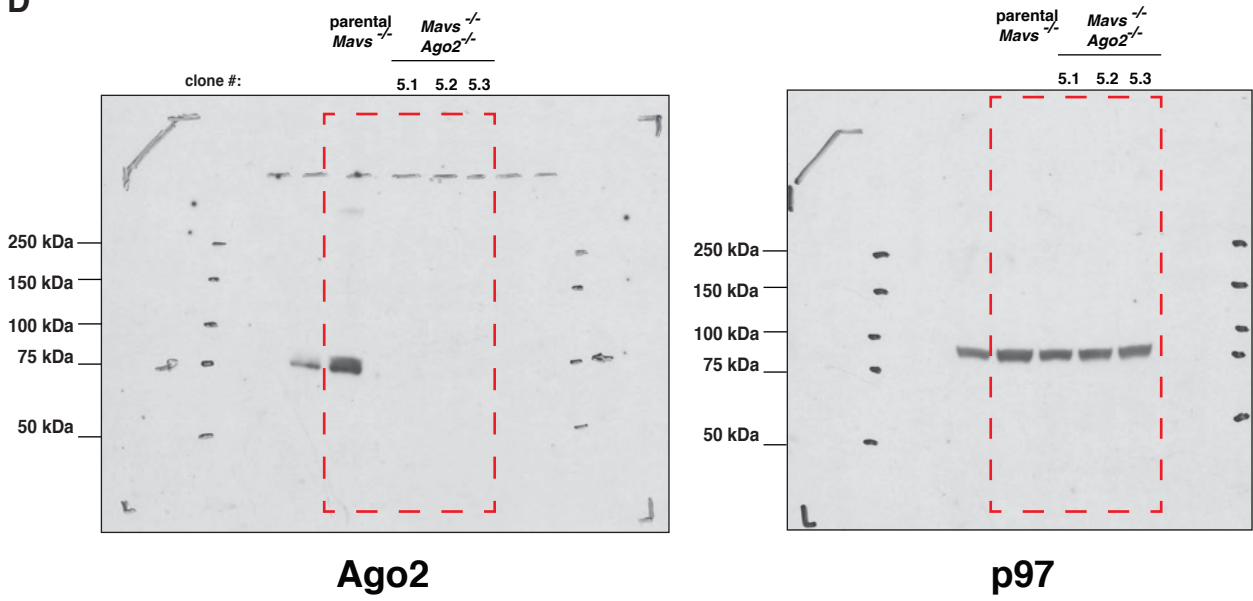


A

Note: Blots were exposed to a storage phosphor screen and scanned using Typhoon FLA 7000 apparatus. The displayed images are the acquired scans after global Auto-Contrast and Brightness/Contrast adjustments.

Figure 4- Source data

B**D****Figure 4- Source data**