


Urinary iodine: comparison of a simple method for its determination in microplates
with measurement by inductively-coupled plasma mass spectrometry

Michael Haap¹, Heinz Jürgen Roth², Thomas Huber², Helmut Dittmann³ and
Richard Wahl¹

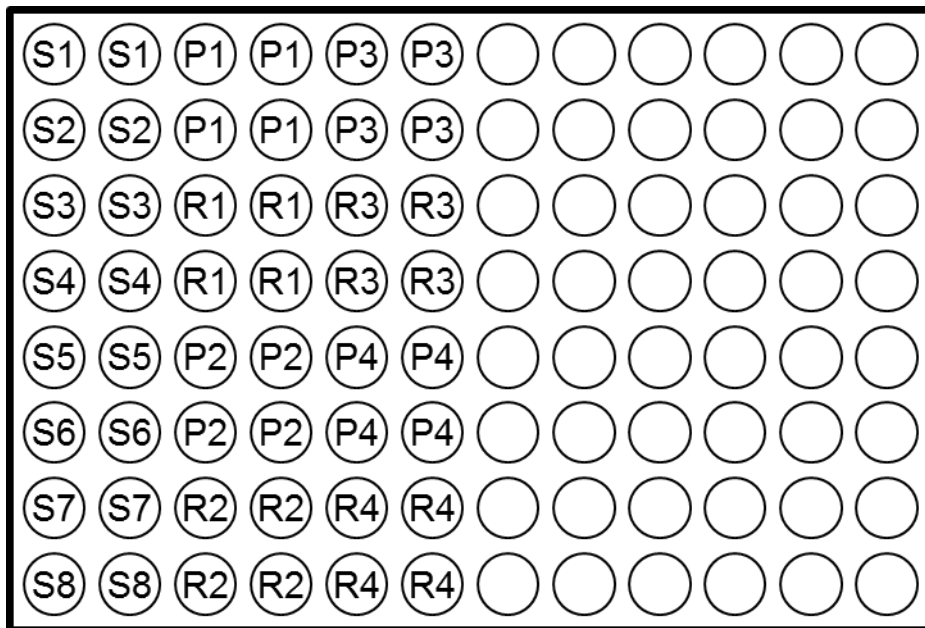

Supplementary Figure S 1: Arrangement of samples in the microplate. S1-S8 standards, P patients, R Recovery of iodine in the patient`s samples. The remaining vials can be filled with additional patient samples.