


Supplementary Figure 1

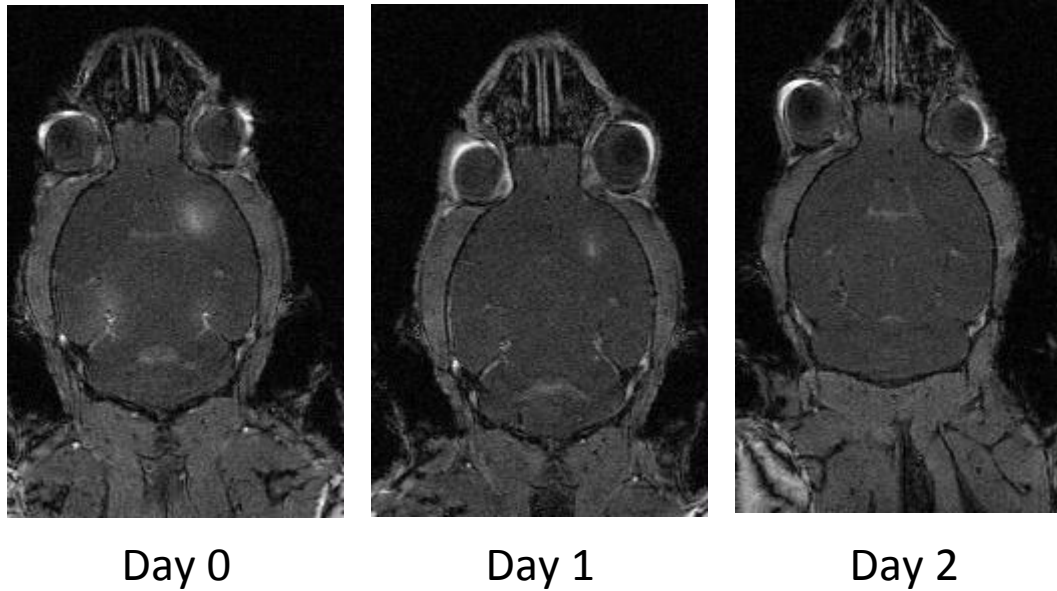

Caption: BBB is closed on day 2 under the ultrasound parameters used in this study (0.45 MPa).