
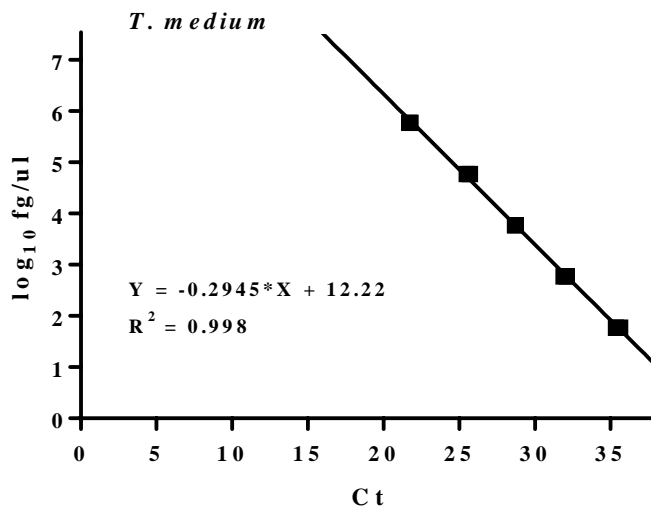
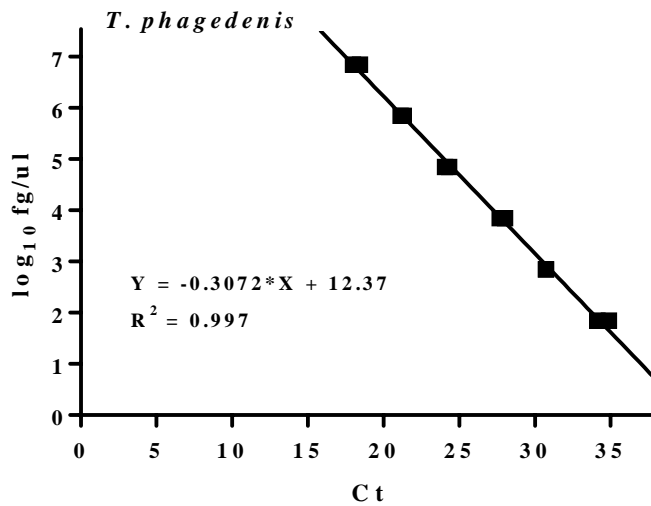


S1 Figure. Real-time PCR treponeme phylotype standard curves.

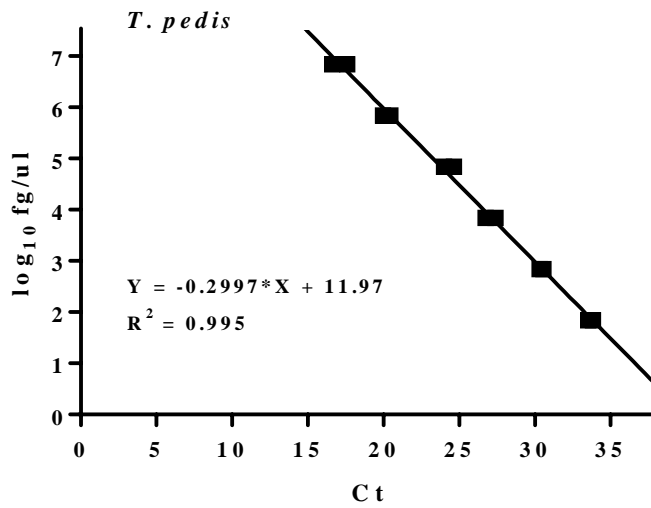

S1 Figure. Standard curves were determined by plotting the Ct value obtained from amplification of each phylotype target sequence against DNA concentration (log fg/μl) for each dilution. Ct represents the real-time PCR cycle at which fluorescence reaches the threshold value.