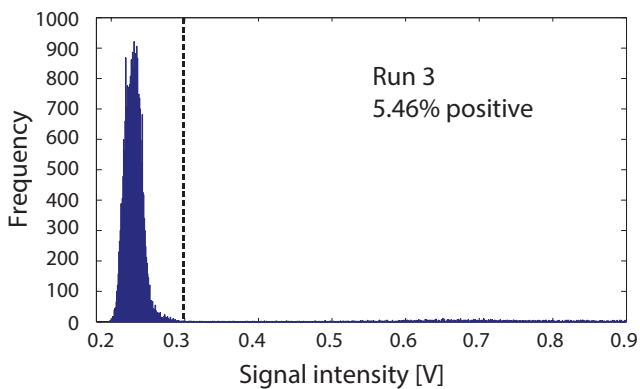
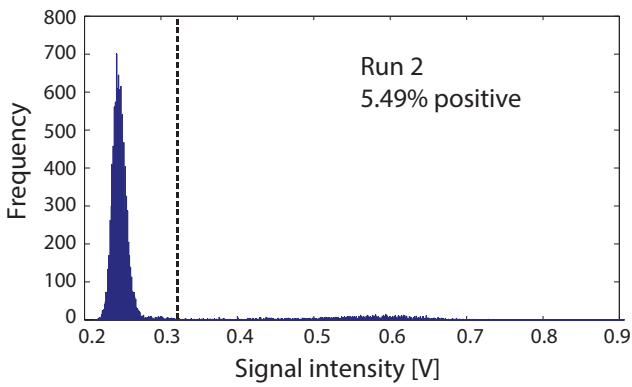
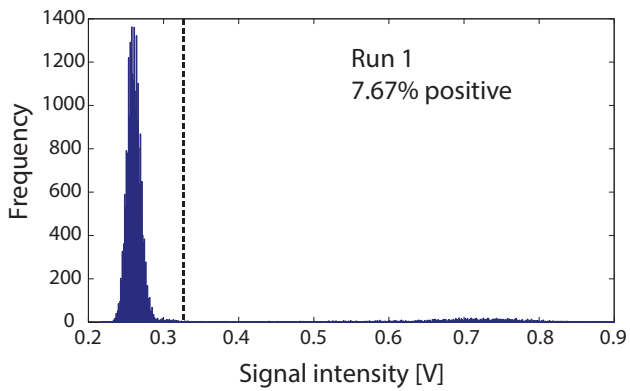
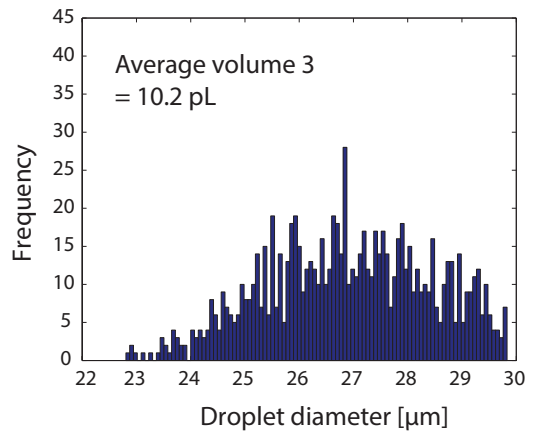
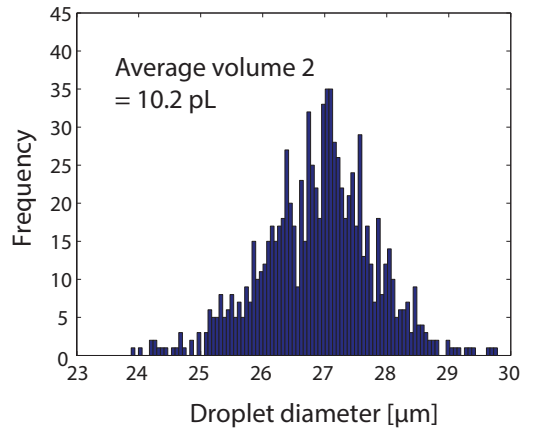
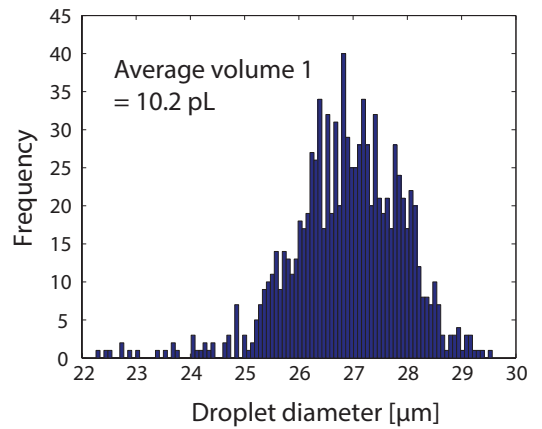


A Φ X174 digital PCR readings**B** Φ X174 droplet size distribution**C**

Run	Positive drops (%)	λ (particles/drop)	Virus conc. (/mL)
1	7.67	0.0798	$7.82 \cdot 10^6$
2	5.49	0.0565	$5.54 \cdot 10^6$
3	5.46	0.0561	$5.35 \cdot 10^6$